


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082118\
 Data File : VN050788.D
 Acq On : 21 Aug 2018 17:41
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
 Title : SW846 8260
 Last Update : Wed Aug 22 05:38:12 2018

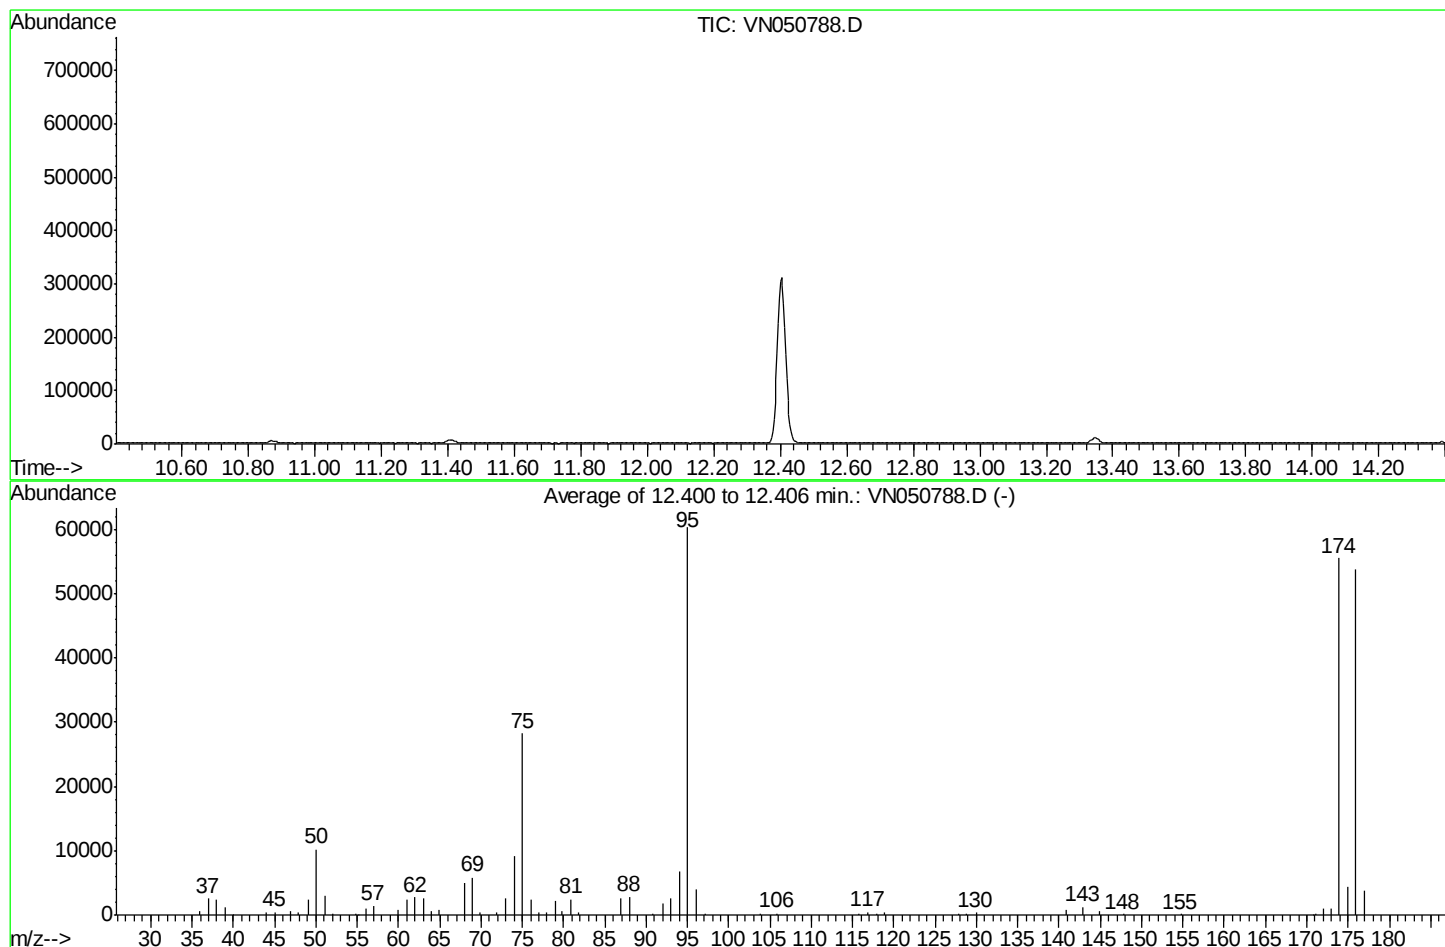

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	10176	PASS
75	95	30	60	46.8	28229	PASS
95	95	100	100	100.0	60317	PASS
96	95	5	9	6.7	4046	PASS
173	174	0.00	2	1.9	1044	PASS
174	95	50	100	92.0	55493	PASS
175	174	5	9	8.0	4412	PASS
176	174	95	101	96.9	53781	PASS
177	176	5	9	6.9	3725	PASS