


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082120\
 Data File : VN063070.D
 Acq On : 21 Aug 2020 8:45
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
 Title : SW846 8260
 Last Update : Wed Aug 19 06:09:27 2020

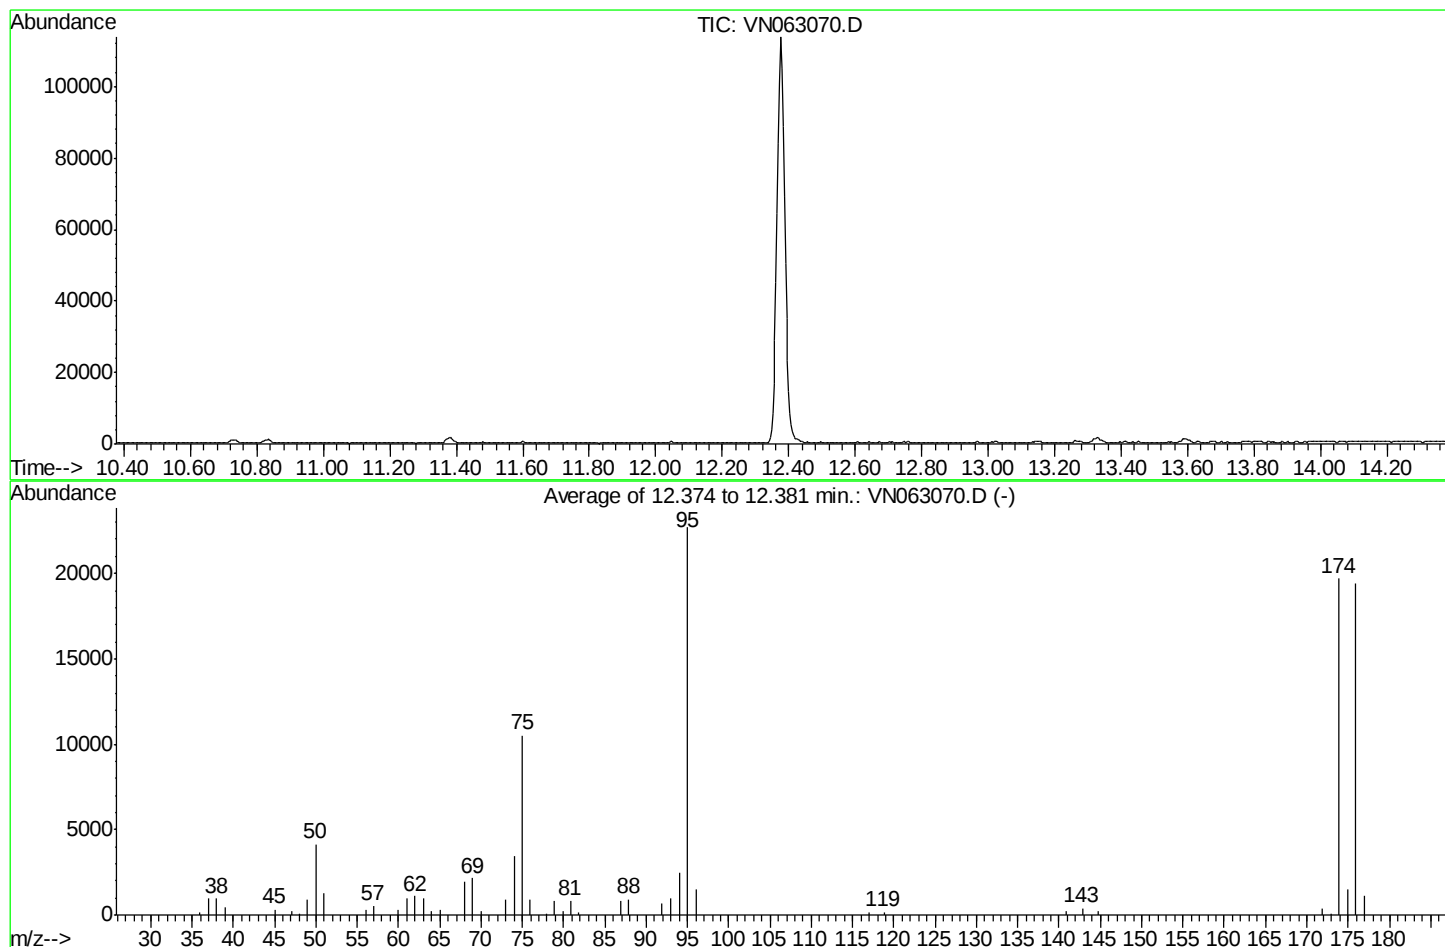

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	4134	PASS
75	95	30	60	46.3	10505	PASS
95	95	100	100	100.0	22698	PASS
96	95	5	9	6.6	1508	PASS
173	174	0.00	2	0.5	104	PASS
174	95	50	100	86.8	19698	PASS
175	174	5	9	7.7	1511	PASS
176	174	95	101	98.7	19442	PASS
177	176	5	9	5.8	1127	PASS