


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082218\
Data File : VN050808.D
Acq On : 22 Aug 2018 10:13
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Title : SW846 8260
Last Update : Wed Aug 22 05:38:12 2018

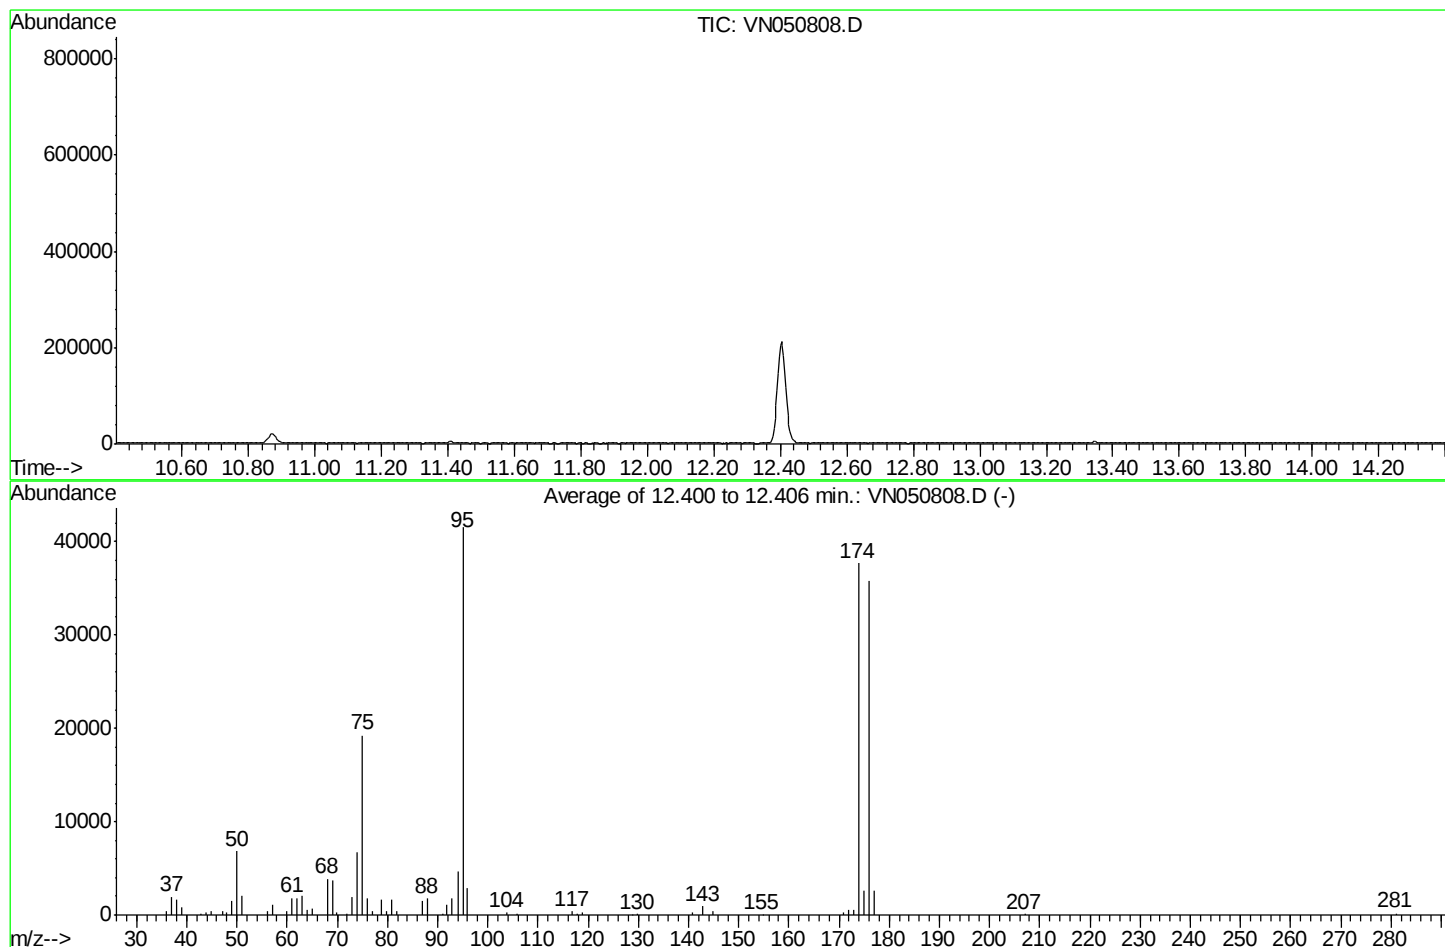

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	6804	PASS
75	95	30	60	46.3	19221	PASS
95	95	100	100	100.0	41538	PASS
96	95	5	9	7.0	2928	PASS
173	174	0.00	2	1.6	602	PASS
174	95	50	100	90.7	37677	PASS
175	174	5	9	6.8	2568	PASS
176	174	95	101	95.0	35802	PASS
177	176	5	9	7.3	2600	PASS