


1,1,2,2-Tetrachloroethane

Response Ratio

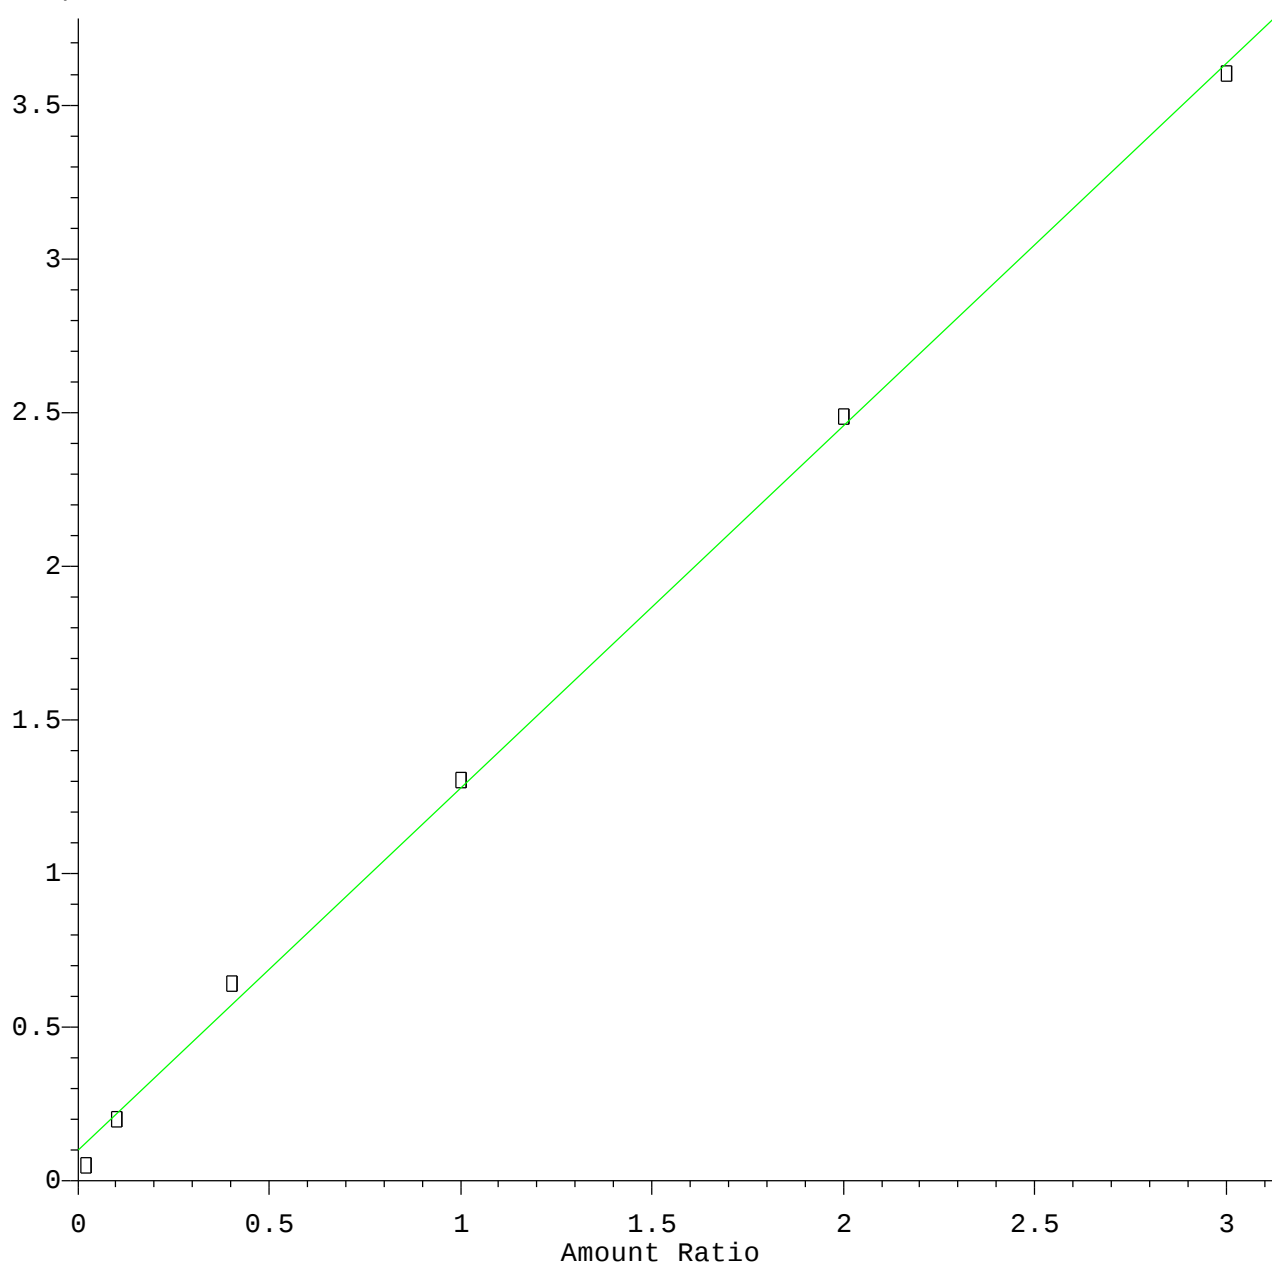


Resp Ratio = 1.18e+000 * Amt + 9.84e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019


1,2,3-Trichloropropane

Response Ratio

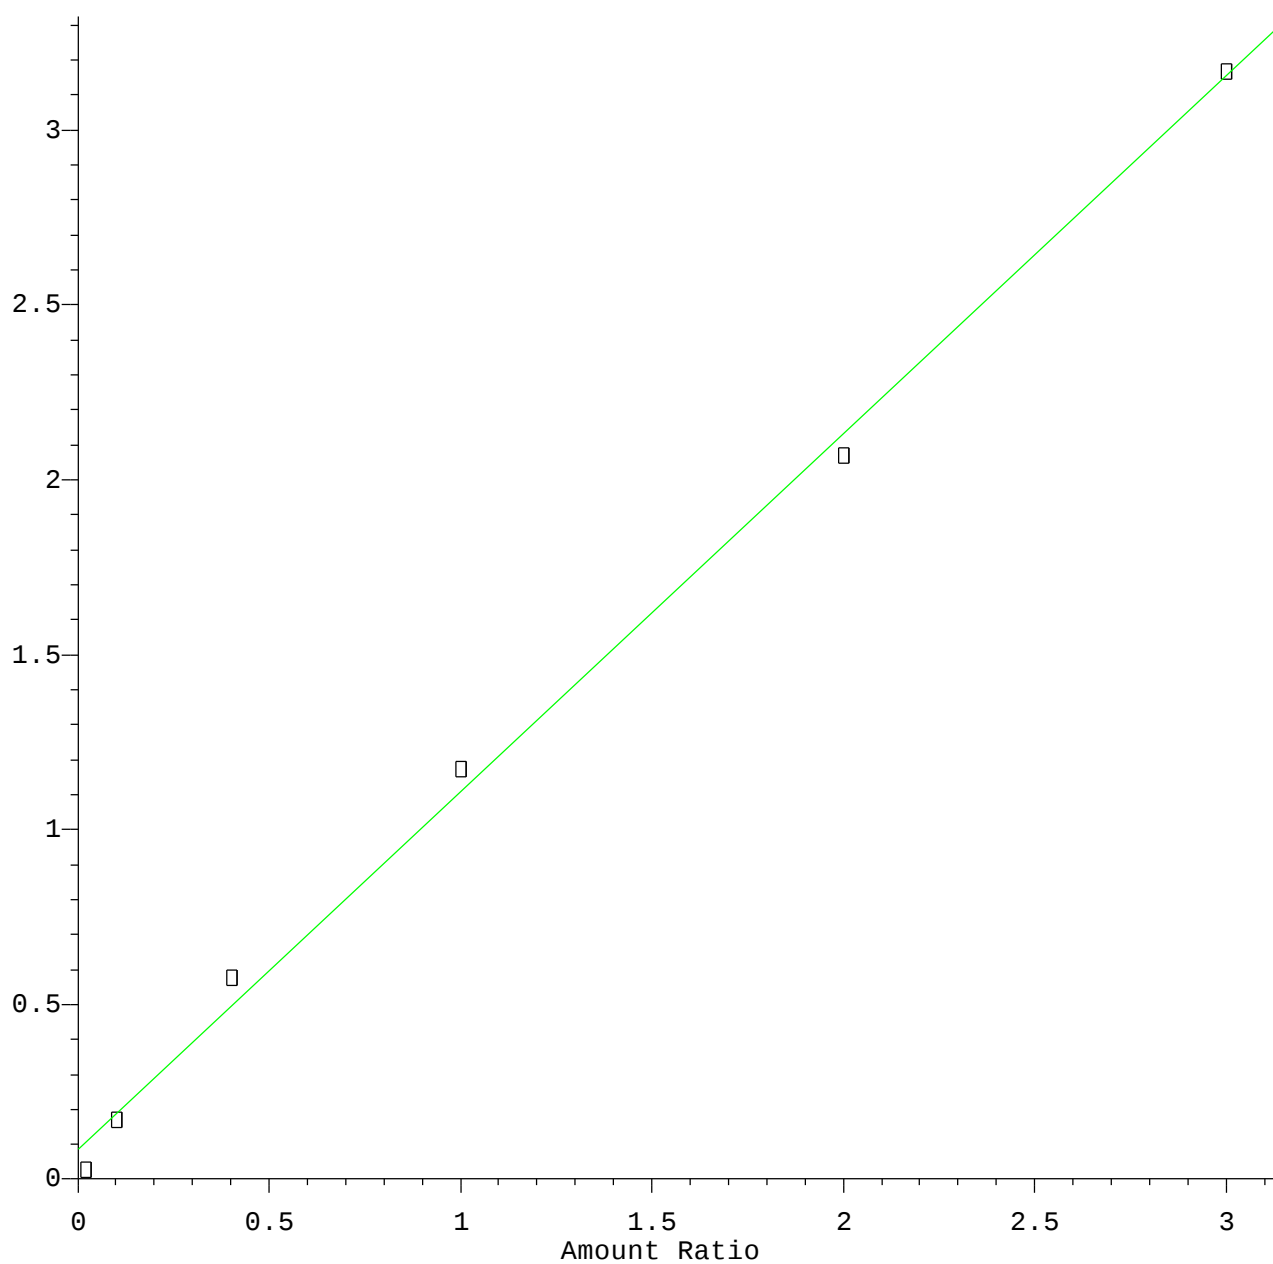


Resp Ratio = 1.02e+000 * Amt + 8.27e-002
Coef of Det (r²) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

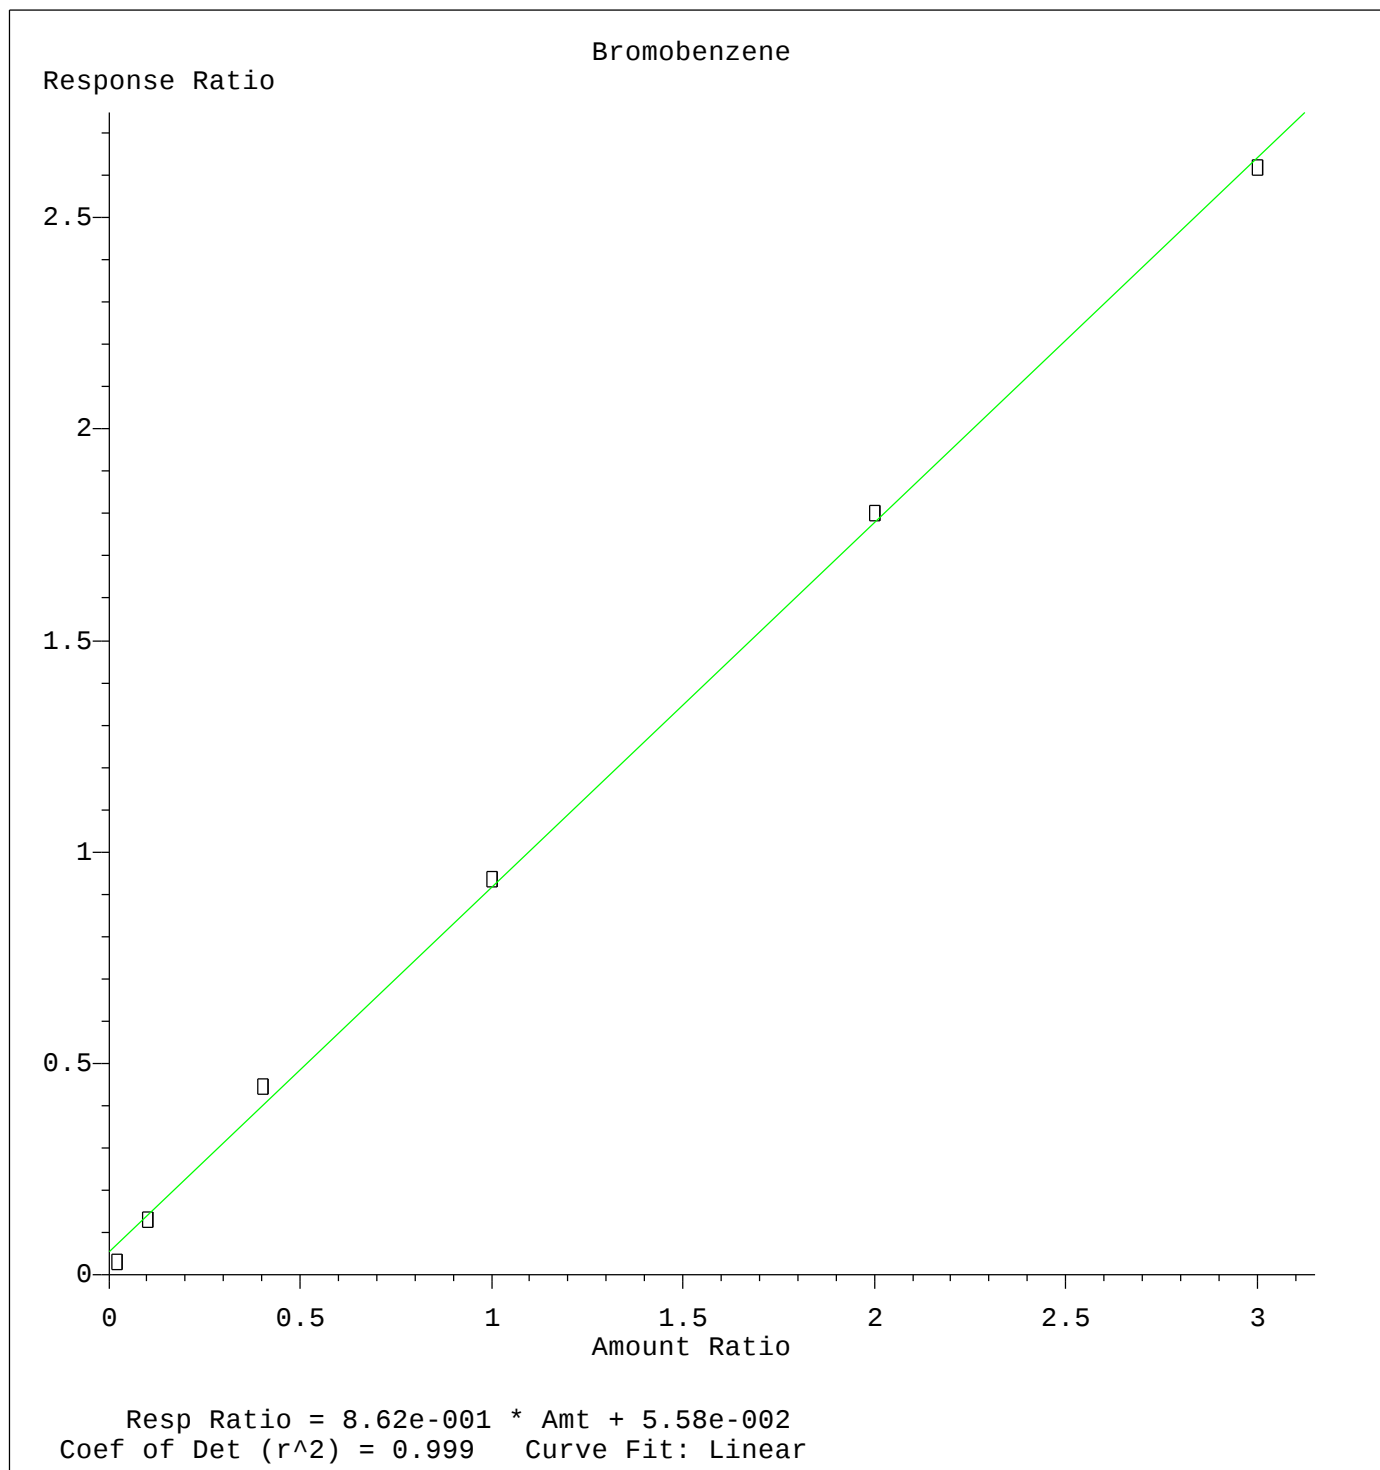


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

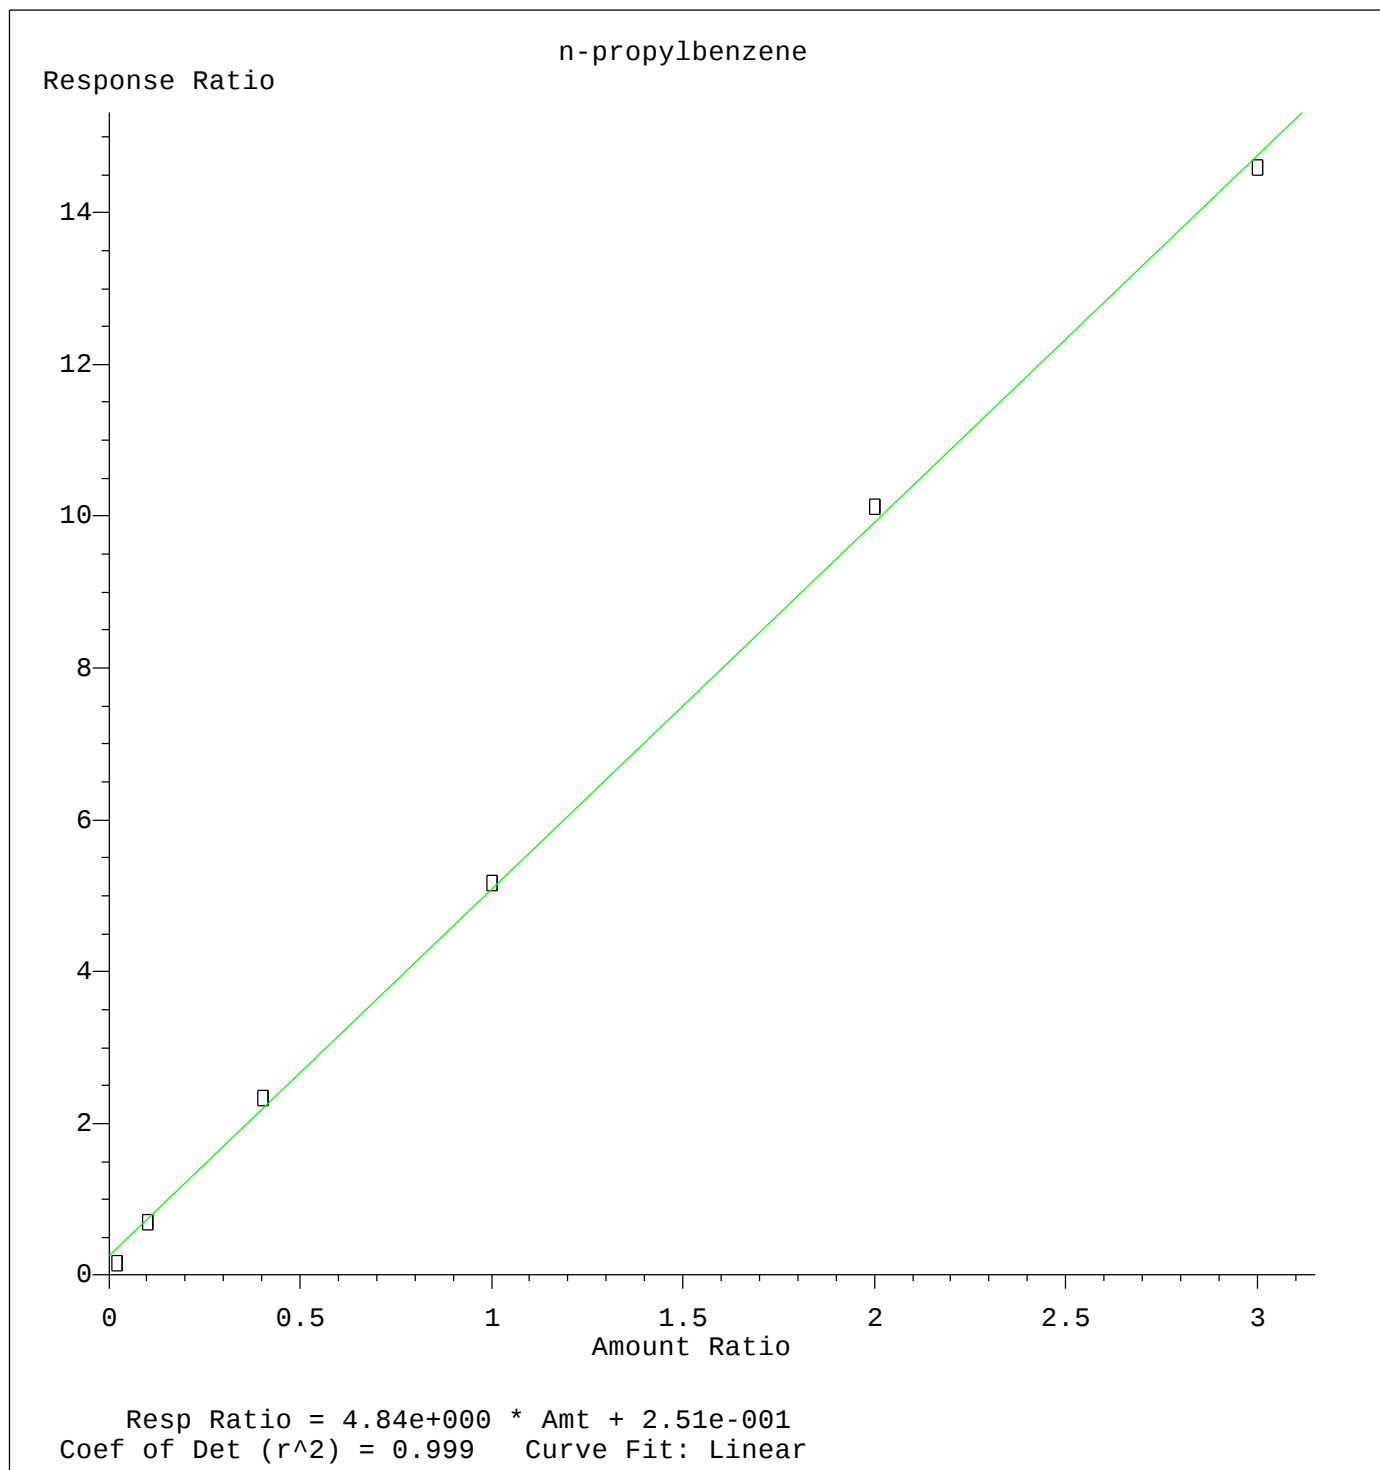

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

2-Chlorotoluene

Response Ratio

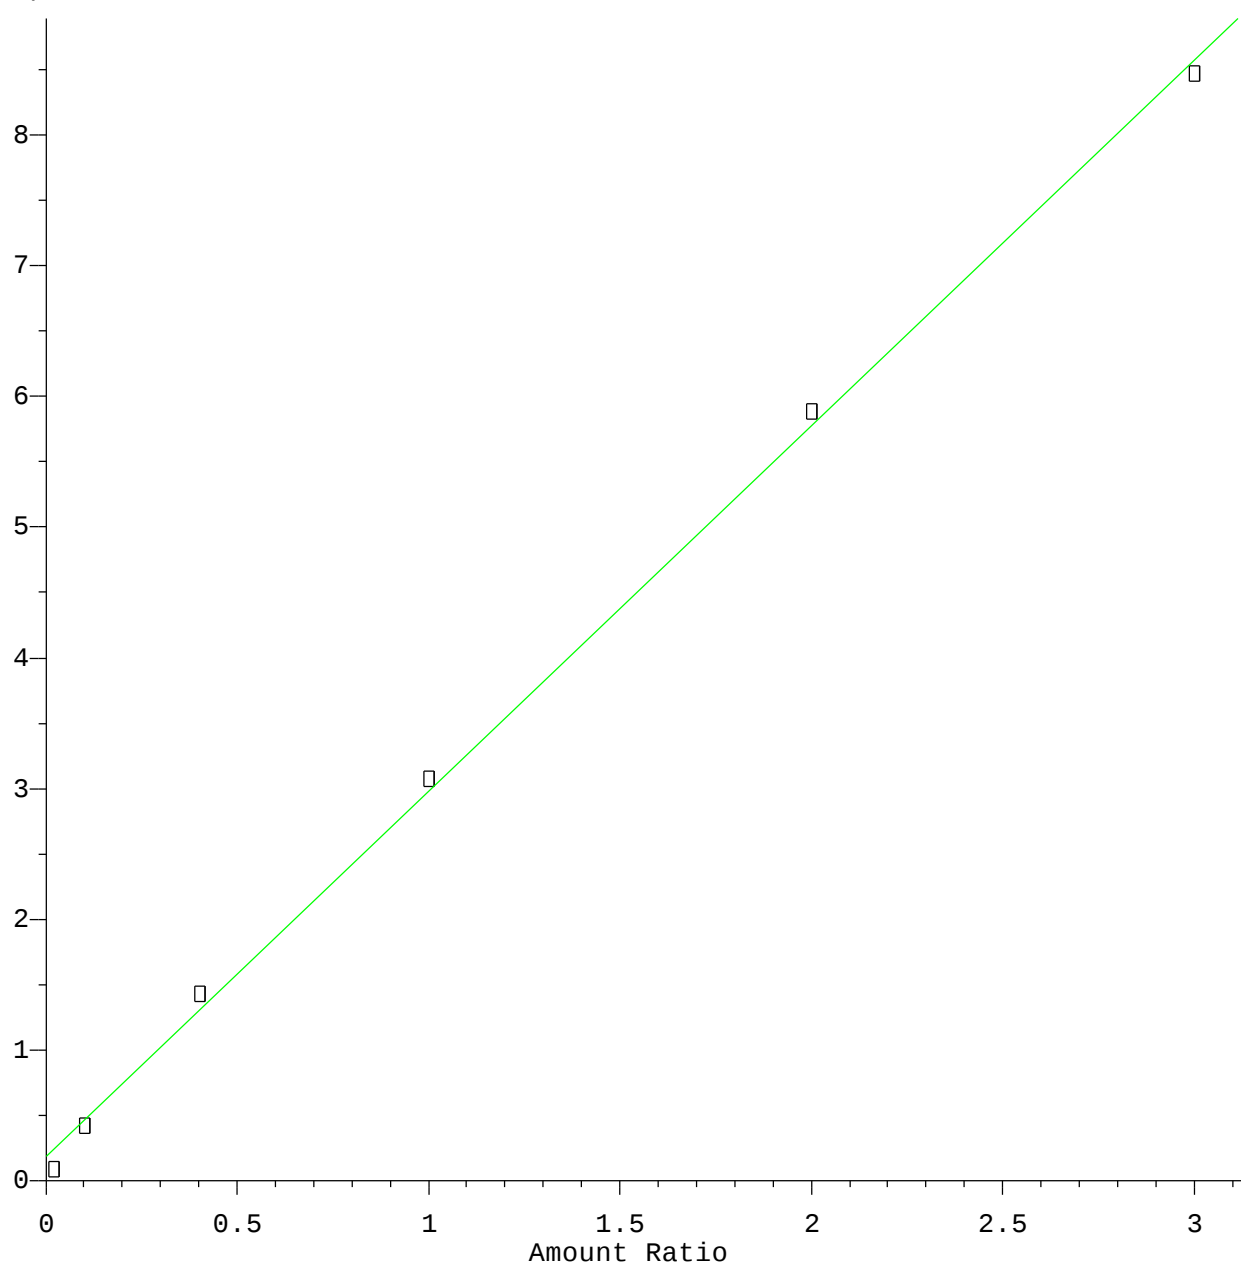


Resp Ratio = 2.79e+000 * Amt + 1.90e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

1,3,5-Trimethylbenzene

Response Ratio

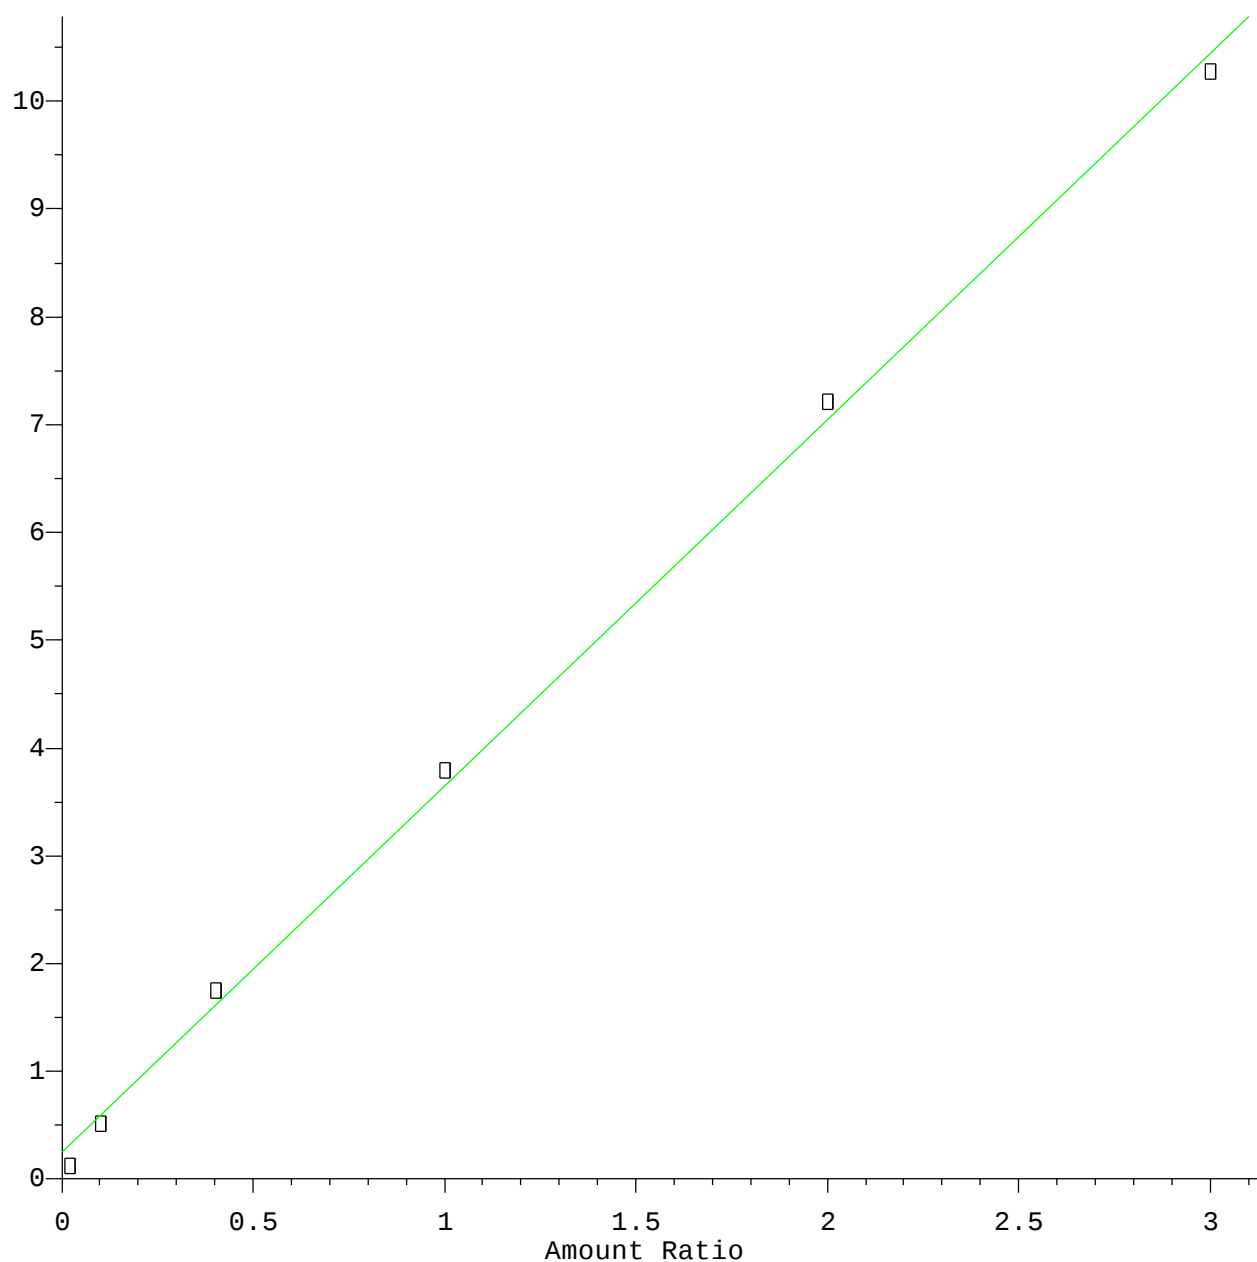


Resp Ratio = $3.40 \times 10^0 \times \text{Amt} + 2.50 \times 10^{-1}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

trans-1,4-Dichloro-2-butene

Response Ratio

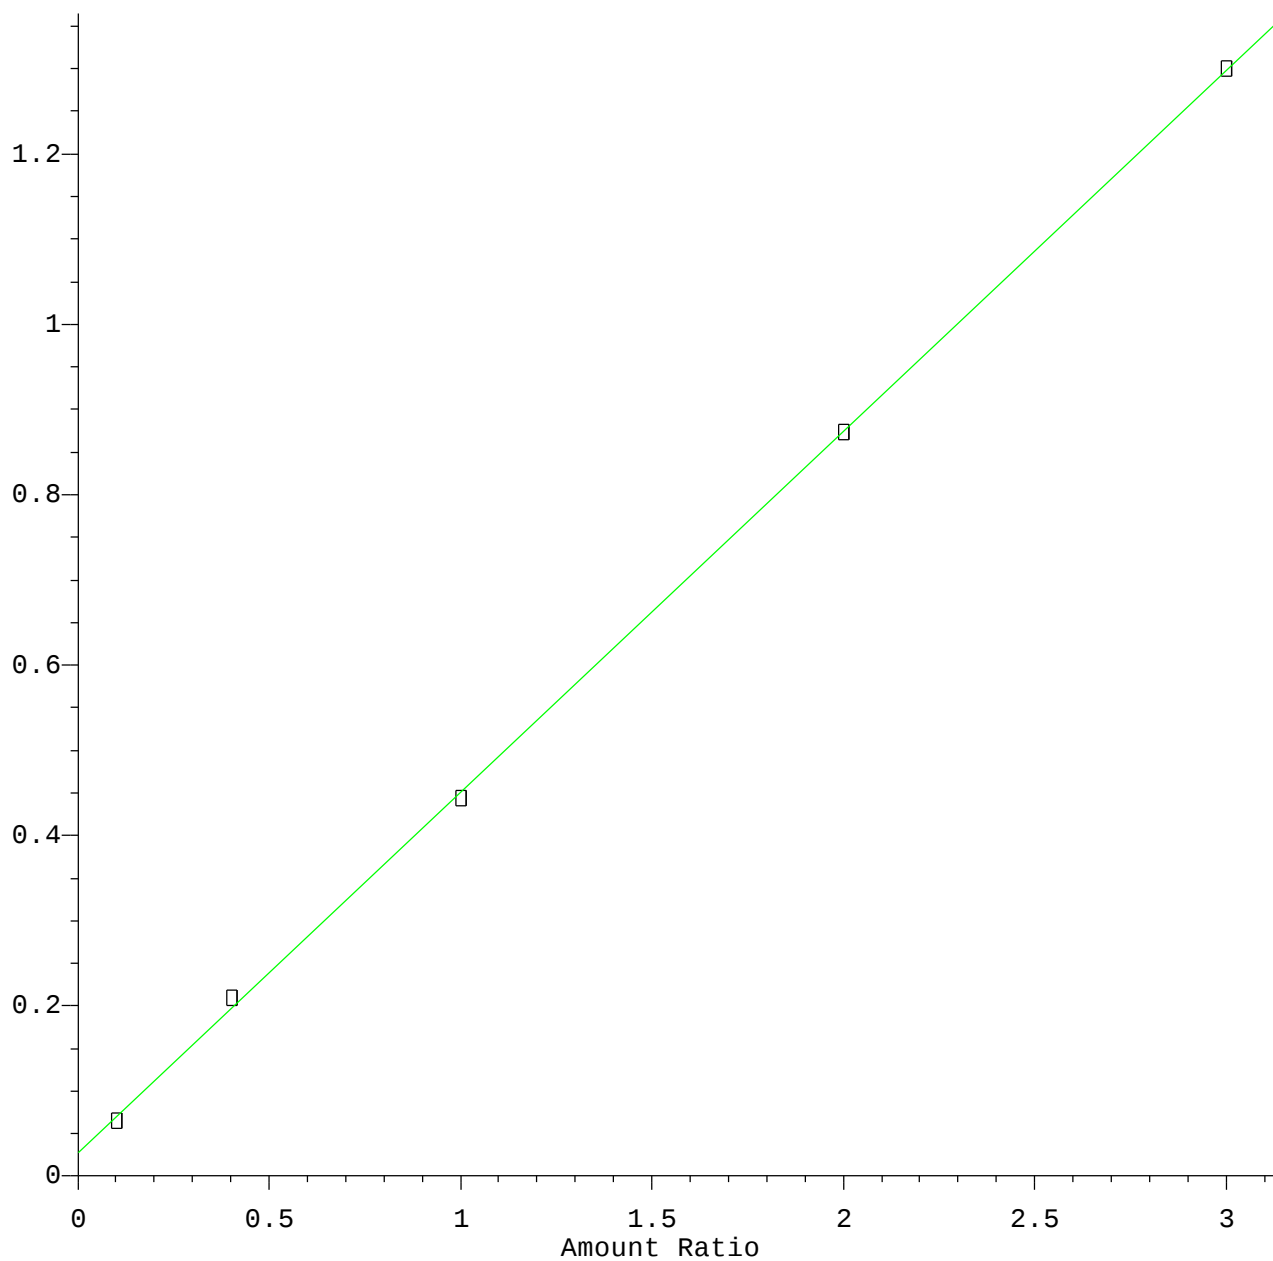


Resp Ratio = $4.24 \times 10^{-1} \times \text{Amt} + 2.73 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

4-Chlorotoluene

Response Ratio

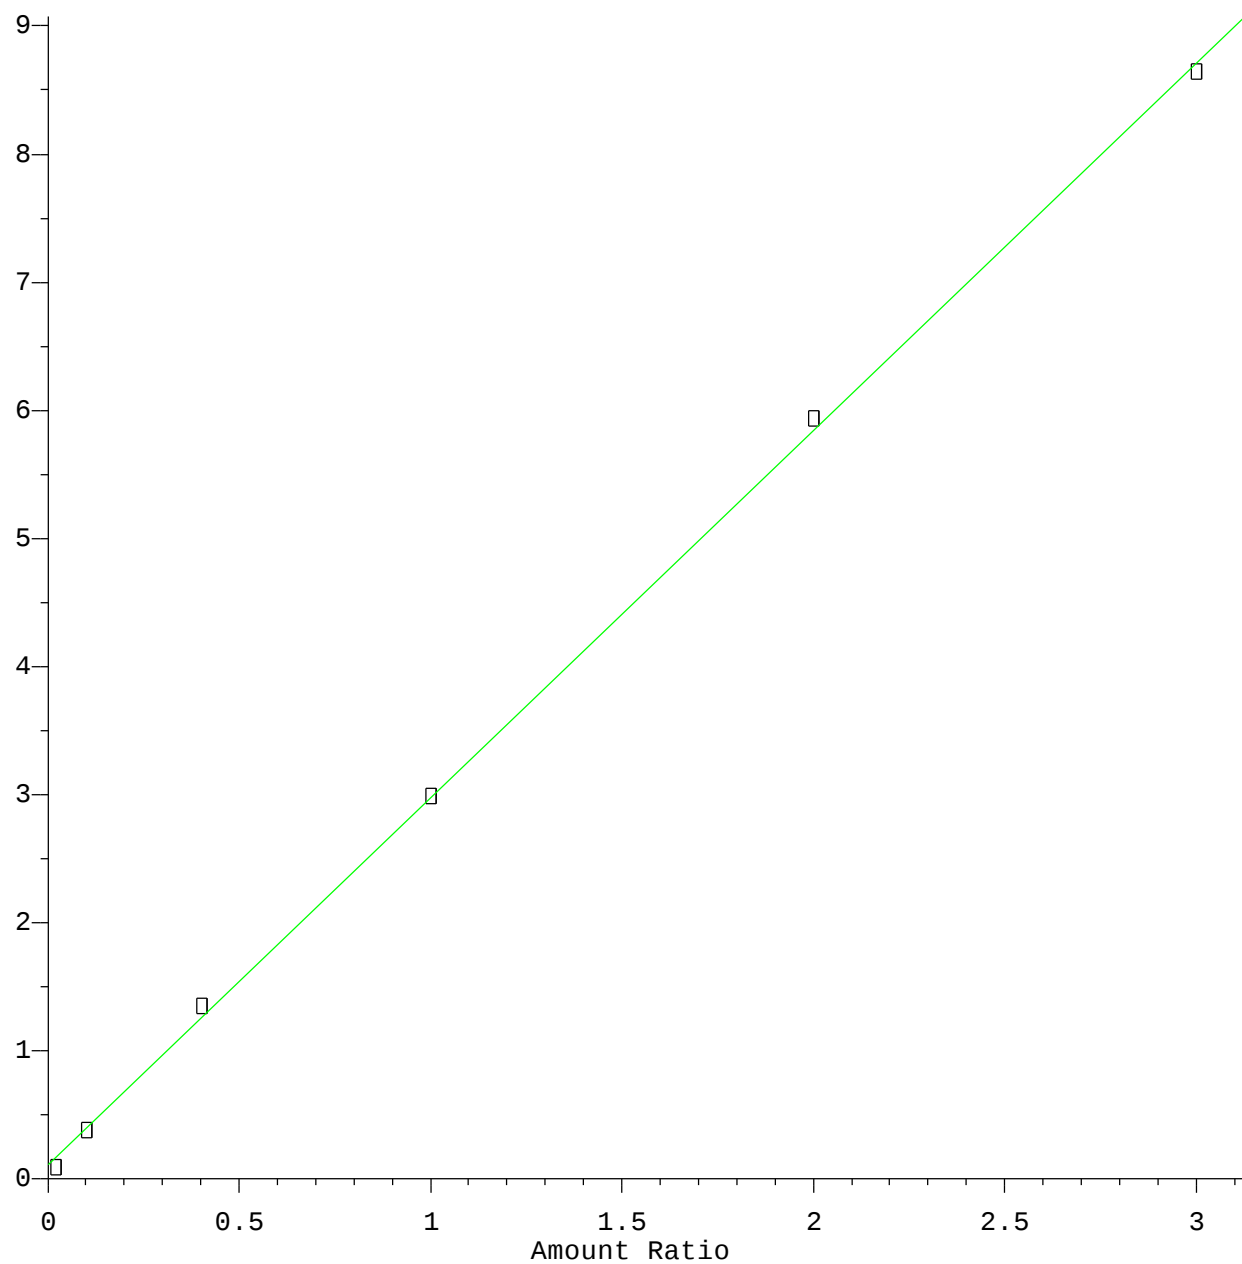


Resp Ratio = 2.87e+000 * Amt + 1.13e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

tert-Butylbenzene

Response Ratio

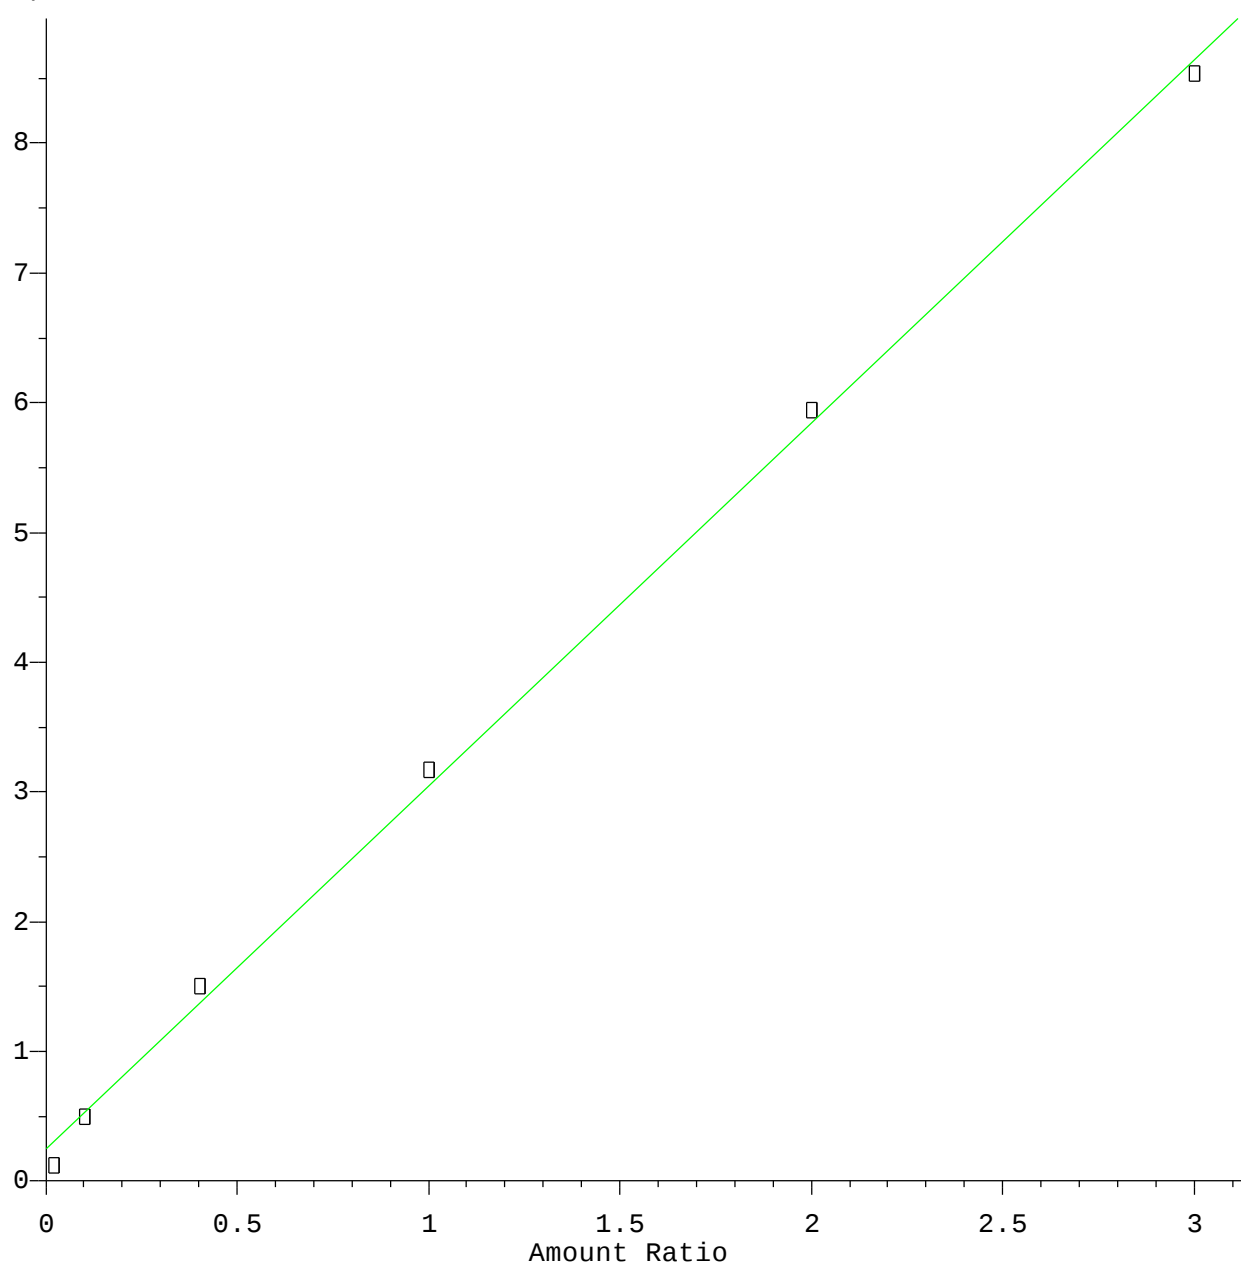


Resp Ratio = 2.80e+000 * Amt + 2.49e-001
Coef of Det (r²) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019


sec-Butylbenzene

Response Ratio

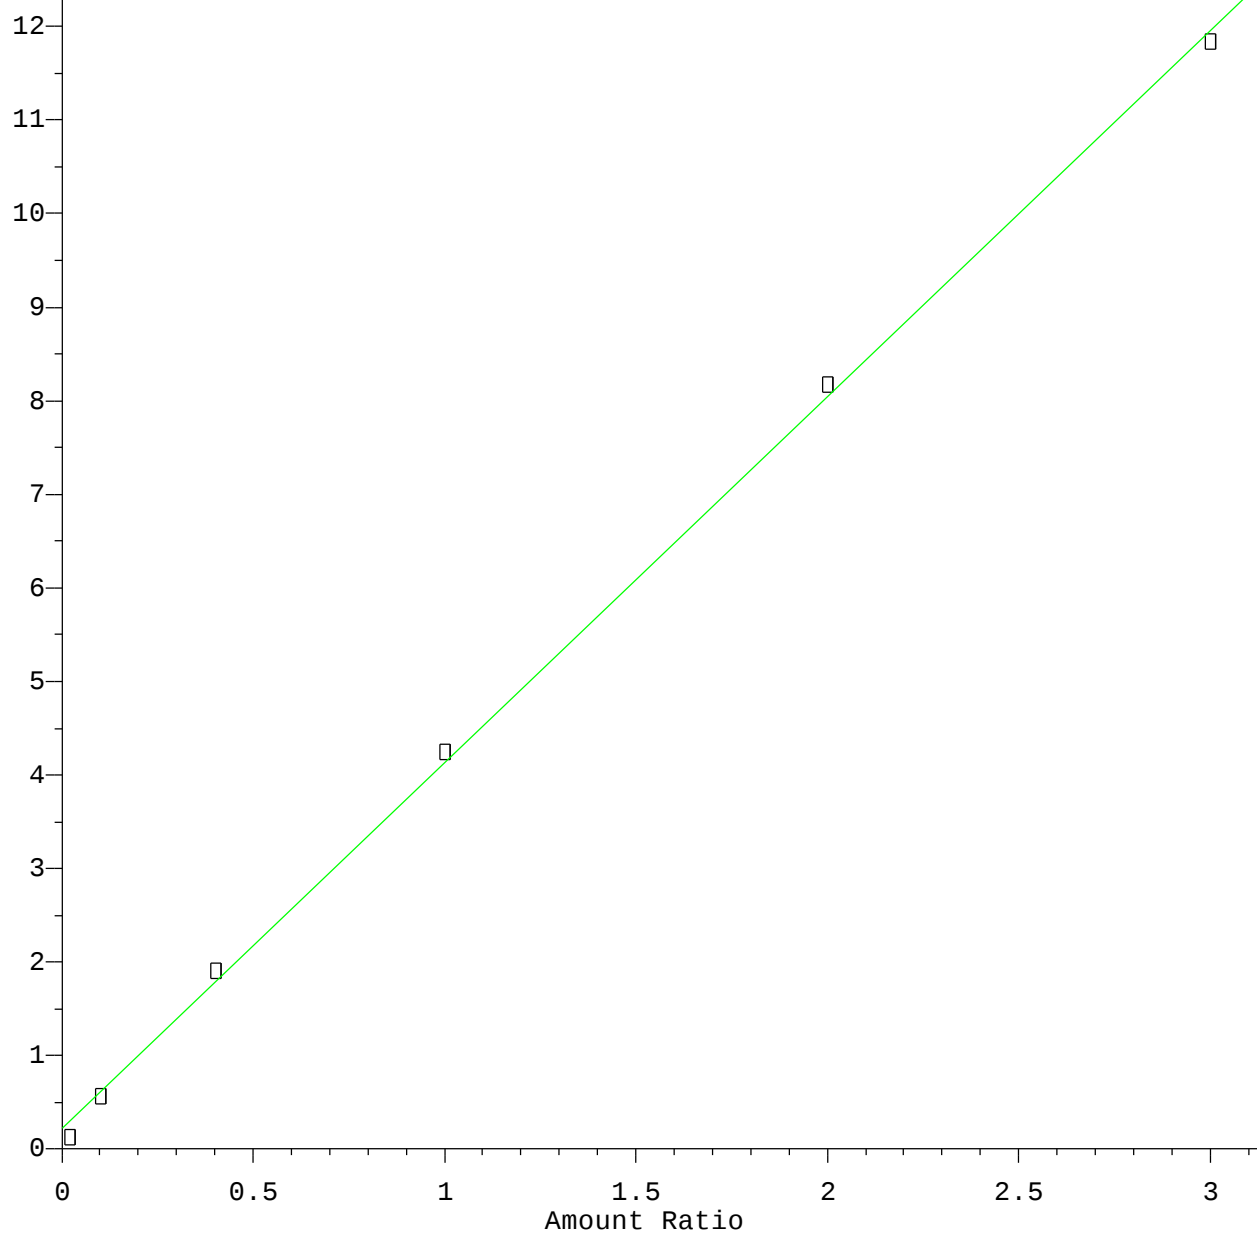

Resp Ratio = $3.91 \times 10^0 \times \text{Amt} + 2.18 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

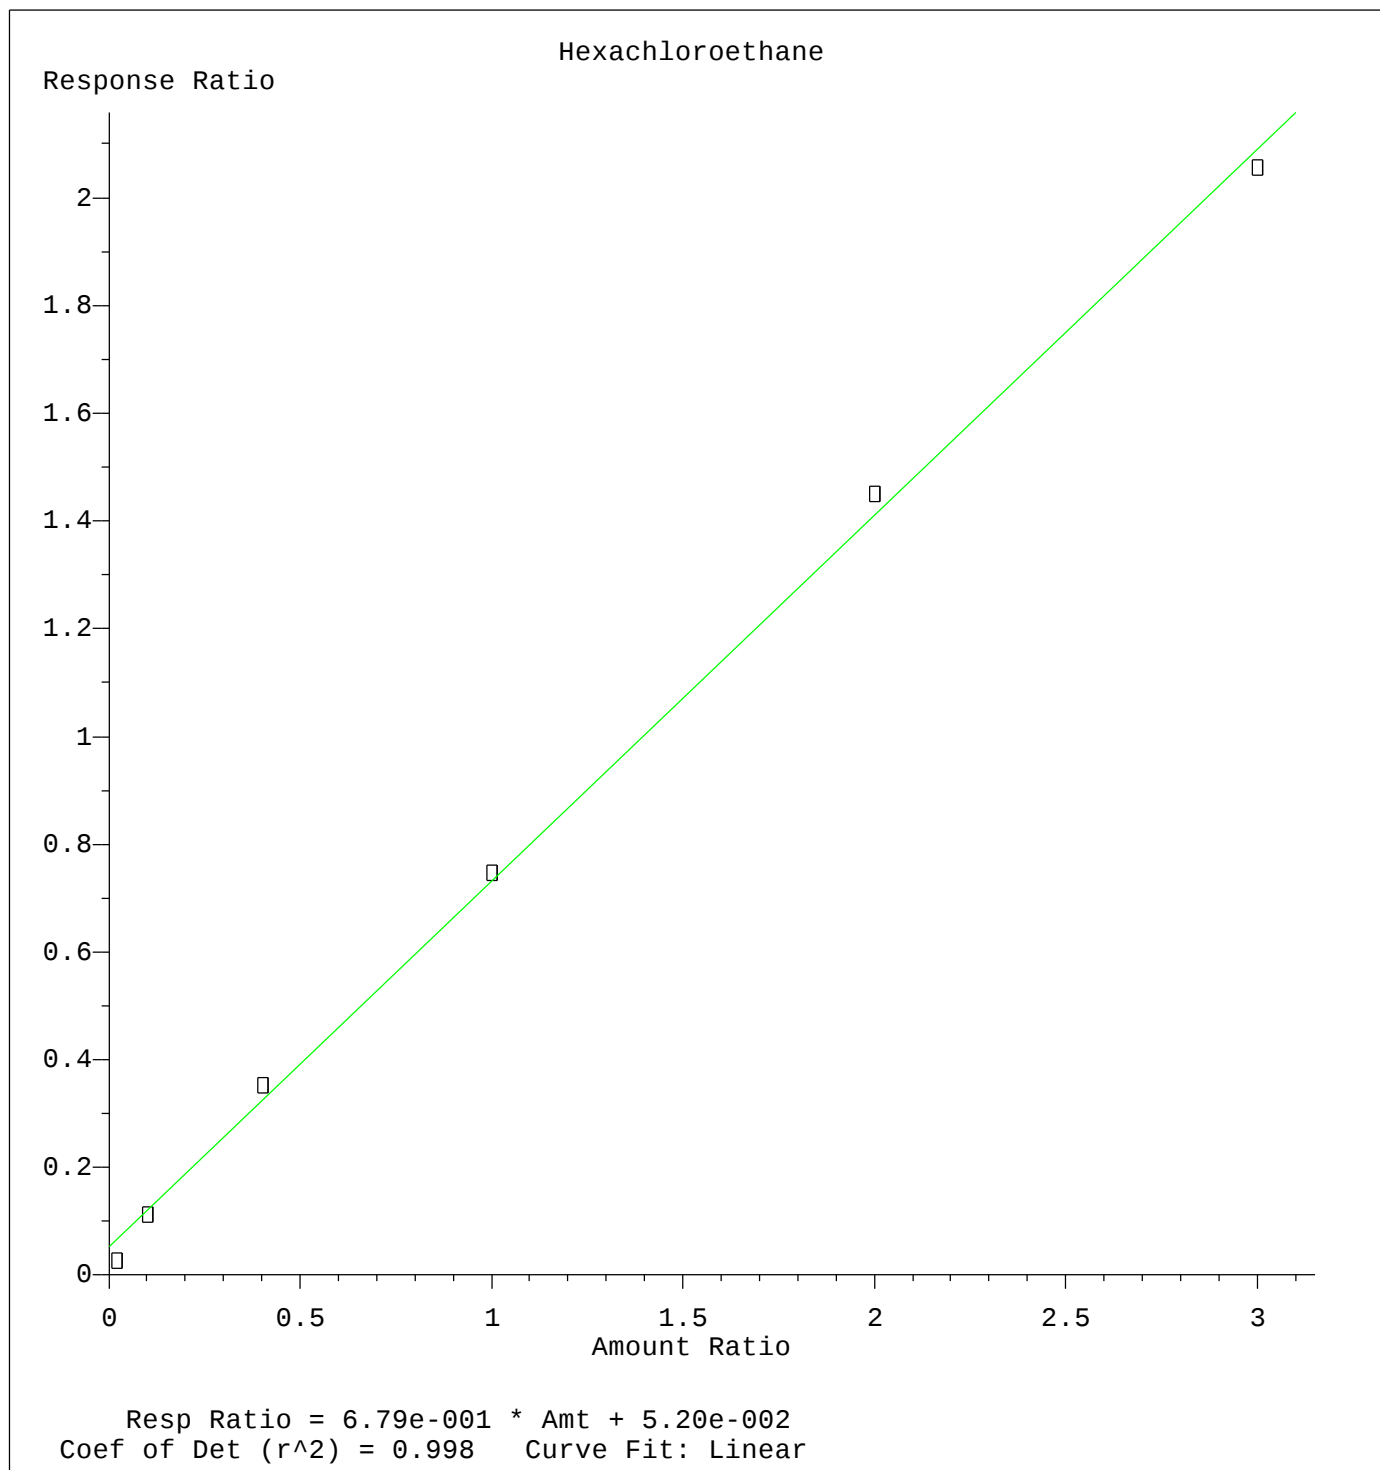

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

1,2-Dibromo-3-Chloropropane

Response Ratio

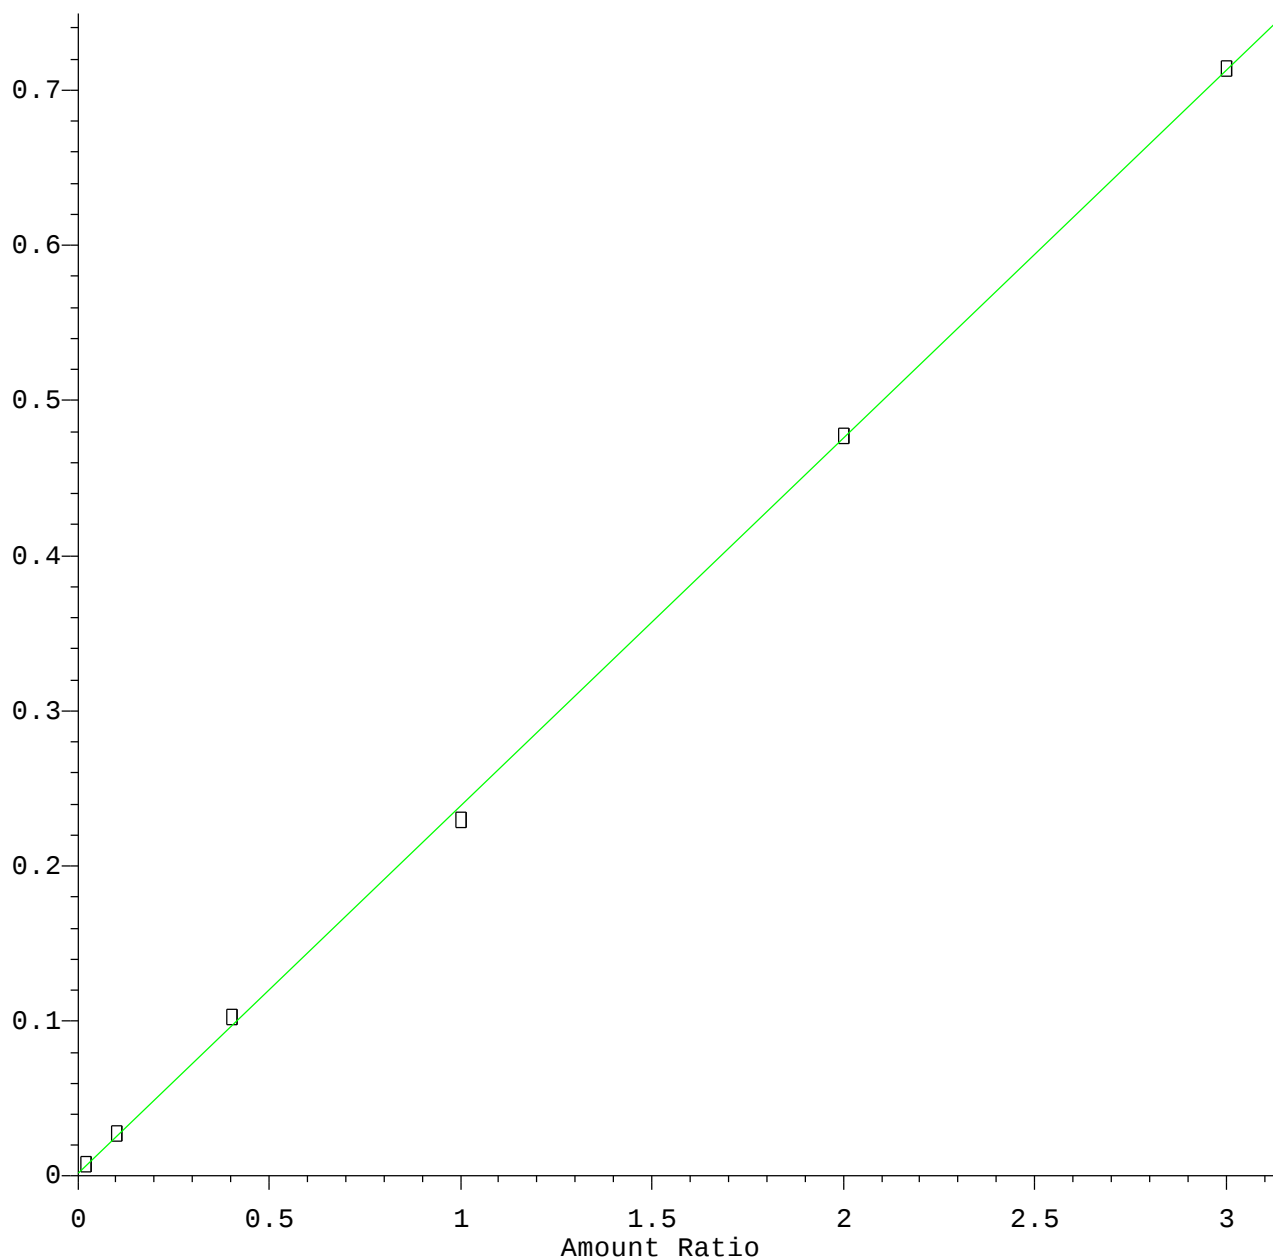


Resp Ratio = $2.37 \times 10^{-1} \times \text{Amt} + 2.36 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019


1,2,4-Trichlorobenzene

Response Ratio

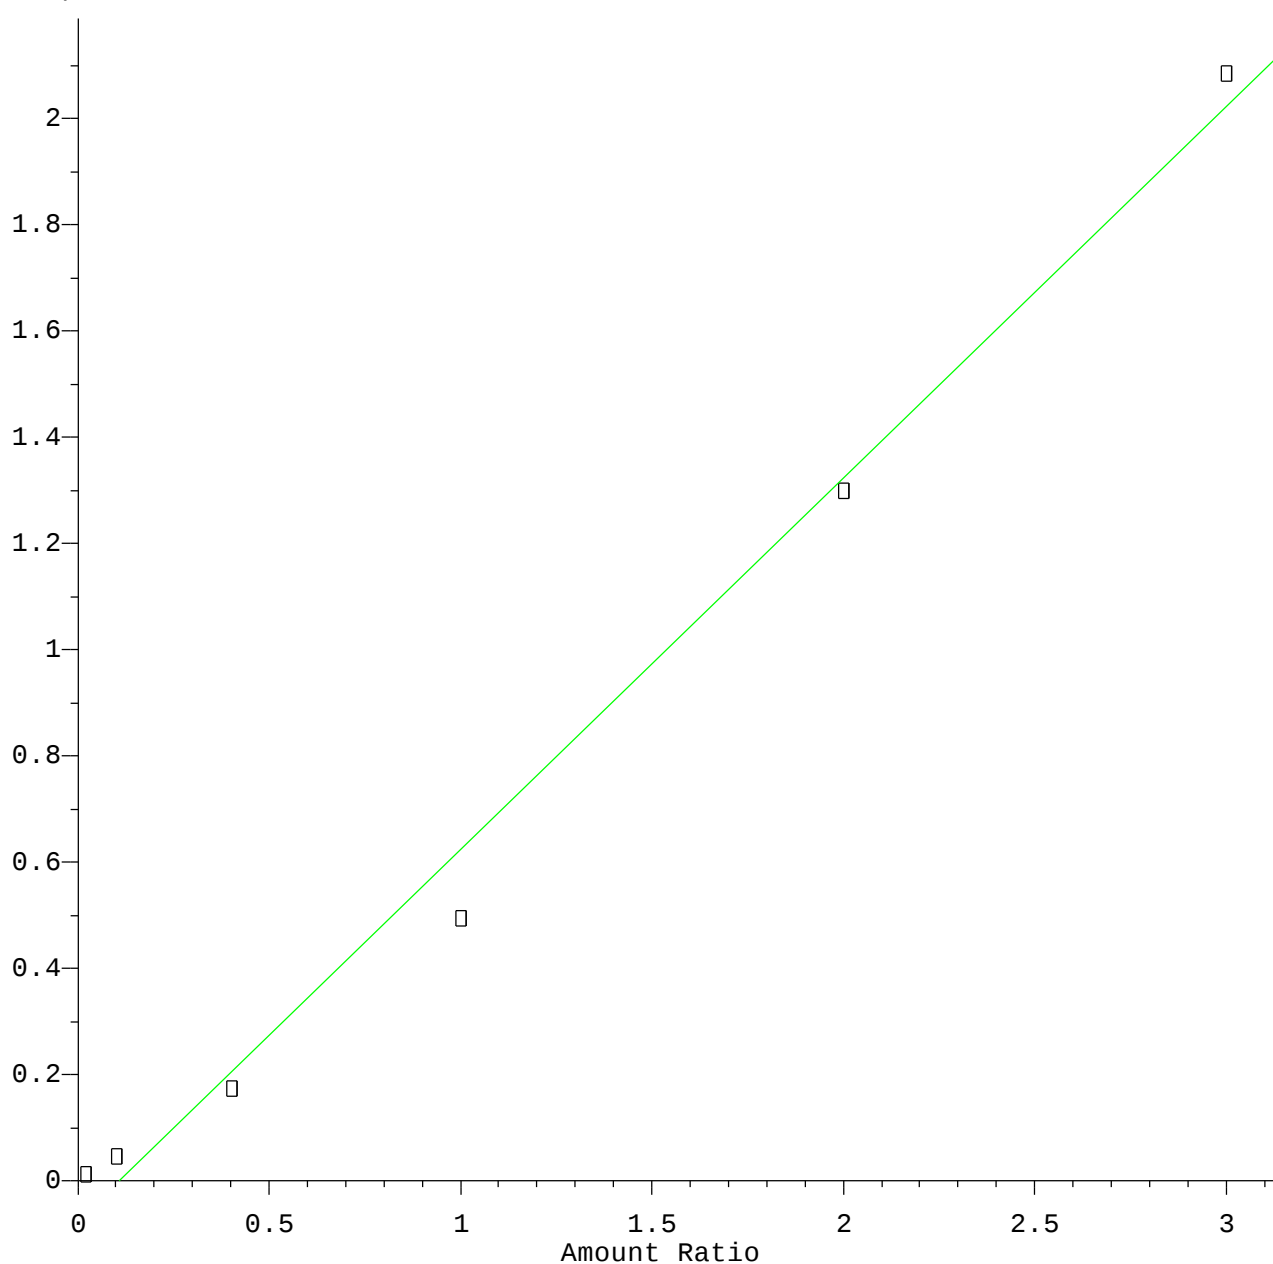

Resp Ratio = $6.99 \times 10^{-1} \times \text{Amt} - 7.51 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

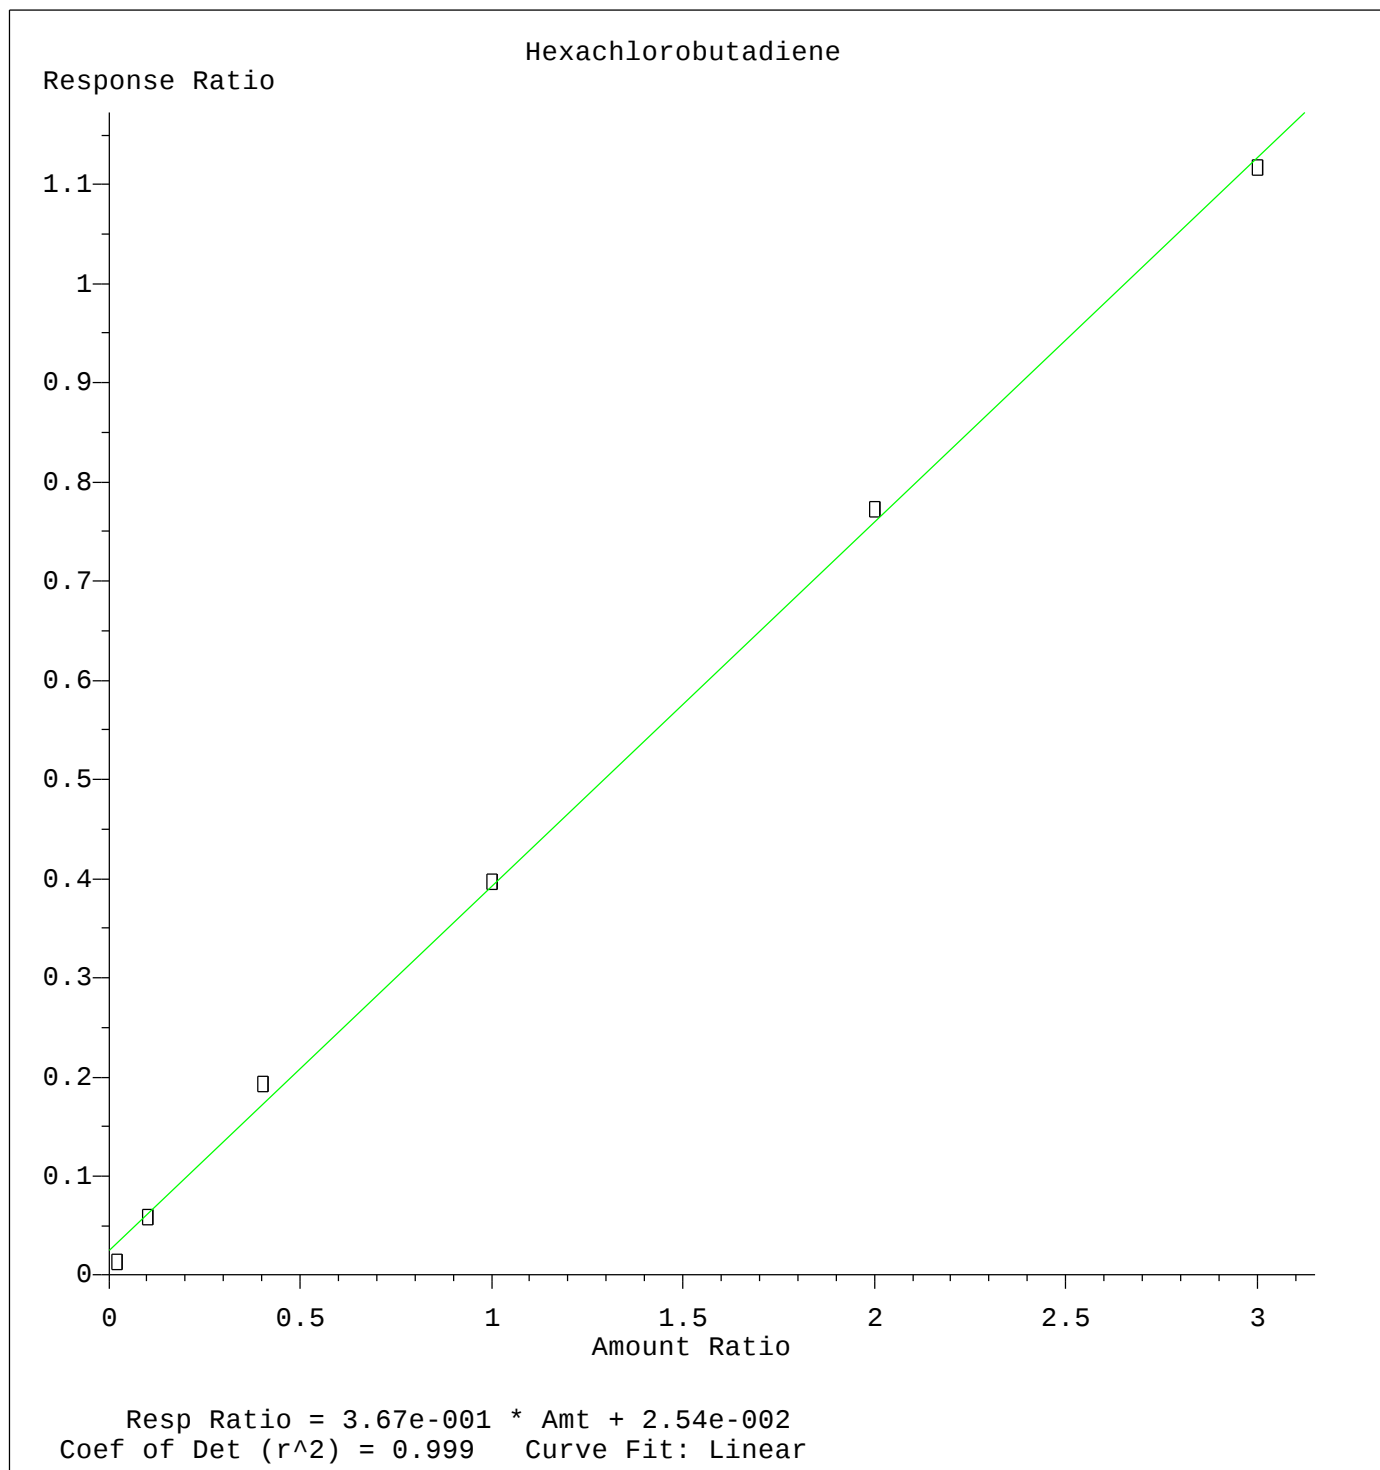

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

Naphthalene

Response Ratio

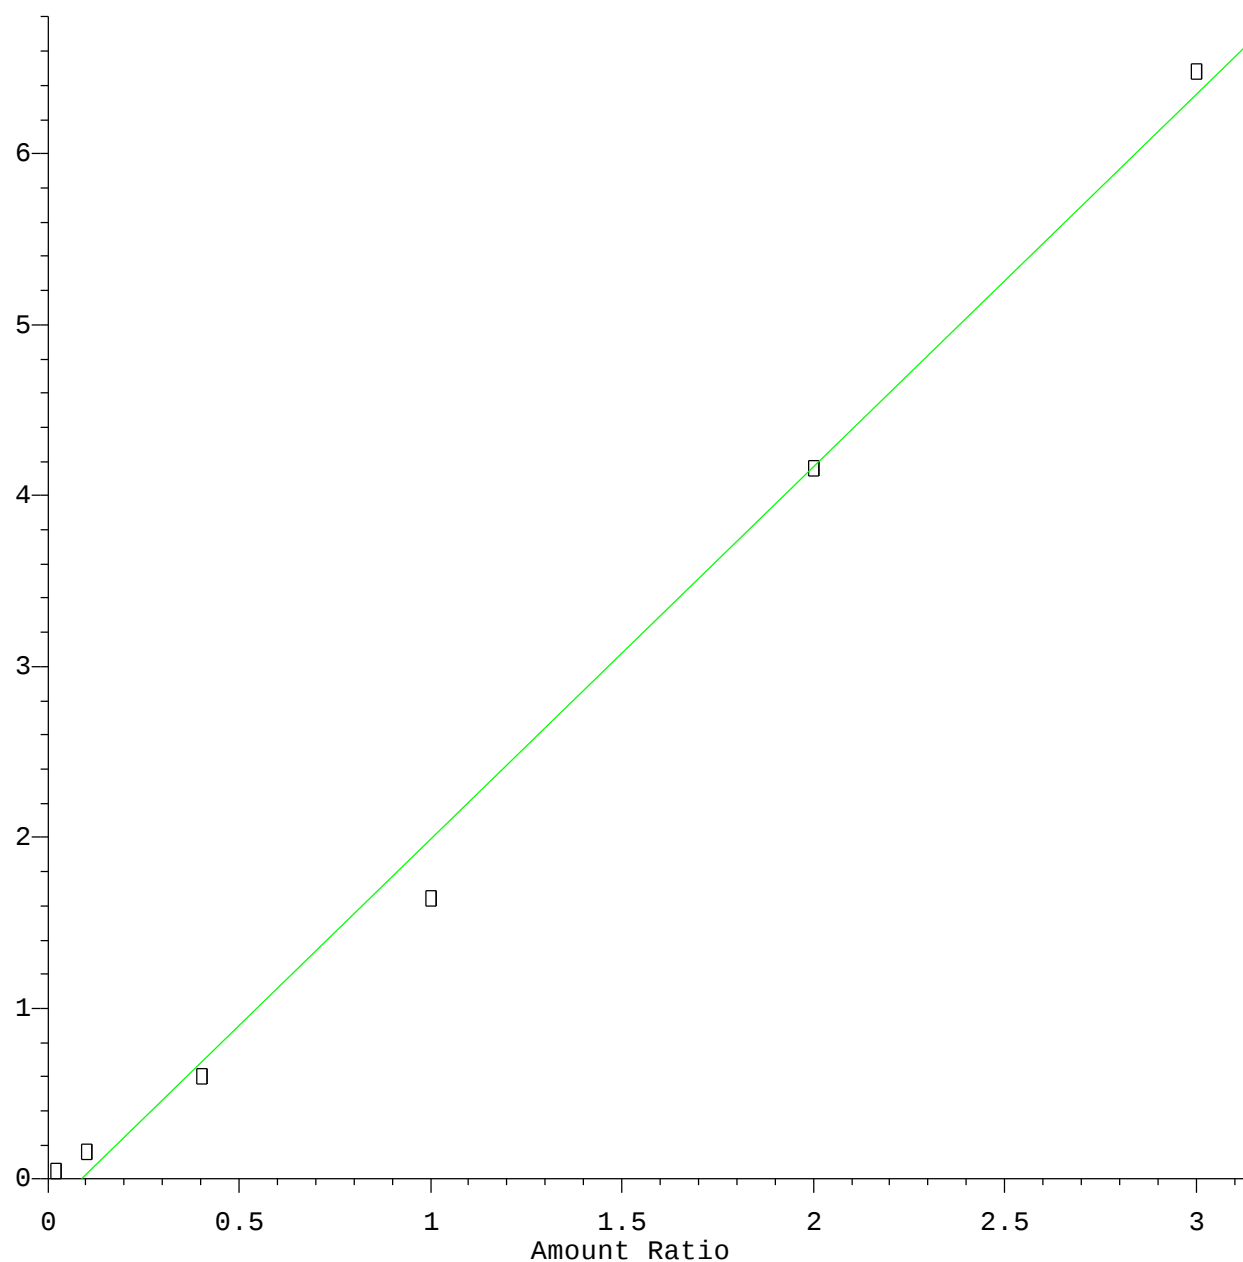


Resp Ratio = 2.18×10^0 * Amt - 1.89×10^{-1}
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019


1,2,3-Trichlorobenzene

Response Ratio

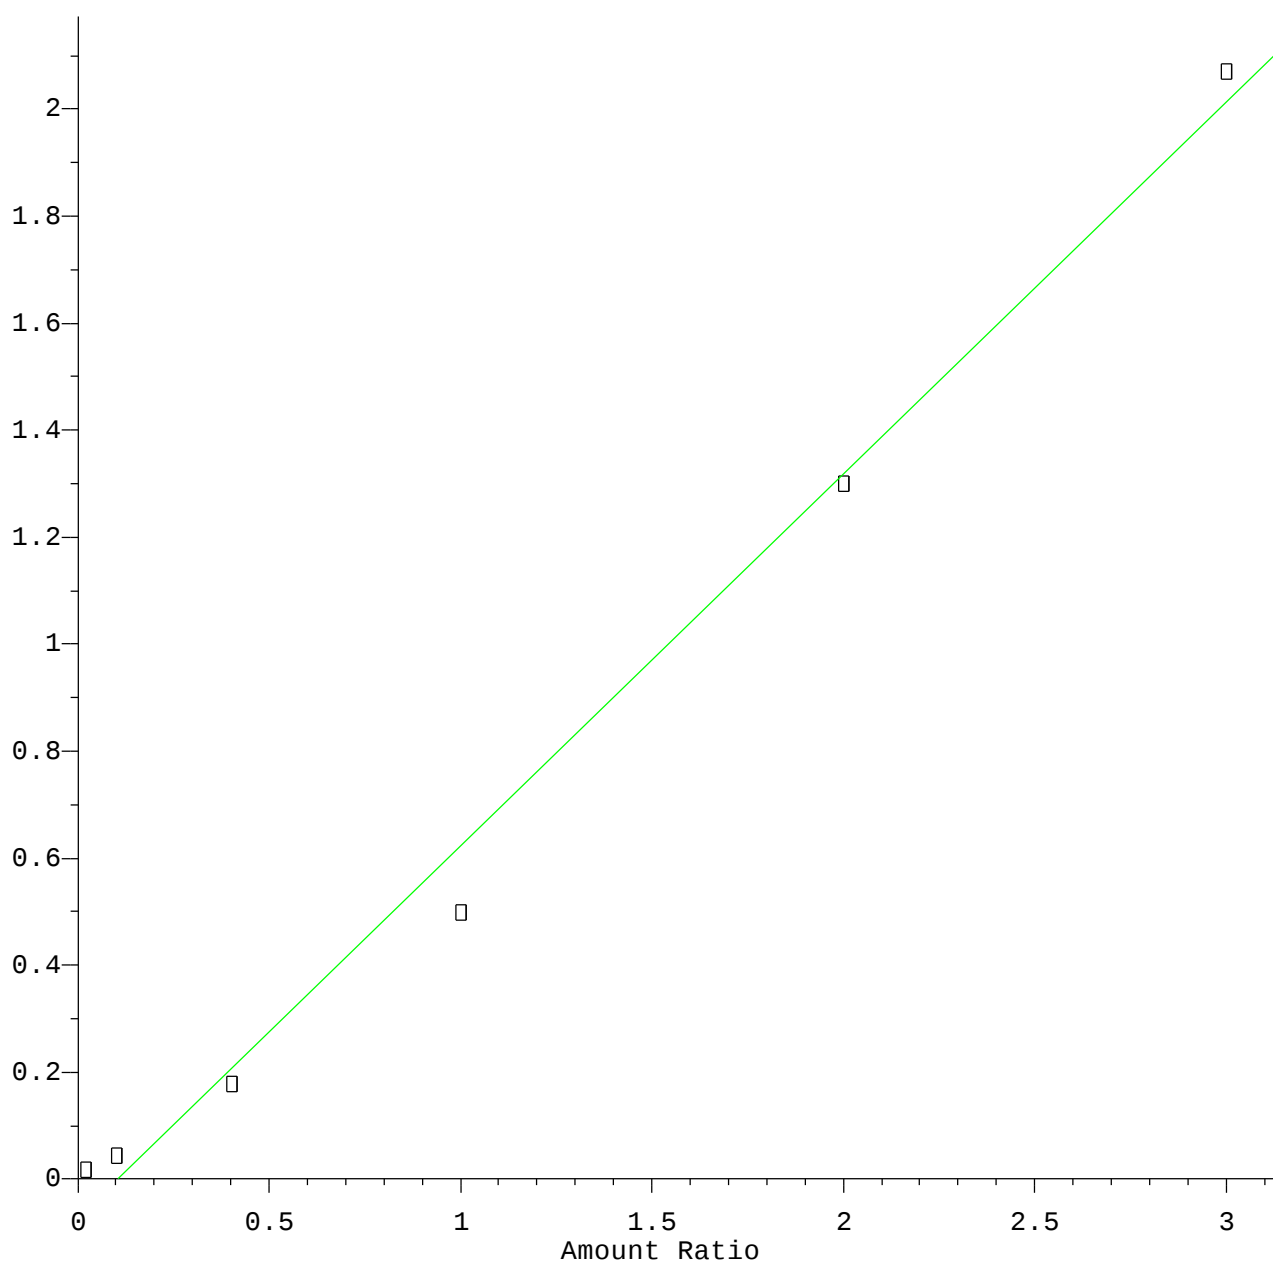

Resp Ratio = $6.94 \times 10^{-1} \times \text{Amt} - 7.10 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

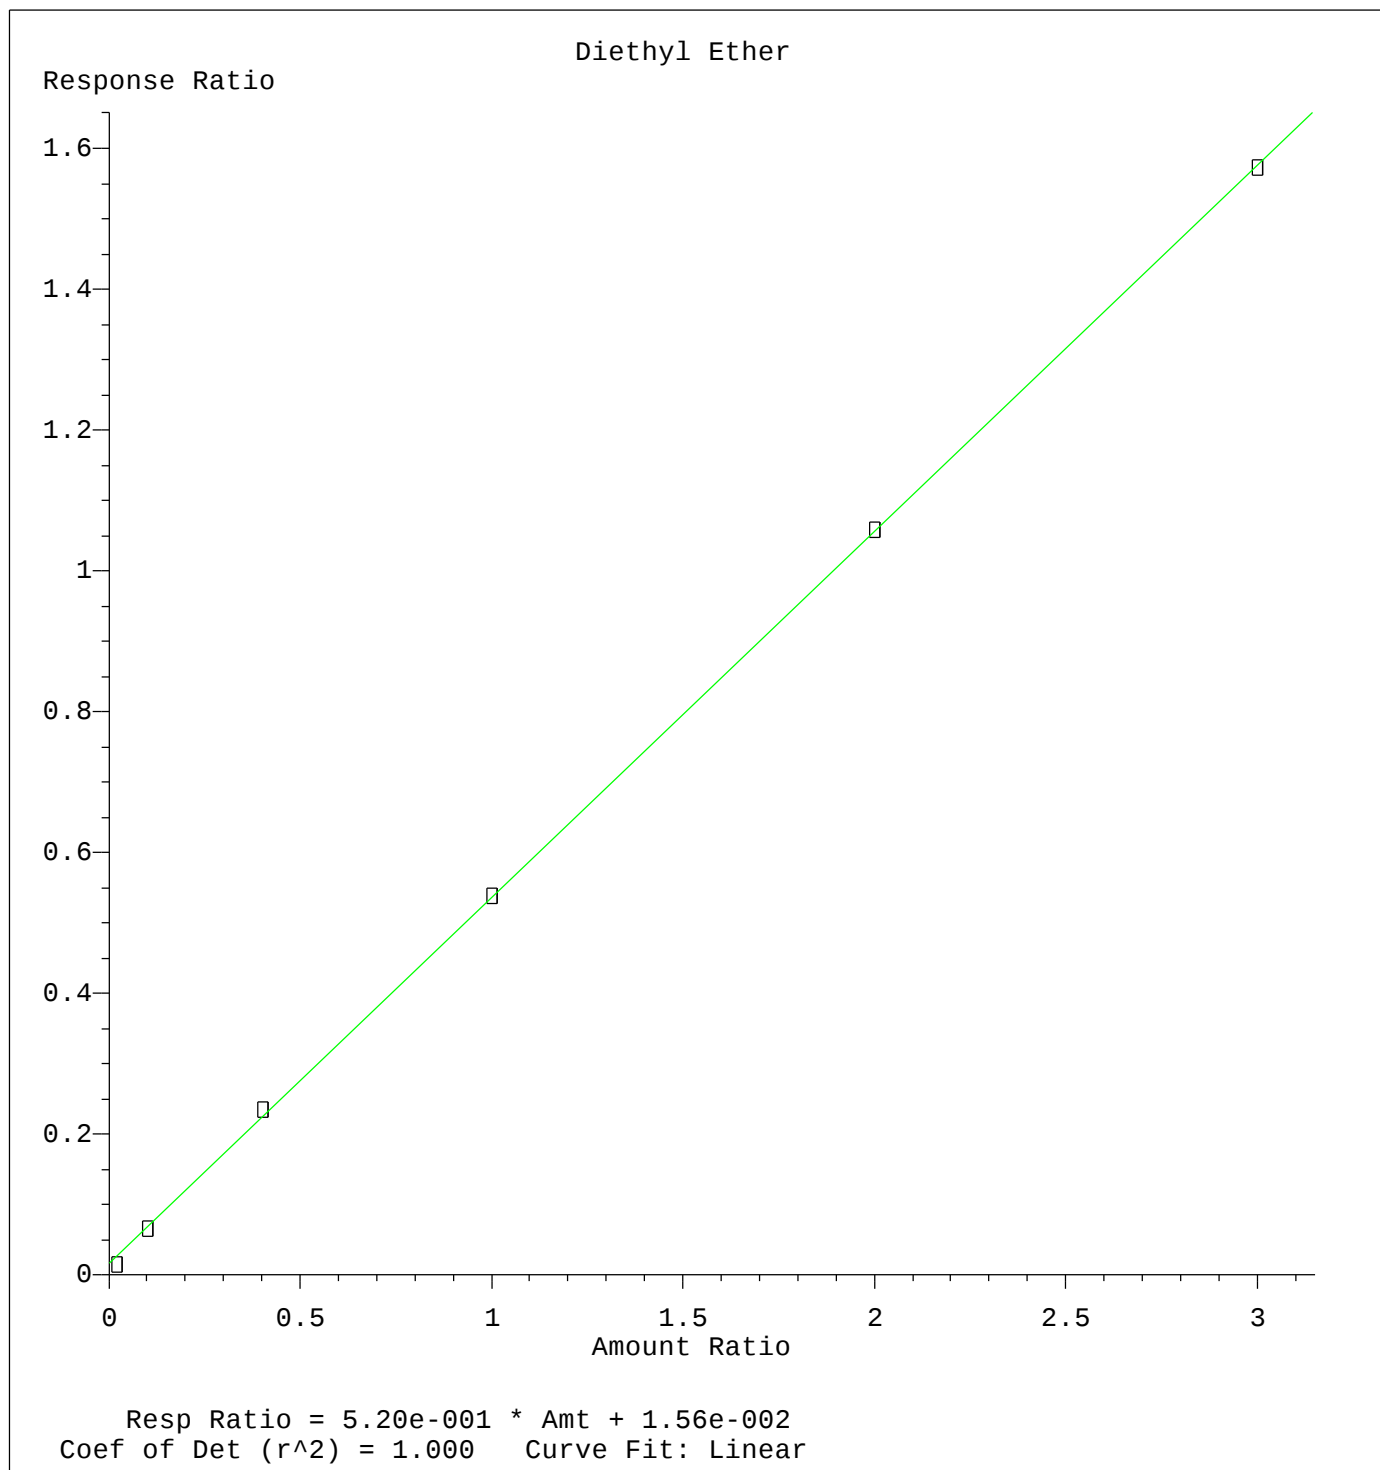

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019


1,1,2-Trichlorotrifluoroethane

Response Ratio

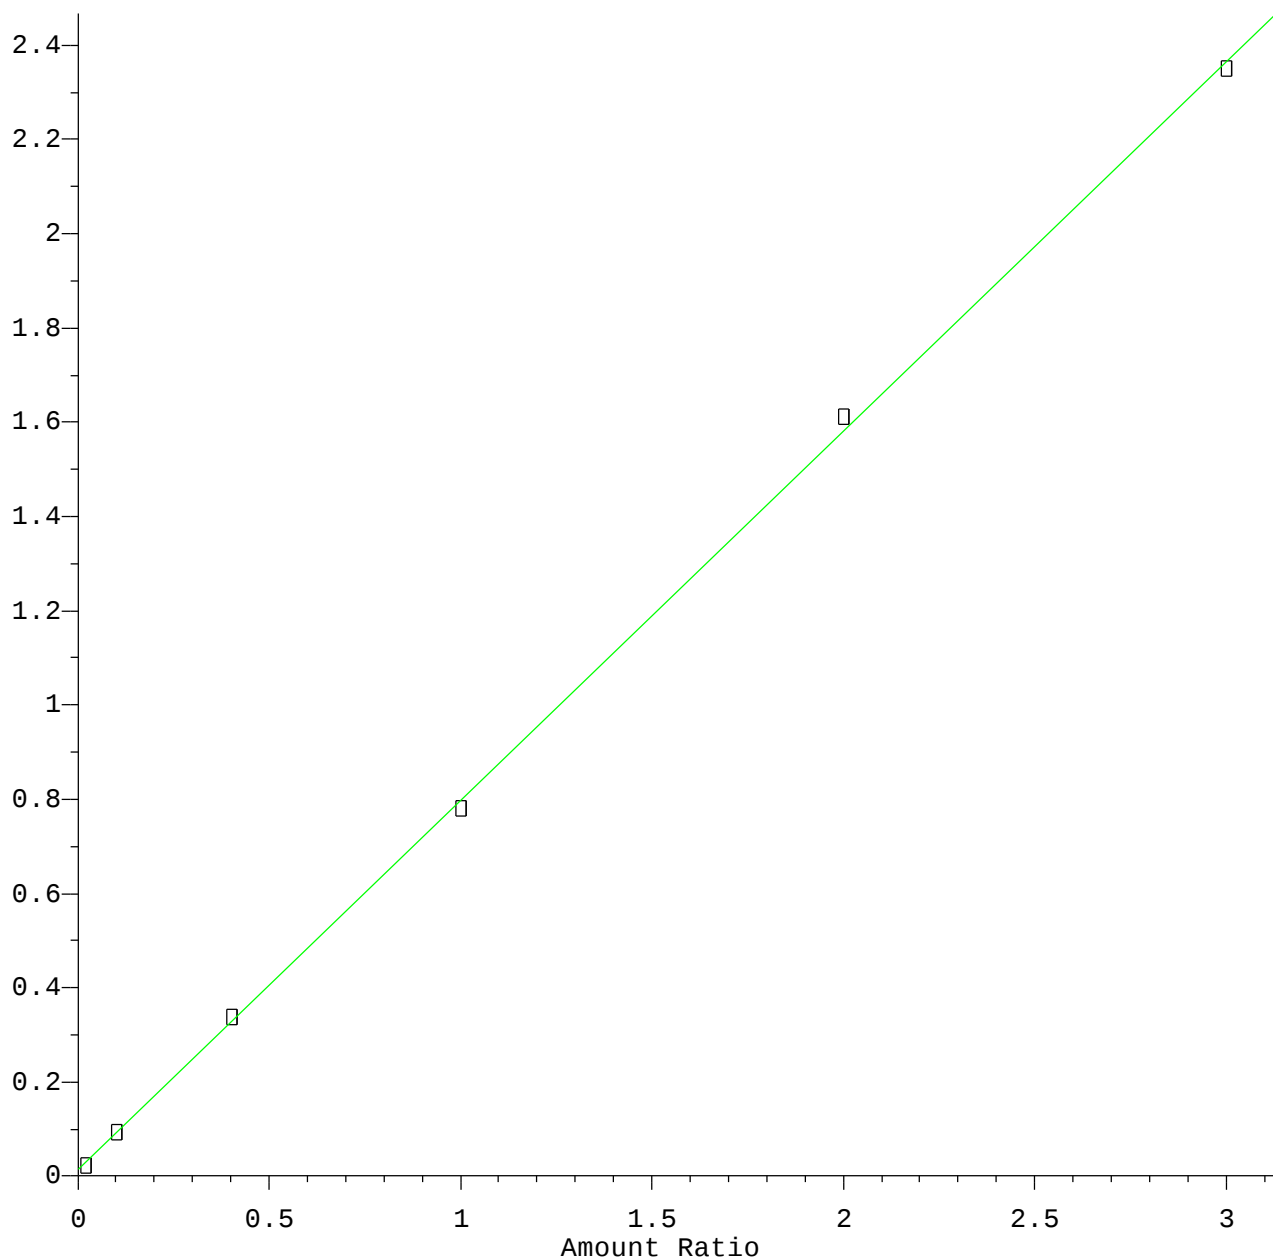


Resp Ratio = $7.83 \times 10^{-1} \times \text{Amt} + 1.38 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

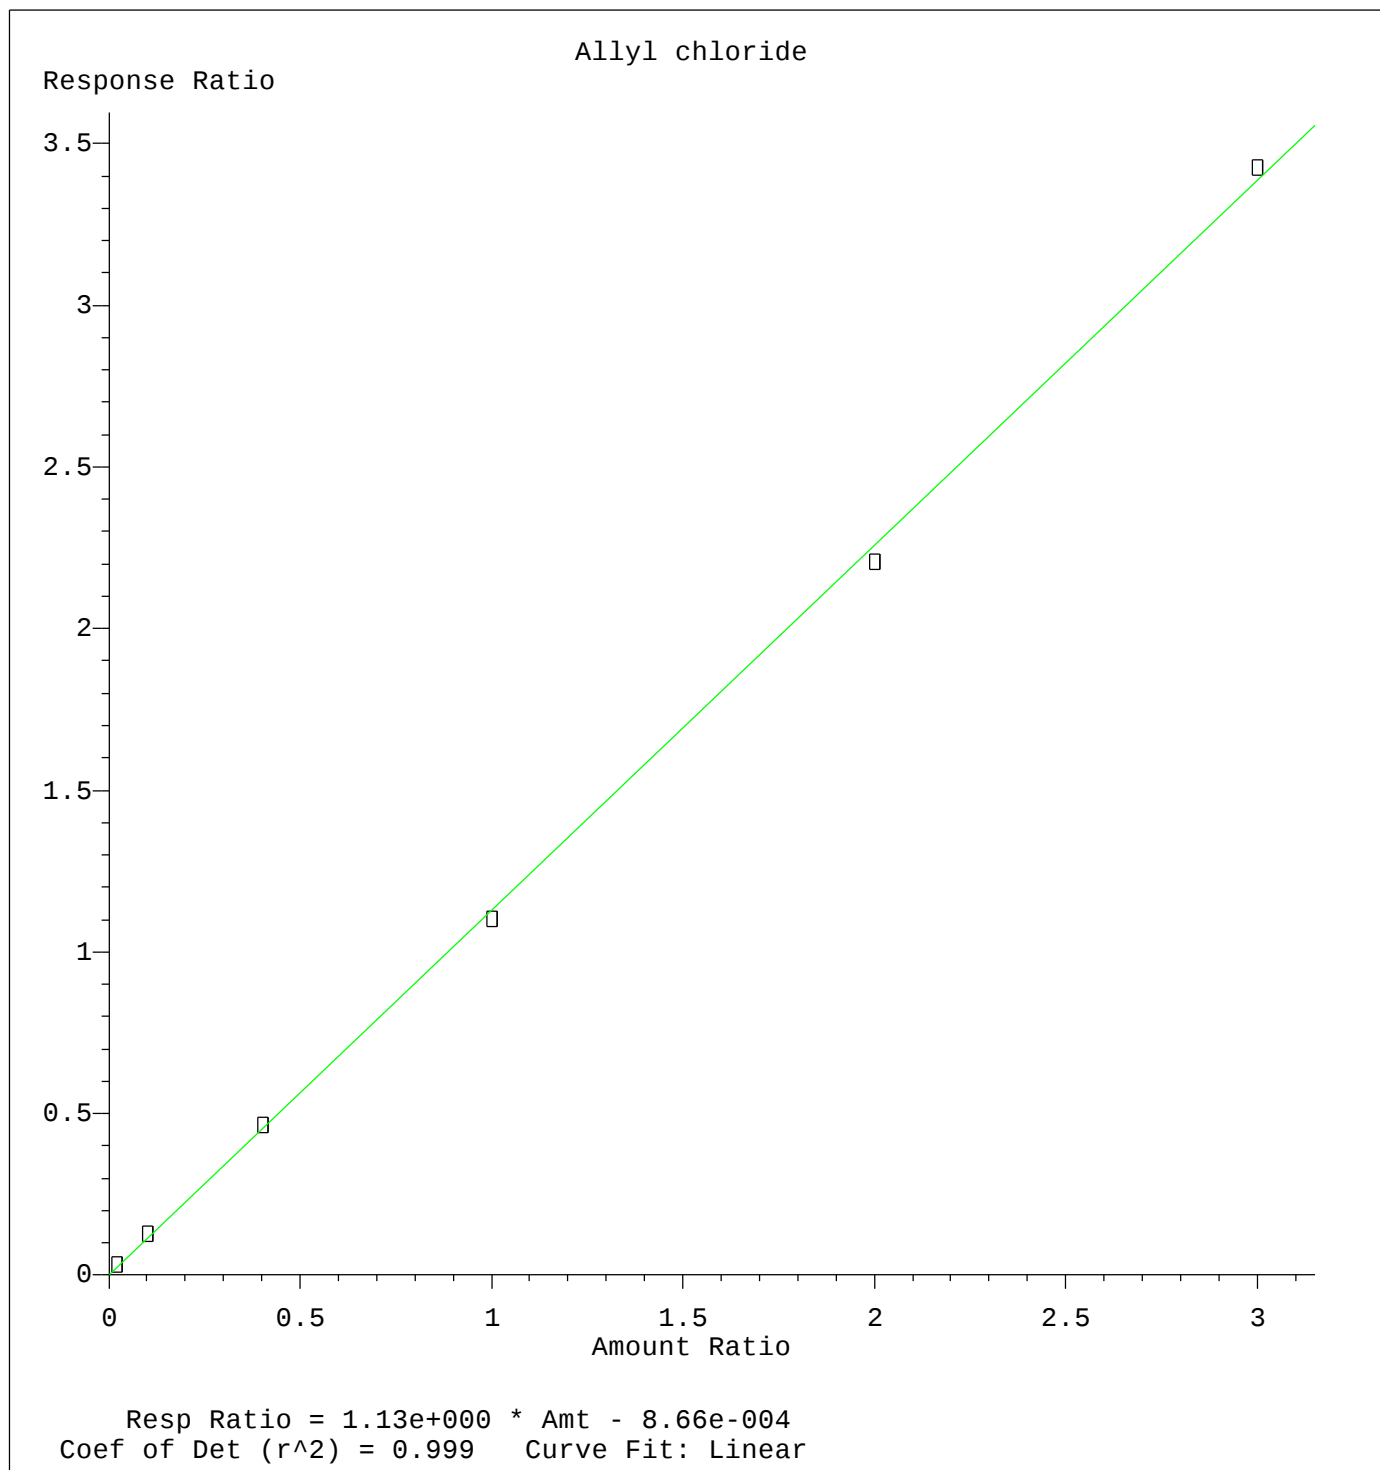


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

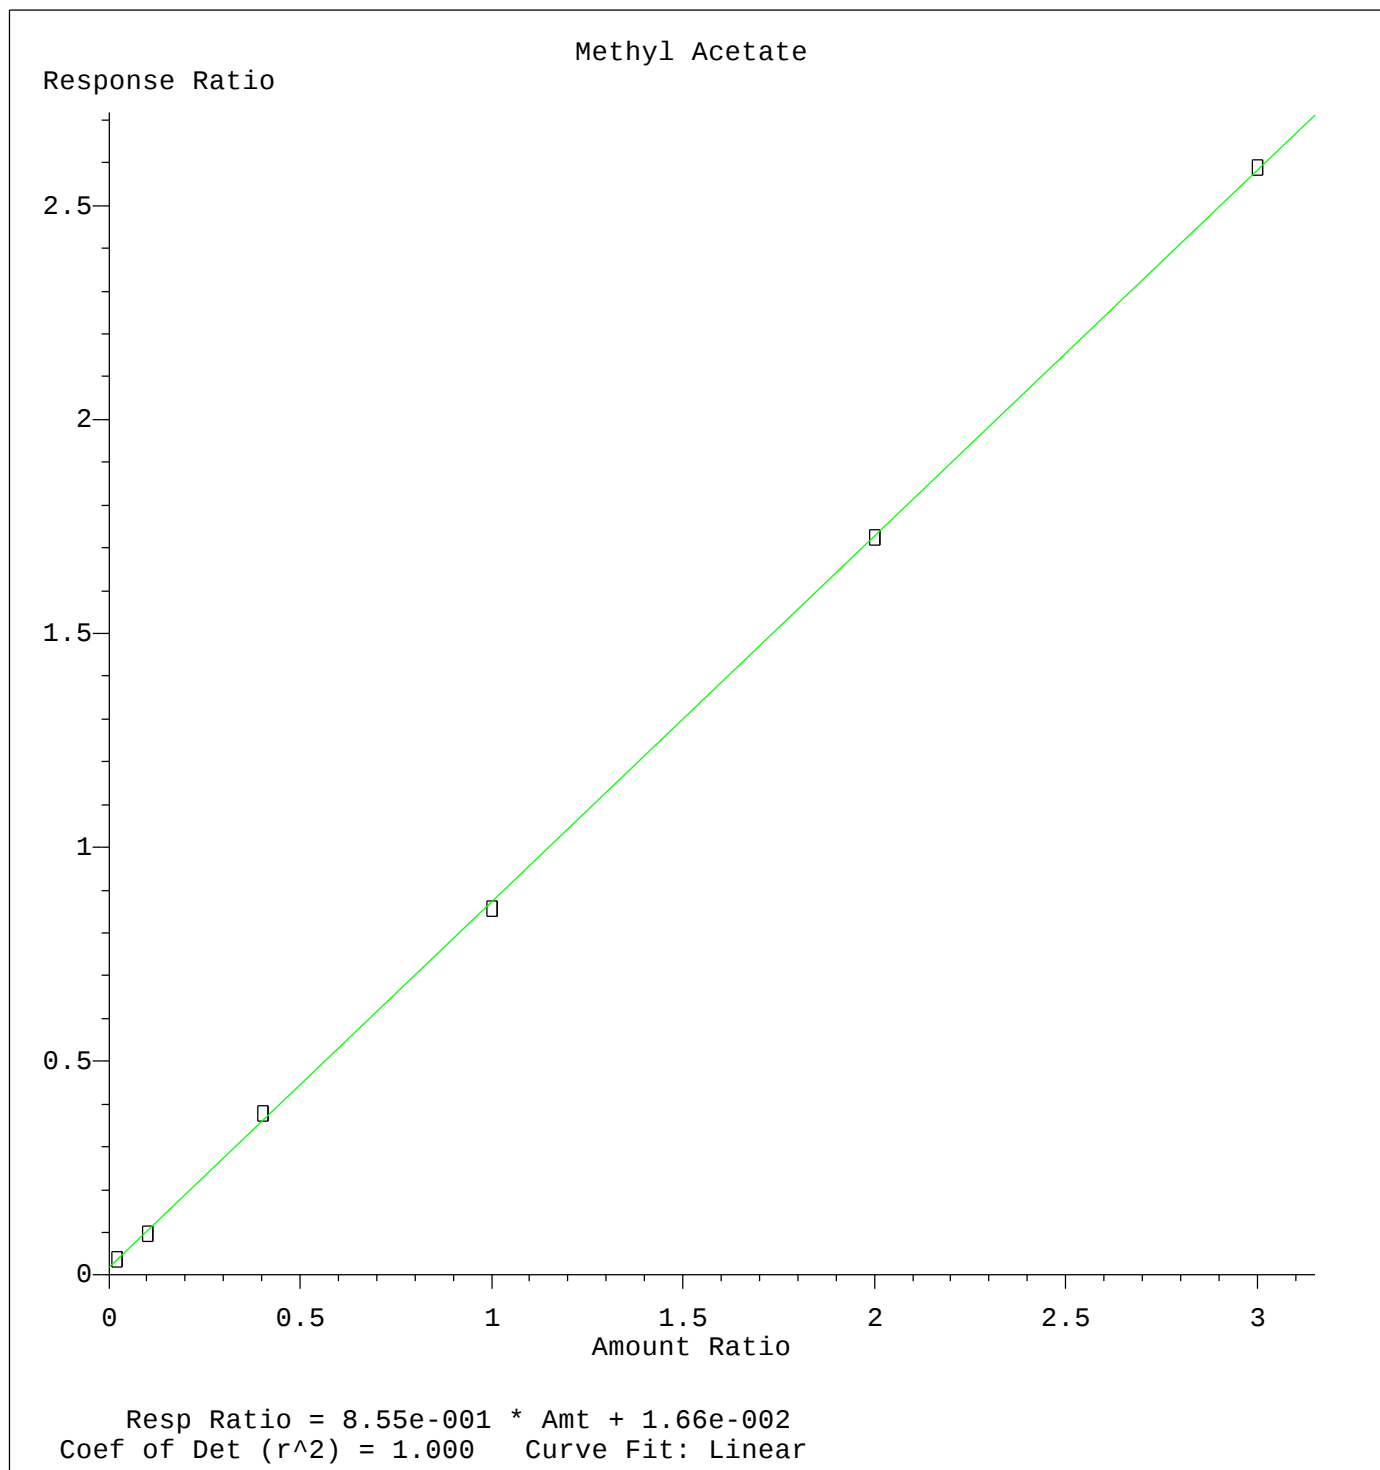

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019


Methylene Chloride

Response Ratio

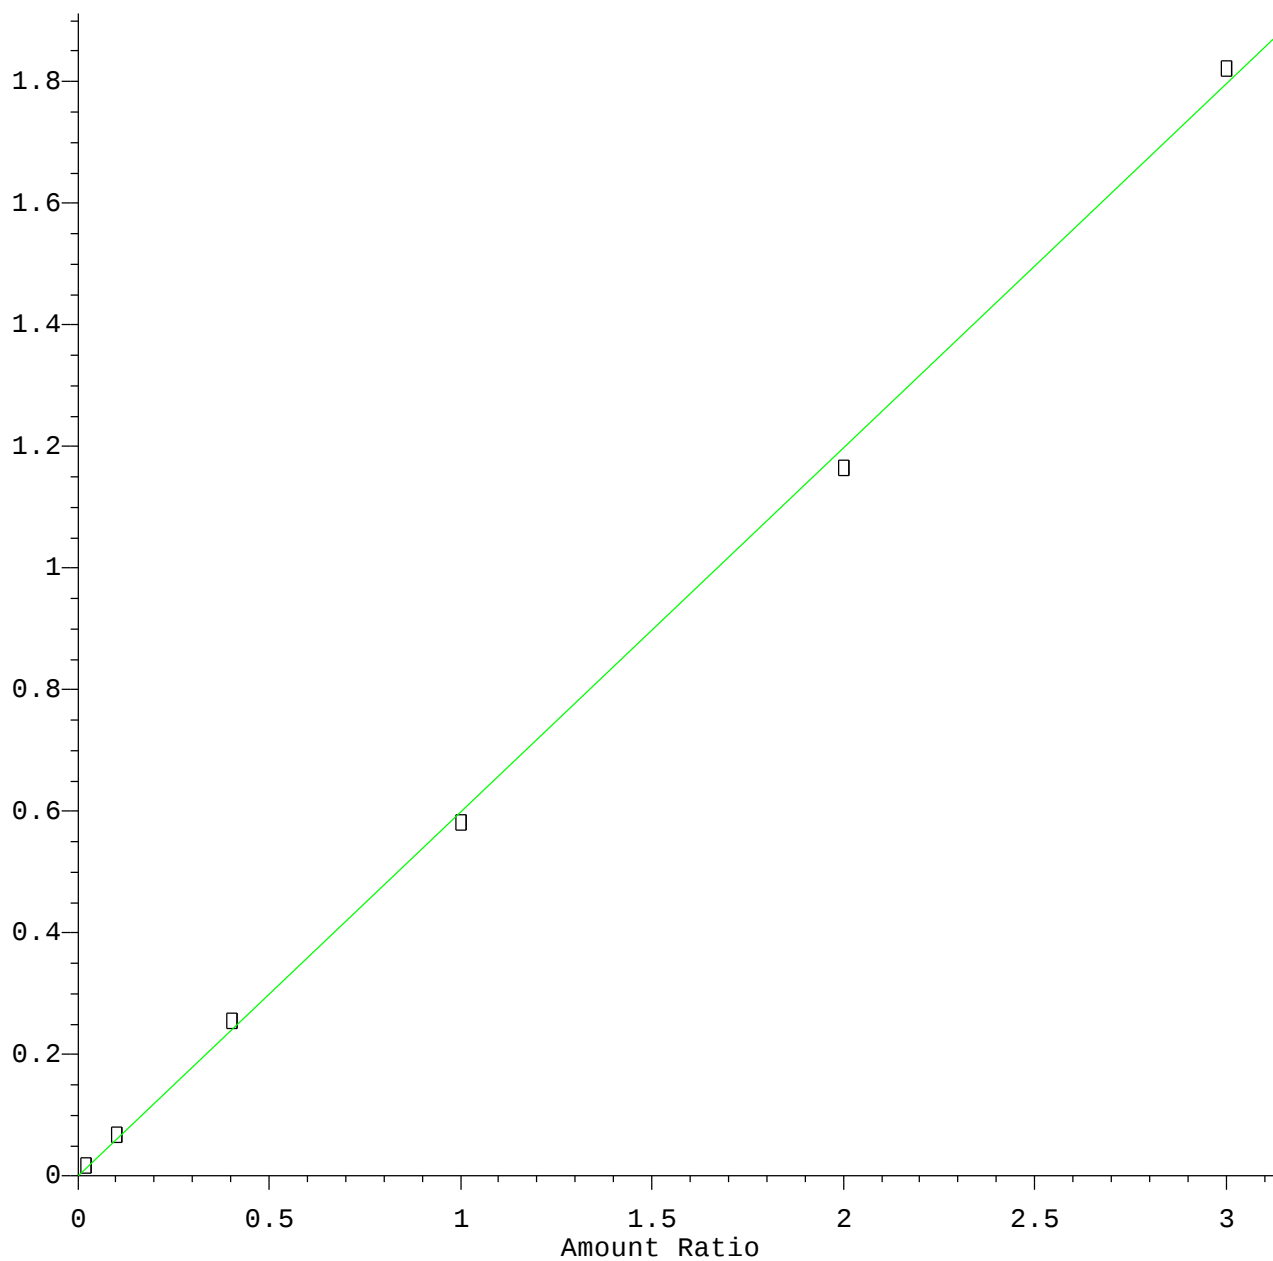


Resp Ratio = $5.98 \times 10^{-1} \times \text{Amt} + 8.97 \times 10^{-4}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

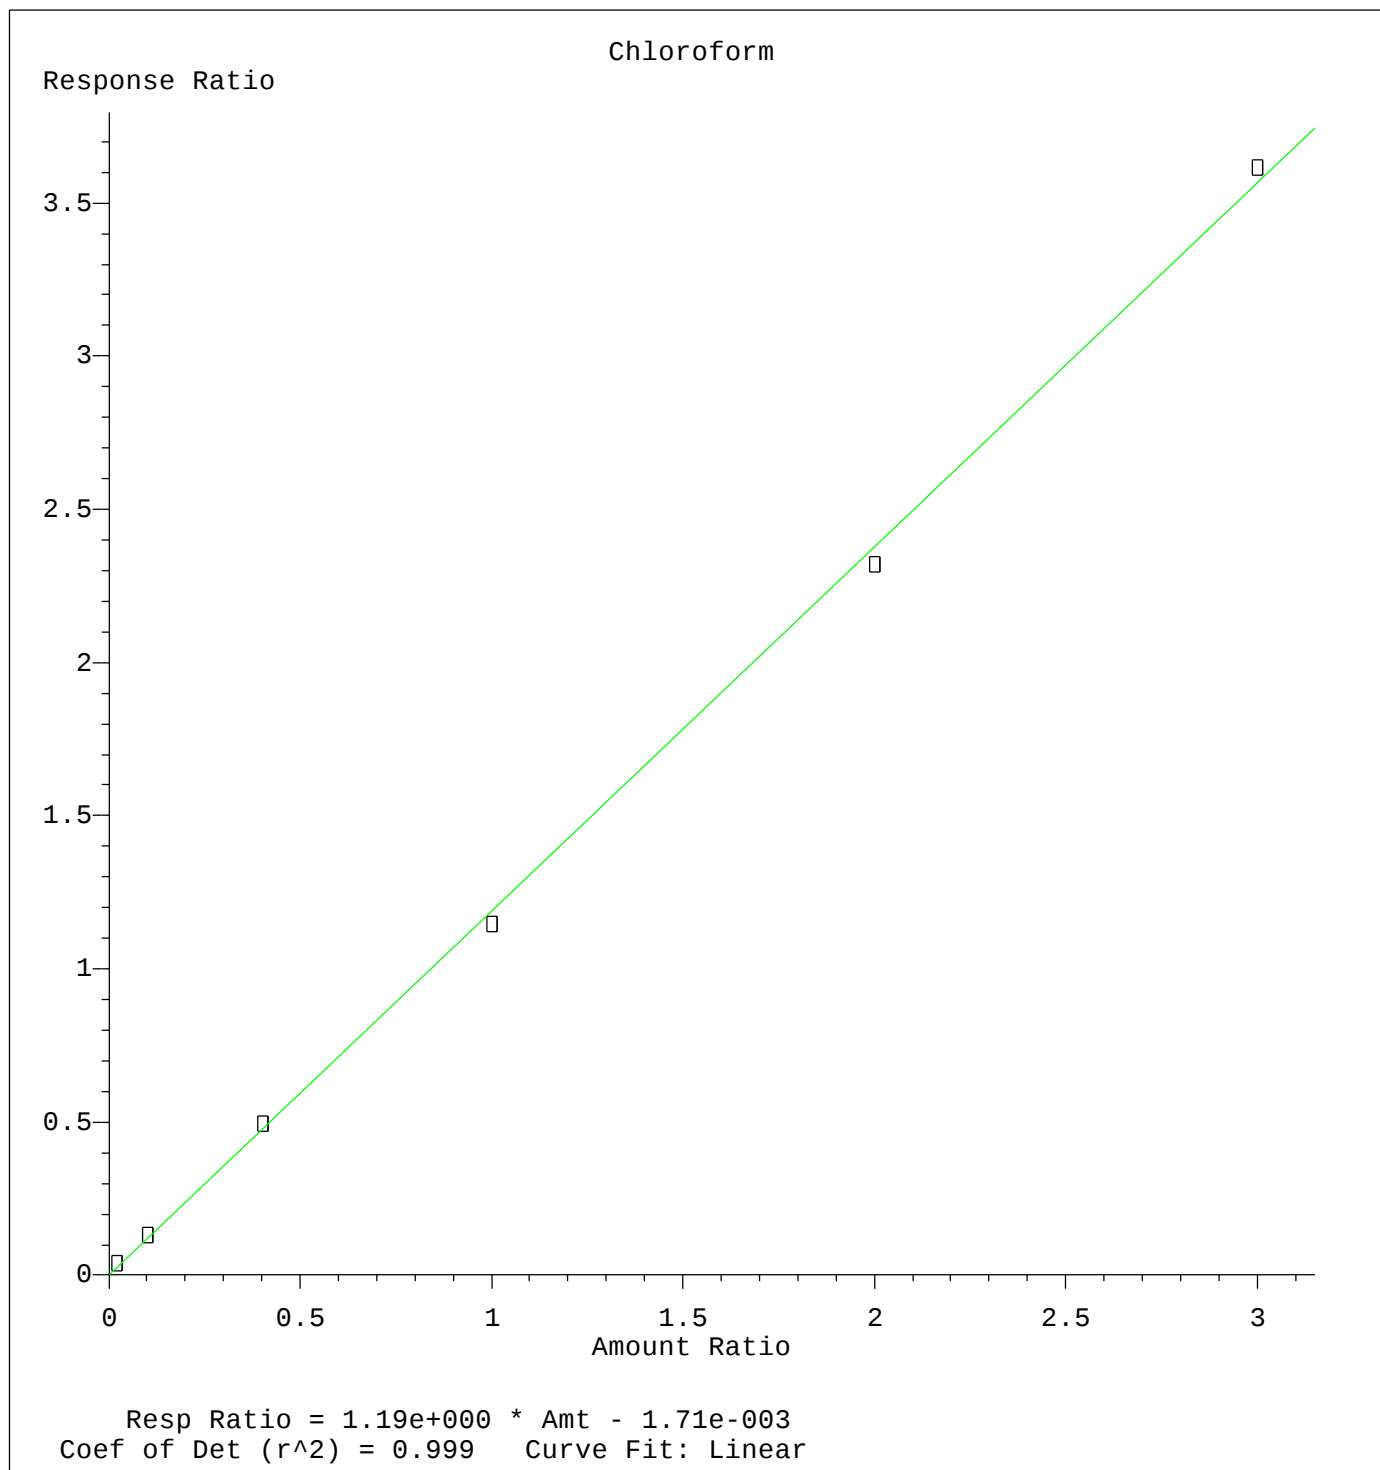


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

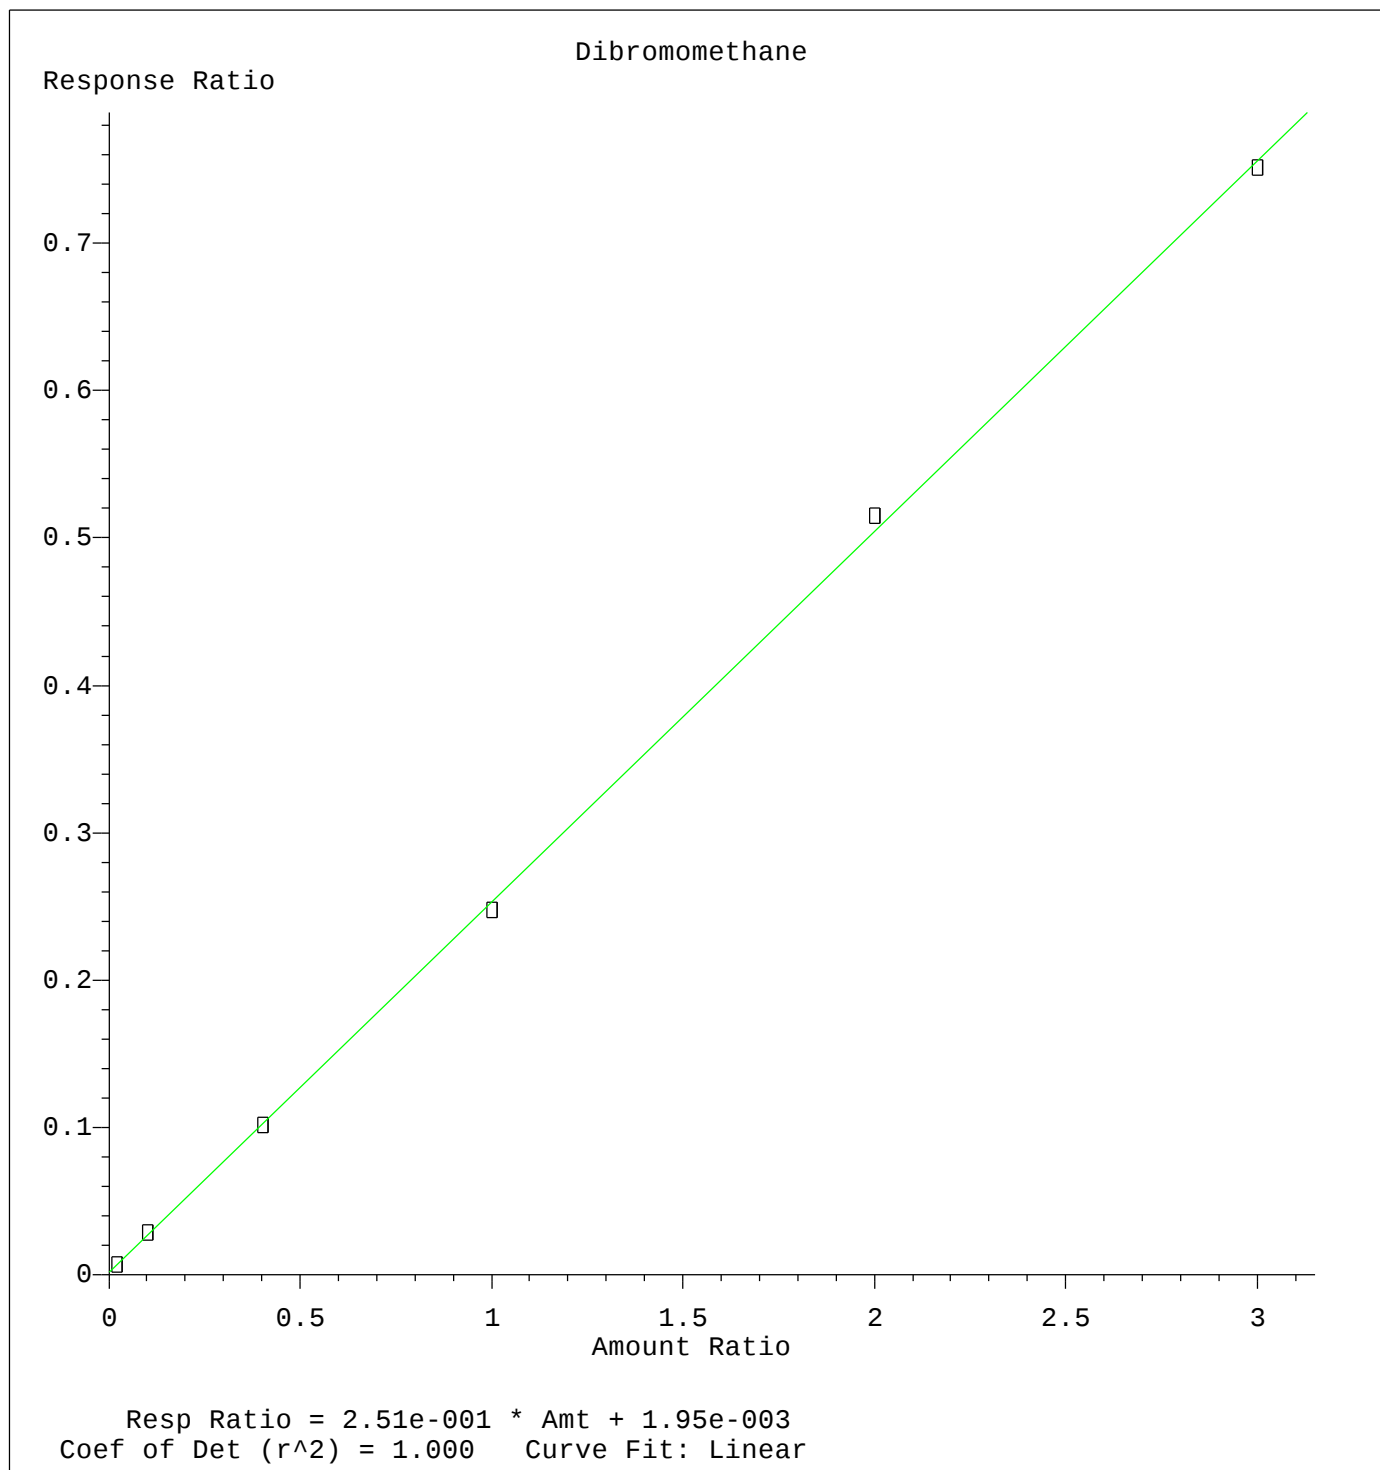

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

2-Chloroethyl Vinyl ether

Response Ratio

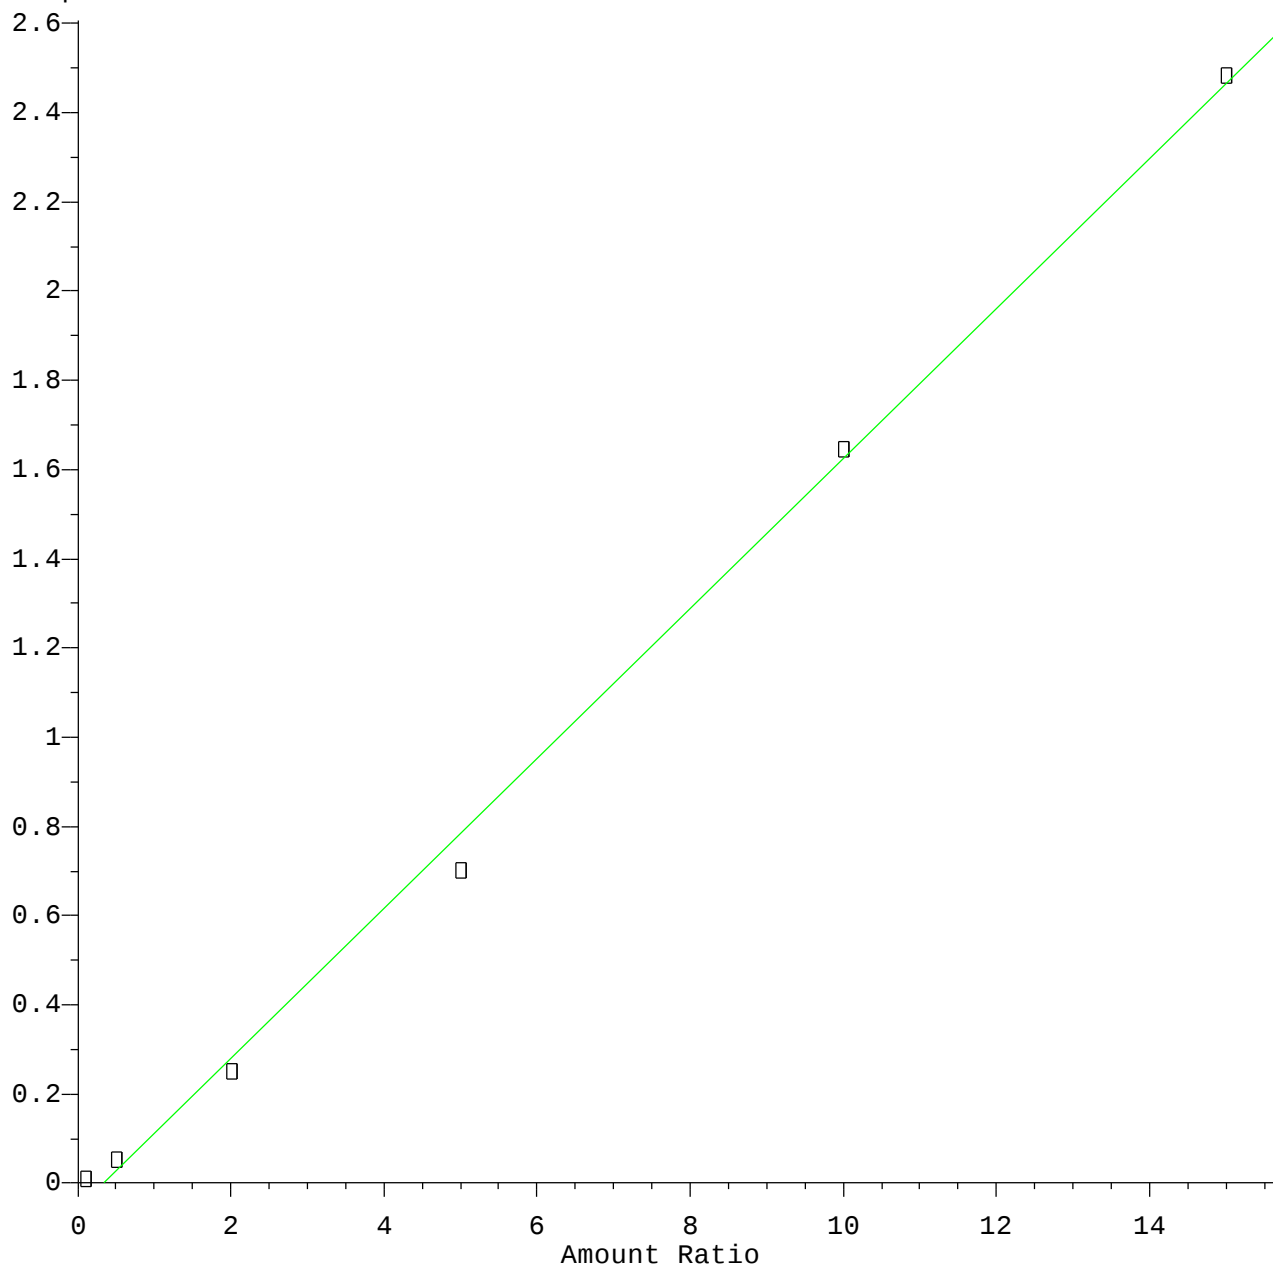


Resp Ratio = $1.68 \times 10^{-1} \times \text{Amt} - 5.74 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019


Isopropylbenzene

Response Ratio

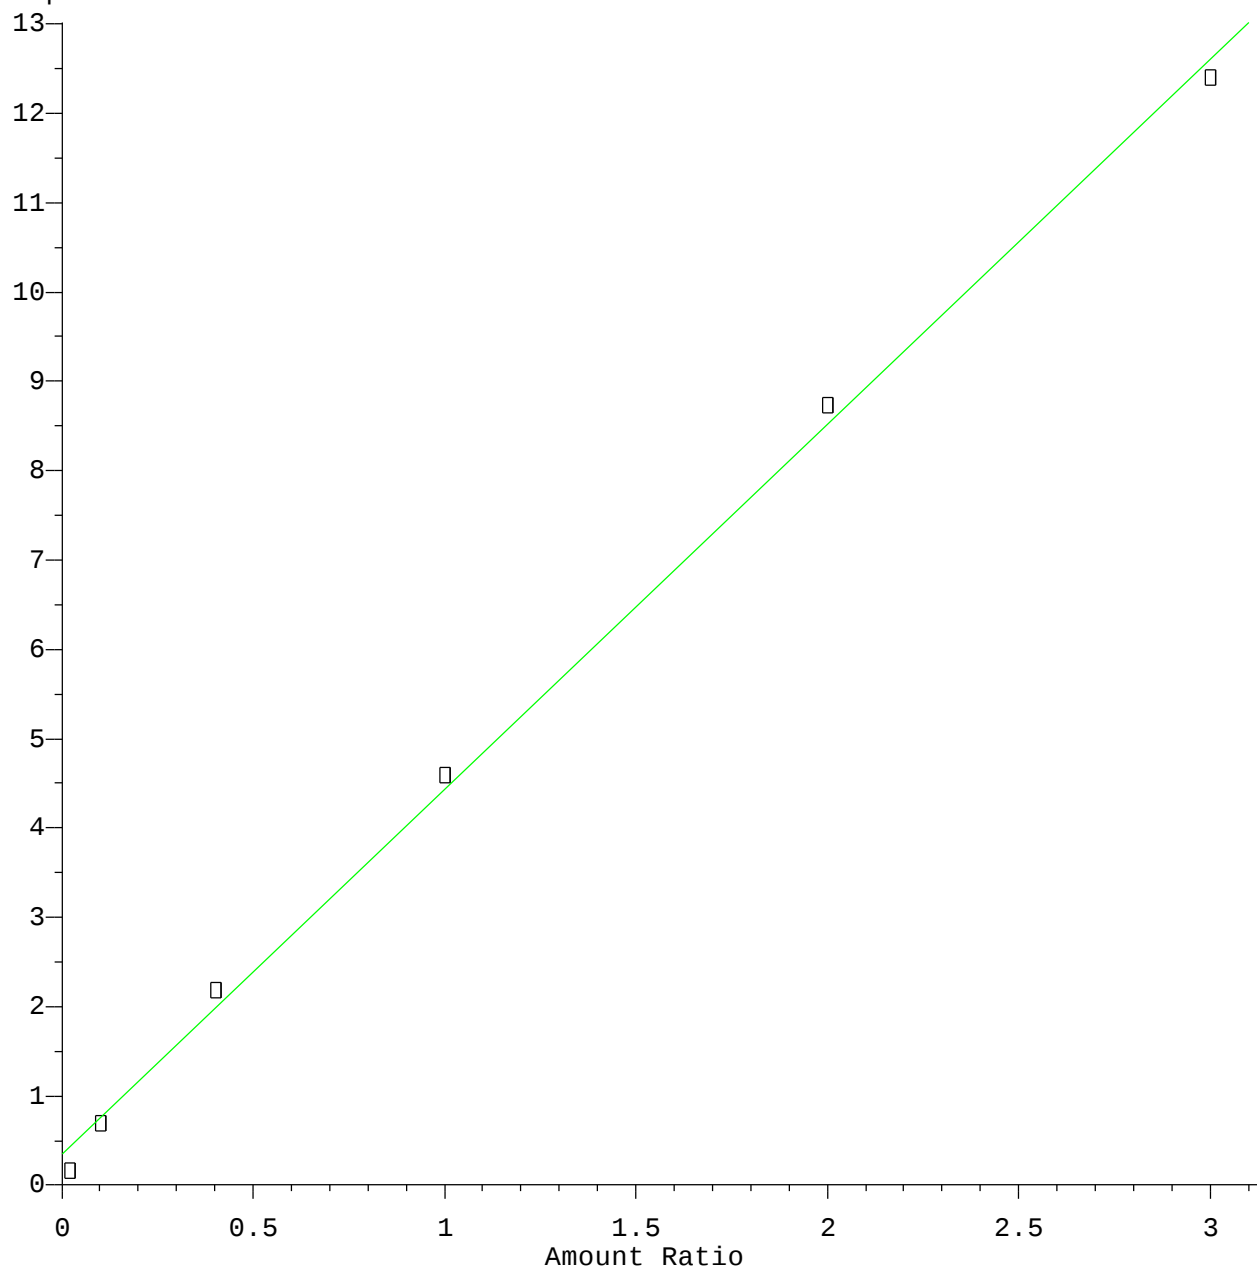

Resp Ratio = $4.09 \times 10^0 * \text{Amt} + 3.51 \times 10^{-1}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019

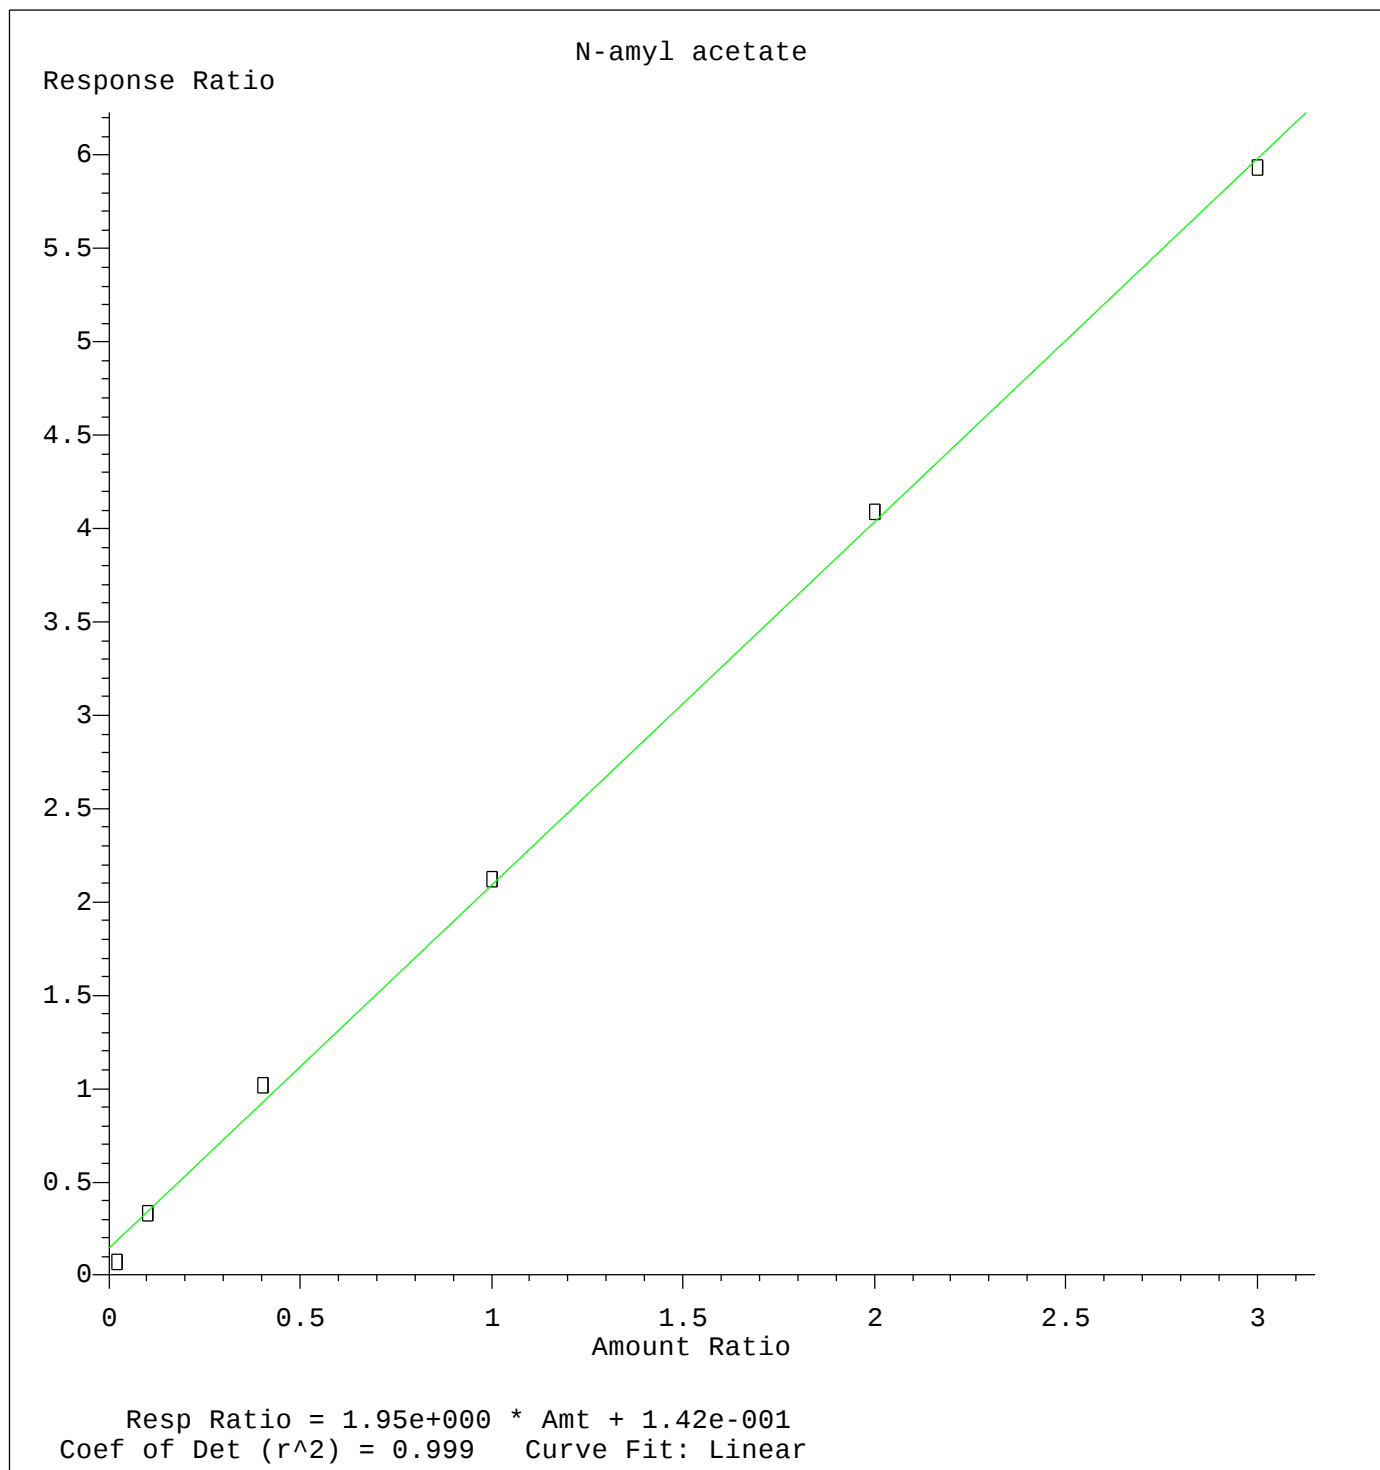

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Calibration Table Last Updated: Fri Aug 23 05:07:29 2019