
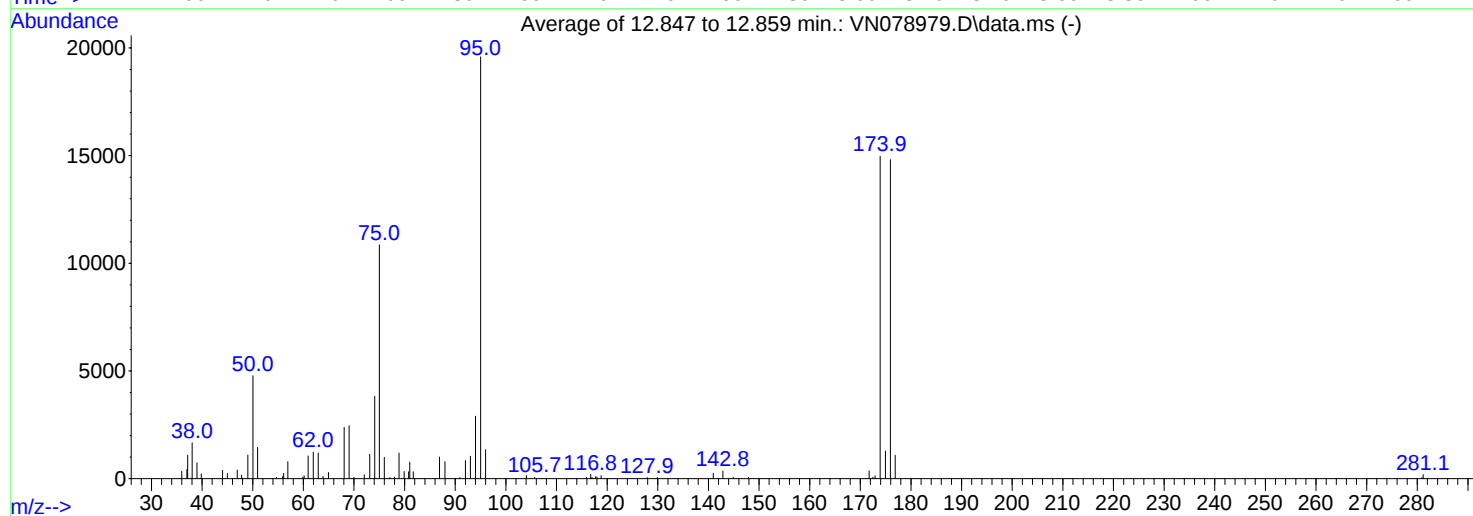


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082223\
Data File : VN078979.D
Acq On : 22 Aug 2023 08:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Title : SW846 8260
Last Update : Wed Aug 16 02:42:02 2023

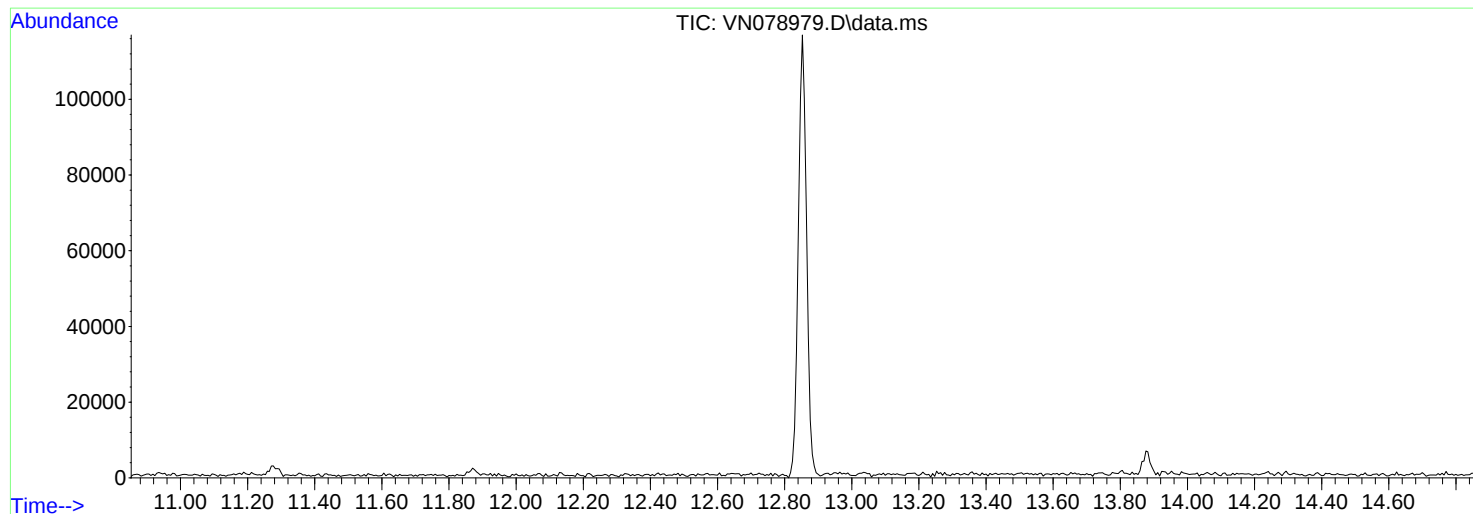

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.4	4776	PASS
75	95	30	60	55.4	10858	PASS
95	95	100	100	100.0	19589	PASS
96	95	5	9	6.9	1346	PASS
173	174	0.00	2	0.9	135	PASS
174	95	50	100	76.4	14973	PASS
175	174	5	9	8.6	1284	PASS
176	174	95	101	98.9	14812	PASS
177	176	5	9	7.3	1082	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	344	50.05	4776	63.90	106	78.00	74
37.00	422	50.95	1451	64.95	284	78.90	119
37.15	1095	54.70	57	68.05	2377	79.90	33
38.05	1664	55.90	96	69.05	2458	80.80	32
39.00	736	56.10	244	70.00	66	81.00	773
39.85	224	56.95	788	72.05	180	81.70	317
44.05	383	59.90	71	73.10	1129	86.90	1001
45.00	239	60.15	135	74.10	3827	87.95	788
46.95	399	60.95	1053	75.00	10858	90.90	54
47.80	161	61.95	1225	76.00	990	92.00	843
49.05	1089	62.95	1186	77.10	59	93.00	1041

Average of 12.847 to 12.859 min.: VN078979.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	2895	127.90	51	175.95	14812		
95.00	19589	129.90	51	176.90	1082		
96.00	1346	140.95	251	280.90	54		
104.05	145	142.85	359	281.15	187		
105.70	62	144.90	56				
115.90	57	147.90	54				
116.75	198	171.75	364				
117.00	56	172.50	64				
117.70	85	172.90	135				
118.00	79	173.90	14973				
118.80	145	174.95	1284				

Instrument :

MSVOA_N

ClientSampleId :

BFB