

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN082318\
 Data File : VN050841.D
 Acq On : 23 Aug 2018 10:15
 Operator : MD\SY
 Sample : J4581-15
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 24 01:07:28 2018
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 22 05:38:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	645493	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1015669	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	874131	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	276103	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	414957	53.40	ug/l	0.00
Spiked Amount			Recovery	=	106.80%	
35) Dibromofluoromethane	7.59	113	399018	49.38	ug/l	0.00
Spiked Amount			Recovery	=	98.76%	
50) Toluene-d8	10.09	98	1426396	47.22	ug/l	0.00
Spiked Amount			Recovery	=	94.44%	
62) 4-Bromofluorobenzene	12.40	95	370300	36.89	ug/l	0.00
Spiked Amount			Recovery	=	73.78%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.06	50	2810	0.26	ug/l	# 75
5) Bromomethane	2.57	94	3335	Below	Cal	97
10) Methyl Iodide	3.96	142	1192	6.49	ug/l	# 78
16) Acetone	3.83	43	4545	Below	Cal	93
17) Carbon Disulfide	4.05	76	5130	0.21	ug/l	# 86
18) Methyl Acetate	4.35	43	4178	0.57	ug/l	# 87
29) Tetrahydrofuran	7.23	42	860	0.48	ug/l	# 38
31) Cyclohexane	7.67	56	11243	1.31	ug/l	# 1
36) 1,1-Dichloropropene	7.67	75	43383	3.62	ug/l	# 48
38) Carbon Tetrachloride	7.67	117	57616	4.76	ug/l	# 18
43) Isopropyl Acetate	8.30	43	42698	3.61	ug/l	# 59
59) 2-Hexanone	10.76	43	1803	0.38	ug/l	# 44
70) Styrene	11.96	104	1067	1.31	ug/l	# 75
74) N-amyl acetate	12.07	43	1172	0.20	ug/l	# 48
75) 1,1,2,2-Tetrachloroethane	12.51	83	408	Below	Cal	# 89
76) 1,2,3-Trichloropropane	12.40	75	176968	36.59	ug/l	# 100
81) trans-1,4-Dichloro-2-buten	12.40	75	176968	123.71	ug/l	# 15
87) 1,3-Dichlorobenzene	13.28	146	2224	0.21	ug/l	93
88) 1,4-Dichlorobenzene	13.28	146	2224	0.21	ug/l	94
91) 1,2-Dichlorobenzene	13.66	146	2202	0.22	ug/l	95
93) 1,2,4-Trichlorobenzene	14.91	180	2787	4.57	ug/l	96
94) Hexachlorobutadiene	15.01	225	1567	Below	Cal	91
95) Naphthalene	15.14	128	5948	5.88	ug/l	# 96
96) 1,2,3-Trichlorobenzene	15.31	180	2788	3.82	ug/l	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN082318\
Data File : VN050841.D
Acq On : 23 Aug 2018 10:15
Operator : MD\SY
Sample : J4581-15
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 24 01:07:28 2018
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 22 05:38:12 2018
Response via : Initial Calibration

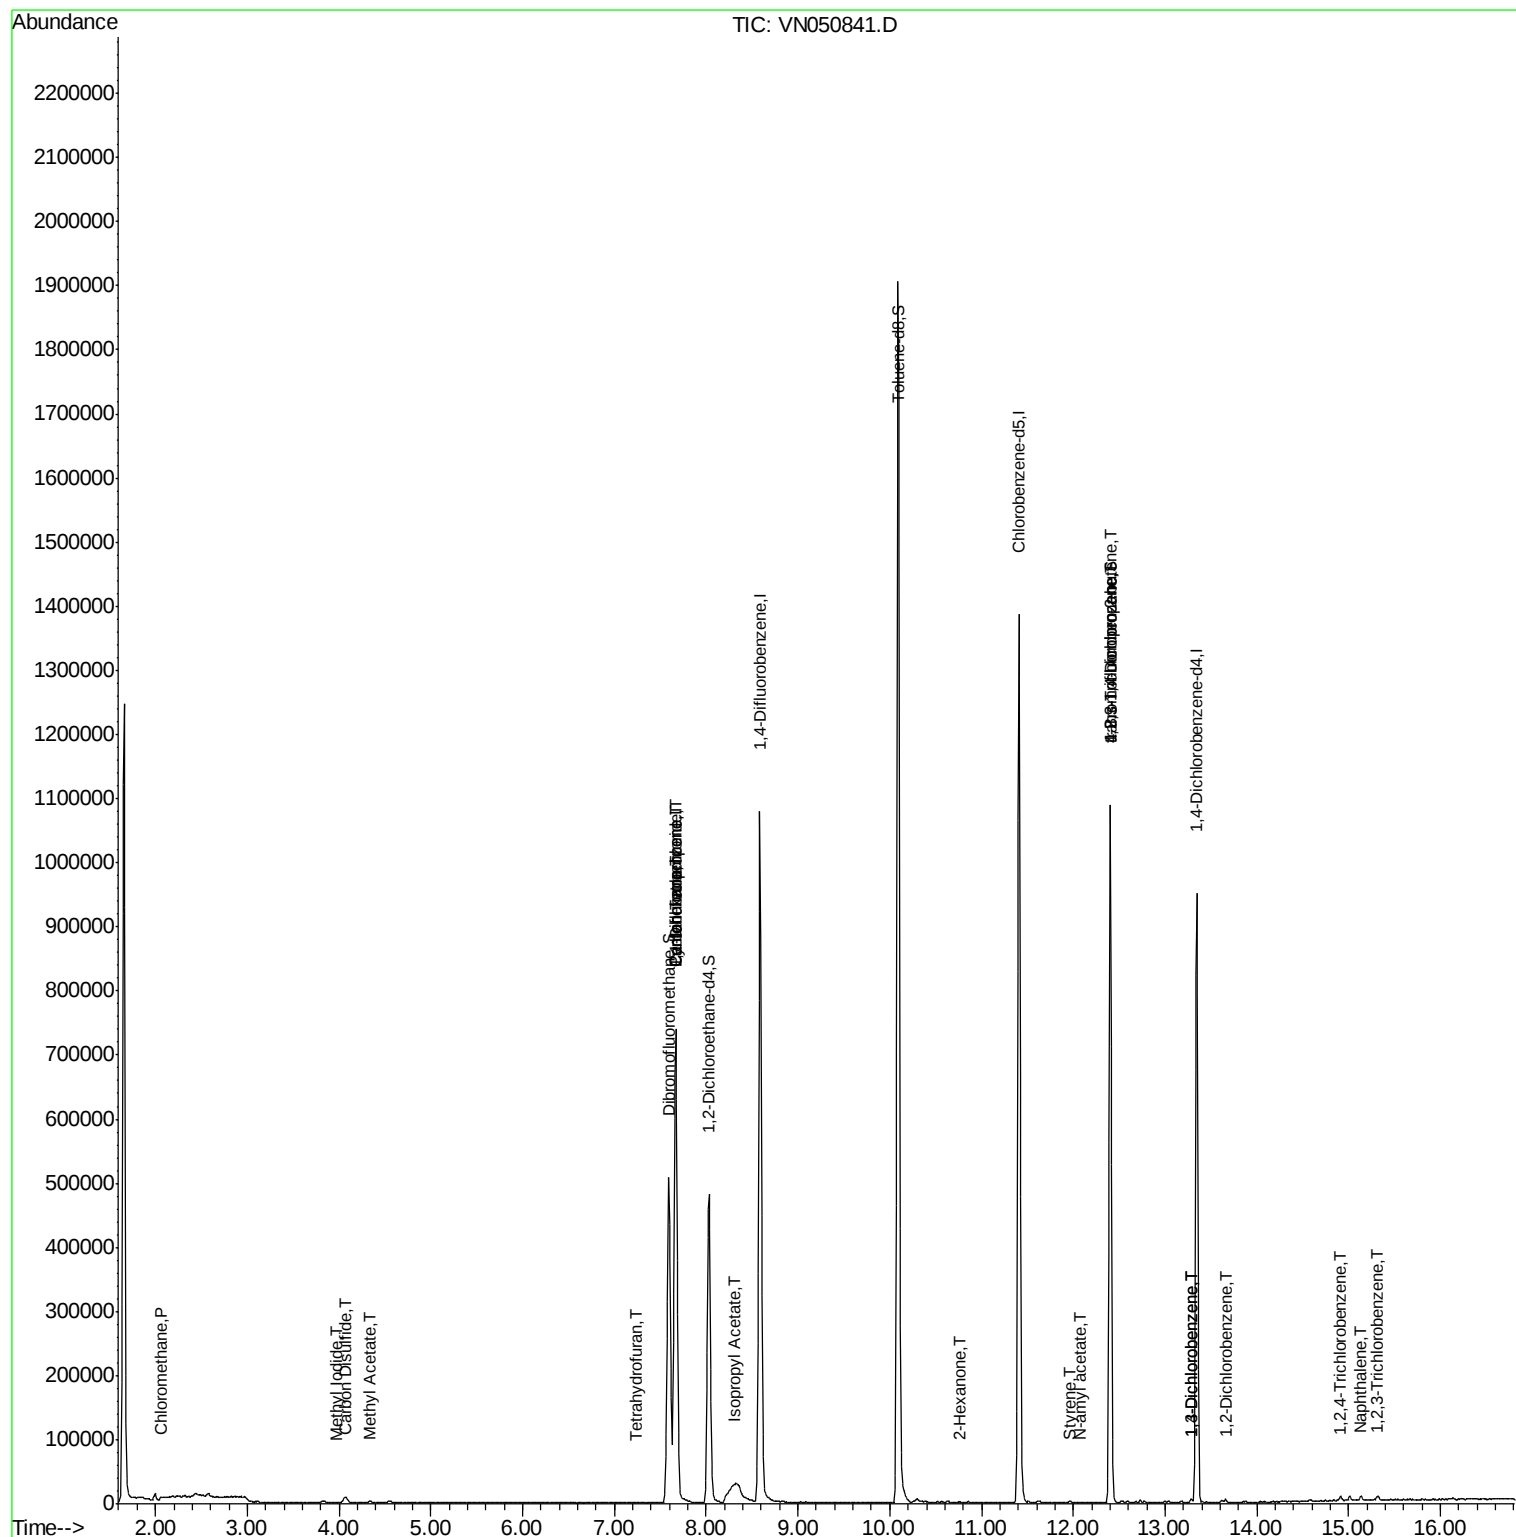



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1890

Delta R.T. 0.00 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15


Instrument :
MSVOA_N
ClientSampleId :

Tot Ion:168 Resp: 645493

Ion Ratio Lower Upper

168 100

99 50.7 39.6 59.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.67

250000

200000



150000

100000

50000

0

Time-->



#3

Chloromethane

Concen: 0.26 ug/l

RT: 2.06 min Scan# 145

Delta R.T. 0.00 min

Lab File: VN050841.D


Acq: 23 Aug 2018 10:15

Tgt Ion: 50 Resp: 2810

Ion Ratio Lower Upper

50 100

52 46.9 26.3 39.5#



Abundance Ion 49.90 (49.60 to 50.60): VNO

Ion 51.90 (51.60 to 52.60): VN

2000


1500


1000

500

0

Time-->





#5

Bromomethane

Concen: Below Cal

RT: 2.57 min Scan# 306

Delta R.T. 0.01 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 94 Resp: 3335

Ion Ratio Lower Upper




94 100

96 98.0 76.2 114.2

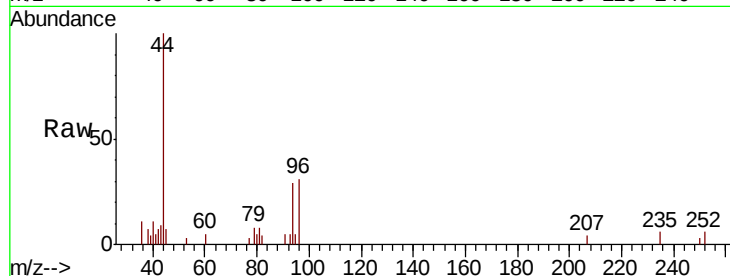

Abundance Ion 93.90 (93.60 to 94.60): VN050782.D (-284) (-)

Ion 95.90 (95.60 to 96.60): VN050782.D (-284) (-)

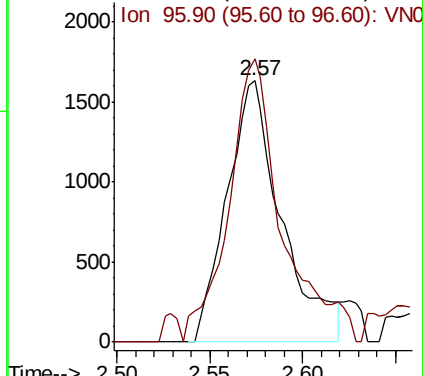

#10

Methyl Iodide

Concen: 6.49 ug/l

RT: 3.96 min Scan# 738

Delta R.T. 0.01 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15


Tgt Ion: 142 Resp: 1192

Ion Ratio Lower Upper

142 100

127 29.2 31.7 47.5#



141 0.0 11.4 17.0#



Abundance Ion 141.80 (141.50 to 142.50): VN050782.D (-713) (-)

Ion 126.80 (126.50 to 127.50): VN050782.D (-713) (-)

Ion 140.80 (140.50 to 141.50): VN050782.D (-713) (-)

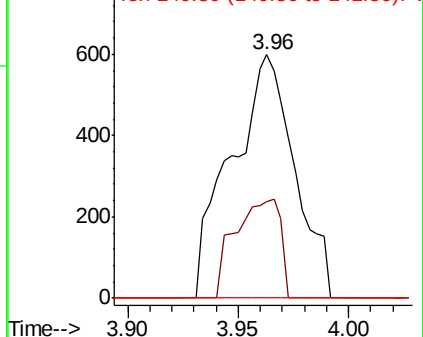



#16

Acetone

Concen: Below Cal

RT: 3.83 min Scan# 696

Delta R.T. 0.01 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15

Instrument :

MSVOA_N





ClientSampled :

Tot Ion: 43 Resp: 4545

Ion Ratio Lower Upper

43 100

58 29.9 27.2 40.8

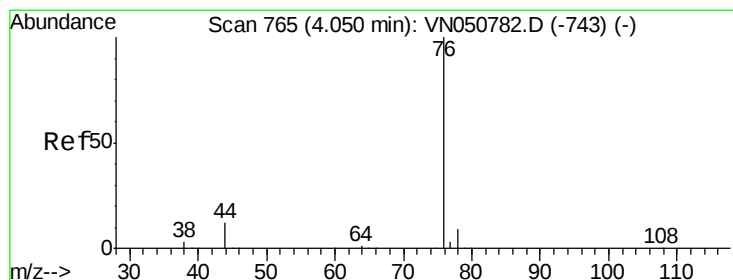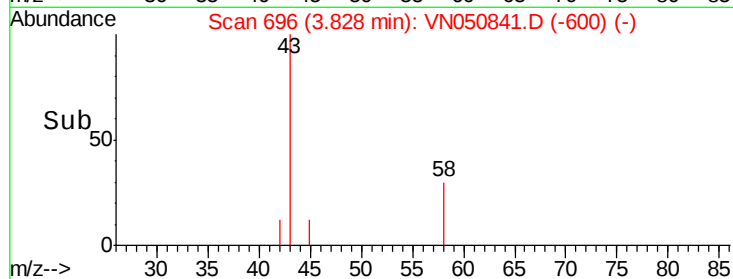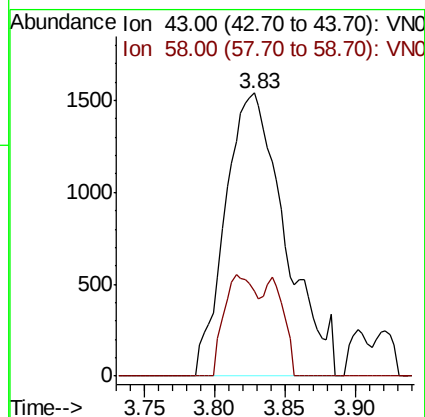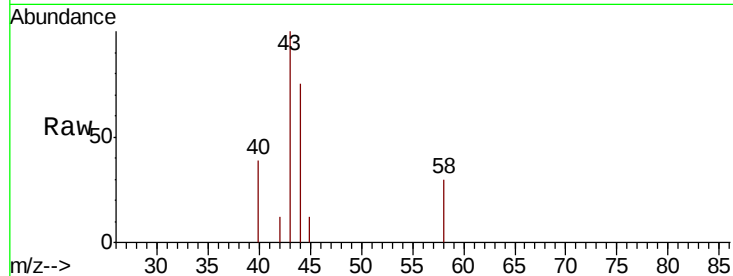

#17

Carbon Disulfide

Concen: 0.21 ug/l

RT: 4.05 min Scan# 766

Delta R.T. 0.00 min

Lab File: VN050841.D




Acq: 23 Aug 2018 10:15


Tgt Ion: 76 Resp: 5130

Ion Ratio Lower Upper

76 100

78 14.1 7.3 10.9#


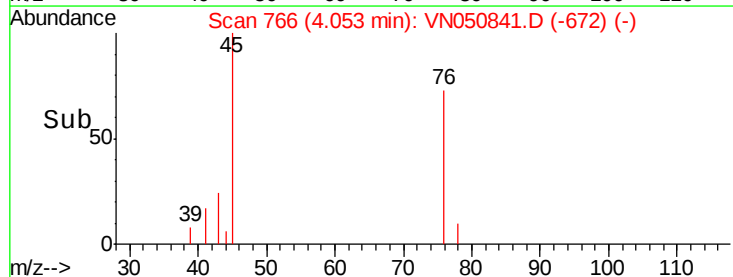
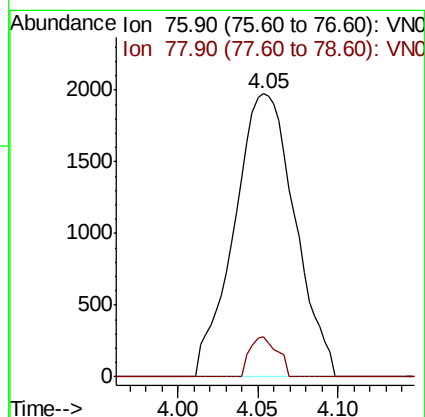
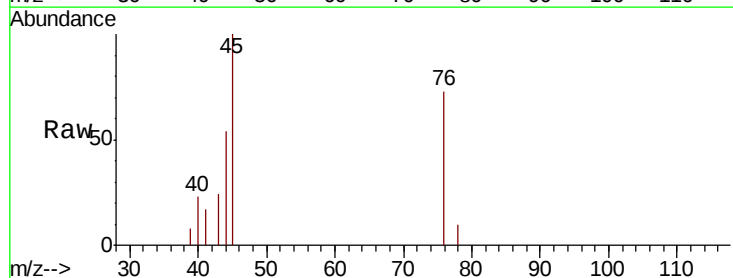


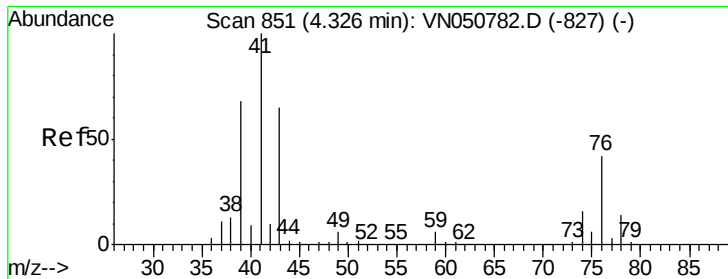

#18
Methvl Acetate
Concen: 0.57 ug/l
RT: 4.35 min Scan# 857
Delta R.T. 0.02 min
Lab File: VN050841.D
Acq: 23 Aug 2018 10:15




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 43 Resp: 4178
Ion Ratio Lower Upper
43 100
74 18.4 19.8 29.8#

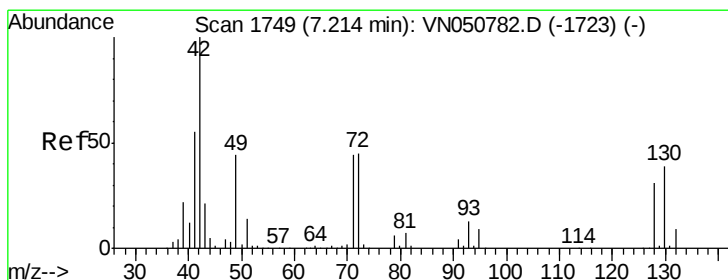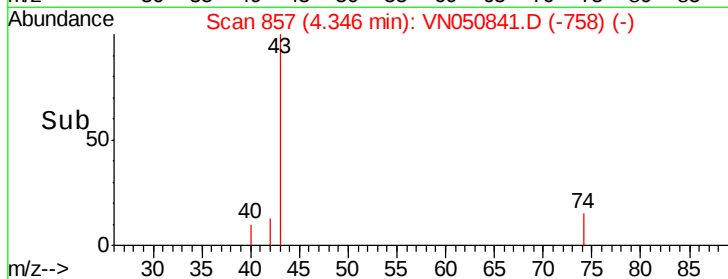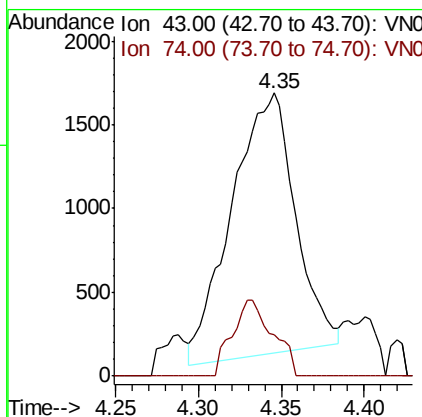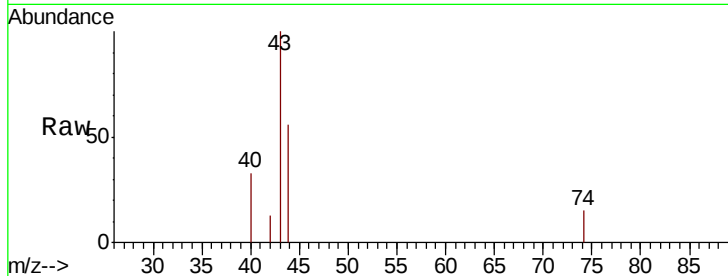

#29
Tetrahydrofuran
Concen: 0.48 ug/l
RT: 7.23 min Scan# 1753
Delta R.T. 0.01 min
Lab File: VN050841.D
Acq: 23 Aug 2018 10:15

Tgt Ion: 42 Resp: 860
Ion Ratio Lower Upper
42 100
72 3.4 35.5 53.3#
71 3.4 33.7 50.5#

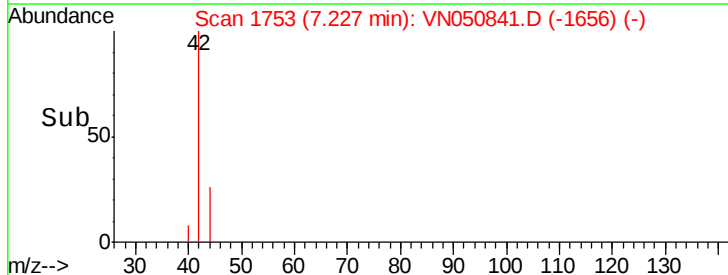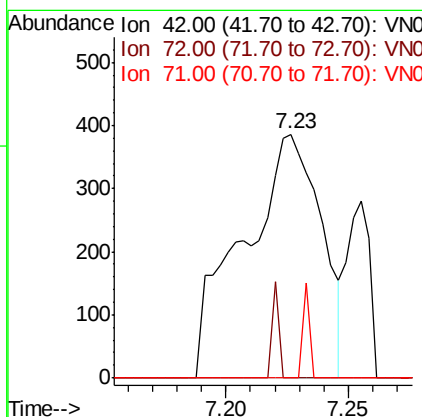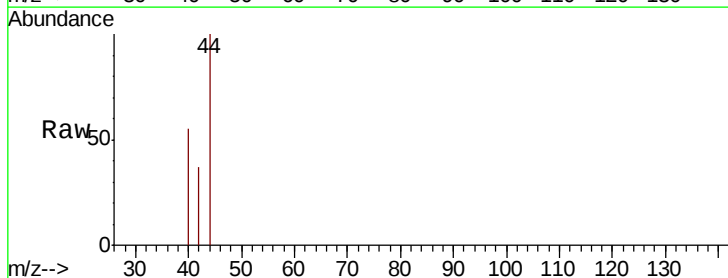







#31
Cyclohexane
Concen: 1.31 ug/l
RT: 7.67 min Scan# 1890
Delta R.T. 0.01 min
Lab File: VN050841.D
Acq: 23 Aug 2018 10:15

Instrument :
MSVOA_N
ClientSampled :

Tot Ion: 56 Resp: 11243
Ion Ratio Lower Upper
56 100
69 188.2 26.2 39.4#
84 154.5 68.3 102.5#

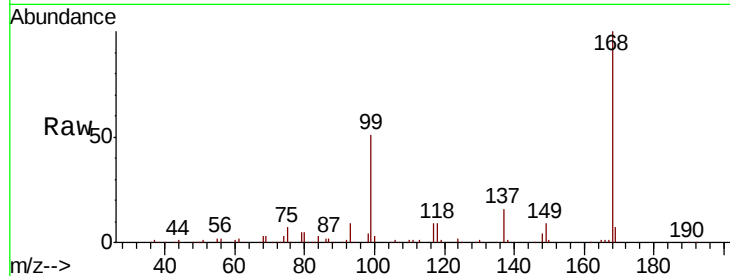


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0


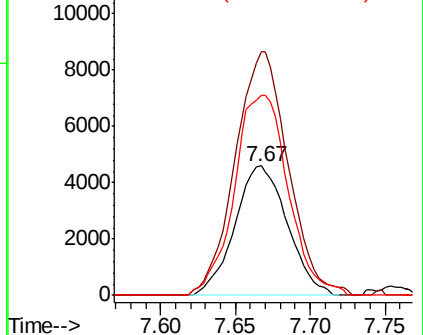



#33
1,2-Dichloroethane-d4
Concen: 53.40 ug/l
RT: 8.03 min Scan# 2002
Delta R.T. 0.00 min
Lab File: VN050841.D
Acq: 23 Aug 2018 10:15

Tgt Ion: 65 Resp: 414957
Ion Ratio Lower Upper
65 100
67 54.3 0.0 110.4



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0




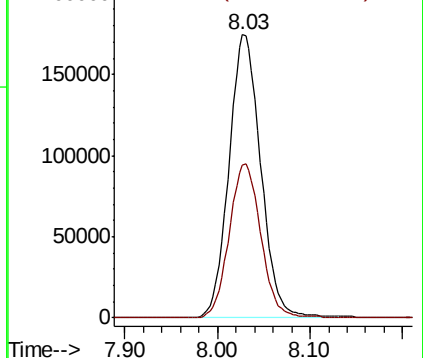


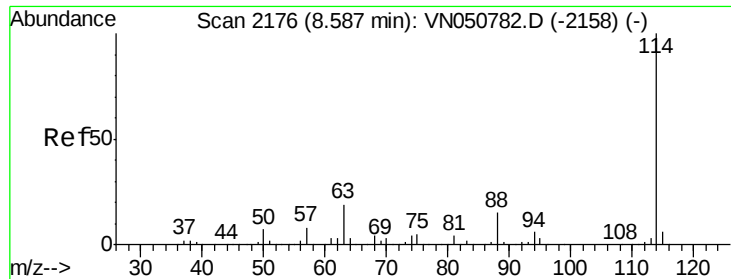

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2176
 Delta R.T. 0.00 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion:114 Resp: 1015669
 Ion Ratio Lower Upper
 114 100
 63 19.2 0.0 38.6
 88 15.2 0.0 30.6

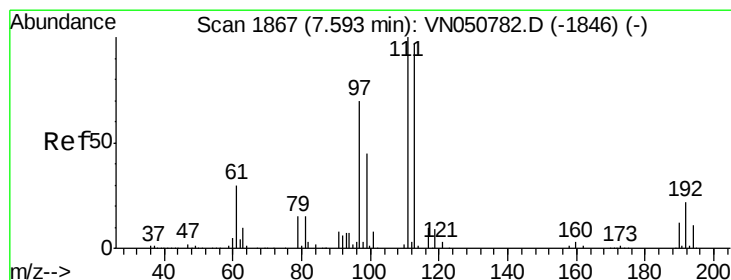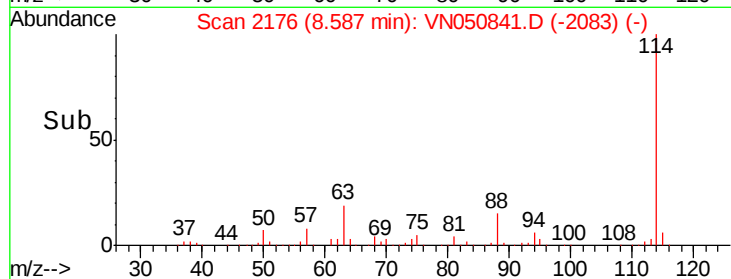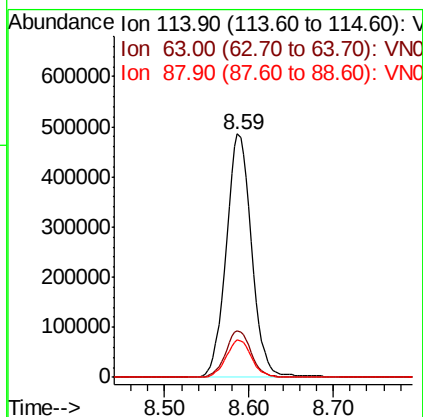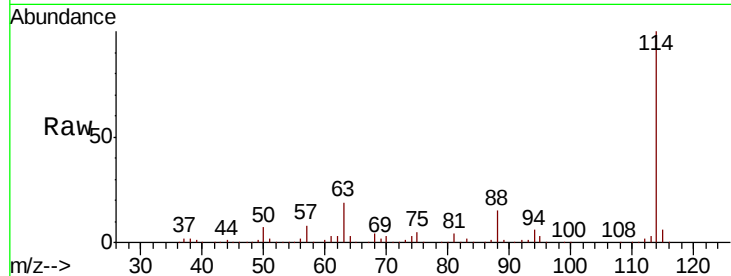

#35
 Dibromofluoromethane
 Concen: 49.38 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15

Tgt Ion:113 Resp: 399018
 Ion Ratio Lower Upper
 113 100
 111 101.7 82.6 123.8
 192 22.3 18.0 27.0


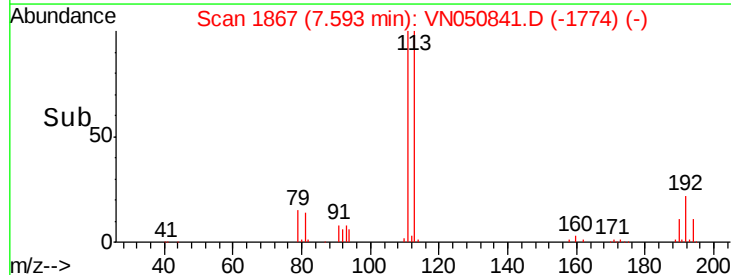
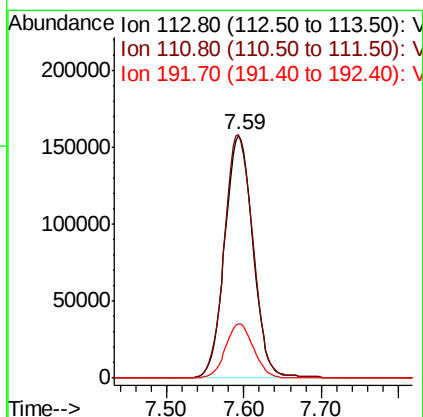



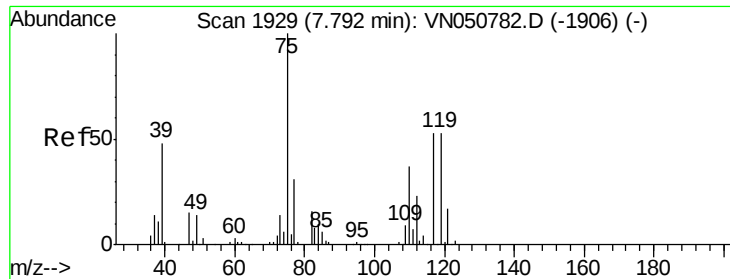

#36
 1,1-Dichloropropene
 Concen: 3.62 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.13 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
75	100		
110	8.1	18.1	54.4#
77	0.0	24.8	37.2#

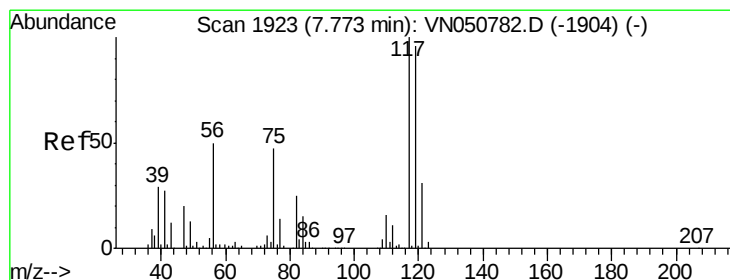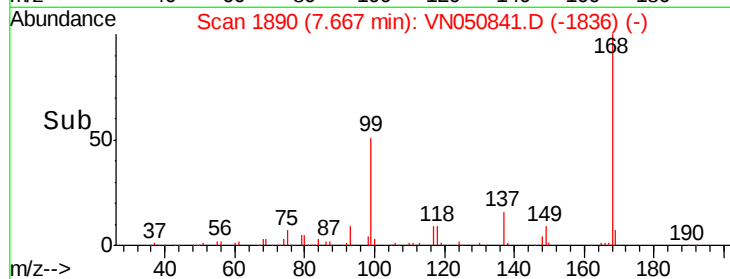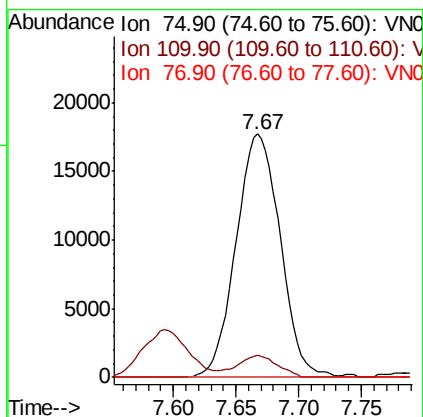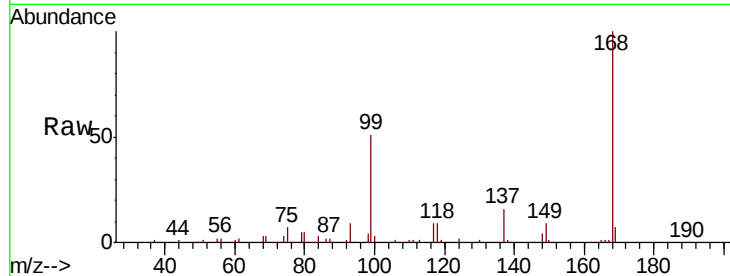

#38
 Carbon Tetrachloride
 Concen: 4.76 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.11 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15

Tgt Ion	Ratio	Lower	Upper
117	100		
119	7.2	76.3	114.5#
121	0.0	24.6	36.8#

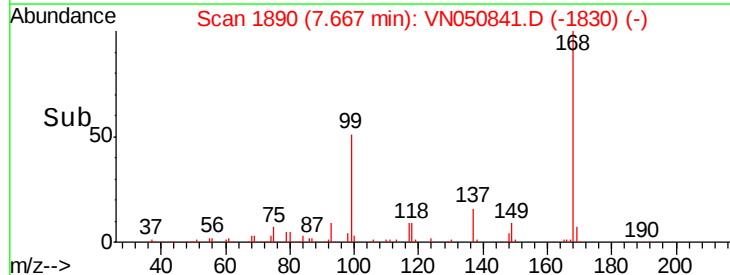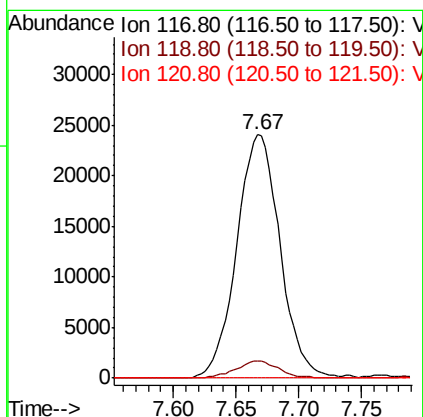







#43

Isopropyl Acetate
 Concen: 3.61 ug/l
 RT: 8.30 min Scan# 2088
 Delta R.T. 0.14 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15

Instrument :
 MSVOA_N
 ClientSampled :




Tot Ion: 43 Resp: 42698
 Ion Ratio Lower Upper
 43 100
 61 0.6 17.5 26.3#
 87 0.0 11.3 16.9#

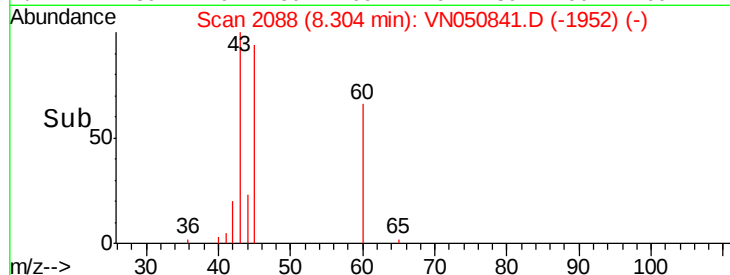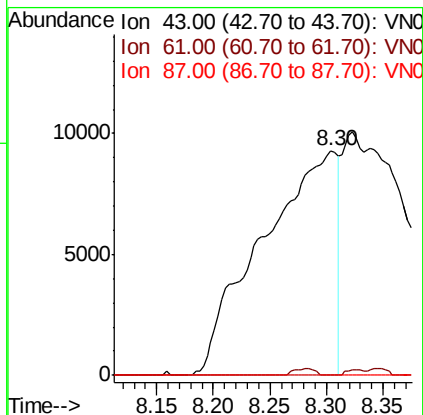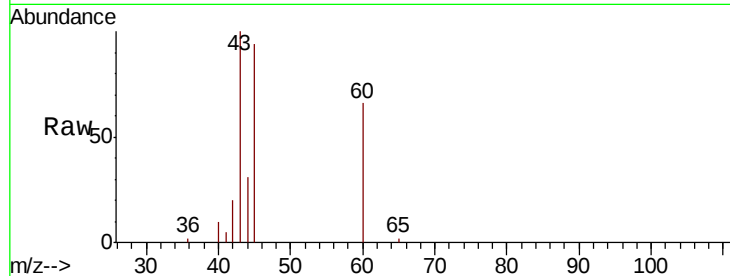


#50

Toluene-d8
 Concen: 47.22 ug/l
 RT: 10.09 min Scan# 2644
 Delta R.T. 0.00 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15

Tgt Ion: 98 Resp: 1426396
 Ion Ratio Lower Upper
 98 100
 100 63.2 51.5 77.3

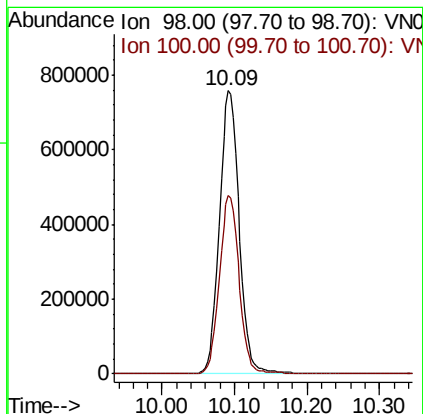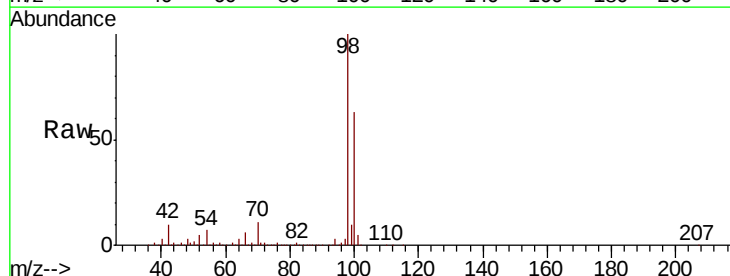

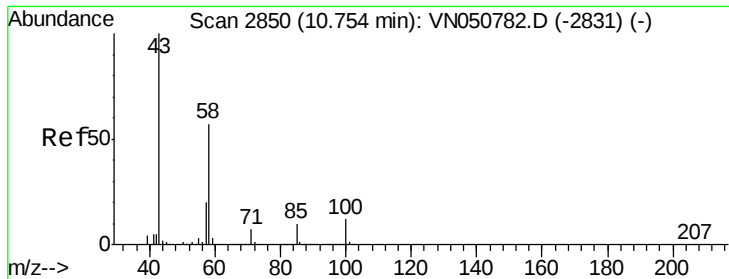

#59

2-Hexanone

Concen: 0.38 ug/l

RT: 10.76 min Scan# 2852

Delta R.T. 0.01 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15

Instrument :

MSVOA_N





ClientSampleId :

Tot Ion: 43 Resp: 1803

Ion Ratio Lower Upper

43 100

58 15.9 28.3 85.0#

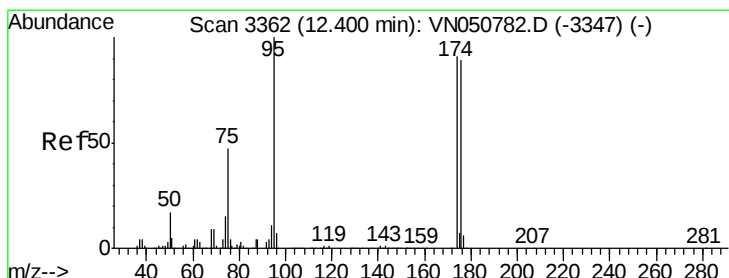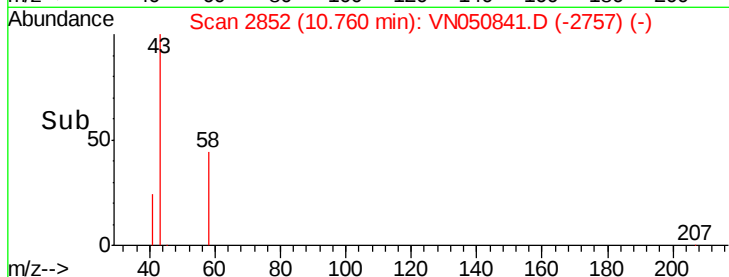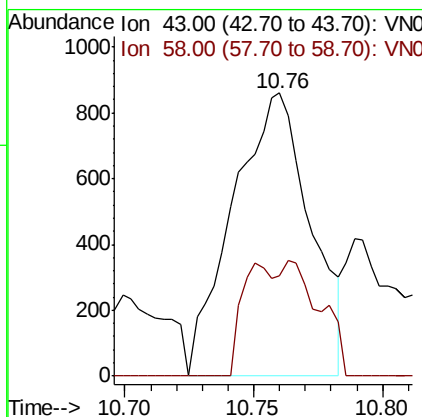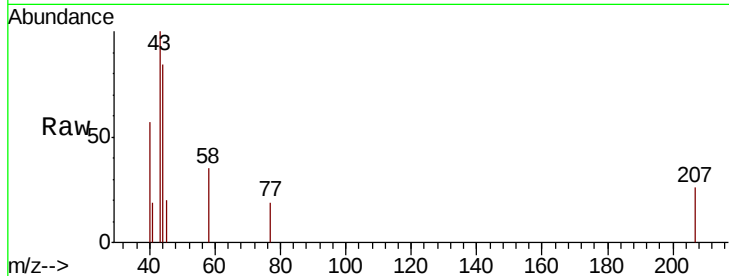

#62

4-Bromofluorobenzene

Concen: 36.89 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15




Tgt Ion: 95 Resp: 370300


Ion Ratio Lower Upper

95 100

174 91.4 0.0 183.0

176 89.1 0.0 178.8

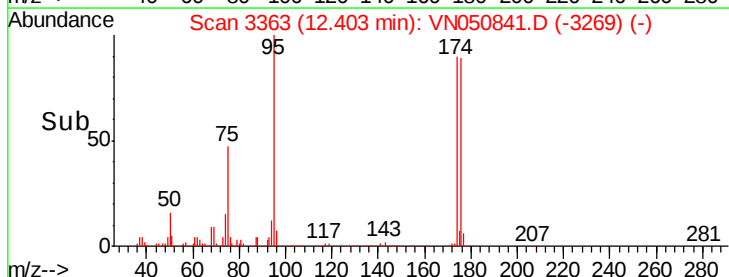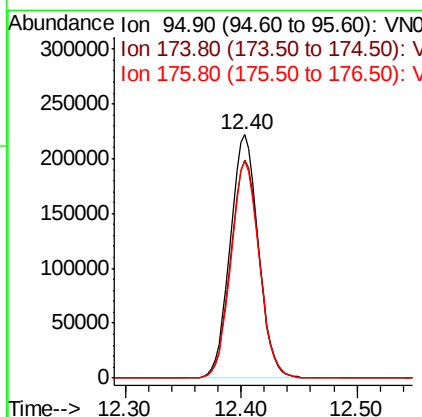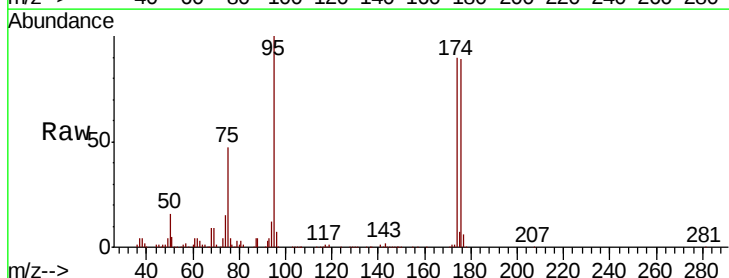


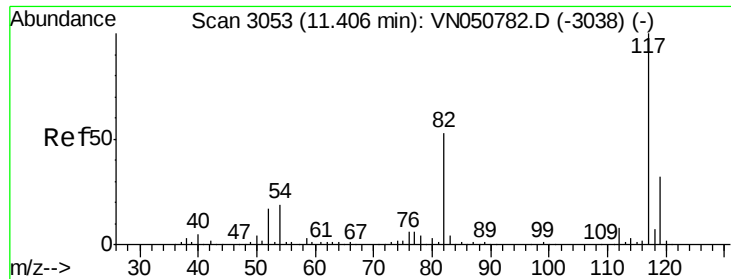




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. 0.00 min
Lab File: VN050841.D
Acq: 23 Aug 2018 10:15

Instrument :
MSVOA_N
ClientSampled :

Tot Ion:117 Resp: 874131
Ion Ratio Lower Upper
117 100
82 52.4 42.6 64.0
119 31.8 25.8 38.6

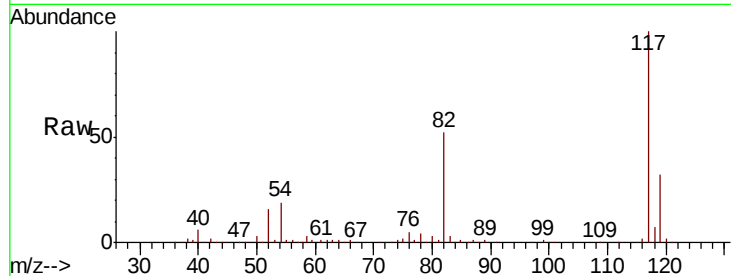


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V

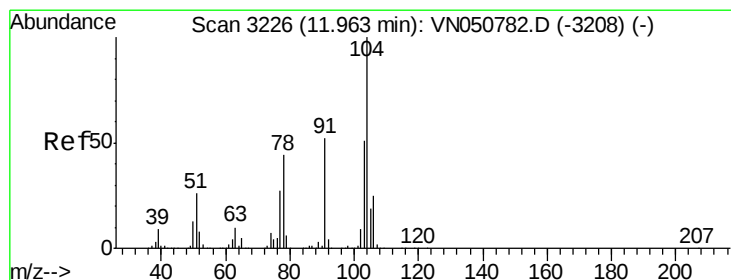
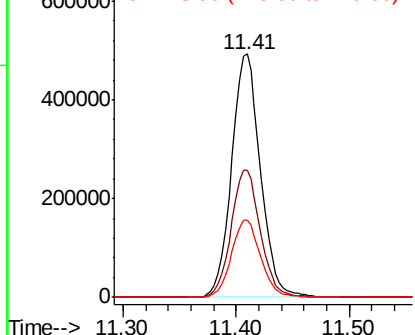



#70
Styrene
Concen: 1.31 ug/l
RT: 11.96 min Scan# 3226
Delta R.T. 0.00 min
Lab File: VN050841.D
Acq: 23 Aug 2018 10:15

Tgt Ion:104 Resp: 1067
Ion Ratio Lower Upper
104 100
78 45.7 38.2 57.4
103 23.4 44.4 66.6#



Abundance Ion 104.00 (103.70 to 104.70): V
Ion 78.00 (77.70 to 78.70): VN
Ion 103.00 (102.70 to 103.70): V

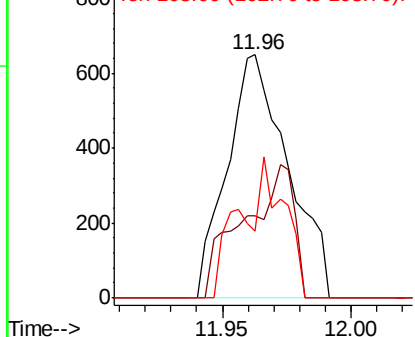

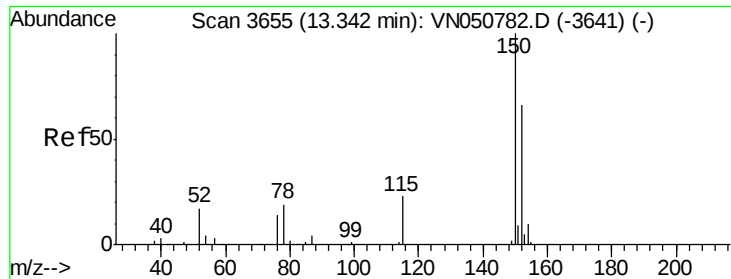

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. 0.00 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:152 Resp: 276103

Ion Ratio Lower Upper

152 100

115 55.4 27.8 83.4




150 158.3 0.0 351.4

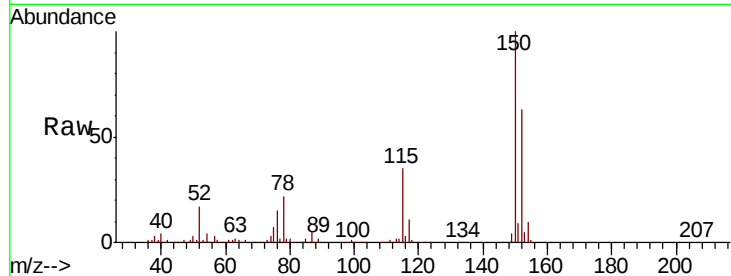

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

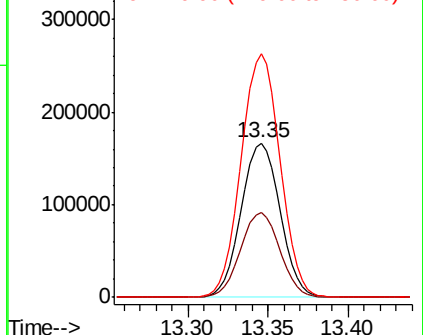

#74

N-ethyl acetate

Concen: 0.20 ug/l

RT: 12.07 min Scan# 3259

Delta R.T. 0.00 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15

Tgt Ion: 43 Resp: 1172


Ion Ratio Lower Upper

43 100

70 10.8 36.2 54.2#

55 0.0 21.8 32.8#

61 0.0 20.5 30.7#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V

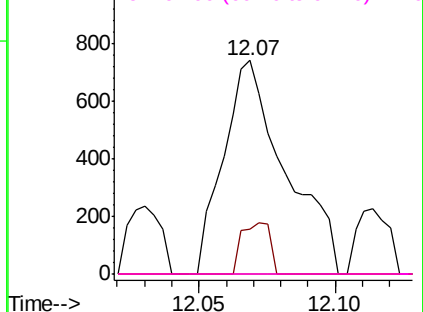

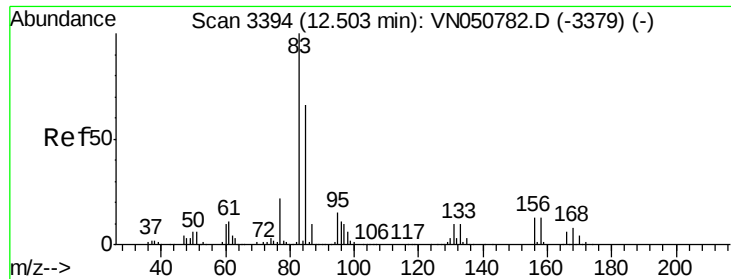

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.51 min Scan# 3396

Delta R.T. 0.01 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 83 Resp: 408

Ion Ratio Lower Upper

83 100

131 0.0 5.3 15.9#




85 57.4 31.9 95.7

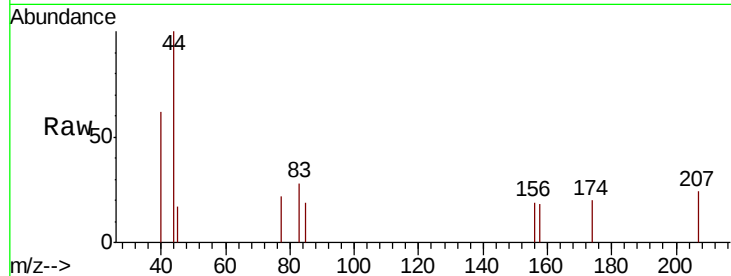

Abundance Ion 82.90 (82.60 to 83.60): VN0

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VN0

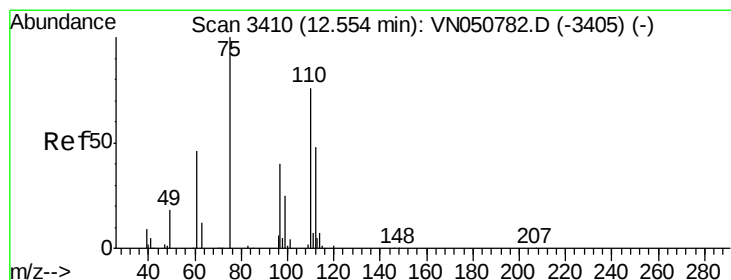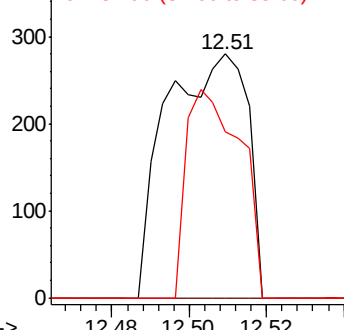

#76

1,2,3-Trichloropropane

Concen: 36.59 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. -0.15 min

Lab File: VN050841.D


Acq: 23 Aug 2018 10:15

Tgt Ion: 75 Resp: 176968

Ion Ratio Lower Upper

75 100

77 1.2 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

120000

100000



80000


60000

40000

20000

0

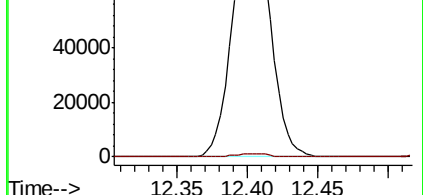



#81

trans-1,4-Dichloro-2-butene

Concen: 123.71 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.10 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15

Instrument :

MSVOA_N

ClientSampled :


Tot Ion: 75 Resp: 176968

Ion Ratio Lower Upper

75 100

53 0.1 68.9 103.3#




89 0.0 36.1 54.1#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0

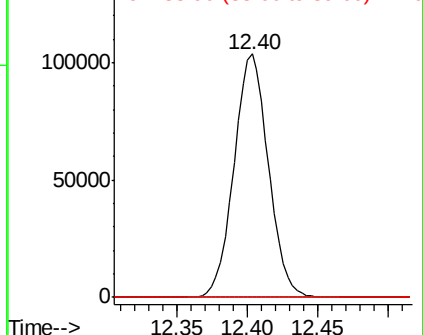

#87

1,3-Dichlorobenzene

Concen: 0.21 ug/l

RT: 13.28 min Scan# 3637

Delta R.T. 0.00 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15


Tgt Ion: 146 Resp: 2224

Ion Ratio Lower Upper

146 100

111 29.0 19.1 57.3



148 65.8 32.2 96.6




Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

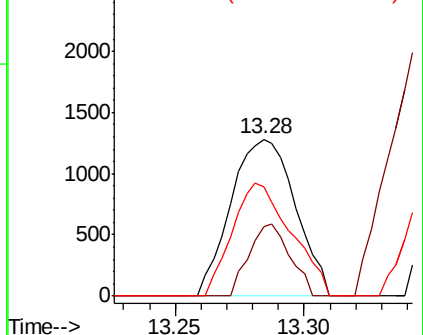







#88
 1,4-Dichlorobenzene
 Concen: 0.21 ug/l
 RT: 13.28 min Scan# 3637
 Delta R.T. -0.08 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15

Instrument :
 MSVOA_N
 ClientSampled :

Tot Ion:146 Resp: 2224
 Ion Ratio Lower Upper
 146 100
 111 29.0 18.8 56.3
 148 65.8 32.2 96.6

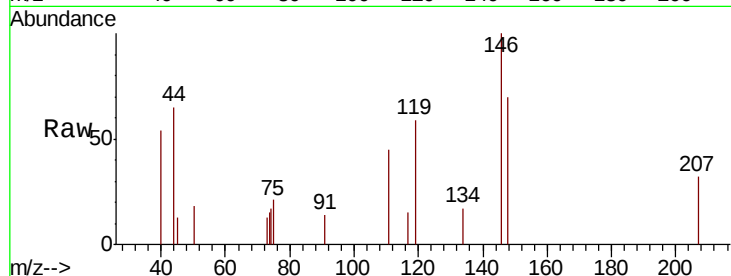


Abundance Ion 145.90 (145.60 to 146.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 147.90 (147.60 to 148.60): V

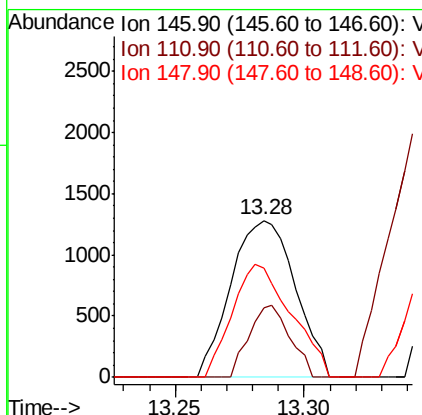




#91
 1,2-Dichlorobenzene
 Concen: 0.22 ug/l
 RT: 13.66 min Scan# 3753
 Delta R.T. 0.00 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15

Tgt Ion:146 Resp: 2202
 Ion Ratio Lower Upper
 146 100
 111 44.6 19.8 59.3
 148 67.3 32.3 96.8



Abundance Ion 145.90 (145.60 to 146.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 147.90 (147.60 to 148.60): V

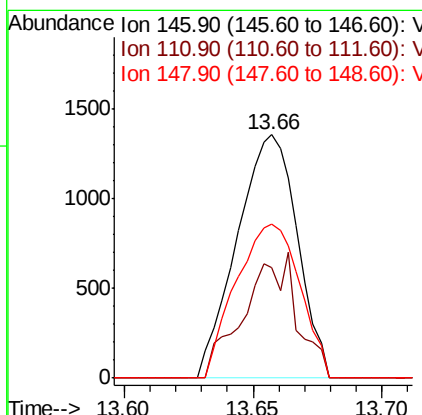


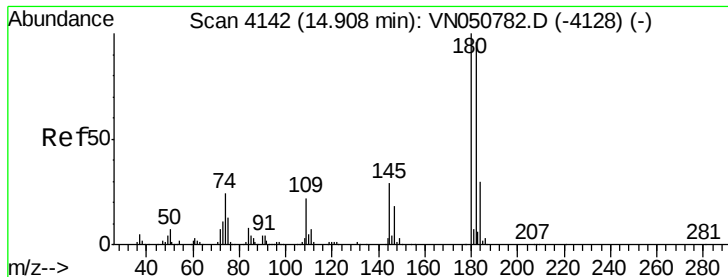




#93
 1,2,4-Trichlorobenzene
 Concen: 4.57 ua/l
 RT: 14.91 min Scan# 4144
 Delta R.T. 0.01 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15

Instrument :
 MSVOA_N
 ClientSampled :

Tot Ion:180 Resp: 2787
 Ion Ratio Lower Upper
 180 100
 182 99.0 48.2 144.6
 145 23.8 14.1 42.2

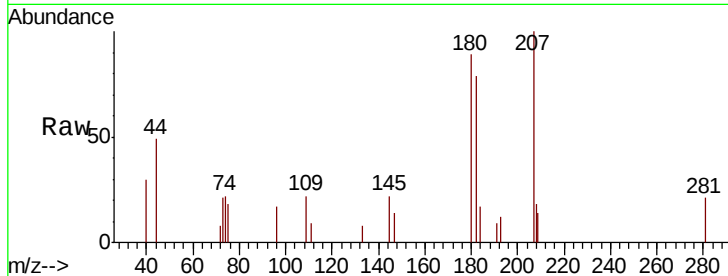


Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.80 (144.50 to 145.50): V

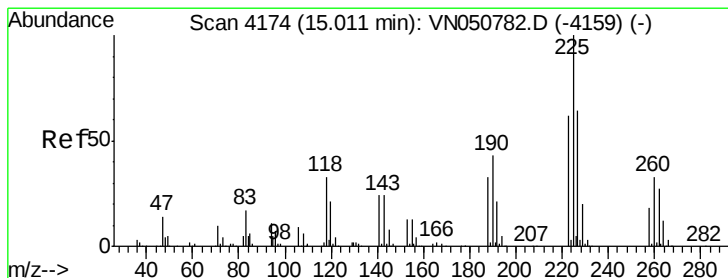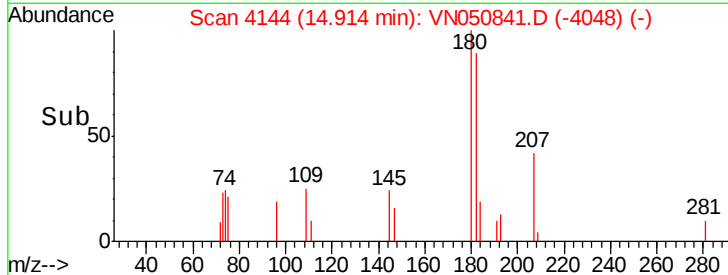
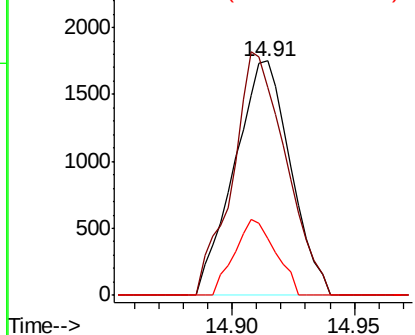



#94
 Hexachlorobutadiene
 Concen: Below Cal
 RT: 15.01 min Scan# 4174
 Delta R.T. 0.00 min
 Lab File: VN050841.D
 Acq: 23 Aug 2018 10:15

Tgt Ion:225 Resp: 1567
 Ion Ratio Lower Upper
 225 100
 223 54.6 31.3 93.8
 227 70.1 32.0 96.2

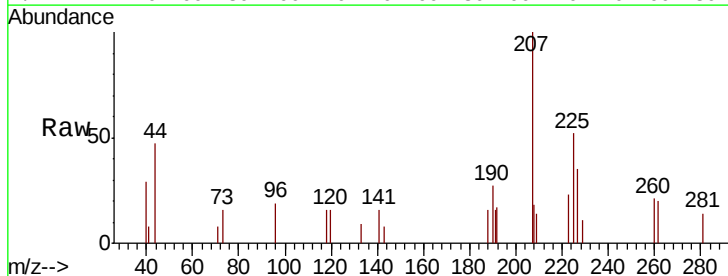

Abundance Ion 224.70 (224.40 to 225.40): V
 Ion 222.70 (222.40 to 223.40): V
 Ion 226.70 (226.40 to 227.40): V

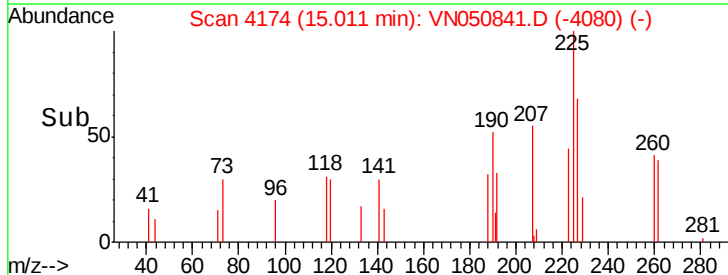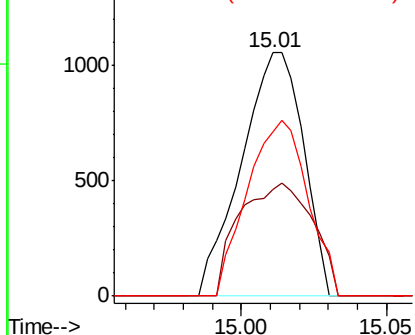



#95

Naphthalene

Concen: 5.88 ug/l

RT: 15.14 min Scan# 4213

Delta R.T. 0.00 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:128 Resp: 5948

Ion Ratio Lower Upper

128 100

127 13.9 10.5 15.7




129 8.2 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

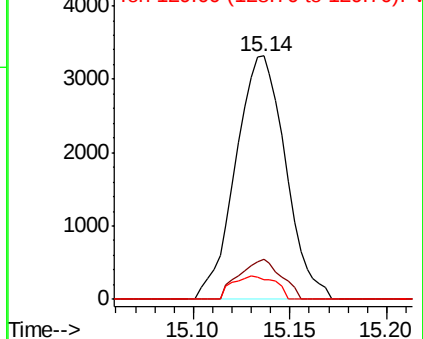

#96

1,2,3-Trichlorobenzene

Concen: 3.82 ug/l

RT: 15.31 min Scan# 4267

Delta R.T. -0.00 min

Lab File: VN050841.D

Acq: 23 Aug 2018 10:15


Tgt Ion:180 Resp: 2788

Ion Ratio Lower Upper

180 100

182 109.2 48.0 144.2

145 38.6 15.2 45.6



Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

