


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082318\
Data File : VN050836.D
Acq On : 23 Aug 2018 8:01
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
Title : SW846 8260
Last Update : Wed Aug 22 05:38:12 2018

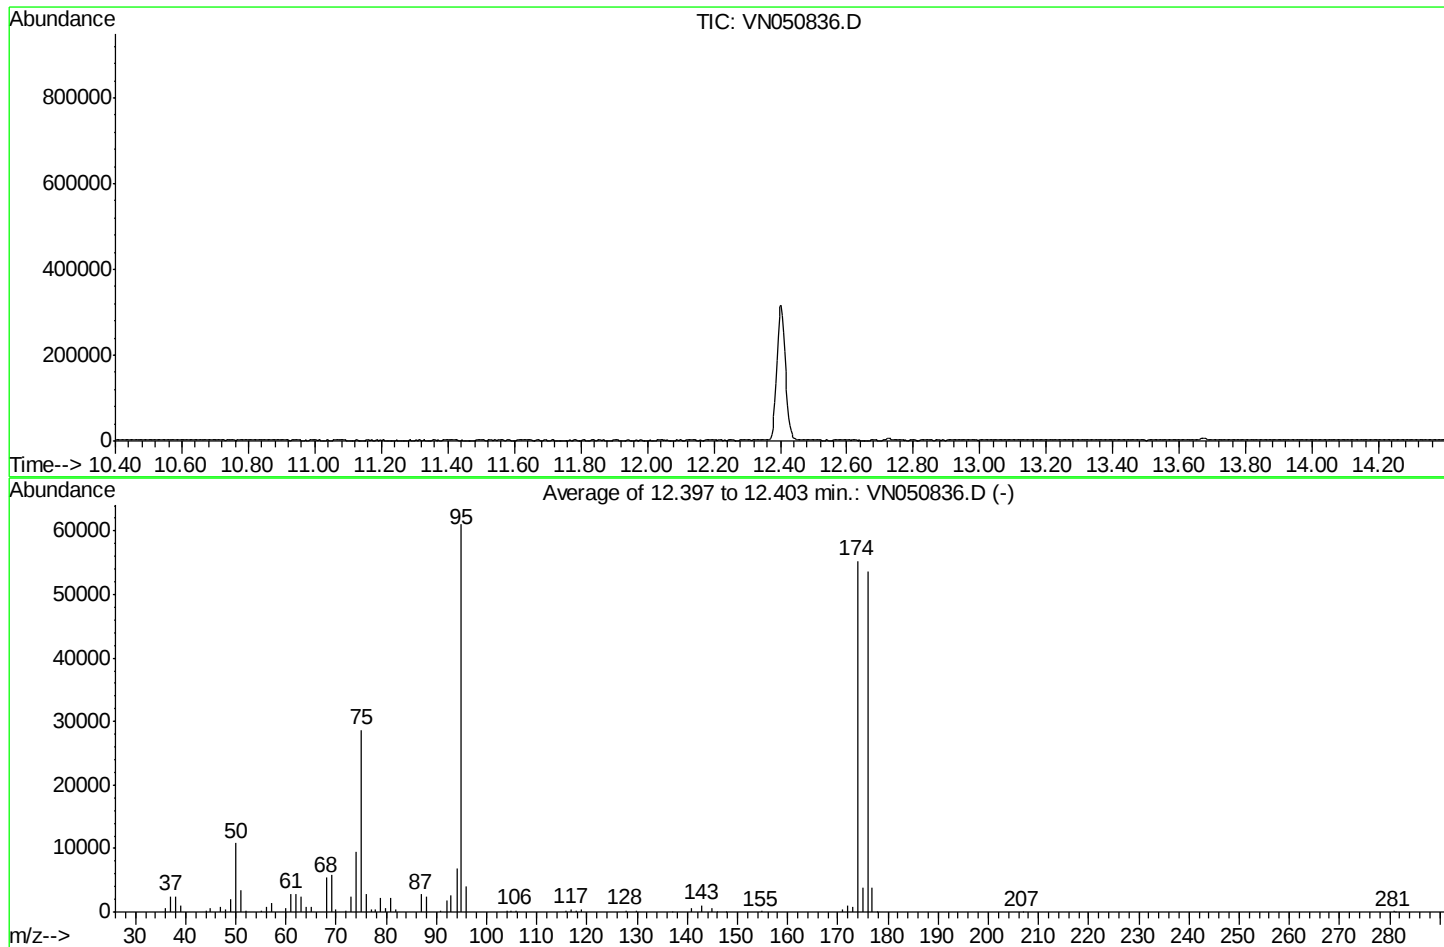

AutoFind: Scans 3361, 3362, 3363; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	10867	PASS
75	95	30	60	46.9	28645	PASS
95	95	100	100	100.0	61056	PASS
96	95	5	9	6.8	4133	PASS
173	174	0.00	2	1.5	824	PASS
174	95	50	100	90.6	55328	PASS
175	174	5	9	6.9	3843	PASS
176	174	95	101	97.0	53658	PASS
177	176	5	9	7.2	3866	PASS