


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082319\
Data File : VN057461.D
Acq On : 23 Aug 2019 8:17
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N082319W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Aug 23 23:15:31 2019

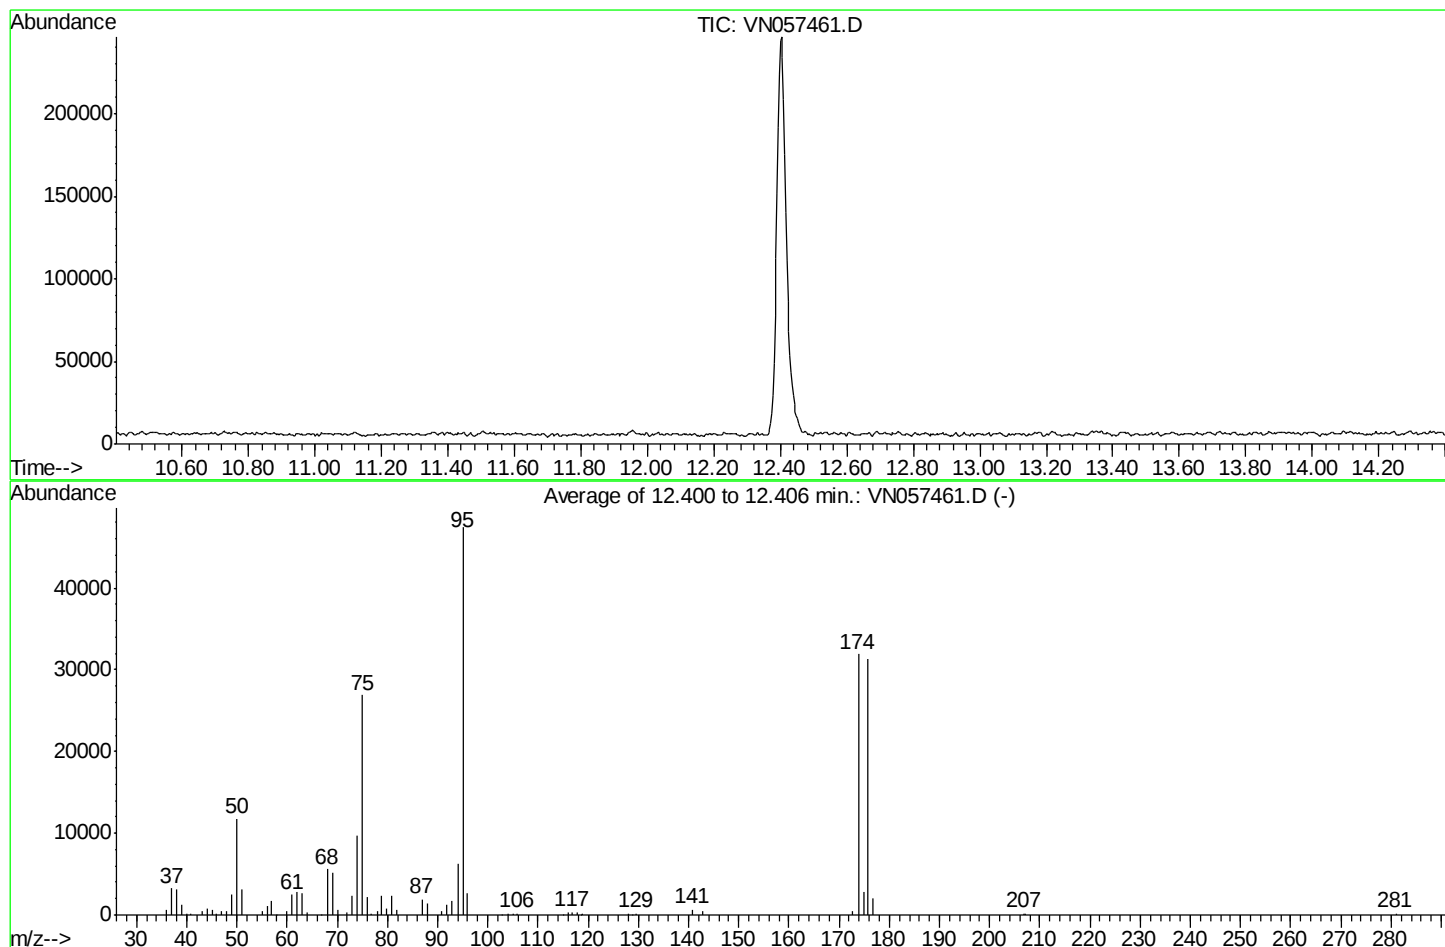

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	11752	PASS
75	95	30	60	56.7	26866	PASS
95	95	100	100	100.0	47418	PASS
96	95	5	9	5.8	2729	PASS
173	174	0.00	2	1.4	457	PASS
174	95	50	100	67.3	31922	PASS
175	174	5	9	8.8	2795	PASS
176	174	95	101	98.0	31280	PASS
177	176	5	9	6.7	2098	PASS