

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082322\
 Data File : VN074076.D
 Acq On : 23 Aug 2022 18:29
 Operator : JC\MD
 Sample : N4247-07
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-7

Quant Time: Aug 23 18:53:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 16 00:45:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	470056	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	736141	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	732223	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	374981	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	248065	54.182	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.360%	
35) Dibromofluoromethane	7.951	113	237282	54.504	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 109.000%	
50) Toluene-d8	10.381	98	806956	47.860	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 95.720%	
62) 4-Bromofluorobenzene	12.675	95	332502	59.421	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 118.840%	

Target Compounds				Qvalue		
3) Chloromethane	2.264	50	1059	0.256	ug/l #	86
11) Tert butyl alcohol	5.299	59	4271	4.170	ug/l #	76
13) Acrolein	3.981	56	971	1.355	ug/l #	67
16) Acetone	4.228	43	69646	32.244	ug/l	95
18) Methyl Acetate	4.781	43	8271	Below Cal		97
20) Methylene Chloride	5.010	84	34702	7.614	ug/l	97
25) 2-Butanone	7.269	43	17145	5.006	ug/l	96
29) Tetrahydrofuran	7.628	42	1677	0.763	ug/l #	80
31) Cyclohexane	8.022	56	8175	1.281	ug/l #	11
36) 1,1-Dichloropropene	8.016	75	31250	5.168	ug/l #	49
37) Ethyl Acetate	7.340	43	70900	9.678	ug/l	97
38) Carbon Tetrachloride	8.022	117	42148	6.098	ug/l #	16
40) Benzene	8.398	78	35681	1.870	ug/l	91
41) Methacrylonitrile	7.628	41	1011	0.305	ug/l #	35
42) 1,2-Dichloroethane	8.498	62	2055	0.313	ug/l #	74
43) Isopropyl Acetate	8.498	43	284702	27.281	ug/l #	92
45) 1,2-Dichloropropane	9.563	63	4003	0.875	ug/l #	44
48) Methyl methacrylate	9.487	41	14011	3.138	ug/l #	38
49) 1,4-Dioxane	9.557	88	550	4.142	ug/l #	1
51) 4-Methyl-2-Pentanone	10.275	43	24184	3.428	ug/l #	79
52) Toluene	10.445	92	30025	2.294	ug/l	96
53) t-1,3-Dichloropropene	10.557	75	1726	0.247	ug/l #	18
54) cis-1,3-Dichloropropene	10.187	75	100797	13.207	ug/l #	60
57) 1,3-Dichloropropane	11.034	76	15189	1.835	ug/l #	43
59) 2-Hexanone	11.034	43	178593	32.889	ug/l #	51
67) Ethyl Benzene	11.781	91	7426	0.287	ug/l	97
68) m/p-Xylenes	11.886	106	10467	0.995	ug/l	95
69) o-Xylene	12.216	106	6908	0.655	ug/l	94
70) Styrene	12.233	104	6159	0.373	ug/l	96
71) Bromoform	12.669	173	1602	0.304	ug/l #	1
74) N-amyl acetate	12.139	43	48615	4.710	ug/l #	50
76) 1,2,3-Trichloropropane	12.675	75	160598	20.605	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.675	75	160598	58.606	ug/l #	10
95) Naphthalene	15.439	128	78460	2.988	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082322\
Data File : VN074076.D
Acq On : 23 Aug 2022 18:29
Operator : JC\MD
Sample : N4247-07
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-7

Quant Time: Aug 23 18:53:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 16 00:45:21 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082322\
Data File : VN074076.D
Acq On : 23 Aug 2022 18:29
Operator : JC\MD
Sample : N4247-07
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-7

Quant Time: Aug 23 18:53:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 16 00:45:21 2022
Response via : Initial Calibration




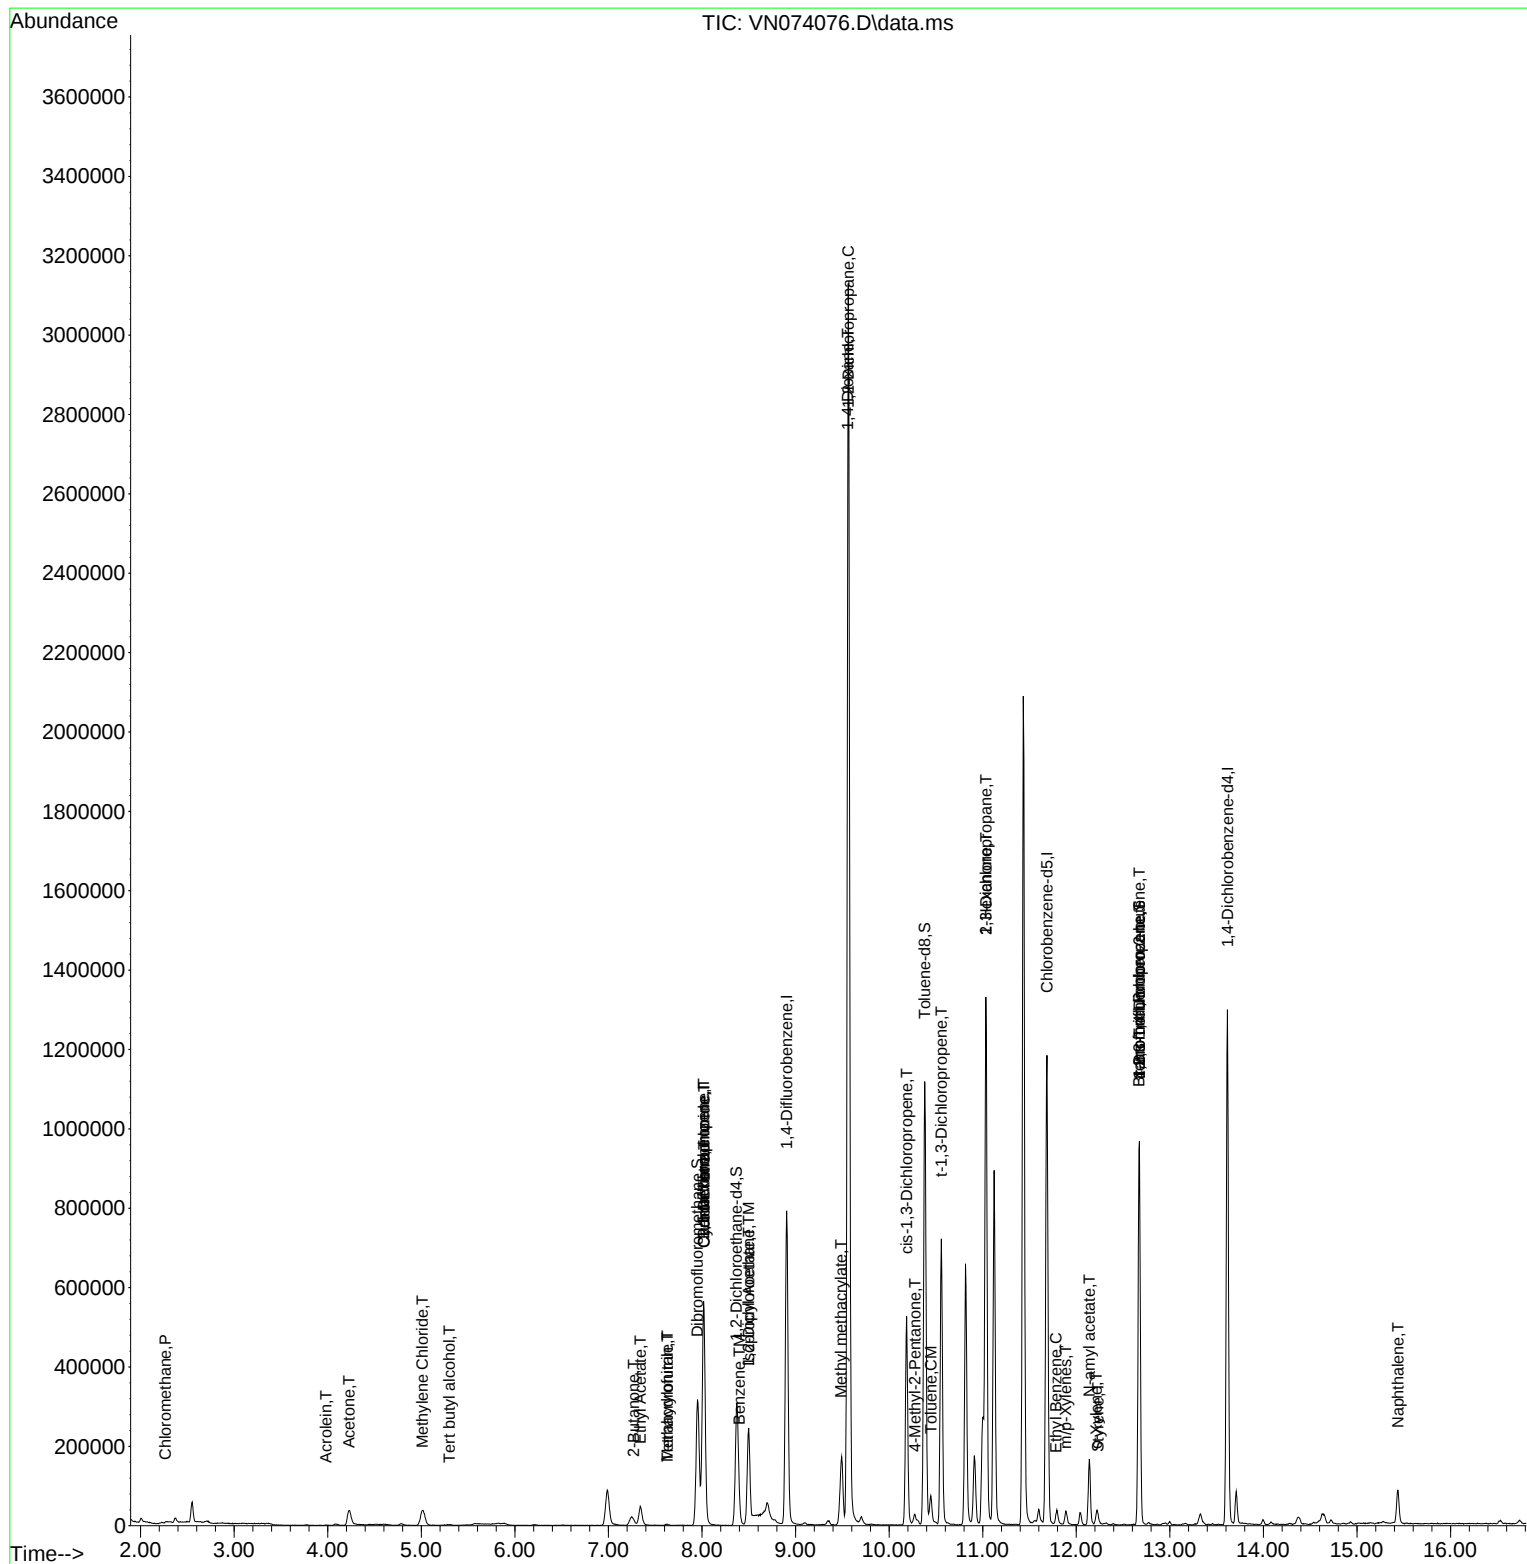




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1
Delta R.T. 0.000 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion:168 Resp: 470056
Ion Ratio Lower Upper
168 100
99 50.6 42.3 63.5

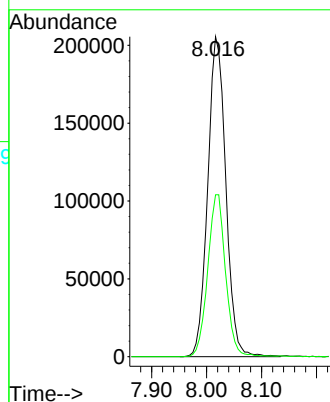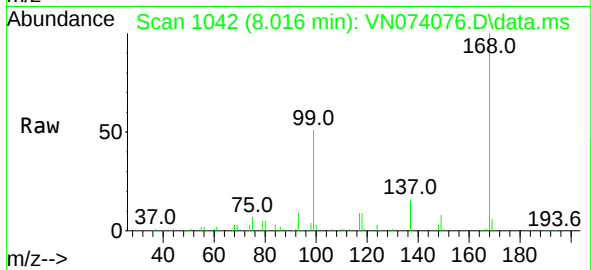

#3
Chloromethane
Concen: 0.256 ug/l
RT: 2.264 min Scan# 64
Delta R.T. -0.005 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 50 Resp: 1059
Ion Ratio Lower Upper
50 100
52 40.0 25.7 38.5#


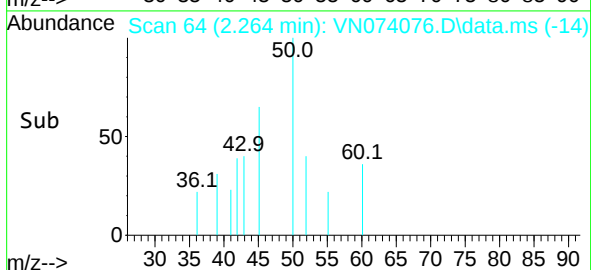

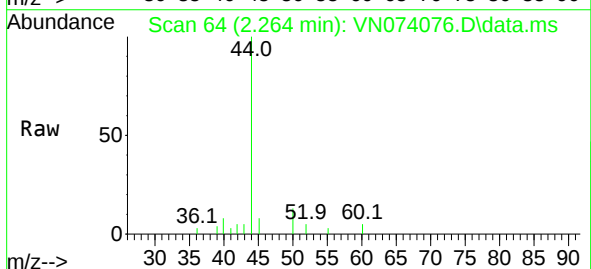




#11
Tert butyl alcohol
Concen: 4.170 ug/l
RT: 5.299 min Scan# 579
Delta R.T. 0.007 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion: 59 Resp: 4271
Ion Ratio Lower Upper
59 100
57 1.6 8.3 12.5#

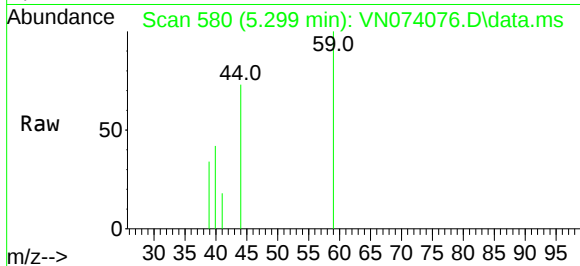

#13
Acrolein
Concen: 1.355 ug/l
RT: 3.981 min Scan# 356
Delta R.T. 0.000 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 56 Resp: 971
Ion Ratio Lower Upper
56 100
55 41.9 54.8 82.2#

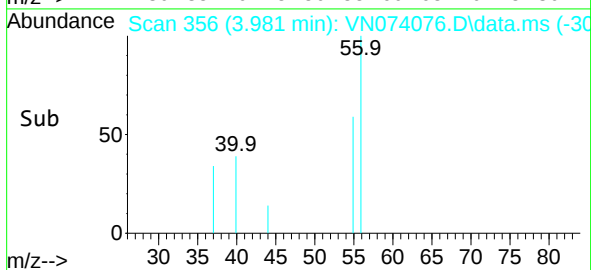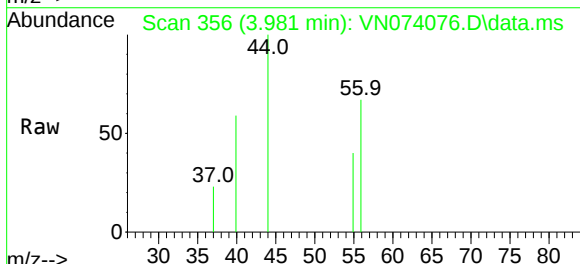



#16

Acetone

Concen: 32.244 ug/l

RT: 4.228 min Scan# 397

Delta R.T. 0.006 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :





SB-7

Tgt Ion: 43 Resp: 69646

Ion Ratio Lower Upper

43 100

58 35.1 26.0 39.0

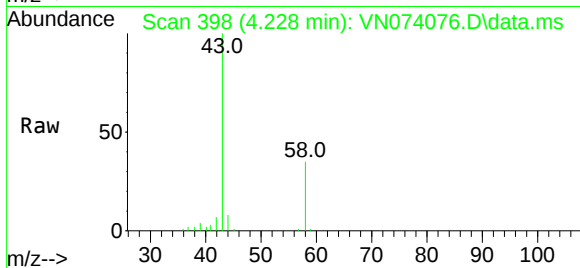

#18

Methyl Acetate

Concen: Below Cal

RT: 4.781 min Scan# 492

Delta R.T. 0.000 min

Lab File: VN074076.D




Acq: 23 Aug 2022 18:29


Tgt Ion: 43 Resp: 8271

Ion Ratio Lower Upper

43 100

74 25.4 21.6 32.4


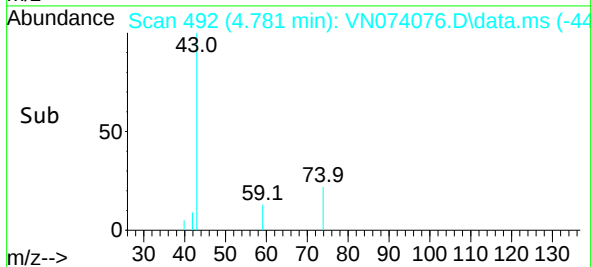

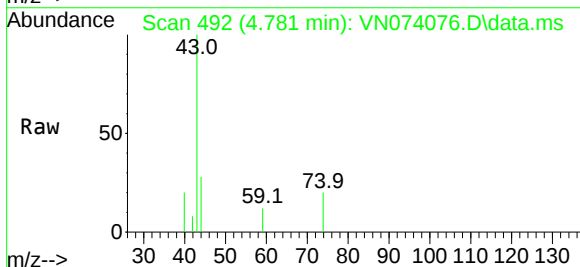




#20
Methylene Chloride
Concen: 7.614 ug/l
RT: 5.010 min Scan# 51
Delta R.T. 0.000 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion:	84	Resp:	34702
Ion	Ratio	Lower	Upper
84	100		
49	109.9	88.3	132.5
51	31.2	28.2	42.2
86	66.5	50.6	76.0



#25
2-Butanone
Concen: 5.006 ug/l
RT: 7.269 min Scan# 915
Delta R.T. 0.012 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion:	43	Resp:	17145
Ion	Ratio	Lower	Upper
43	100		
72	27.5	23.7	35.5

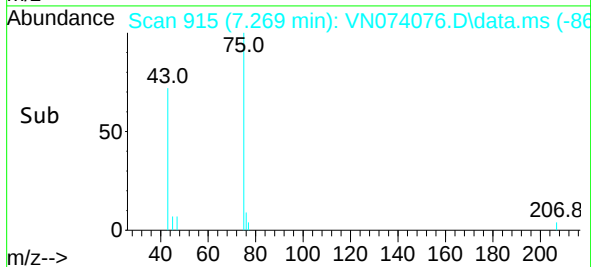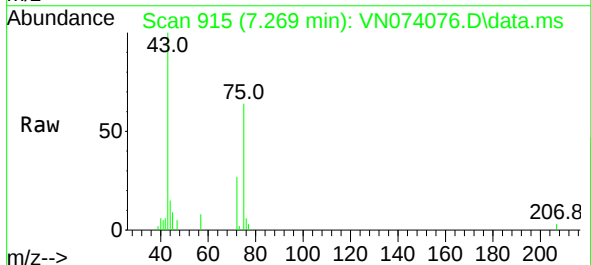



#29

Tetrahydrofuran

Concen: 0.763 ug/l

RT: 7.628 min Scan# 91

Delta R.T. 0.018 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :

SB-7





Tgt Ion: 42 Resp: 1677

Ion Ratio Lower Upper

42 100

72 32.6 39.7 59.5#

71 36.0 36.6 55.0#

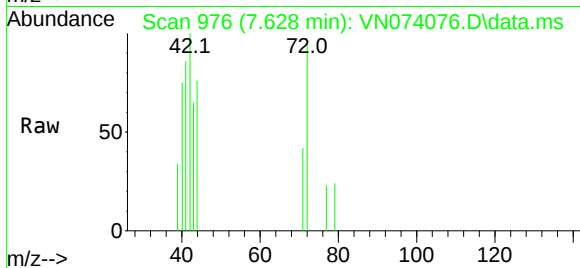

#31

Cyclohexane

Concen: 1.281 ug/l

RT: 8.022 min Scan# 1043

Delta R.T. 0.000 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29




Tgt Ion: 56 Resp: 8175


Ion Ratio Lower Upper

56 100

69 151.6 27.8 41.8#

84 143.8 76.9 115.3#

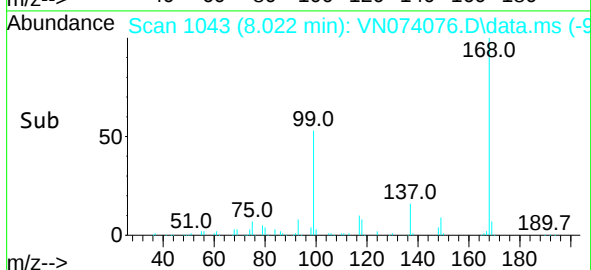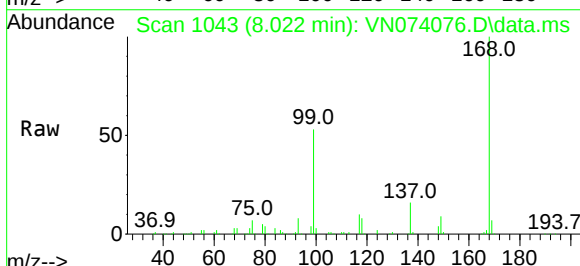

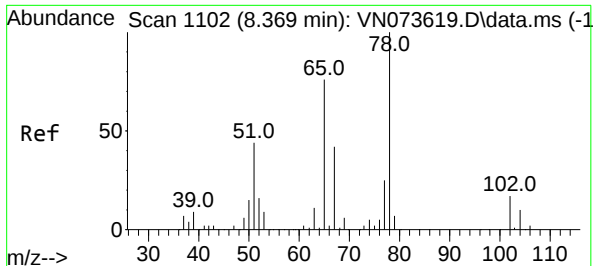

#33

1,2-Dichloroethane-d4

Concen: 54.182 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. 0.000 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :





SB-7

Tgt Ion: 65 Resp: 248065

Ion Ratio Lower Upper

65 100

67 53.6 0.0 104.8

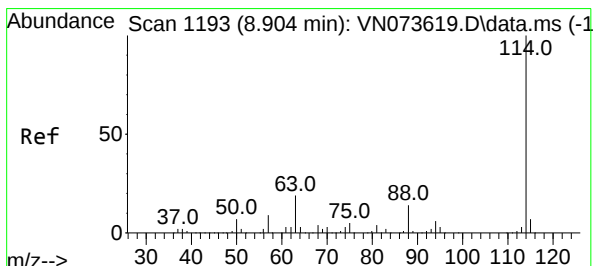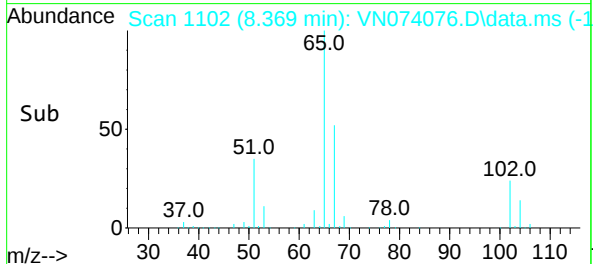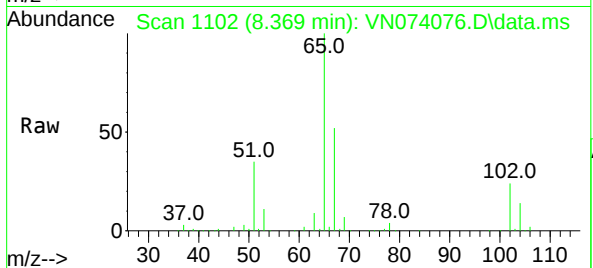

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29




Tgt Ion: 114 Resp: 736141


Ion Ratio Lower Upper

114 100

63 19.4 0.0 40.0

88 15.5 0.0 32.6


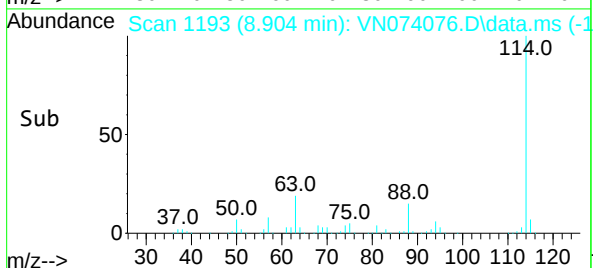
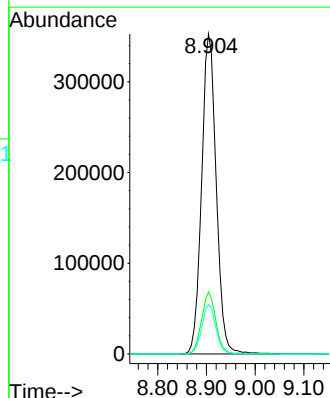
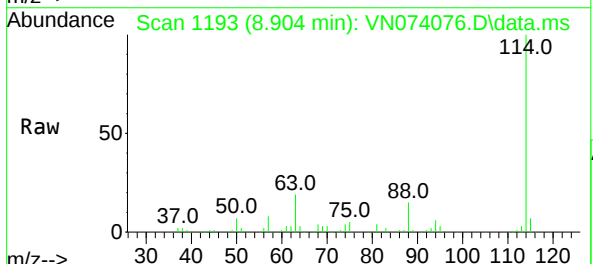


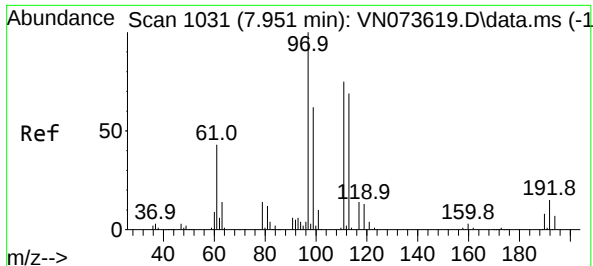

#35
Dibromofluoromethane
Concen: 54.504 ug/l
RT: 7.951 min Scan# 1031
Delta R.T. 0.000 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion:113 Resp: 237282
Ion Ratio Lower Upper
113 100
111 103.3 81.4 122.0
192 22.3 17.0 25.6

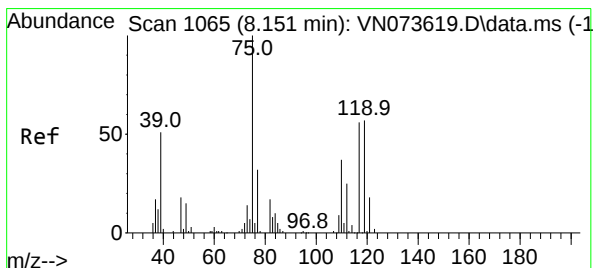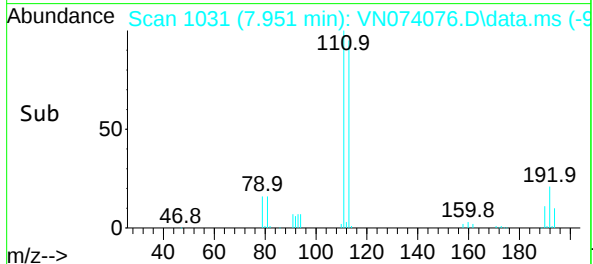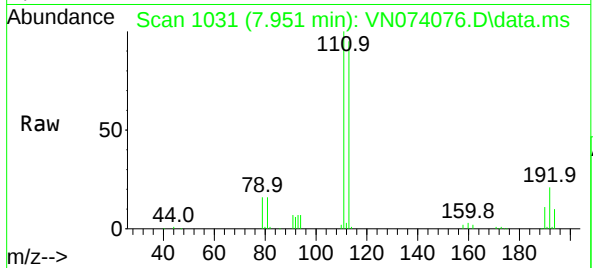

#36
1,1-Dichloropropene
Concen: 5.168 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.135 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 75 Resp: 31250
Ion Ratio Lower Upper
75 100
110 9.0 18.3 54.8#
77 0.0 25.1 37.7#


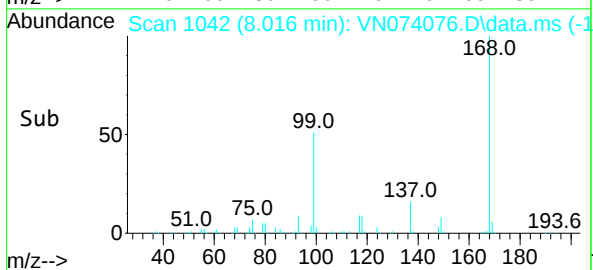

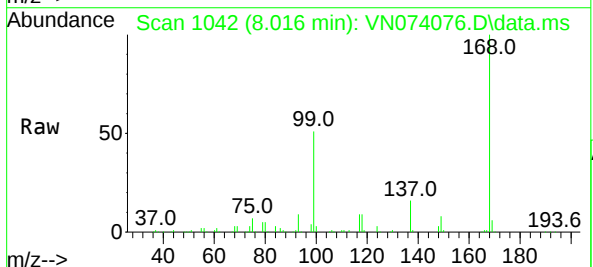




#37
Ethyl Acetate
Concen: 9.678 ug/l
RT: 7.340 min Scan# 91
Delta R.T. 0.001 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion:	43	Resp:	70900
Ion	Ratio	Lower	Upper
43	100		
61	15.7	11.8	17.6
70	12.9	9.3	13.9



#38
Carbon Tetrachloride
Concen: 6.098 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.111 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion:	117	Resp:	42148
Ion	Ratio	Lower	Upper
117	100		
119	4.4	75.8	113.8#
121	0.0	24.6	37.0#



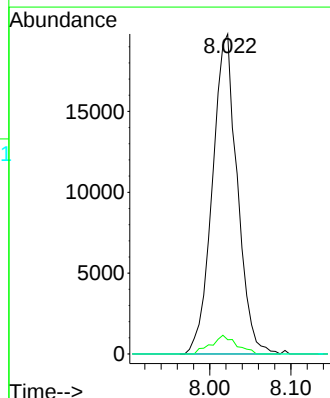



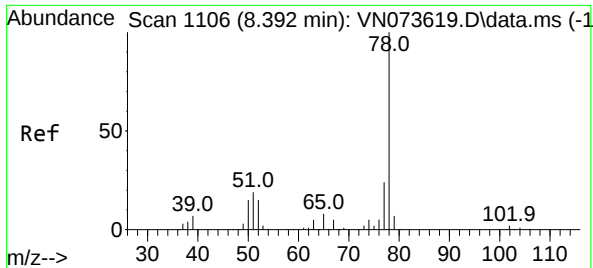

#40
Benzene
Concen: 1.870 ug/l
RT: 8.398 min Scan# 1107
Delta R.T. 0.006 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion: 78 Resp: 35681
Ion Ratio Lower Upper
78 100
77 19.6 19.4 29.0

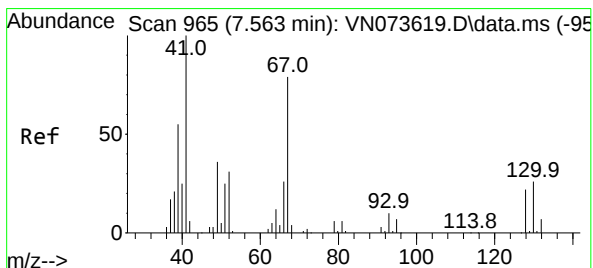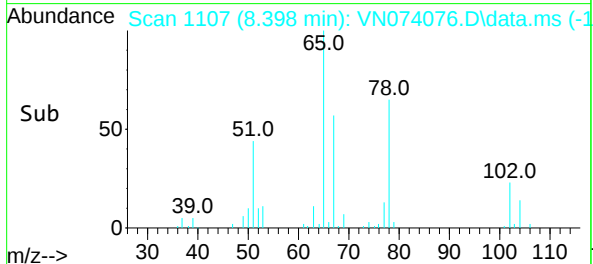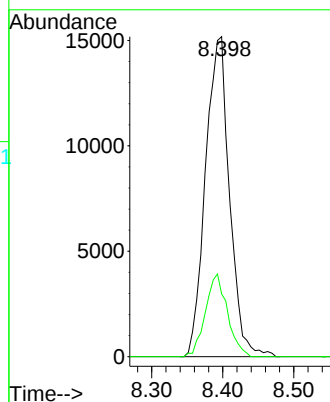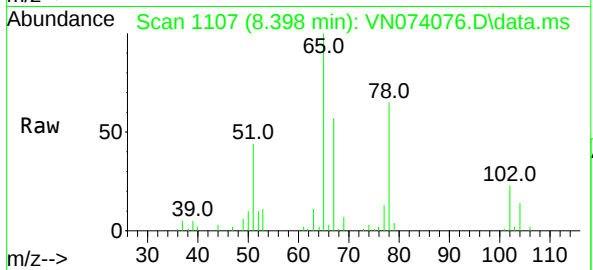

#41
Methacrylonitrile
Concen: 0.305 ug/l
RT: 7.628 min Scan# 976
Delta R.T. 0.065 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 41 Resp: 1011
Ion Ratio Lower Upper
41 100
39 44.1 48.6 73.0#
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

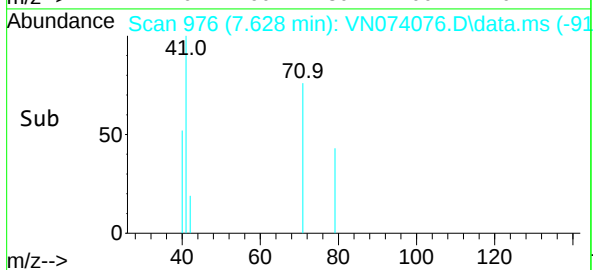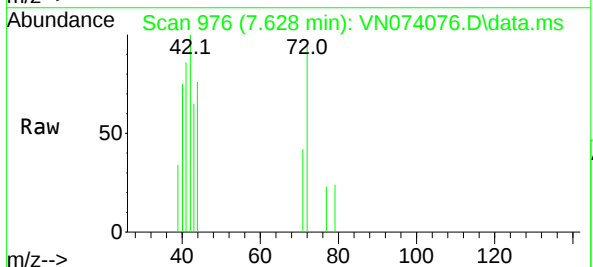

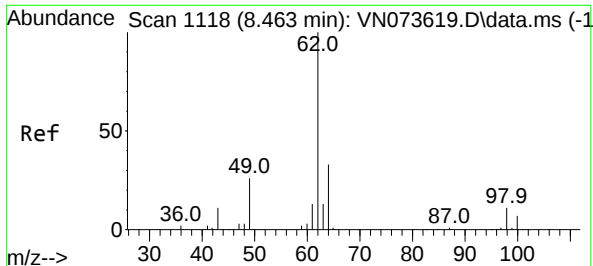

#42

1,2-Dichloroethane

Concen: 0.313 ug/l

RT: 8.498 min Scan# 1118

Delta R.T. 0.035 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :





SB-7

Tgt Ion: 62 Resp: 2055

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.4

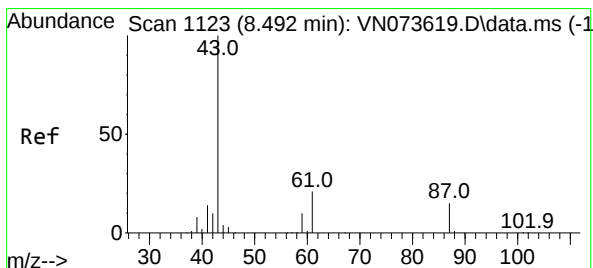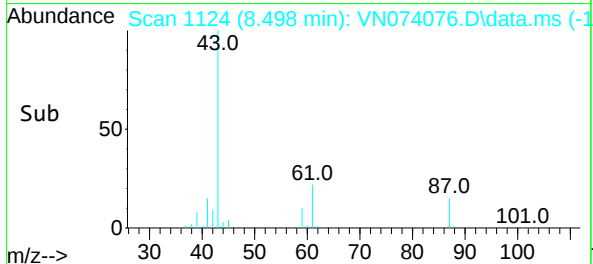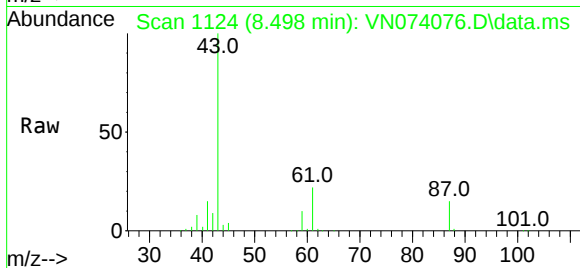

#43

Isopropyl Acetate

Concen: 27.281 ug/l

RT: 8.498 min Scan# 1124

Delta R.T. 0.006 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29




Tgt Ion: 43 Resp: 284702


Ion Ratio Lower Upper

43 100

61 21.3 21.9 32.9#

87 14.5 12.0 18.0

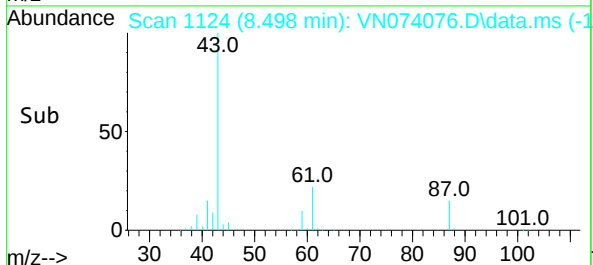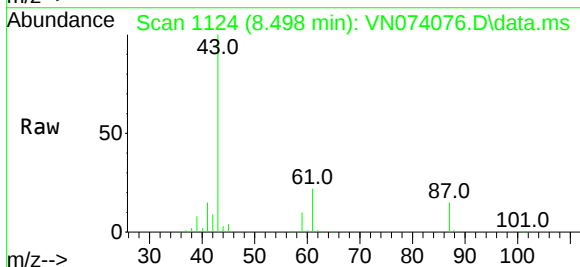

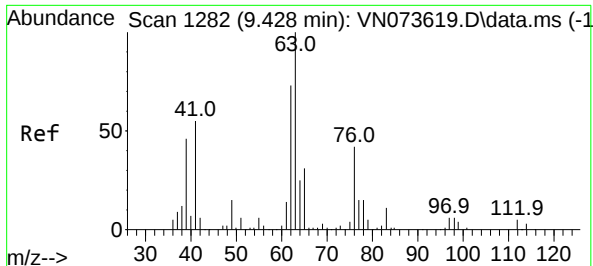

#45

1,2-Dichloropropane

Concen: 0.875 ug/l

RT: 9.563 min Scan# 11

Delta R.T. 0.135 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :





SB-7

Tgt Ion: 63 Resp: 4003

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

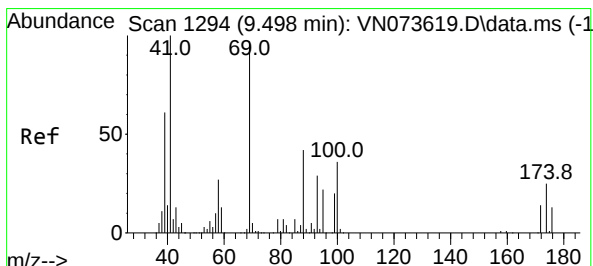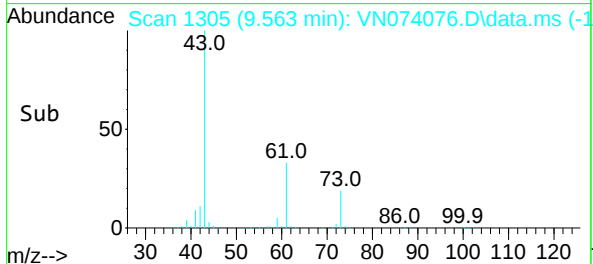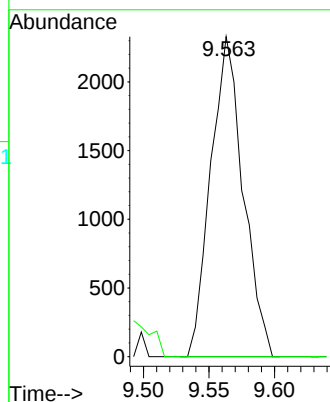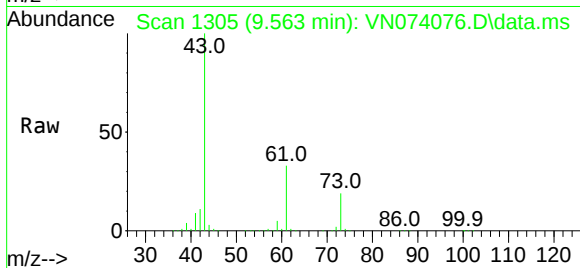

#48

Methyl methacrylate

Concen: 3.138 ug/l

RT: 9.487 min Scan# 1292

Delta R.T. -0.011 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29




Tgt Ion: 41 Resp: 14011


Ion Ratio Lower Upper

41 100

69 2.1 74.7 112.1#

39 51.5 45.6 68.4


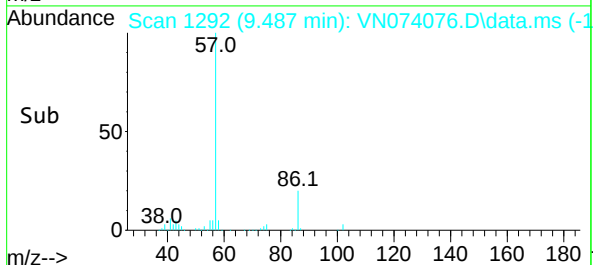

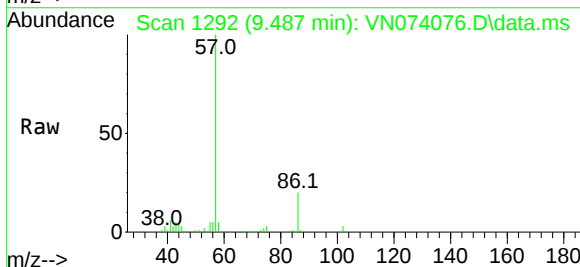


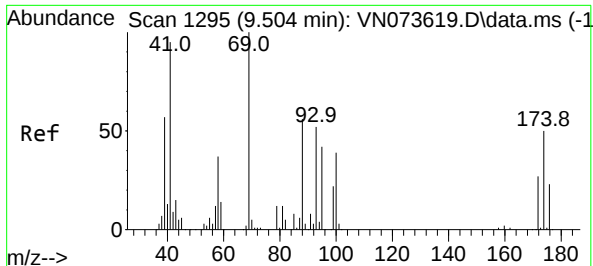

#49
1,4-Dioxane
Concen: 4.142 ug/l
RT: 9.557 min Scan# 11
Delta R.T. 0.053 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion: 88 Resp: 550
Ion Ratio Lower Upper
88 100
43 529856.5 20.2 30.4#
58 2546.9 54.2 81.4#

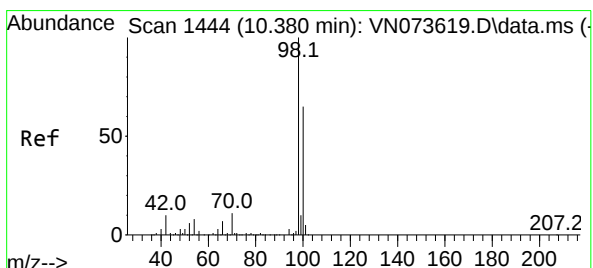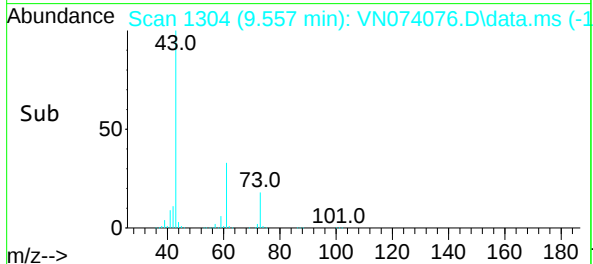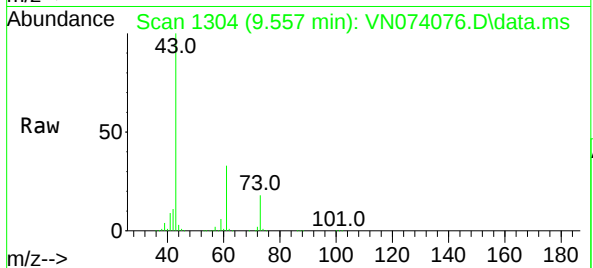

#50
Toluene-d8
Concen: 47.860 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.001 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 98 Resp: 806956
Ion Ratio Lower Upper
98 100
100 64.6 52.6 78.8


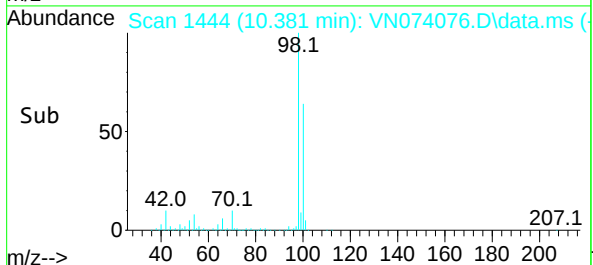

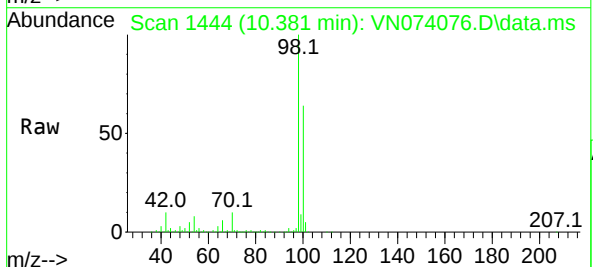




#51
4-Methyl-2-Pentanone
Concen: 3.428 ug/l
RT: 10.275 min Scan# 1426
Delta R.T. -0.000 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion: 43 Resp: 24184
Ion Ratio Lower Upper
43 100
58 29.3 34.1 51.1#

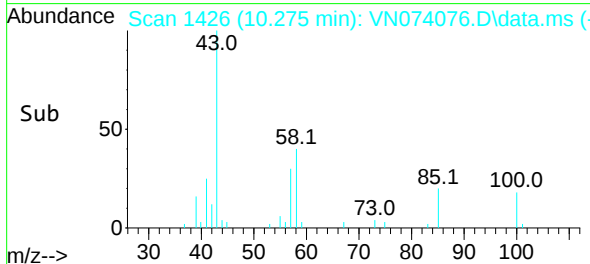

#52
Toluene
Concen: 2.294 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.000 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 92 Resp: 30025
Ion Ratio Lower Upper
92 100
91 178.8 138.6 207.8


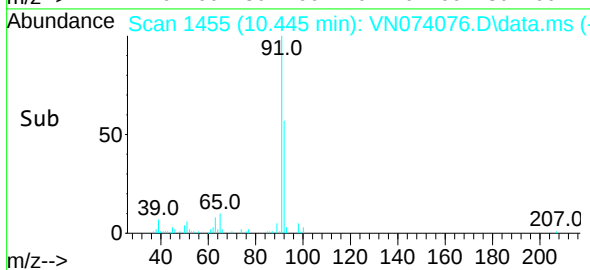

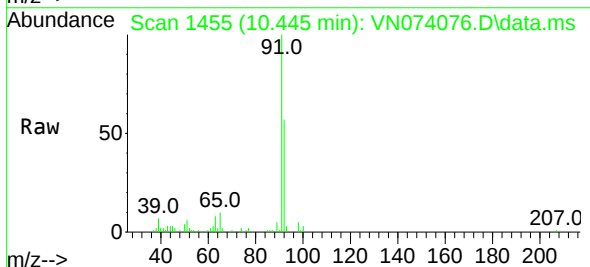




#53
t-1,3-Dichloropropene
Concen: 0.247 ug/l
RT: 10.557 min Scan# 1410
Delta R.T. -0.106 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion: 75 Resp: 1726
Ion Ratio Lower Upper
75 100
77 77.9 25.6 38.4#

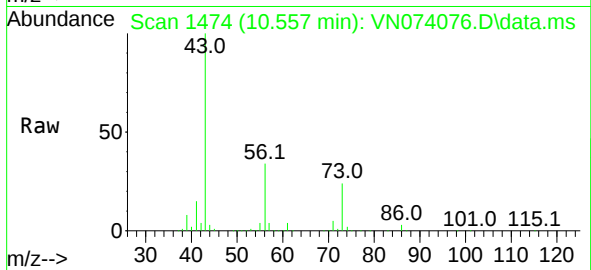

#54
cis-1,3-Dichloropropene
Concen: 13.207 ug/l
RT: 10.187 min Scan# 1411
Delta R.T. 0.060 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 75 Resp: 100797
Ion Ratio Lower Upper
75 100
77 0.5 25.2 37.8#
39 26.4 35.7 53.5#


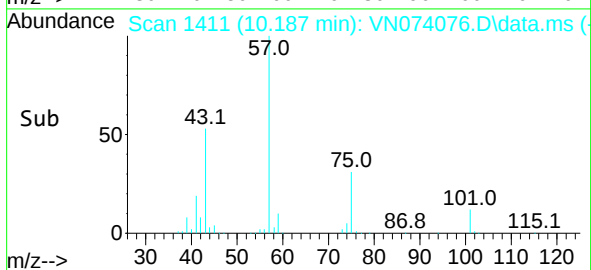

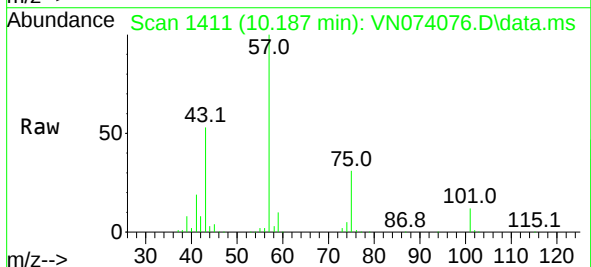


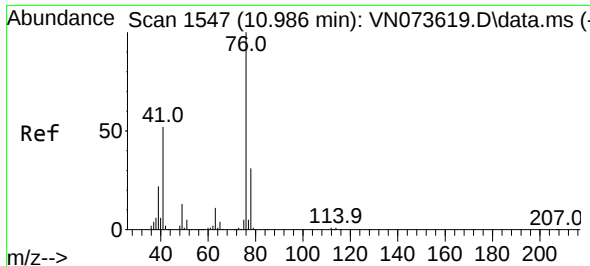

#57
1,3-Dichloropropane
Concen: 1.835 ug/l
RT: 11.034 min Scan# 1555
Delta R.T. 0.048 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion: 76 Resp: 15189
Ion Ratio Lower Upper
76 100
78 0.4 26.2 39.2#

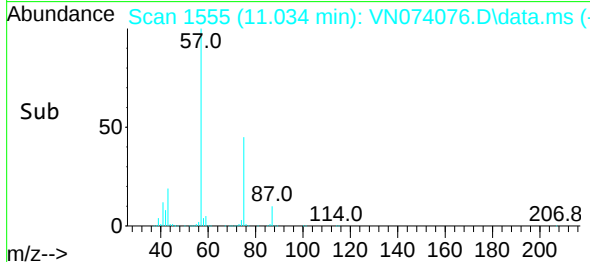

#59
2-Hexanone
Concen: 32.889 ug/l
RT: 11.034 min Scan# 1555
Delta R.T. 0.007 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 43 Resp: 178593
Ion Ratio Lower Upper
43 100
58 22.7 29.7 89.1#


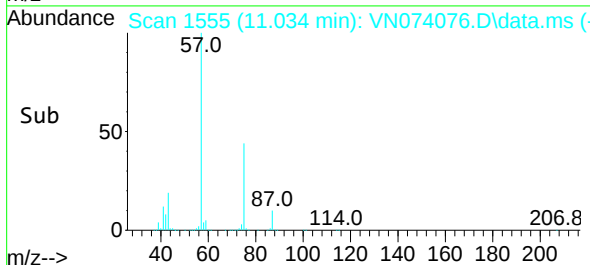

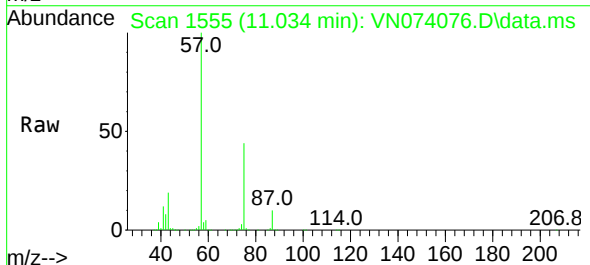




#62
4-Bromofluorobenzene
Concen: 59.421 ug/l
RT: 12.675 min Scan# 1834
Delta R.T. 0.001 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion: 95 Resp: 332502
Ion Ratio Lower Upper
95 100
174 89.8 0.0 167.6
176 86.2 0.0 163.4

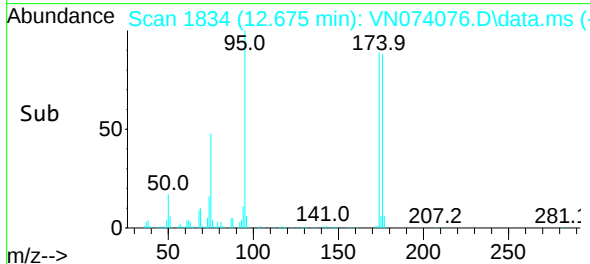

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion: 117 Resp: 732223
Ion Ratio Lower Upper
117 100
82 52.5 44.2 66.2
119 32.8 25.4 38.0

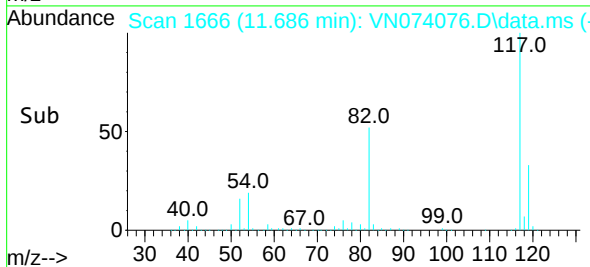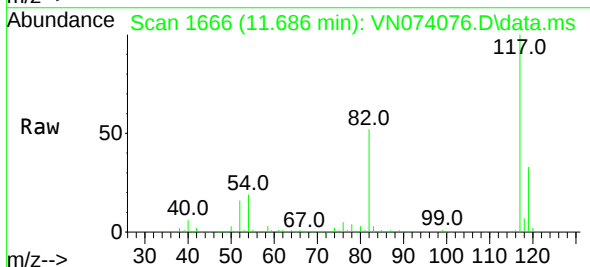

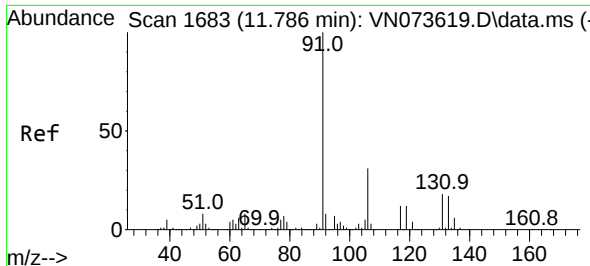

#67

Ethyl Benzene

Concen: 0.287 ug/l

RT: 11.781 min Scan# 1

Delta R.T. -0.005 min

Lab File: VN074076.D

Acq: 23 Aug 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :





SB-7

Tgt Ion: 91 Resp: 7426

Ion Ratio Lower Upper

91 100

106 32.7 24.9 37.3

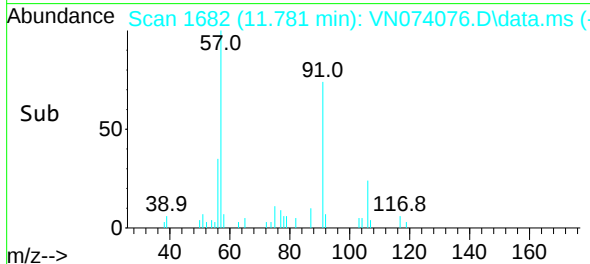

#68

m/p-Xylenes

Concen: 0.995 ug/l

RT: 11.886 min Scan# 1700

Delta R.T. -0.012 min

Lab File: VN074076.D




Acq: 23 Aug 2022 18:29


Tgt Ion:106 Resp: 10467

Ion Ratio Lower Upper

106 100

91 205.6 158.9 238.3


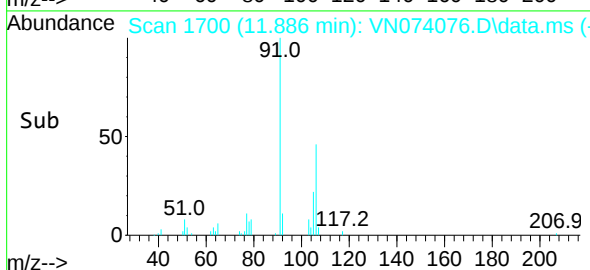

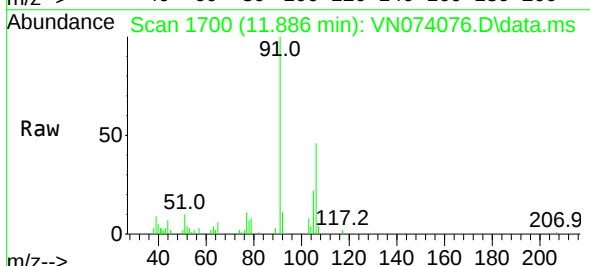




#69
o-Xylene
Concen: 0.655 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. -0.005 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion:106 Resp: 6908
Ion Ratio Lower Upper
106 100
91 220.8 106.0 318.0



#70
Styrene
Concen: 0.373 ug/l
RT: 12.233 min Scan# 1759
Delta R.T. 0.000 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion:104 Resp: 6159
Ion Ratio Lower Upper
104 100
78 52.7 39.5 59.3
103 58.0 44.0 66.0


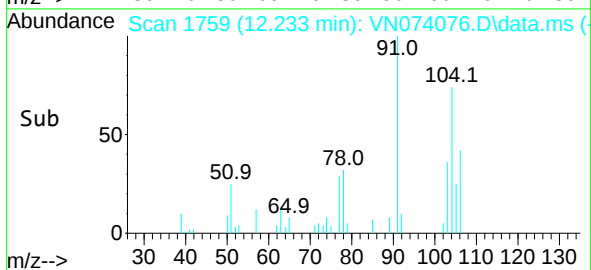






#71
Bromoform
Concen: 0.304 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.271 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion:173 Resp: 1602
Ion Ratio Lower Upper
173 100
175 907.0 24.6 73.6#
254 0.0 0.1 0.1#

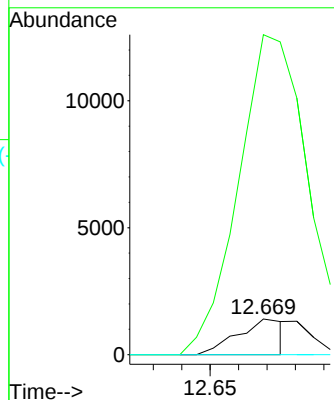

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.001 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion:152 Resp: 374981
Ion Ratio Lower Upper
152 100
115 55.3 28.9 86.7
150 158.3 0.0 356.2


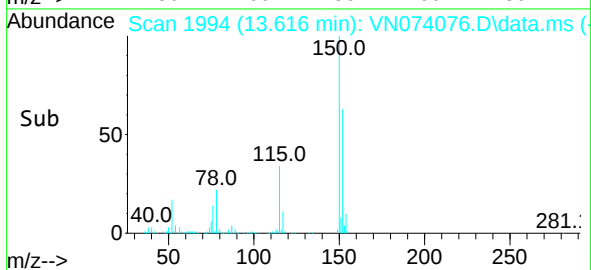
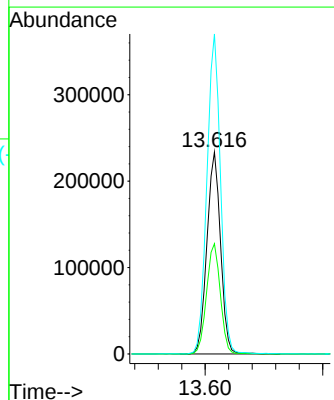





#74
N-amy1 acetate
Concen: 4.710 ug/l
RT: 12.139 min Scan# 11
Delta R.T. -0.188 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
SB-7


Tgt Ion:	43	Resp:	48615
Ion	Ratio	Lower	Upper
43	100		
70	2.9	39.0	58.4#
55	6.5	21.1	31.7#
61	11.2	21.1	31.7#

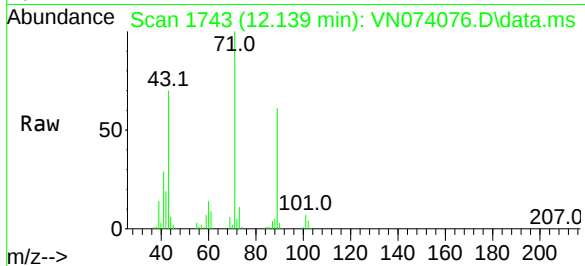

#76
1,2,3-Trichloropropane
Concen: 20.605 ug/l
RT: 12.675 min Scan# 1834
Delta R.T. -0.146 min
Lab File: VN074076.D
Acq: 23 Aug 2022 18:29

Tgt Ion:	75	Resp:	160598
Ion	Ratio	Lower	Upper
75	100		
77	1.3	98.5	295.5#


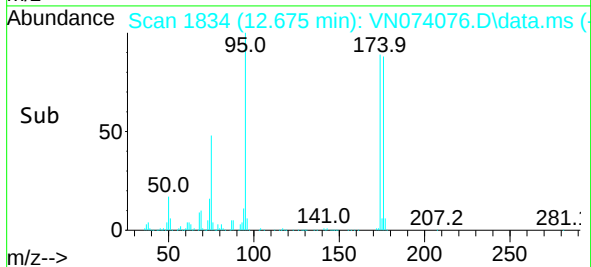

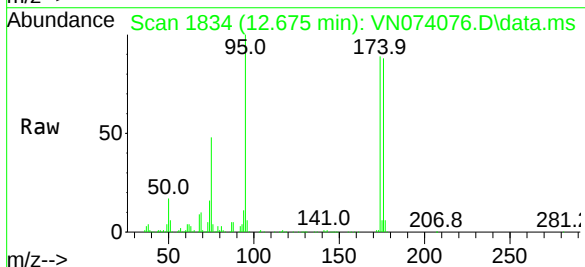




#81
 trans-1,4-Dichloro-2-butene
 Concen: 58.606 ug/l
 RT: 12.675 min Scan# 1816
 Delta R.T. 0.107 min
 Lab File: VN074076.D
 Acq: 23 Aug 2022 18:29

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-7

Tgt Ion: 75 Resp: 160598
 Ion Ratio Lower Upper
 75 100
 53 0.0 78.0 117.0#
 89 0.0 37.2 55.8#

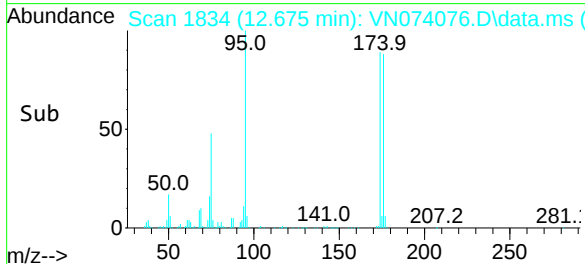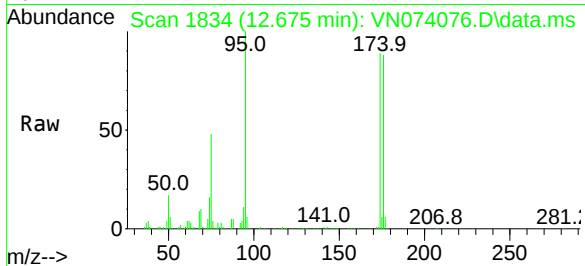

#95
 Naphthalene
 Concen: 2.988 ug/l
 RT: 15.439 min Scan# 2304
 Delta R.T. 0.006 min
 Lab File: VN074076.D
 Acq: 23 Aug 2022 18:29

Tgt Ion:128 Resp: 78460
 Ion Ratio Lower Upper
 128 100
 127 13.4 10.3 15.5
 129 11.2 8.6 13.0

