


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082420\
Data File : VN063086.D
Acq On : 24 Aug 2020 10:35
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Title : SW846 8260
Last Update : Wed Aug 19 06:09:27 2020

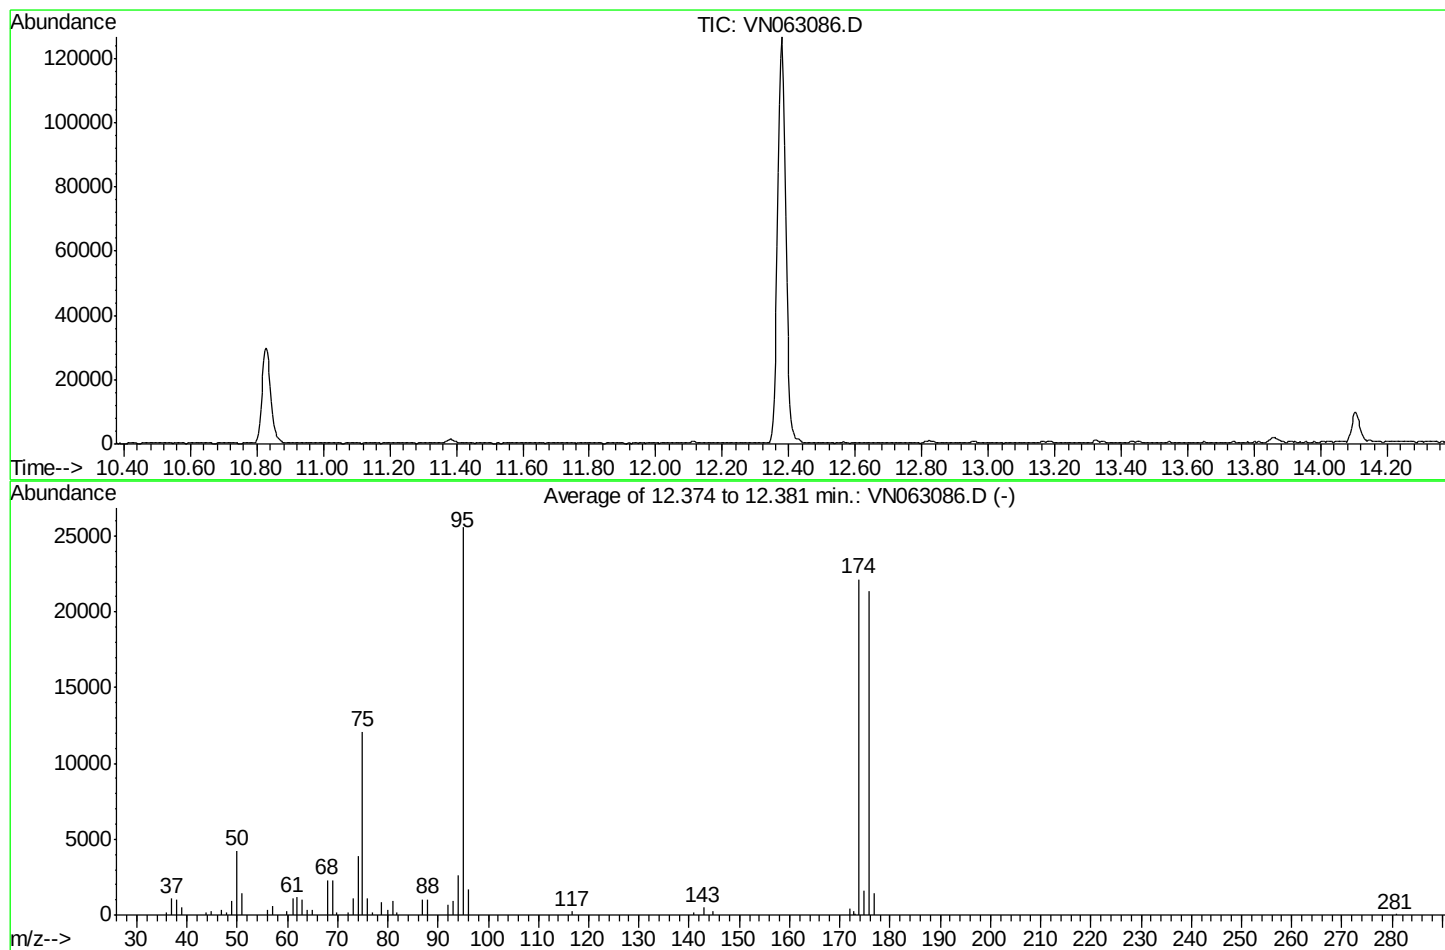

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3285

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	4268	PASS
75	95	30	60	47.3	12102	PASS
95	95	100	100	100.0	25584	PASS
96	95	5	9	6.7	1719	PASS
173	174	0.00	2	1.0	221	PASS
174	95	50	100	86.5	22133	PASS
175	174	5	9	7.3	1612	PASS
176	174	95	101	96.6	21378	PASS
177	176	5	9	6.8	1463	PASS