

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082421\
 Data File : VN068288.D
 Acq On : 24 Aug 2021 16:07
 Operator : JC/MD
 Sample : M3463-17
 Misc : 3.8g/5.0mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SWCS-18-0002

Quant Time: Aug 25 03:11:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 13:09:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.080	168	441310	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.965	114	736307	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	820897	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.680	152	352450	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.432	65	256330	54.400	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 108.800%			
35) Dibromofluoromethane	8.018	113	228705	49.474	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 98.940%			
50) Toluene-d8	10.440	98	935219	53.095	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 106.180%			
62) 4-Bromofluorobenzene	12.733	95	353489	60.284	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 120.560%			
Target Compounds						
5) Bromomethane	2.807	94	1363	Below Cal		92
6) Chloroethane	2.925	64	46	Below Cal	#	83
13) Acrolein	4.036	56	109	Below Cal	#	14
16) Acetone	4.296	43	8436	6.132	ug/l	99
17) Carbon Disulfide	4.470	76	2296	0.248	ug/l	# 74
18) Methyl Acetate	4.848	43	39122	8.454	ug/l	# 89
20) Methylene Chloride	5.058	84	4923	Below Cal	#	78
25) 2-Butanone	7.348	43	4138	1.930	ug/l	97
27) cis-1,2-Dichloroethene	7.316	96	2109	0.440	ug/l	78
31) Cyclohexane	8.078	56	7768	1.252	ug/l	# 11
32) 1,1,1-Trichloroethane	8.000	97	3045	0.429	ug/l	# 49
36) 1,1-Dichloropropene	8.078	75	29471	4.896	ug/l	# 53
37) Ethyl Acetate	7.348	43	4138	0.807	ug/l	# 69
38) Carbon Tetrachloride	8.075	117	40829	5.881	ug/l	# 17
43) Isopropyl Acetate	8.617	43	2170	0.264	ug/l	# 58
44) Trichloroethene	9.212	130	5692	1.030	ug/l	85
51) 4-Methyl-2-Pentanone	10.336	43	1077	0.213	ug/l	# 39
52) Toluene	10.505	92	30548	2.439	ug/l	98
59) 2-Hexanone	11.095	43	1208	0.345	ug/l	93
60) Dibromochloromethane	10.977	129	5171	0.916	ug/l	# 11
64) Tetrachloroethene	10.977	164	5083	0.801	ug/l	97
65) Chlorobenzene	11.773	112	7805	0.464	ug/l	100
68) m/p-Xylenes	11.953	106	2846	0.257	ug/l	79
71) Bromoform	12.733	173	1549	0.305	ug/l	# 1
76) 1,2,3-Trichloropropane	12.733	75	182339	31.126	ug/l	# 100
81) trans-1,4-Dichloro-2-b...	12.733	75	182339	101.974	ug/l	# 6
84) 1,2,4-Trimethylbenzene	13.366	105	4801	0.243	ug/l	98
93) 1,2,4-Trichlorobenzene	15.265	180	759	2.807	ug/l	# 72
95) Naphthalene	15.509	128	6927	3.812	ug/l	# 86
96) 1,2,3-Trichlorobenzene	15.710	180	549	2.924	ug/l	# 47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082421\
Data File : VN068288.D
Acq On : 24 Aug 2021 16:07
Operator : JC/MD
Sample : M3463-17
Misc : 3.8g/5.0mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002

Quant Time: Aug 25 03:11:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 13:09:49 2021
Response via : Initial Calibration

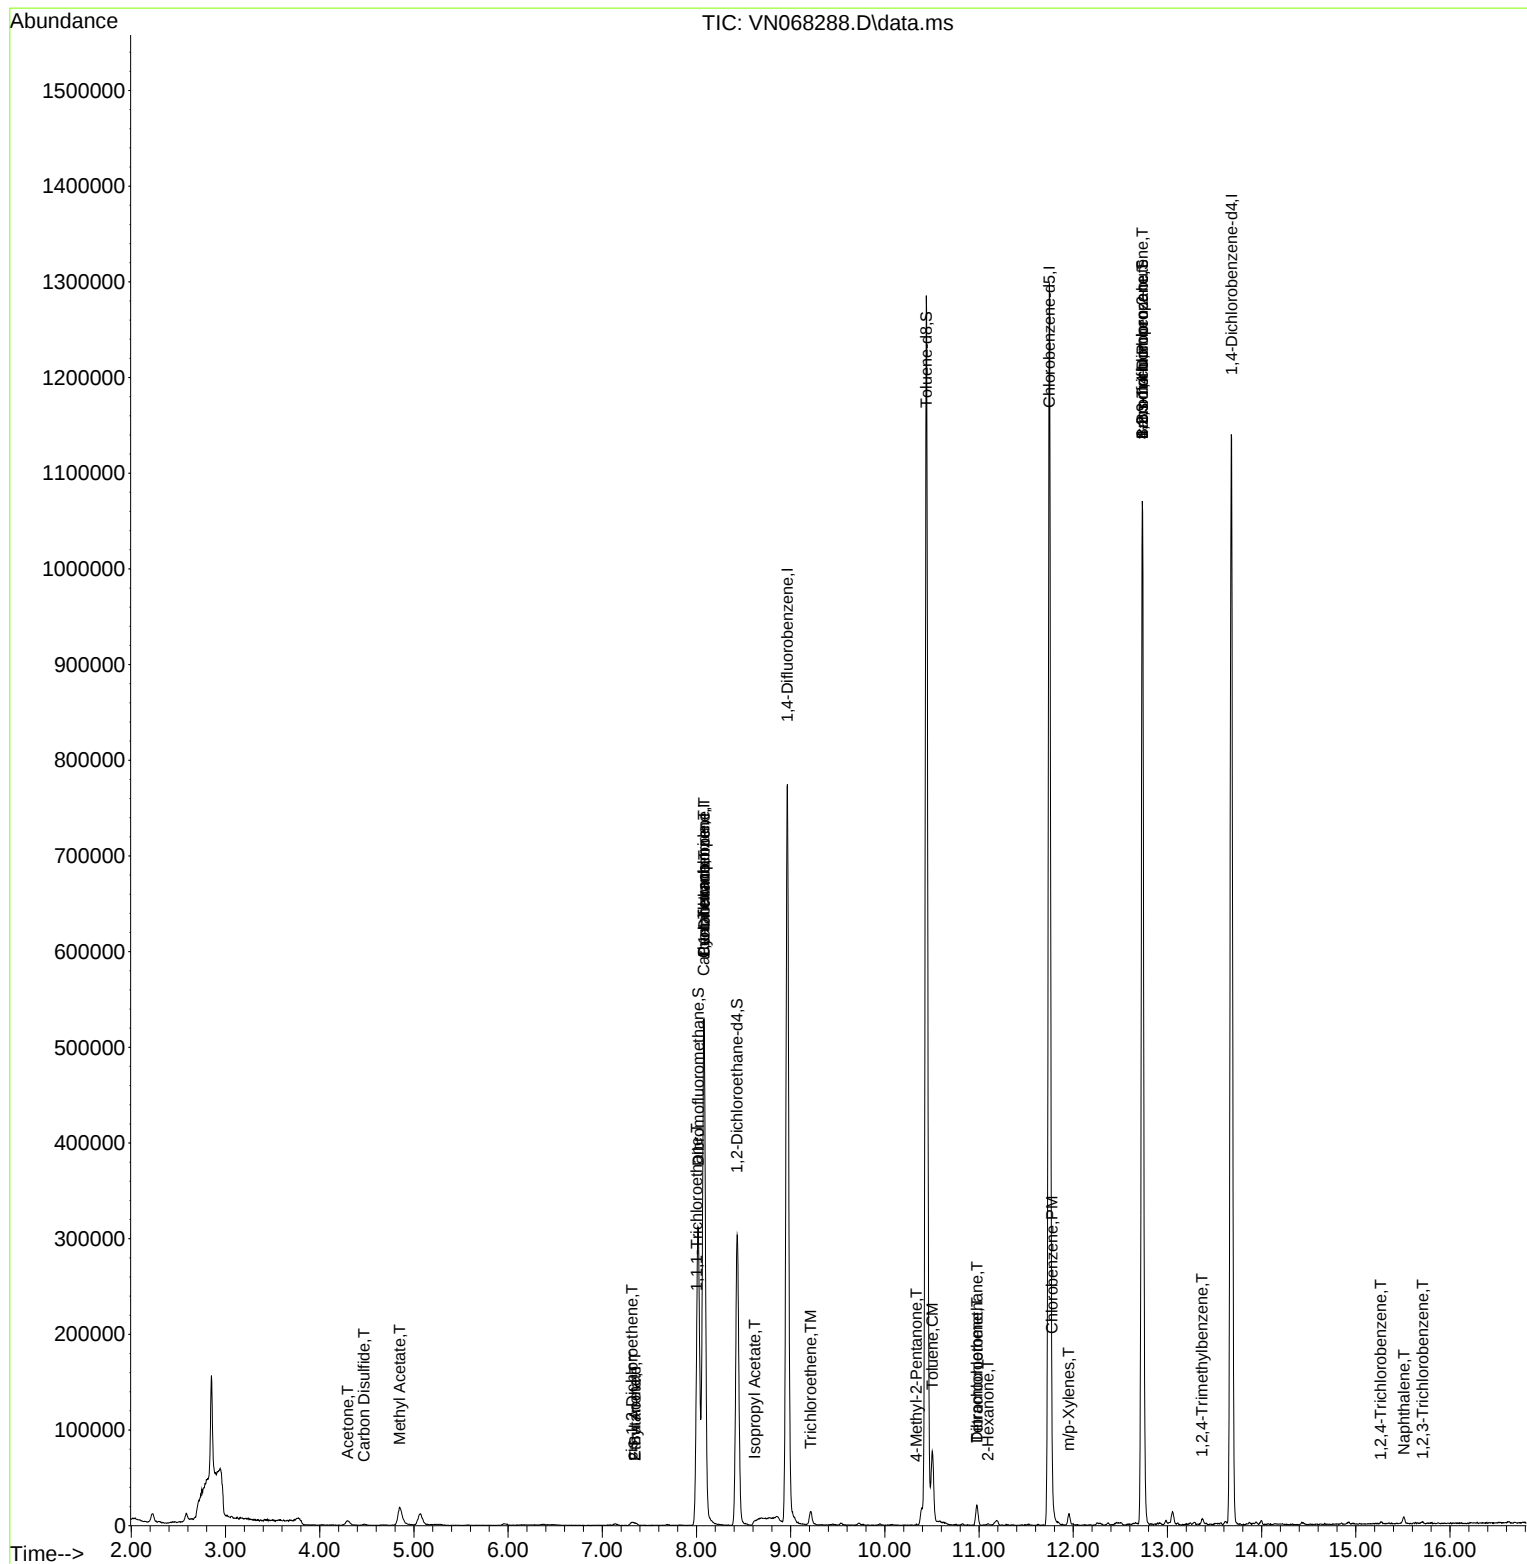



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.080 min Scan# 2271

Delta R.T. -0.008 min





Lab File: VN068288.D

Acq: 24 Aug 2021 16:07

Tgt Ion:168 Resp: 441310

Ion Ratio Lower Upper

168 100
99 50.5 62.9 94.3#

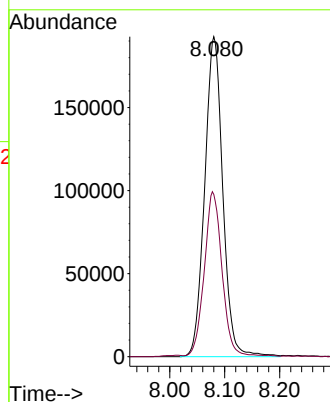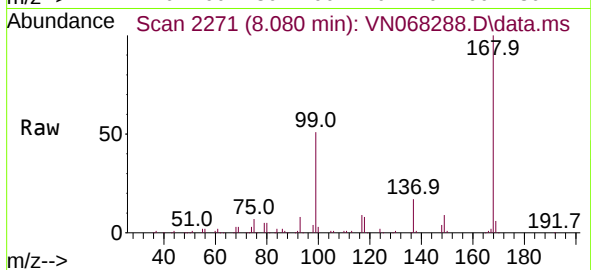

#5

Bromomethane

Concen: Below Cal

RT: 2.807 min Scan# 305

Delta R.T. -0.030 min




Lab File: VN068288.D


Acq: 24 Aug 2021 16:07

Tgt Ion: 94 Resp: 1363

Ion Ratio Lower Upper

94 100
96 84.0 73.7 110.5


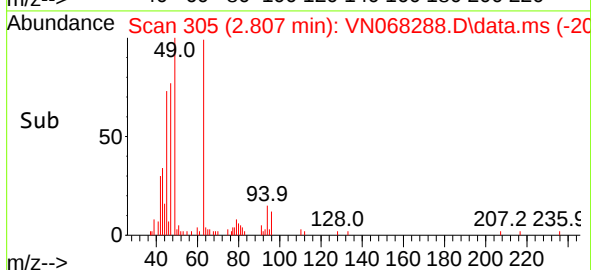
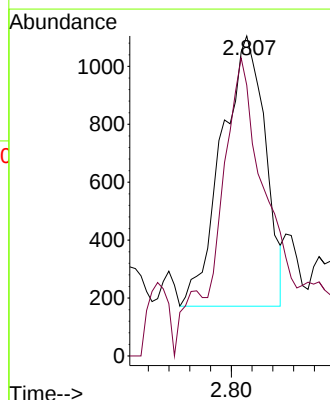





#6
Chloroethane
Concen: Below Cal
RT: 2.925 min Scan# 349
Delta R.T. -0.081 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion: 64 Resp: 46
Ion Ratio Lower Upper
64 100
66 21.6 24.7 37.1#

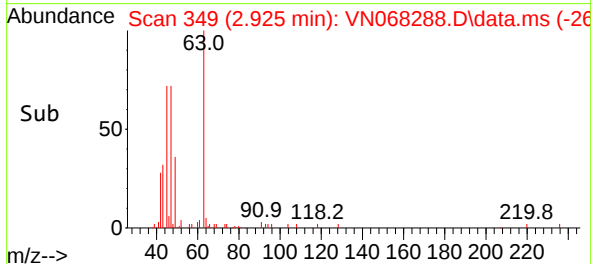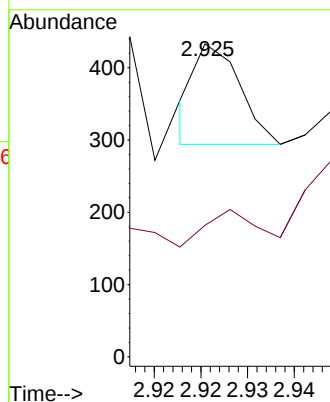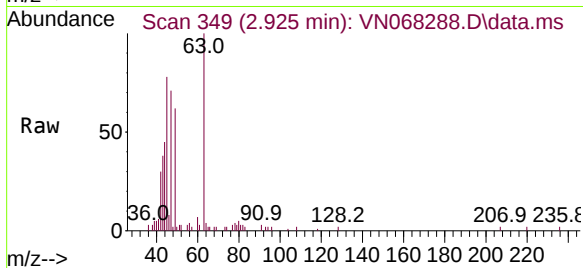

#13
Acrolein
Concen: Below Cal
RT: 4.036 min Scan# 763
Delta R.T. -0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 56 Resp: 109
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.0#


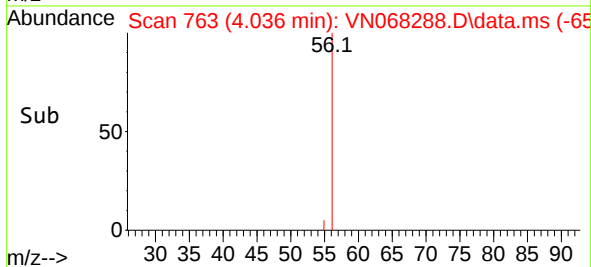
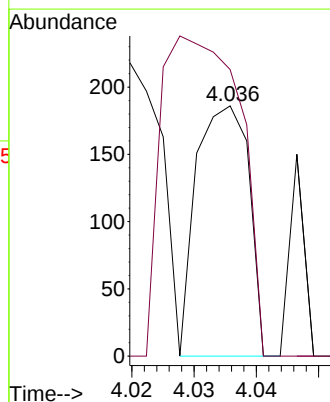
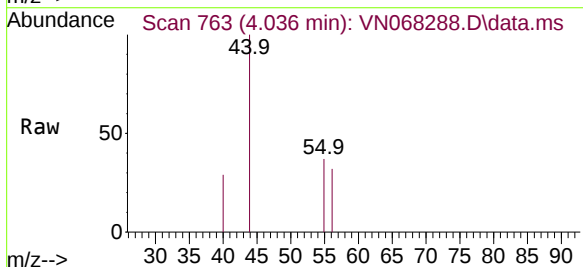




#16
Acetone
Concen: 6.132 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.008 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion: 43 Resp: 8436
Ion Ratio Lower Upper
43 100
58 25.7 21.2 31.8

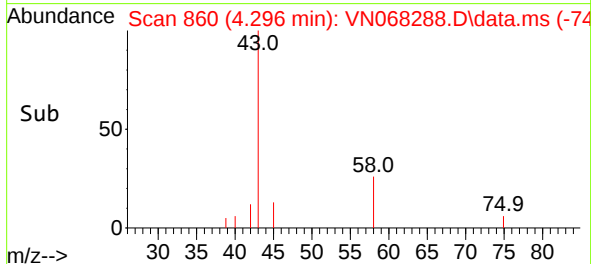

#17
Carbon Disulfide
Concen: 0.248 ug/l
RT: 4.470 min Scan# 925
Delta R.T. -0.051 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 76 Resp: 2296
Ion Ratio Lower Upper
76 100
78 0.0 7.7 11.5#

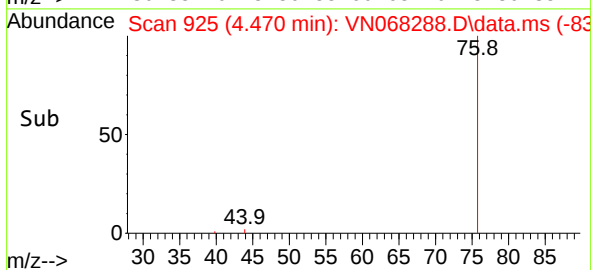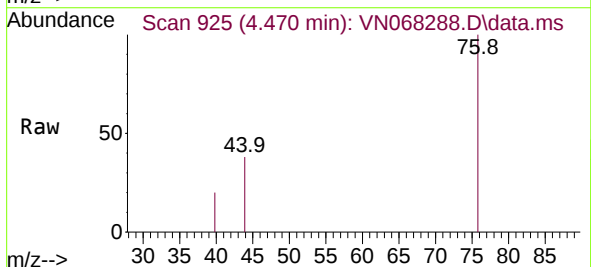

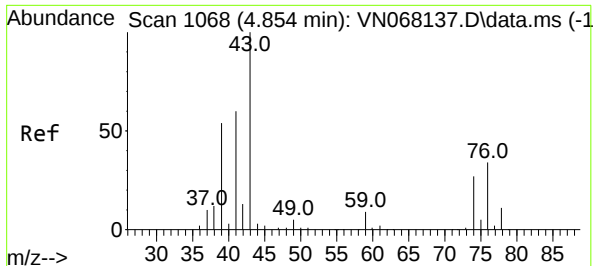

#18

Methyl Acetate

Concen: 8.454 ug/l

RT: 4.848 min Scan# 1066

Delta R.T. -0.006 min

Lab File: VN068288.D

Acq: 24 Aug 2021 16:07

Instrument :

MSVOA_N

ClientSampleId :





SWCS-18-0002

Tgt Ion: 43 Resp: 39122

Ion Ratio Lower Upper

43 100

74 27.0 17.4 26.0#

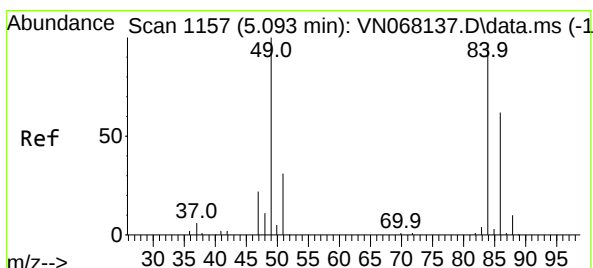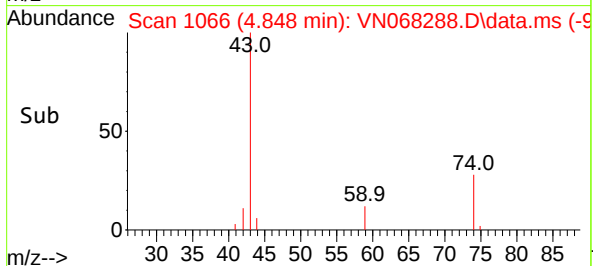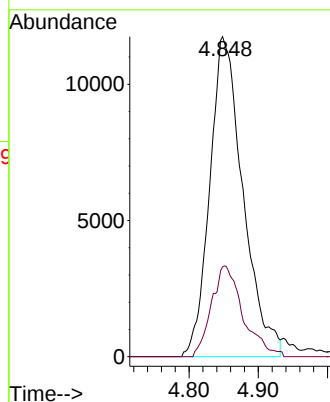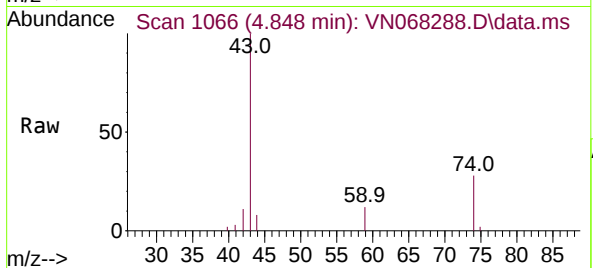

#20

Methylene Chloride

Concen: Below Cal

RT: 5.058 min Scan# 1144

Delta R.T. -0.035 min

Lab File: VN068288.D

Acq: 24 Aug 2021 16:07

Tgt Ion: 84 Resp: 4923




Ion Ratio Lower Upper


84 100

49 98.2 110.9 166.3#

51 31.2 32.6 49.0#

86 64.4 51.6 77.4


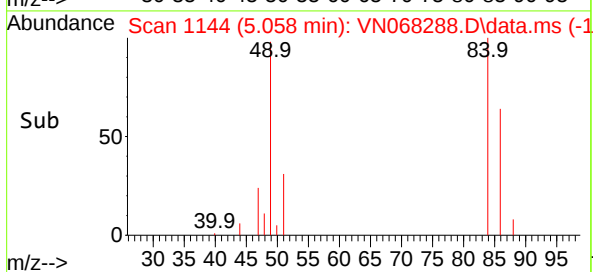
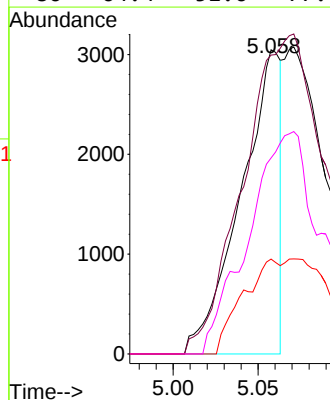
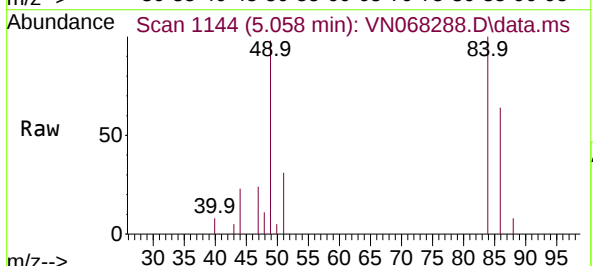


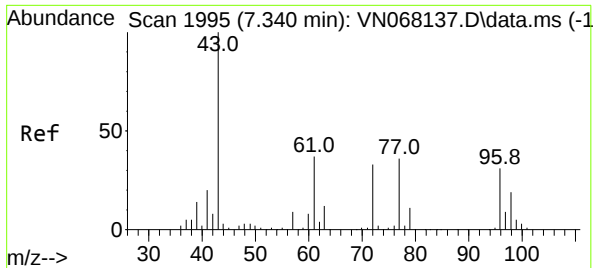

#25
2-Butanone
Concen: 1.930 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. 0.008 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampled :
SWCS-18-0002


Tgt Ion: 43 Resp: 4138
Ion Ratio Lower Upper
43 100
72 26.3 19.7 29.5

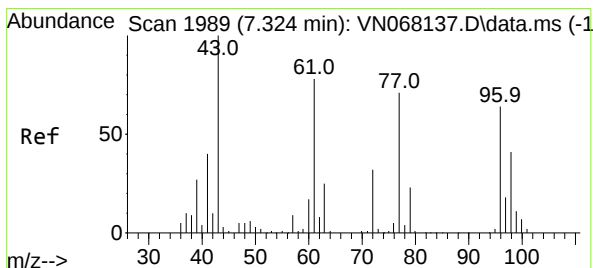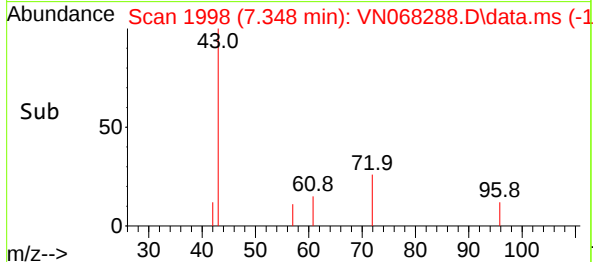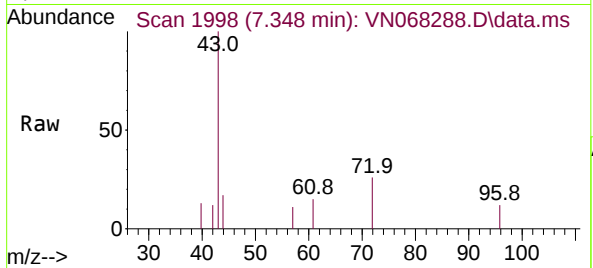

#27
cis-1,2-Dichloroethene
Concen: 0.440 ug/l
RT: 7.316 min Scan# 1986
Delta R.T. -0.008 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 96 Resp: 2109
Ion Ratio Lower Upper
96 100
61 127.1 0.0 338.8
98 65.1 0.0 129.8


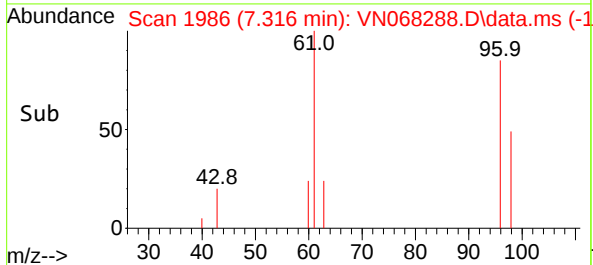

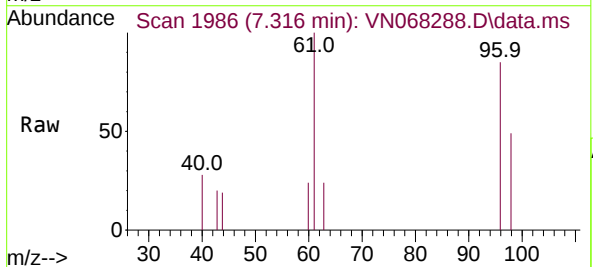




#31
Cyclohexane
Concen: 1.252 ug/l
RT: 8.078 min Scan# 2270
Delta R.T. -0.016 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion: 56 Resp: 7768
Ion Ratio Lower Upper
56 100
69 167.3 27.3 40.9#
84 107.1 64.9 97.3#

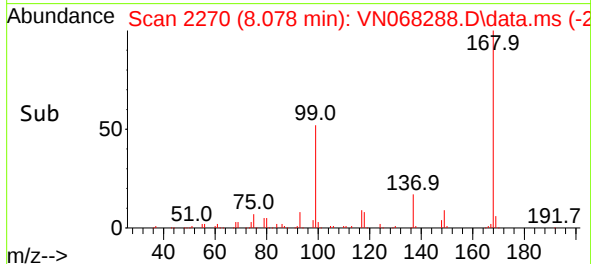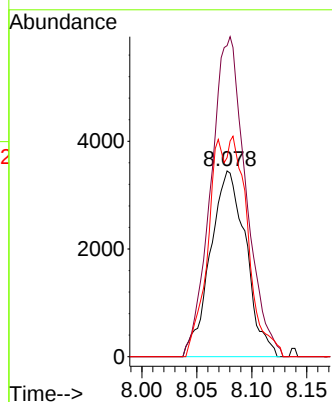

#32
1,1,1-Trichloroethane
Concen: 0.429 ug/l
RT: 8.000 min Scan# 2241
Delta R.T. -0.016 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 97 Resp: 3045
Ion Ratio Lower Upper
97 100
99 0.0 50.2 75.2#
61 39.4 38.2 57.2


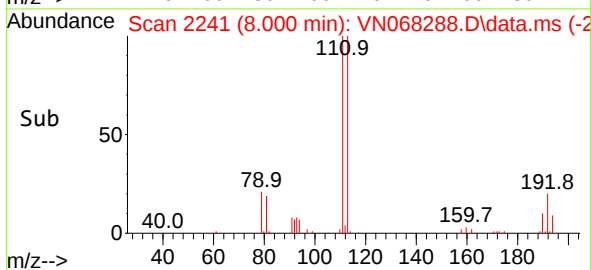

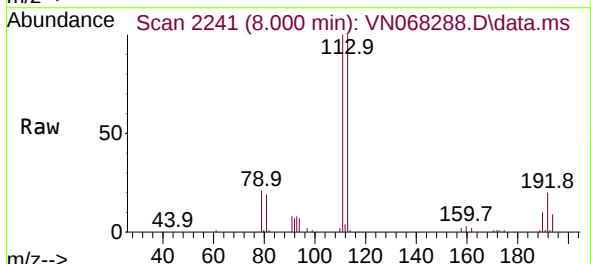


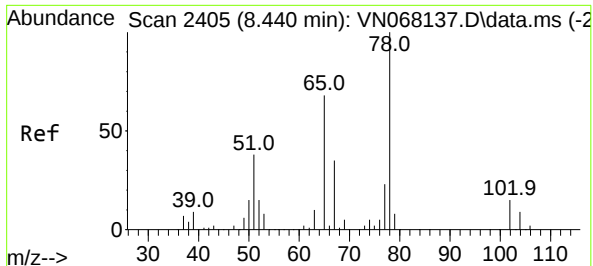

#33
1,2-Dichloroethane-d4
Concen: 54.400 ug/l
RT: 8.432 min Scan# 2402
Delta R.T. -0.008 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion: 65 Resp: 256330
Ion Ratio Lower Upper
65 100
67 52.7 0.0 98.6

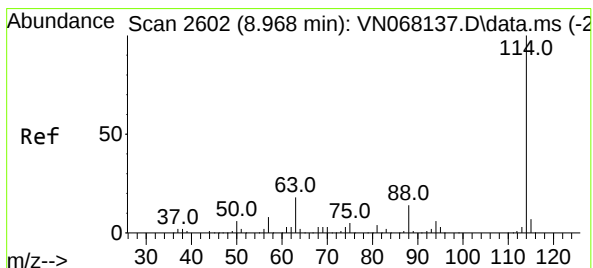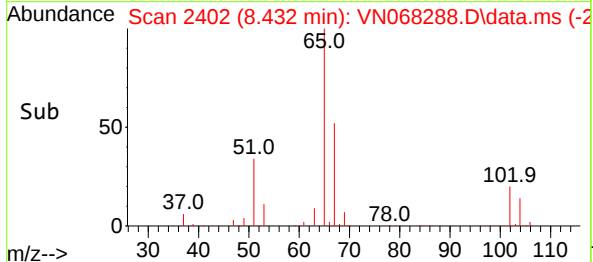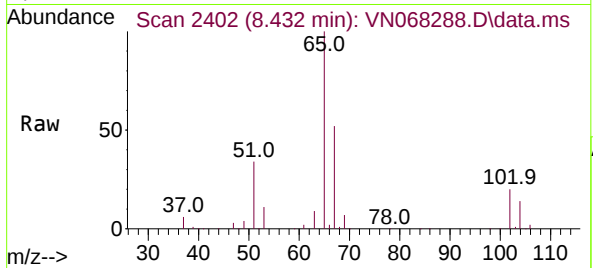

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.965 min Scan# 2601
Delta R.T. -0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 114 Resp: 736307
Ion Ratio Lower Upper
114 100
63 16.8 0.0 49.0
88 13.8 0.0 36.6


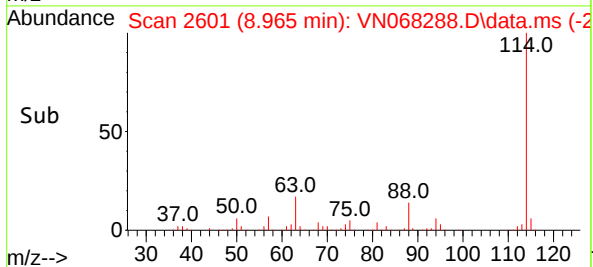

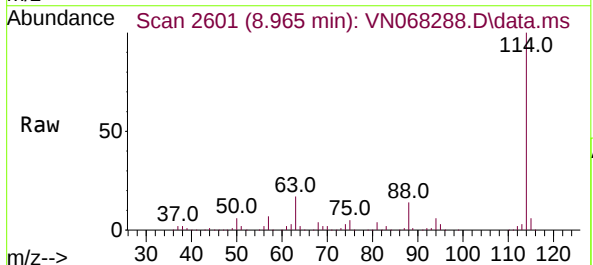




#35
Dibromofluoromethane
Concen: 49.474 ug/l
RT: 8.018 min Scan# 2248
Delta R.T. -0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion:113 Resp: 228705
Ion Ratio Lower Upper
113 100
111 102.6 83.8 125.8
192 20.8 13.4 20.0#

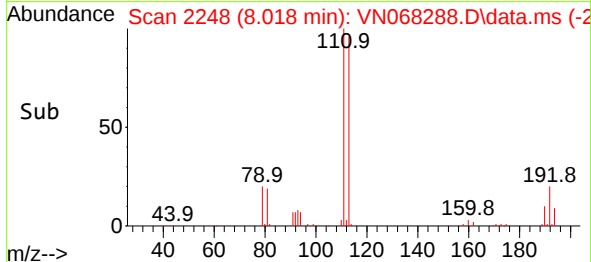

#36
1,1-Dichloropropene
Concen: 4.896 ug/l
RT: 8.078 min Scan# 2270
Delta R.T. -0.146 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 75 Resp: 29471
Ion Ratio Lower Upper
75 100
110 9.8 15.7 47.0#
77 0.0 24.6 37.0#

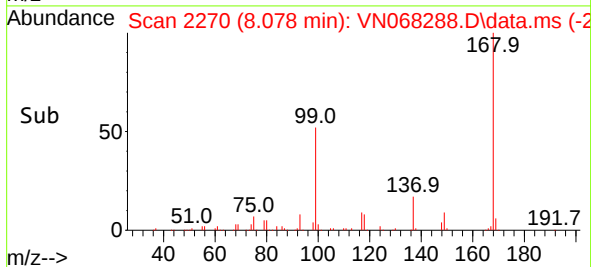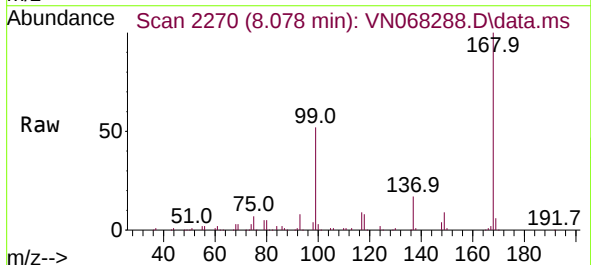

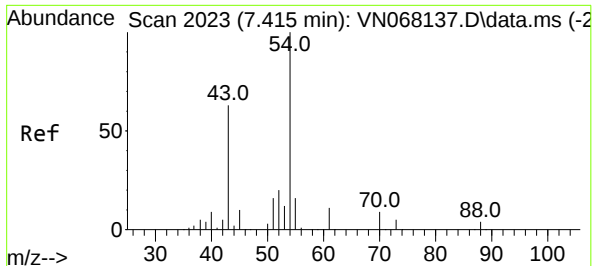

#37

Ethyl Acetate

Concen: 0.807 ug/l

RT: 7.348 min Scan# 1998

Delta R.T. -0.067 min

Lab File: VN068288.D

Acq: 24 Aug 2021 16:07





Instrument :

MSVOA_N

ClientSampleId :

SWCS-18-0002

Tgt Ion:	43	Resp:	4138
Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.6	16.0#
70	0.0	8.1	12.1#

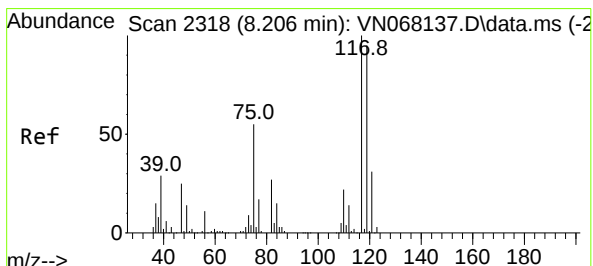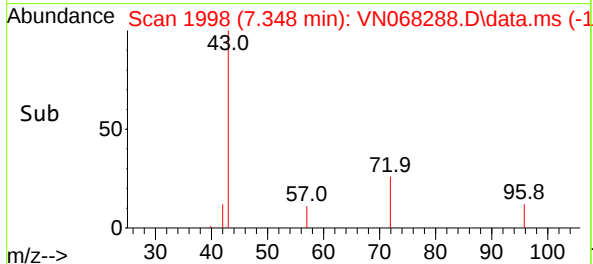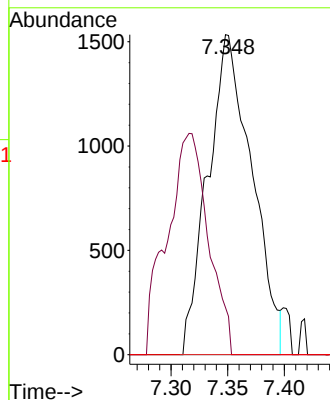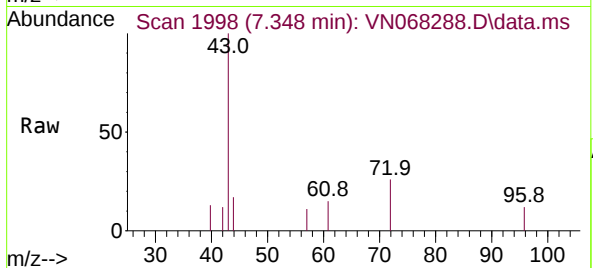

#38

Carbon Tetrachloride

Concen: 5.881 ug/l




RT: 8.075 min Scan# 2269


Delta R.T. -0.131 min

Lab File: VN068288.D

Acq: 24 Aug 2021 16:07

Tgt Ion:	117	Resp:	40829
Ion	Ratio	Lower	Upper
117	100		
119	6.1	75.4	113.2#
121	0.0	23.5	35.3#


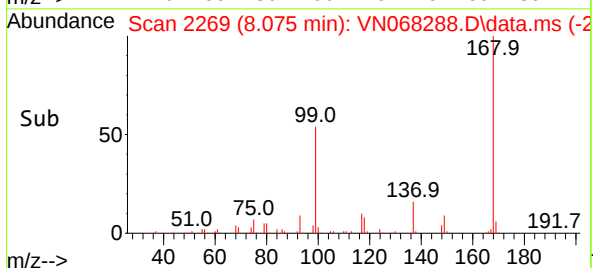
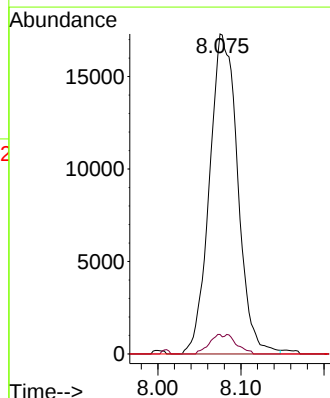
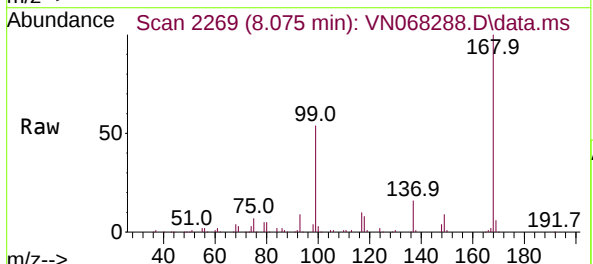




#43
Isopropyl Acetate
Concen: 0.264 ug/l
RT: 8.617 min Scan# 2471
Delta R.T. 0.051 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion: 43 Resp: 2170
Ion Ratio Lower Upper
43 100
61 0.0 19.0 28.4#
87 0.0 9.5 14.3#

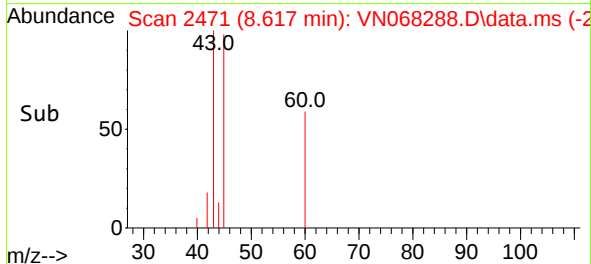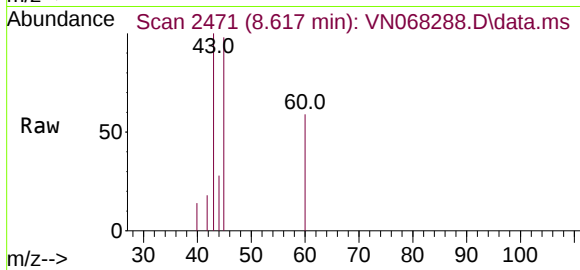

#44
Trichloroethene
Concen: 1.030 ug/l
RT: 9.212 min Scan# 2693
Delta R.T. -0.006 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 130 Resp: 5692
Ion Ratio Lower Upper
130 100
95 101.0 0.0 234.4


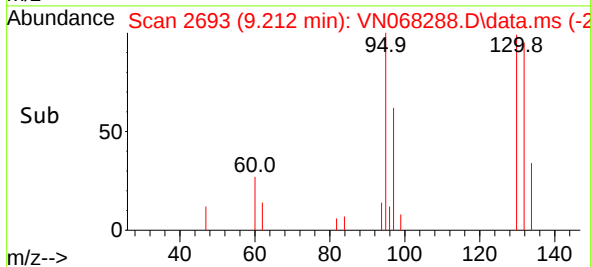

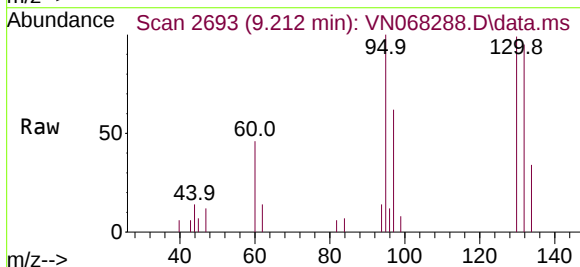




#50
Toluene-d8
Concen: 53.095 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. -0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion: 98 Resp: 935219
Ion Ratio Lower Upper
98 100
100 64.4 51.7 77.5

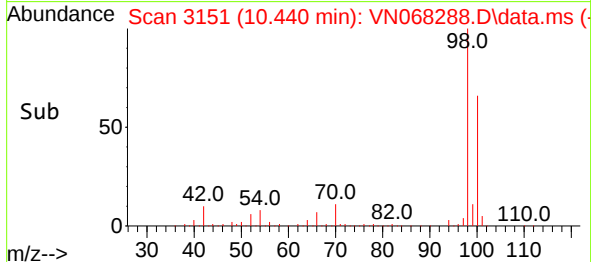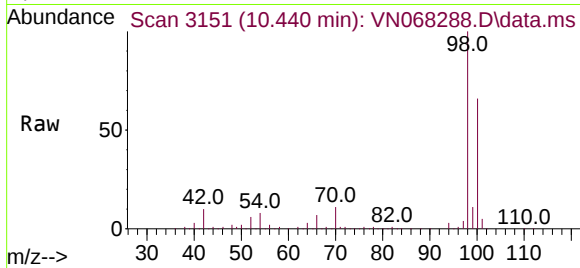

#51
4-Methyl-2-Pentanone
Concen: 0.213 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 43 Resp: 1077
Ion Ratio Lower Upper
43 100
58 0.0 28.6 43.0#


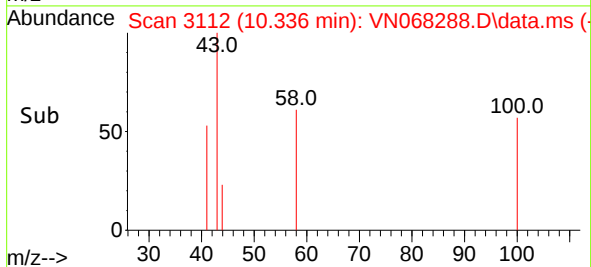

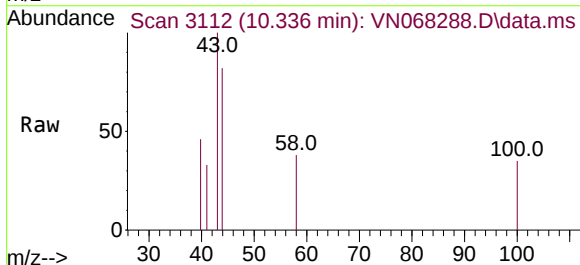




#52
Toluene
Concen: 2.439 ug/l
RT: 10.505 min Scan# 3175
Delta R.T. -0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion: 92 Resp: 30548
Ion Ratio Lower Upper
92 100
91 176.7 139.6 209.4

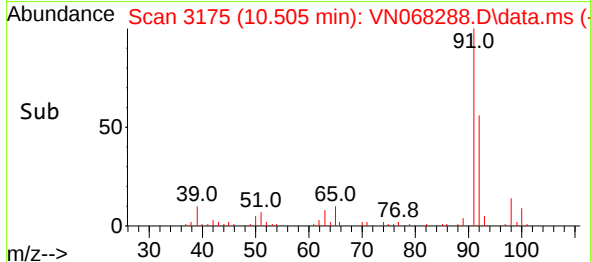

#59
2-Hexanone
Concen: 0.345 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 43 Resp: 1208
Ion Ratio Lower Upper
43 100
58 44.7 24.7 74.1


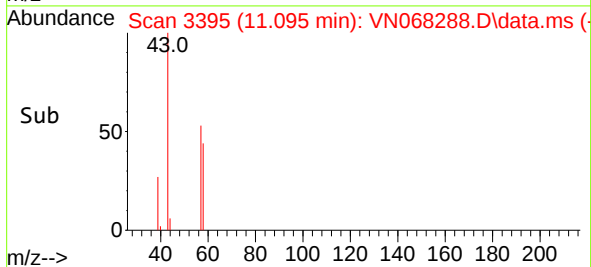

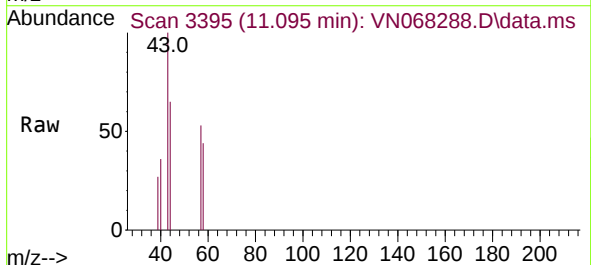




#60
Dibromochloromethane
Concen: 0.916 ug/l
RT: 10.977 min Scan# 3351
Delta R.T. -0.263 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion:129 Resp: 5171
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

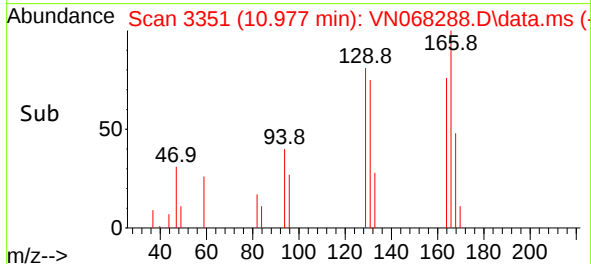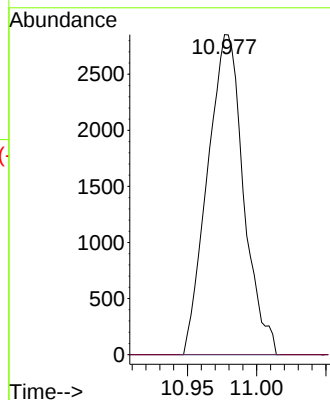

#62
4-Bromofluorobenzene
Concen: 60.284 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.001 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 95 Resp: 353489
Ion Ratio Lower Upper
95 100
174 94.8 0.0 122.0
176 89.0 0.0 117.6



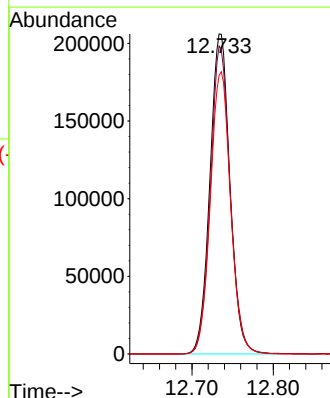
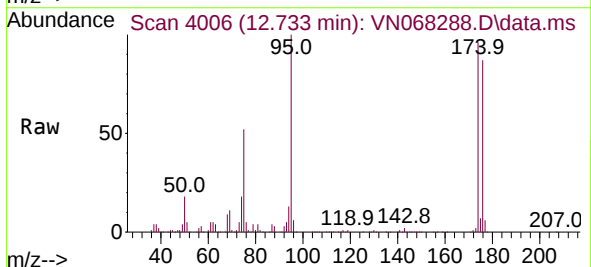


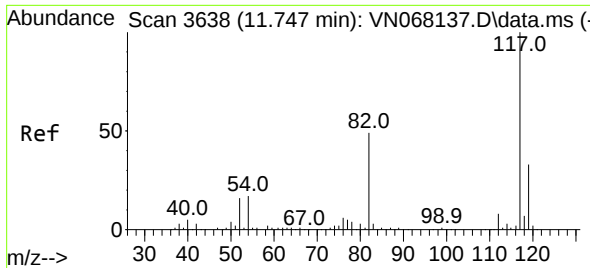

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.001 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion:117 Resp: 820897
Ion Ratio Lower Upper
117 100
82 50.0 53.1 79.7#
119 32.7 25.5 38.3

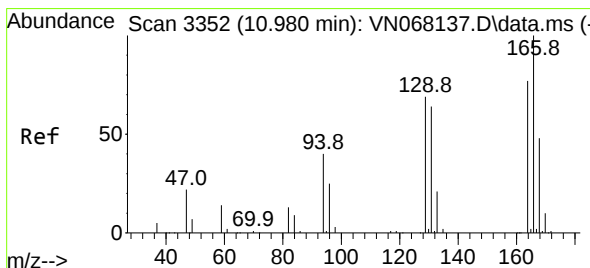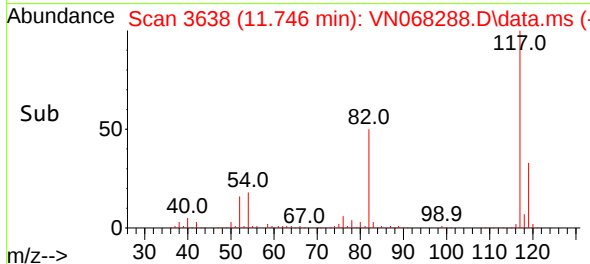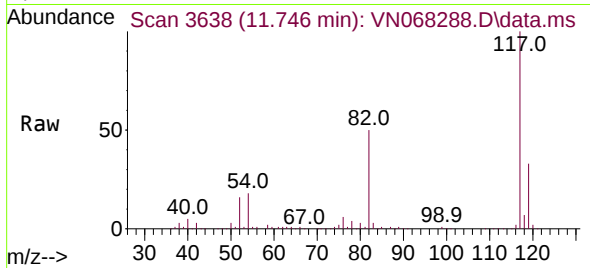

#64
Tetrachloroethene
Concen: 0.801 ug/l
RT: 10.977 min Scan# 3351
Delta R.T. -0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion:164 Resp: 5083
Ion Ratio Lower Upper
164 100
166 132.1 102.1 153.1
129 107.5 86.9 130.3
131 99.4 83.6 125.4


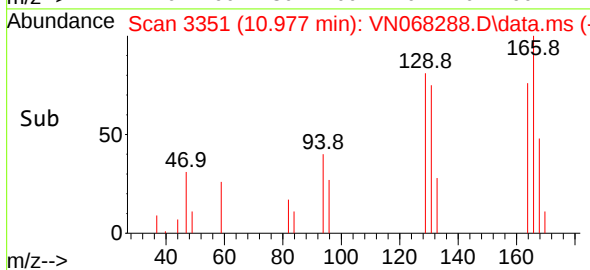

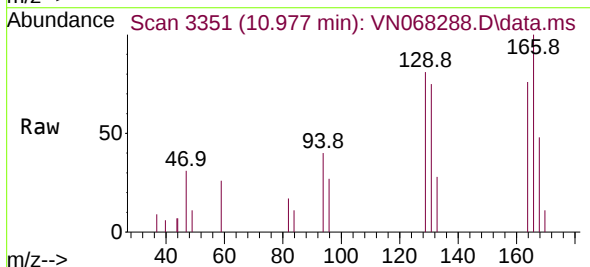




#65
Chlorobenzene
Concen: 0.464 ug/l
RT: 11.773 min Scan# 3648
Delta R.T. 0.000 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampled :
SWCS-18-0002


Tgt Ion:112 Resp: 7805
Ion Ratio Lower Upper
112 100
114 30.8 24.6 37.0

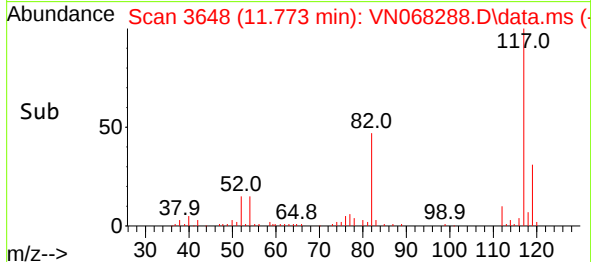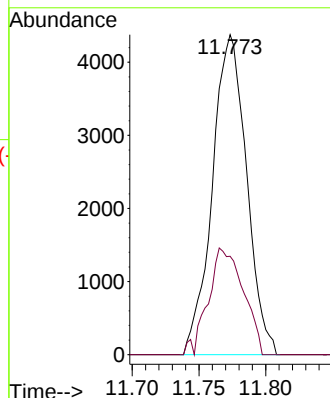

#68
m/p-Xylenes
Concen: 0.257 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. -0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion:106 Resp: 2846
Ion Ratio Lower Upper
106 100
91 191.8 180.6 270.8


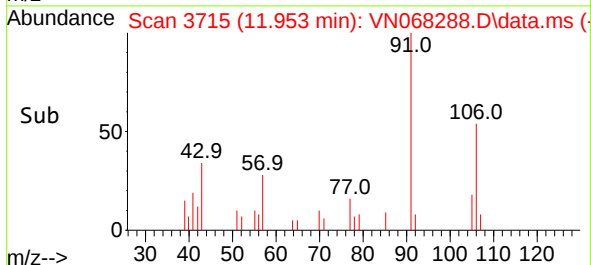
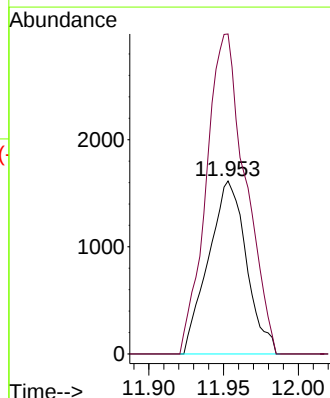
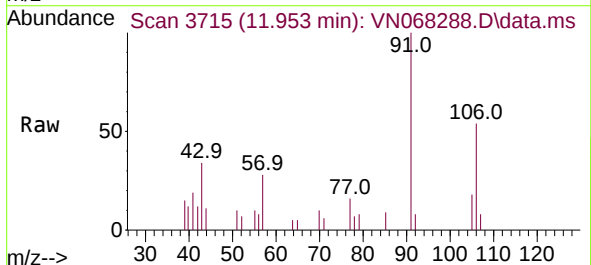


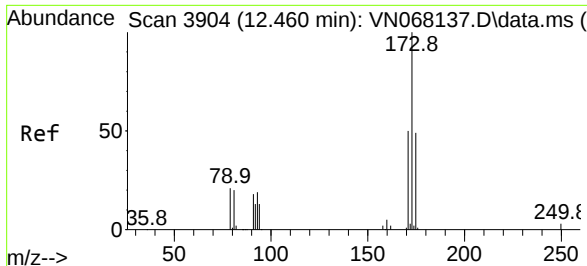

#71
Bromoform
Concen: 0.305 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.273 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampled :
SWCS-18-0002


Tgt Ion:173 Resp: 1549
Ion Ratio Lower Upper
173 100
175 1560.2 23.9 71.8#
254 0.0 0.0 0.0

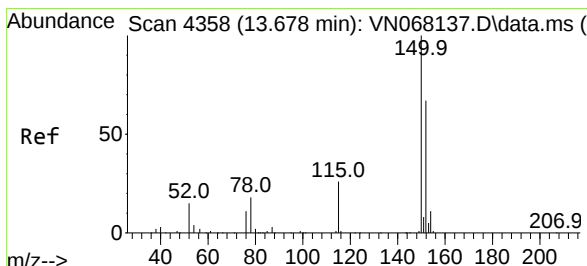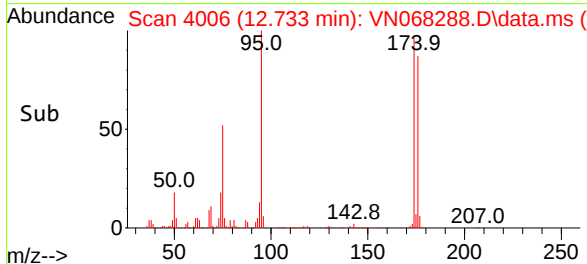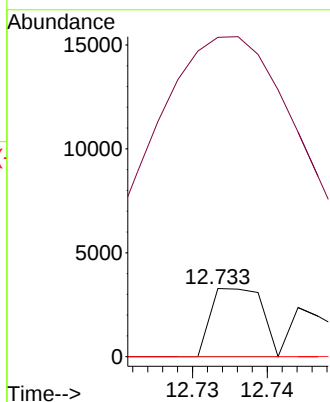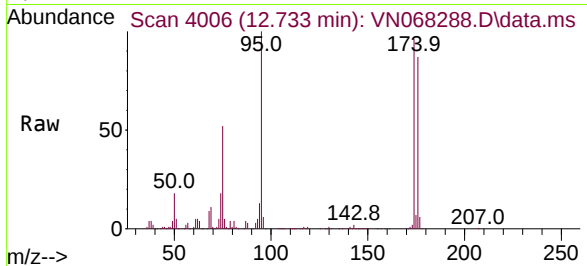

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.680 min Scan# 4359
Delta R.T. 0.002 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion:152 Resp: 352450
Ion Ratio Lower Upper
152 100
115 54.4 36.1 108.5
150 156.9 0.0 351.8


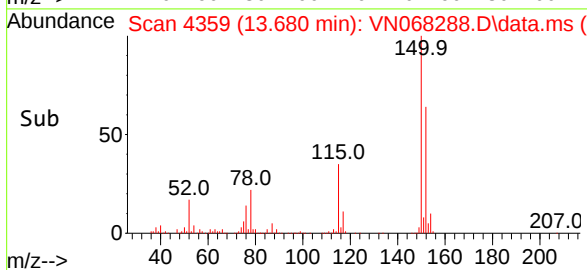
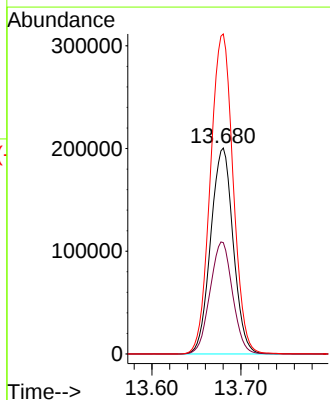
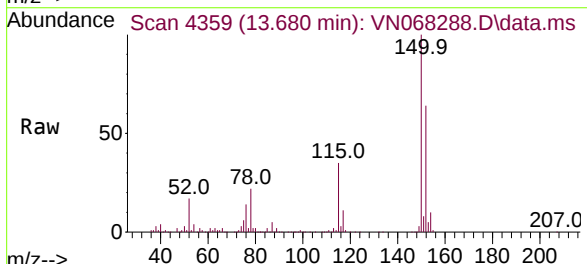


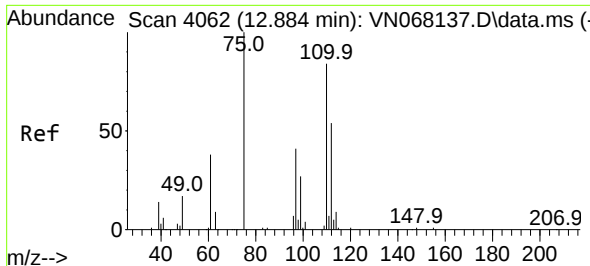

#76
1,2,3-Trichloropropane
Concen: 31.126 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion: 75 Resp: 182339
Ion Ratio Lower Upper
75 100
77 1.1 0.0 0.0#

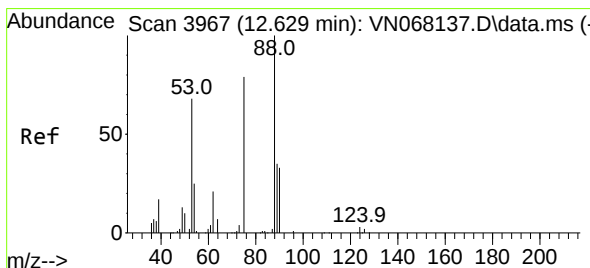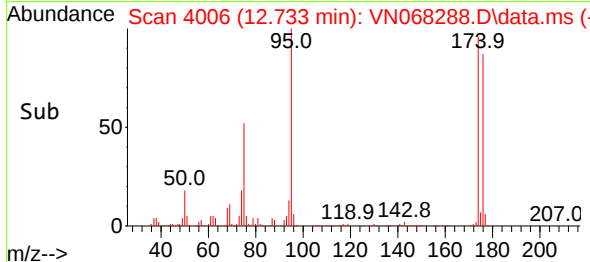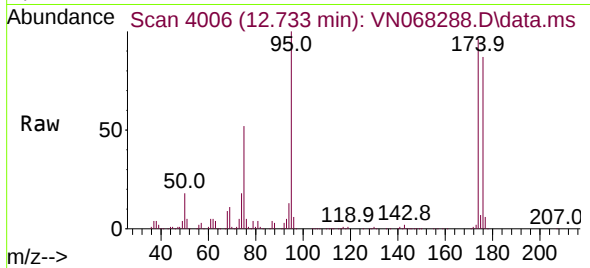

#81
trans-1,4-Dichloro-2-butene
Concen: 101.974 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion: 75 Resp: 182339
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#


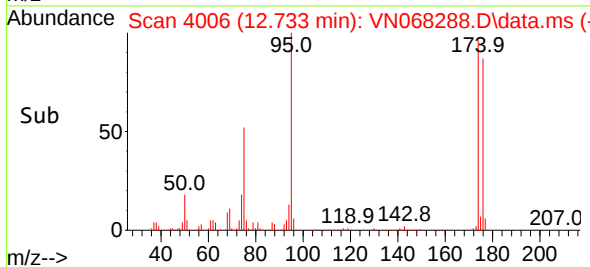

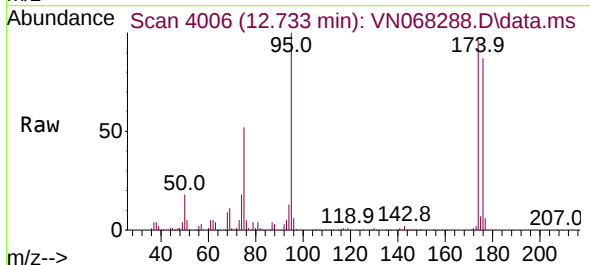




#84
1,2,4-Trimethylbenzene
Concen: 0.243 ug/l
RT: 13.366 min Scan# 4242
Delta R.T. -0.003 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07




Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002


Tgt Ion:105 Resp: 4801
Ion Ratio Lower Upper
105 100
120 42.5 20.6 61.8

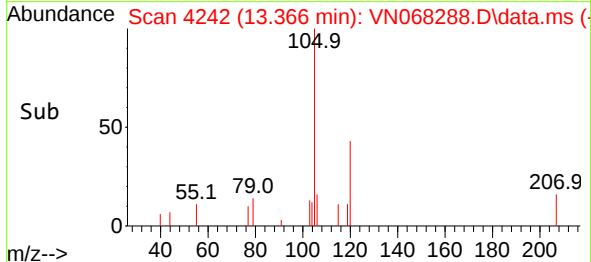

#93
1,2,4-Trichlorobenzene
Concen: 2.807 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion:180 Resp: 759
Ion Ratio Lower Upper
180 100
182 118.3 47.5 142.5
145 11.2 17.2 51.6#


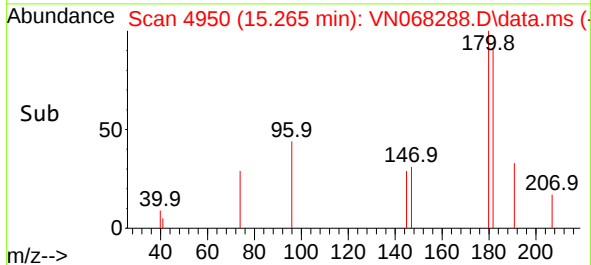

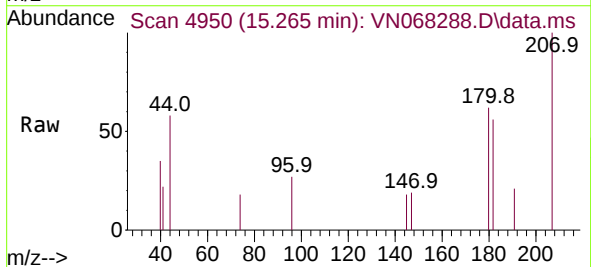




#95
Naphthalene
Concen: 3.812 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Instrument :
MSVOA_N
ClientSampleId :
SWCS-18-0002

Tgt Ion:	128	Resp:	6927
Ion	Ratio	Lower	Upper
128	100		
127	5.8	10.6	15.8#
129	7.7	8.6	12.8#

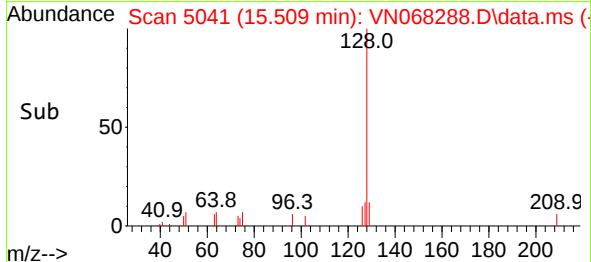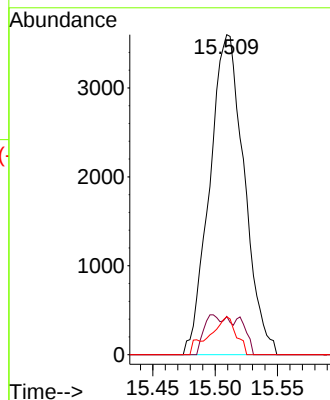

#96
1,2,3-Trichlorobenzene
Concen: 2.924 ug/l
RT: 15.710 min Scan# 5116
Delta R.T. 0.007 min
Lab File: VN068288.D
Acq: 24 Aug 2021 16:07

Tgt Ion:	180	Resp:	549
Ion	Ratio	Lower	Upper
180	100		
182	164.7	47.8	143.3#
145	40.8	18.2	54.6

