

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082422\
 Data File : VN074087.D
 Acq On : 24 Aug 2022 13:22
 Operator : JC\MD
 Sample : N4244-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-105D

Quant Time: Aug 25 07:53:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 16 00:45:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	620526	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	924666	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	757492	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	300417	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	302886	50.114	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	100.220%
35) Dibromofluoromethane	7.951	113	275897	50.453	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.900%
50) Toluene-d8	10.380	98	1022661	48.288	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	96.580%
62) 4-Bromofluorobenzene	12.674	95	303512	43.181	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082422\
Data File : VN074087.D
Acq On : 24 Aug 2022 13:22
Operator : JC\MD
Sample : N4244-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-105D

Quant Time: Aug 25 07:53:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 16 00:45:21 2022
Response via : Initial Calibration




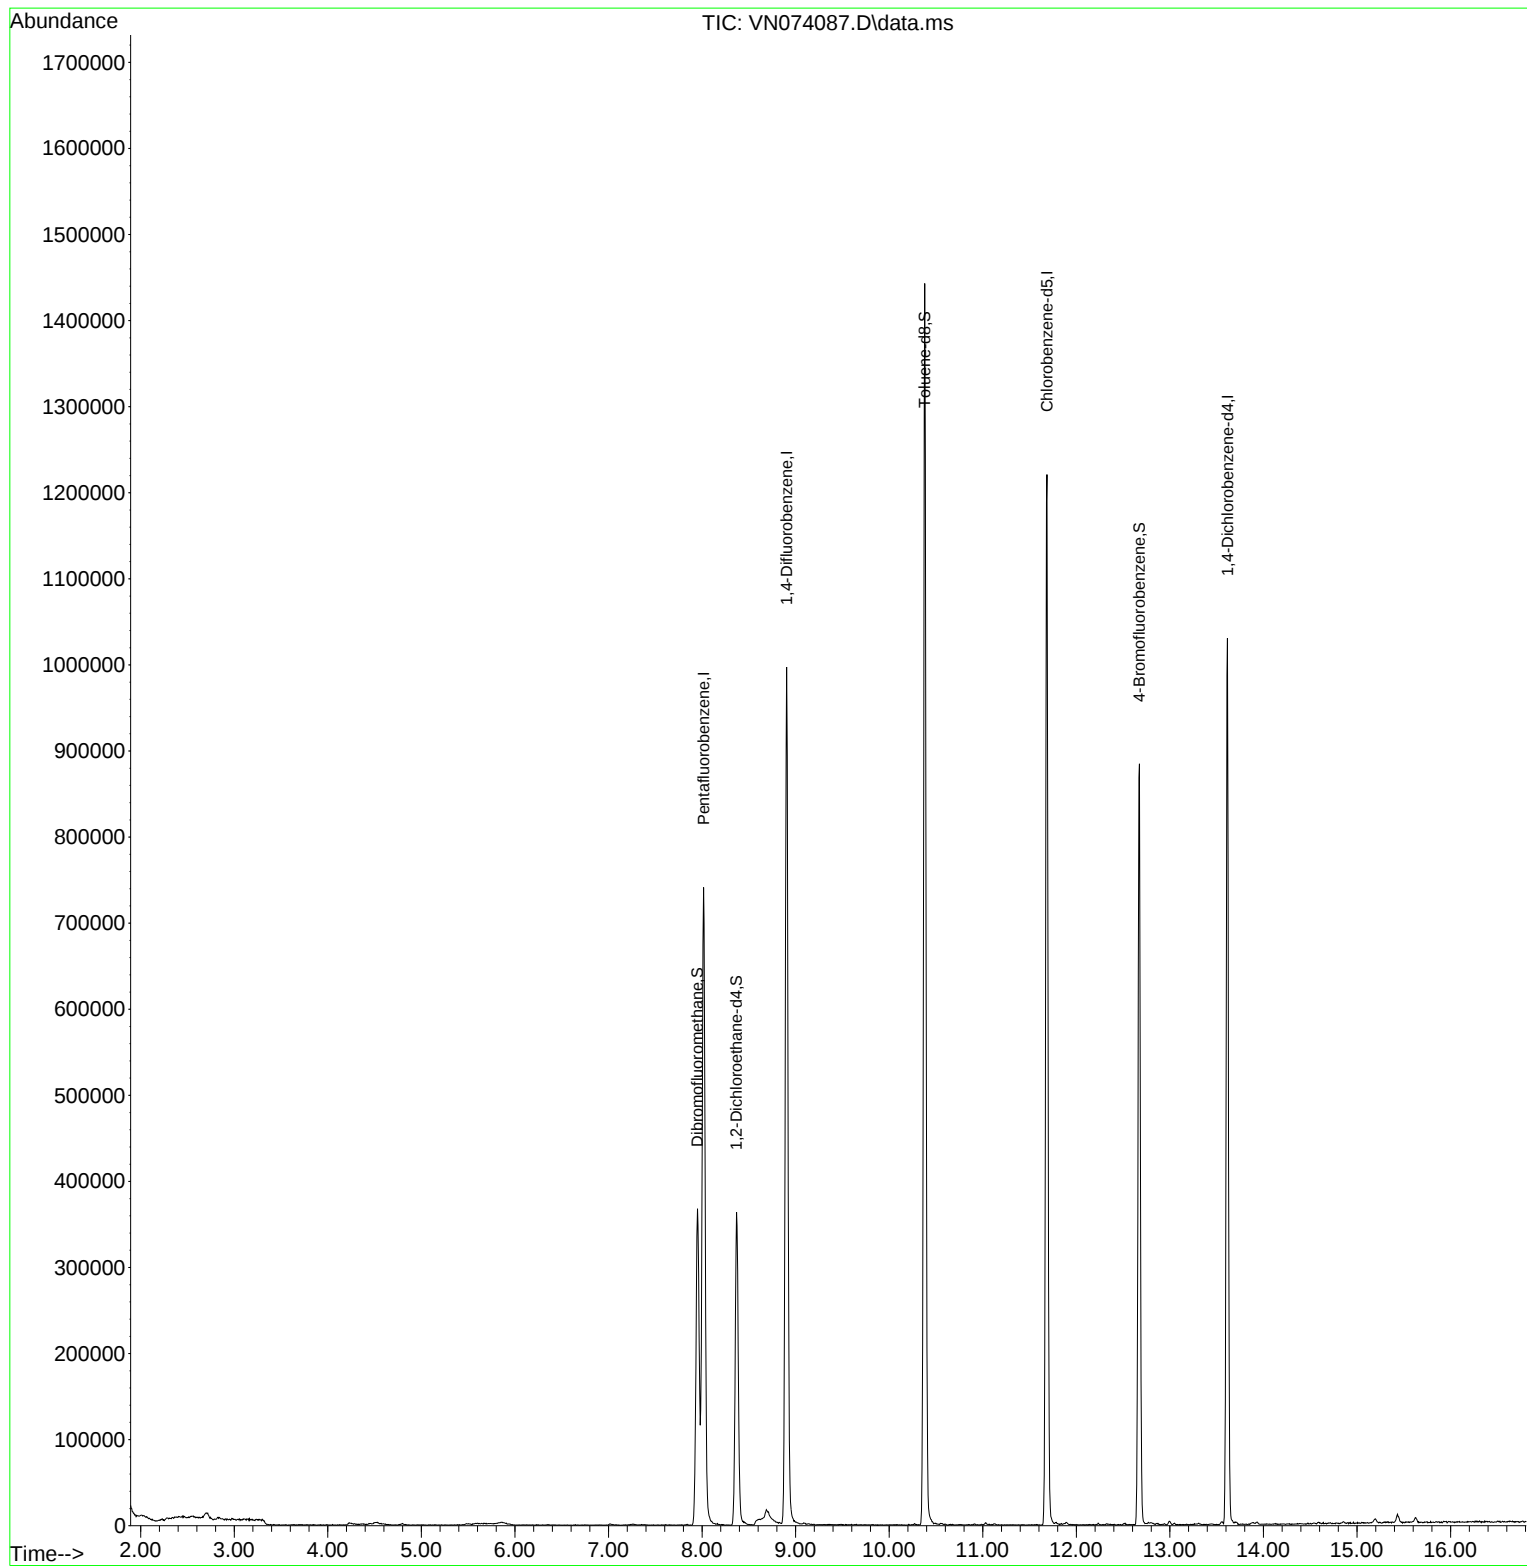


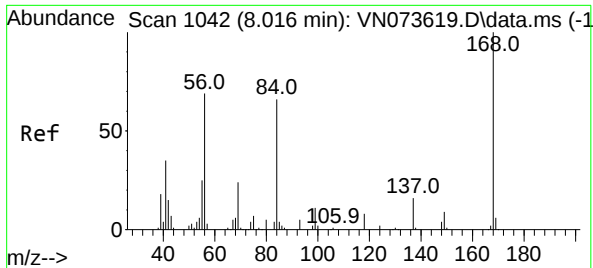

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074087.D
Acq: 24 Aug 2022 13:22




Instrument :
MSVOA_N
ClientSampleId :
MW-105D


Tgt Ion:168 Resp: 620526
Ion Ratio Lower Upper
168 100
99 50.6 42.3 63.5

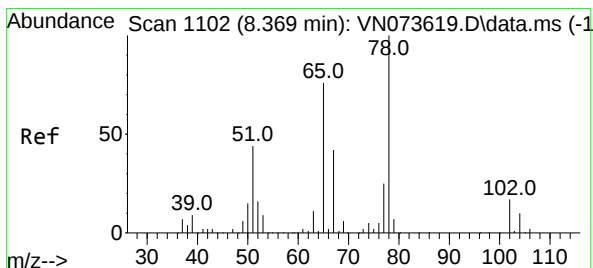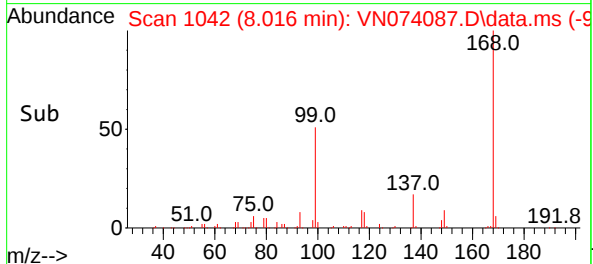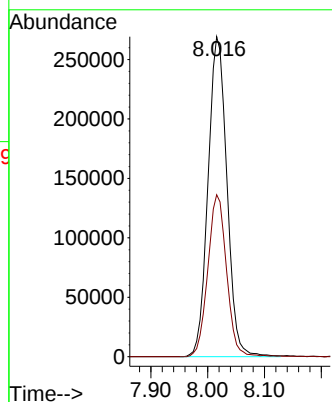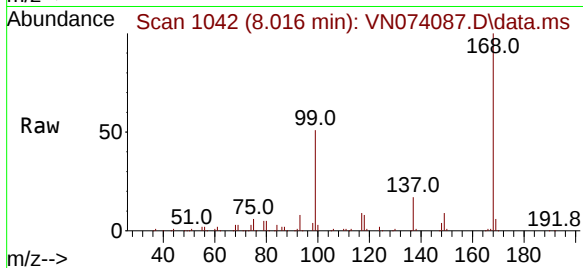

#33
1,2-Dichloroethane-d4
Concen: 50.114 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN074087.D
Acq: 24 Aug 2022 13:22

Tgt Ion: 65 Resp: 302886
Ion Ratio Lower Upper
65 100
67 53.8 0.0 104.8

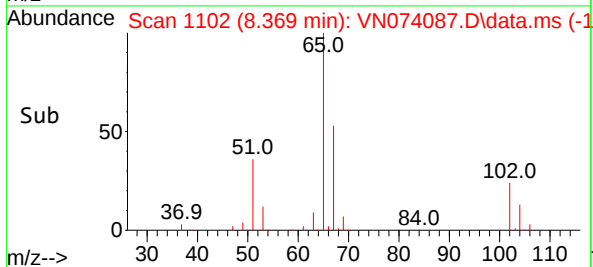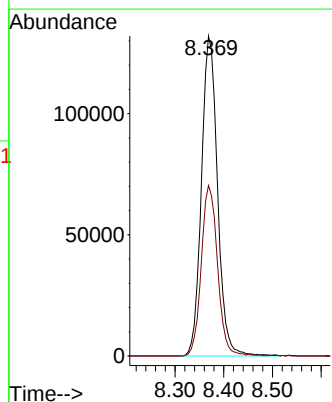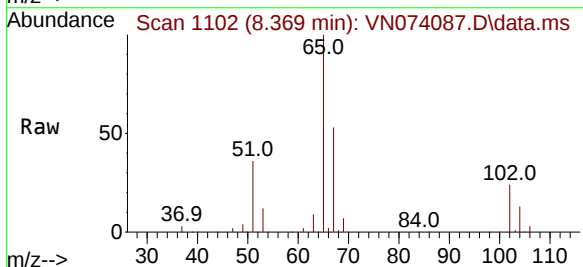

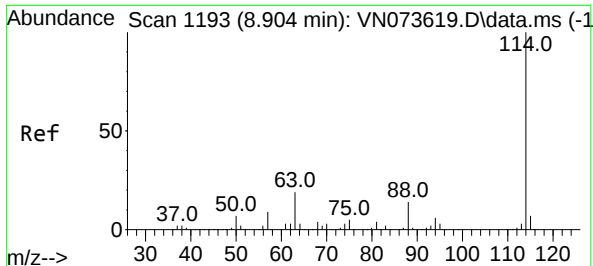

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN074087.D

Acq: 24 Aug 2022 13:22

Instrument :

MSVOA_N

ClientSampleId :

MW-105D





Tgt Ion:114 Resp: 924666

Ion Ratio Lower Upper

114 100

63 18.9 0.0 40.0

88 15.2 0.0 32.6

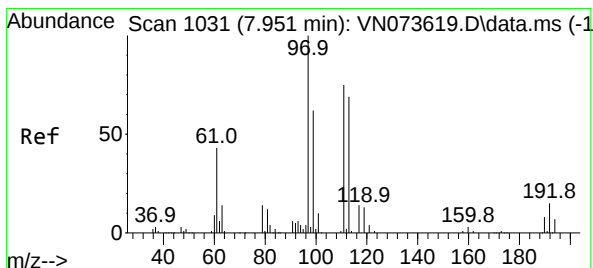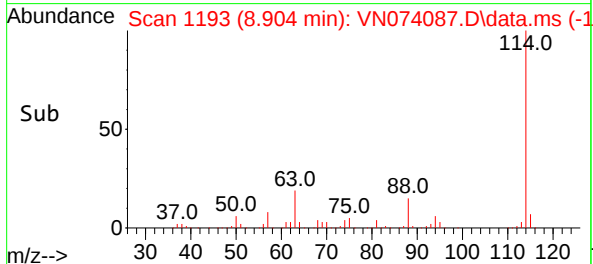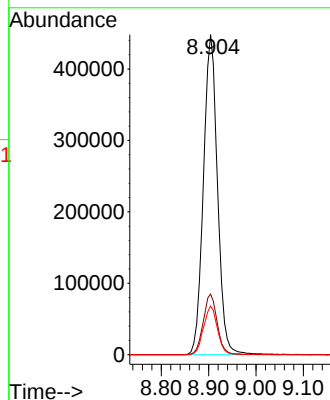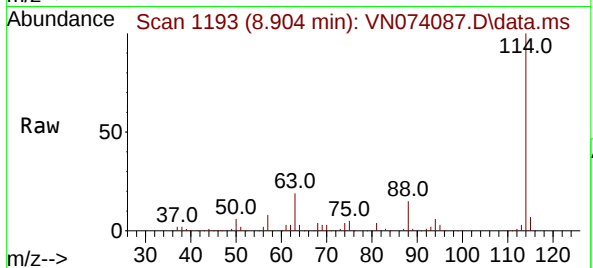

#35

Dibromofluoromethane

Concen: 50.453 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN074087.D

Acq: 24 Aug 2022 13:22




Tgt Ion:113 Resp: 275897


Ion Ratio Lower Upper

113 100

111 102.1 81.4 122.0

192 22.3 17.0 25.6


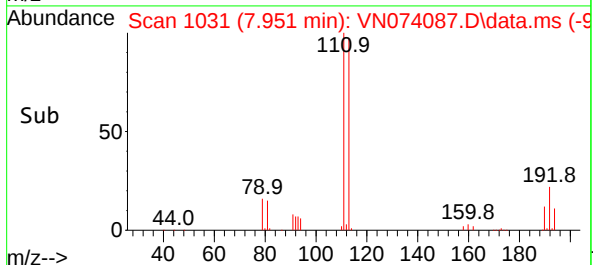
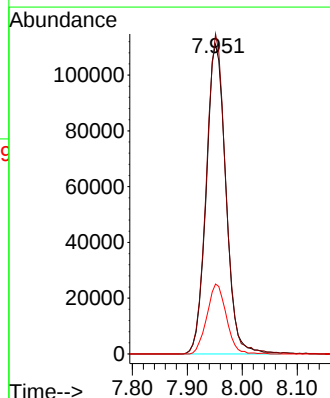
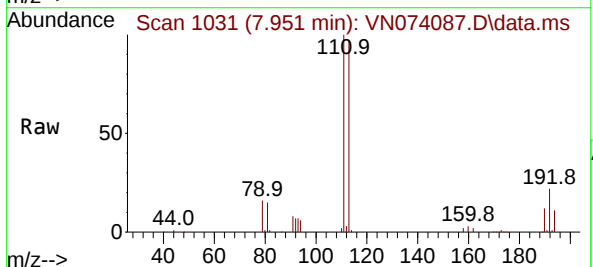


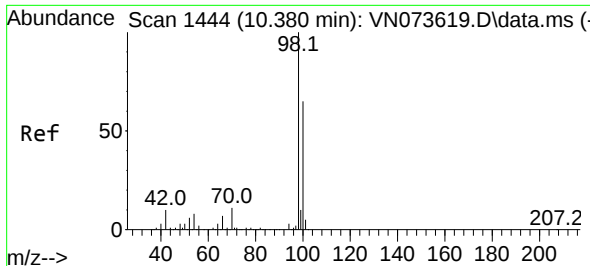

#50
Toluene-d8
Concen: 48.288 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN074087.D
Acq: 24 Aug 2022 13:22




Instrument :
MSVOA_N
ClientSampleId :
MW-105D


Tgt Ion: 98 Resp: 1022661
Ion Ratio Lower Upper
98 100
100 65.2 52.6 78.8

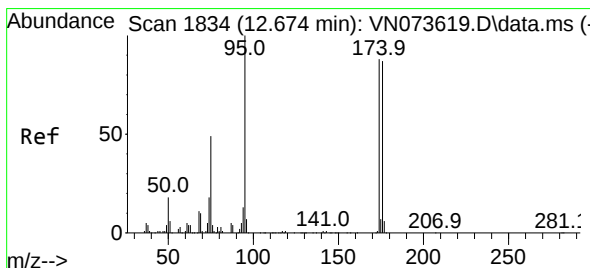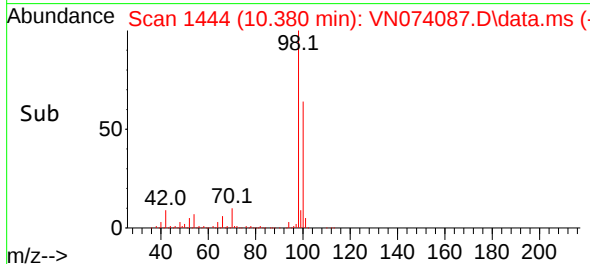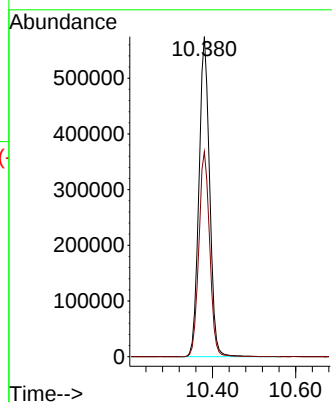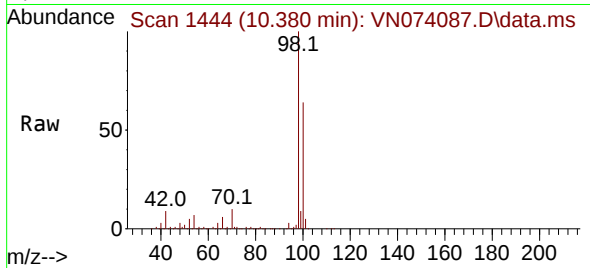

#62
4-Bromofluorobenzene
Concen: 43.181 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN074087.D
Acq: 24 Aug 2022 13:22

Tgt Ion: 95 Resp: 303512
Ion Ratio Lower Upper
95 100
174 90.9 0.0 167.6
176 86.6 0.0 163.4


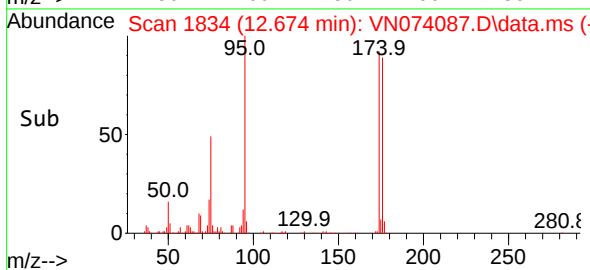
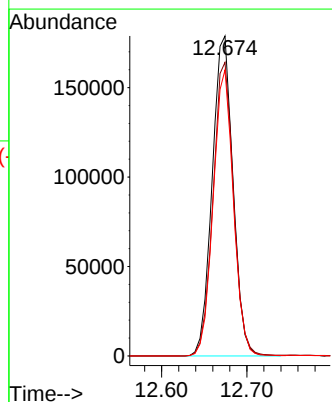
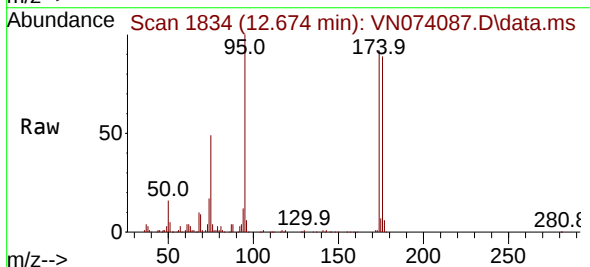


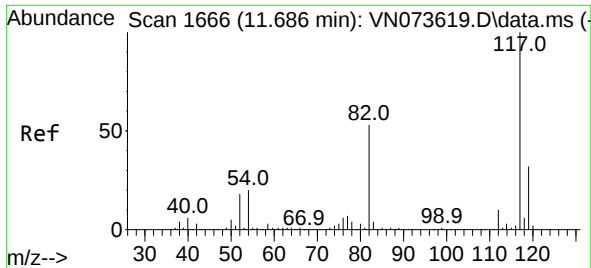

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN074087.D
Acq: 24 Aug 2022 13:22

Instrument :
MSVOA_N
ClientSampleId :
MW-105D

Tgt Ion:117 Resp: 757492
Ion Ratio Lower Upper
117 100
82 51.4 44.2 66.2
119 31.8 25.4 38.0

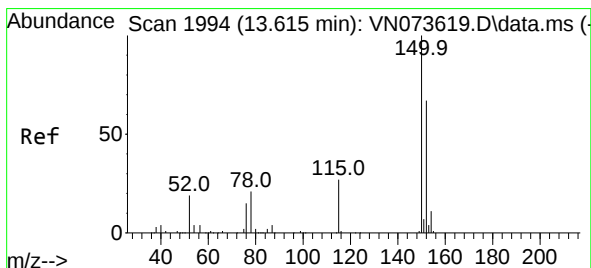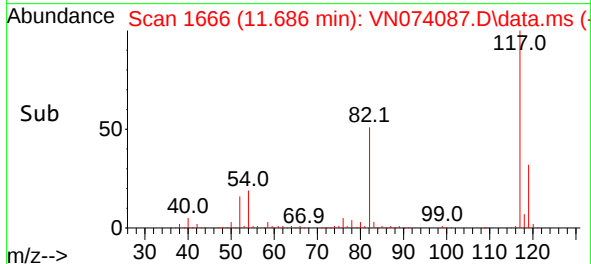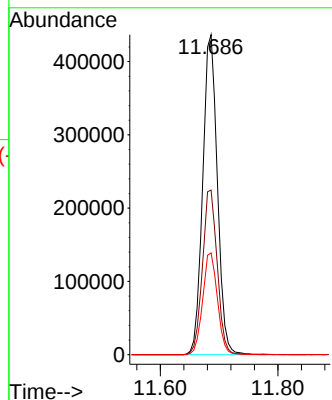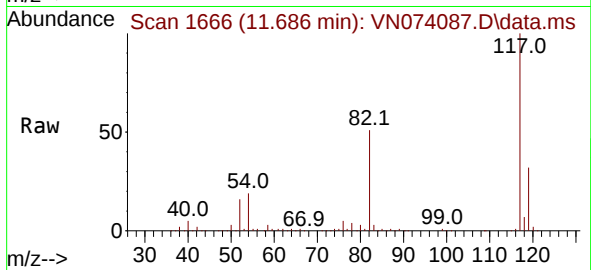

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN074087.D
Acq: 24 Aug 2022 13:22

Tgt Ion:152 Resp: 300417
Ion Ratio Lower Upper
152 100
115 55.6 28.9 86.7
150 154.6 0.0 356.2

