

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082423\
 Data File : VN079033.D
 Acq On : 24 Aug 2023 15:54
 Operator : JC\MD
 Sample : 04075-02 20X
 Misc : 7.22g/5.0mL/100uL/5.0mL/MSVOA_N/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 25 02:54:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 16 02:42:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	253348	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	466274	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	443850	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	220442	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	183704	46.598	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	93.200%		
35) Dibromofluoromethane	8.171	113	152194	48.489	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.980%		
50) Toluene-d8	10.571	98	558284	47.904	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	95.800%		
62) 4-Bromofluorobenzene	12.853	95	218687	57.408	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	114.820%		
Target Compounds			Qvalue			
18) Methyl Acetate	5.036	43	2026	0.295	ug/l #	48
31) Cyclohexane	8.236	56	9545	Below Cal	#	65
36) 1,1-Dichloropropene	8.230	75	21552	4.565	ug/l #	49
38) Carbon Tetrachloride	8.230	117	27437	5.800	ug/l #	15
39) Methylcyclohexane	9.606	83	8387	1.931	ug/l #	79
40) Benzene	8.612	78	1439664	103.162	ug/l	100
42) 1,2-Dichloroethane	8.612	62	14812	2.841	ug/l	74
43) Isopropyl Acetate	8.724	43	5893	0.631	ug/l #	49
48) Methyl methacrylate	9.606	41	4939	1.167	ug/l #	53
52) Toluene	10.641	92	22788	2.660	ug/l	98
59) 2-Hexanone	11.171	43	973	0.243	ug/l #	19
65) Chlorobenzene	12.047	112	2910	0.308	ug/l #	43
67) Ethyl Benzene	11.971	91	3993060	232.407	ug/l	97
68) m/p-Xylenes	12.076	106	651754	101.460	ug/l	97
69) o-Xylene	12.400	106	428152	68.517	ug/l	96
70) Styrene	12.406	104	23993	2.303	ug/l #	1
73) Isopropylbenzene	12.700	105	223110	12.138	ug/l	99
76) 1,2,3-Trichloropropane	13.135	75	10659	2.007	ug/l #	1
78) n-propylbenzene	13.041	91	91193	4.278	ug/l	98
79) 2-Chlorotoluene	13.135	91	95898	7.253	ug/l #	42
80) 1,3,5-Trimethylbenzene	13.176	105	228208	15.667	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.853	75	121761	58.560	ug/l #	15
82) 4-Chlorotoluene	13.176	91	26328	2.035	ug/l #	41
83) tert-Butylbenzene	13.488	119	113048	9.237	ug/l #	58
84) 1,2,4-Trimethylbenzene	13.488	105	866175	60.055	ug/l	98
85) sec-Butylbenzene	13.488	105	866175	51.427	ug/l #	57
86) p-Isopropyltoluene	13.735	119	80999	6.019	ug/l #	74
89) n-Butylbenzene	14.000	91	1309654	118.263	ug/l #	42
90) Hexachloroethane	14.329	117	57412	21.284	ug/l #	21
92) 1,2-Dibromo-3-Chloropr...	14.735	75	1845	Below Cal	#	14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082423\
Data File : VN079033.D
Acq On : 24 Aug 2023 15:54
Operator : JC\MD
Sample : 04075-02 20X
Misc : 7.22g/5.0mL/100uL/5.0mL/MSVOA_N/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 25 02:54:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 16 02:42:02 2023
Response via : Initial Calibration

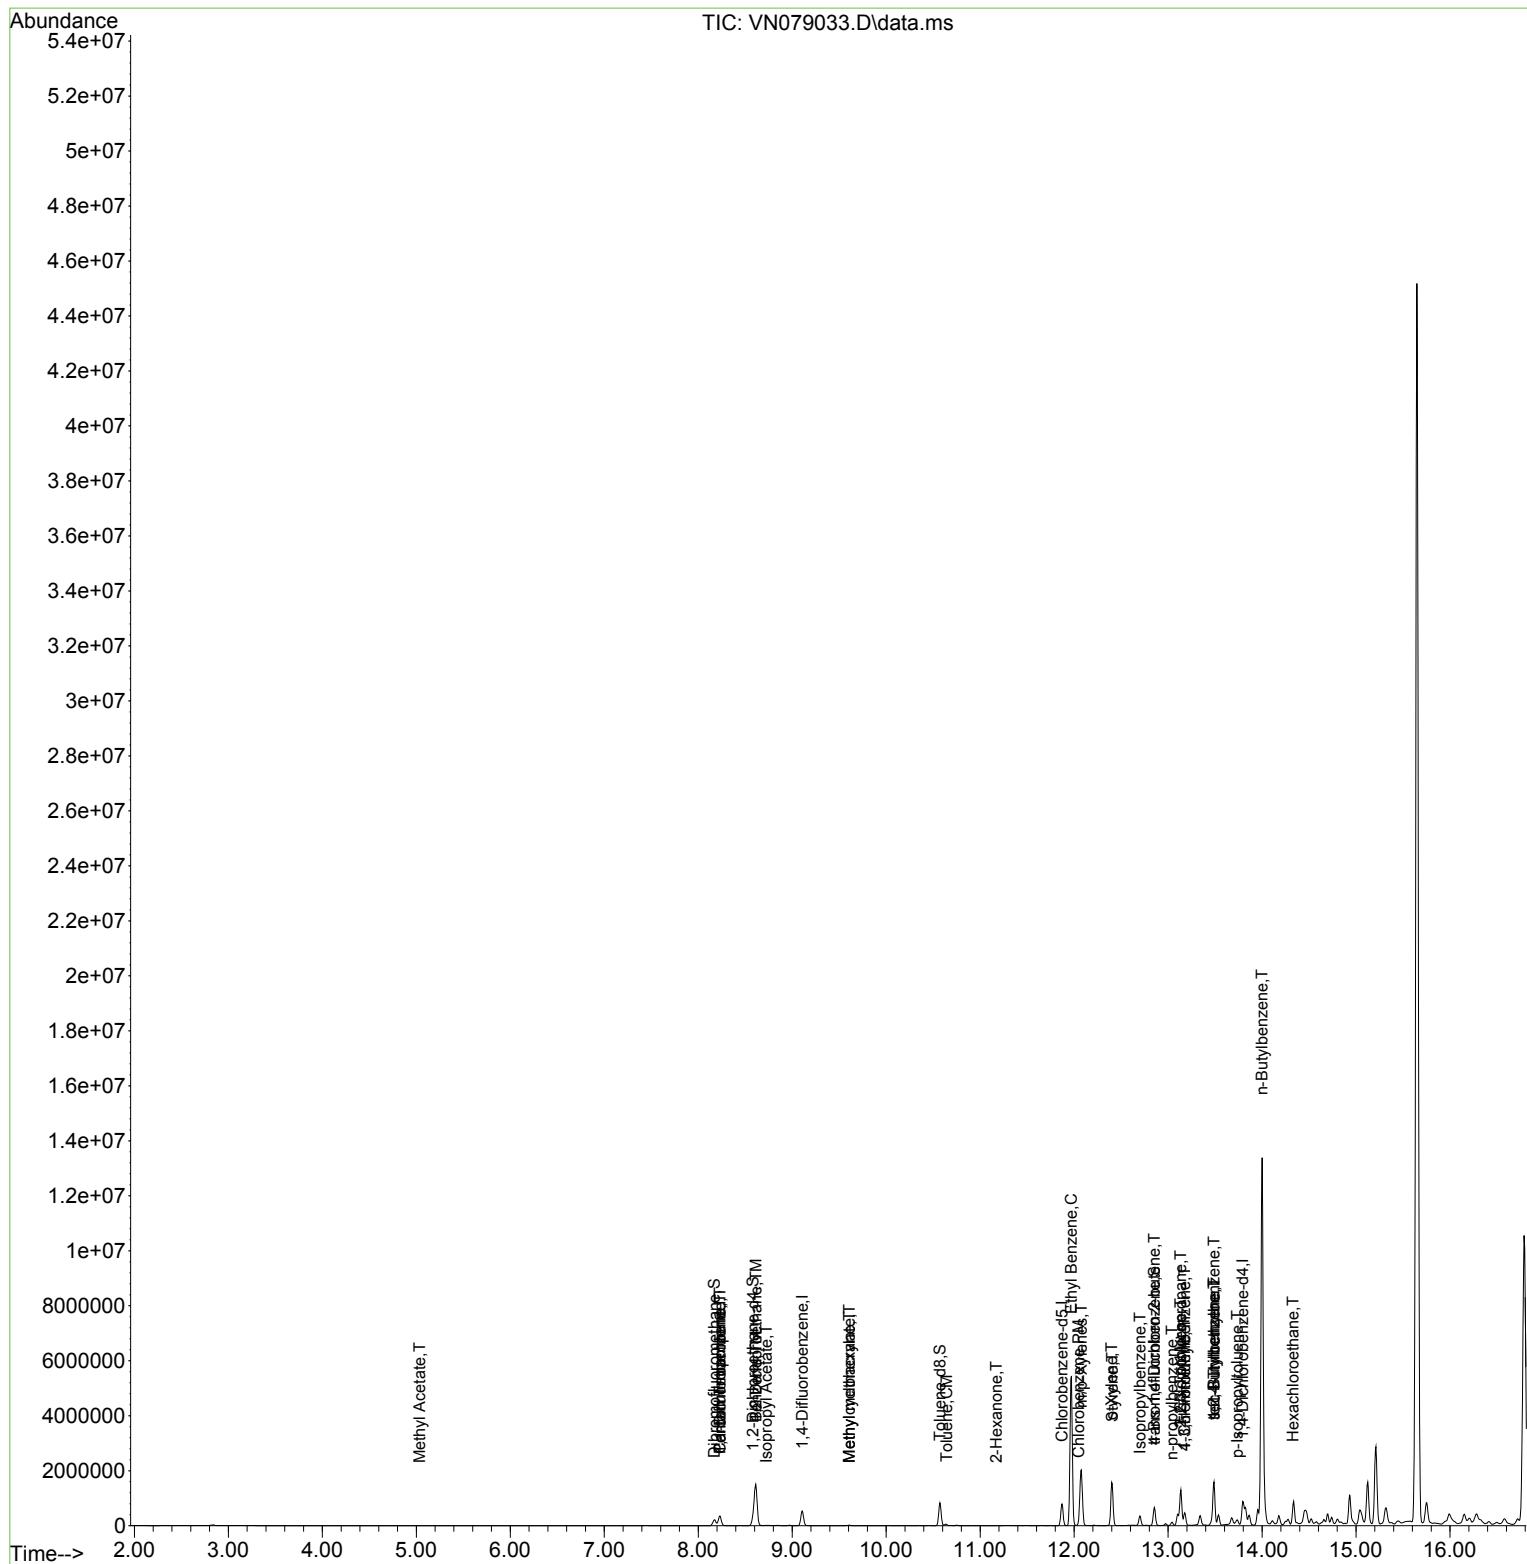



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:168 Resp: 253348

Ion Ratio Lower Upper

168 100

99 56.7 53.0 79.6



#18

Methyl Acetate

Concen: 0.295 ug/l

RT: 5.036 min Scan# 524

Delta R.T. -0.006 min

Lab File: VN079033.D




Acq: 24 Aug 2023 15:54


Tgt Ion: 43 Resp: 2026

Ion Ratio Lower Upper

43 100


74 3.5 26.2 39.4#

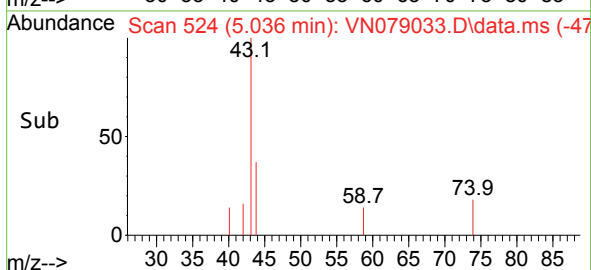






#31
Cyclohexane
Concen: Below Cal
RT: 8.236 min Scan# 1068
Delta R.T. -0.029 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 9545
Ion Ratio Lower Upper
56 100
69 97.4 26.8 40.2#
84 112.2 81.8 122.6



#33
1,2-Dichloroethane-d4
Concen: 46.598 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion: 65 Resp: 183704
Ion Ratio Lower Upper
65 100
67 51.9 0.0 106.6

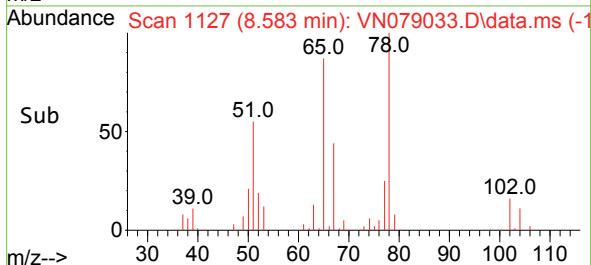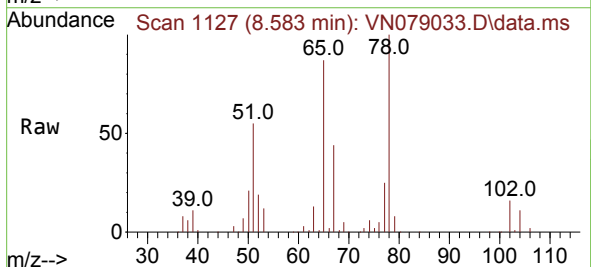



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 466274

Ion Ratio Lower Upper

114 100

63 19.5 0.0 36.4

88 14.6 0.0 30.6



#35

Dibromofluoromethane

Concen: 48.489 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54




Tgt Ion:113 Resp: 152194


Ion Ratio Lower Upper

113 100

111 105.3 82.6 123.8

192 18.8 12.7 19.1

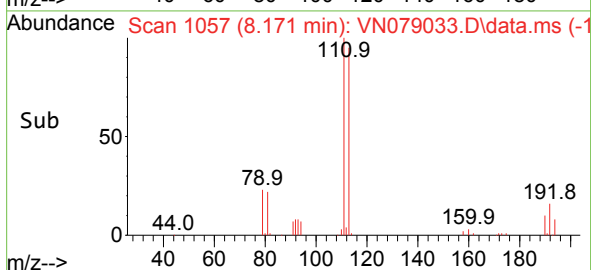



#36

1,1-Dichloropropene

Concen: 4.565 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.147 min


Lab File: VN079033.D

Acq: 24 Aug 2023 15:54




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	75	Resp:	21552
Ion Ratio	Lower	Upper	
75	100		
110	9.9	19.1	57.3#
77	0.0	25.0	37.4#



#38

Carbon Tetrachloride

Concen: 5.800 ug/l




RT: 8.230 min Scan# 1067


Delta R.T. -0.141 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Tgt Ion:	117	Resp:	27437
Ion Ratio	Lower	Upper	
117	100		
119	4.2	77.3	115.9#
121	0.0	23.3	34.9#


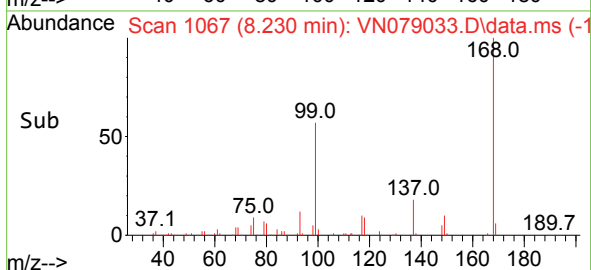






#39
Methylcyclohexane
Concen: 1.931 ug/l
RT: 9.606 min Scan# 1130
Delta R.T. 0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 83 Resp: 8387
Ion Ratio Lower Upper
83 100
55 87.3 49.1 73.7#
98 54.8 40.6 61.0

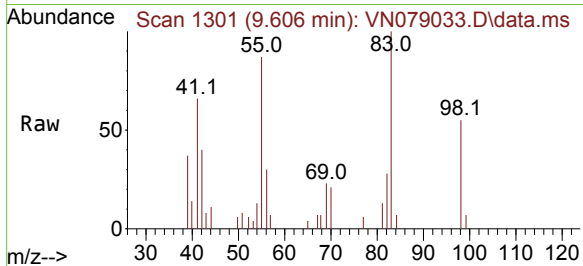

#40
Benzene
Concen: 103.162 ug/l
RT: 8.612 min Scan# 1132
Delta R.T. -0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion: 78 Resp: 1439664
Ion Ratio Lower Upper
78 100
77 24.0 19.0 28.6

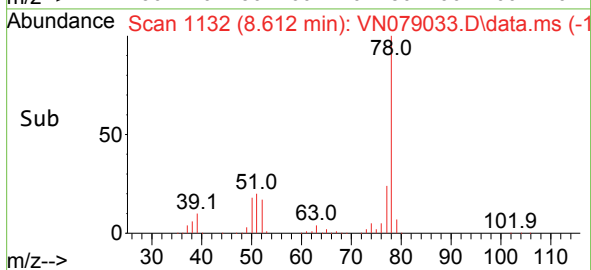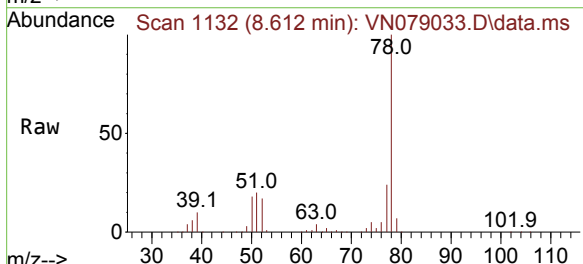



#42

1,2-Dichloroethane

Concen: 2.841 ug/l

RT: 8.612 min Scan# 1151

Delta R.T. -0.065 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 14812

Ion Ratio Lower Upper

62 100

98 0.4 0.0 19.8

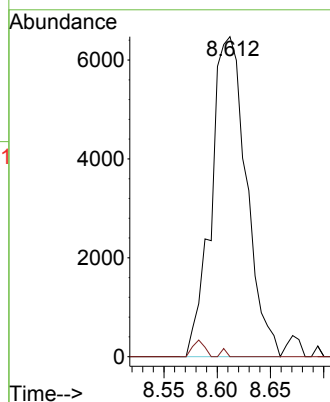

#43

Isopropyl Acetate

Concen: 0.631 ug/l

RT: 8.724 min Scan# 1151

Delta R.T. 0.030 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54




Tgt Ion: 43 Resp: 5893


Ion Ratio Lower Upper

43 100

61 0.0 24.7 37.1#


87 0.0 14.6 21.8#

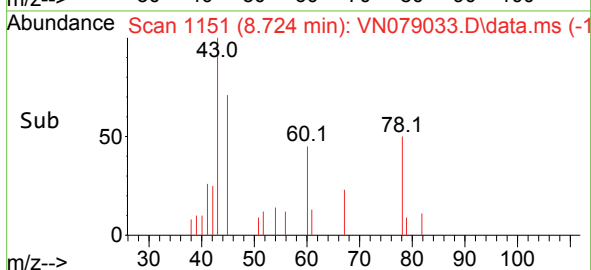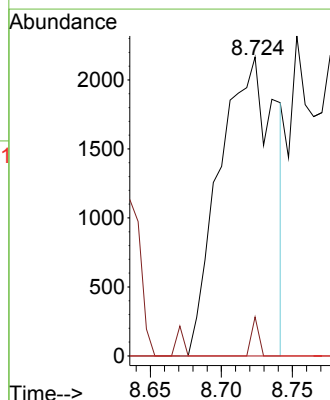






#48
Methyl methacrylate
Concen: 1.167 ug/l
RT: 9.606 min Scan# 11
Delta R.T. -0.082 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Instrument :
MSVOA_N
ClientSampleId :



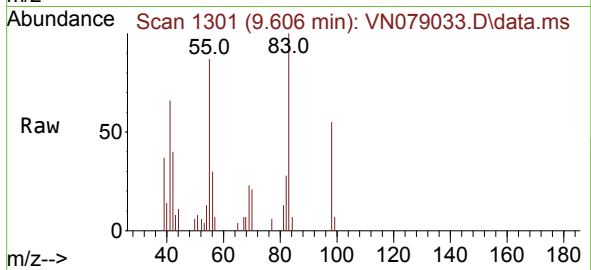



Tgt Ion: 41 Resp: 4939
Ion Ratio Lower Upper
41 100
69 38.2 90.4 135.6#
39 61.3 54.6 81.8



#50
Toluene-d8
Concen: 47.904 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion: 98 Resp: 558284
Ion Ratio Lower Upper
98 100
100 63.8 52.0 78.0




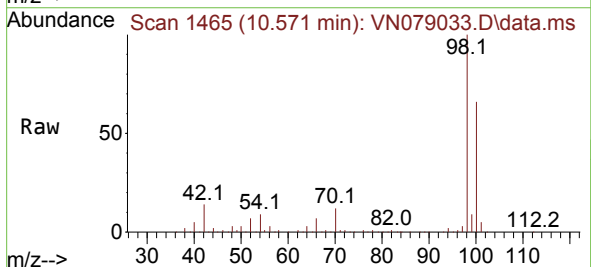


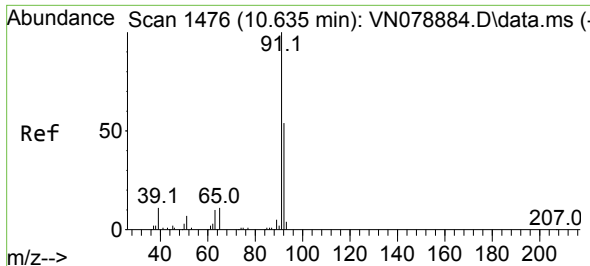

#52
Toluene
Concen: 2.660 ug/l
RT: 10.641 min Scan# 1476
Delta R.T. 0.006 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 92 Resp: 22788
Ion Ratio Lower Upper
92 100
91 169.4 137.4 206.0

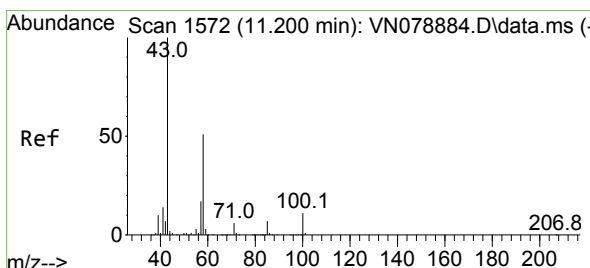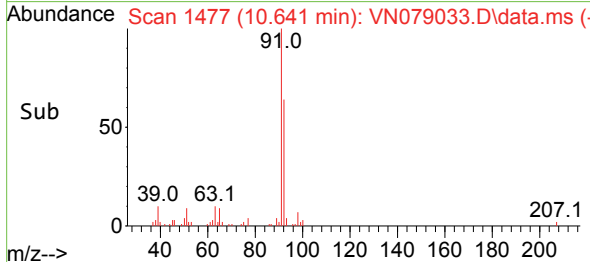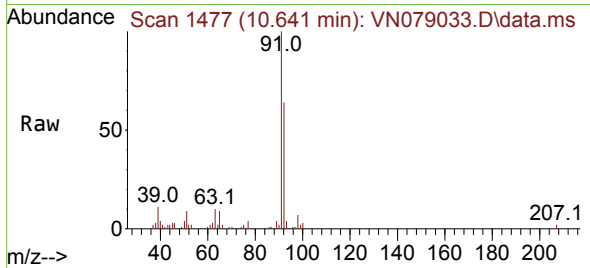

#59
2-Hexanone
Concen: 0.243 ug/l
RT: 11.171 min Scan# 1567
Delta R.T. -0.029 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion: 43 Resp: 973
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#


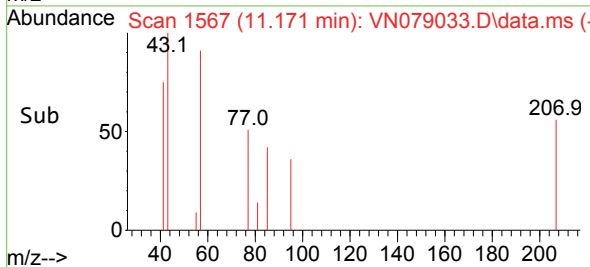

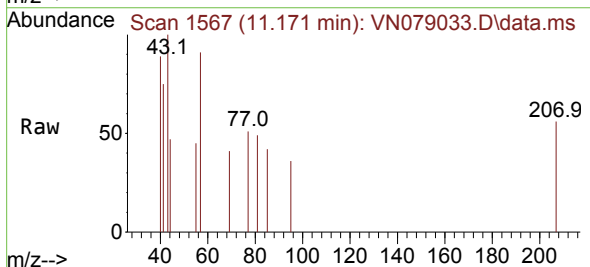


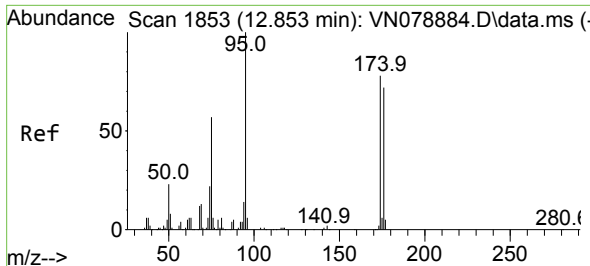

#62
4-Bromofluorobenzene
Concen: 57.408 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 218687
Ion Ratio Lower Upper
95 100
174 78.0 0.0 143.8
176 75.3 0.0 135.8

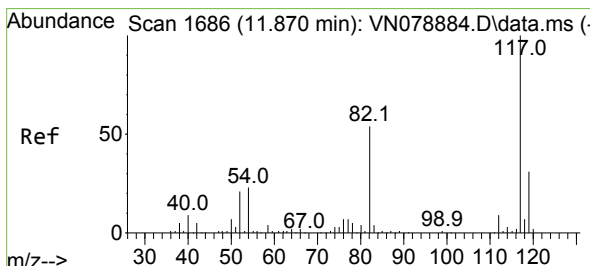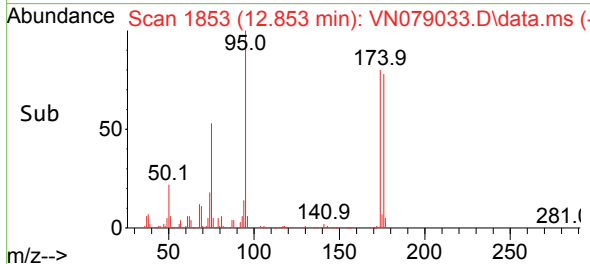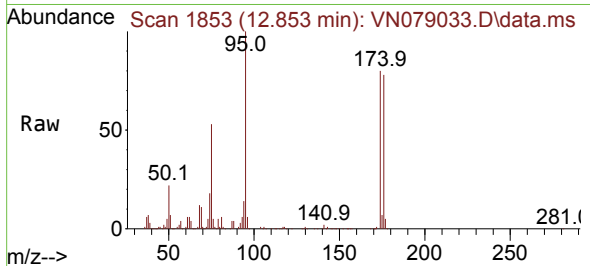

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion: 117 Resp: 443850
Ion Ratio Lower Upper
117 100
82 58.8 44.0 66.0
119 32.4 25.6 38.4


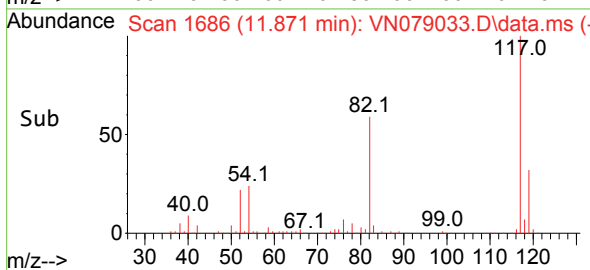

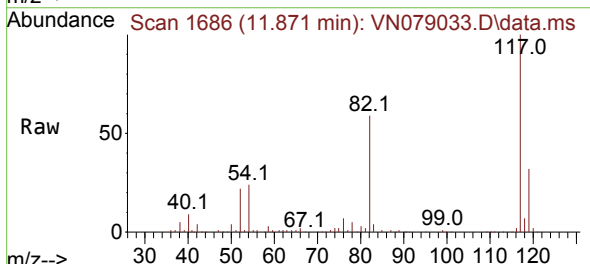




#65
Chlorobenzene
Concen: 0.308 ug/l
RT: 12.047 min Scan# 1716
Delta R.T. 0.153 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:112 Resp: 2910
Ion Ratio Lower Upper
112 100
114 0.0 25.0 37.4#



#67
Ethyl Benzene
Concen: 232.407 ug/l
RT: 11.971 min Scan# 1703
Delta R.T. -0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion: 91 Resp: 3993060
Ion Ratio Lower Upper
91 100
106 30.4 25.6 38.4


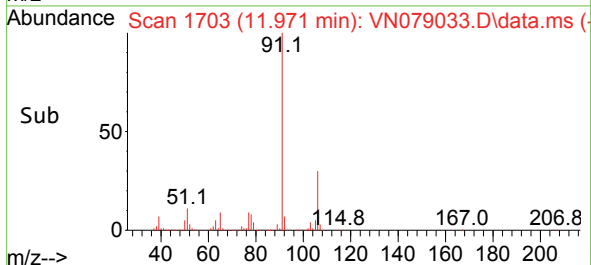

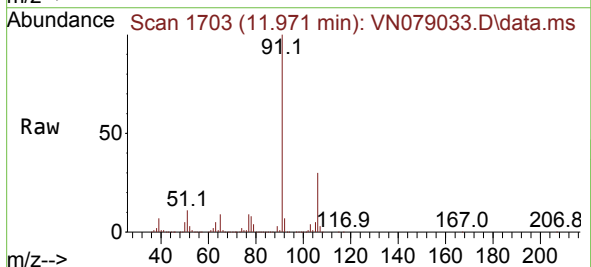




#68
m/p-Xylenes
Concen: 101.460 ug/l
RT: 12.076 min Scan# 1721
Delta R.T. 0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 651754
Ion Ratio Lower Upper
106 100
91 204.6 159.6 239.4

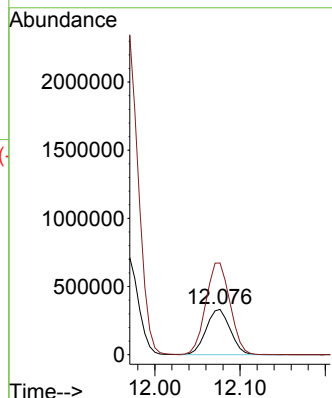

#69
o-Xylene
Concen: 68.517 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion:106 Resp: 428152
Ion Ratio Lower Upper
106 100
91 216.3 105.2 315.5


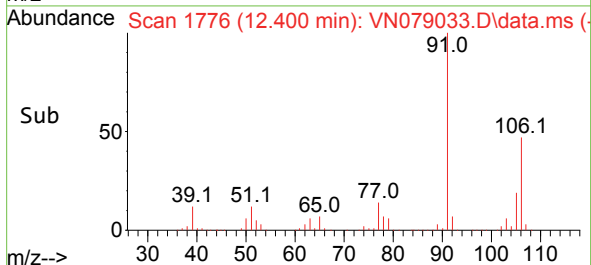

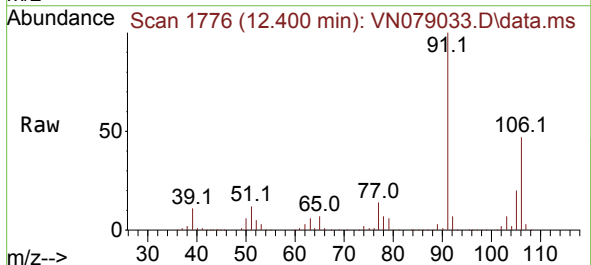




#70
Styrene
Concen: 2.303 ug/l
RT: 12.406 min Scan# 1777
Delta R.T. -0.012 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:104 Resp: 23993
Ion Ratio Lower Upper
104 100
78 282.5 39.5 59.3#
103 260.9 43.2 64.8#

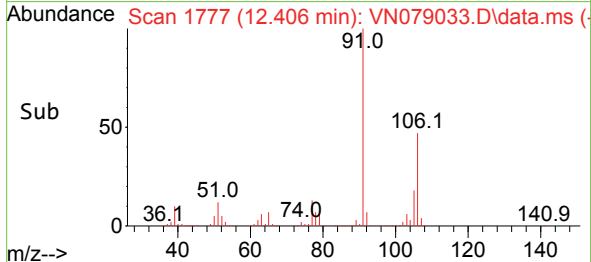

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion:152 Resp: 220442
Ion Ratio Lower Upper
152 100
115 64.0 32.3 96.8
150 155.2 0.0 355.8

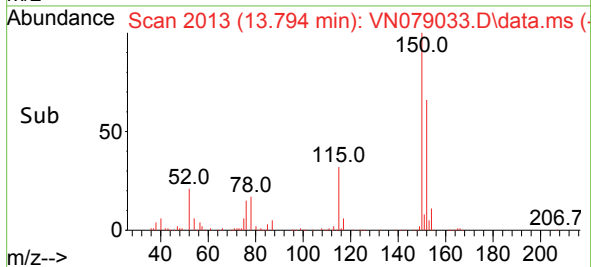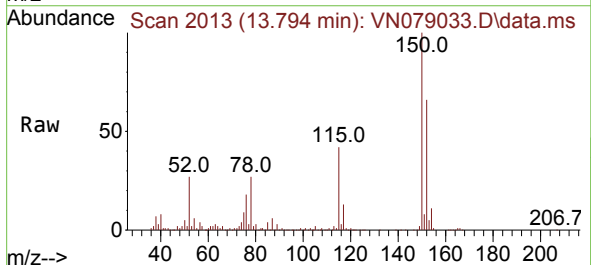

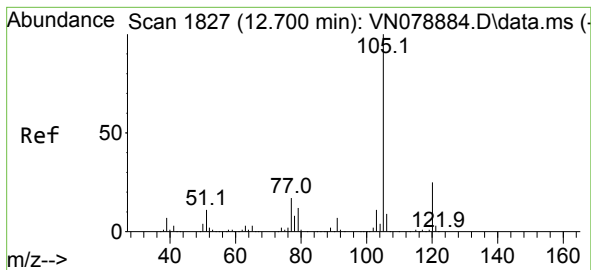

#73

Isopropylbenzene

Concen: 12.138 ug/l

RT: 12.700 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 223110

Ion Ratio Lower Upper

105 100

120 26.8 13.1 39.1

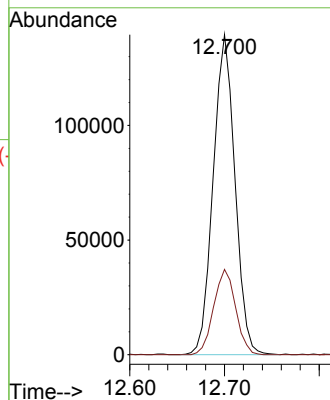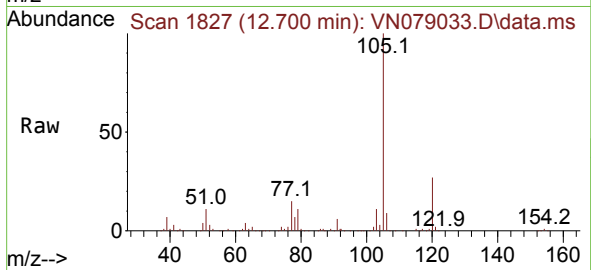

#76

1,2,3-Trichloropropane

Concen: 2.007 ug/l

RT: 13.135 min Scan# 1901

Delta R.T. 0.135 min

Lab File: VN079033.D




Acq: 24 Aug 2023 15:54


Tgt Ion: 75 Resp: 10659

Ion Ratio Lower Upper

75 100

77 1183.7 84.5 253.5#



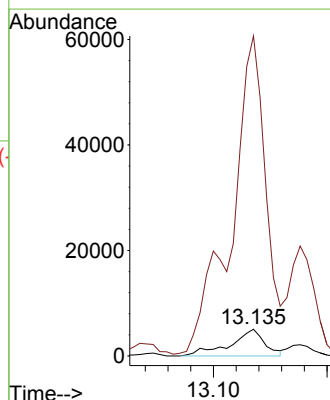
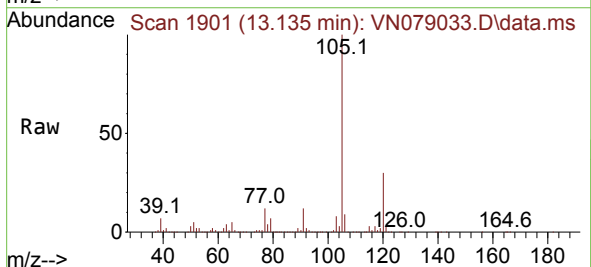


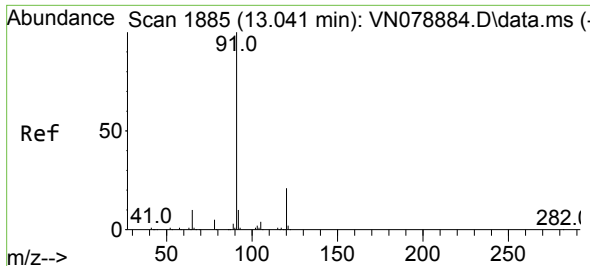

#78
n-propylbenzene
Concen: 4.278 ug/l
RT: 13.041 min Scan# 1885
Delta R.T. 0.000 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 91193
Ion Ratio Lower Upper
91 100
120 23.7 11.5 34.4

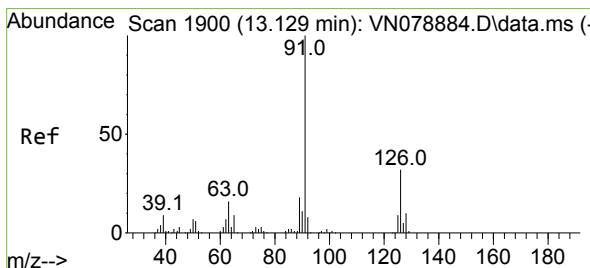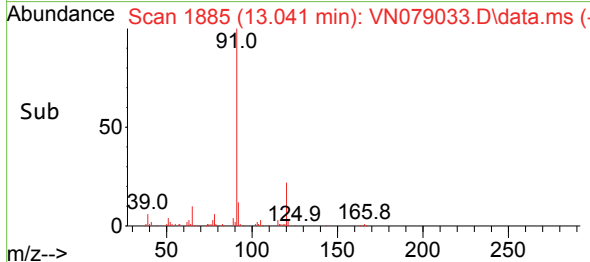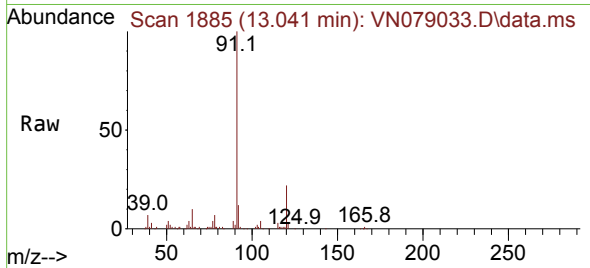

#79
2-Chlorotoluene
Concen: 7.253 ug/l
RT: 13.135 min Scan# 1901
Delta R.T. 0.006 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion: 91 Resp: 95898
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#


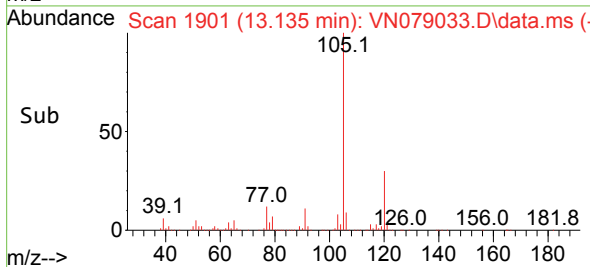

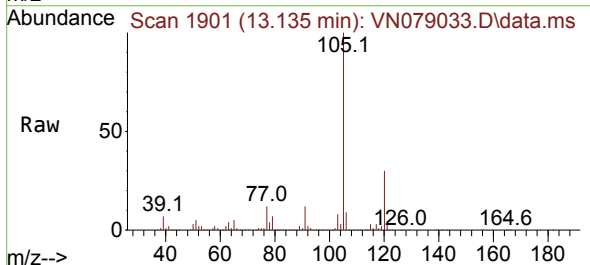




#80
 1,3,5-Trimethylbenzene
 Concen: 15.667 ug/l
 RT: 13.176 min Scan# 1908
 Delta R.T. 0.000 min
 Lab File: VN079033.D
 Acq: 24 Aug 2023 15:54




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:105 Resp: 228208
 Ion Ratio Lower Upper
 105 100
 120 48.7 24.1 72.3



#81
 trans-1,4-Dichloro-2-butene
 Concen: 58.560 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. 0.112 min
 Lab File: VN079033.D
 Acq: 24 Aug 2023 15:54

Tgt Ion: 75 Resp: 121761
 Ion Ratio Lower Upper
 75 100
 53 0.3 67.4 101.2#
 89 0.0 38.8 58.2#


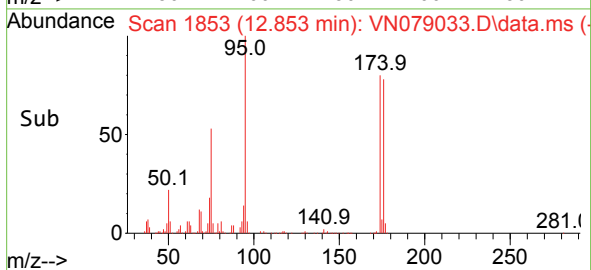




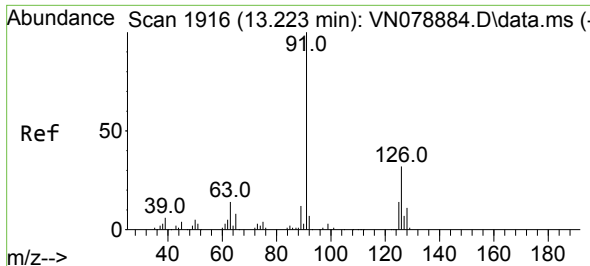

#82
4-Chlorotoluene
Concen: 2.035 ug/l
RT: 13.176 min Scan# 1908
Delta R.T. -0.053 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 26328
Ion Ratio Lower Upper
91 100
126 0.0 16.7 50.0#

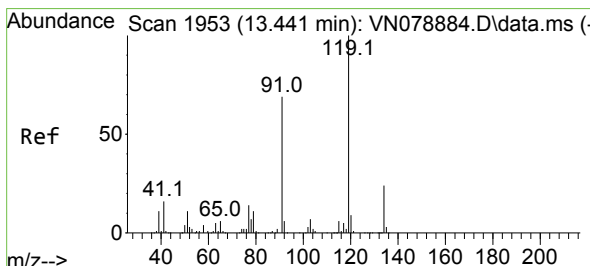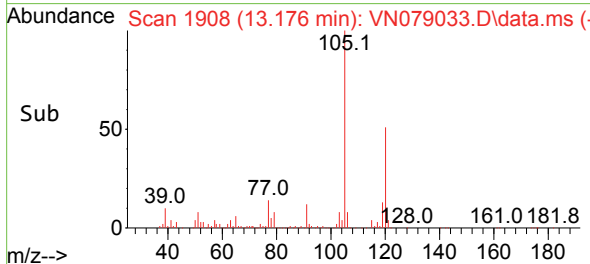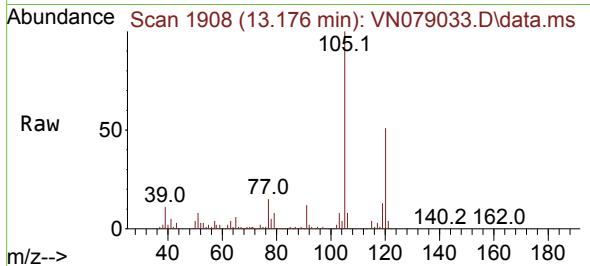

#83
tert-Butylbenzene
Concen: 9.237 ug/l
RT: 13.488 min Scan# 1961
Delta R.T. 0.047 min
Lab File: VN079033.D
Acq: 24 Aug 2023 15:54

Tgt Ion: 119 Resp: 113048
Ion Ratio Lower Upper
119 100
91 99.2 33.9 101.7
134 0.0 13.2 39.6#

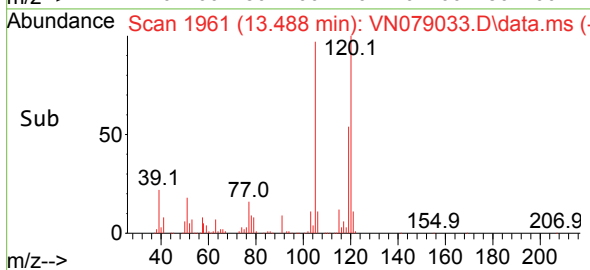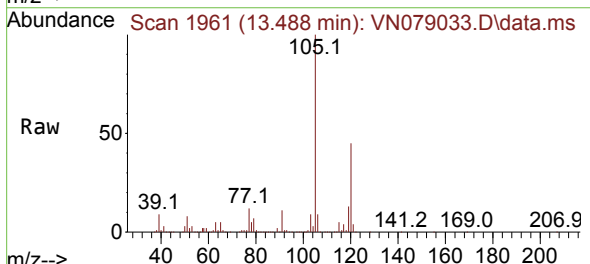



#84

1,2,4-Trimethylbenzene

Concen: 60.055 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. 0.000 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 866175

Ion Ratio Lower Upper

105 100

120 45.6 22.0 66.0

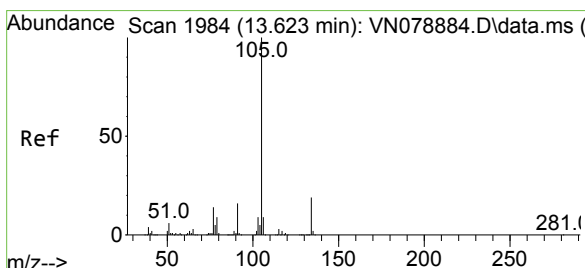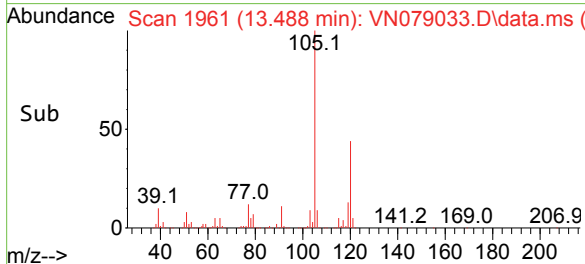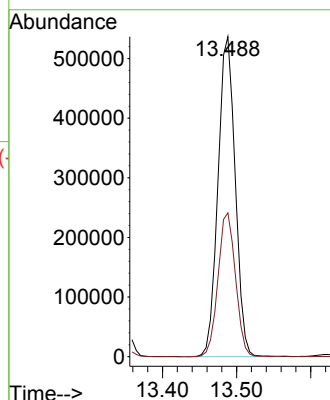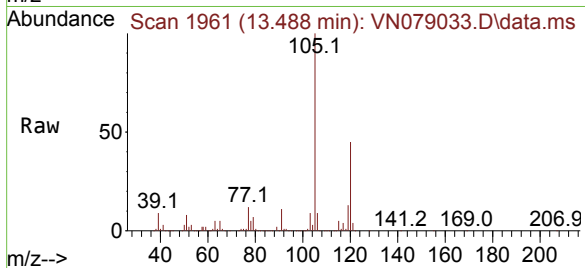

#85

sec-Butylbenzene

Concen: 51.427 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. -0.135 min

Lab File: VN079033.D




Acq: 24 Aug 2023 15:54


Tgt Ion:105 Resp: 866175

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.3#

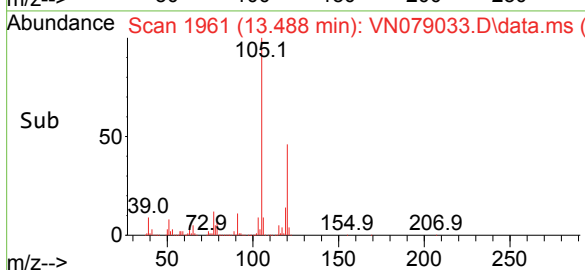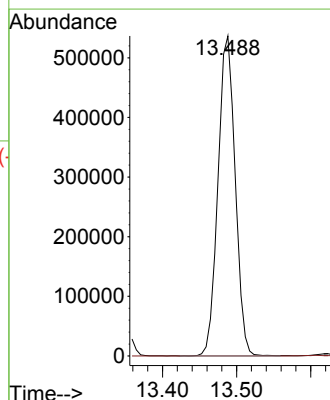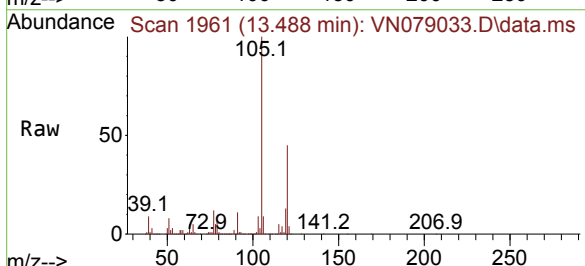

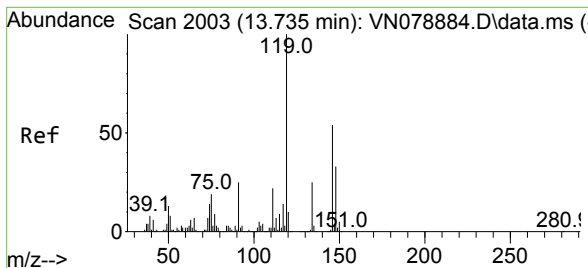

#86

p-Isopropyltoluene

Concen: 6.019 ug/l

RT: 13.735 min Scan# 2003

Delta R.T. 0.000 min


Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Instrument :

MSVOA_N

ClientSampleId :

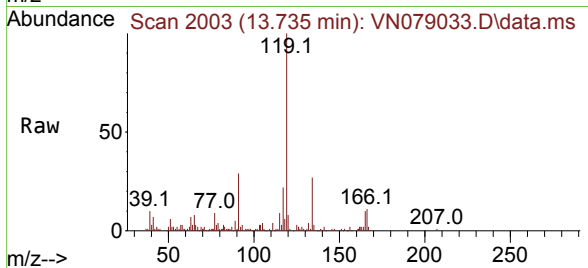




Tgt Ion:119 Resp: 80999

Ion Ratio Lower Upper

119 100

134 26.7 12.6 37.8

91 0.0 12.4 37.2#

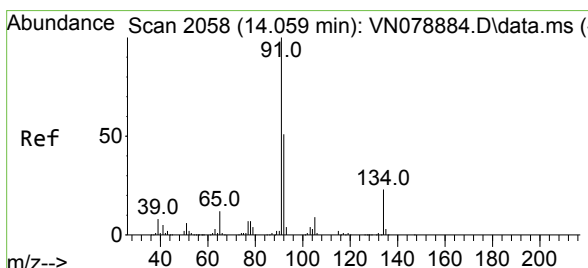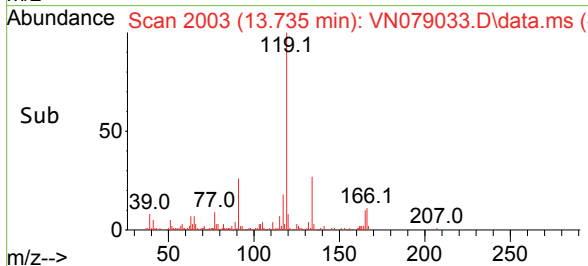

#89

n-Butylbenzene

Concen: 118.263 ug/l

RT: 14.000 min Scan# 2048

Delta R.T. -0.059 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54




Tgt Ion: 91 Resp: 1309654


Ion Ratio Lower Upper

91 100

92 9.4 26.4 79.0#

134 0.0 12.6 37.6#

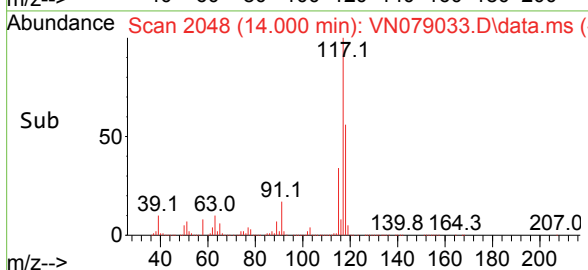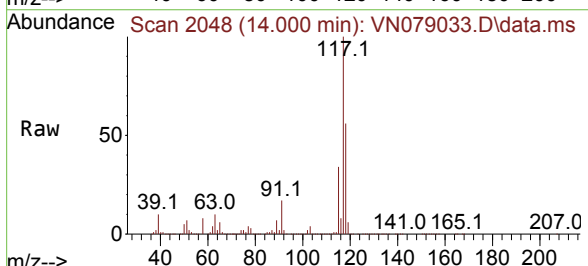

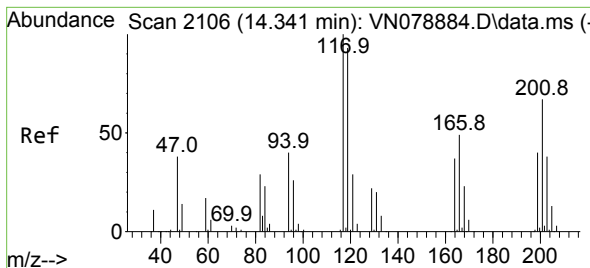

#90

Hexachloroethane

Concen: 21.284 ug/l

RT: 14.329 min Scan# 2104

Delta R.T. -0.006 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:117 Resp: 57412

Ion Ratio Lower Upper

117 100

201 0.0 29.3 88.0#

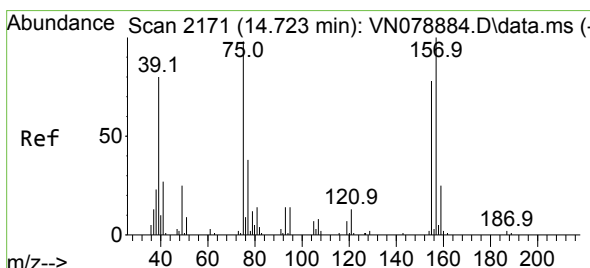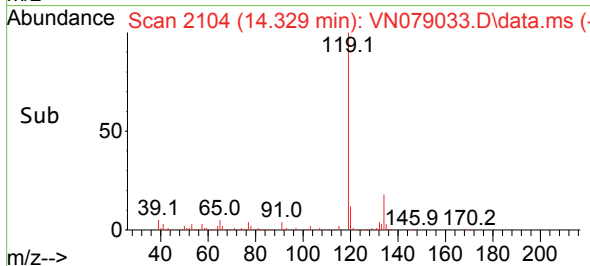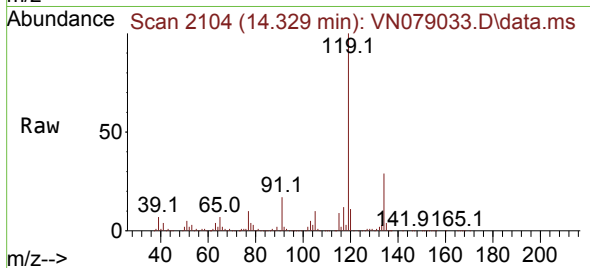

#92

1,2-Dibromo-3-Chloropropane

Concen: Below Cal

RT: 14.735 min Scan# 2173

Delta R.T. 0.012 min

Lab File: VN079033.D

Acq: 24 Aug 2023 15:54

Tgt Ion: 75 Resp: 1845

Ion Ratio Lower Upper

75 100

155 14.3 39.1 117.2#

157 3.8 50.3 150.9#

