
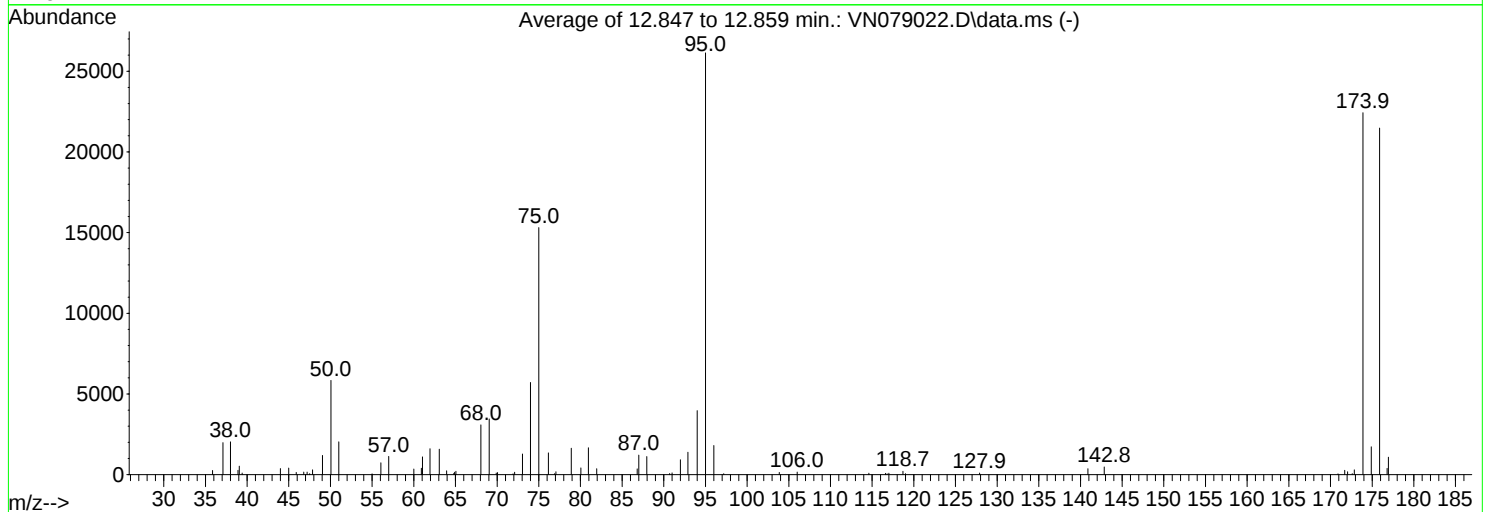


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082423\
Data File : VN079022.D
Acq On : 24 Aug 2023 10:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Title : SW846 8260
Last Update : Wed Aug 16 02:42:02 2023

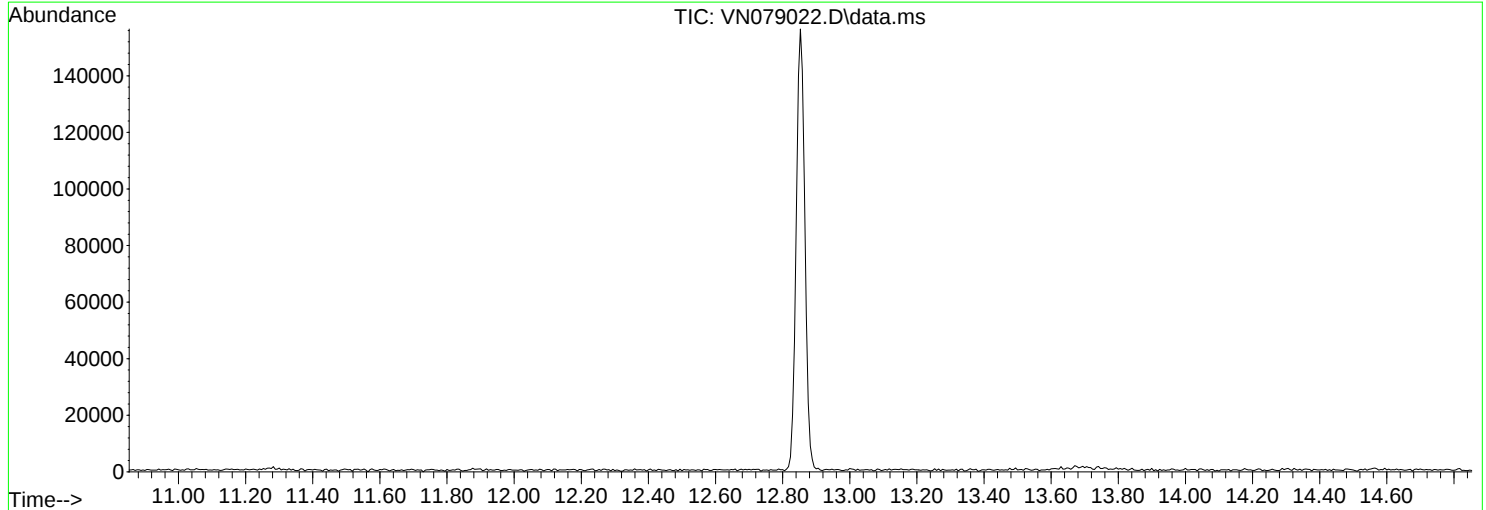

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.3	5838	PASS
75	95	30	60	58.6	15315	PASS
95	95	100	100	100.0	26141	PASS
96	95	5	9	6.9	1804	PASS
173	174	0.00	2	1.3	297	PASS
174	95	50	100	85.8	22432	PASS
175	174	5	9	7.7	1730	PASS
176	174	95	101	95.7	21477	PASS
177	176	5	9	5.1	1086	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	262	47.50	56	61.95	1606	72.10	151
37.10	1980	47.85	300	63.05	1573	73.05	127
38.00	2037	49.05	1187	63.95	239	74.00	571
38.90	271	50.05	5838	64.80	83	75.00	1531
39.05	528	51.00	2030	64.90	146	76.15	1352
39.40	102	55.00	53	65.05	213	76.90	59
44.00	375	56.05	737	68.05	3082	77.05	176
45.00	409	57.00	1126	69.05	3448	78.90	1633
45.90	135	60.00	348	69.90	103	80.05	416
46.80	156	60.90	399	70.05	126	80.95	1666
47.20	161	61.05	1105	71.90	54	81.95	365

Average of 12.847 to 12.859 min.: VN079022.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.80	362	103.85	144	170.90	53		
87.00	1212	106.00	157	171.70	266		
87.95	1119	114.60	94	172.05	178		
90.70	65	116.60	79	172.60	61		
91.00	109	116.80	53	172.85	297		
92.00	926	117.00	87	173.90	22432		
92.90	1392	118.70	208	174.90	1730		
94.00	3964	119.00	60	175.90	21477		
95.00	26141	127.90	98	176.80	384		
96.00	1804	140.90	372	176.95	1086		
97.20	58	142.85	474				

Instrument :

MSVOA_N

ClientSampleId :

BFB