


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082520\
 Data File : VN063103.D
 Acq On : 25 Aug 2020 9:22
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
 Title : SW846 8260
 Last Update : Wed Aug 19 06:09:27 2020

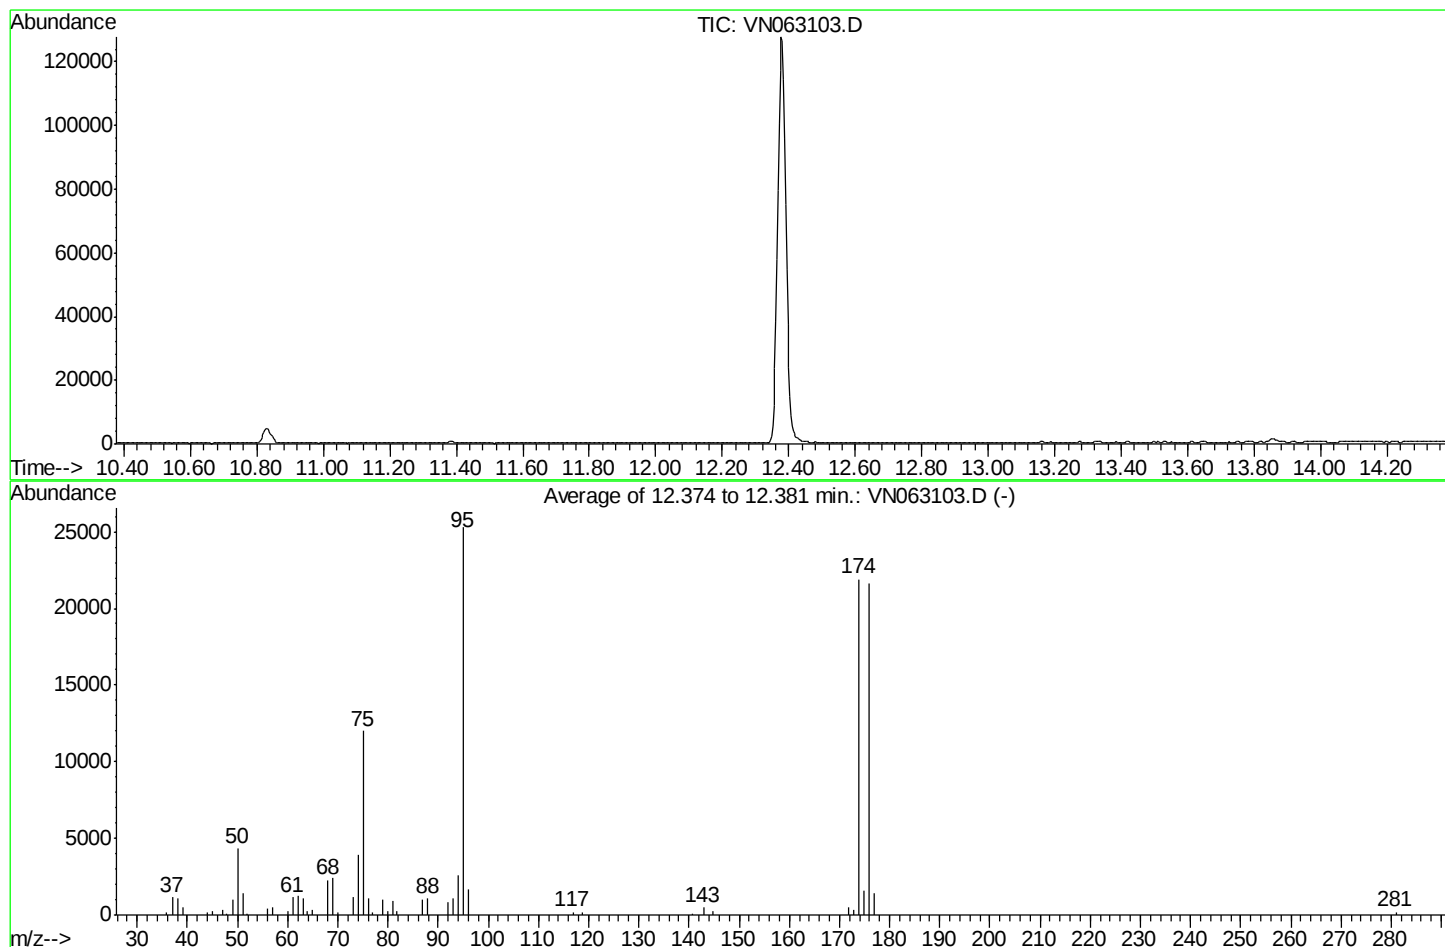

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3285

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	4313	PASS
75	95	30	60	47.5	12020	PASS
95	95	100	100	100.0	25288	PASS
96	95	5	9	6.5	1656	PASS
173	174	0.00	2	1.6	346	PASS
174	95	50	100	86.6	21893	PASS
175	174	5	9	7.1	1563	PASS
176	174	95	101	99.0	21666	PASS
177	176	5	9	6.6	1422	PASS