

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082523\
 Data File : VN079050.D
 Acq On : 25 Aug 2023 15:10
 Operator : JC\MD
 Sample : 04047-04DL 400X
 Misc : 6.72g/5.0mL/100uL/5.0mL/MSVOA_N/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 25 23:04:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 16 02:42:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	266845	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	467633	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	404942	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	175762	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	185555	44.687	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	89.380%		
35) Dibromofluoromethane	8.171	113	160593	51.017	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	102.040%		
50) Toluene-d8	10.571	98	519405	44.438	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	88.880%		
62) 4-Bromofluorobenzene	12.853	95	186263	48.754	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.500%		
Target Compounds						Qvalue
11) Tert butyl alcohol	5.518	59	580	0.832	ug/l #	72
20) Methylene Chloride	5.271	84	1262	0.346	ug/l #	74
31) Cyclohexane	8.218	56	6669	Below Cal	#	66
36) 1,1-Dichloropropene	8.230	75	21313	4.501	ug/l #	49
38) Carbon Tetrachloride	8.230	117	26896	5.669	ug/l #	15
40) Benzene	8.612	78	192882	13.781	ug/l	95
43) Isopropyl Acetate	8.753	43	2907	0.310	ug/l #	49
51) 4-Methyl-2-Pentanone	10.571	43	2577	0.464	ug/l #	1
52) Toluene	10.635	92	194573	22.643	ug/l	96
53) t-1,3-Dichloropropene	10.635	75	3044	0.562	ug/l #	8
67) Ethyl Benzene	11.971	91	443292	28.280	ug/l	99
68) m/p-Xylenes	12.076	106	115192	19.655	ug/l	99
69) o-Xylene	12.406	106	52133	9.144	ug/l	95
70) Styrene	12.412	104	27456	2.888	ug/l #	73
71) Bromoform	12.847	173	840	0.355	ug/l #	1
73) Isopropylbenzene	12.700	105	8529	0.582	ug/l	100
76) 1,2,3-Trichloropropane	12.853	75	101494	23.965	ug/l #	1
78) n-propylbenzene	13.041	91	12881	0.758	ug/l	94
79) 2-Chlorotoluene	13.135	91	7668	0.727	ug/l #	42
80) 1,3,5-Trimethylbenzene	13.176	105	32151	2.768	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.853	75	101494	61.221	ug/l #	15
82) 4-Chlorotoluene	13.176	91	3712	0.360	ug/l #	41
83) tert-Butylbenzene	13.482	119	14741	1.511	ug/l #	57
84) 1,2,4-Trimethylbenzene	13.488	105	114201	9.931	ug/l	97
85) sec-Butylbenzene	13.488	105	114201	8.504	ug/l #	57
86) p-Isopropyltoluene	13.729	119	5099	0.475	ug/l	87
89) n-Butylbenzene	14.059	91	2806	0.318	ug/l #	78
90) Hexachloroethane	14.370	117	12507	5.815	ug/l #	21
92) 1,2-Dibromo-3-Chloropr...	14.700	75	548	Below Cal	#	4
95) Naphthalene	15.647	128	3896916	458.926	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082523\
Data File : VN079050.D
Acq On : 25 Aug 2023 15:10
Operator : JC\MD
Sample : 04047-04DL 400X
Misc : 6.72g/5.0mL/100uL/5.0mL/MSVOA_N/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 25 23:04:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 16 02:42:02 2023
Response via : Initial Calibration

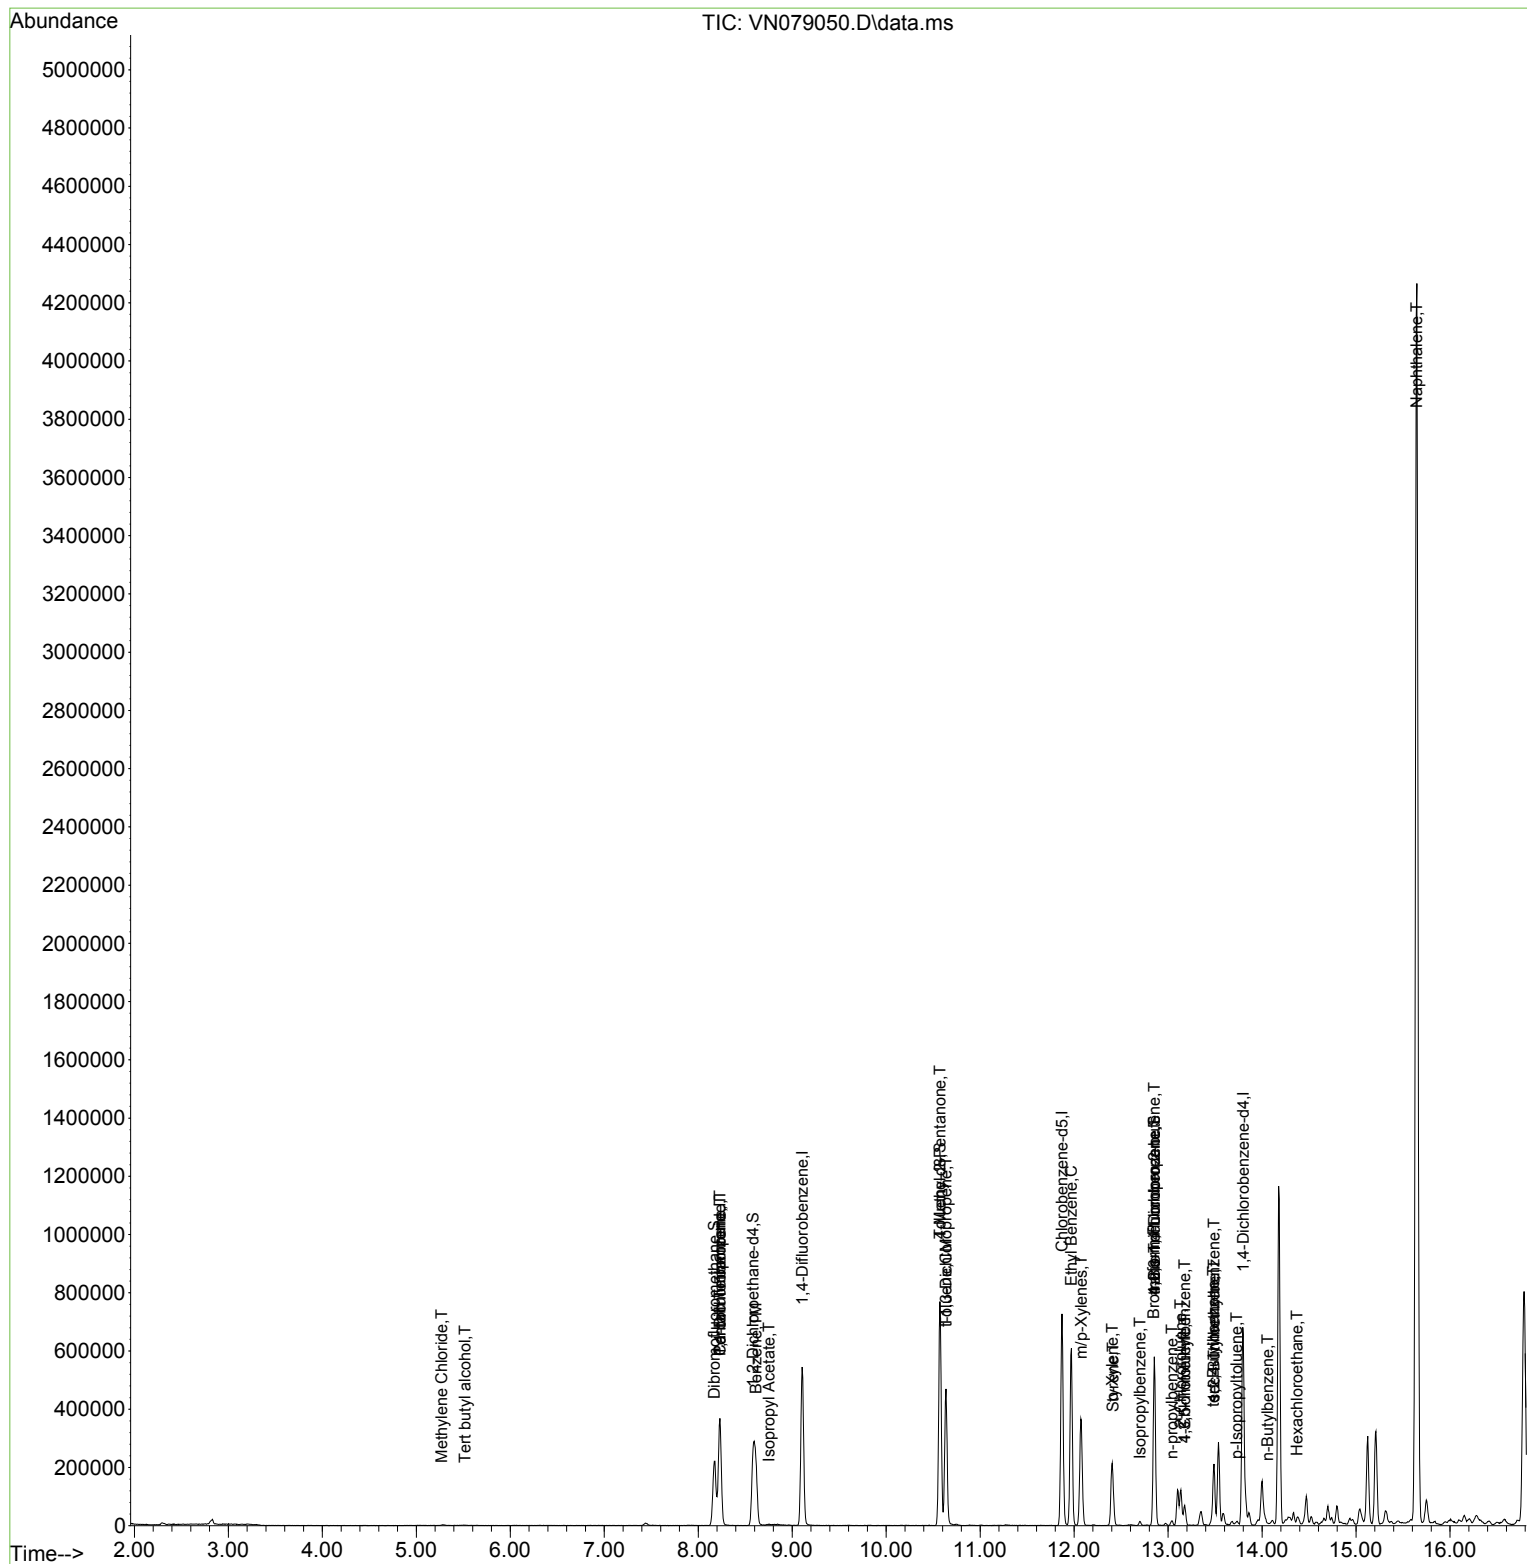



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:168 Resp: 266845

Ion Ratio Lower Upper

168 100

99 58.9 53.0 79.6



#11

Tert butyl alcohol

Concen: 0.832 ug/l

RT: 5.518 min Scan# 606

Delta R.T. -0.024 min

Lab File: VN079050.D




Acq: 25 Aug 2023 15:10


Tgt Ion: 59 Resp: 580

Ion Ratio Lower Upper

59 100


57 0.0 8.2 12.4#







#20
Methylene Chloride
Concen: 0.346 ug/l
RT: 5.271 min Scan# 51
Delta R.T. -0.012 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:	84	Resp:	1262
Ion	Ratio	Lower	Upper
84	100		
49	77.3	79.7	119.5#
51	0.0	25.2	37.8#
86	52.0	53.3	79.9#

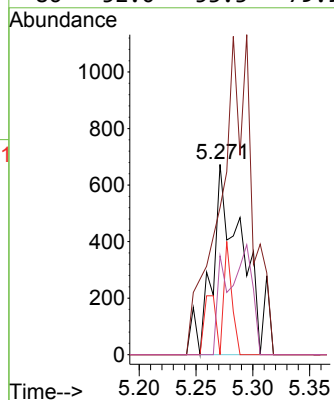

#31
Cyclohexane
Concen: Below Cal
RT: 8.218 min Scan# 1065
Delta R.T. -0.047 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion:	56	Resp:	6669
Ion	Ratio	Lower	Upper
56	100		
69	99.5	26.8	40.2#
84	95.3	81.8	122.6

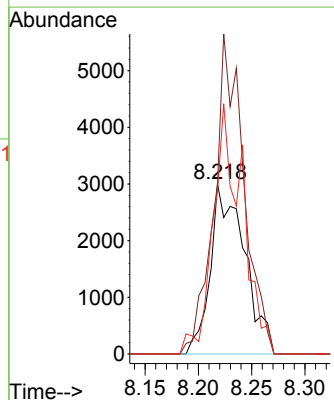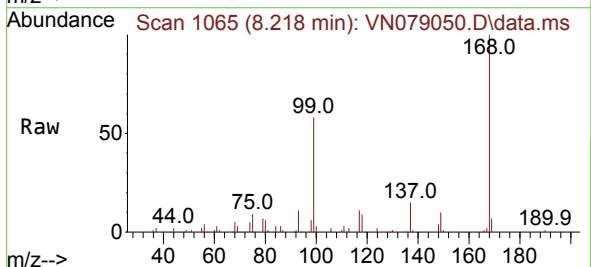



#33

1,2-Dichloroethane-d4

Concen: 44.687 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 185555

Ion Ratio Lower Upper

65 100

67 53.1 0.0 106.6

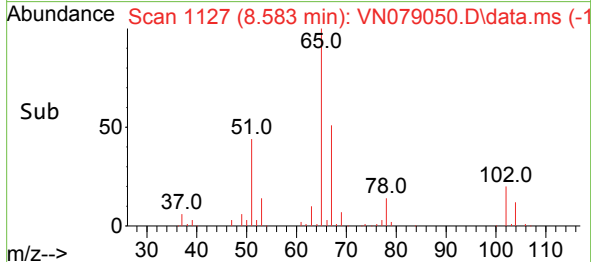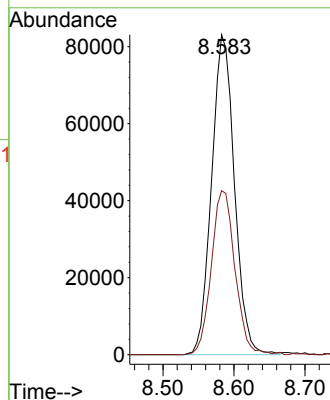

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.006 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10




Tgt Ion: 114 Resp: 467633


Ion Ratio Lower Upper

114 100

63 21.8 0.0 36.4


88 15.1 0.0 30.6

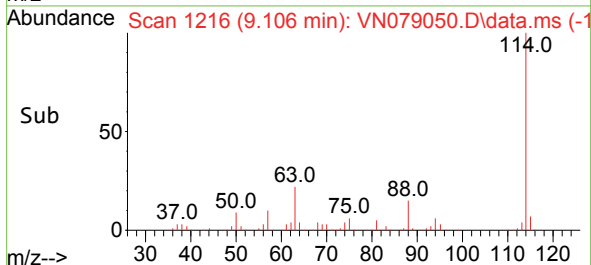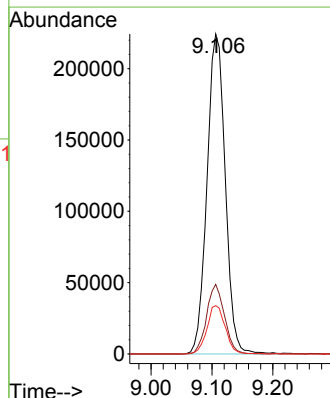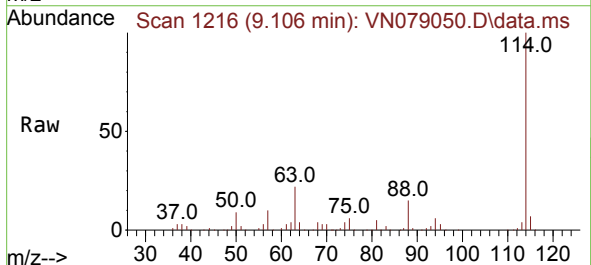






#35
Dibromofluoromethane
Concen: 51.017 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:113 Resp: 160593
Ion Ratio Lower Upper
113 100
111 101.9 82.6 123.8
192 18.4 12.7 19.1



#36
1,1-Dichloropropene
Concen: 4.501 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion: 75 Resp: 21313
Ion Ratio Lower Upper
75 100
110 9.6 19.1 57.3#
77 0.0 25.0 37.4#

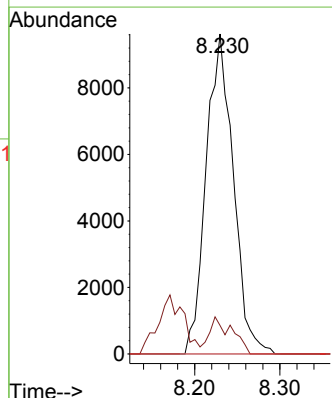



#38

Carbon Tetrachloride

Concen: 5.669 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.141 min


Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:117 Resp: 26896

Ion Ratio Lower Upper

117 100

119 4.8 77.3 115.9#

121 0.0 23.3 34.9#



#40

Benzene

Concen: 13.781 ug/l

RT: 8.612 min Scan# 1132

Delta R.T. 0.000 min

Lab File: VN079050.D




Acq: 25 Aug 2023 15:10


Tgt Ion: 78 Resp: 192882

Ion Ratio Lower Upper

78 100

77 26.4 19.0 28.6









#43
Isopropyl Acetate
Concen: 0.310 ug/l
RT: 8.753 min Scan# 1146
Delta R.T. 0.059 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2907
Ion Ratio Lower Upper
43 100
61 0.0 24.7 37.1#
87 0.0 14.6 21.8#

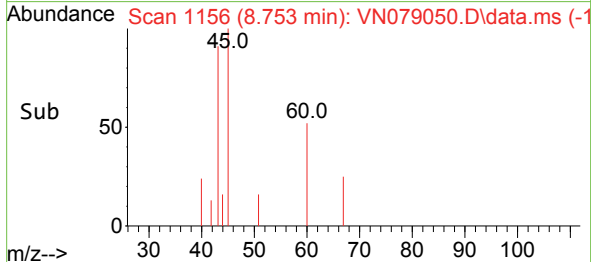

#50
Toluene-d8
Concen: 44.438 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion: 98 Resp: 519405
Ion Ratio Lower Upper
98 100
100 65.5 52.0 78.0



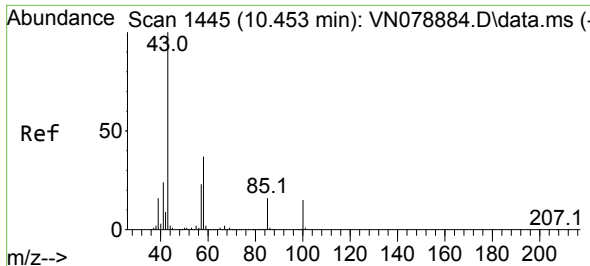

#51

4-Methyl-2-Pentanone

Concen: 0.464 ug/l

RT: 10.571 min Scan# 1445

Delta R.T. 0.118 min


Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 43 Resp: 2577

Ion Ratio Lower Upper

43 100

58 199.3 36.6 54.8#

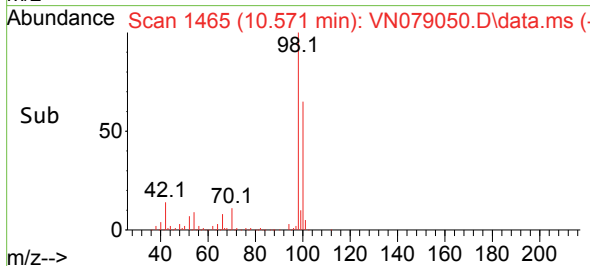

#52

Toluene

Concen: 22.643 ug/l

RT: 10.635 min Scan# 1476

Delta R.T. 0.000 min

Lab File: VN079050.D




Acq: 25 Aug 2023 15:10


Tgt Ion: 92 Resp: 194573

Ion Ratio Lower Upper

92 100

91 176.6 137.4 206.0


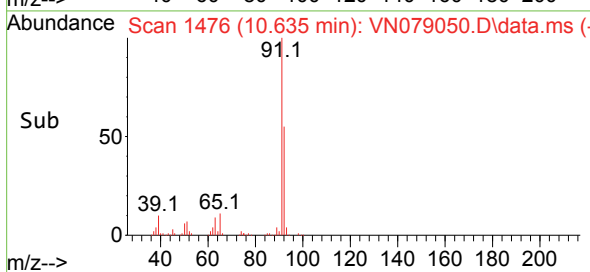
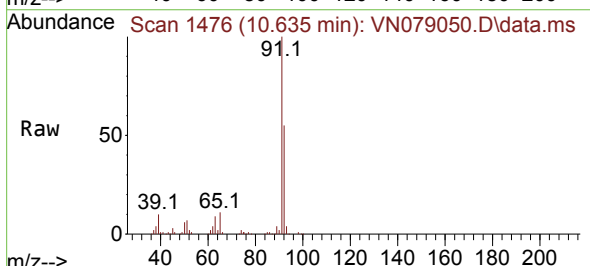





#53
 t-1,3-Dichloropropene
 Concen: 0.562 ug/l
 RT: 10.635 min Scan# 1476
 Delta R.T. -0.206 min
 Lab File: VN079050.D
 Acq: 25 Aug 2023 15:10




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 3044
 Ion Ratio Lower Upper
 75 100
 77 82.9 25.4 38.0#



#62
 4-Bromofluorobenzene
 Concen: 48.754 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.000 min
 Lab File: VN079050.D
 Acq: 25 Aug 2023 15:10


Tgt Ion: 95 Resp: 186263
 Ion Ratio Lower Upper
 95 100
 174 78.4 0.0 143.8
 176 76.7 0.0 135.8

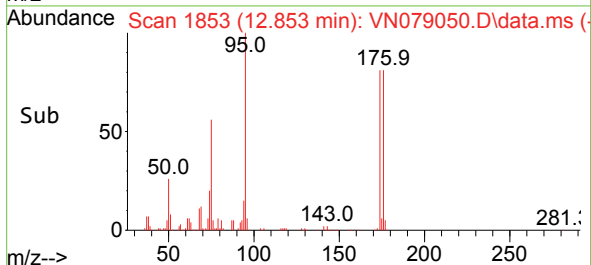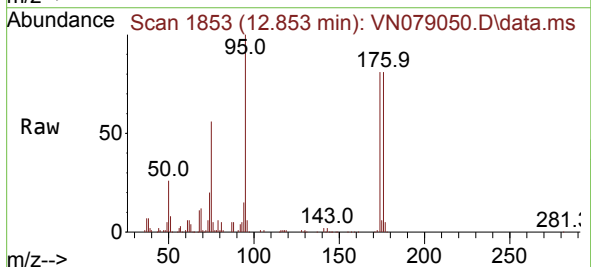






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 404942
Ion Ratio Lower Upper
117 100
82 55.7 44.0 66.0
119 31.2 25.6 38.4



#67
Ethyl Benzene
Concen: 28.280 ug/l
RT: 11.971 min Scan# 1703
Delta R.T. -0.000 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion: 91 Resp: 443292
Ion Ratio Lower Upper
91 100
106 31.2 25.6 38.4


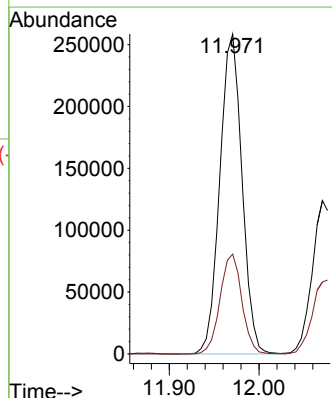
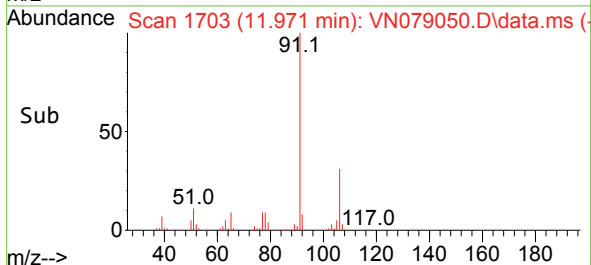
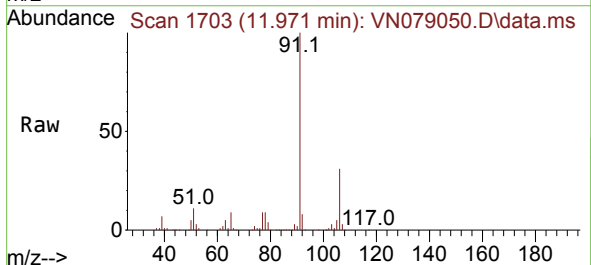




#68
m/p-Xylenes
Concen: 19.655 ug/l
RT: 12.076 min Scan# 1721
Delta R.T. 0.000 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 115192
Ion Ratio Lower Upper
106 100
91 201.6 159.6 239.4



#69
o-Xylene
Concen: 9.144 ug/l
RT: 12.406 min Scan# 1777
Delta R.T. 0.006 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion:106 Resp: 52133
Ion Ratio Lower Upper
106 100
91 218.1 105.2 315.5

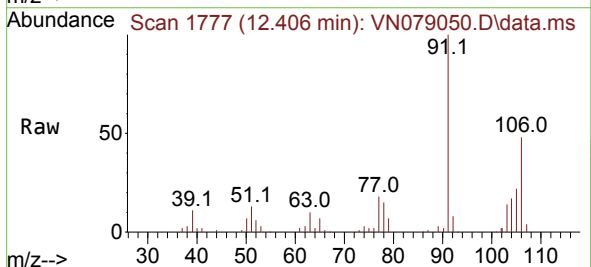



#70

Styrene

Concen: 2.888 ug/l

RT: 12.412 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:104 Resp: 27456

Ion Ratio Lower Upper

104 100

78 67.3 39.5 59.3#

103 73.7 43.2 64.8#

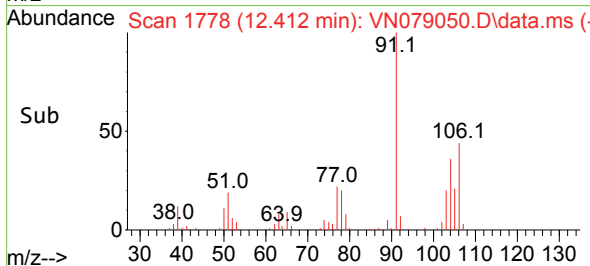

#71

Bromoform

Concen: 0.355 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.265 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10




Tgt Ion:173 Resp: 840


Ion Ratio Lower Upper

173 100

175 1104.3 24.3 73.0#

254 0.0 0.0 0.0


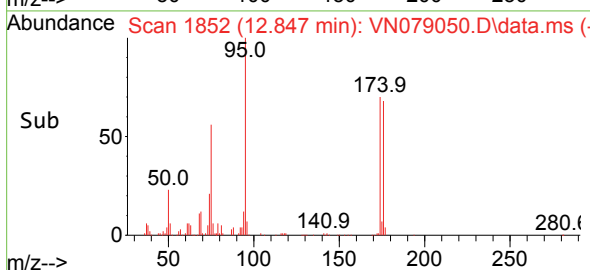

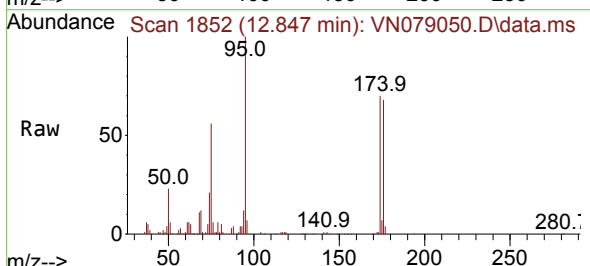




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. 0.006 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 175762
Ion Ratio Lower Upper
152 100
115 60.8 32.3 96.8
150 159.3 0.0 355.8



#73
Isopropylbenzene
Concen: 0.582 ug/l
RT: 12.700 min Scan# 1827
Delta R.T. 0.000 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion:105 Resp: 8529
Ion Ratio Lower Upper
105 100
120 26.0 13.1 39.1





#76

1,2,3-Trichloropropane

Concen: 23.965 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 75 Resp: 101494

Ion Ratio Lower Upper

75 100

77 1.3 84.5 253.5#

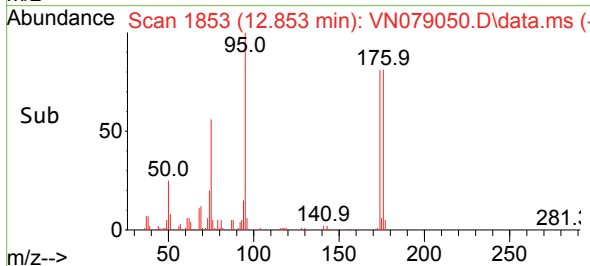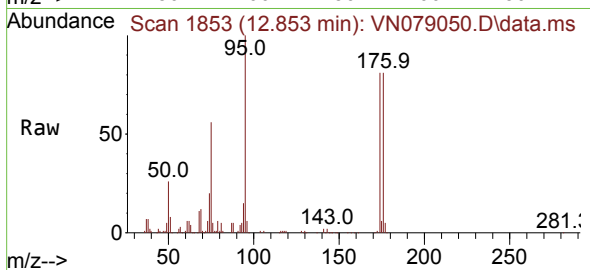

#78

n-propylbenzene

Concen: 0.758 ug/l

RT: 13.041 min Scan# 1885

Delta R.T. 0.000 min

Lab File: VN079050.D




Acq: 25 Aug 2023 15:10


Tgt Ion: 91 Resp: 12881

Ion Ratio Lower Upper

91 100

120 20.0 11.5 34.4

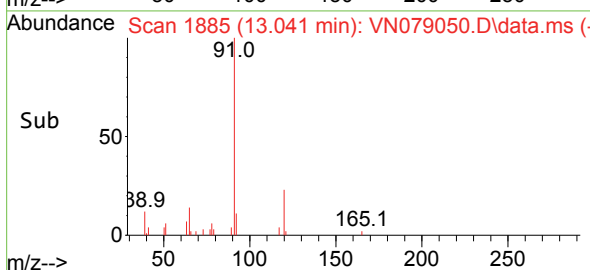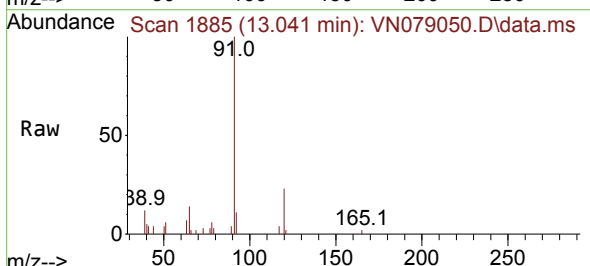



#79

2-Chlorotoluene

Concen: 0.727 ug/l

RT: 13.135 min Scan# 1901

Delta R.T. 0.006 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 91 Resp: 7668

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.8#



#80

1,3,5-Trimethylbenzene

Concen: 2.768 ug/l

RT: 13.176 min Scan# 1908

Delta R.T. 0.000 min

Lab File: VN079050.D




Acq: 25 Aug 2023 15:10


Tgt Ion:105 Resp: 32151

Ion Ratio Lower Upper

105 100

120 50.9 24.1 72.3




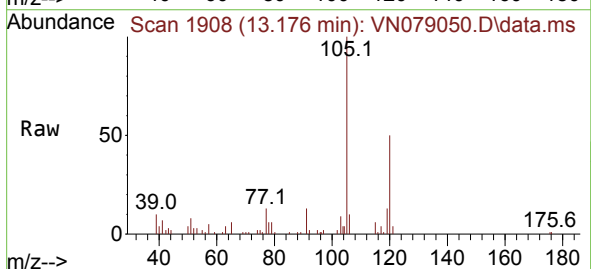




#81
trans-1,4-Dichloro-2-butene
Concen: 61.221 ug/l
RT: 12.853 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 101494
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#

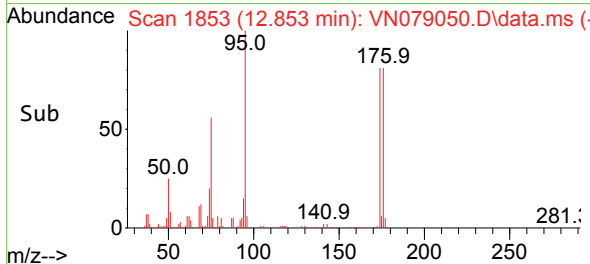

#82
4-Chlorotoluene
Concen: 0.360 ug/l
RT: 13.176 min Scan# 1908
Delta R.T. -0.053 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion: 91 Resp: 3712
Ion Ratio Lower Upper
91 100
126 0.0 16.7 50.0#

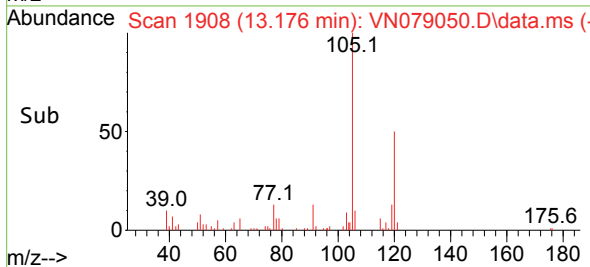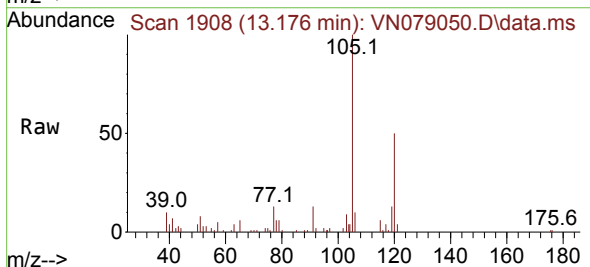



#83

tert-Butylbenzene

Concen: 1.511 ug/l

RT: 13.482 min Scan# 1953

Delta R.T. 0.041 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:119 Resp: 14741

Ion Ratio Lower Upper

119 100

91 100.3 33.9 101.7

134 0.0 13.2 39.6#

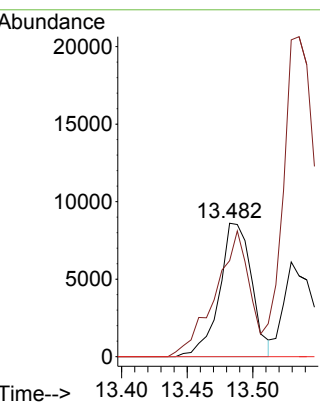

#84

1,2,4-Trimethylbenzene

Concen: 9.931 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. 0.000 min

Lab File: VN079050.D




Acq: 25 Aug 2023 15:10


Tgt Ion:105 Resp: 114201

Ion Ratio Lower Upper

105 100

120 46.2 22.0 66.0

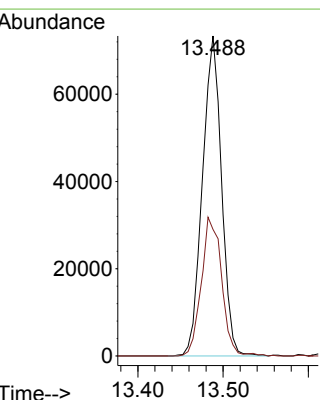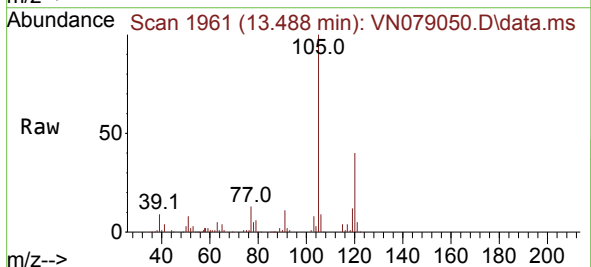



#85

sec-Butylbenzene

Concen: 8.504 ug/l

RT: 13.488 min Scan# 1984

Delta R.T. -0.135 min


Lab File: VN079050.D

Acq: 25 Aug 2023 15:10

Instrument :

MSVOA_N

ClientSampleId :



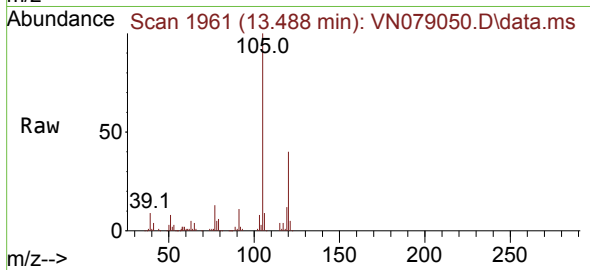


Tgt Ion:105 Resp: 114201

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.3#

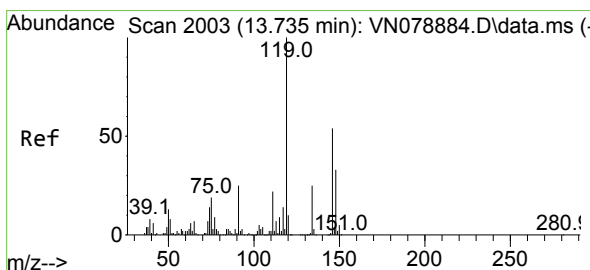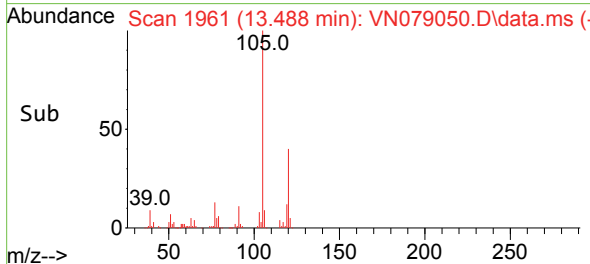

#86

p-Isopropyltoluene

Concen: 0.475 ug/l

RT: 13.729 min Scan# 2002

Delta R.T. -0.006 min

Lab File: VN079050.D

Acq: 25 Aug 2023 15:10




Tgt Ion:119 Resp: 5099


Ion Ratio Lower Upper

119 100

134 26.2 12.6 37.8

91 36.8 12.4 37.2


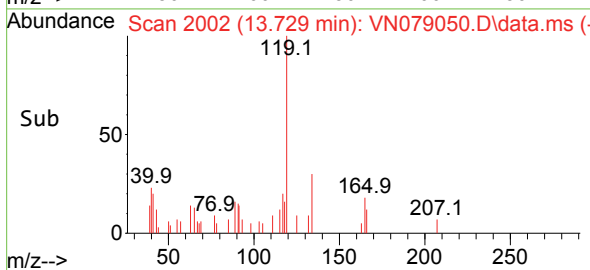
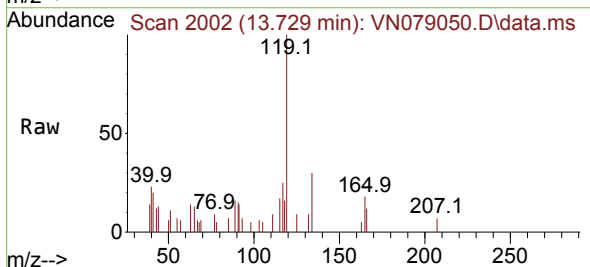





#89
n-Butylbenzene
Concen: 0.318 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. -0.000 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 2806
Ion Ratio Lower Upper
91 100
92 58.7 26.4 79.0
134 0.0 12.6 37.6#



#90
Hexachloroethane
Concen: 5.815 ug/l
RT: 14.370 min Scan# 2111
Delta R.T. 0.035 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion: 117 Resp: 12507
Ion Ratio Lower Upper
117 100
201 0.0 29.3 88.0#


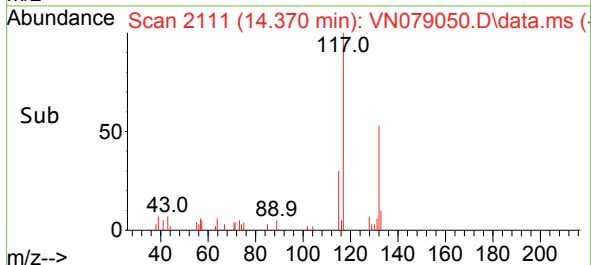

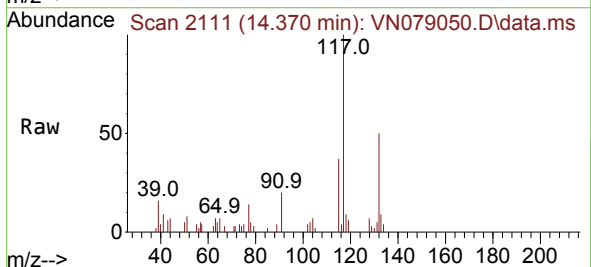




#92
1,2-Dibromo-3-Chloropropane
Concen: Below Cal
RT: 14.700 min Scan# 2171
Delta R.T. -0.023 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion: 75 Resp: 548
Ion Ratio Lower Upper
75 100
155 0.0 39.1 117.2#
157 0.0 50.3 150.9#

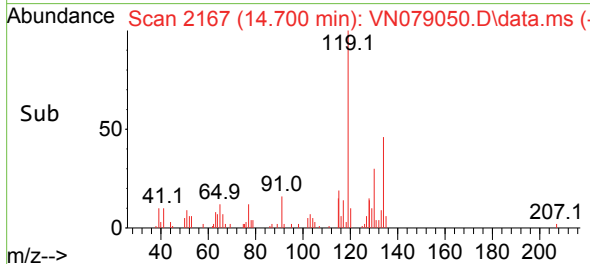

#95
Naphthalene
Concen: 458.926 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. -0.000 min
Lab File: VN079050.D
Acq: 25 Aug 2023 15:10

Tgt Ion:128 Resp: 3896916
Ion Ratio Lower Upper
128 100
127 13.4 10.0 15.0
129 11.0 8.7 13.1

