
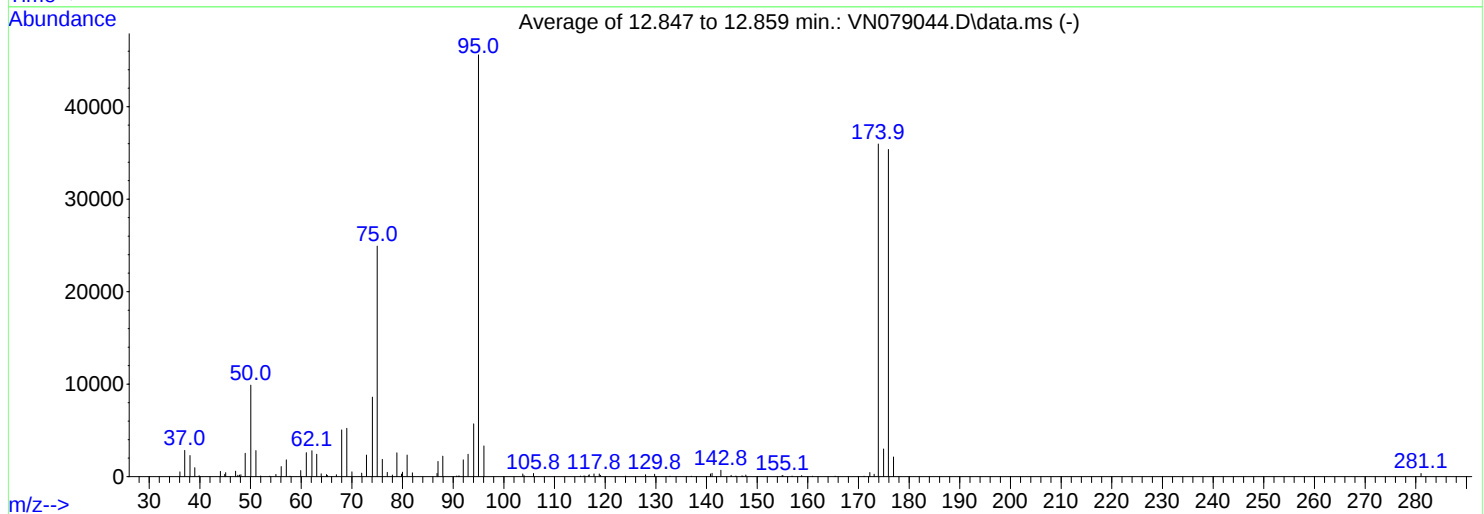


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082523\
Data File : VN079044.D
Acq On : 25 Aug 2023 09:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Title : SW846 8260
Last Update : Wed Aug 16 02:42:02 2023

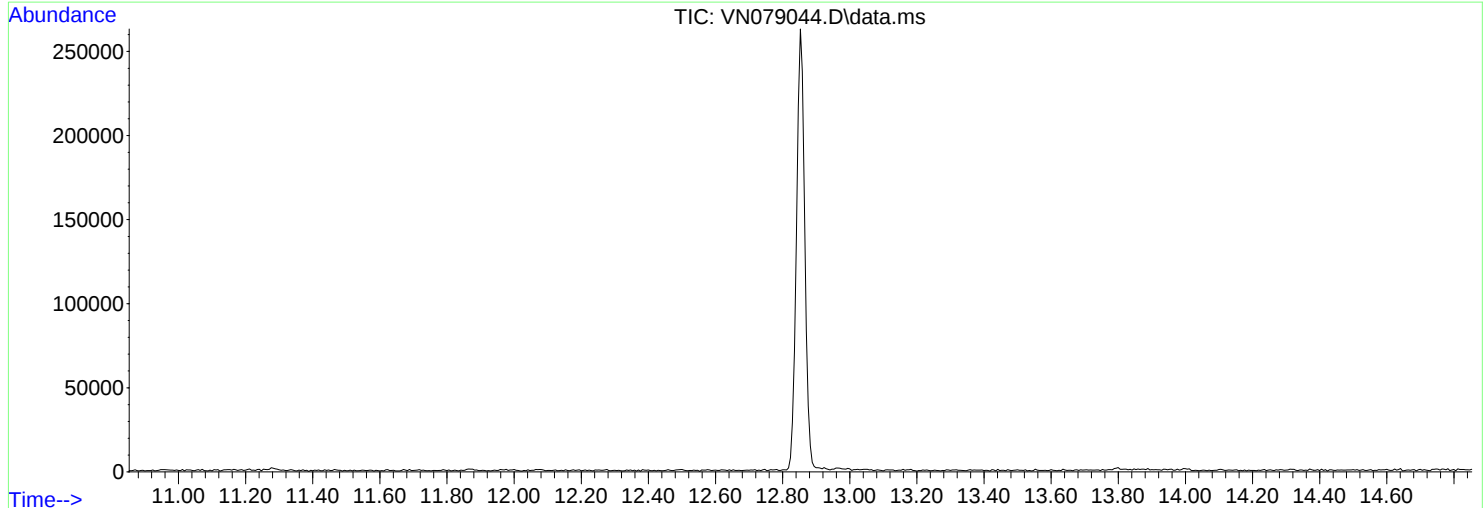

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	9890	PASS
75	95	30	60	54.7	24933	PASS
95	95	100	100	100.0	45605	PASS
96	95	5	9	7.3	3331	PASS
173	174	0.00	2	0.7	263	PASS
174	95	50	100	78.9	35965	PASS
175	174	5	9	8.3	2987	PASS
176	174	95	101	98.4	35384	PASS
177	176	5	9	6.0	2129	PASS

Average of 12.847 to 12.859 min.: VN079044.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	522	48.10	214	61.00	2595	72.90	234
37.00	2847	48.95	2521	62.10	2805	74.05	860
38.05	2289	50.05	9890	63.05	2419	75.00	2493
39.00	962	51.05	2816	63.95	317	76.00	186
39.85	96	52.00	70	65.00	222	77.00	477
44.05	568	53.80	51	65.15	135	78.00	180
44.90	242	55.00	247	66.95	201	78.90	2572
45.10	427	56.05	1094	68.00	5053	79.80	275
47.05	586	57.05	1812	69.00	5226	80.00	488
47.50	162	57.80	53	70.00	528	80.90	2329
47.80	183	59.90	654	71.95	389	81.95	413

Average of 12.847 to 12.859 min.: VN079044.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.80	342	103.75	292	124.00	60	147.20	57
87.00	1649	104.00	110	127.95	201	147.75	182
87.95	2214	105.85	340	129.75	264	154.90	82
90.70	74	115.10	79	132.80	53	155.05	143
91.00	66	115.80	68	137.00	50	156.90	63
91.20	78	116.00	75	140.80	292	158.80	118
92.00	1824	116.70	113	141.10	370	160.90	50
92.95	2424	116.85	207	142.85	698	165.40	54
94.05	5717	117.80	303	144.85	145	171.10	54
95.00	45605	118.85	298	145.80	62	172.25	458
96.05	3331	119.10	134	147.00	80	173.10	263

Average of 12.847 to 12.859 min.: VN079044.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.90	35965						
174.95	2987						
175.90	35384						
176.90	2129						
281.05	349						

Instrument :

MSVOA_N

ClientSampleId :

BFB