

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082525\
 Data File : VN087657.D
 Acq On : 25 Aug 2025 15:01
 Operator : JC\MD
 Sample : Q2936-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-19A-082125

Quant Time: Aug 26 01:36:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 22 02:55:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.212	168	213929	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	506260	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	481175	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	228100	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.565	65	255422	58.273	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 116.540%	
35) Dibromofluoromethane	8.147	113	185124	50.647	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.300%	
50) Toluene-d8	10.547	98	669638	48.948	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 97.900%	
62) 4-Bromofluorobenzene	12.829	95	229279	47.125	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 94.260%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082525\
Data File : VN087657.D
Acq On : 25 Aug 2025 15:01
Operator : JC\MD
Sample : Q2936-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-19A-082125

Quant Time: Aug 26 01:36:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 22 02:55:42 2025
Response via : Initial Calibration




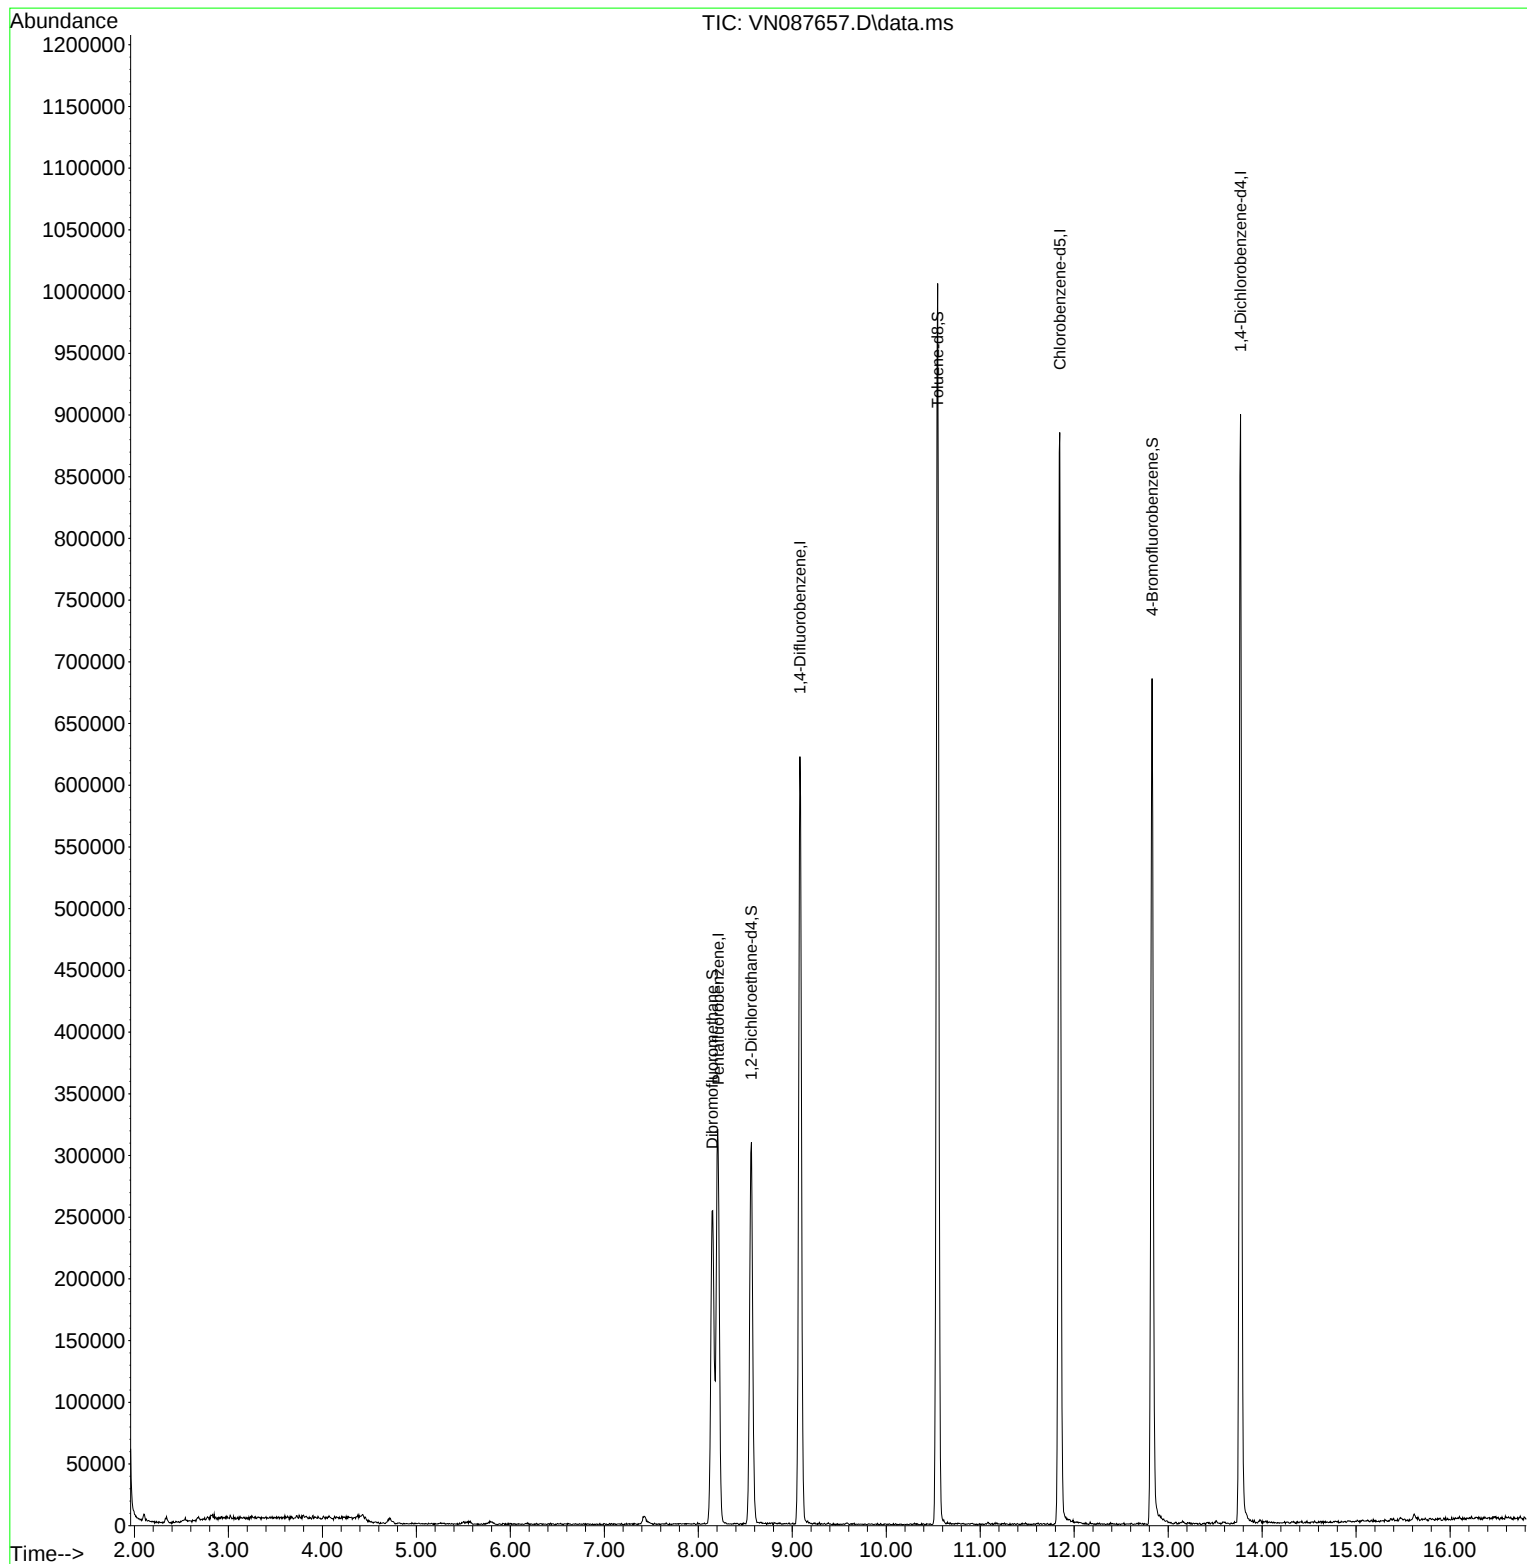


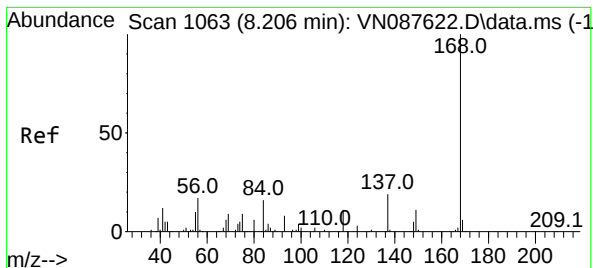

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.212 min Scan# 1064
Delta R.T. 0.006 min
Lab File: VN087657.D
Acq: 25 Aug 2025 15:01




Instrument :
MSVOA_N
ClientSampleId :
MW-19A-082125


Tgt Ion:168 Resp: 213929
Ion Ratio Lower Upper
168 100
99 68.2 57.2 85.8

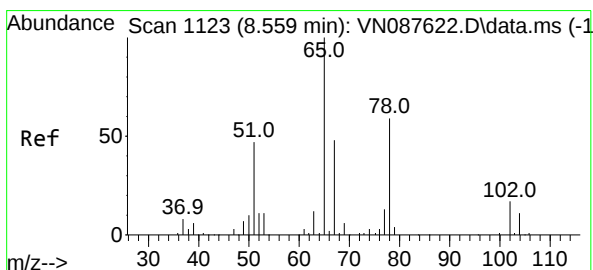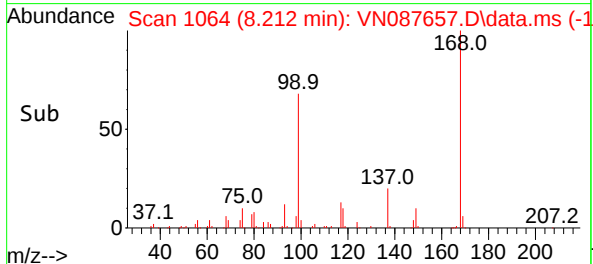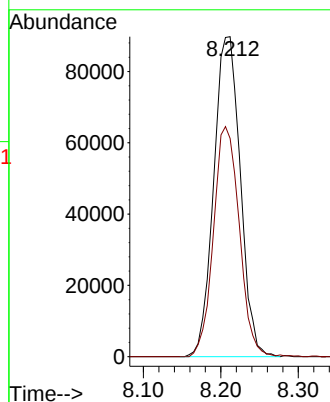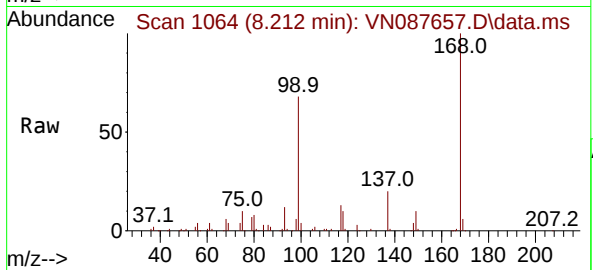

#33
1,2-Dichloroethane-d4
Concen: 58.273 ug/l
RT: 8.565 min Scan# 1124
Delta R.T. 0.006 min
Lab File: VN087657.D
Acq: 25 Aug 2025 15:01

Tgt Ion: 65 Resp: 255422
Ion Ratio Lower Upper
65 100
67 51.2 0.0 100.0

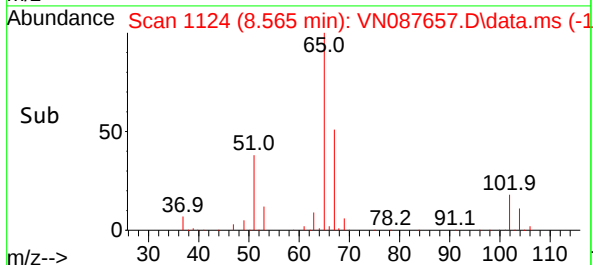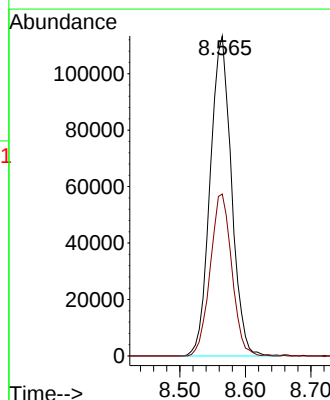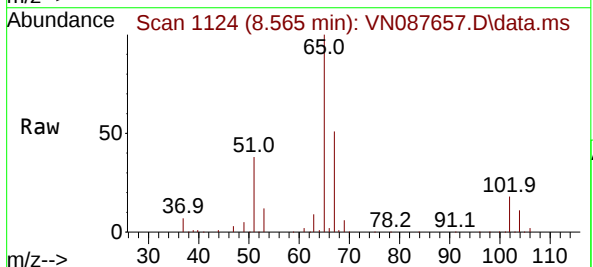

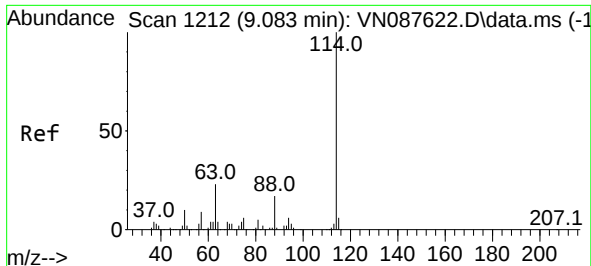

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN087657.D

Acq: 25 Aug 2025 15:01

Instrument :

MSVOA_N

ClientSampleId :

MW-19A-082125





Tgt Ion:114 Resp: 506260

Ion Ratio Lower Upper

114 100

63 22.7 0.0 45.2

88 16.8 0.0 33.4

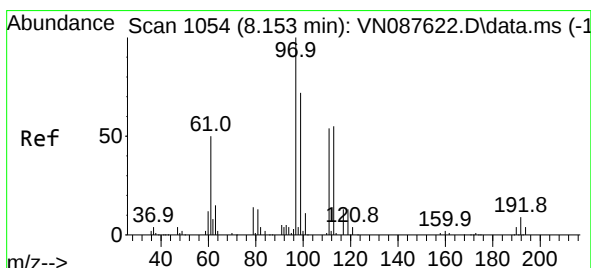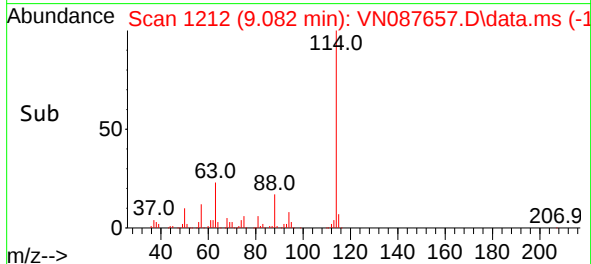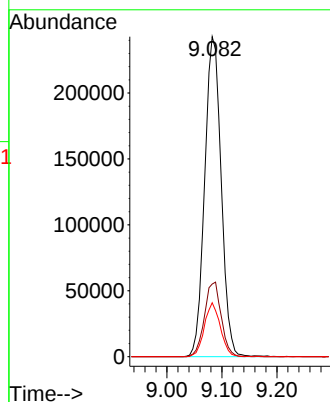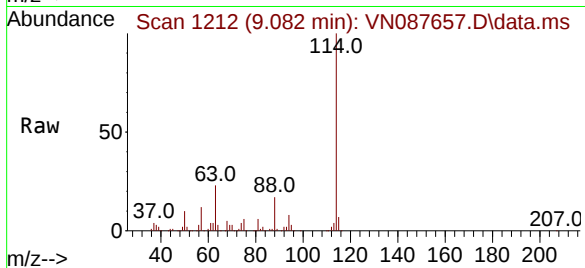

#35

Dibromofluoromethane

Concen: 50.647 ug/l

RT: 8.147 min Scan# 1053

Delta R.T. -0.006 min

Lab File: VN087657.D

Acq: 25 Aug 2025 15:01




Tgt Ion:113 Resp: 185124


Ion Ratio Lower Upper

113 100

111 103.2 82.8 124.2

192 15.9 12.8 19.2


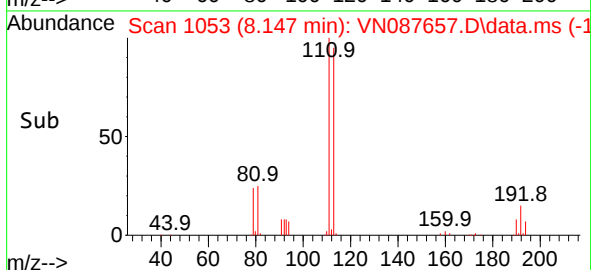
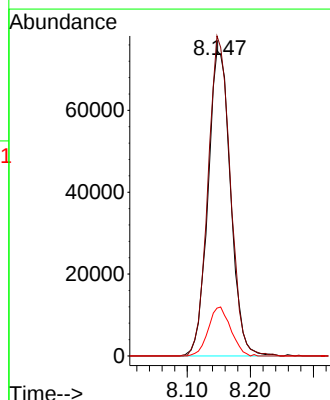
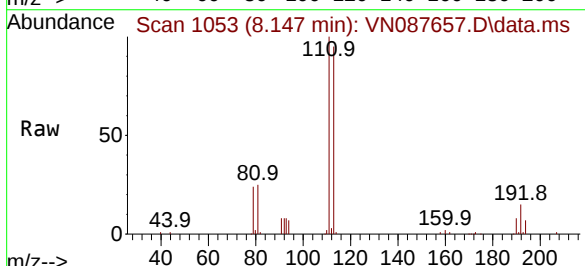


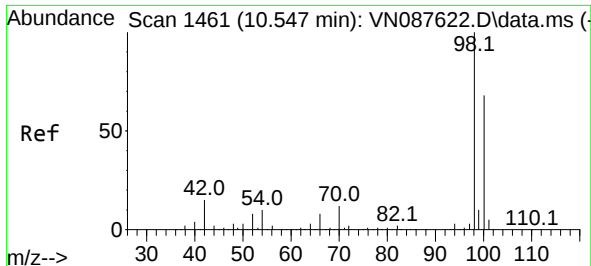

#50
Toluene-d8
Concen: 48.948 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087657.D
Acq: 25 Aug 2025 15:01




Instrument :
MSVOA_N
ClientSampleId :
MW-19A-082125


Tgt Ion: 98 Resp: 669638
Ion Ratio Lower Upper
98 100
100 63.7 52.8 79.2

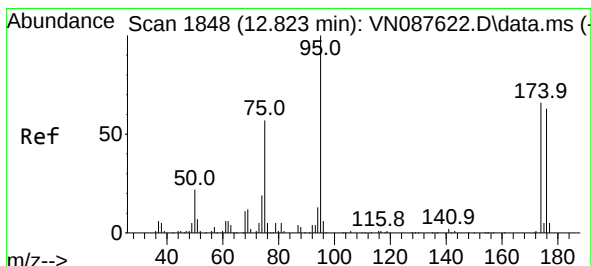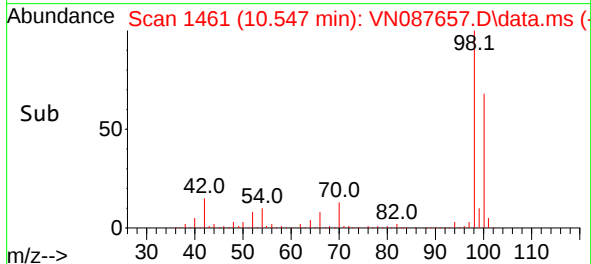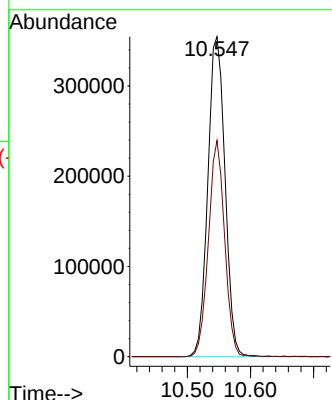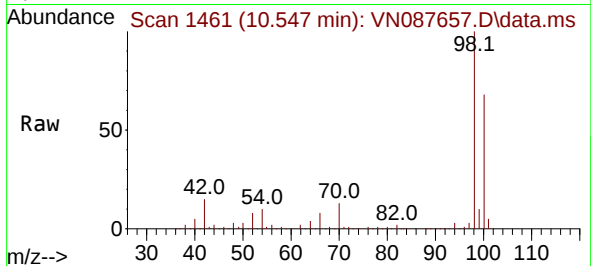

#62
4-Bromofluorobenzene
Concen: 47.125 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN087657.D
Acq: 25 Aug 2025 15:01

Tgt Ion: 95 Resp: 229279
Ion Ratio Lower Upper
95 100
174 71.9 0.0 138.4
176 68.7 0.0 132.6


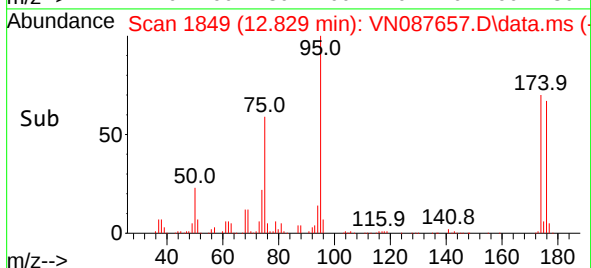
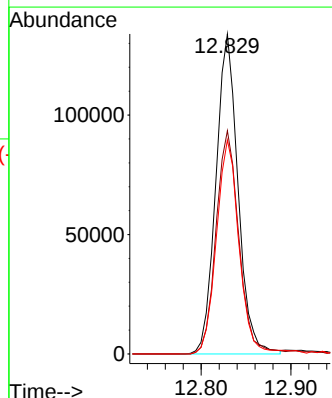
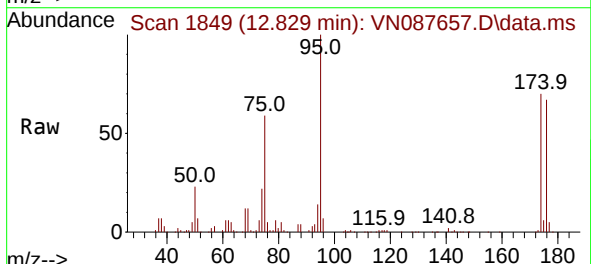


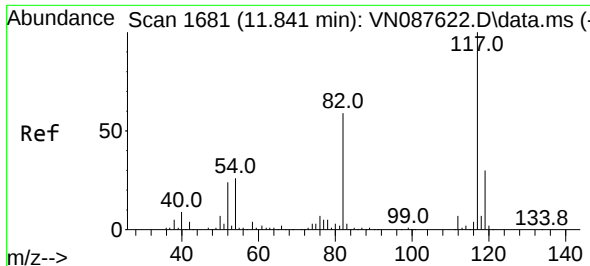

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN087657.D
Acq: 25 Aug 2025 15:01

Instrument :
MSVOA_N
ClientSampleId :
MW-19A-082125

Tgt Ion:117 Resp: 481175
Ion Ratio Lower Upper
117 100
82 55.5 47.4 71.2
119 31.7 24.3 36.5

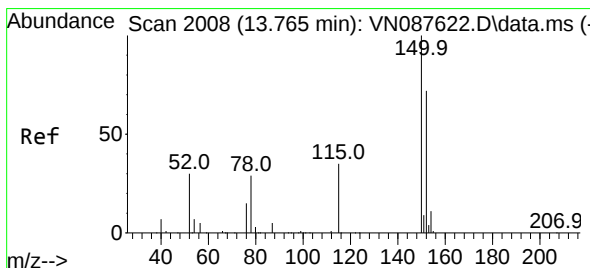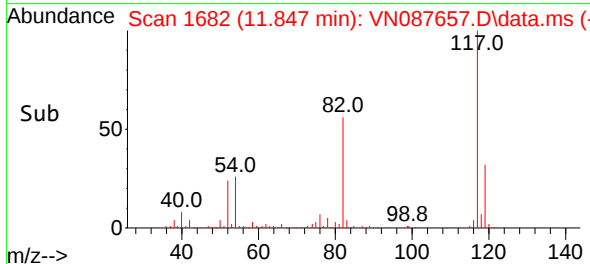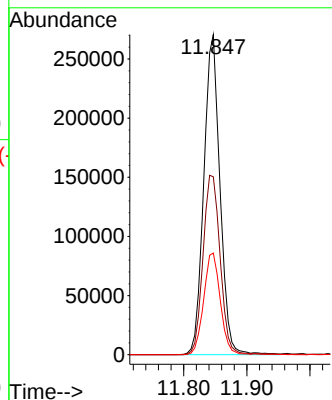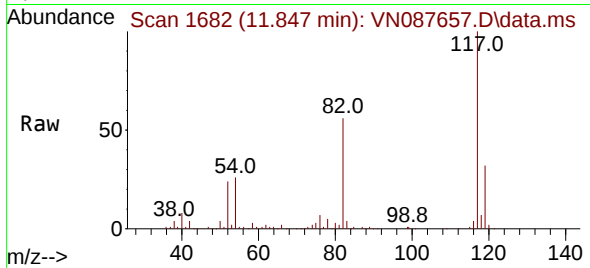

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN087657.D
Acq: 25 Aug 2025 15:01

Tgt Ion:152 Resp: 228100
Ion Ratio Lower Upper
152 100
115 65.4 32.3 96.8
150 157.1 0.0 351.0

