


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082619\
Data File : VN057512.D
Acq On : 26 Aug 2019 15:56
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082219W.M
Title : SW846 8260
Last Update : Fri Aug 23 05:07:29 2019

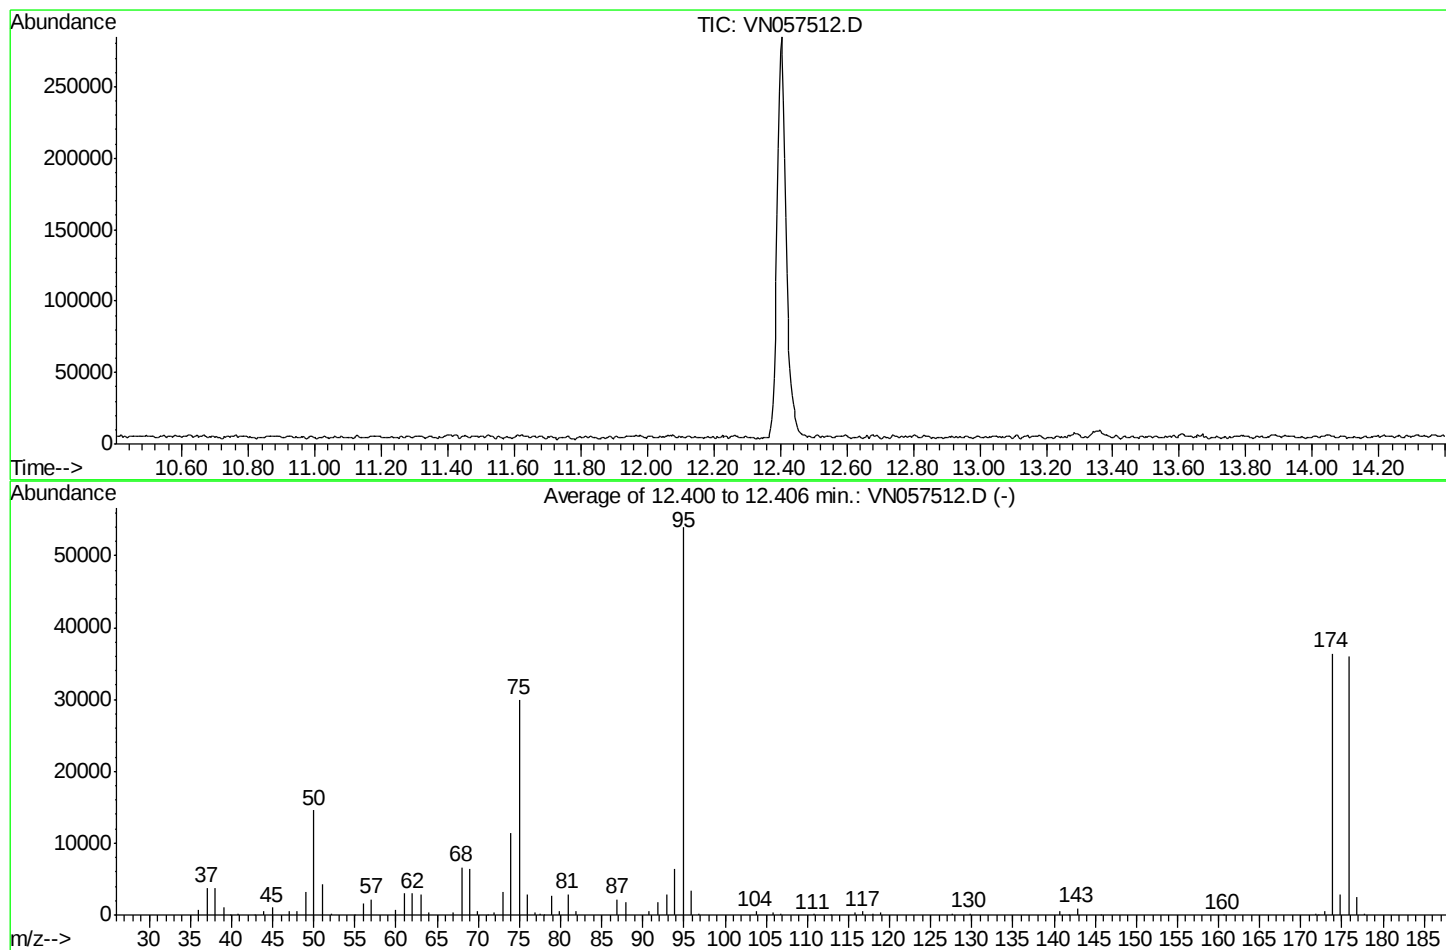

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	27.0	14581	PASS
75	95	30	60	55.5	29965	PASS
95	95	100	100	100.0	53954	PASS
96	95	5	9	6.2	3348	PASS
173	174	0.00	2	1.7	609	PASS
174	95	50	100	67.5	36416	PASS
175	174	5	9	7.7	2794	PASS
176	174	95	101	98.7	35957	PASS
177	176	5	9	6.9	2493	PASS