


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082620\
Data File : VN063126.D
Acq On : 26 Aug 2020 12:10
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Title : SW846 8260
Last Update : Wed Aug 19 06:09:27 2020

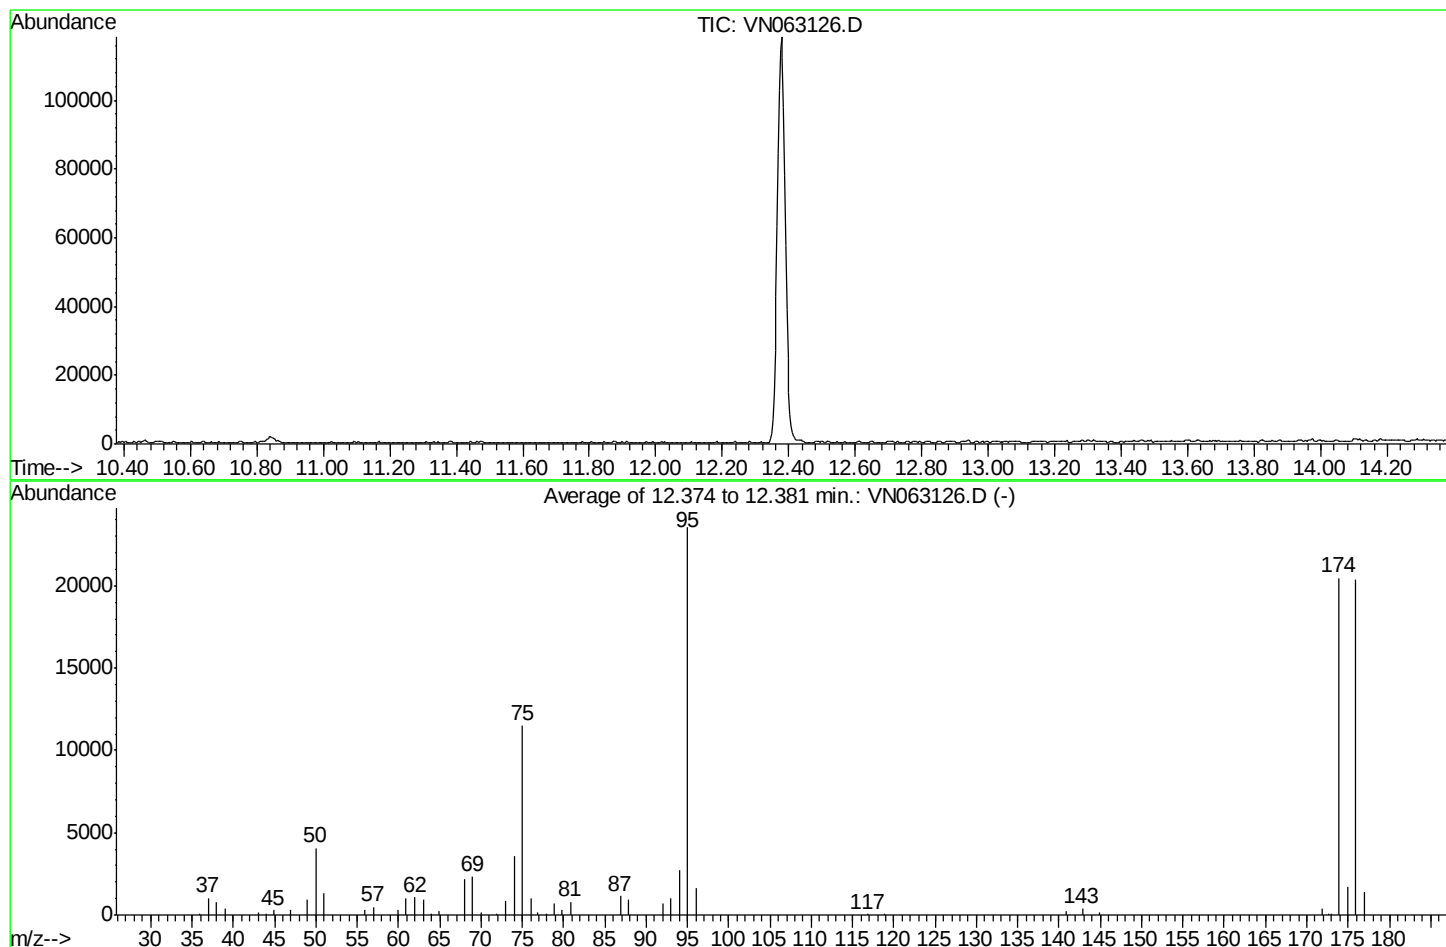

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3285

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	4066	PASS
75	95	30	60	48.7	11479	PASS
95	95	100	100	100.0	23557	PASS
96	95	5	9	6.9	1617	PASS
173	174	0.00	2	0.5	98	PASS
174	95	50	100	87.0	20488	PASS
175	174	5	9	8.4	1718	PASS
176	174	95	101	99.4	20362	PASS
177	176	5	9	6.7	1364	PASS