

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082624\
Data File : VN083491.D
Acq On : 26 Aug 2024 18:34
Operator : JC\MD
Sample : P3633-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DSN001

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M

Title : SW846 8260

Signal : TIC: VN083490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.289	50	57	77	rVB2	84194	195723	22.71%	3.883%
2	2.812	141	146	147	rBV4	5796	9146	1.06%	0.181%
3	4.436	412	422	435	rBV	70248	199532	23.15%	3.958%
4	8.165	1046	1056	1061	rBV	109706	268459	31.15%	5.326%
5	8.224	1061	1066	1078	rVB	176955	387084	44.92%	7.679%
6	8.577	1116	1126	1139	rBV	118769	265187	30.77%	5.261%
7	9.100	1207	1215	1226	rBV	297220	608718	70.64%	12.076%
8	10.565	1456	1464	1474	rBV	412681	760100	88.20%	15.079%
9	11.865	1677	1685	1700	rBV	496673	861766	100.00%	17.096%
10	12.847	1845	1852	1860	rBV	369874	626805	72.73%	12.435%
11	13.794	2005	2013	2023	rBV	495785	858211	99.59%	17.026%




Sum of corrected areas: 5040731

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082624\
Data File : VN083491.D
Acq On : 26 Aug 2024 18:34
Operator : JC\MD
Sample : P3633-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DSN001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

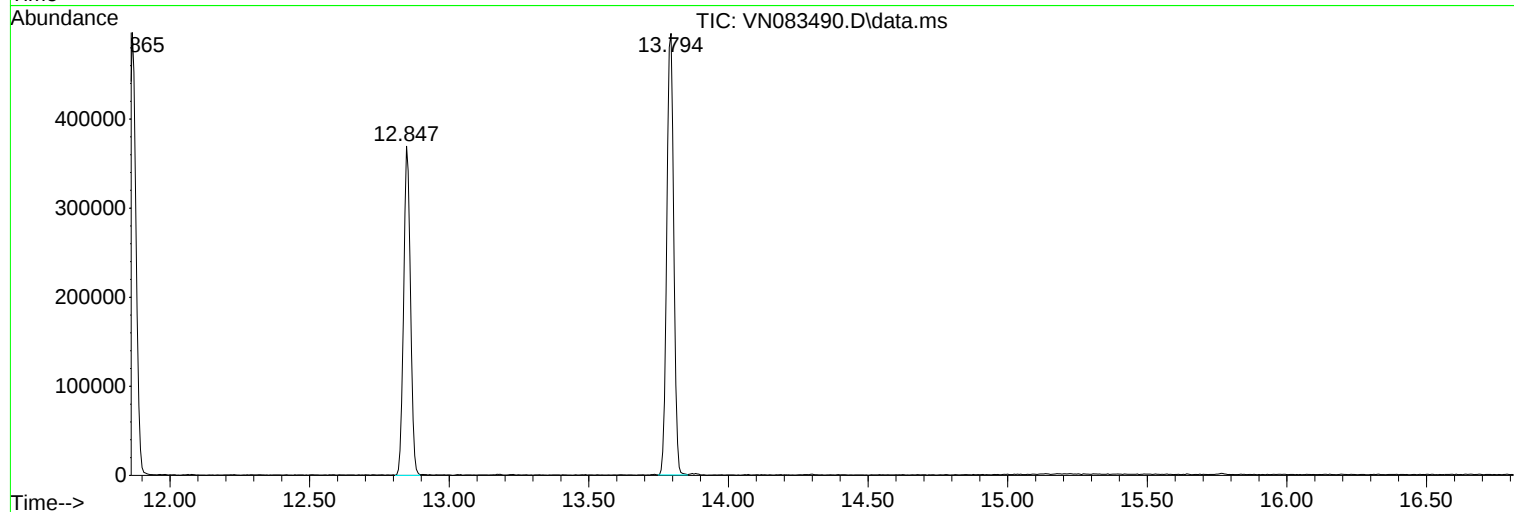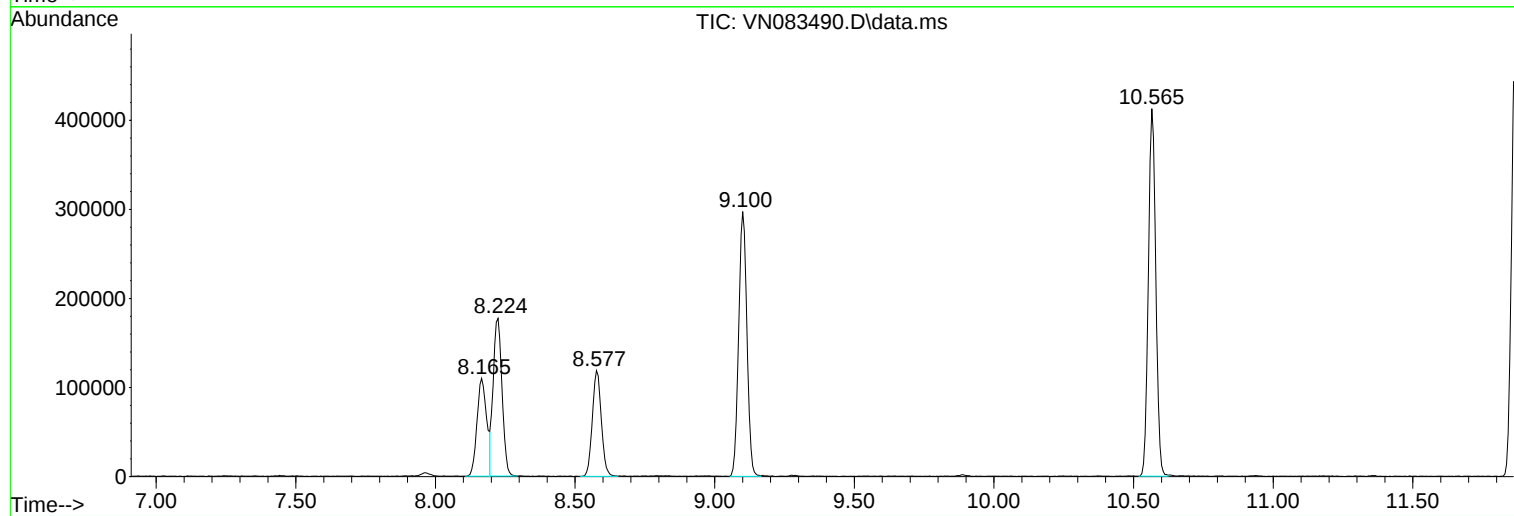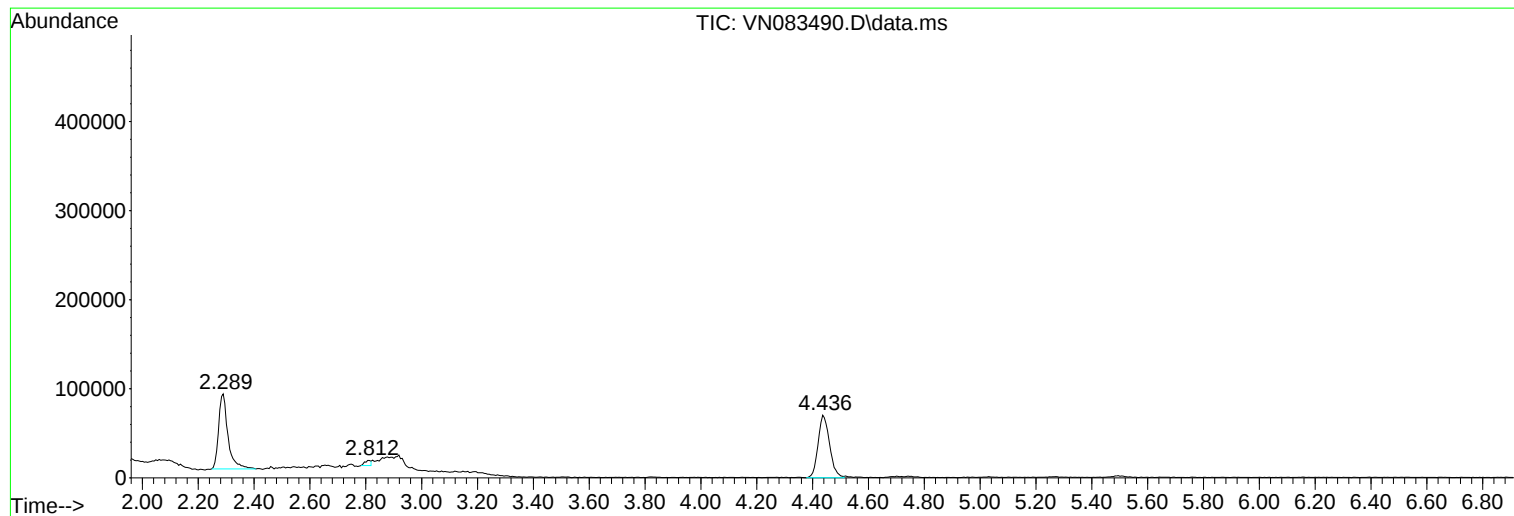

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082624\
Data File : VN083491.D
Acq On : 26 Aug 2024 18:34
Operator : JC\MD
Sample : P3633-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DSN001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	2.289	25.3	ug/l	195723	1	8.224	387084	50.0