
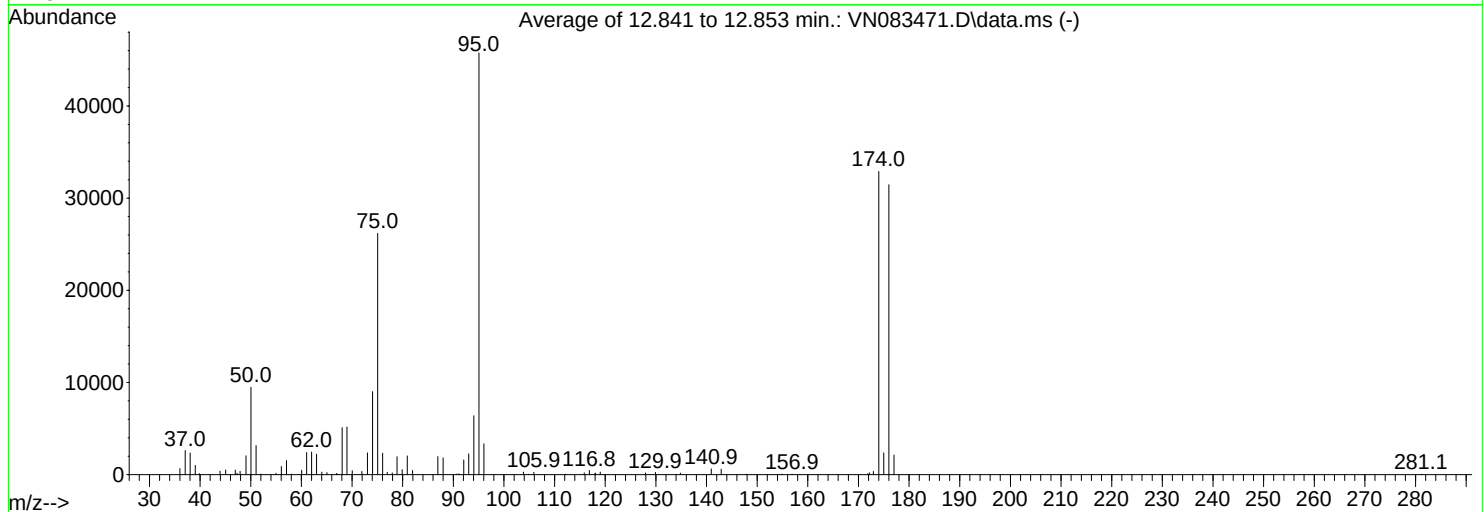


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082624\
Data File : VN083471.D
Acq On : 26 Aug 2024 08:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

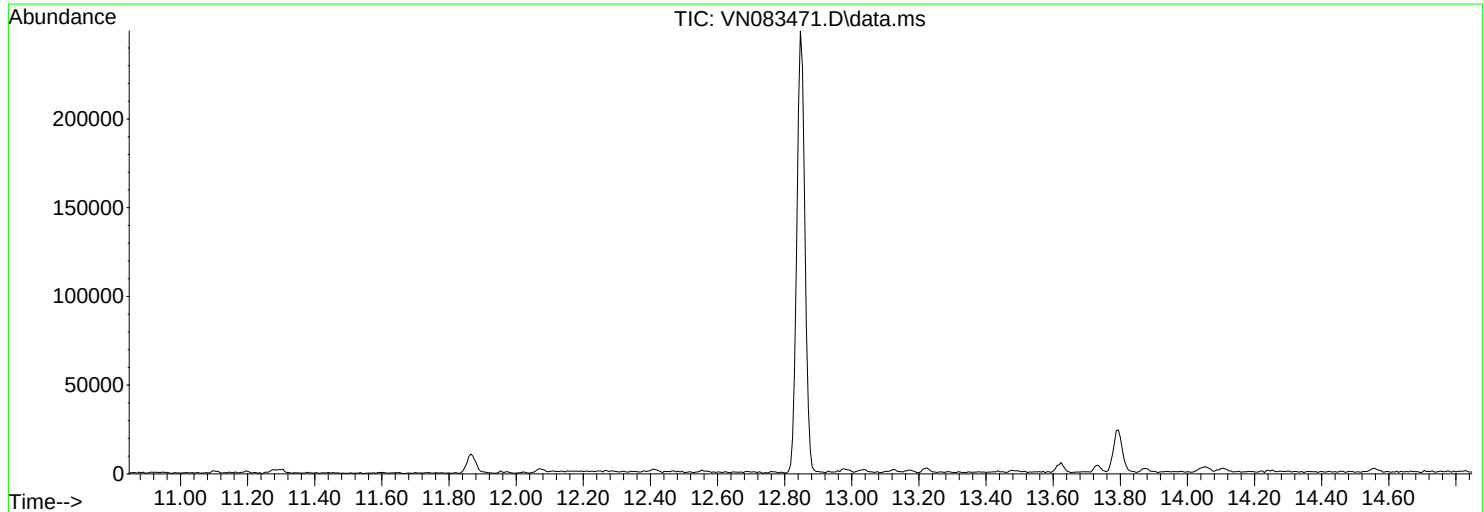

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	9484	PASS
75	95	30	60	57.2	26184	PASS
95	95	100	100	100.0	45763	PASS
96	95	5	9	7.3	3353	PASS
173	174	0.00	2	1.1	351	PASS
174	95	50	100	71.9	32901	PASS
175	174	5	9	7.2	2368	PASS
176	174	95	101	95.6	31451	PASS
177	176	5	9	6.8	2129	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	653	50.05	9484	64.05	271	76.05	233
37.05	2619	51.05	3154	65.05	224	76.95	26
38.05	2348	52.00	70	66.90	125	77.95	19
39.05	1013	55.00	154	67.10	79	78.90	194
39.85	115	56.05	891	68.05	5104	79.90	541
43.95	389	57.05	1531	69.00	5173	80.90	2031
45.05	505	58.10	68	70.05	430	81.95	446
46.95	506	60.05	493	71.95	351	86.95	1957
47.30	150	61.05	2398	73.05	2357	88.00	1827
47.90	363	62.00	2456	74.05	9007	90.70	72
49.05	2048	63.00	2220	75.05	26184	91.10	91

Average of 12.841 to 12.853 min.: VN083471.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.05	1596	117.90	91	171.80	94		
93.05	2260	118.05	169	172.15	214		
94.05	6387	119.00	277	172.95	351		
95.05	45763	127.95	190	174.00	32901		
96.05	3353	129.90	237	175.00	2368		
103.85	280	134.85	177	176.00	31451		
104.90	60	140.95	623	177.00	2129		
105.90	260	142.90	586	281.10	59		
112.20	50	147.80	50				
115.85	189	154.90	56				
116.85	448	156.90	57				

Instrument :

MSVOA_N

ClientSampleId :

BFB