

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082625\
 Data File : VN087669.D
 Acq On : 26 Aug 2025 14:48
 Operator : JC\MD
 Sample : VN0826MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0826MBL01

Quant Time: Aug 27 01:47:44 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 22 02:55:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.212	168	164593	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	384956	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	350926	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	157400	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	187925	55.726	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	111.460%
35) Dibromofluoromethane	8.147	113	142905	51.416	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.840%
50) Toluene-d8	10.547	98	498001	47.872	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.740%
62) 4-Bromofluorobenzene	12.829	95	167062	45.158	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	90.320%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082625\
Data File : VN087669.D
Acq On : 26 Aug 2025 14:48
Operator : JC\MD
Sample : VN0826MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0826MBL01

Quant Time: Aug 27 01:47:44 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 22 02:55:42 2025
Response via : Initial Calibration




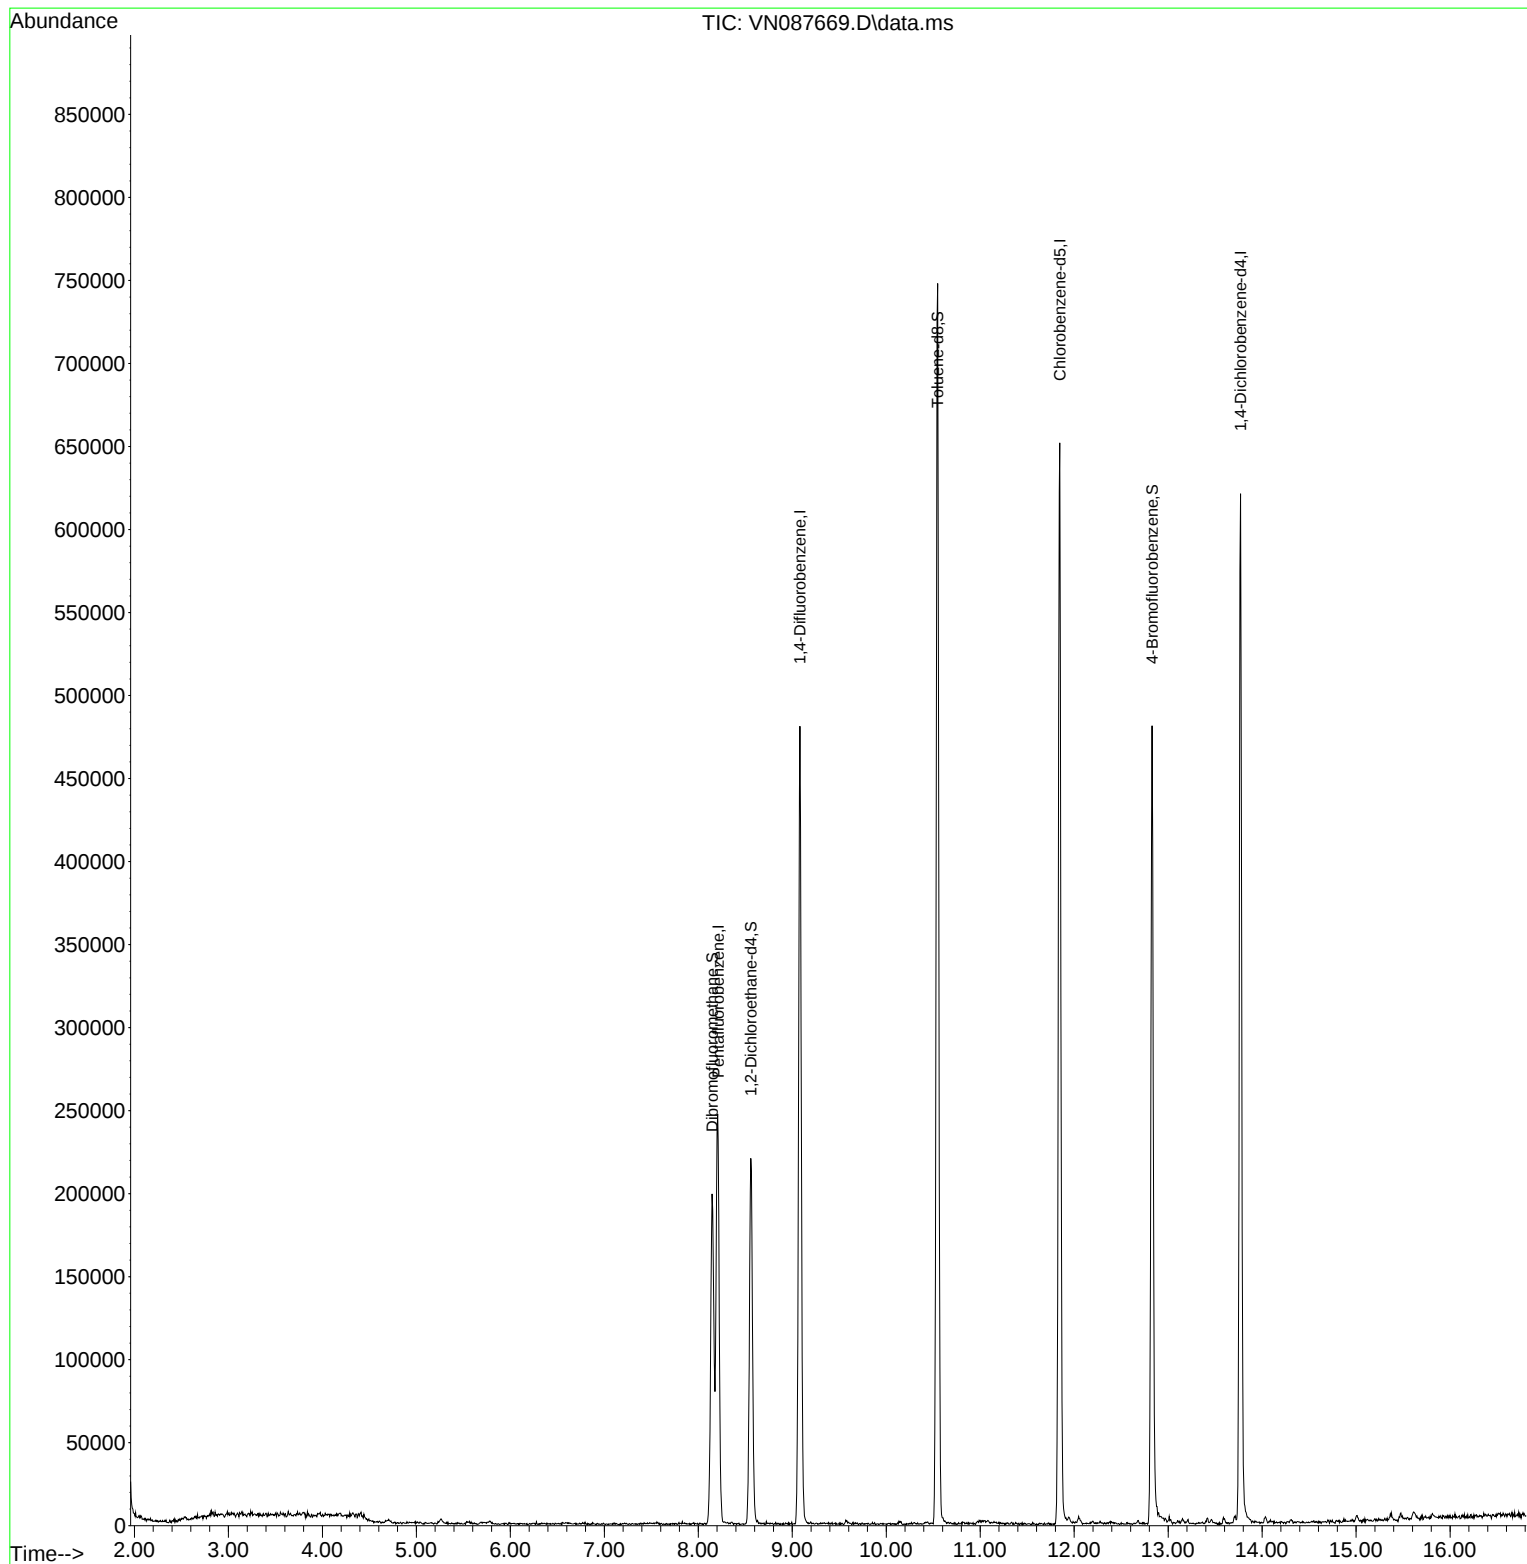


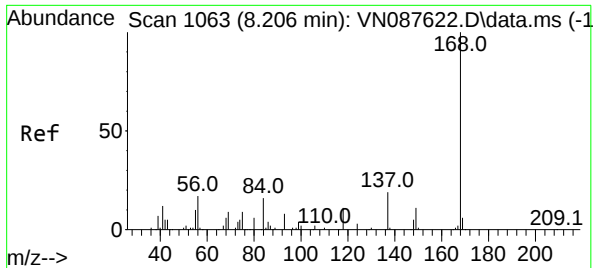

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.212 min Scan# 1064
Delta R.T. 0.006 min
Lab File: VN087669.D
Acq: 26 Aug 2025 14:48




Instrument :
MSVOA_N
ClientSampleId :
VN0826MBL01


Tgt Ion:168 Resp: 164593
Ion Ratio Lower Upper
168 100
99 61.7 57.2 85.8

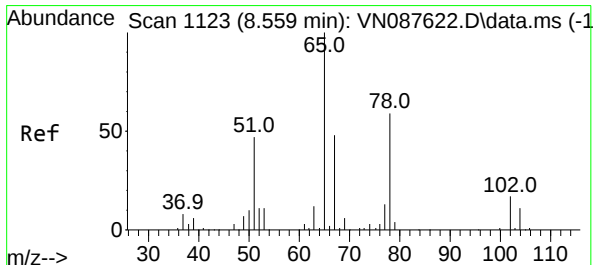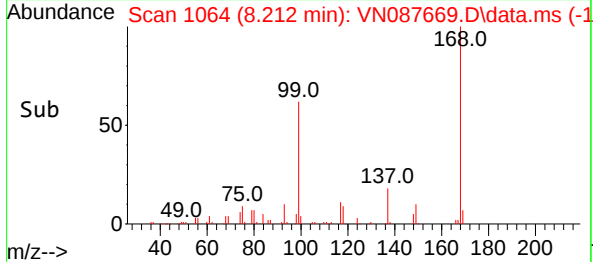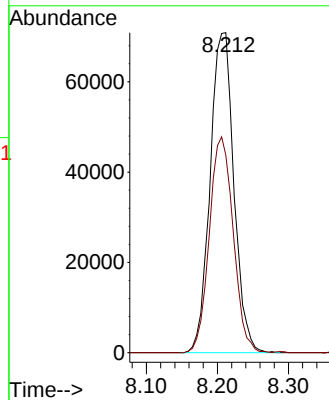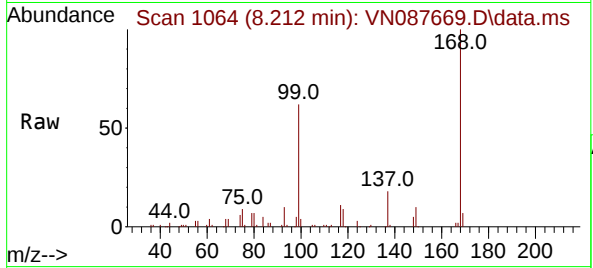

#33
1,2-Dichloroethane-d4
Concen: 55.726 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.000 min
Lab File: VN087669.D
Acq: 26 Aug 2025 14:48

Tgt Ion: 65 Resp: 187925
Ion Ratio Lower Upper
65 100
67 48.5 0.0 100.0

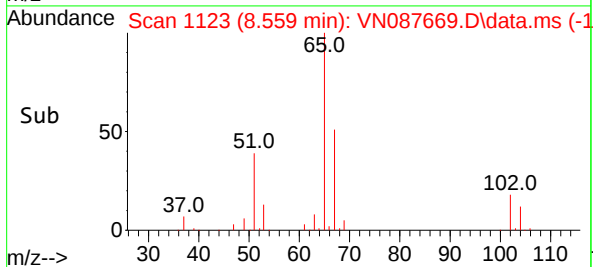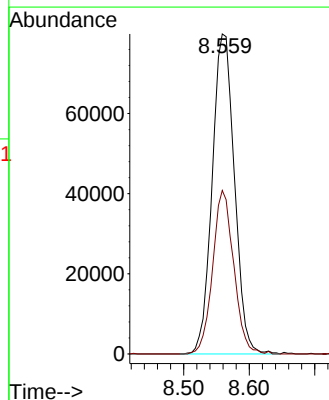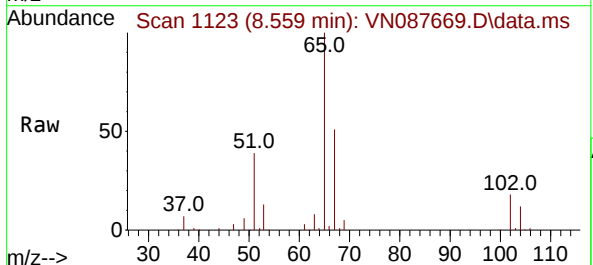

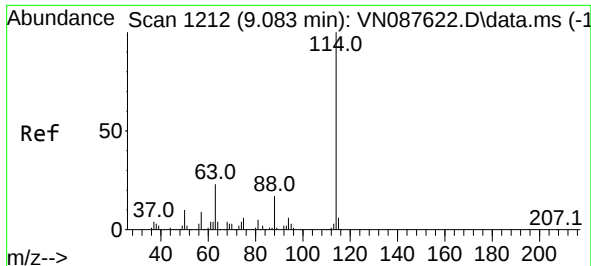

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN087669.D

Acq: 26 Aug 2025 14:48

Instrument :

MSVOA_N

ClientSampleId :

VN0826MBL01





Tgt Ion:114 Resp: 384956

Ion Ratio Lower Upper

114 100

63 23.3 0.0 45.2

88 15.2 0.0 33.4

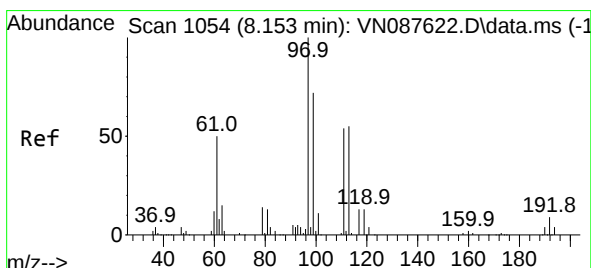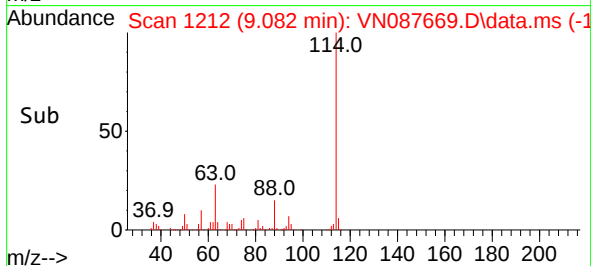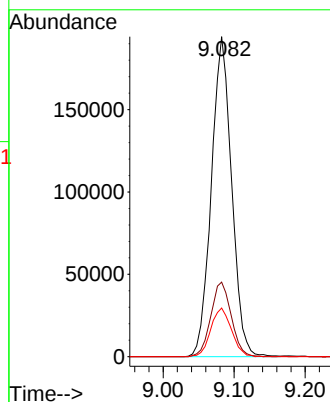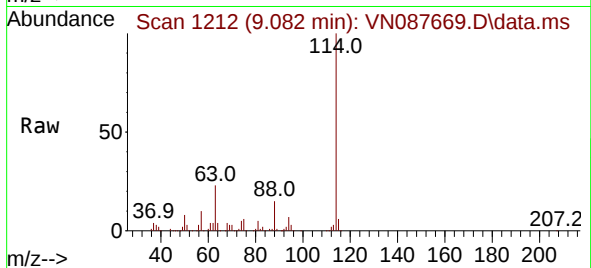

#35

Dibromofluoromethane

Concen: 51.416 ug/l

RT: 8.147 min Scan# 1053

Delta R.T. -0.006 min

Lab File: VN087669.D

Acq: 26 Aug 2025 14:48




Tgt Ion:113 Resp: 142905


Ion Ratio Lower Upper

113 100

111 101.5 82.8 124.2

192 16.0 12.8 19.2


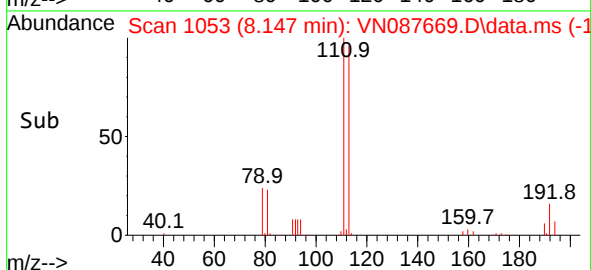
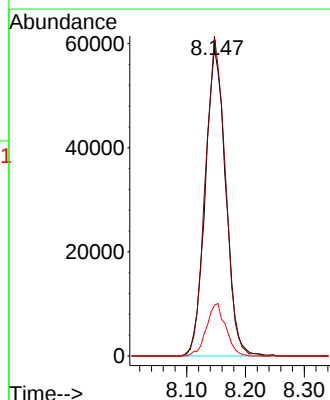
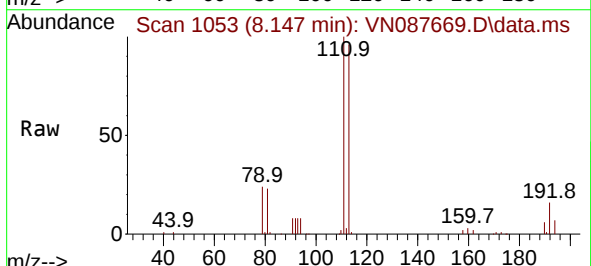


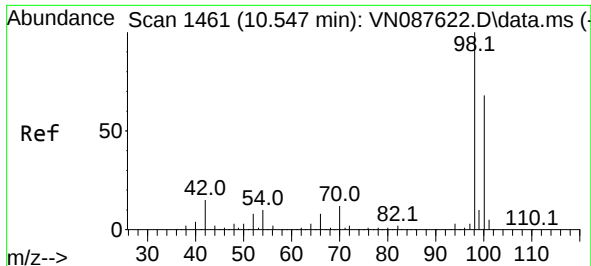

#50
Toluene-d8
Concen: 47.872 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087669.D
Acq: 26 Aug 2025 14:48




Instrument :
MSVOA_N
ClientSampleId :
VN0826MBL01


Tgt Ion: 98 Resp: 498001
Ion Ratio Lower Upper
98 100
100 63.3 52.8 79.2

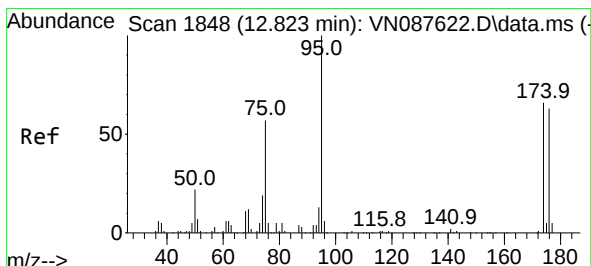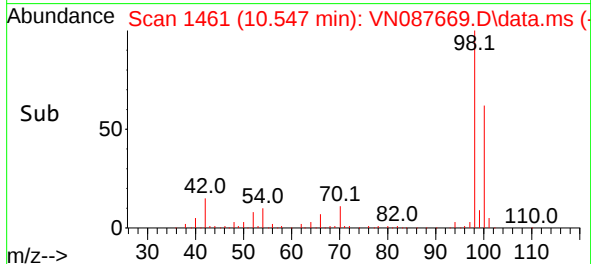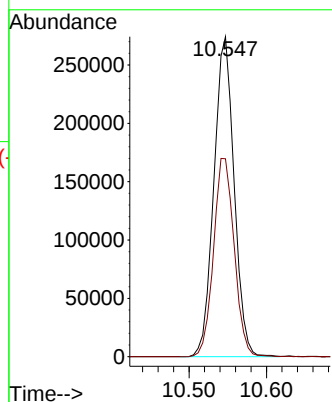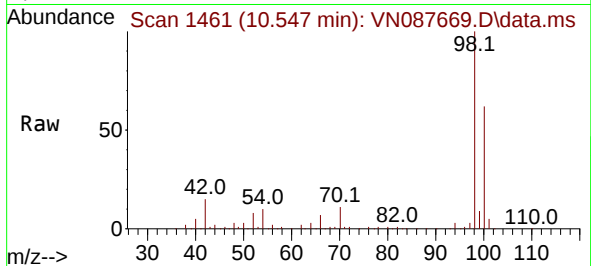

#62
4-Bromofluorobenzene
Concen: 45.158 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN087669.D
Acq: 26 Aug 2025 14:48

Tgt Ion: 95 Resp: 167062
Ion Ratio Lower Upper
95 100
174 68.3 0.0 138.4
176 68.1 0.0 132.6


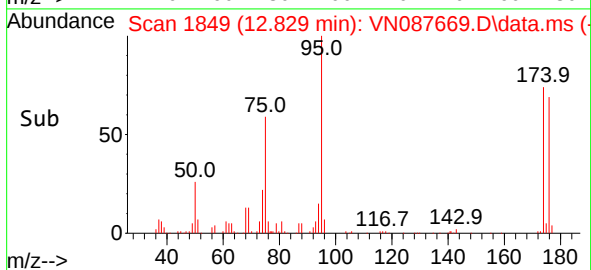
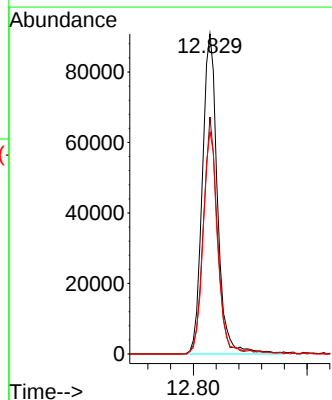
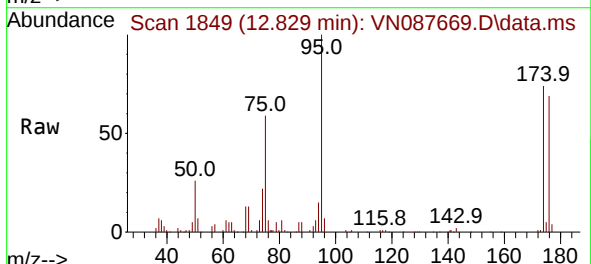


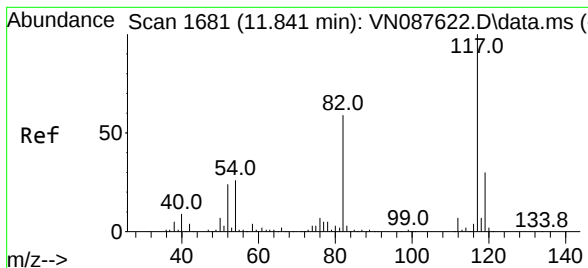

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN087669.D
Acq: 26 Aug 2025 14:48

Instrument :
MSVOA_N
ClientSampleId :
VN0826MBL01

Tgt Ion:117 Resp: 350926
Ion Ratio Lower Upper
117 100
82 60.1 47.4 71.2
119 33.0 24.3 36.5

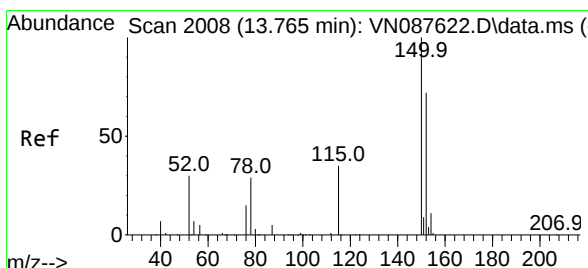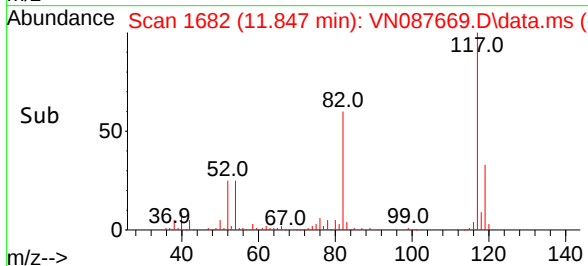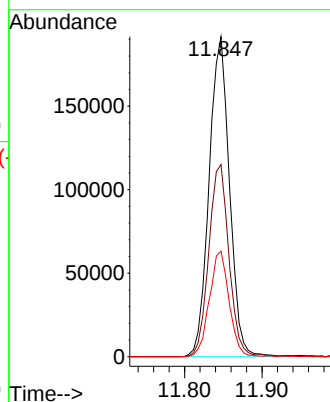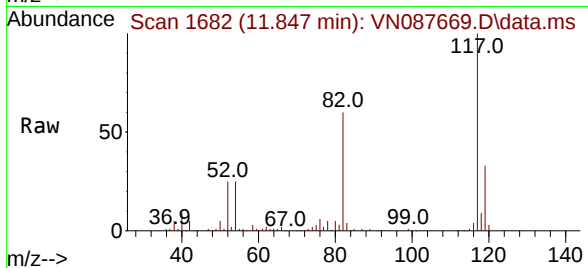

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN087669.D
Acq: 26 Aug 2025 14:48

Tgt Ion:152 Resp: 157400
Ion Ratio Lower Upper
152 100
115 65.8 32.3 96.8
150 157.8 0.0 351.0

