


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082718\
Data File : VN050886.D
Acq On : 27 Aug 2018 9:41
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
Title : SW846 8260
Last Update : Wed Aug 22 05:38:12 2018

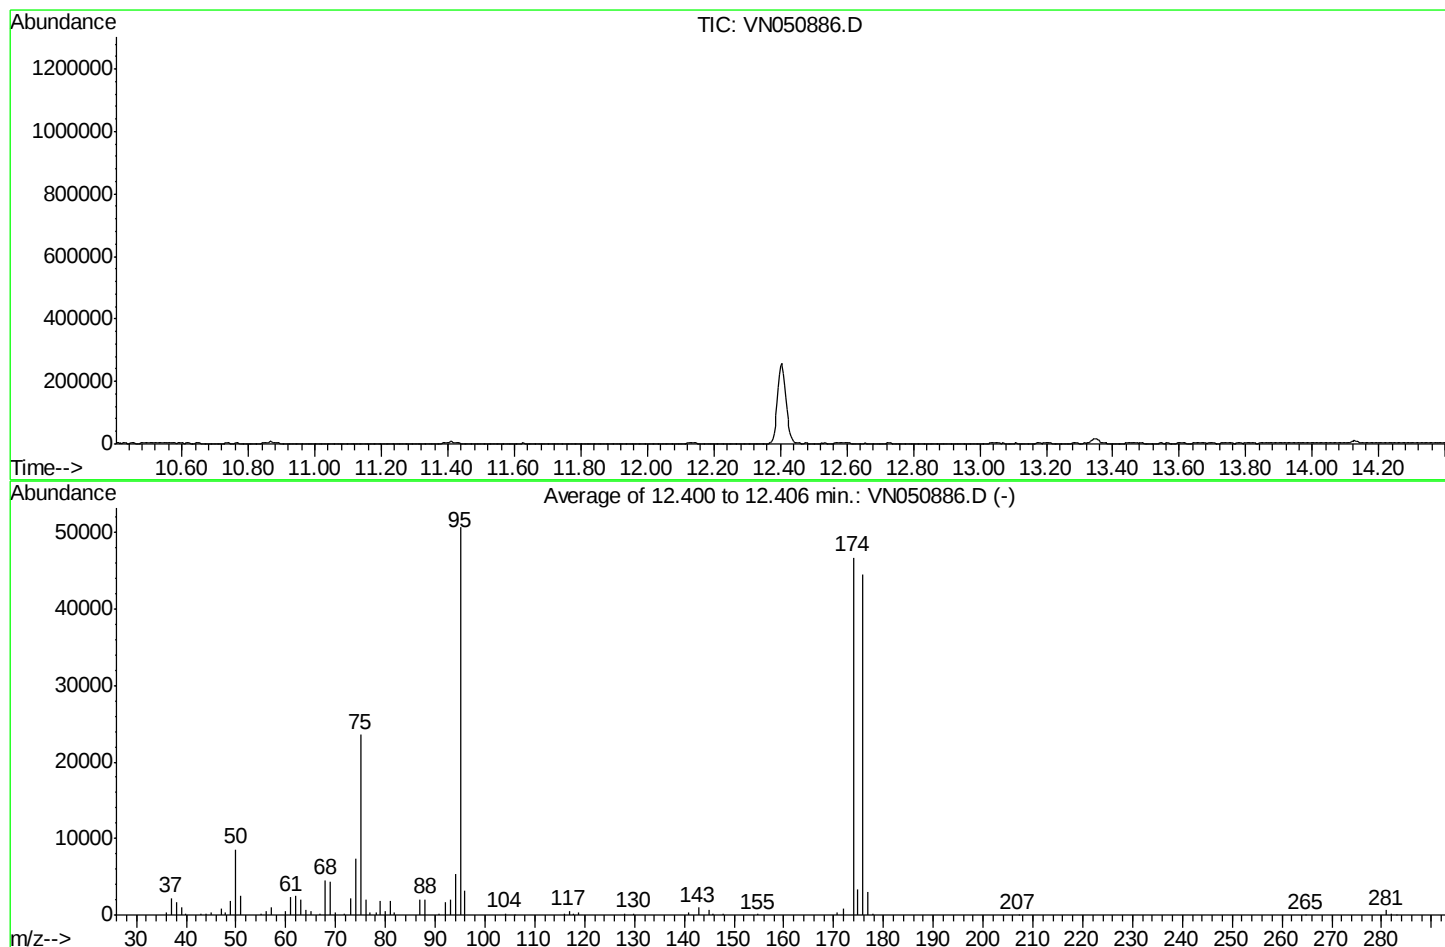

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	8571	PASS
75	95	30	60	46.4	23525	PASS
95	95	100	100	100.0	50674	PASS
96	95	5	9	6.1	3105	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.3	46768	PASS
175	174	5	9	7.0	3274	PASS
176	174	95	101	95.2	44522	PASS
177	176	5	9	6.7	2975	PASS