

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082724\
 Data File : VN083513.D
 Acq On : 27 Aug 2024 16:42
 Operator : JC\MD
 Sample : P3727-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 28 01:48:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:30:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	141774	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	285137	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	314284	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	156125	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	113532	56.260	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 112.520%	
35) Dibromofluoromethane	8.165	113	90821	51.030	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.060%	
50) Toluene-d8	10.565	98	324727	48.912	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 97.820%	
62) 4-Bromofluorobenzene	12.847	95	159159	61.493	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 122.980%#	
Target Compounds						
					Qvalue	
3) Chloromethane	2.354	50	664	0.403	ug/l #	43
6) Chloroethane	2.989	64	676	0.643	ug/l	92
11) Tert butyl alcohol	5.536	59	426	1.016	ug/l #	71
13) Acrolein	4.189	56	142	0.520	ug/l #	38
16) Acetone	4.436	43	20569	26.049	ug/l	100
17) Carbon Disulfide	4.695	76	2249	0.489	ug/l #	75
18) Methyl Acetate	5.030	43	8723	3.708	ug/l #	78
20) Methylene Chloride	5.265	84	7456	4.103	ug/l #	80
25) 2-Butanone	7.483	43	5768	4.757	ug/l	99
29) Tetrahydrofuran	7.836	42	242	0.309	ug/l #	38
31) Cyclohexane	8.224	56	3673	1.228	ug/l #	25
36) 1,1-Dichloropropene	8.218	75	12586	4.675	ug/l #	53
37) Ethyl Acetate	7.565	43	3651	1.211	ug/l #	80
38) Carbon Tetrachloride	8.218	117	16686	5.503	ug/l #	16
42) 1,2-Dichloroethane	8.688	62	959	0.328	ug/l #	78
43) Isopropyl Acetate	8.688	43	269368	51.635	ug/l #	76
45) 1,2-Dichloropropane	9.741	63	994	0.522	ug/l #	44
48) Methyl methacrylate	9.665	41	3548	1.424	ug/l #	53
51) 4-Methyl-2-Pentanone	10.447	43	6623	2.323	ug/l	97
54) cis-1,3-Dichloropropene	10.359	75	37044	11.081	ug/l #	56
56) Ethyl methacrylate	10.994	69	763	0.223	ug/l #	1
57) 1,3-Dichloropropane	11.200	76	3306	1.021	ug/l #	43
59) 2-Hexanone	11.171	43	90566	41.067	ug/l #	28
71) Bromoform	12.841	173	534	0.288	ug/l #	29
76) 1,2,3-Trichloropropane	12.847	75	86753	25.318	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.171	105	4398	0.402	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.847	75	86753	55.072	ug/l #	6
84) 1,2,4-Trimethylbenzene	13.476	105	4169	0.378	ug/l	95
90) Hexachloroethane	14.335	117	3149	1.494	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	14.682	75	329	0.367	ug/l #	7
95) Naphthalene	15.647	128	8019	0.765	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082724\
Data File : VN083513.D
Acq On : 27 Aug 2024 16:42
Operator : JC\MD
Sample : P3727-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Aug 28 01:48:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:30:41 2024
Response via : Initial Calibration

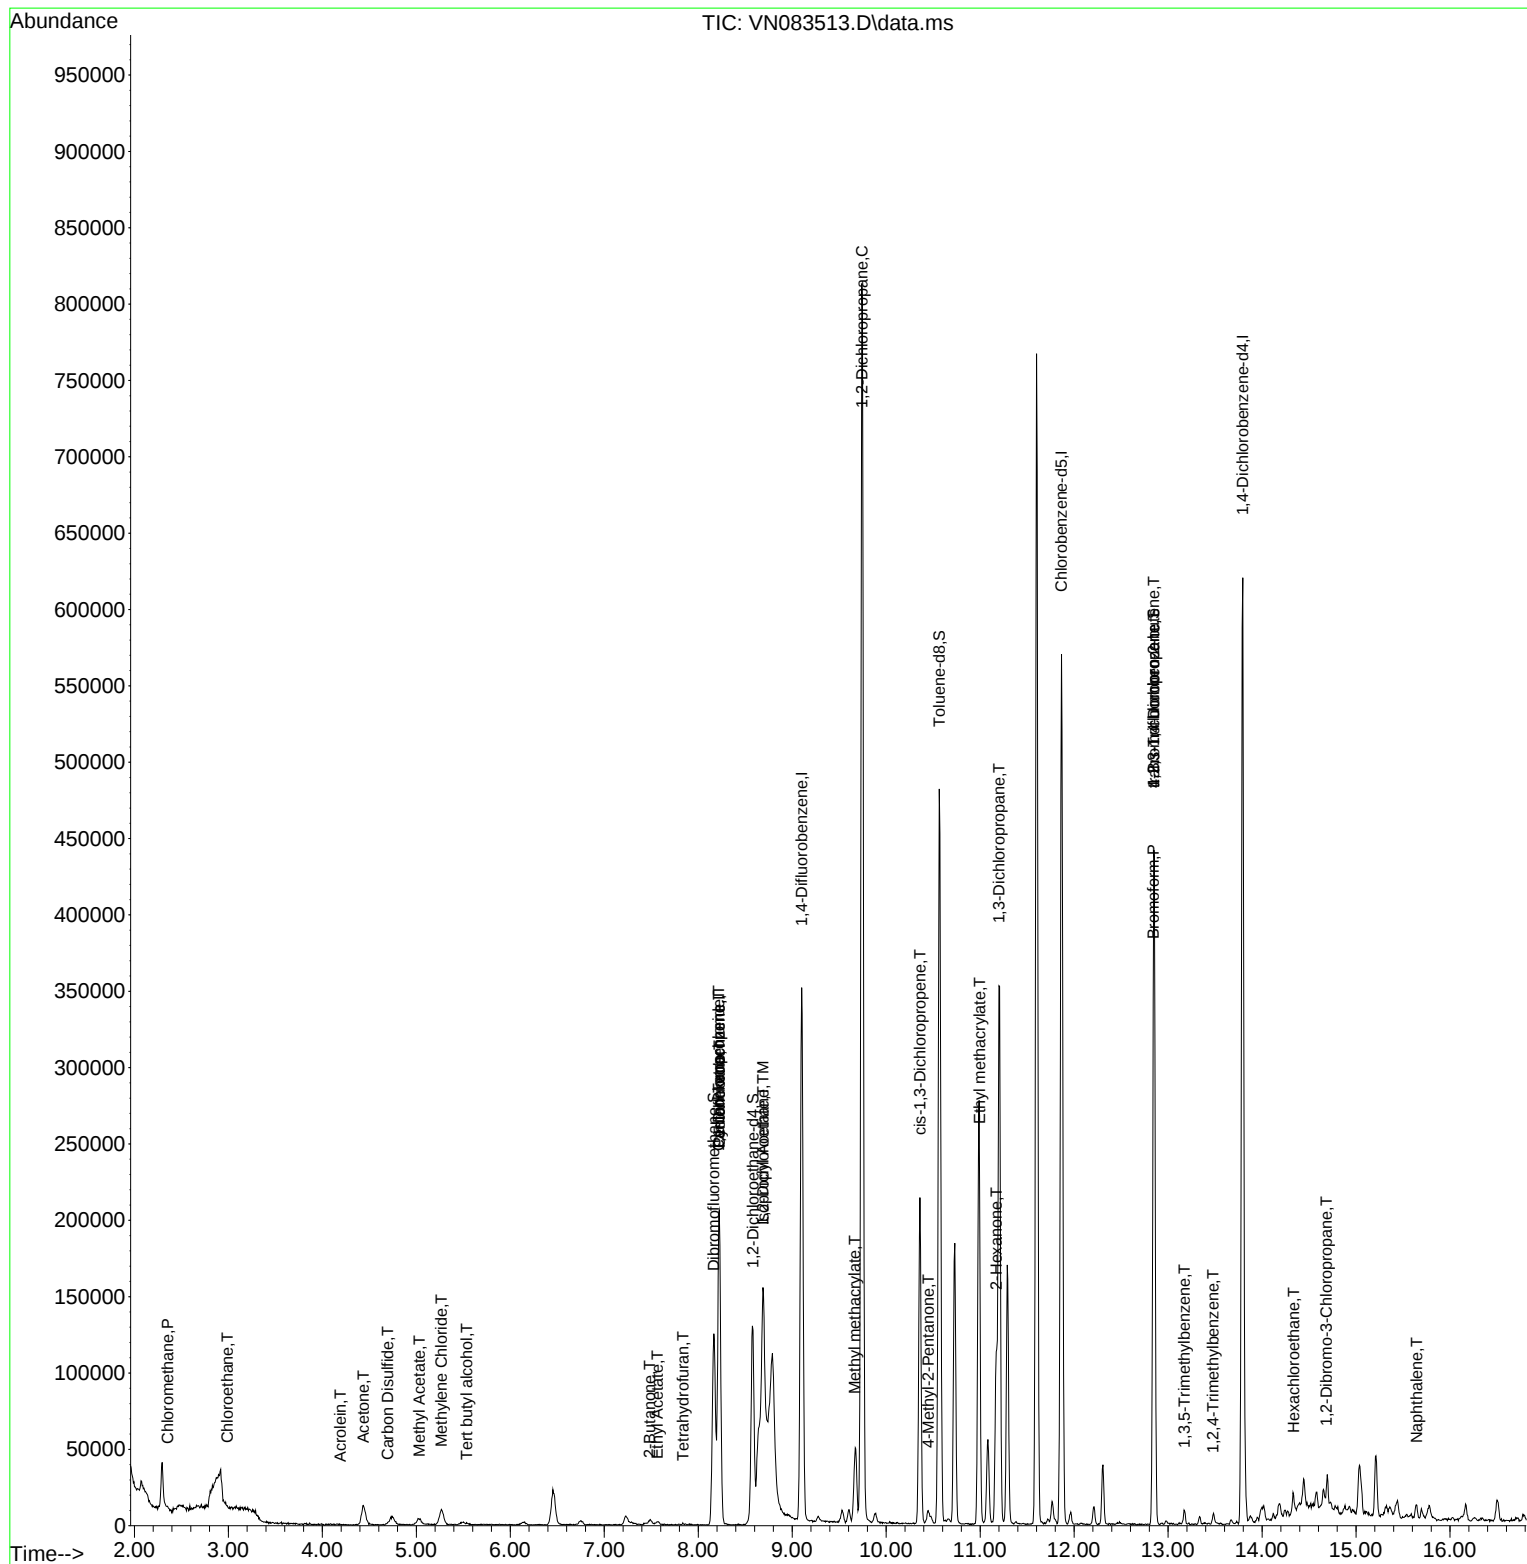






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Instrument :
MSVOA_N
ClientSampleId :



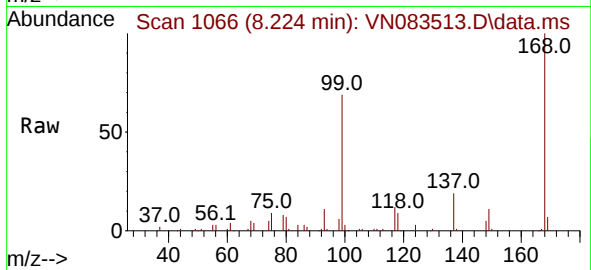



Tgt Ion:168 Resp: 141774
Ion Ratio Lower Upper
168 100
99 69.4 48.2 72.4



#3
Chloromethane
Concen: 0.403 ug/l
RT: 2.354 min Scan# 68
Delta R.T. -0.006 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Tgt Ion: 50 Resp: 664
Ion Ratio Lower Upper
50 100
52 0.0 25.0 37.4#


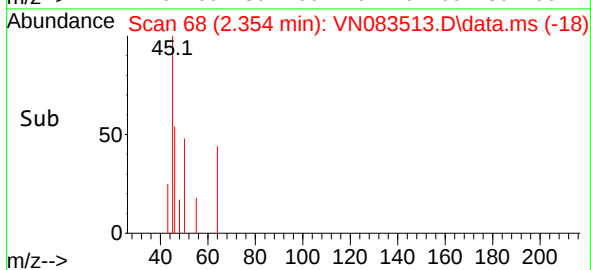






#6
Chloroethane
Concen: 0.643 ug/l
RT: 2.989 min Scan# 11
Delta R.T. -0.123 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 676
Ion Ratio Lower Upper
64 100
66 38.0 26.6 40.0



#11
Tert butyl alcohol
Concen: 1.016 ug/l
RT: 5.536 min Scan# 609
Delta R.T. 0.006 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Tgt Ion: 59 Resp: 426
Ion Ratio Lower Upper
59 100
57 0.0 8.9 13.3#









#13
Acrolein
Concen: 0.520 ug/l
RT: 4.189 min Scan# 379
Delta R.T. 0.006 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 142
Ion Ratio Lower Upper
56 100
55 121.8 56.4 84.6#

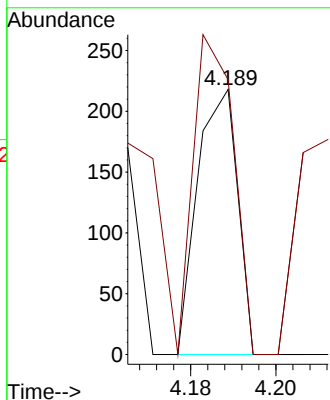

#16
Acetone
Concen: 26.049 ug/l
RT: 4.436 min Scan# 422
Delta R.T. 0.006 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42


Tgt Ion: 43 Resp: 20569
Ion Ratio Lower Upper
43 100
58 27.3 21.8 32.6

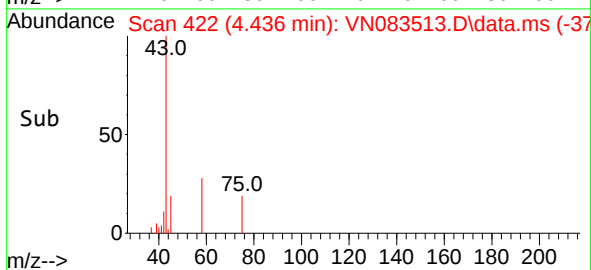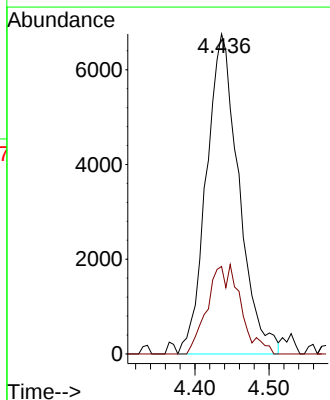






#17
Carbon Disulfide
Concen: 0.489 ug/l
RT: 4.695 min Scan# 466
Delta R.T. -0.018 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 76 Resp: 2249
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

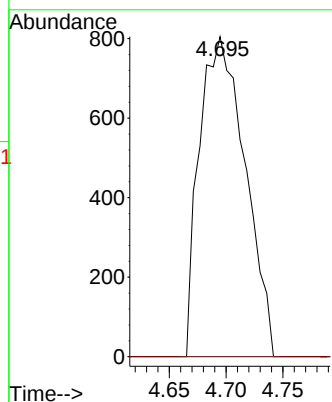

#18
Methyl Acetate
Concen: 3.708 ug/l
RT: 5.030 min Scan# 523
Delta R.T. 0.006 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42


Tgt Ion: 43 Resp: 8723
Ion Ratio Lower Upper
43 100
74 10.3 16.3 24.5#

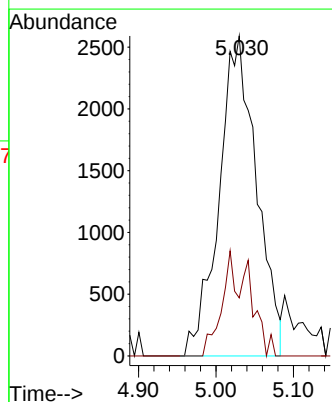






#20
Methylene Chloride
Concen: 4.103 ug/l
RT: 5.265 min Scan# 51
Delta R.T. -0.012 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 84 Resp: 7456
Ion Ratio Lower Upper
84 100
49 110.8 119.6 179.4#
51 39.2 34.8 52.2
86 62.8 52.9 79.3

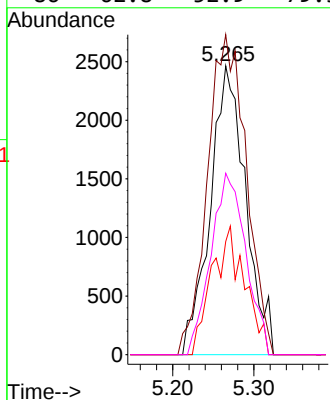


#25
2-Butanone
Concen: 4.757 ug/l
RT: 7.483 min Scan# 940
Delta R.T. 0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42



Tgt Ion: 43 Resp: 5768
Ion Ratio Lower Upper
43 100
72 22.4 18.2 27.2

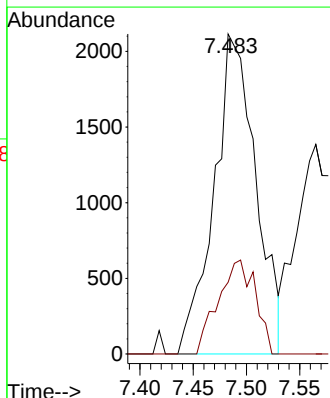



#29

Tetrahydrofuran

Concen: 0.309 ug/l

RT: 7.836 min Scan# 1066

Delta R.T. 0.000 min


Lab File: VN083513.D

Acq: 27 Aug 2024 16:42




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	42	Resp:	242
Ion	Ratio	Lower	Upper
42	100		
72	0.0	30.0	45.0#
71	0.0	28.3	42.5#

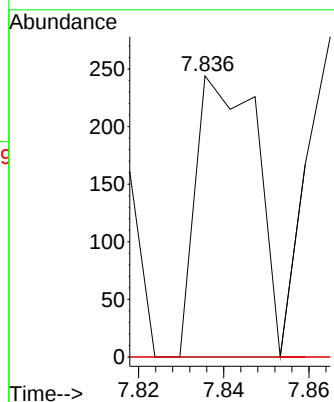

#31

Cyclohexane

Concen: 1.228 ug/l




RT: 8.224 min Scan# 1066


Delta R.T. -0.035 min

Lab File: VN083513.D

Acq: 27 Aug 2024 16:42

Tgt Ion:	56	Resp:	3673
Ion	Ratio	Lower	Upper
56	100		
69	151.6	24.5	36.7#
84	101.2	66.0	99.0#

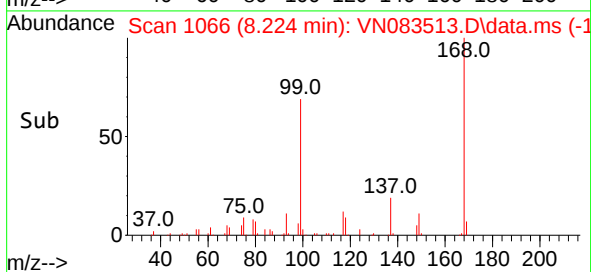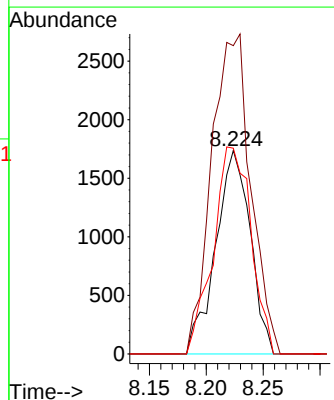



#33

1,2-Dichloroethane-d4

Concen: 56.260 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. 0.001 min

Lab File: VN083513.D

Acq: 27 Aug 2024 16:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 113532

Ion Ratio Lower Upper

65 100

67 49.8 0.0 104.4



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. 0.000 min

Lab File: VN083513.D

Acq: 27 Aug 2024 16:42




Tgt Ion: 114 Resp: 285137


Ion Ratio Lower Upper

114 100

63 23.0 0.0 44.6

88 17.6 0.0 31.4



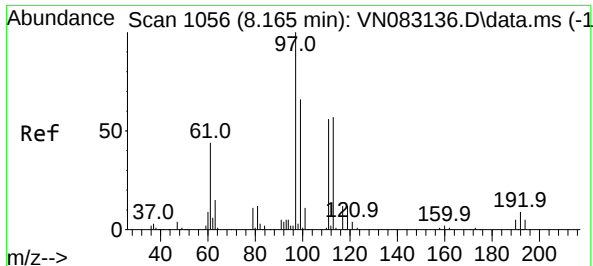

#35

Dibromofluoromethane

Concen: 51.030 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN083513.D





Acq: 27 Aug 2024 16:42

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:113	Resp:	90821
Ion	Ratio	Lower Upper
113	100	
111	102.2	82.4 123.6
192	16.8	14.9 22.3

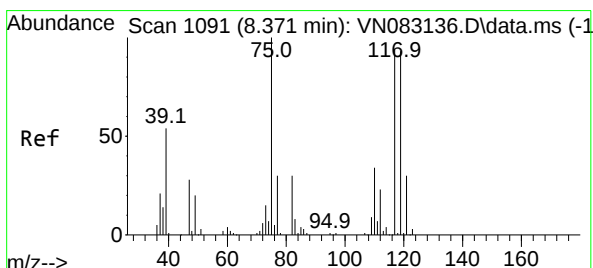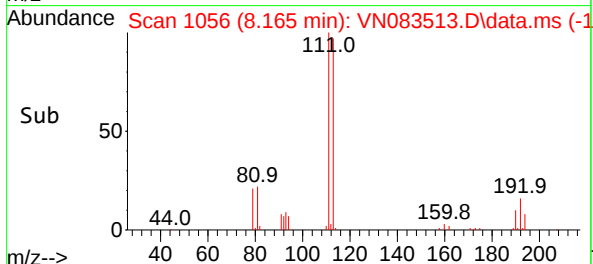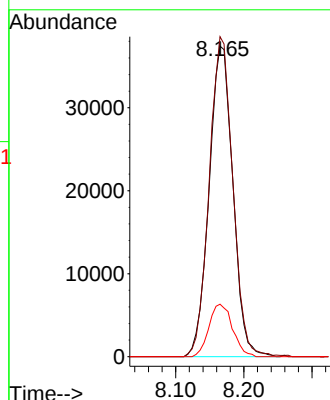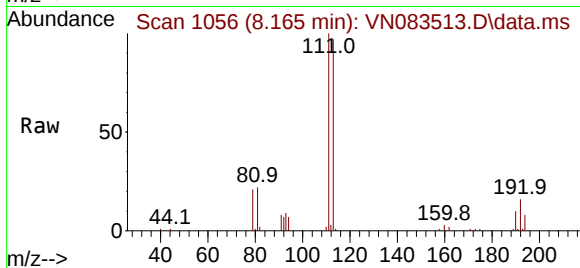

#36

1,1-Dichloropropene

Concen: 4.675 ug/l




RT: 8.218 min Scan# 1065


Delta R.T. -0.153 min

Lab File: VN083513.D

Acq: 27 Aug 2024 16:42


Tgt Ion: 75	Resp:	12586
Ion	Ratio	Lower Upper
75	100	
110	10.7	16.3 48.9#
77	0.0	24.6 37.0#

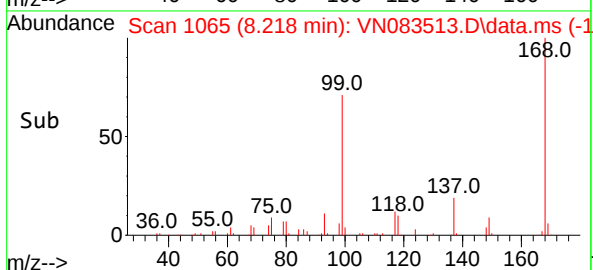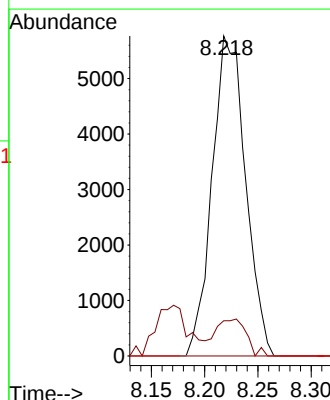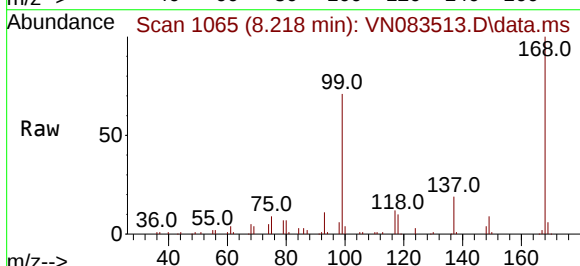






#37
Ethyl Acetate
Concen: 1.211 ug/l
RT: 7.565 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 3651
Ion Ratio Lower Upper
43 100
61 20.0 9.3 13.9#
70 2.5 7.0 10.6#

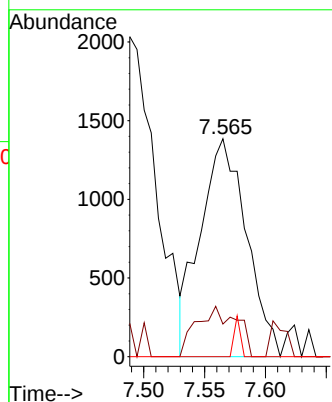

#38
Carbon Tetrachloride
Concen: 5.503 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.141 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Tgt Ion: 117 Resp: 16686
Ion Ratio Lower Upper
117 100
119 3.9 74.9 112.3#
121 0.0 24.3 36.5#



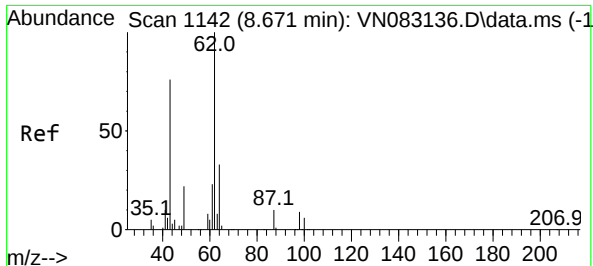

#42

1,2-Dichloroethane

Concen: 0.328 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.018 min


Lab File: VN083513.D

Acq: 27 Aug 2024 16:42

Instrument :

MSVOA_N

ClientSampleId :



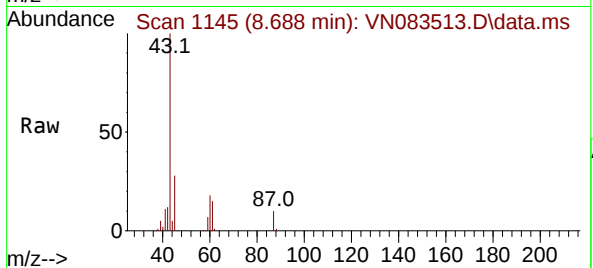


Tgt Ion: 62 Resp: 959

Ion Ratio Lower Upper

62 100

98 0.0 0.0 15.8

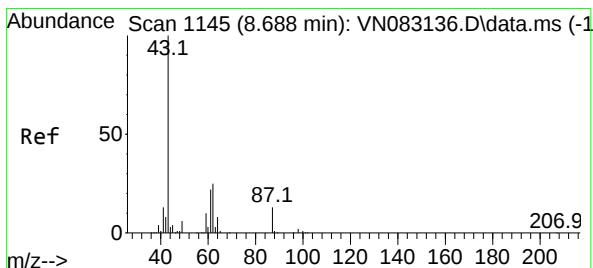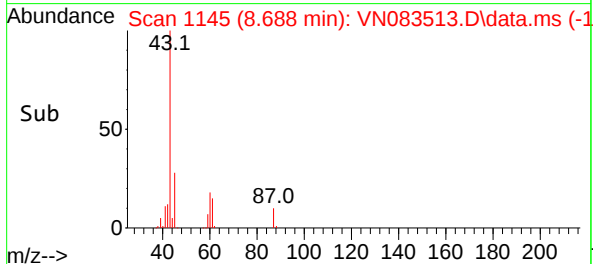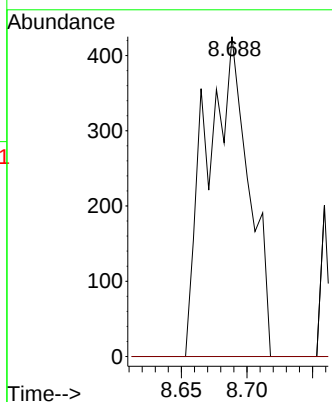

#43

Isopropyl Acetate

Concen: 51.635 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.000 min

Lab File: VN083513.D

Acq: 27 Aug 2024 16:42




Tgt Ion: 43 Resp: 269368


Ion Ratio Lower Upper

43 100

61 8.3 17.8 26.6#

87 5.4 8.2 12.2#

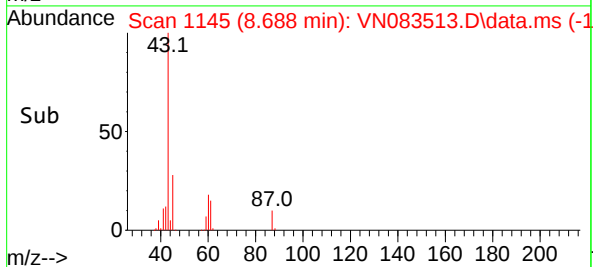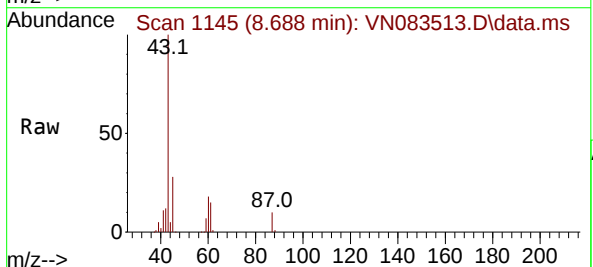

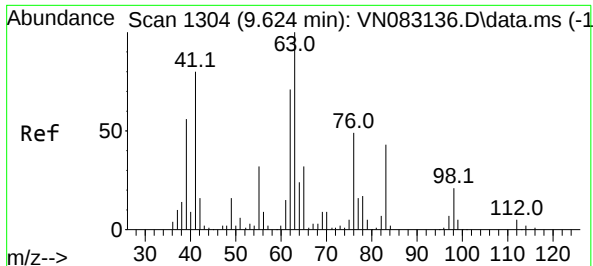

#45

1,2-Dichloropropane

Concen: 0.522 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.118 min

Lab File: VN083513.D

Acq: 27 Aug 2024 16:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 63 Resp: 994

Ion Ratio Lower Upper

63 100

65 0.0 24.4 36.6#

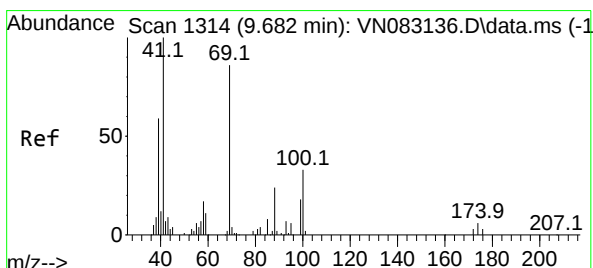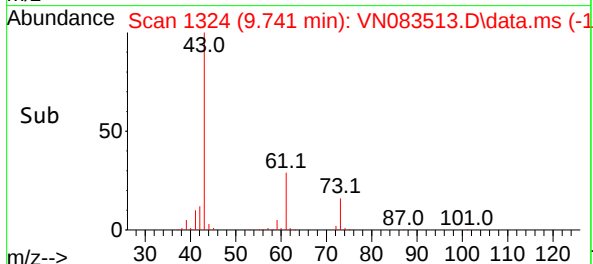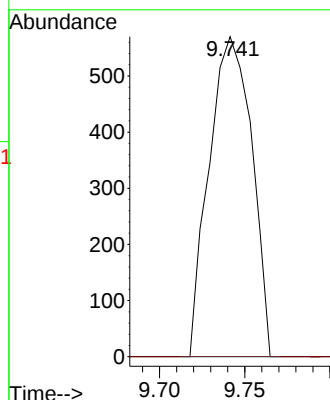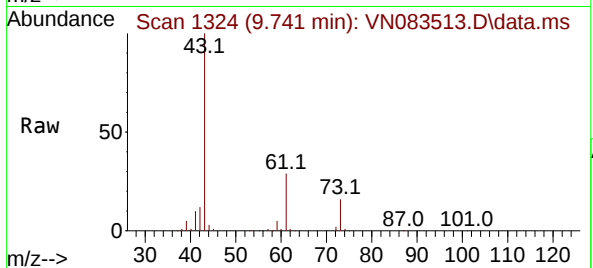

#48

Methyl methacrylate

Concen: 1.424 ug/l

RT: 9.665 min Scan# 1311

Delta R.T. -0.018 min

Lab File: VN083513.D

Acq: 27 Aug 2024 16:42




Tgt Ion: 41 Resp: 3548


Ion Ratio Lower Upper

41 100

69 0.0 56.3 84.5#

39 60.4 50.3 75.5


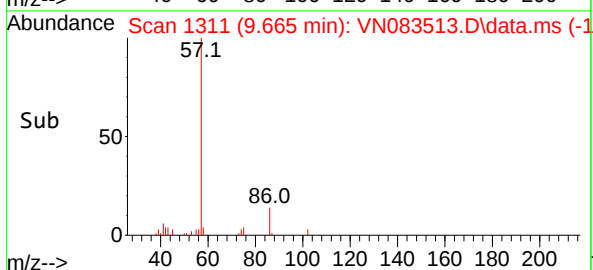
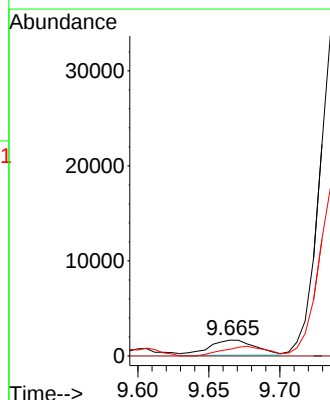
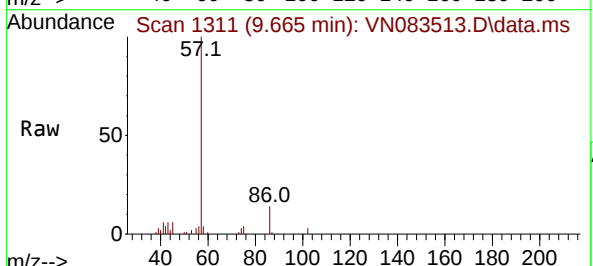




#50
Toluene-d8
Concen: 48.912 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 324727
Ion Ratio Lower Upper
98 100
100 65.6 51.5 77.3



#51
4-Methyl-2-Pentanone
Concen: 2.323 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Tgt Ion: 43 Resp: 6623
Ion Ratio Lower Upper
43 100
58 33.4 28.2 42.4


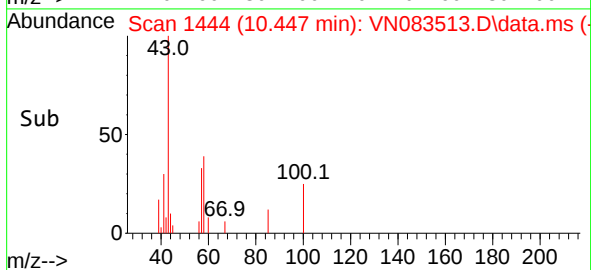




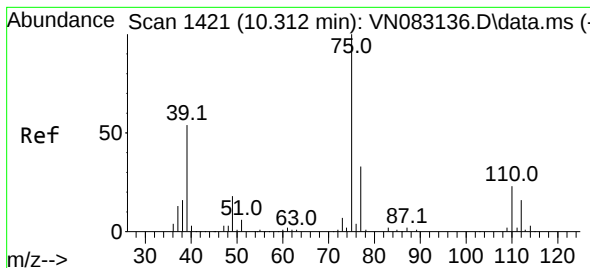

#54
 cis-1,3-Dichloropropene
 Concen: 11.081 ug/l
 RT: 10.359 min Scan# 1429
 Delta R.T. 0.047 min
 Lab File: VN083513.D
 Acq: 27 Aug 2024 16:42




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 37044
 Ion Ratio Lower Upper
 75 100
 77 1.0 24.3 36.5#
 39 32.5 50.5 75.7#

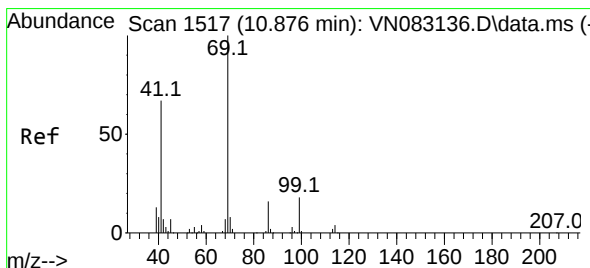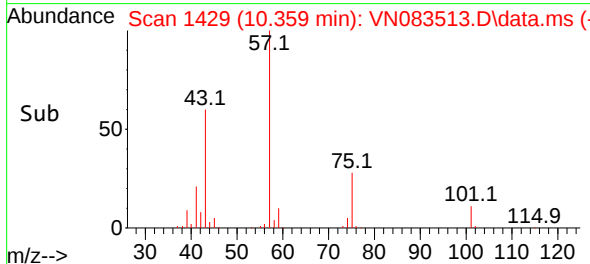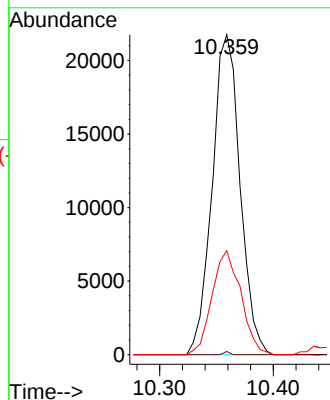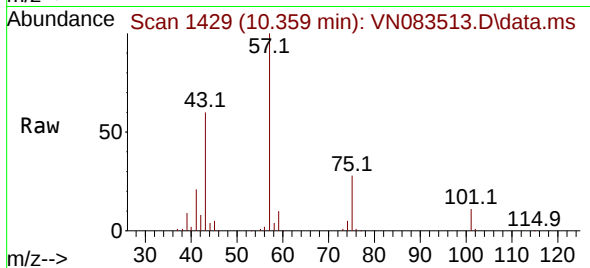

#56
 Ethyl methacrylate
 Concen: 0.223 ug/l
 RT: 10.994 min Scan# 1537
 Delta R.T. 0.118 min
 Lab File: VN083513.D
 Acq: 27 Aug 2024 16:42

Tgt Ion: 69 Resp: 763
 Ion Ratio Lower Upper
 69 100
 41 6987.4 63.4 95.2#
 39 2962.8 37.4 56.0#

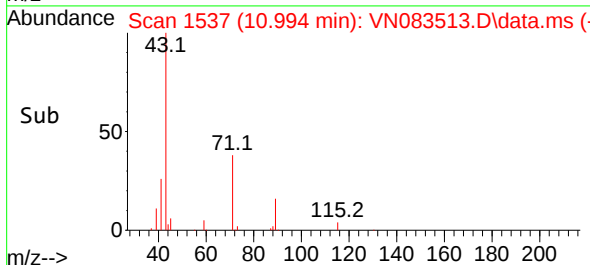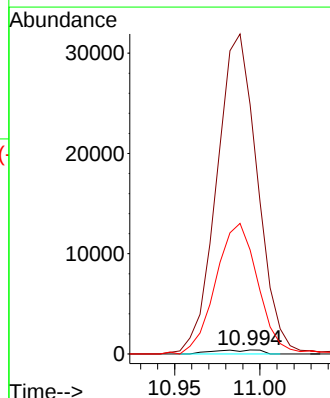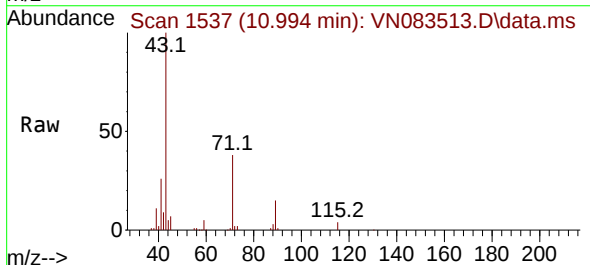

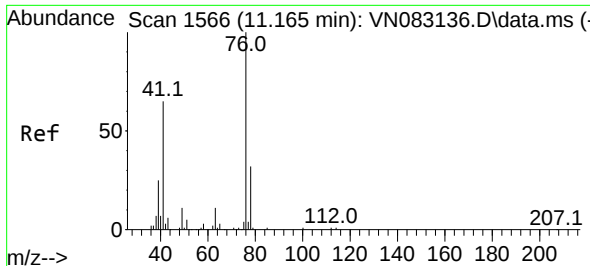

#57

1,3-Dichloropropane

Concen: 1.021 ug/l

RT: 11.200 min Scan# 1

Delta R.T. 0.035 min

Lab File: VN083513.D

Acq: 27 Aug 2024 16:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 76 Resp: 3306

Ion Ratio Lower Upper

76 100

78 0.0 25.6 38.4#

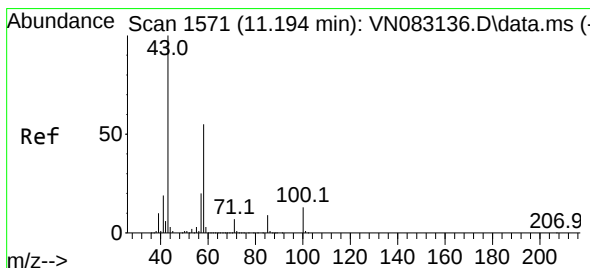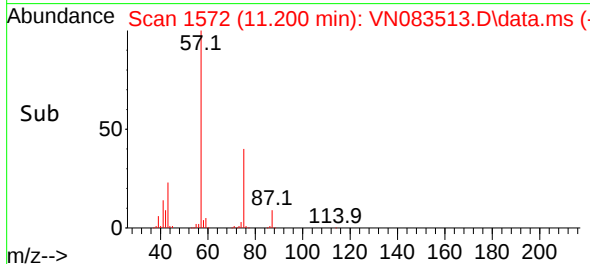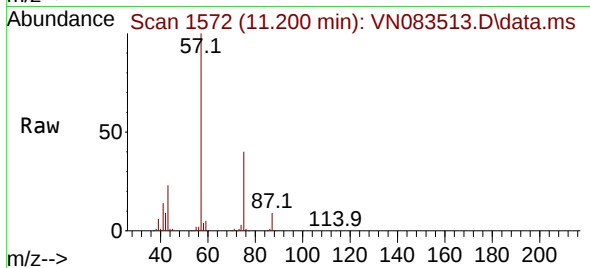

#59

2-Hexanone

Concen: 41.067 ug/l

RT: 11.171 min Scan# 1567

Delta R.T. -0.023 min

Lab File: VN083513.D




Acq: 27 Aug 2024 16:42


Tgt Ion: 43 Resp: 90566

Ion Ratio Lower Upper

43 100

58 0.0 24.6 73.8#


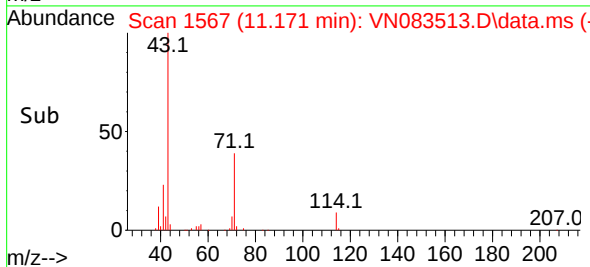

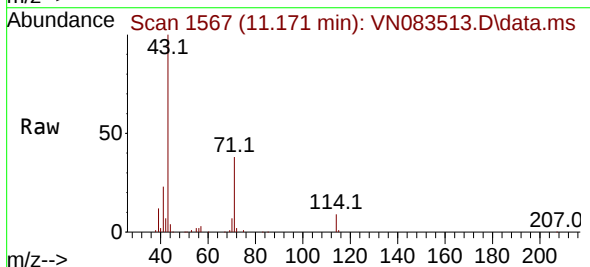




#62
4-Bromofluorobenzene
Concen: 61.493 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 159159
Ion Ratio Lower Upper
95 100
174 69.7 0.0 159.2
176 66.5 0.0 147.6



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42


Tgt Ion: 117 Resp: 314284
Ion Ratio Lower Upper
117 100
82 60.6 47.5 71.3
119 31.6 25.6 38.4

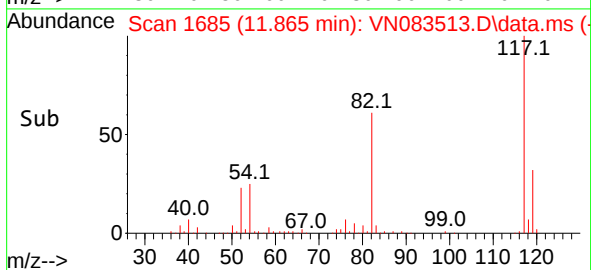






#71
Bromoform
Concen: 0.288 ug/l
RT: 12.841 min Scan# 1806
Delta R.T. 0.265 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:173 Resp: 534
Ion Ratio Lower Upper
173 100
175 0.0 24.0 72.0#
254 0.0 0.0 0.0

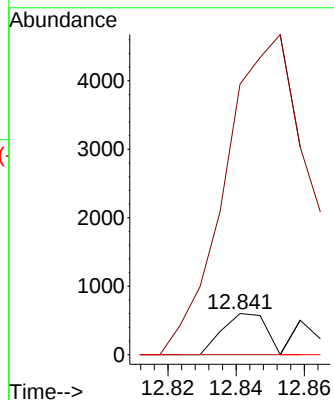

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Tgt Ion:152 Resp: 156125
Ion Ratio Lower Upper
152 100
115 65.1 30.6 91.6
150 159.7 0.0 348.6



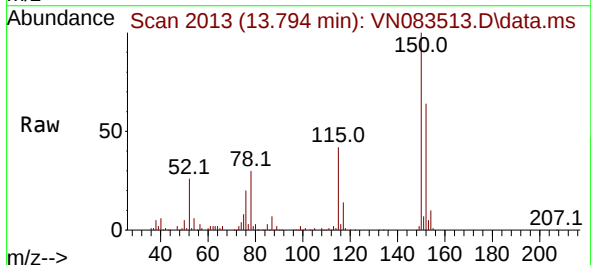
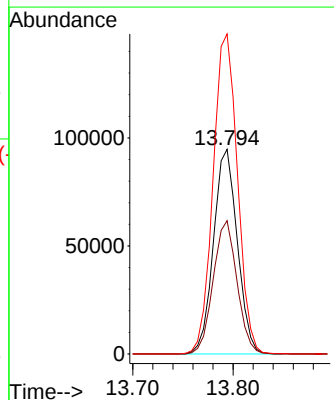


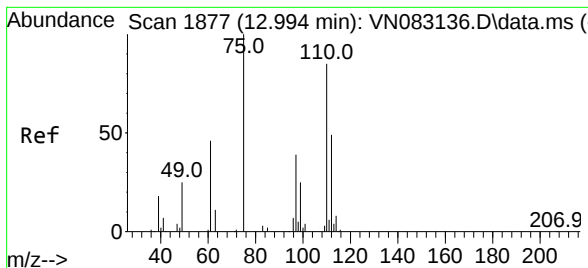

#76
1,2,3-Trichloropropane
Concen: 25.318 ug/l
RT: 12.847 min Scan# 1877
Delta R.T. -0.147 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 86753
Ion Ratio Lower Upper
75 100
77 1.3 110.9 332.6#

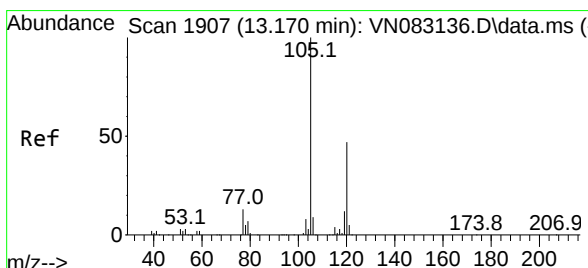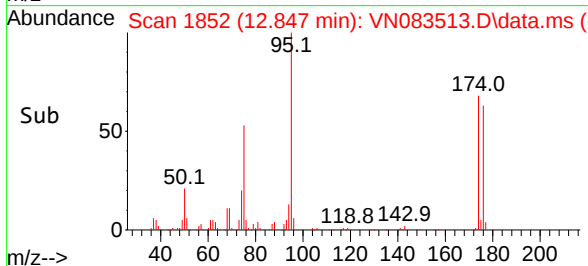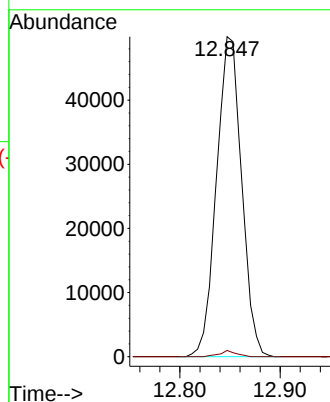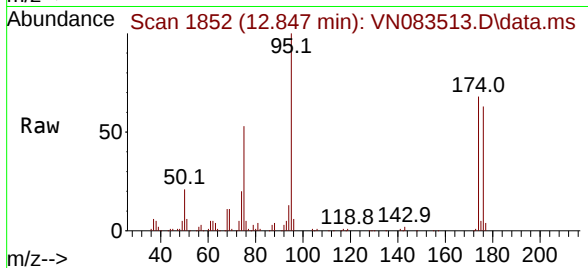

#80
1,3,5-Trimethylbenzene
Concen: 0.402 ug/l
RT: 13.171 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Tgt Ion: 105 Resp: 4398
Ion Ratio Lower Upper
105 100
120 47.5 24.3 72.8


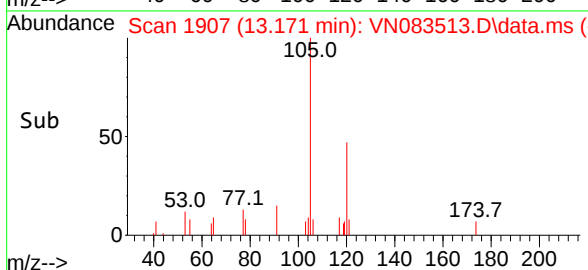
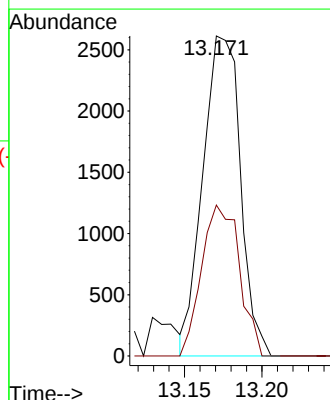
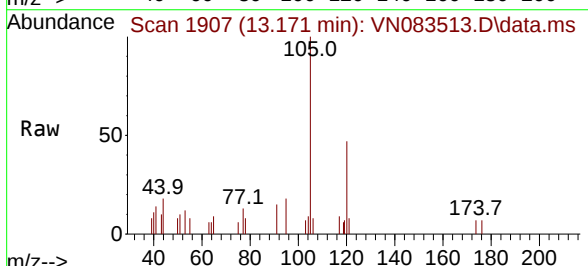


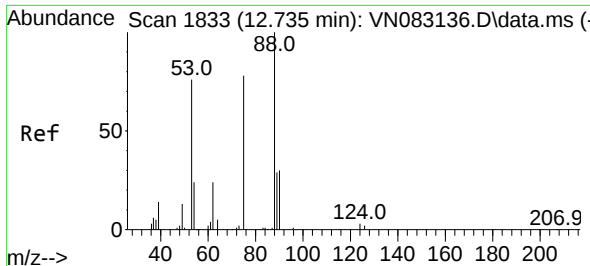

#81
trans-1,4-Dichloro-2-butene
Concen: 55.072 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 86753
Ion Ratio Lower Upper
75 100
53 0.0 88.4 132.6#
89 0.0 36.3 54.5#

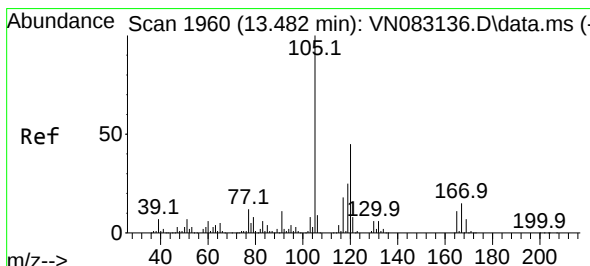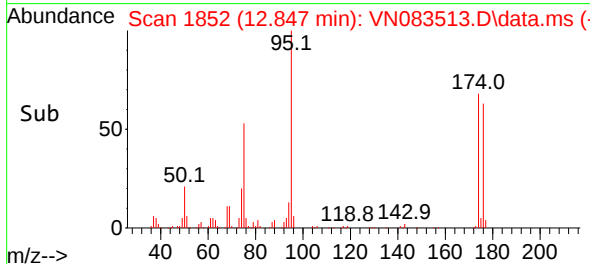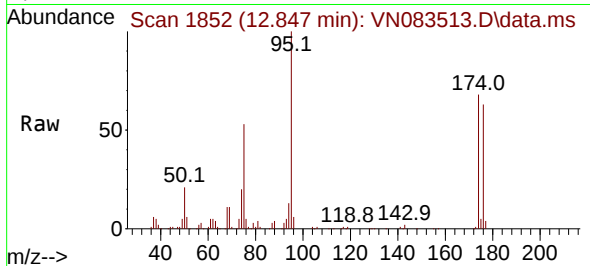

#84
1,2,4-Trimethylbenzene
Concen: 0.378 ug/l
RT: 13.476 min Scan# 1959
Delta R.T. -0.006 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42


Tgt Ion: 105 Resp: 4169
Ion Ratio Lower Upper
105 100
120 46.9 21.9 65.8

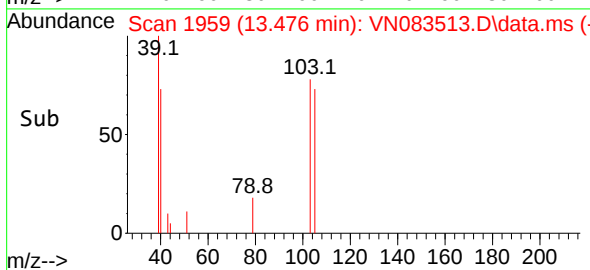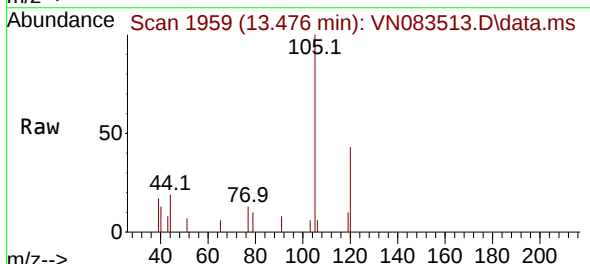



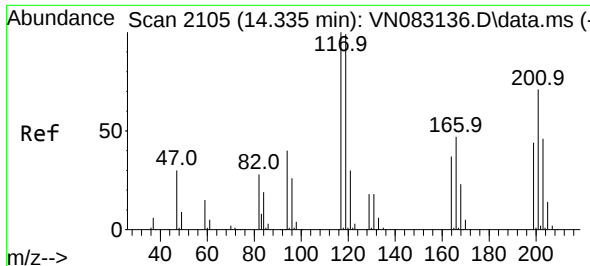


#90
Hexachloroethane
Concen: 1.494 ug/l
RT: 14.335 min Scan# 2105
Delta R.T. 0.000 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Instrument :
MSVOA_N
ClientSampleId :



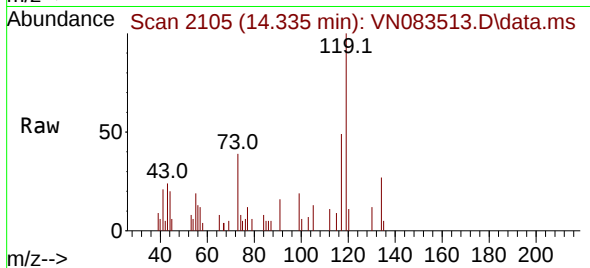



Tgt Ion:117 Resp: 3149
Ion Ratio Lower Upper
117 100
201 0.0 35.8 107.3#

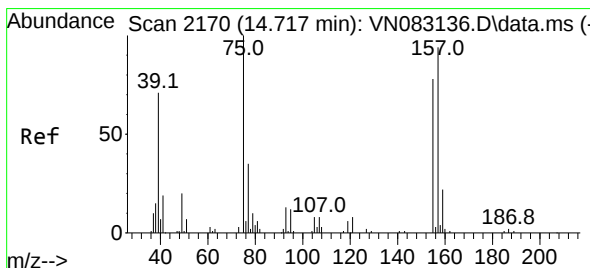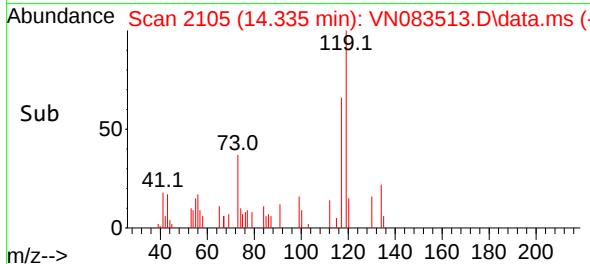

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.367 ug/l
RT: 14.682 min Scan# 2164
Delta R.T. -0.035 min
Lab File: VN083513.D
Acq: 27 Aug 2024 16:42

Tgt Ion: 75 Resp: 329
Ion Ratio Lower Upper
75 100
155 0.0 36.6 109.8#
157 0.0 46.9 140.6#

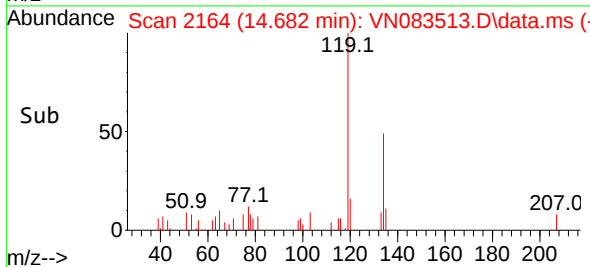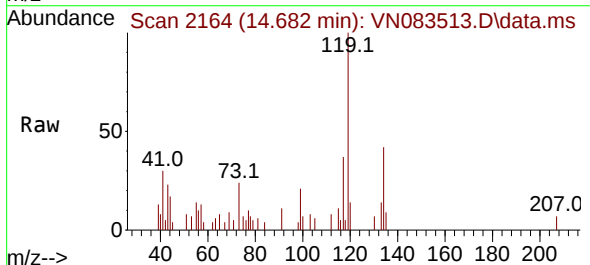



#95

Naphthalene

Concen: 0.765 ug/l

RT: 15.647 min Scan# 21

Delta R.T. 0.006 min


Lab File: VN083513.D

Acq: 27 Aug 2024 16:42

Instrument :

MSVOA_N

ClientSampleId :

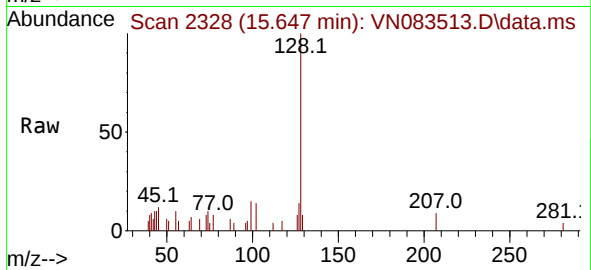

Tgt Ion:128 Resp: 8019

Ion Ratio Lower Upper

128 100

127 13.4 10.6 16.0

129 9.0 8.6 12.8

