
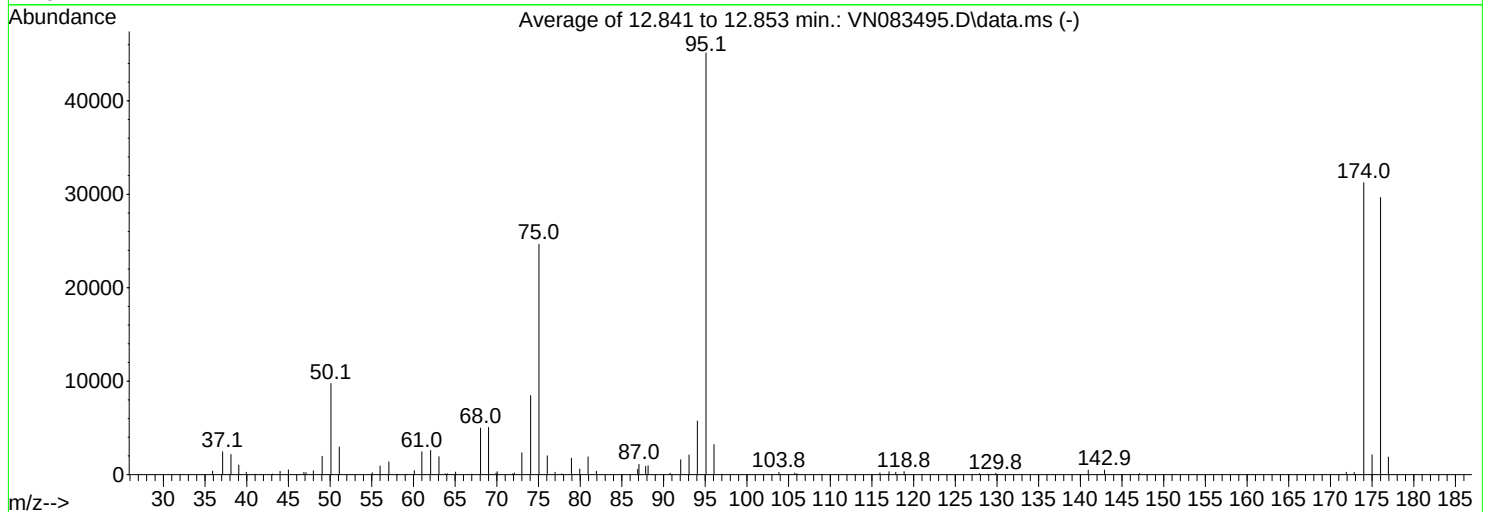


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082724\
Data File : VN083495.D
Acq On : 27 Aug 2024 08:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

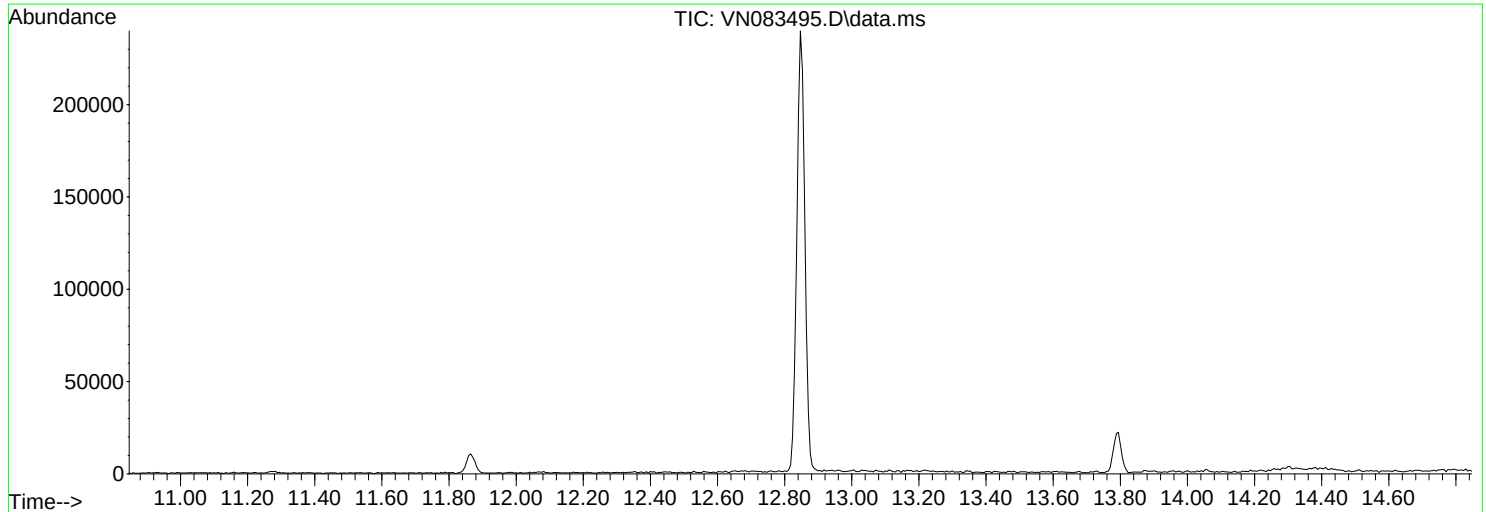

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.6	9748	PASS
75	95	30	60	54.6	24656	PASS
95	95	100	100	100.0	45131	PASS
96	95	5	9	7.1	3217	PASS
173	174	0.00	2	0.8	235	PASS
174	95	50	100	69.2	31243	PASS
175	174	5	9	6.8	2128	PASS
176	174	95	101	94.9	29656	PASS
177	176	5	9	6.3	1877	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	379	48.00	407	62.05	2590	72.10	1914
37.10	2449	49.05	1975	63.05	1914	73.00	2341
38.10	2160	50.10	9748	63.80	108	74.05	845
39.05	1021	51.10	2955	64.10	110	75.05	2465
39.95	265	55.05	201	65.05	271	76.05	2020
41.00	56	56.00	931	67.00	51	77.00	263
43.10	68	57.05	1367	68.05	4976	77.80	85
44.00	357	58.00	51	69.00	5051	78.95	1756
45.00	510	59.10	57	69.90	171	79.95	605
46.85	252	60.10	435	70.05	319	80.95	1898
47.10	225	61.00	2448	71.90	92	81.95	366

Average of 12.841 to 12.853 min.: VN083495.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.90	563	103.85	243	142.90	497		
87.05	1104	105.75	177	147.10	117		
87.85	890	106.00	100	171.90	251		
88.15	963	115.95	189	172.85	235		
90.80	152	117.05	329	174.00	31243		
92.05	1589	117.85	263	175.00	2128		
93.05	2110	118.85	333	176.00	29656		
94.05	5732	127.90	116	176.95	1877		
95.10	45131	128.90	54				
96.05	3217	129.85	136				
97.00	51	140.95	488				

Instrument :

MSVOA_N

ClientSampleId :

BFB