


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN082818\
 Data File : VN050906.D
 Acq On : 28 Aug 2018 11:31
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N082818W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Aug 29 01:38:44 2018

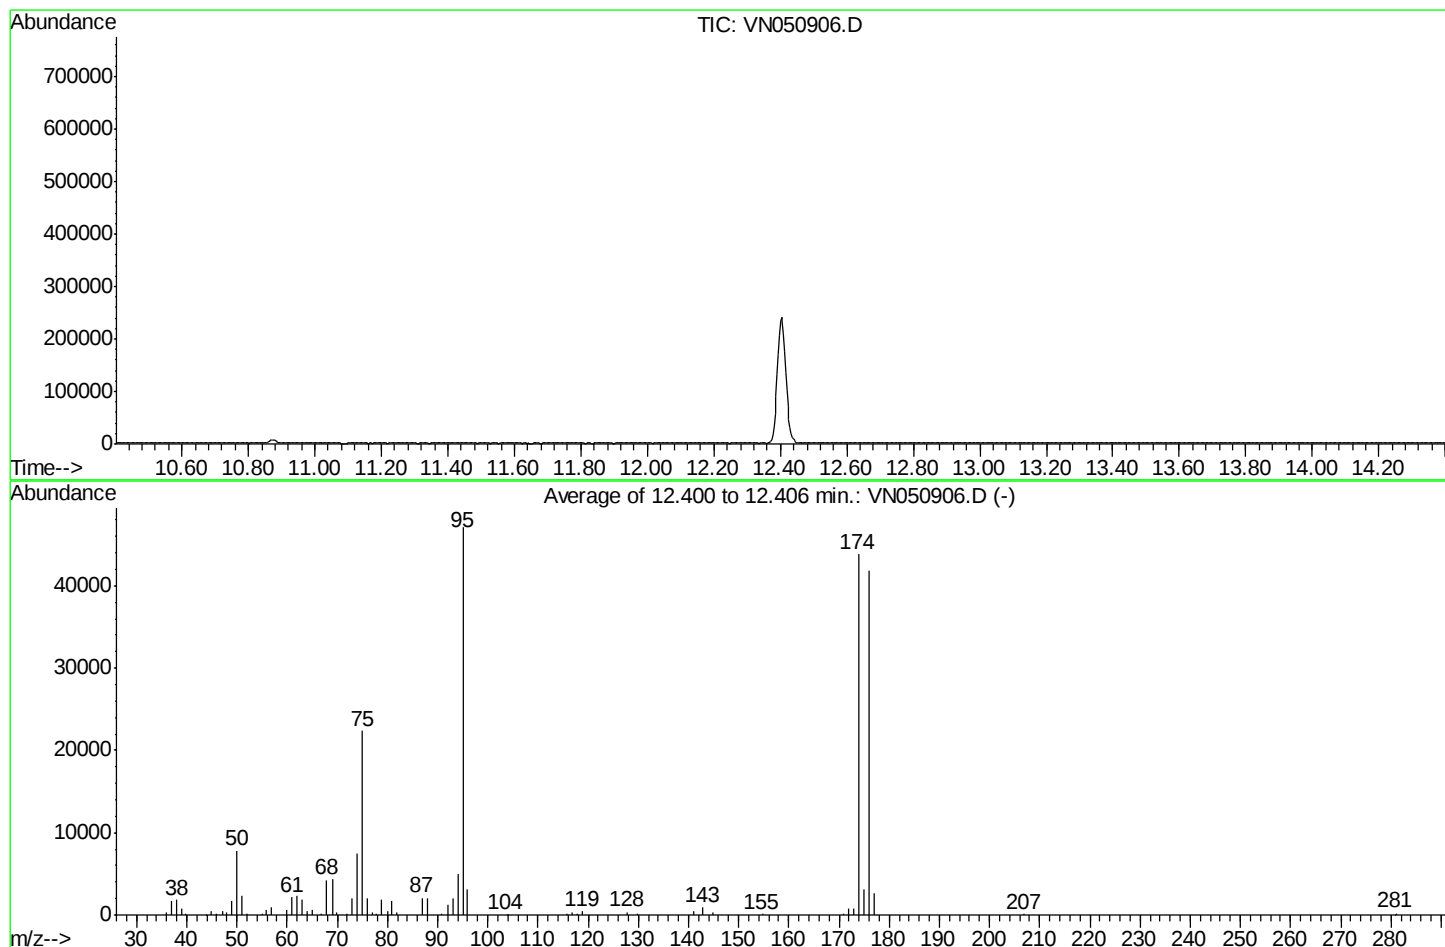

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	7851	PASS
75	95	30	60	47.5	22384	PASS
95	95	100	100	100.0	47093	PASS
96	95	5	9	6.6	3128	PASS
173	174	0.00	2	1.7	744	PASS
174	95	50	100	93.1	43826	PASS
175	174	5	9	7.2	3175	PASS
176	174	95	101	95.3	41765	PASS
177	176	5	9	6.3	2647	PASS