

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082823\
 Data File : VN079067.D
 Acq On : 28 Aug 2023 15:18
 Operator : JC\MD
 Sample : PB155094TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 29 04:05:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 16 02:42:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	212905	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	386093	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	375873	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	125277	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	158021	47.698	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	95.400%		
35) Dibromofluoromethane	8.171	113	132615	51.026	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	102.060%		
50) Toluene-d8	10.571	98	488820	50.654	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	101.300%		
62) 4-Bromofluorobenzene	12.853	95	153693	48.725	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.460%		
Target Compounds						Qvalue
6) Chloroethane	3.124	64	542	0.214	ug/l #	43
13) Acrolein	4.212	56	76	7.055	ug/l #	16
16) Acetone	4.442	43	26311	19.247	ug/l	88
18) Methyl Acetate	5.030	43	4180	0.724	ug/l #	55
20) Methylene Chloride	5.271	84	8381	2.877	ug/l #	85
25) 2-Butanone	7.494	43	10651	4.860	ug/l #	70
29) Tetrahydrofuran	7.853	42	433	0.298	ug/l #	39
31) Cyclohexane	8.236	56	5410	Below Cal	#	12
36) 1,1-Dichloropropene	8.230	75	18006	4.606	ug/l #	50
37) Ethyl Acetate	7.577	43	4237	0.969	ug/l #	73
38) Carbon Tetrachloride	8.230	117	22224	5.673	ug/l #	16
43) Isopropyl Acetate	8.694	43	156735	20.273	ug/l #	78
45) 1,2-Dichloropropane	9.753	63	1618	0.526	ug/l #	45
48) Methyl methacrylate	9.671	41	4341	1.239	ug/l #	34
49) 1,4-Dioxane	9.741	88	83	1.391	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	38084	8.305	ug/l #	77
54) cis-1,3-Dichloropropene	10.359	75	51966	10.678	ug/l #	73
57) 1,3-Dichloropropane	11.206	76	6881	1.352	ug/l #	42
59) 2-Hexanone	11.177	43	146764	44.189	ug/l #	19
71) Bromoform	12.847	173	1552	0.706	ug/l #	1
74) N-amyl acetate	12.494	43	2473	0.469	ug/l #	45
76) 1,2,3-Trichloropropane	12.853	75	85390	28.288	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	85390	72.264	ug/l #	15
82) 4-Chlorotoluene	13.235	91	1557	0.212	ug/l #	37
87) 1,3-Dichlorobenzene	13.741	146	1049	0.243	ug/l #	82
88) 1,4-Dichlorobenzene	13.818	146	1459	0.337	ug/l #	45
89) n-Butylbenzene	14.065	91	1507	0.239	ug/l	89
92) 1,2-Dibromo-3-Chloropr...	14.712	75	333	Below Cal	#	4
93) 1,2,4-Trichlorobenzene	15.394	180	1382	0.907	ug/l #	73
94) Hexachlorobutadiene	15.506	225	574	0.445	ug/l #	38
95) Naphthalene	15.647	128	4293	3.280	ug/l #	92
96) 1,2,3-Trichlorobenzene	15.847	180	1332	0.798	ug/l #	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082823\
Data File : VN079067.D
Acq On : 28 Aug 2023 15:18
Operator : JC\MD
Sample : PB155094TB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Aug 29 04:05:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 16 02:42:02 2023
Response via : Initial Calibration

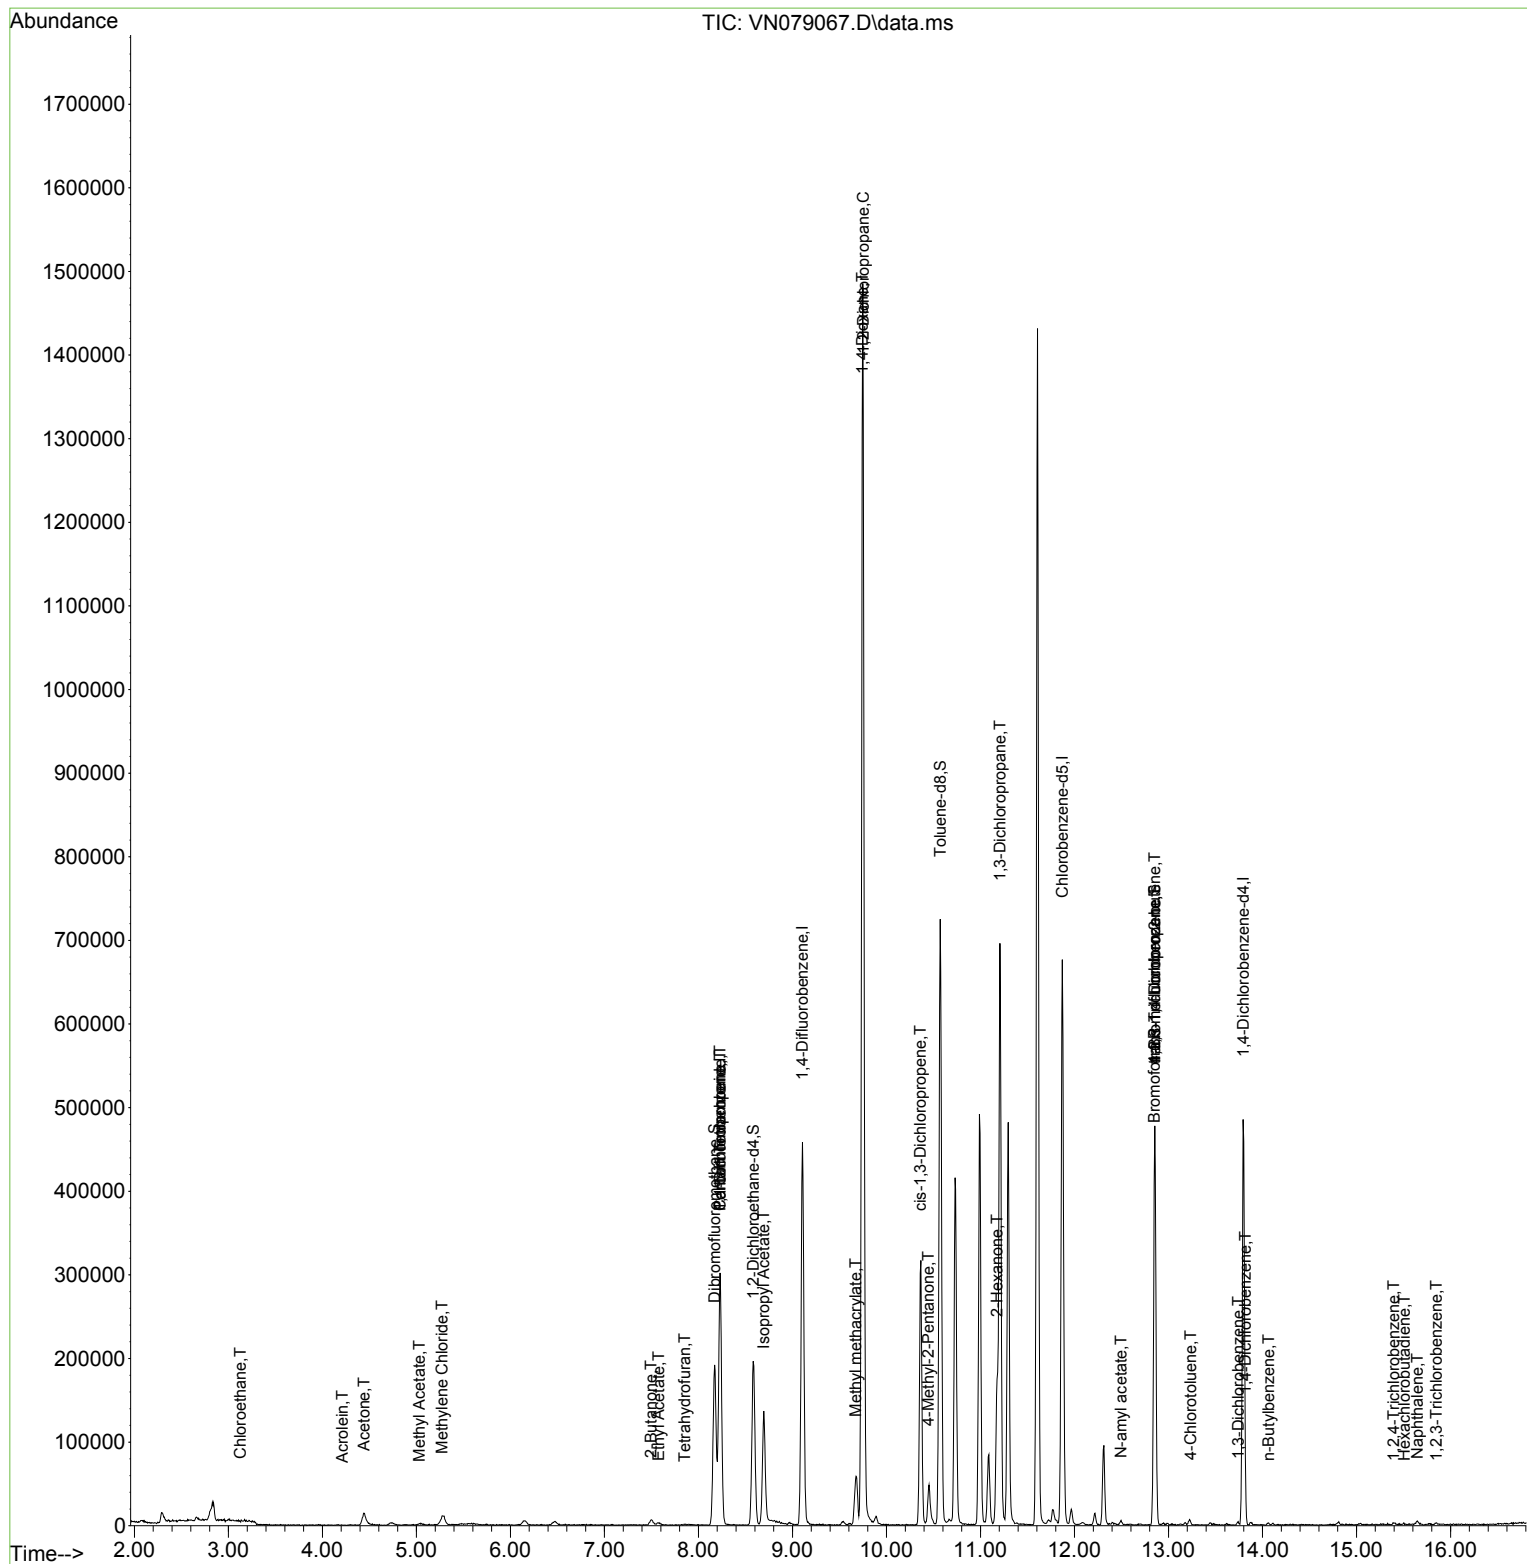






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.000 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 212905
Ion Ratio Lower Upper
168 100
99 56.8 53.0 79.6



#6
Chloroethane
Concen: 0.214 ug/l
RT: 3.124 min Scan# 199
Delta R.T. 0.006 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18


Tgt Ion: 64 Resp: 542
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

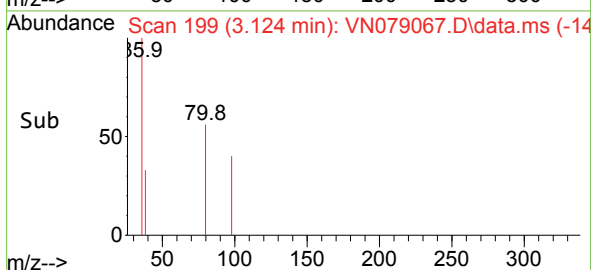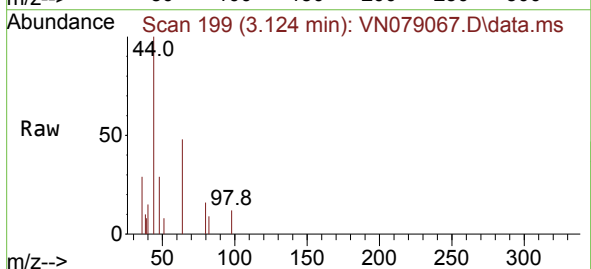






#13
Acrolein
Concen: 7.055 ug/l
RT: 4.212 min Scan# 384
Delta R.T. 0.017 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 76
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#

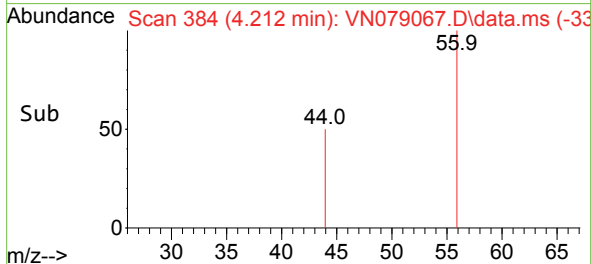

#16
Acetone
Concen: 19.247 ug/l
RT: 4.442 min Scan# 423
Delta R.T. -0.000 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Tgt Ion: 43 Resp: 26311
Ion Ratio Lower Upper
43 100
58 28.1 28.0 42.0

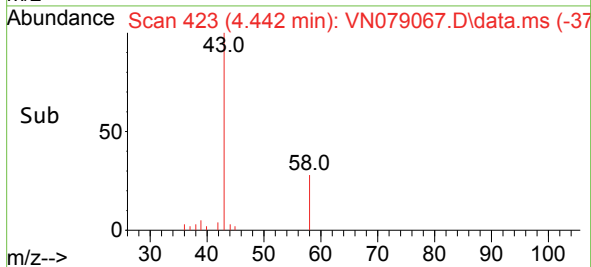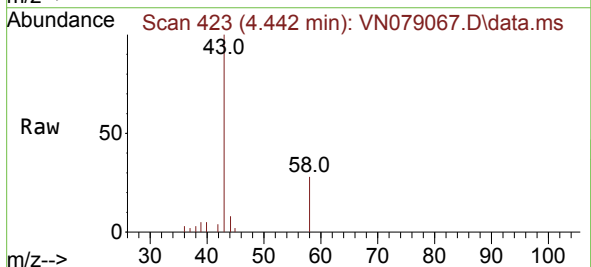



#18

Methyl Acetate

Concen: 0.724 ug/l

RT: 5.030 min Scan# 51

Delta R.T. -0.012 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 4180

Ion Ratio Lower Upper

43 100

74 7.6 26.2 39.4#

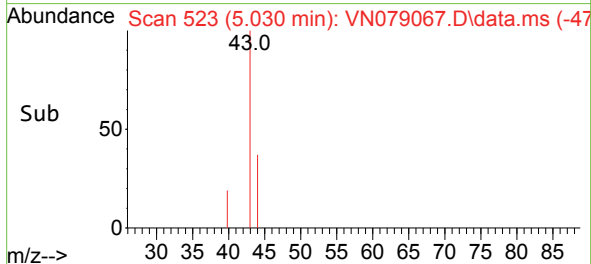

#20

Methylene Chloride

Concen: 2.877 ug/l

RT: 5.271 min Scan# 564

Delta R.T. -0.012 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Tgt Ion: 84 Resp: 8381




Ion Ratio Lower Upper


84 100

49 120.6 79.7 119.5#

51 27.6 25.2 37.8

86 59.4 53.3 79.9

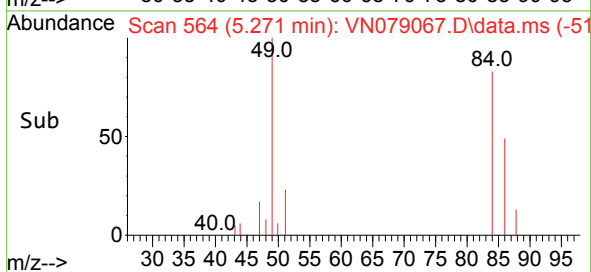

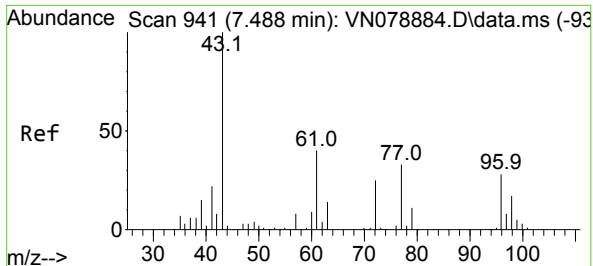

#25

2-Butanone

Concen: 4.860 ug/l

RT: 7.494 min Scan# 941

Delta R.T. 0.000 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 10651

Ion Ratio Lower Upper

43 100

72 19.4 30.2 45.2#

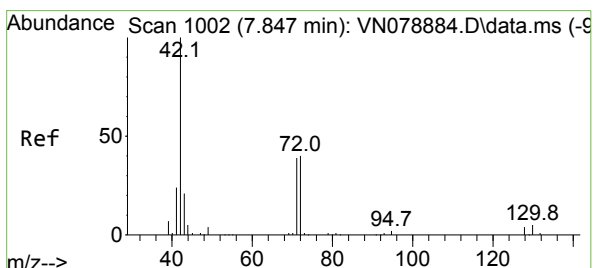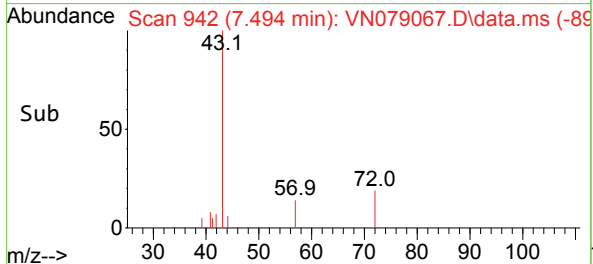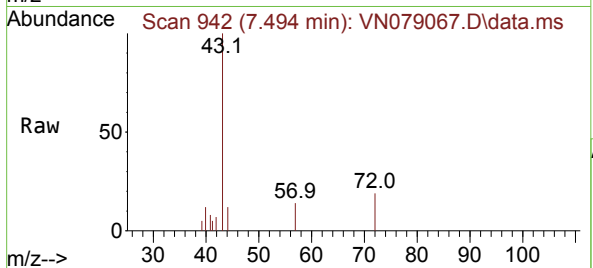

#29

Tetrahydrofuran

Concen: 0.298 ug/l

RT: 7.853 min Scan# 1003

Delta R.T. 0.006 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18




Tgt Ion: 42 Resp: 433


Ion Ratio Lower Upper

42 100

72 15.5 49.8 74.6#

71 13.9 47.4 71.2#

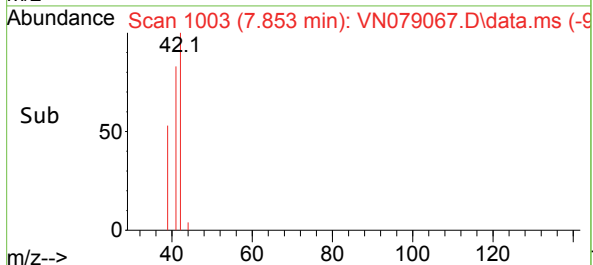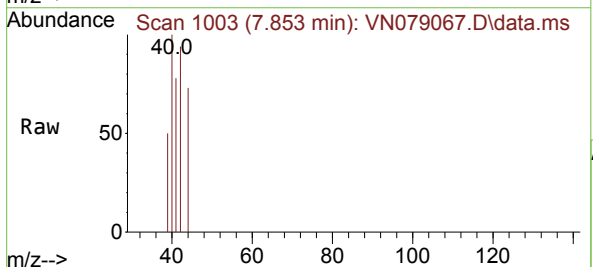

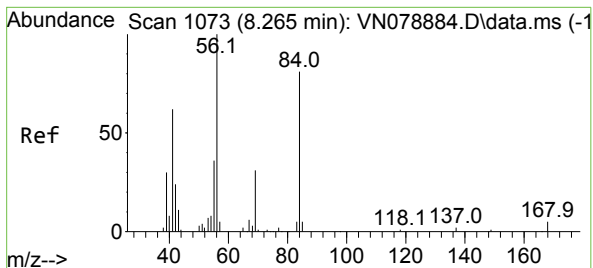

#31

Cyclohexane

Concen: Below Cal

RT: 8.236 min Scan# 1068

Delta R.T. -0.029 min


Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N

ClientSampleId :

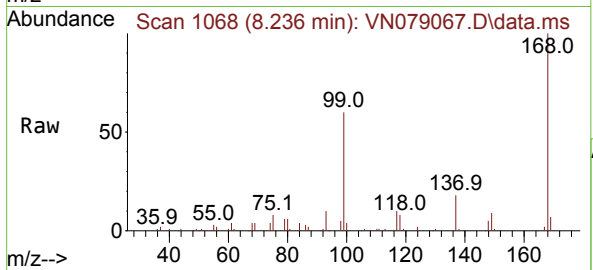




Tgt Ion: 56 Resp: 5410

Ion Ratio Lower Upper

56 100

69 144.0 26.8 40.2#

84 156.6 81.8 122.6#

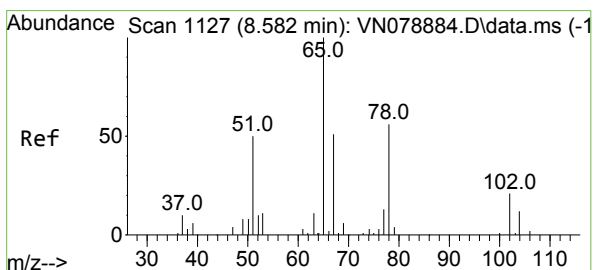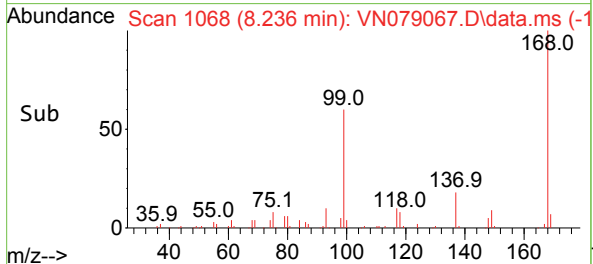

#33

1,2-Dichloroethane-d4

Concen: 47.698 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VN079067.D




Acq: 28 Aug 2023 15:18


Tgt Ion: 65 Resp: 158021

Ion Ratio Lower Upper

65 100

67 52.5 0.0 106.6

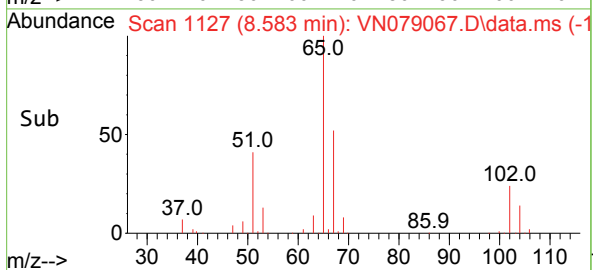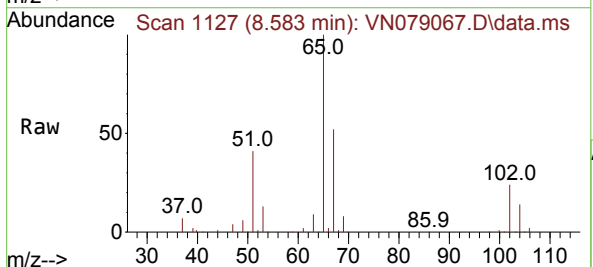



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 386093

Ion Ratio Lower Upper

114 100

63 20.7 0.0 36.4

88 15.8 0.0 30.6

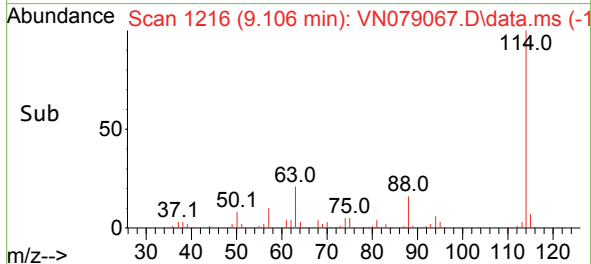

#35

Dibromofluoromethane

Concen: 51.026 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18




Tgt Ion:113 Resp: 132615


Ion Ratio Lower Upper

113 100

111 104.9 82.6 123.8

192 18.5 12.7 19.1

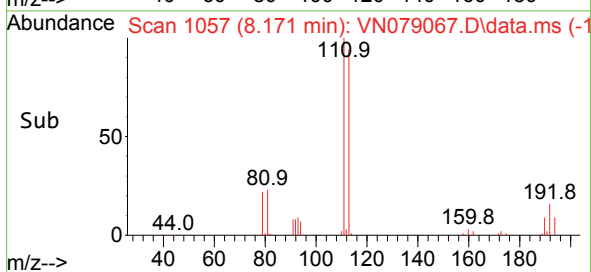



#36

1,1-Dichloropropene

Concen: 4.606 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.147 min


Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 75 Resp: 18006

Ion Ratio Lower Upper

75 100

110 10.9 19.1 57.3#

77 0.0 25.0 37.4#

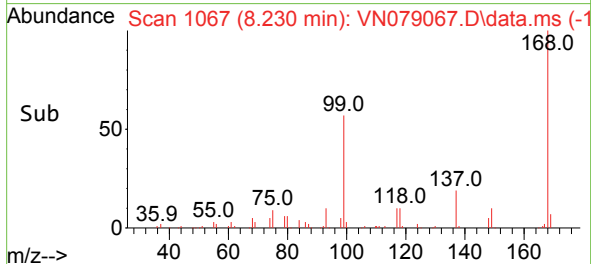

#37

Ethyl Acetate

Concen: 0.969 ug/l

RT: 7.577 min Scan# 956

Delta R.T. 0.006 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18




Tgt Ion: 43 Resp: 4237


Ion Ratio Lower Upper

43 100

61 0.0 13.2 19.8#

70 8.3 11.3 16.9#

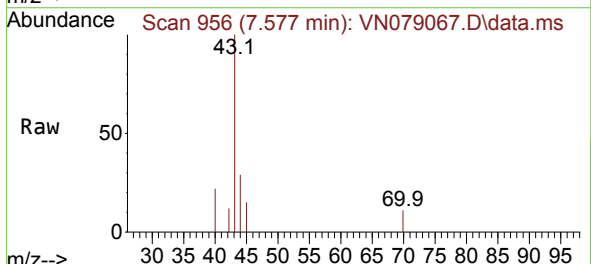



#38

Carbon Tetrachloride

Concen: 5.673 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.141 min


Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N

ClientSampleId :

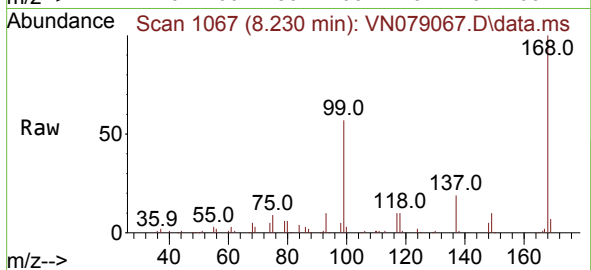




Tgt Ion:117 Resp: 22224

Ion Ratio Lower Upper

117 100

119 5.5 77.3 115.9#

121 0.0 23.3 34.9#

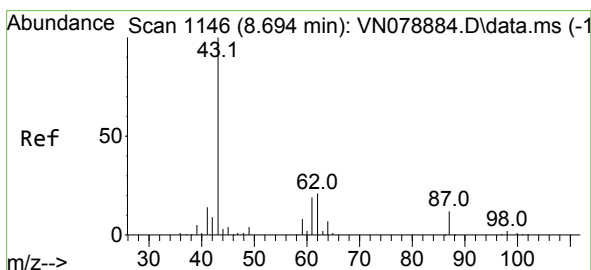

#43

Isopropyl Acetate

Concen: 20.273 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.000 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18




Tgt Ion: 43 Resp: 156735


Ion Ratio Lower Upper

43 100

61 16.5 24.7 37.1#

87 11.6 14.6 21.8#


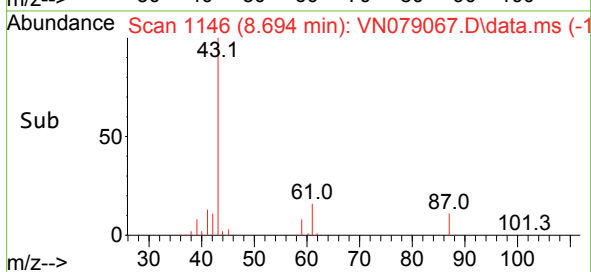
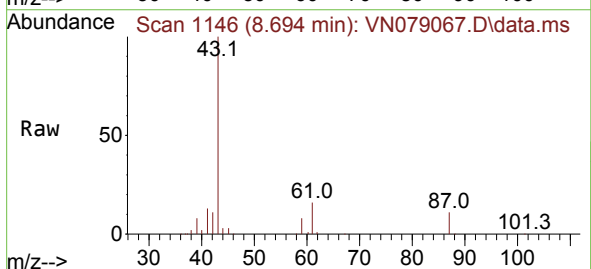





#45
1,2-Dichloropropane
Concen: 0.526 ug/l
RT: 9.753 min Scan# 11
Delta R.T. 0.129 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 1618
Ion Ratio Lower Upper
63 100
65 0.0 23.9 35.9#

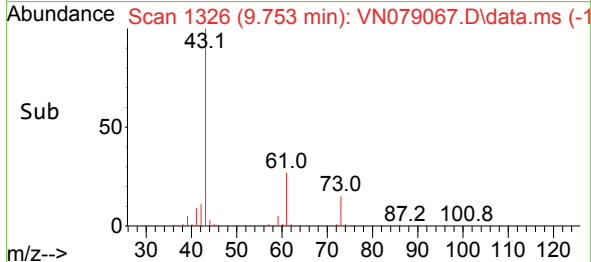

#48
Methyl methacrylate
Concen: 1.239 ug/l
RT: 9.671 min Scan# 1312
Delta R.T. -0.017 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Tgt Ion: 41 Resp: 4341
Ion Ratio Lower Upper
41 100
69 2.6 90.4 135.6#
39 64.5 54.6 81.8

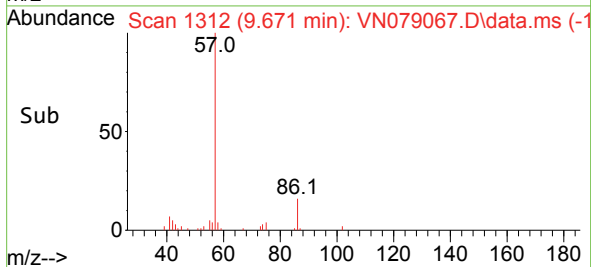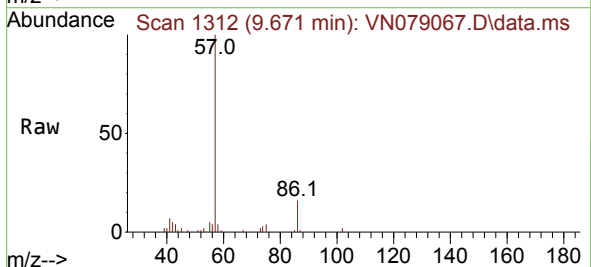



#49

1,4-Dioxane

Concen: 1.391 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.041 min


Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 88 Resp: 83

Ion Ratio Lower Upper

88 100

43 1757700.0 17.0 25.6#

58 8672.3 47.0 70.4#



#50

Toluene-d8

Concen: 50.654 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. -0.000 min

Lab File: VN079067.D




Acq: 28 Aug 2023 15:18


Tgt Ion: 98 Resp: 488820

Ion Ratio Lower Upper

98 100

100 64.0 52.0 78.0


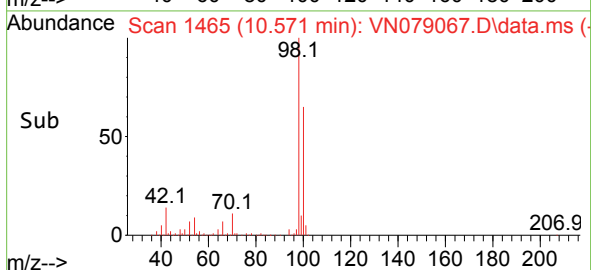




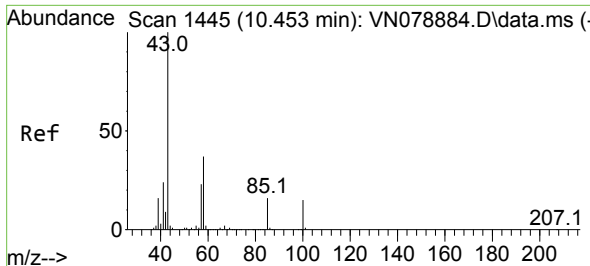

#51
4-Methyl-2-Pentanone
Concen: 8.305 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. -0.006 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 38084
Ion Ratio Lower Upper
43 100
58 30.4 36.6 54.8#

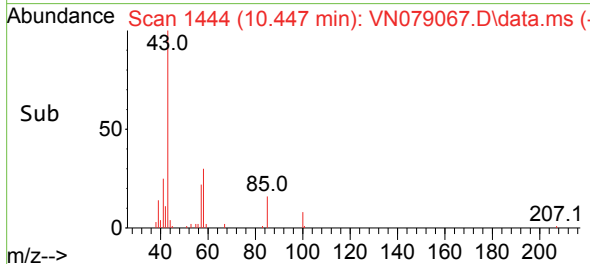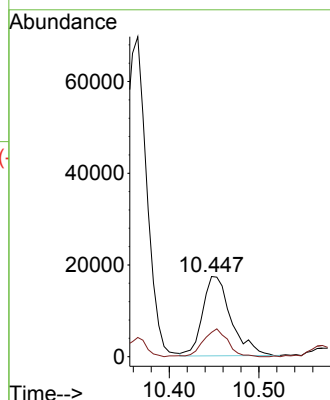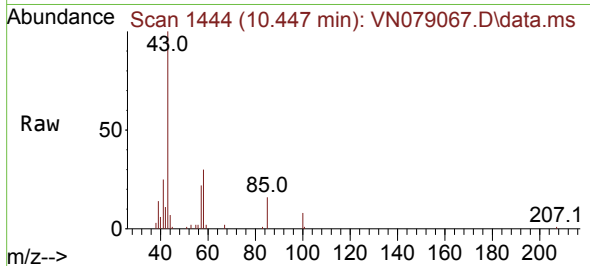

#54
cis-1,3-Dichloropropene
Concen: 10.678 ug/l
RT: 10.359 min Scan# 1429
Delta R.T. 0.041 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Tgt Ion: 75 Resp: 51966
Ion Ratio Lower Upper
75 100
77 0.0 26.1 39.1#
39 40.1 31.6 47.4

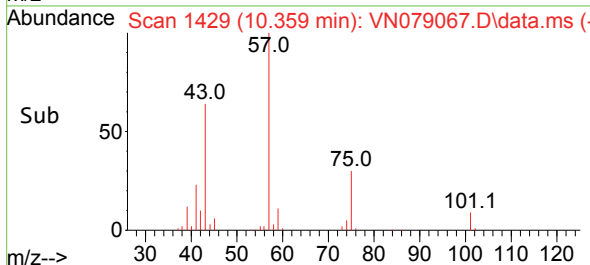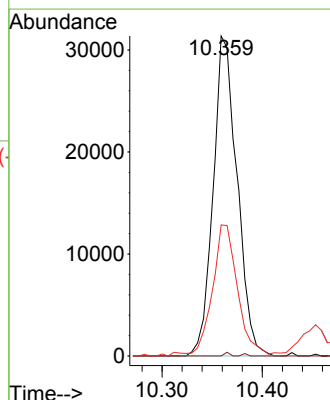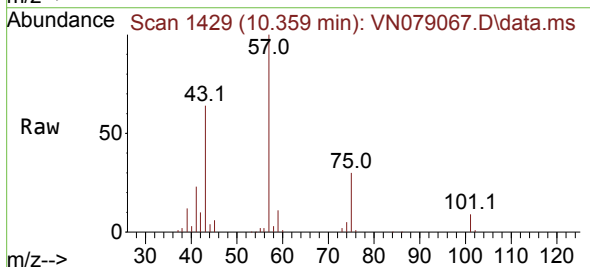

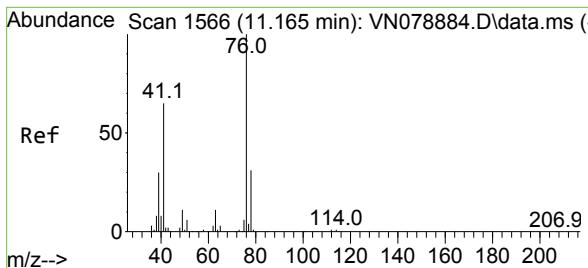

#57

1,3-Dichloropropane

Concen: 1.352 ug/l

RT: 11.206 min Scan# 11

Delta R.T. 0.041 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 76 Resp: 6881

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

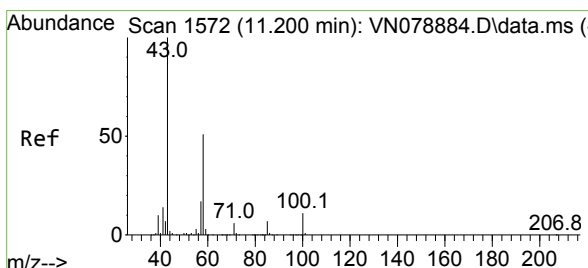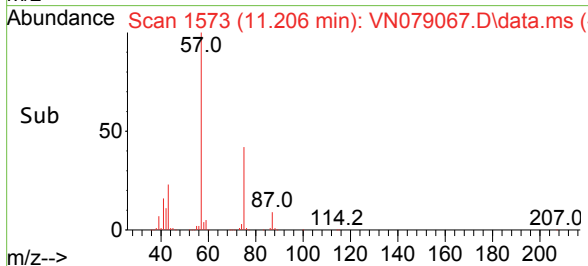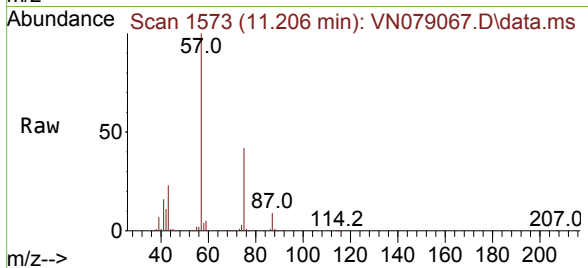

#59

2-Hexanone

Concen: 44.189 ug/l

RT: 11.177 min Scan# 1568

Delta R.T. -0.023 min

Lab File: VN079067.D




Acq: 28 Aug 2023 15:18


Tgt Ion: 43 Resp: 146764

Ion Ratio Lower Upper

43 100

58 0.0 31.7 95.1#


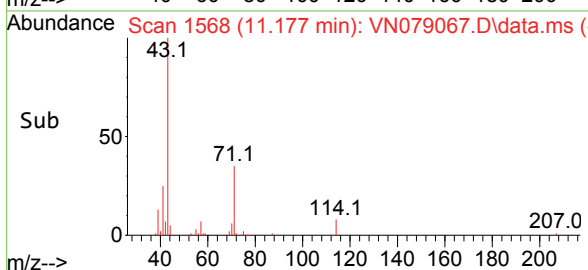

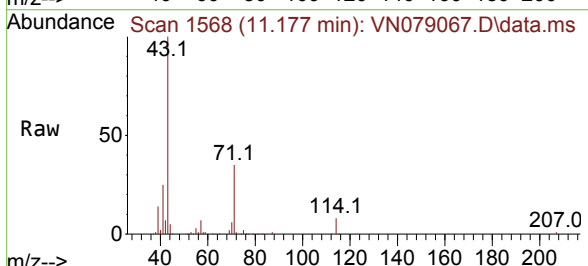


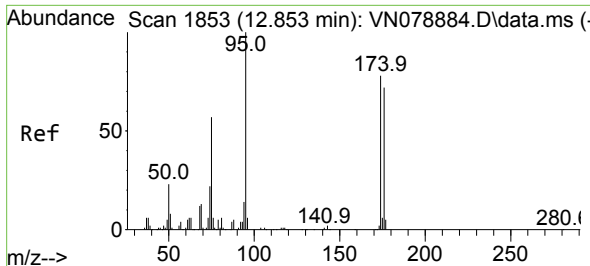

#62
4-Bromofluorobenzene
Concen: 48.725 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 153693
Ion Ratio Lower Upper
95 100
174 80.8 0.0 143.8
176 76.7 0.0 135.8

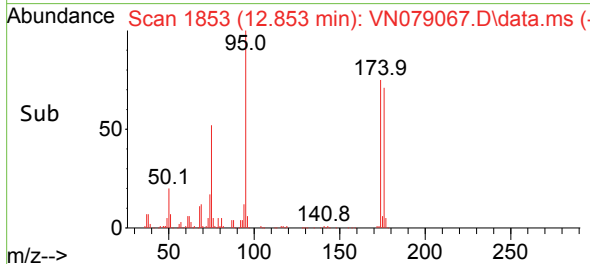

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Tgt Ion: 117 Resp: 375873
Ion Ratio Lower Upper
117 100
82 56.3 44.0 66.0
119 32.9 25.6 38.4

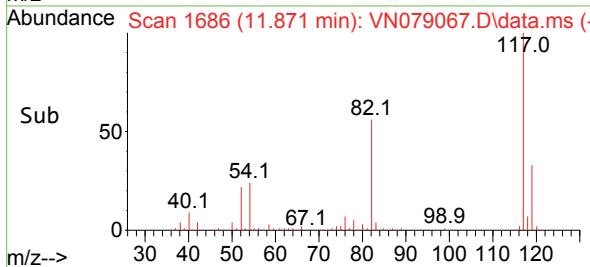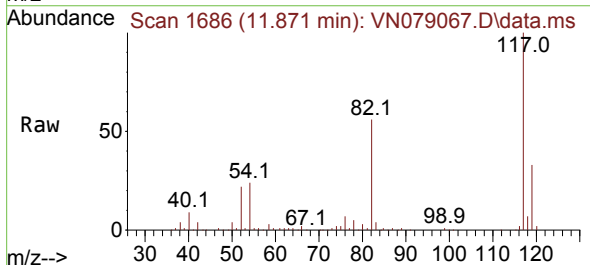



#71

Bromoform

Concen: 0.706 ug/l

RT: 12.847 min Scan# 11

Delta R.T. 0.265 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18





Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:173 Resp: 1552

Ion	Ratio	Lower	Upper
173	100		
175	474.7	24.3	73.0#
254	0.0	0.0	0.0

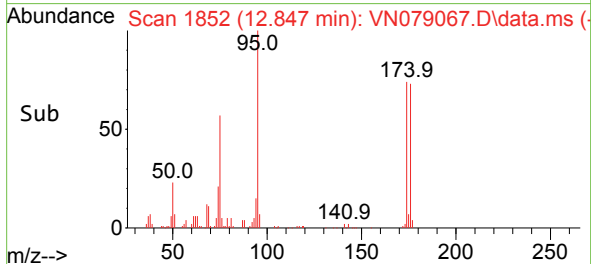

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013




Delta R.T. 0.000 min


Lab File: VN079067.D

Acq: 28 Aug 2023 15:18

Tgt Ion:152 Resp: 125277


Ion	Ratio	Lower	Upper
152	100		
115	59.8	32.3	96.8
150	152.9	0.0	355.8

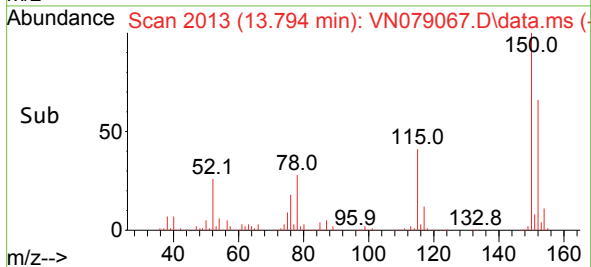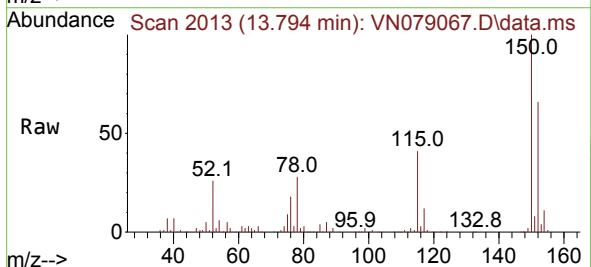






#74
N-amy1 acetate
Concen: 0.469 ug/l
RT: 12.494 min Scan# 1
Delta R.T. -0.006 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43	Resp: 2473
Ion Ratio	Lower Upper
43 100	
70 7.1	43.4 65.2#
55 9.7	21.4 32.0#
61 0.0	22.8 34.2#

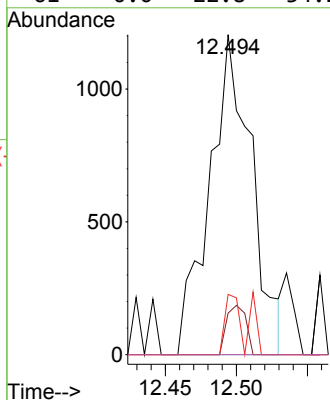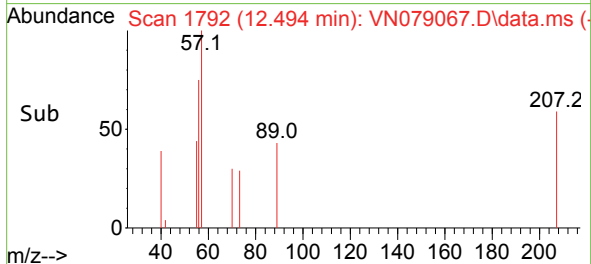

#76
1,2,3-Trichloropropane
Concen: 28.288 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Tgt Ion: 75	Resp: 85390
Ion Ratio	Lower Upper
75 100	
77 1.8	84.5 253.5#


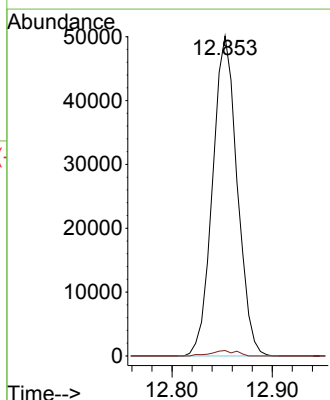

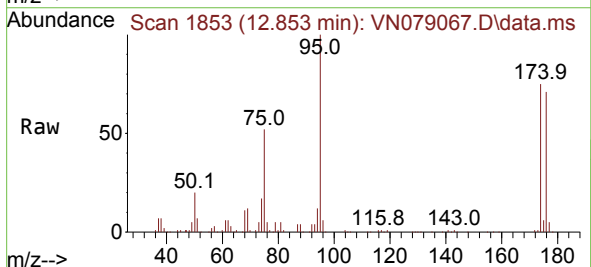




#81
 trans-1,4-Dichloro-2-butene
 Concen: 72.264 ug/l
 RT: 12.853 min Scan# 11
 Delta R.T. 0.112 min
 Lab File: VN079067.D
 Acq: 28 Aug 2023 15:18




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 85390
 Ion Ratio Lower Upper
 75 100
 53 0.0 67.4 101.2#
 89 0.1 38.8 58.2#

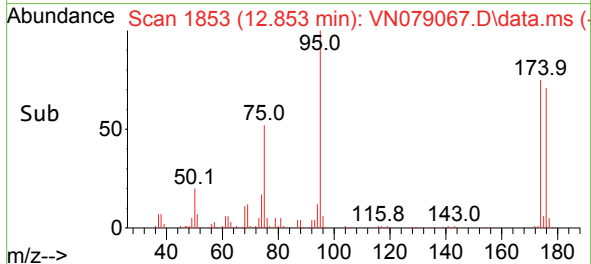

#82
 4-Chlorotoluene
 Concen: 0.212 ug/l
 RT: 13.235 min Scan# 1918
 Delta R.T. 0.006 min
 Lab File: VN079067.D
 Acq: 28 Aug 2023 15:18

Tgt Ion: 91 Resp: 1557
 Ion Ratio Lower Upper
 91 100
 126 69.3 16.7 50.0#


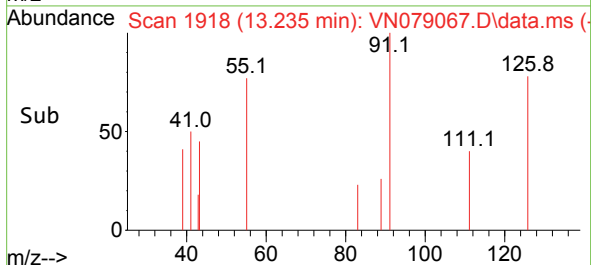

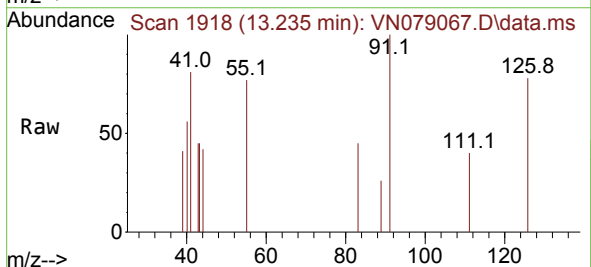


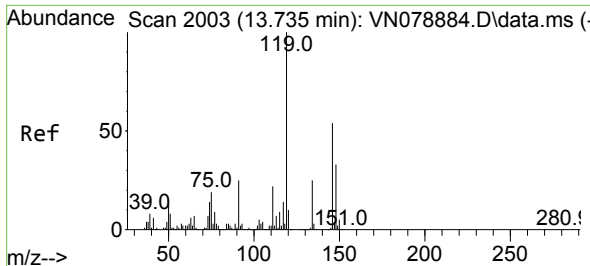

#87
1,3-Dichlorobenzene
Concen: 0.243 ug/l
RT: 13.741 min Scan# 2003
Delta R.T. 0.000 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:146 Resp: 1049
Ion Ratio Lower Upper
146 100
111 19.5 22.1 66.3#
148 67.3 32.0 96.0

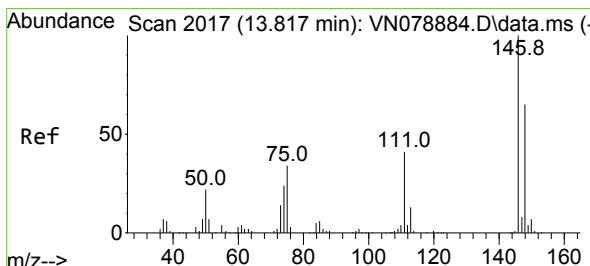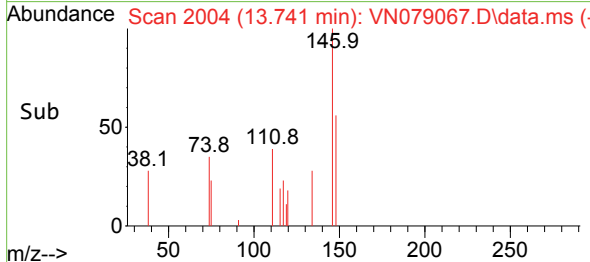

#88
1,4-Dichlorobenzene
Concen: 0.337 ug/l
RT: 13.818 min Scan# 2017
Delta R.T. -0.000 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Tgt Ion:146 Resp: 1459
Ion Ratio Lower Upper
146 100
111 0.0 20.6 61.8#
148 100.6 31.6 94.8#

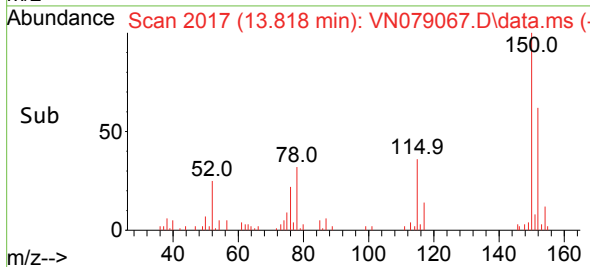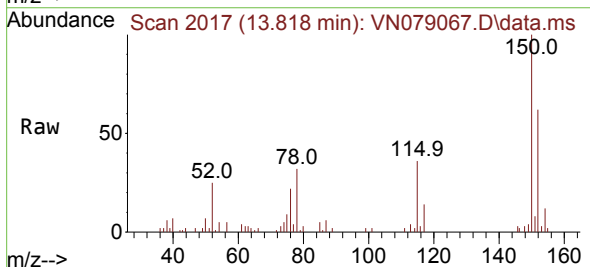



#89

n-Butylbenzene

Concen: 0.239 ug/l

RT: 14.065 min Scan# 2059

Delta R.T. 0.006 min

Lab File: VN079067.D





Acq: 28 Aug 2023 15:18

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:	91	Resp:	1507
Ion	Ratio	Lower	Upper
91	100		
92	63.0	26.4	79.0
134	27.6	12.6	37.6

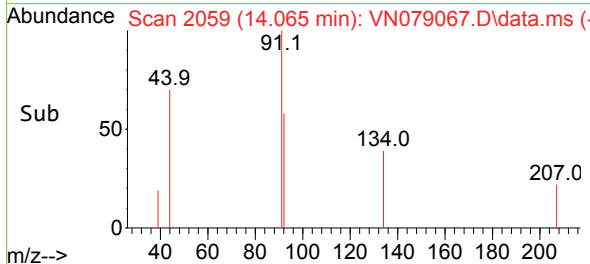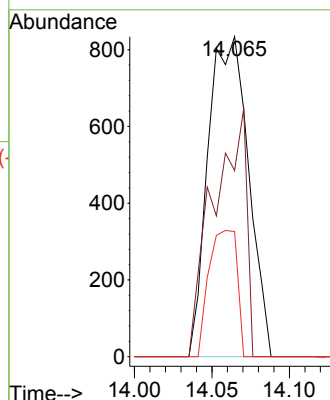

#92

1,2-Dibromo-3-Chloropropane

Concen: Below Cal




RT: 14.712 min Scan# 2169


Delta R.T. -0.011 min

Lab File: VN079067.D

Acq: 28 Aug 2023 15:18


Tgt Ion:	75	Resp:	333
Ion	Ratio	Lower	Upper
75	100		
155	0.0	39.1	117.2#
157	0.0	50.3	150.9#

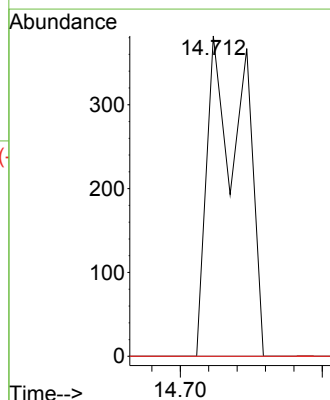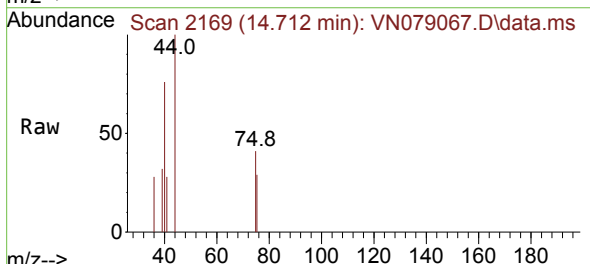






#93
 1,2,4-Trichlorobenzene
 Concen: 0.907 ug/l
 RT: 15.394 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN079067.D
 Acq: 28 Aug 2023 15:18

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion:180 Resp: 1382
 Ion Ratio Lower Upper
 180 100
 182 70.5 46.1 138.2
 145 11.4 16.6 49.8#

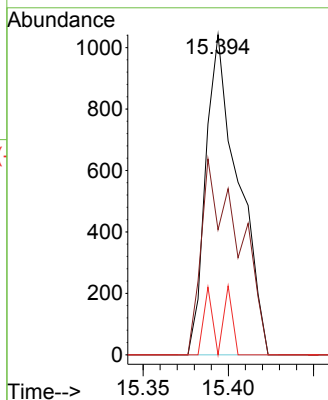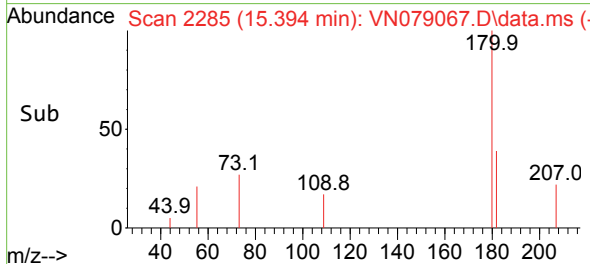

#94
 Hexachlorobutadiene
 Concen: 0.445 ug/l
 RT: 15.506 min Scan# 2304
 Delta R.T. -0.000 min
 Lab File: VN079067.D
 Acq: 28 Aug 2023 15:18

Tgt Ion:225 Resp: 574
 Ion Ratio Lower Upper
 225 100
 223 20.2 31.3 93.8#
 227 9.9 31.9 95.9#


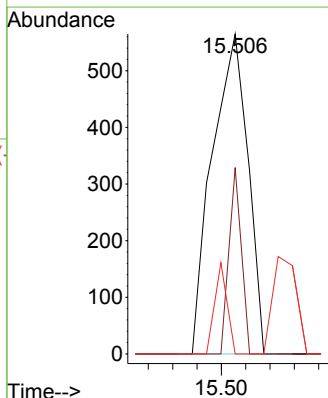
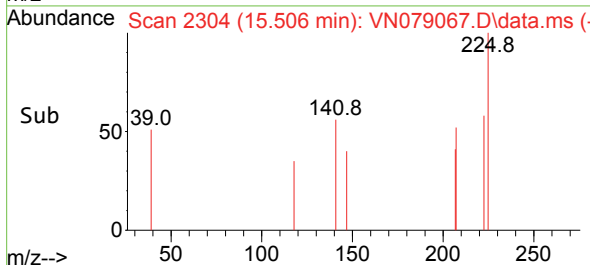
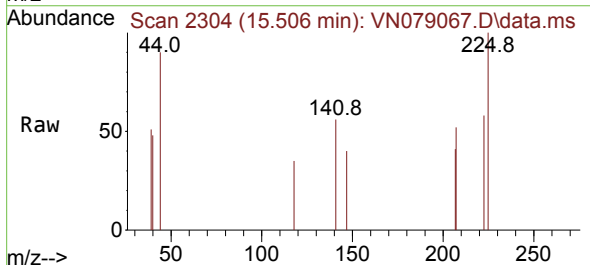


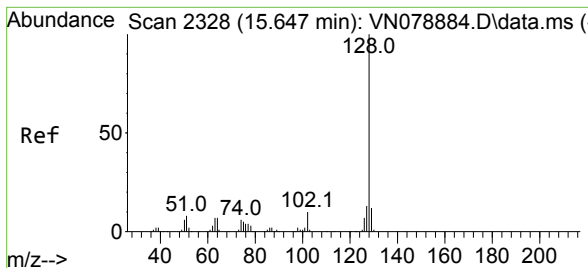

#95
Naphthalene
Concen: 3.280 ug/l
RT: 15.647 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 4293
Ion Ratio Lower Upper
128 100
127 7.9 10.0 15.0#
129 12.2 8.7 13.1

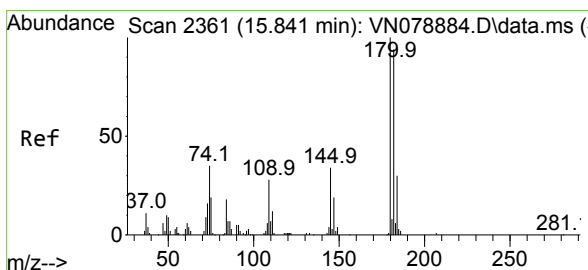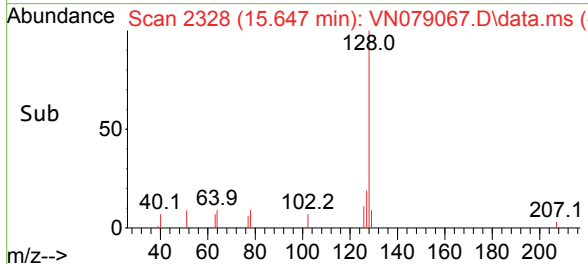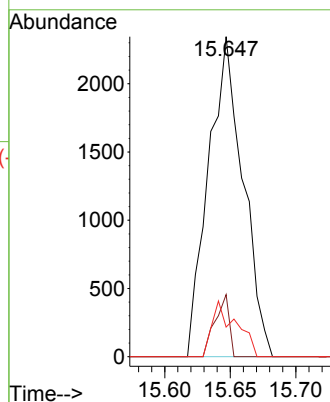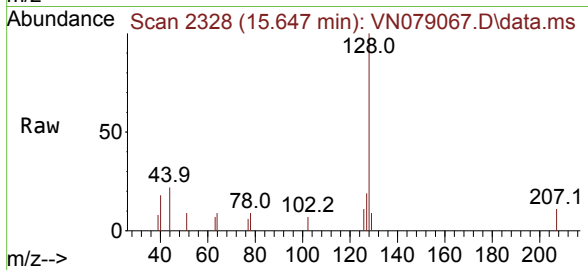

#96
1,2,3-Trichlorobenzene
Concen: 0.798 ug/l
RT: 15.847 min Scan# 2362
Delta R.T. -0.000 min
Lab File: VN079067.D
Acq: 28 Aug 2023 15:18

Tgt Ion:180 Resp: 1332
Ion Ratio Lower Upper
180 100
182 73.0 46.2 138.6
145 4.1 17.5 52.6#

