
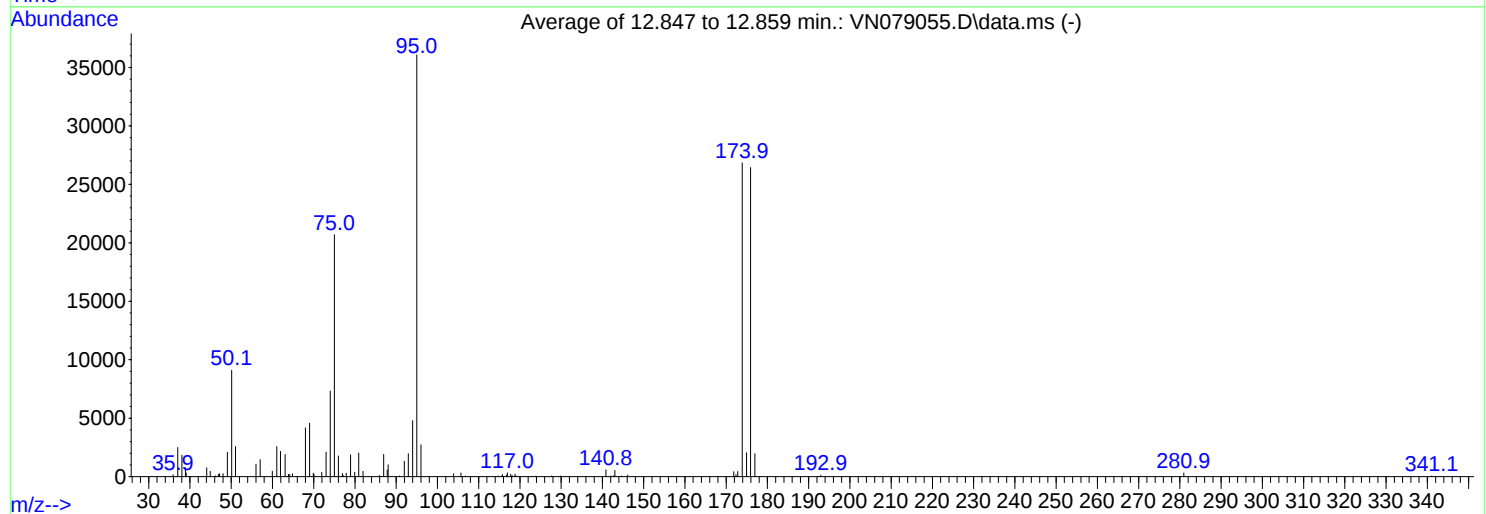


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082823\
Data File : VN079055.D
Acq On : 28 Aug 2023 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Title : SW846 8260
Last Update : Wed Aug 16 02:42:02 2023

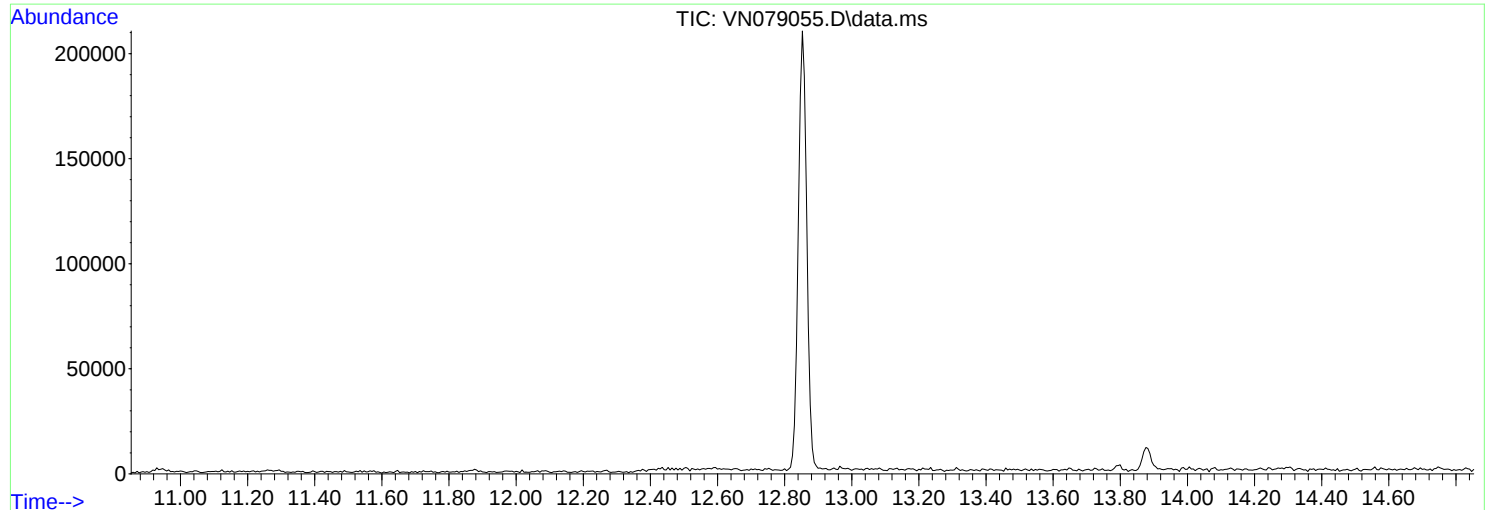

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.2	9101	PASS
75	95	30	60	57.3	20691	PASS
95	95	100	100	100.0	36080	PASS
96	95	5	9	7.5	2718	PASS
173	174	0.00	2	1.6	440	PASS
174	95	50	100	74.4	26845	PASS
175	174	5	9	7.6	2044	PASS
176	174	95	101	98.5	26445	PASS
177	176	5	9	7.4	1956	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	161	49.05	2074	64.85	246	77.20	82
37.05	2497	50.10	9101	68.00	4179	77.90	286
38.05	1828	51.05	2572	69.00	4589	78.95	1858
38.90	758	56.00	1073	69.90	302	79.95	388
39.10	320	57.00	1449	70.10	190	80.90	2015
44.05	760	59.95	472	71.95	372	81.95	457
44.90	456	61.05	2573	73.00	2098	85.90	90
46.20	75	61.95	2159	74.00	7317	86.95	1902
46.90	195	63.05	1888	75.00	20691	87.80	571
47.15	252	63.90	195	76.00	1771	88.05	1018
48.00	258	64.20	191	76.95	269	90.80	56

Average of 12.847 to 12.859 min.: VN079055.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.95	1315	116.70	127	142.70	81	192.95	118
92.95	1954	116.95	326	143.00	533	280.95	321
94.00	4792	117.75	203	144.70	52	341.10	51
95.00	36080	118.10	92	146.10	135		
96.00	2718	118.80	210	171.85	431		
103.90	250	119.00	79	172.40	159		
105.70	315	123.90	59	172.80	440		
106.80	52	127.70	58	173.90	26845		
114.80	63	129.80	63	174.95	2044		
115.60	63	140.85	588	175.90	26445		
115.75	184	142.00	61	176.95	1956		