
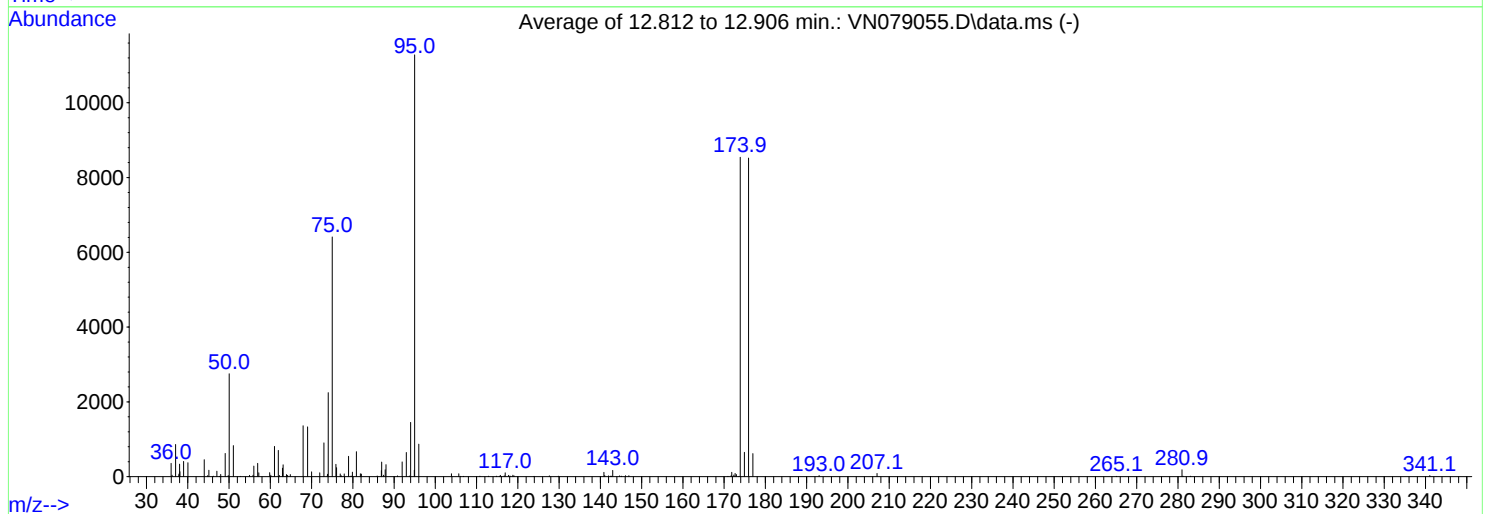


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082823\
Data File : VN079055.D
Acq On : 28 Aug 2023 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N081723W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Aug 18 05:21:14 2023

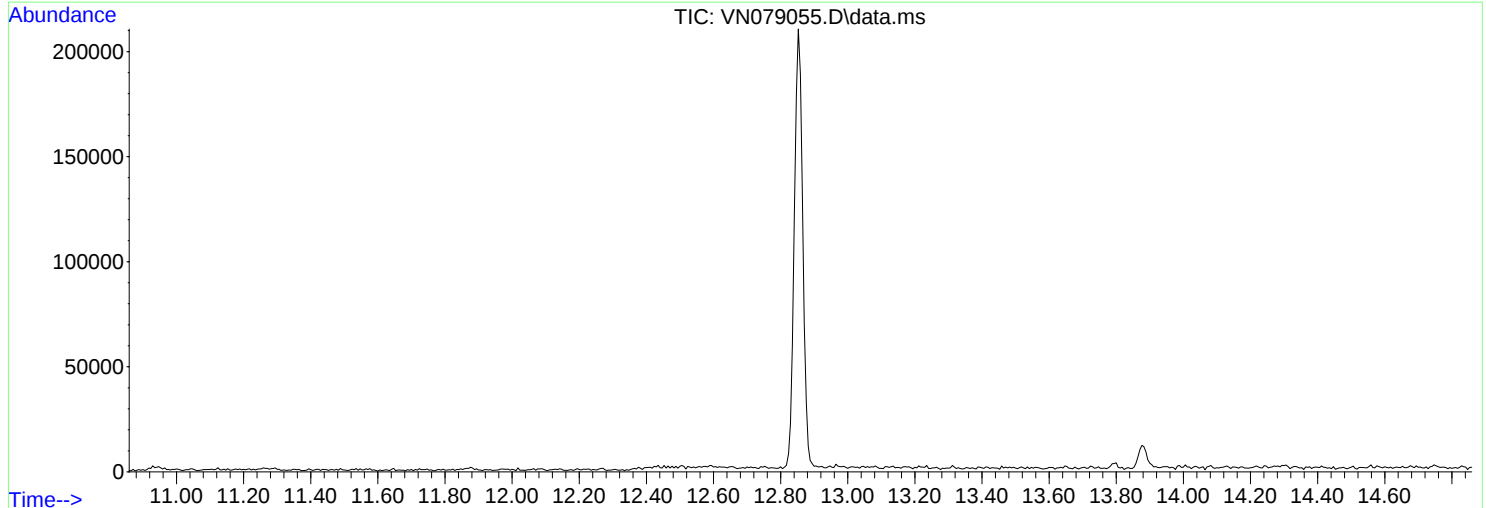

AutoFind: Averaged scan 1846 to 1862; Bkg corrected with scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	2751	PASS
75	95	30	60	56.8	6412	PASS
95	95	100	100	100.0	11282	PASS
96	95	5	9	7.7	867	PASS
173	174	0.00	2	0.6	55	PASS
174	95	50	100	75.7	8543	PASS
175	174	5	9	7.6	650	PASS
176	174	95	101	99.8	8523	PASS
177	176	5	9	7.3	618	PASS