

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082825\
 Data File : VN087683.D
 Acq On : 28 Aug 2025 14:26
 Operator : JC\MD
 Sample : Q2959-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 NWB-2200

Quant Time: Aug 29 03:18:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 22 02:55:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.212	168	168668	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	398620	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	399523	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	179426	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	196898	56.976	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 113.960%			
35) Dibromofluoromethane	8.153	113	146312	50.838	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.680%			
50) Toluene-d8	10.547	98	532406	49.425	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 98.860%			
62) 4-Bromofluorobenzene	12.829	95	187691	48.995	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 97.980%			
Target Compounds					Qvalue	
3) Chloromethane	2.383	50	24405	9.913	ug/l	97
5) Bromomethane	2.995	94	915	0.621	ug/l #	71
10) Methyl Iodide	4.583	142	552	7.080	ug/l #	38
11) Tert butyl alcohol	5.530	59	2349	3.915	ug/l #	79
13) Acrolein	4.177	56	209	0.283	ug/l #	48
14) Allyl chloride	5.024	41	1573	0.357	ug/l #	33
16) Acetone	4.424	43	45858	24.377	ug/l	98
17) Carbon Disulfide	4.694	76	1374	0.205	ug/l #	74
18) Methyl Acetate	5.024	43	157973	40.106	ug/l	98
20) Methylene Chloride	5.271	84	20370	6.404	ug/l	85
25) 2-Butanone	7.471	43	25285	10.216	ug/l #	89
29) Tetrahydrofuran	7.830	42	1747	1.097	ug/l #	38
31) Cyclohexane	8.218	56	5783	1.330	ug/l #	21
36) 1,1-Dichloropropene	8.212	75	17150	3.884	ug/l #	51
37) Ethyl Acetate	7.553	43	22223	3.683	ug/l #	93
38) Carbon Tetrachloride	8.206	117	19566	4.488	ug/l #	18
40) Benzene	8.582	78	3264	0.241	ug/l #	90
43) Isopropyl Acetate	8.677	43	15531	1.649	ug/l #	92
45) 1,2-Dichloropropane	9.724	63	1934	0.542	ug/l #	43
48) Methyl methacrylate	9.629	41	4244	0.953	ug/l #	13
51) 4-Methyl-2-Pentanone	10.424	43	8122	1.429	ug/l #	71
52) Toluene	10.606	92	3078	0.367	ug/l	91
54) cis-1,3-Dichloropropene	10.341	75	63492	11.347	ug/l #	68
57) 1,3-Dichloropropane	11.194	76	4375	0.761	ug/l #	44
59) 2-Hexanone	11.182	43	87199	24.277	ug/l #	52
68) m/p-Xylenes	12.041	106	1670	0.265	ug/l	93
69) o-Xylene	12.370	106	1323	0.214	ug/l	67
76) 1,2,3-Trichloropropane	12.829	75	111097	26.404	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.829	75	111097	69.901	ug/l #	1
95) Naphthalene	15.611	128	17867	1.315	ug/l #	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082825\
Data File : VN087683.D
Acq On : 28 Aug 2025 14:26
Operator : JC\MD
Sample : Q2959-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-2200

Quant Time: Aug 29 03:18:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 22 02:55:42 2025
Response via : Initial Calibration




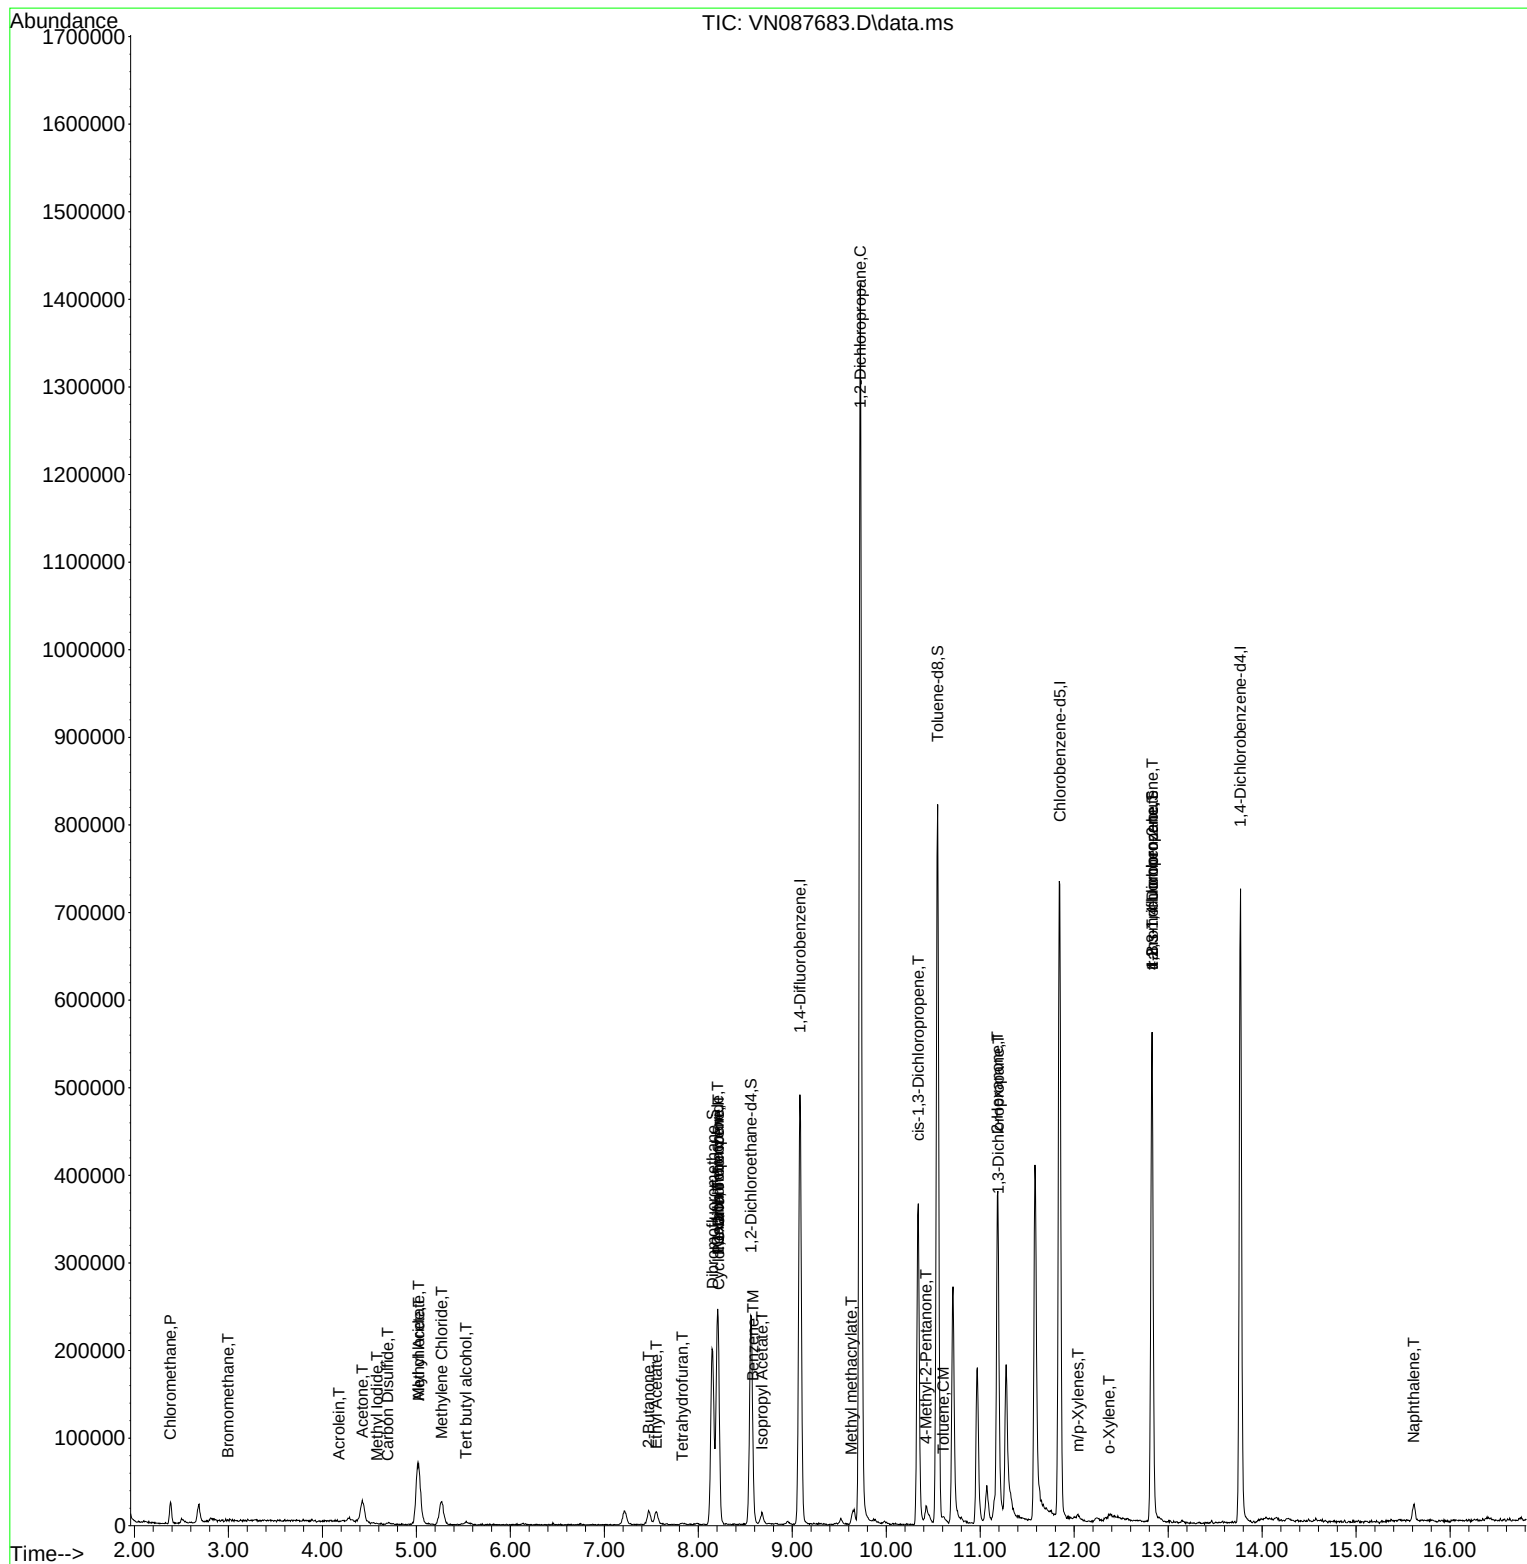




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.212 min Scan# 1064
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion:168 Resp: 168668
Ion Ratio Lower Upper
168 100
99 64.5 57.2 85.8

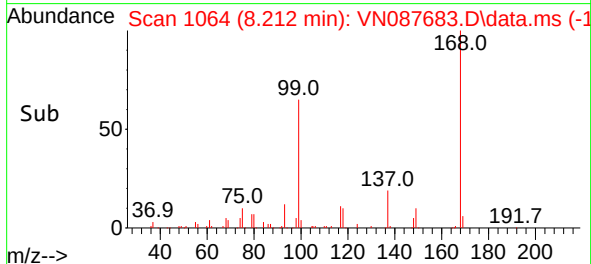

#3
Chloromethane
Concen: 9.913 ug/l
RT: 2.383 min Scan# 73
Delta R.T. -0.000 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion: 50 Resp: 24405
Ion Ratio Lower Upper
50 100
52 31.1 26.2 39.4



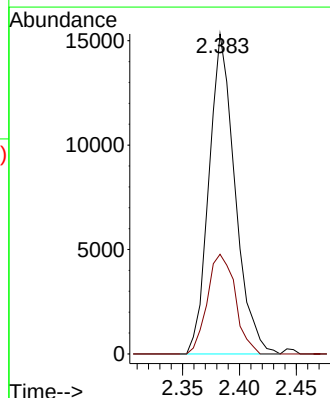
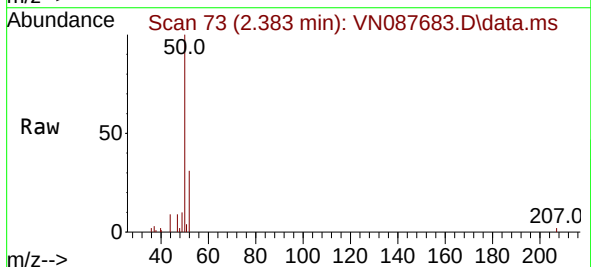




#5
Bromomethane
Concen: 0.621 ug/l
RT: 2.995 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion: 94 Resp: 915
Ion Ratio Lower Upper
94 100
96 122.0 75.4 113.2#

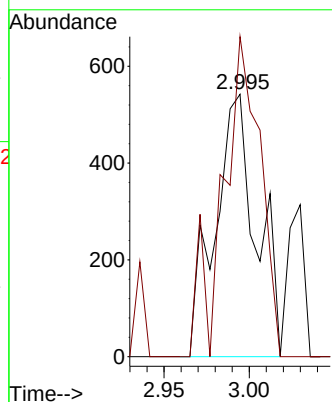

#10
Methyl Iodide
Concen: 7.080 ug/l
RT: 4.583 min Scan# 447
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion:142 Resp: 552
Ion Ratio Lower Upper
142 100
127 0.0 38.0 57.0#
141 0.0 12.0 18.0#


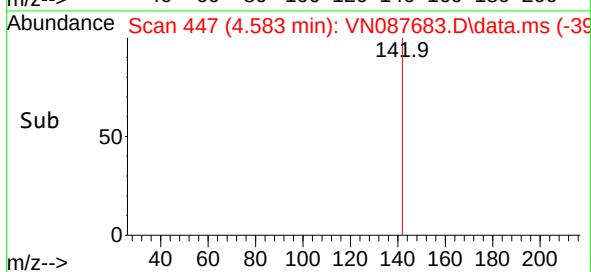
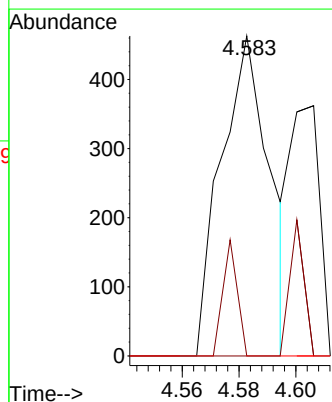



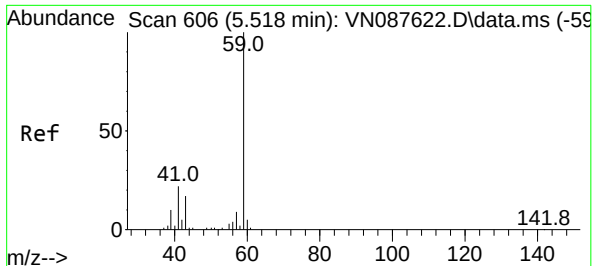

#11
Tert butyl alcohol
Concen: 3.915 ug/l
RT: 5.530 min Scan# 606
Delta R.T. 0.012 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion: 59 Resp: 2349
Ion Ratio Lower Upper
59 100
57 3.1 9.0 13.4#

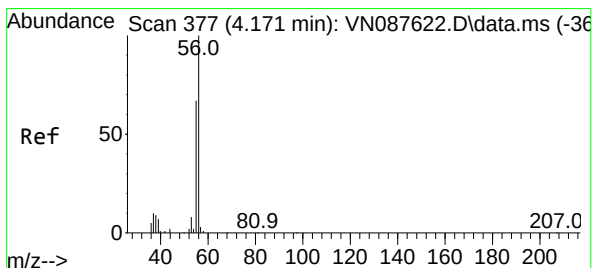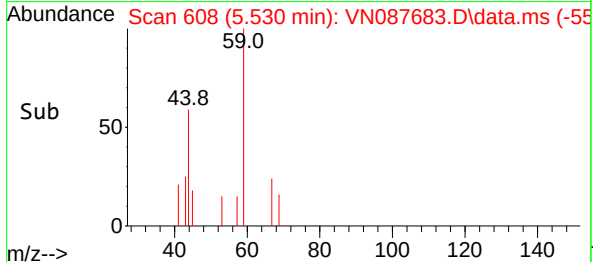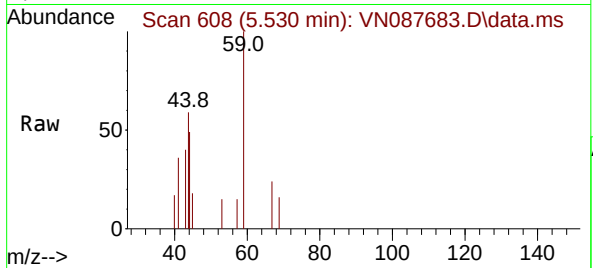

#13
Acrolein
Concen: 0.283 ug/l
RT: 4.177 min Scan# 378
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion: 56 Resp: 209
Ion Ratio Lower Upper
56 100
55 114.8 57.3 85.9#

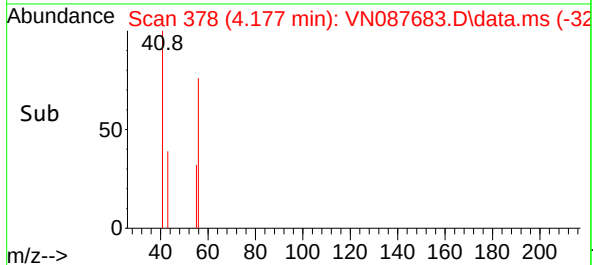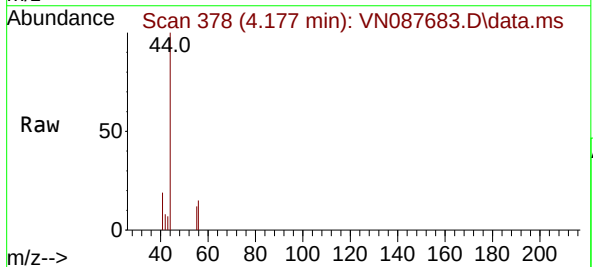



#14

Allyl chloride

Concen: 0.357 ug/l

RT: 5.024 min Scan# 51

Delta R.T. 0.018 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26

Instrument :

MSVOA_N

ClientSampleId :

NWB-2200





Tgt Ion: 41 Resp: 1573

Ion Ratio Lower Upper

41 100

39 14.2 63.9 95.9#

76 5.3 28.1 42.1#

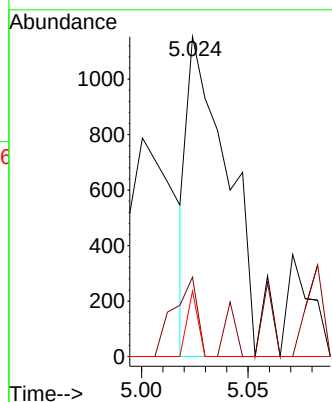

#16

Acetone

Concen: 24.377 ug/l

RT: 4.424 min Scan# 420

Delta R.T. -0.000 min

Lab File: VN087683.D




Acq: 28 Aug 2025 14:26


Tgt Ion: 43 Resp: 45858

Ion Ratio Lower Upper

43 100

58 27.2 22.6 33.8


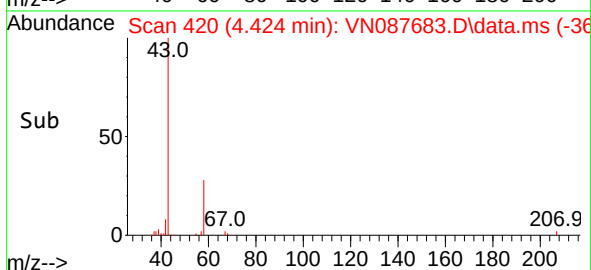






#17
Carbon Disulfide
Concen: 0.205 ug/l
RT: 4.694 min Scan# 466
Delta R.T. -0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion: 76 Resp: 1374
Ion Ratio Lower Upper
76 100
78 0.0 7.6 11.4#

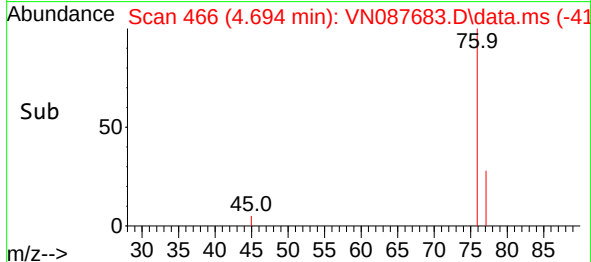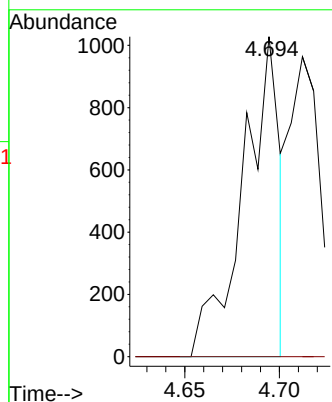

#18
Methyl Acetate
Concen: 40.106 ug/l
RT: 5.024 min Scan# 522
Delta R.T. 0.012 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion: 43 Resp: 157973
Ion Ratio Lower Upper
43 100
74 23.0 17.6 26.4


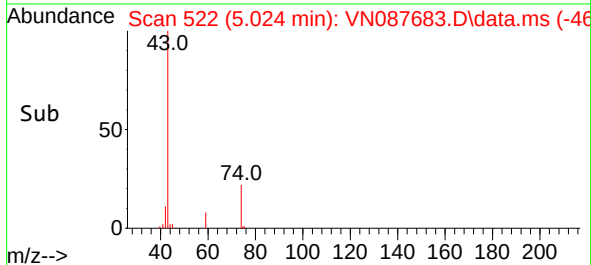
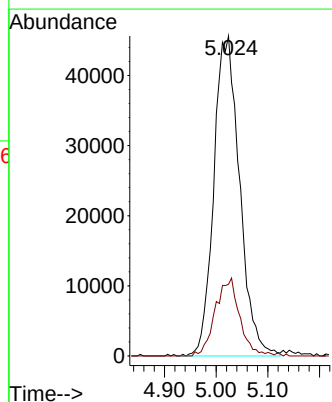
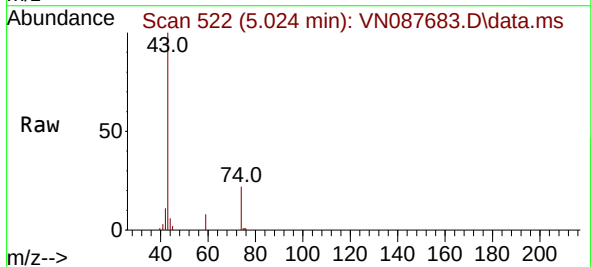




#20
Methylene Chloride
Concen: 6.404 ug/l
RT: 5.271 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion:	84	Resp:	20370
Ion	Ratio	Lower	Upper
84	100		
49	104.8	103.4	155.2
51	47.0	33.8	50.8
86	55.0	49.6	74.4

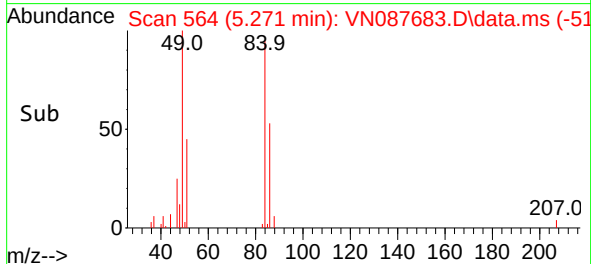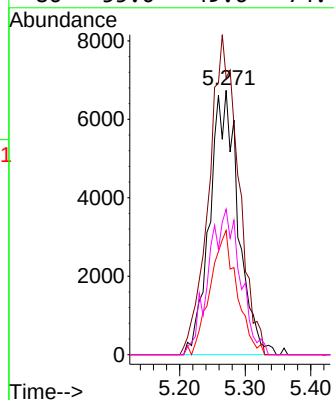

#25
2-Butanone
Concen: 10.216 ug/l
RT: 7.471 min Scan# 938
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion:	43	Resp:	25285
Ion	Ratio	Lower	Upper
43	100		
72	30.4	19.9	29.9#

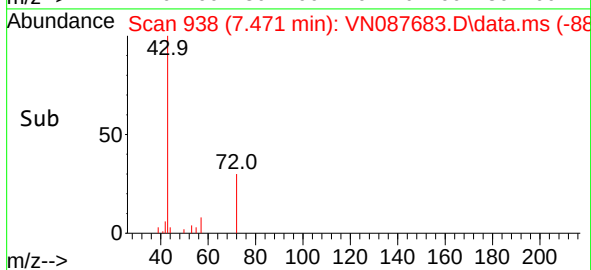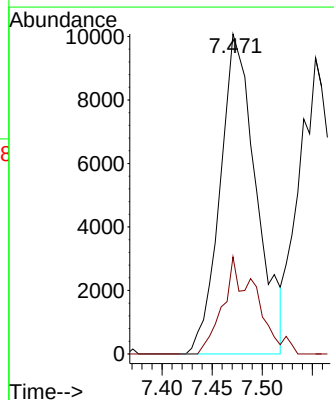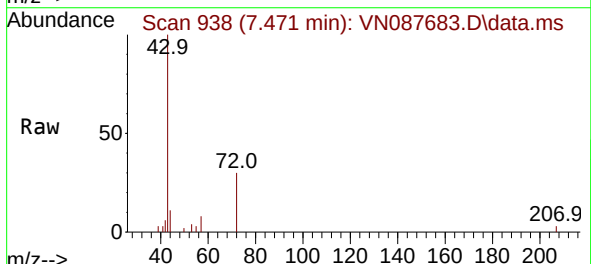



#29

Tetrahydrofuran

Concen: 1.097 ug/l

RT: 7.830 min Scan# 998

Delta R.T. 0.006 min

Lab File: VN087683.D


Acq: 28 Aug 2025 14:26

Instrument :




MSVOA_N

ClientSampleId :

NWB-2200



Tgt Ion:	42	Resp:	1747
Ion Ratio	100	Lower	Upper
42	100		
72	4.1	33.7	50.5#
71	0.0	31.9	47.9#

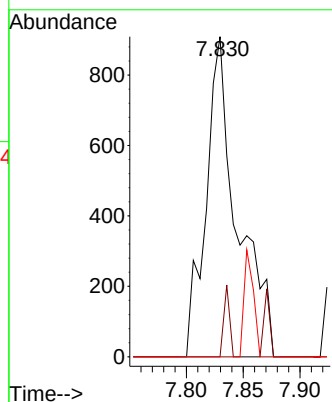

#31

Cyclohexane

Concen: 1.330 ug/l




RT: 8.218 min Scan# 1065


Delta R.T. -0.018 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26

Tgt Ion:	56	Resp:	5783
Ion Ratio	100	Lower	Upper
56	100		
69	97.3	23.7	35.5#
84	136.3	64.7	97.1#

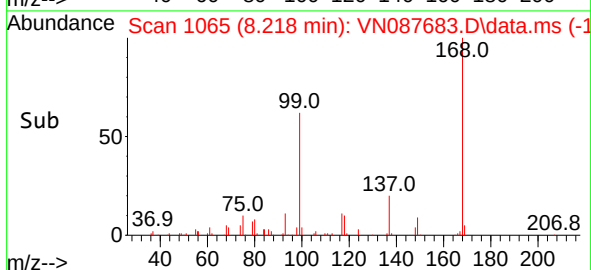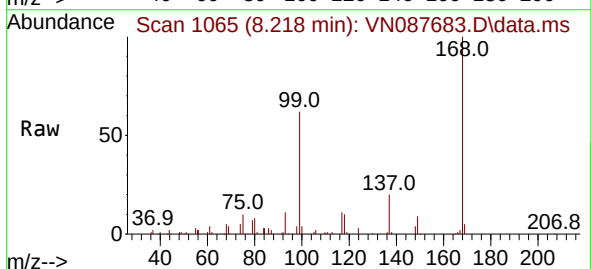

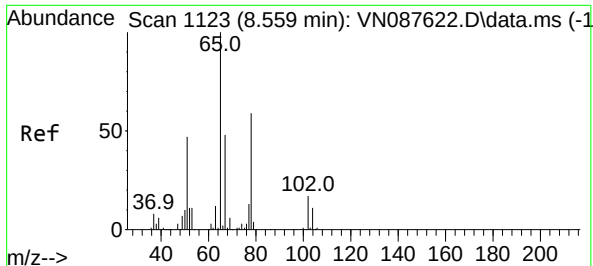

#33

1,2-Dichloroethane-d4

Concen: 56.976 ug/l

RT: 8.559 min Scan# 1123

Delta R.T. -0.000 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26

Instrument :

MSVOA_N

ClientSampleId :





NWB-2200

Tgt Ion: 65 Resp: 196898

Ion Ratio Lower Upper

65 100

67 51.0 0.0 100.0

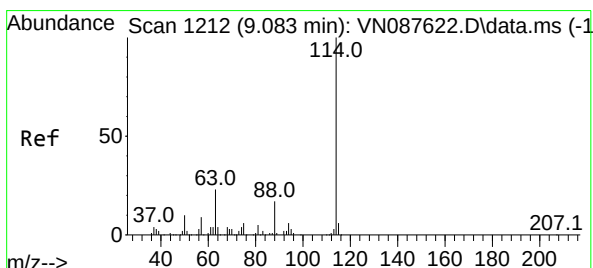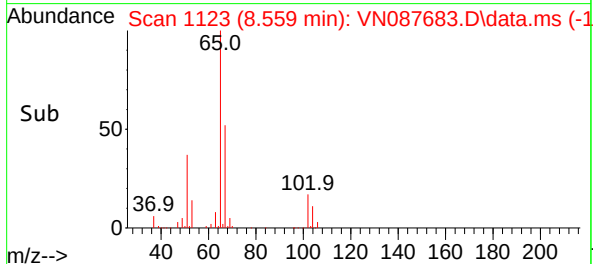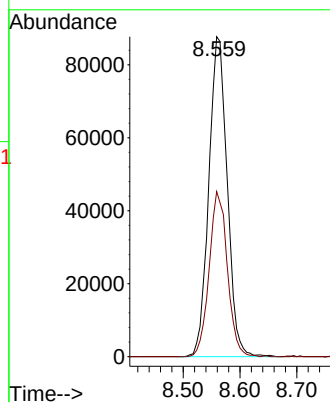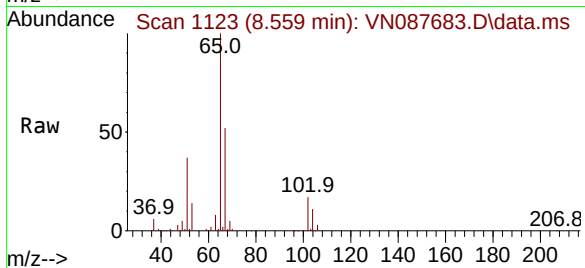

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 1212

Delta R.T. -0.000 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26




Tgt Ion: 114 Resp: 398620


Ion Ratio Lower Upper

114 100

63 22.6 0.0 45.2

88 16.3 0.0 33.4

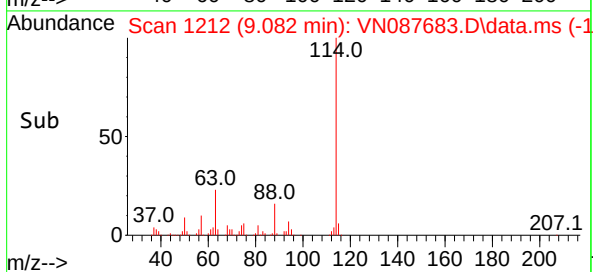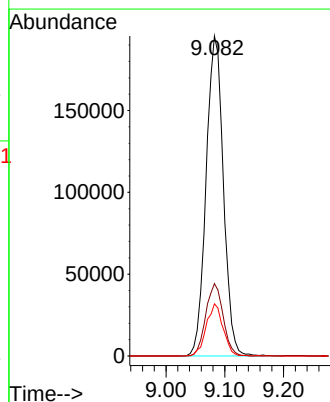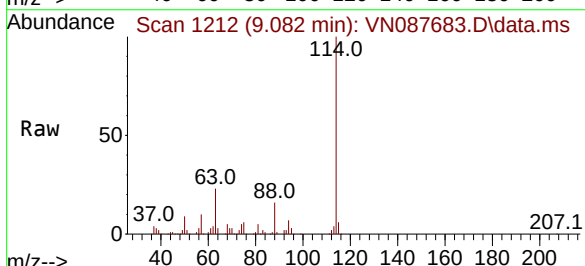

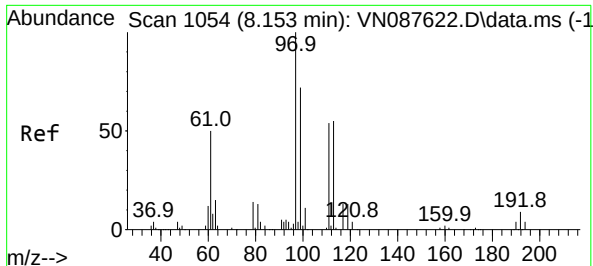

#35

Dibromofluoromethane

Concen: 50.838 ug/l

RT: 8.153 min Scan# 1064

Delta R.T. -0.000 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26

Instrument :

MSVOA_N

ClientSampleId :

NWB-2200





Tgt Ion:113 Resp: 146312

Ion Ratio Lower Upper

113 100

111 102.7 82.8 124.2

192 16.0 12.8 19.2

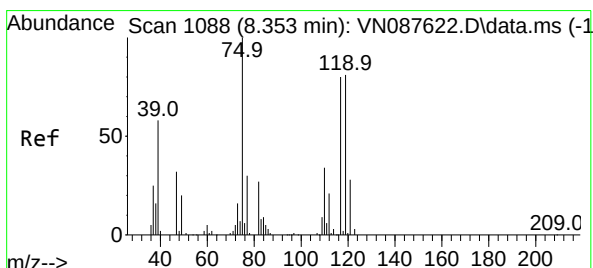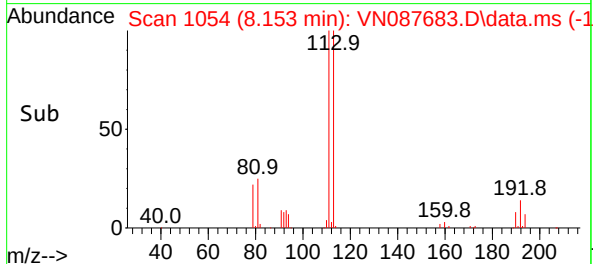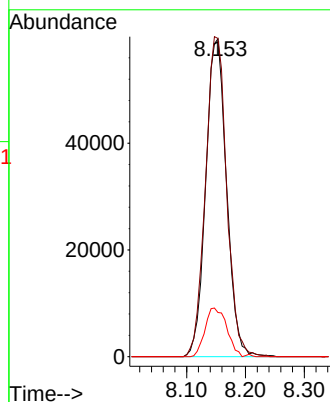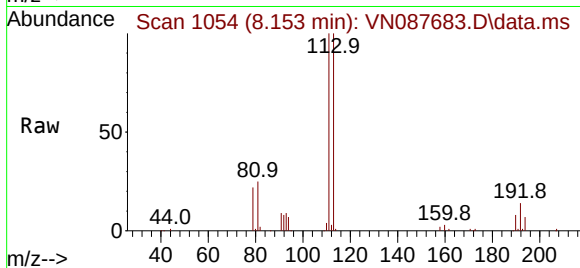

#36

1,1-Dichloropropene

Concen: 3.884 ug/l

RT: 8.212 min Scan# 1064

Delta R.T. -0.141 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26




Tgt Ion: 75 Resp: 17150


Ion Ratio Lower Upper

75 100

110 7.7 15.9 47.6#

77 0.0 24.4 36.6#

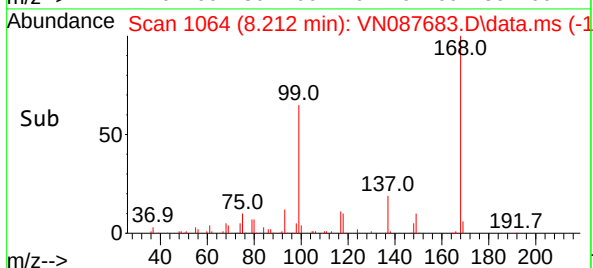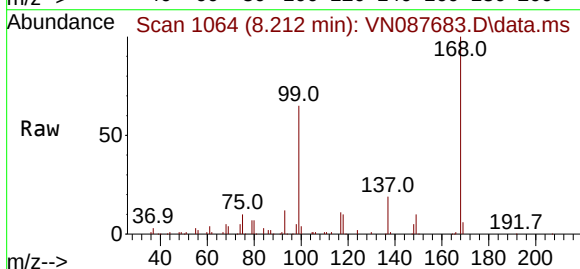



#37

Ethyl Acetate

Concen: 3.683 ug/l

RT: 7.553 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26

Instrument :

MSVOA_N

ClientSampleId :

NWB-2200





Tgt Ion: 43 Resp: 22223

Ion Ratio Lower Upper

43 100

61 15.4 9.3 13.9#

70 10.4 7.0 10.6

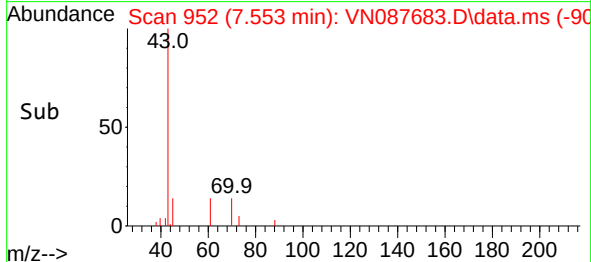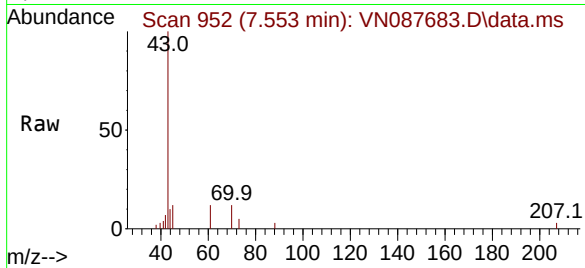

#38

Carbon Tetrachloride

Concen: 4.488 ug/l

RT: 8.206 min Scan# 1063

Delta R.T. -0.135 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26




Tgt Ion: 117 Resp: 19566


Ion Ratio Lower Upper

117 100

119 9.8 79.0 118.6#

121 0.0 25.0 37.6#


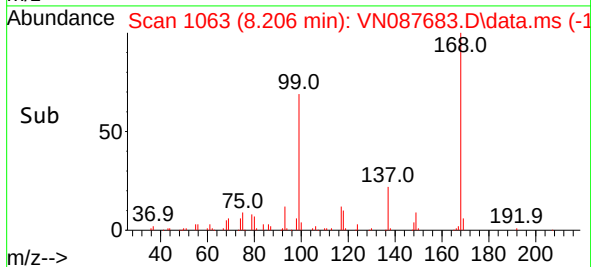

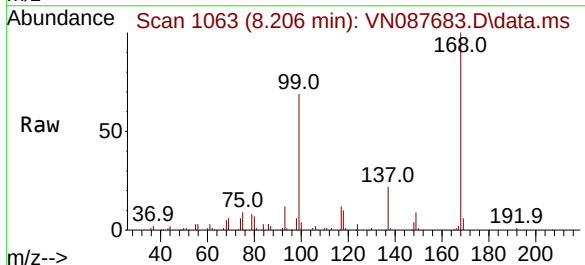


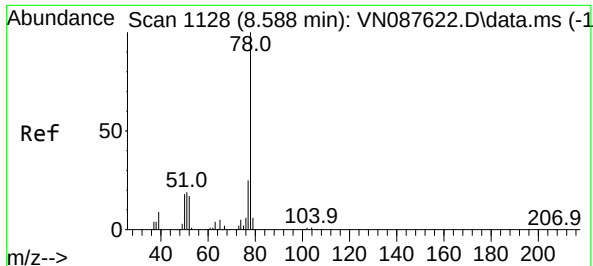

#40
Benzene
Concen: 0.241 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion: 78 Resp: 3264
Ion Ratio Lower Upper
78 100
77 19.5 19.7 29.5#

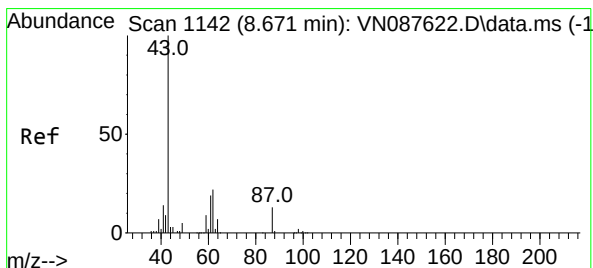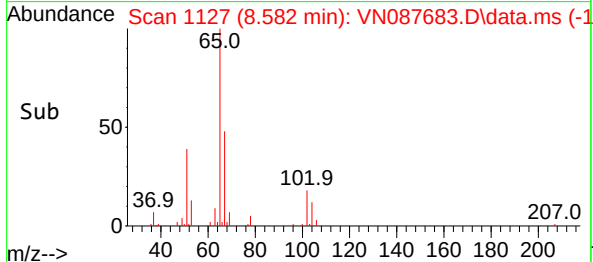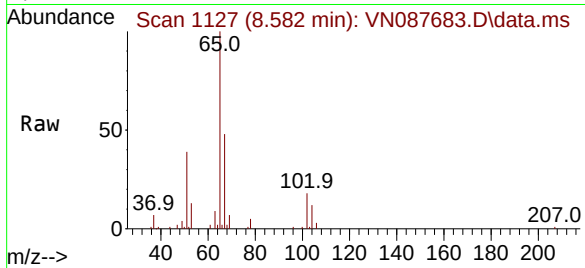

#43
Isopropyl Acetate
Concen: 1.649 ug/l
RT: 8.677 min Scan# 1143
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion: 43 Resp: 15531
Ion Ratio Lower Upper
43 100
61 18.4 18.8 28.2#
87 12.9 9.6 14.4

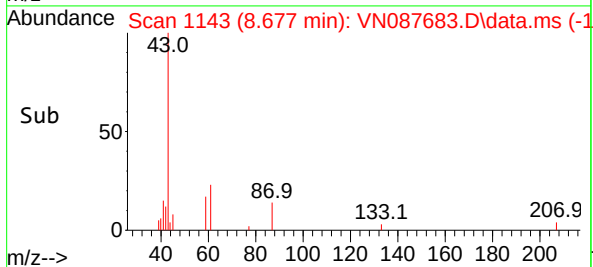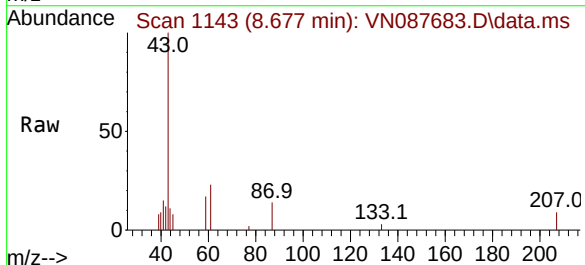

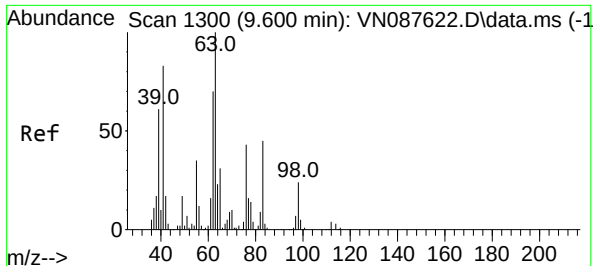

#45

1,2-Dichloropropane

Concen: 0.542 ug/l

RT: 9.724 min Scan# 11

Delta R.T. 0.123 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26

Instrument :

MSVOA_N

ClientSampleId :





NWB-2200

Tgt Ion: 63 Resp: 1934

Ion Ratio Lower Upper

63 100

65 0.0 25.0 37.4#

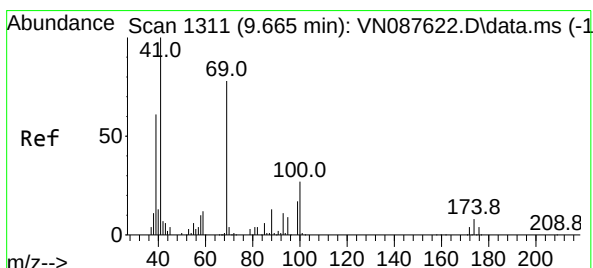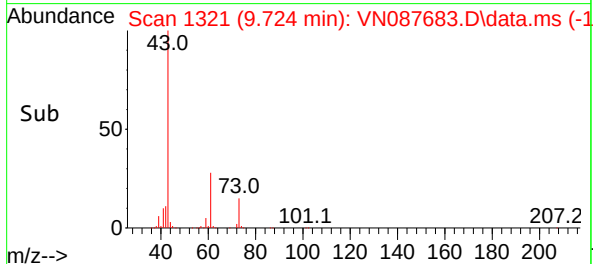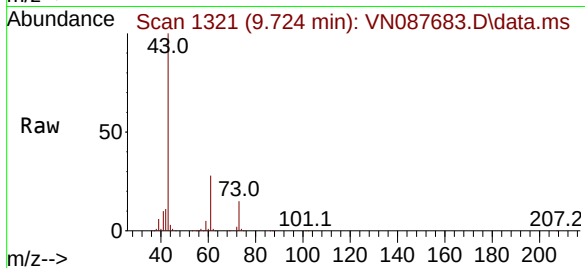

#48

Methyl methacrylate

Concen: 0.953 ug/l

RT: 9.629 min Scan# 1305

Delta R.T. -0.035 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26




Tgt Ion: 41 Resp: 4244


Ion Ratio Lower Upper

41 100

69 0.0 62.7 94.1#

39 0.0 52.9 79.3#


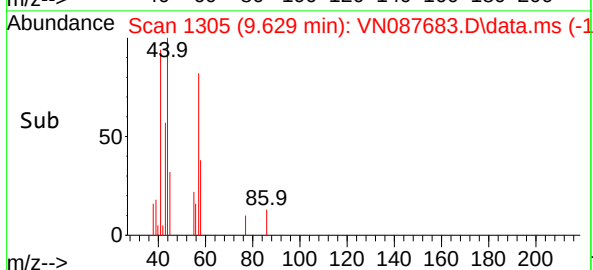

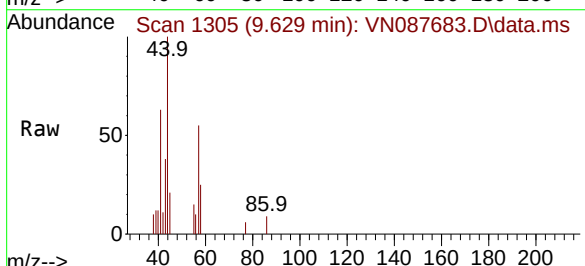




#50
Toluene-d8
Concen: 49.425 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion: 98 Resp: 532406
Ion Ratio Lower Upper
98 100
100 65.1 52.8 79.2

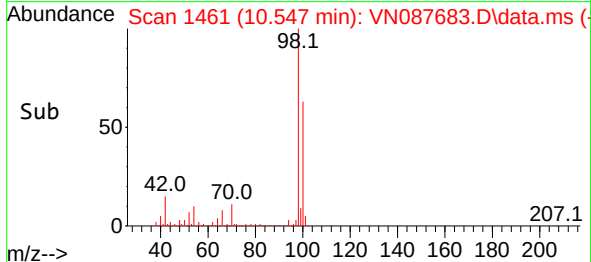

#51
4-Methyl-2-Pentanone
Concen: 1.429 ug/l
RT: 10.424 min Scan# 1440
Delta R.T. -0.000 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion: 43 Resp: 8122
Ion Ratio Lower Upper
43 100
58 54.3 29.6 44.4#


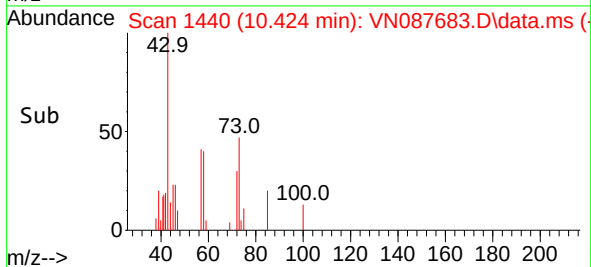

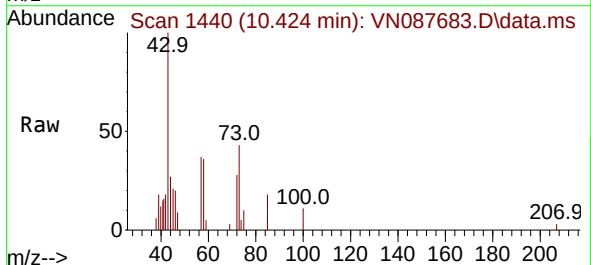




#52
Toluene
Concen: 0.367 ug/l
RT: 10.606 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion: 92 Resp: 3078
Ion Ratio Lower Upper
92 100
91 162.7 140.4 210.6

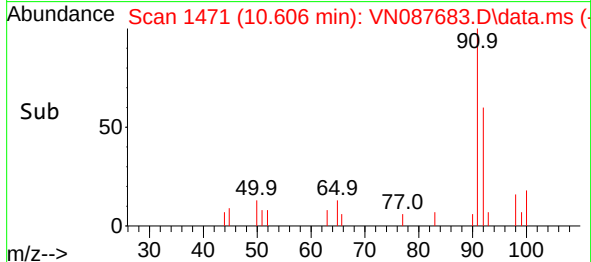

#54
cis-1,3-Dichloropropene
Concen: 11.347 ug/l
RT: 10.341 min Scan# 1426
Delta R.T. 0.053 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion: 75 Resp: 63492
Ion Ratio Lower Upper
75 100
77 0.8 24.6 37.0#
39 41.9 45.2 67.8#

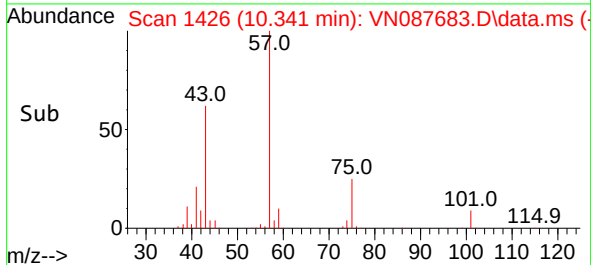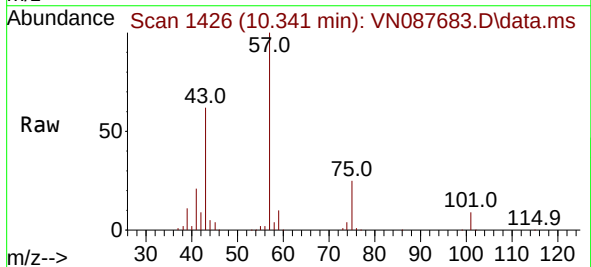

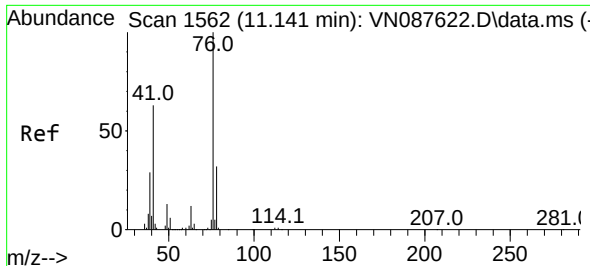

#57

1,3-Dichloropropane

Concen: 0.761 ug/l

RT: 11.194 min Scan# 1571

Delta R.T. 0.053 min

Lab File: VN087683.D

Acq: 28 Aug 2025 14:26

Instrument :

MSVOA_N

ClientSampleId :





NWB-2200

Tgt Ion: 76 Resp: 4375

Ion Ratio Lower Upper

76 100

78 1.2 26.2 39.4#

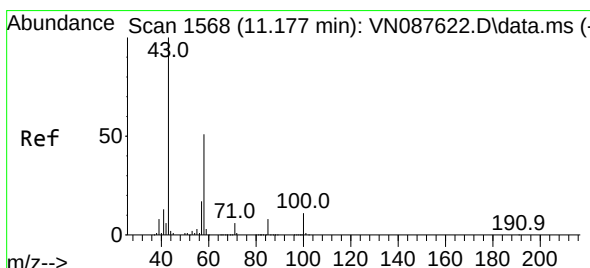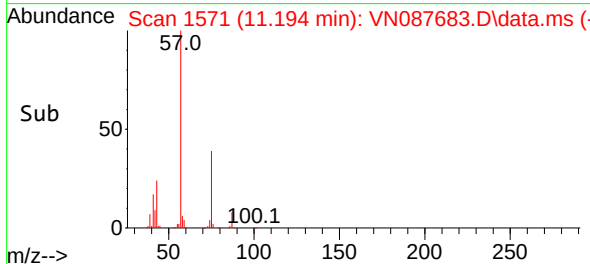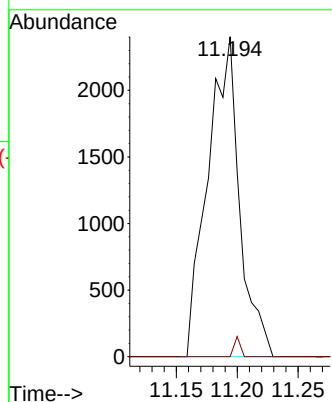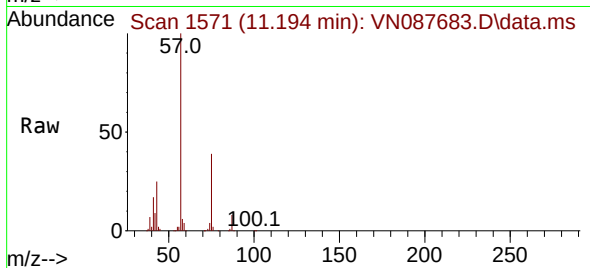

#59

2-Hexanone

Concen: 24.277 ug/l

RT: 11.182 min Scan# 1569

Delta R.T. 0.006 min

Lab File: VN087683.D




Acq: 28 Aug 2025 14:26


Tgt Ion: 43 Resp: 87199

Ion Ratio Lower Upper

43 100

58 17.9 25.9 77.8#


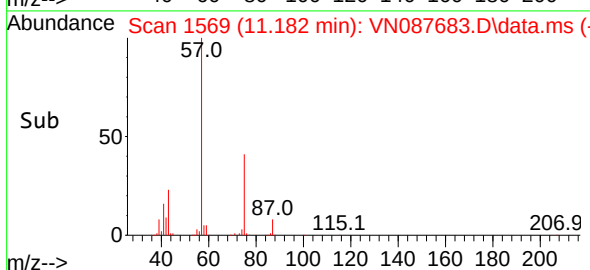

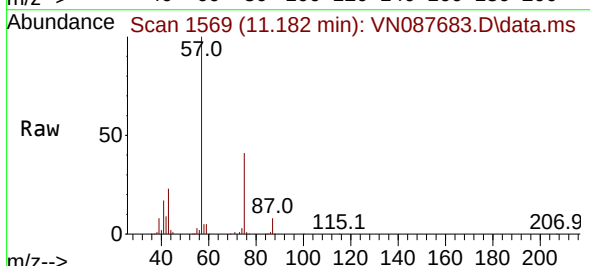




#62
4-Bromofluorobenzene
Concen: 48.995 ug/l
RT: 12.829 min Scan# 1848
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion: 95 Resp: 187691
Ion Ratio Lower Upper
95 100
174 70.9 0.0 138.4
176 67.4 0.0 132.6

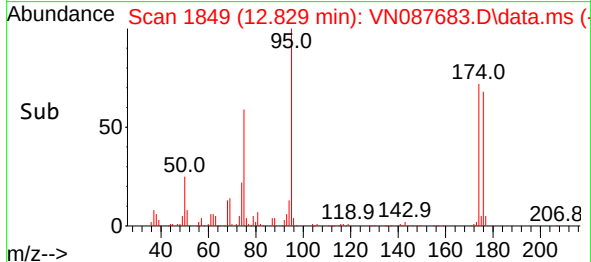

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 1682
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion: 117 Resp: 399523
Ion Ratio Lower Upper
117 100
82 57.8 47.4 71.2
119 33.5 24.3 36.5


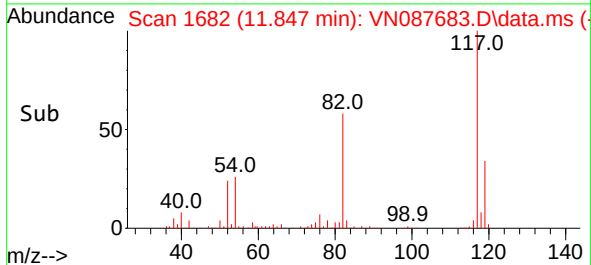

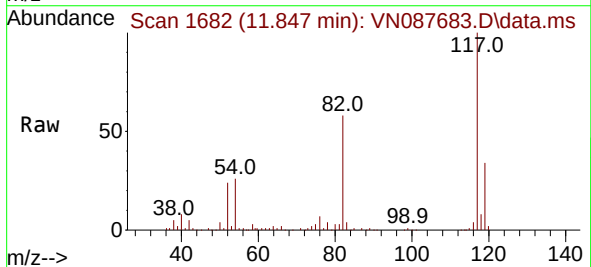




#68
m/p-Xylenes
Concen: 0.265 ug/l
RT: 12.041 min Scan# 1715
Delta R.T. -0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26




Instrument :
MSVOA_N
ClientSampleId :
NWB-2200


Tgt Ion:106 Resp: 1670
Ion Ratio Lower Upper
106 100
91 222.8 169.3 253.9

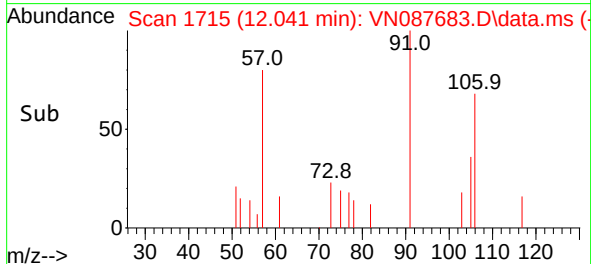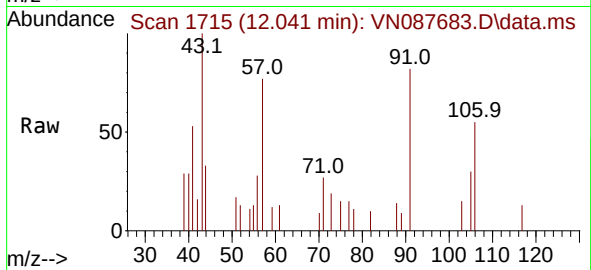

#69
o-Xylene
Concen: 0.214 ug/l
RT: 12.370 min Scan# 1771
Delta R.T. -0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26


Tgt Ion:106 Resp: 1323
Ion Ratio Lower Upper
106 100
91 169.0 111.4 334.2

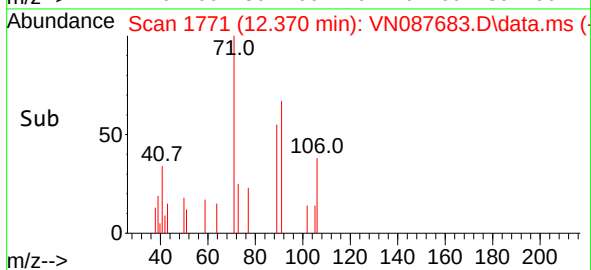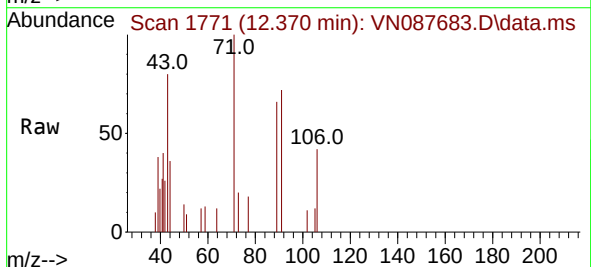






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2008
Delta R.T. 0.006 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Instrument :
MSVOA_N
ClientSampleId :
NWB-2200



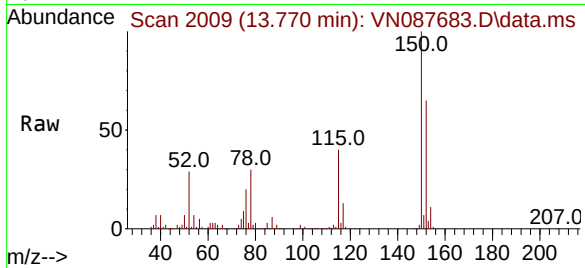



Tgt Ion:152 Resp: 179426
Ion Ratio Lower Upper
152 100
115 65.0 32.3 96.8
150 159.9 0.0 351.0

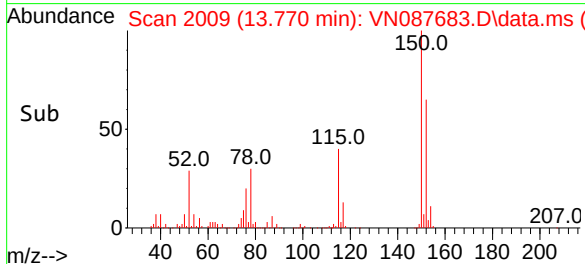

#76
1,2,3-Trichloropropane
Concen: 26.404 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. -0.141 min
Lab File: VN087683.D
Acq: 28 Aug 2025 14:26

Tgt Ion: 75 Resp: 111097
Ion Ratio Lower Upper
75 100
77 1.0 89.1 267.4#


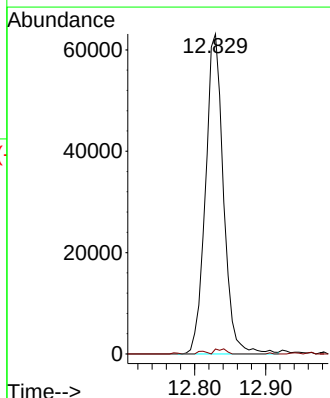

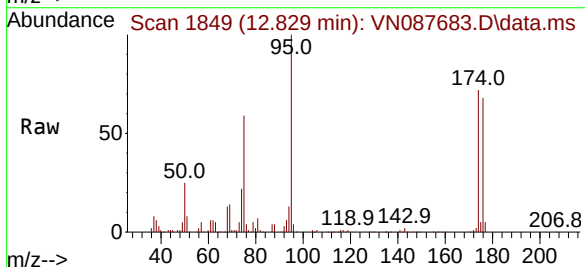


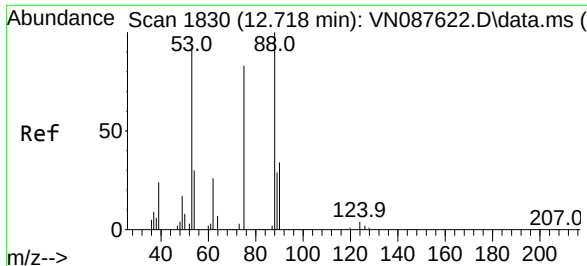

#81
 trans-1,4-Dichloro-2-butene
 Concen: 69.901 ug/l
 RT: 12.829 min Scan# 111097
 Delta R.T. 0.112 min
 Lab File: VN087683.D
 Acq: 28 Aug 2025 14:26

Instrument :
 MSVOA_N
 ClientSampleId :
 NWB-2200

Tgt Ion: 75 Resp: 111097
 Ion Ratio Lower Upper
 75 100
 53 0.1 101.8 152.6#
 89 0.0 35.6 53.4#

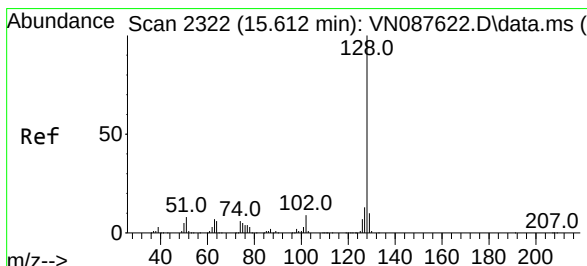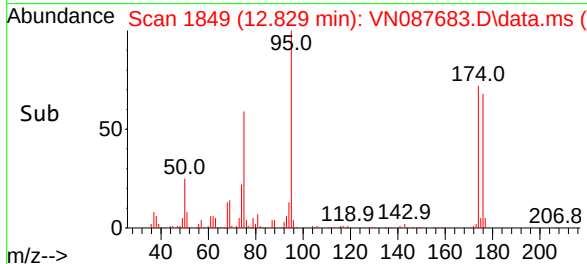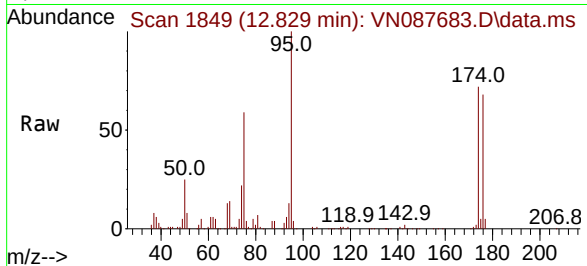

#95
 Naphthalene
 Concen: 1.315 ug/l
 RT: 15.611 min Scan# 2322
 Delta R.T. -0.000 min
 Lab File: VN087683.D
 Acq: 28 Aug 2025 14:26

Tgt Ion: 128 Resp: 17867
 Ion Ratio Lower Upper
 128 100
 127 13.9 10.6 15.8
 129 13.6 8.6 12.8#

