

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082825\
 Data File : VN087690.D
 Acq On : 28 Aug 2025 16:53
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Aug 29 03:21:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 22 02:55:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	196862	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	462634	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.841	117	440525	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	200991	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.565	65	219841	54.504	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.000%
35) Dibromofluoromethane	8.153	113	167798	50.236	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.480%
50) Toluene-d8	10.547	98	605594	48.441	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	96.880%
62) 4-Bromofluorobenzene	12.829	95	206000	46.333	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	92.660%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082825\
Data File : VN087690.D
Acq On : 28 Aug 2025 16:53
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Aug 29 03:21:47 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082125W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 22 02:55:42 2025
Response via : Initial Calibration




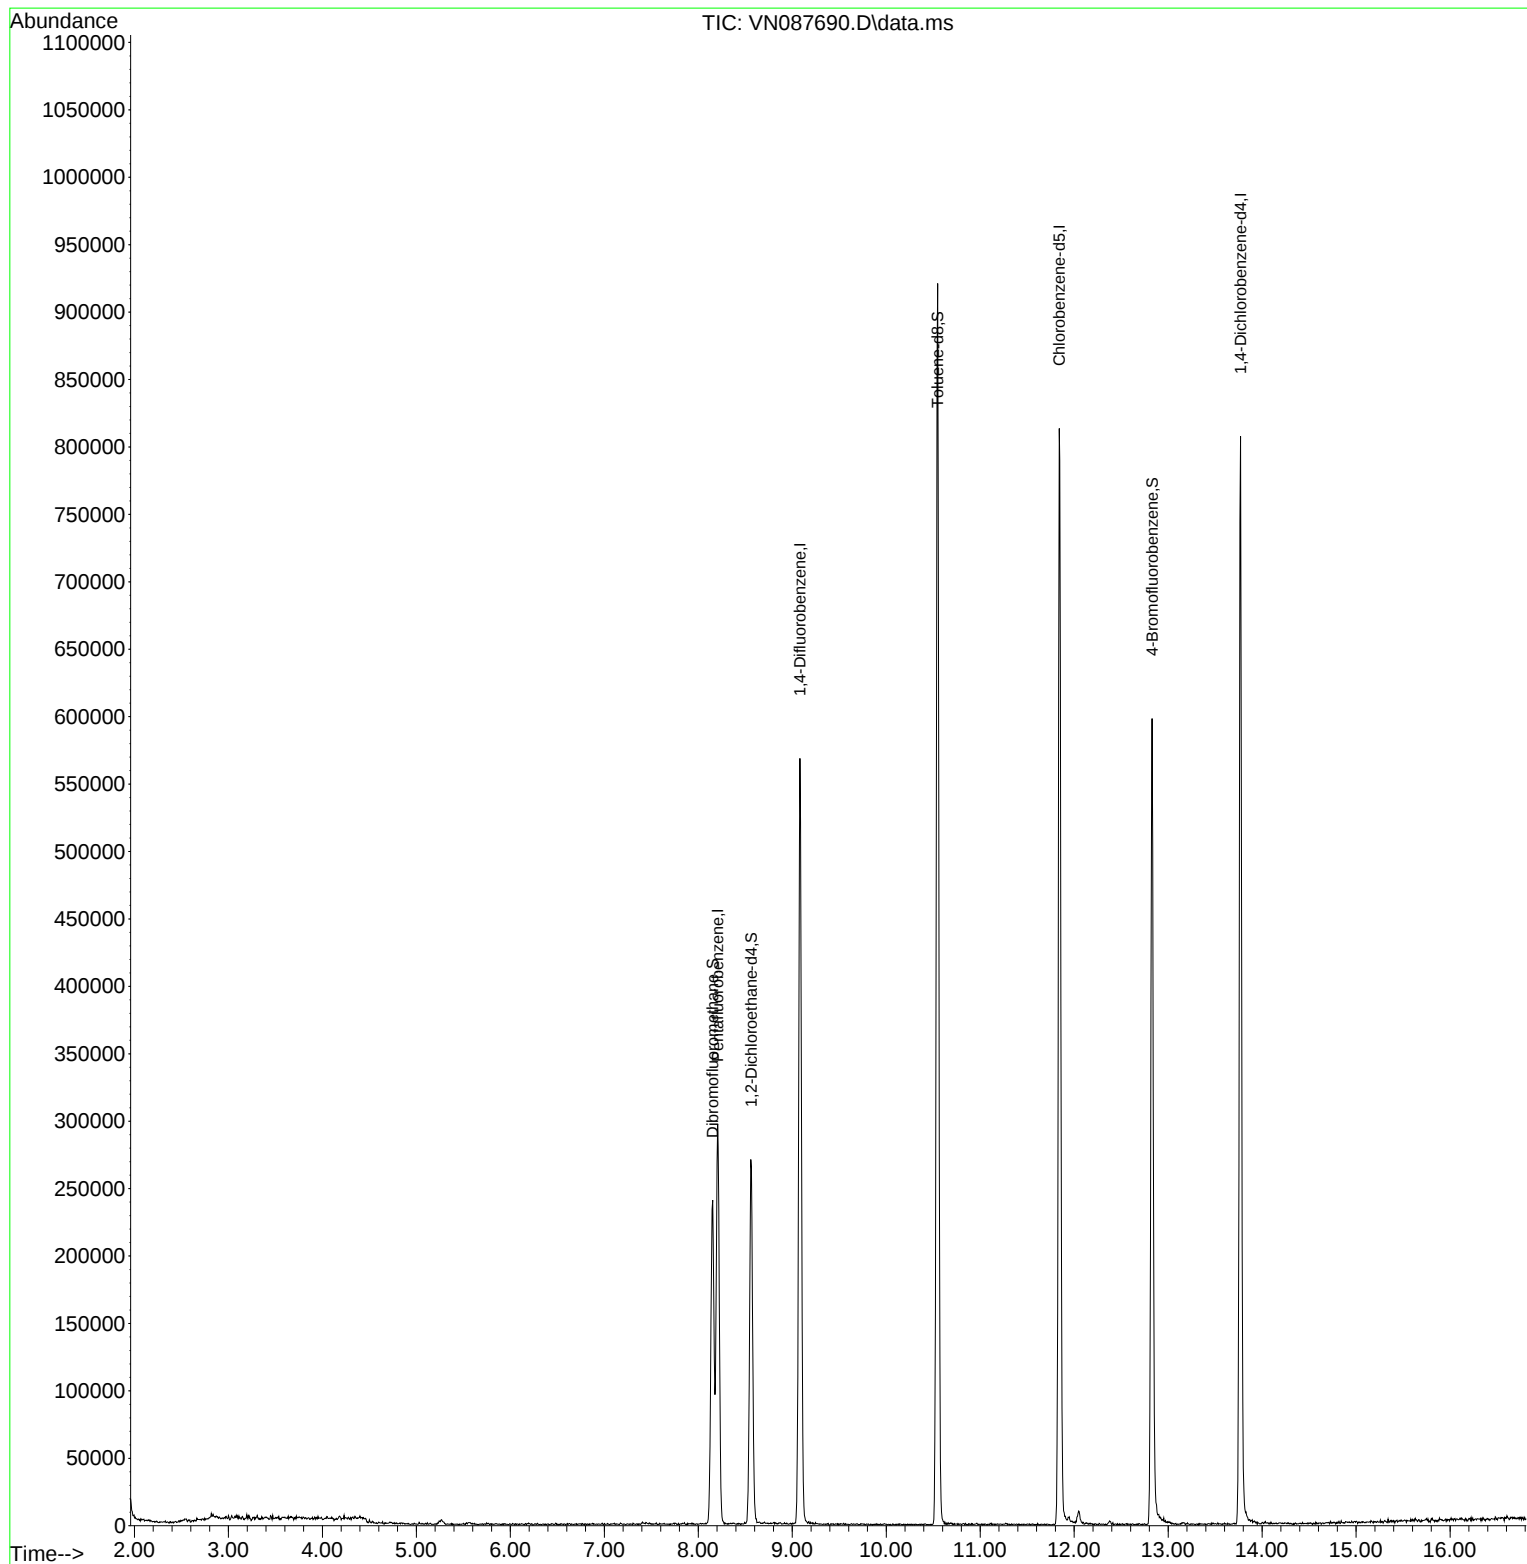


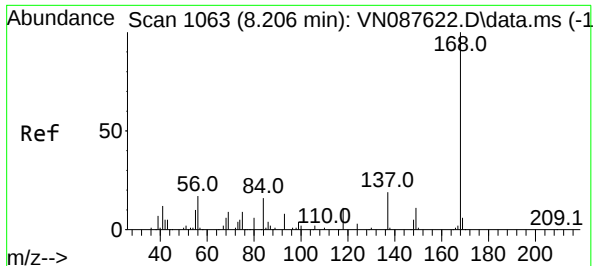

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. 0.000 min
Lab File: VN087690.D
Acq: 28 Aug 2025 16:53




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 196862
Ion Ratio Lower Upper
168 100
99 64.7 57.2 85.8

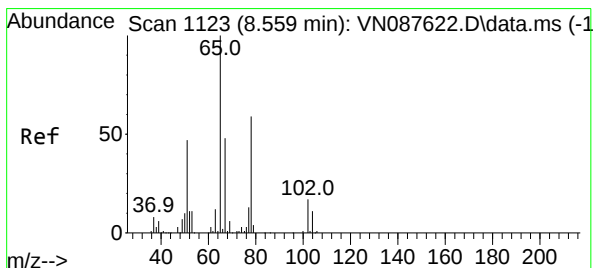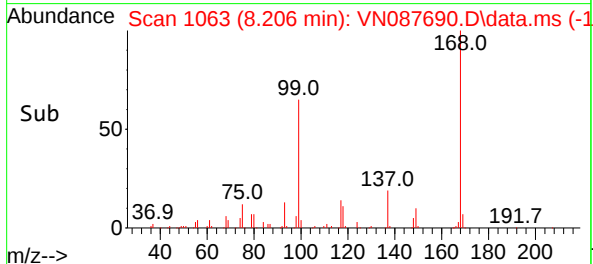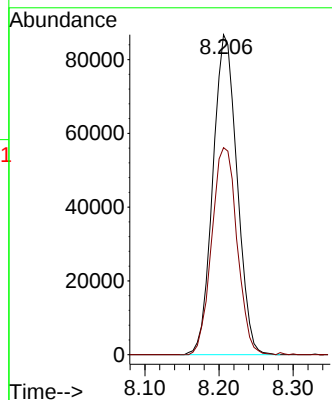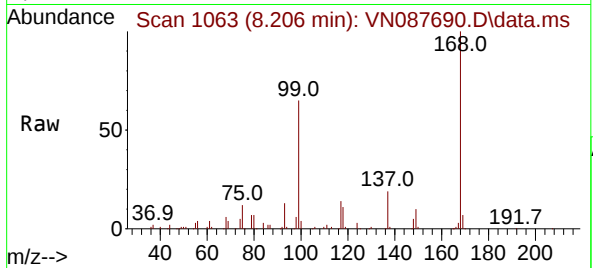

#33
1,2-Dichloroethane-d4
Concen: 54.504 ug/l
RT: 8.565 min Scan# 1124
Delta R.T. 0.006 min
Lab File: VN087690.D
Acq: 28 Aug 2025 16:53

Tgt Ion: 65 Resp: 219841
Ion Ratio Lower Upper
65 100
67 51.8 0.0 100.0


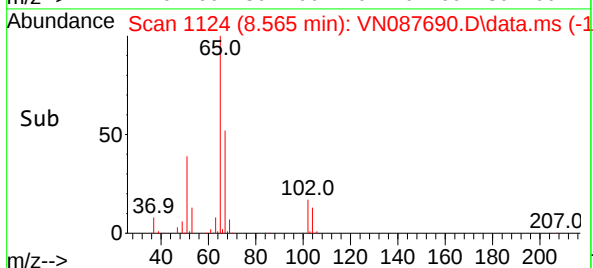
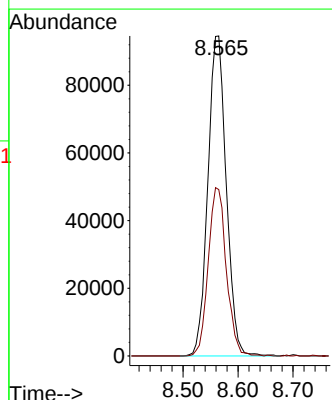
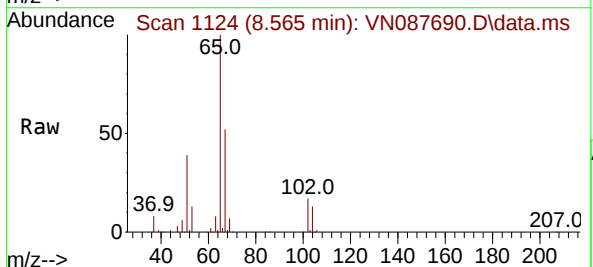


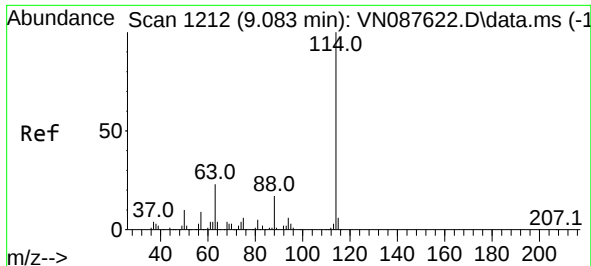

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.082 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN087690.D
Acq: 28 Aug 2025 16:53




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 462634
Ion Ratio Lower Upper
114 100
63 23.6 0.0 45.2
88 15.9 0.0 33.4

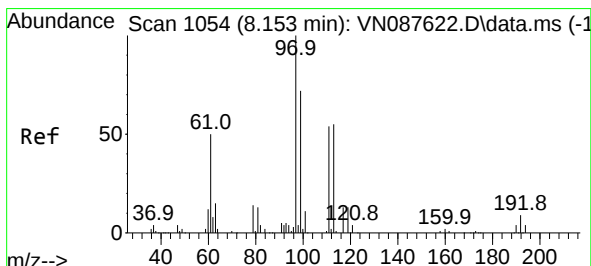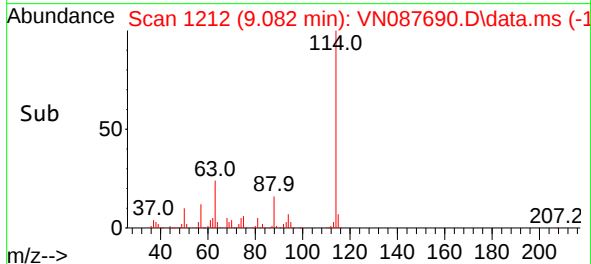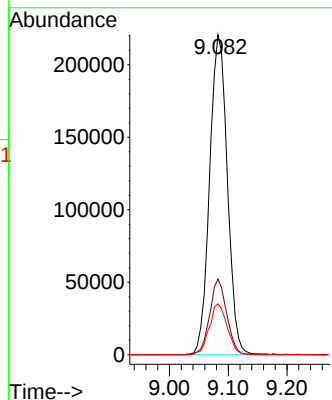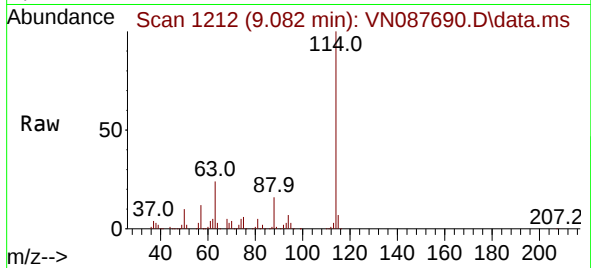

#35
Dibromofluoromethane
Concen: 50.236 ug/l
RT: 8.153 min Scan# 1054
Delta R.T. -0.000 min
Lab File: VN087690.D
Acq: 28 Aug 2025 16:53

Tgt Ion:113 Resp: 167798
Ion Ratio Lower Upper
113 100
111 104.6 82.8 124.2
192 16.4 12.8 19.2


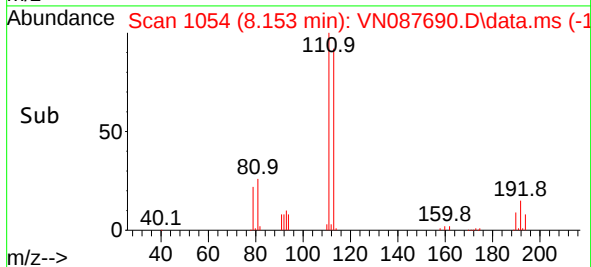
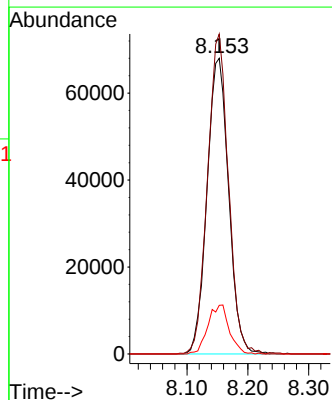
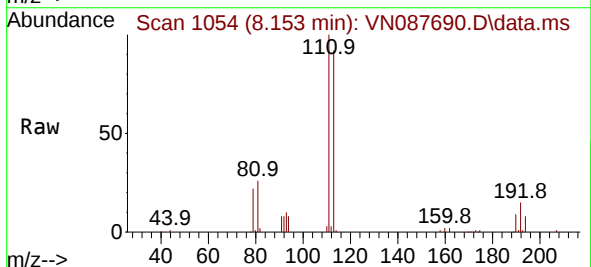


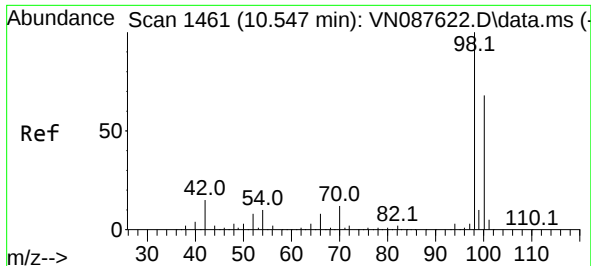

#50
Toluene-d8
Concen: 48.441 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087690.D
Acq: 28 Aug 2025 16:53




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 605594
Ion Ratio Lower Upper
98 100
100 64.1 52.8 79.2

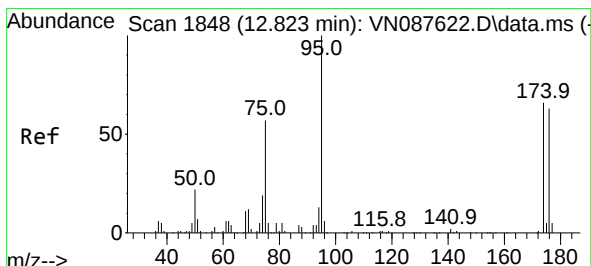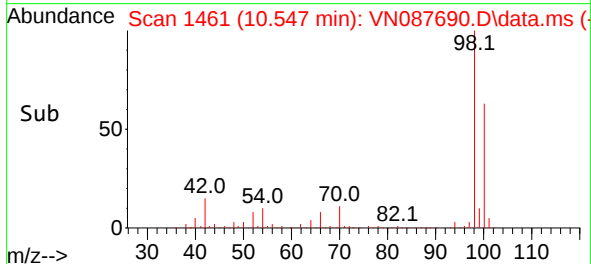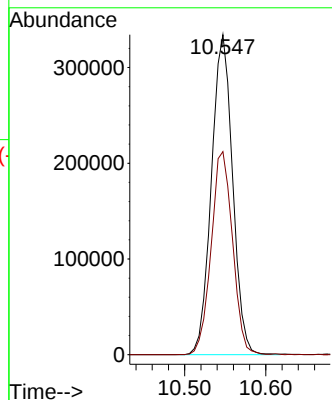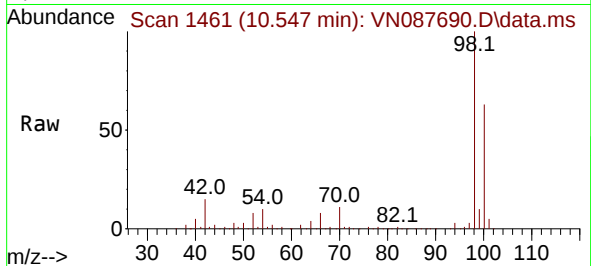

#62
4-Bromofluorobenzene
Concen: 46.333 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN087690.D
Acq: 28 Aug 2025 16:53

Tgt Ion: 95 Resp: 206000
Ion Ratio Lower Upper
95 100
174 69.8 0.0 138.4
176 67.9 0.0 132.6


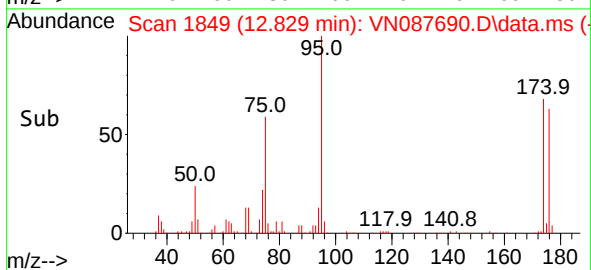
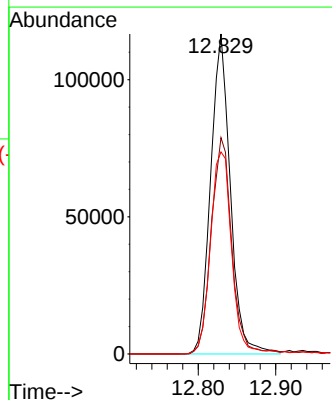
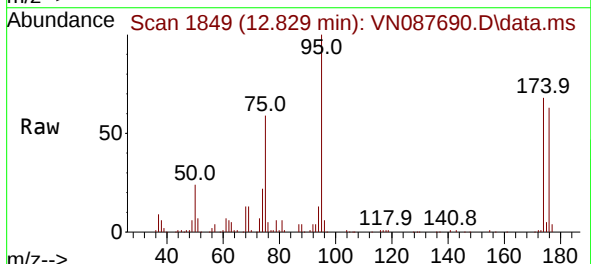


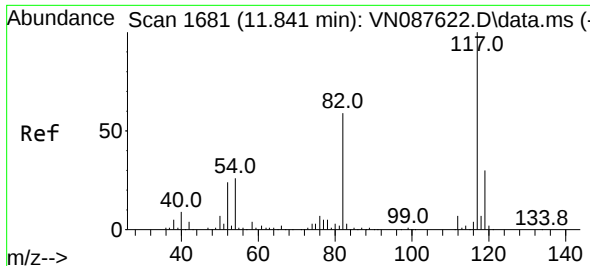

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.841 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN087690.D
Acq: 28 Aug 2025 16:53

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 440525
Ion Ratio Lower Upper
117 100
82 57.7 47.4 71.2
119 29.2 24.3 36.5

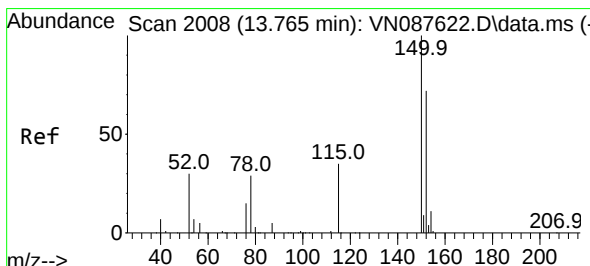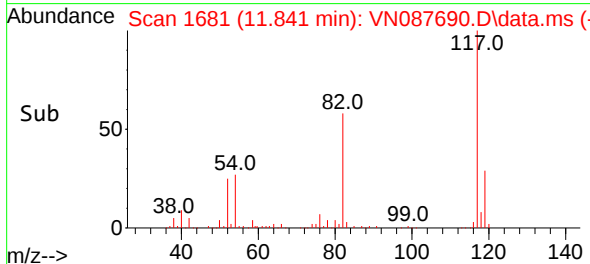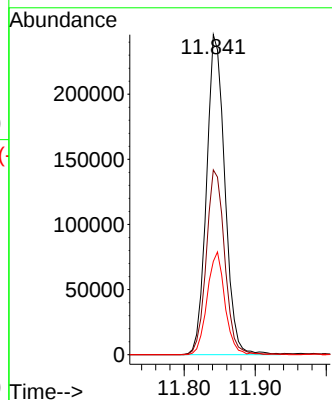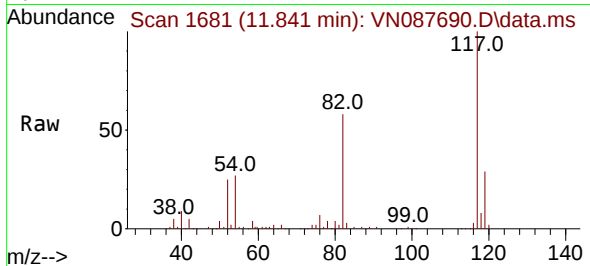

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN087690.D
Acq: 28 Aug 2025 16:53

Tgt Ion:152 Resp: 200991
Ion Ratio Lower Upper
152 100
115 63.3 32.3 96.8
150 161.5 0.0 351.0

