

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN082918\
 Data File : VN050936.D
 Acq On : 29 Aug 2018 9:04
 Operator : MD\SY
 Sample : VN0829MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0829MBL01

Quant Time: Aug 29 14:44:58 2018
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 22 05:38:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	627145	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	982503	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	818616	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	236748	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	397553	52.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.32%	
35) Dibromofluoromethane	7.59	113	383387	49.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.10%	
50) Toluene-d8	10.09	98	1362467	46.62	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.24%	
62) 4-Bromofluorobenzene	12.40	95	338239	34.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	69.66%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN082918\
Data File : VN050936.D
Acq On : 29 Aug 2018 9:04
Operator : MD\SY
Sample : VN0829MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0829MBL01

Quant Time: Aug 29 14:44:58 2018
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 22 05:38:12 2018
Response via : Initial Calibration




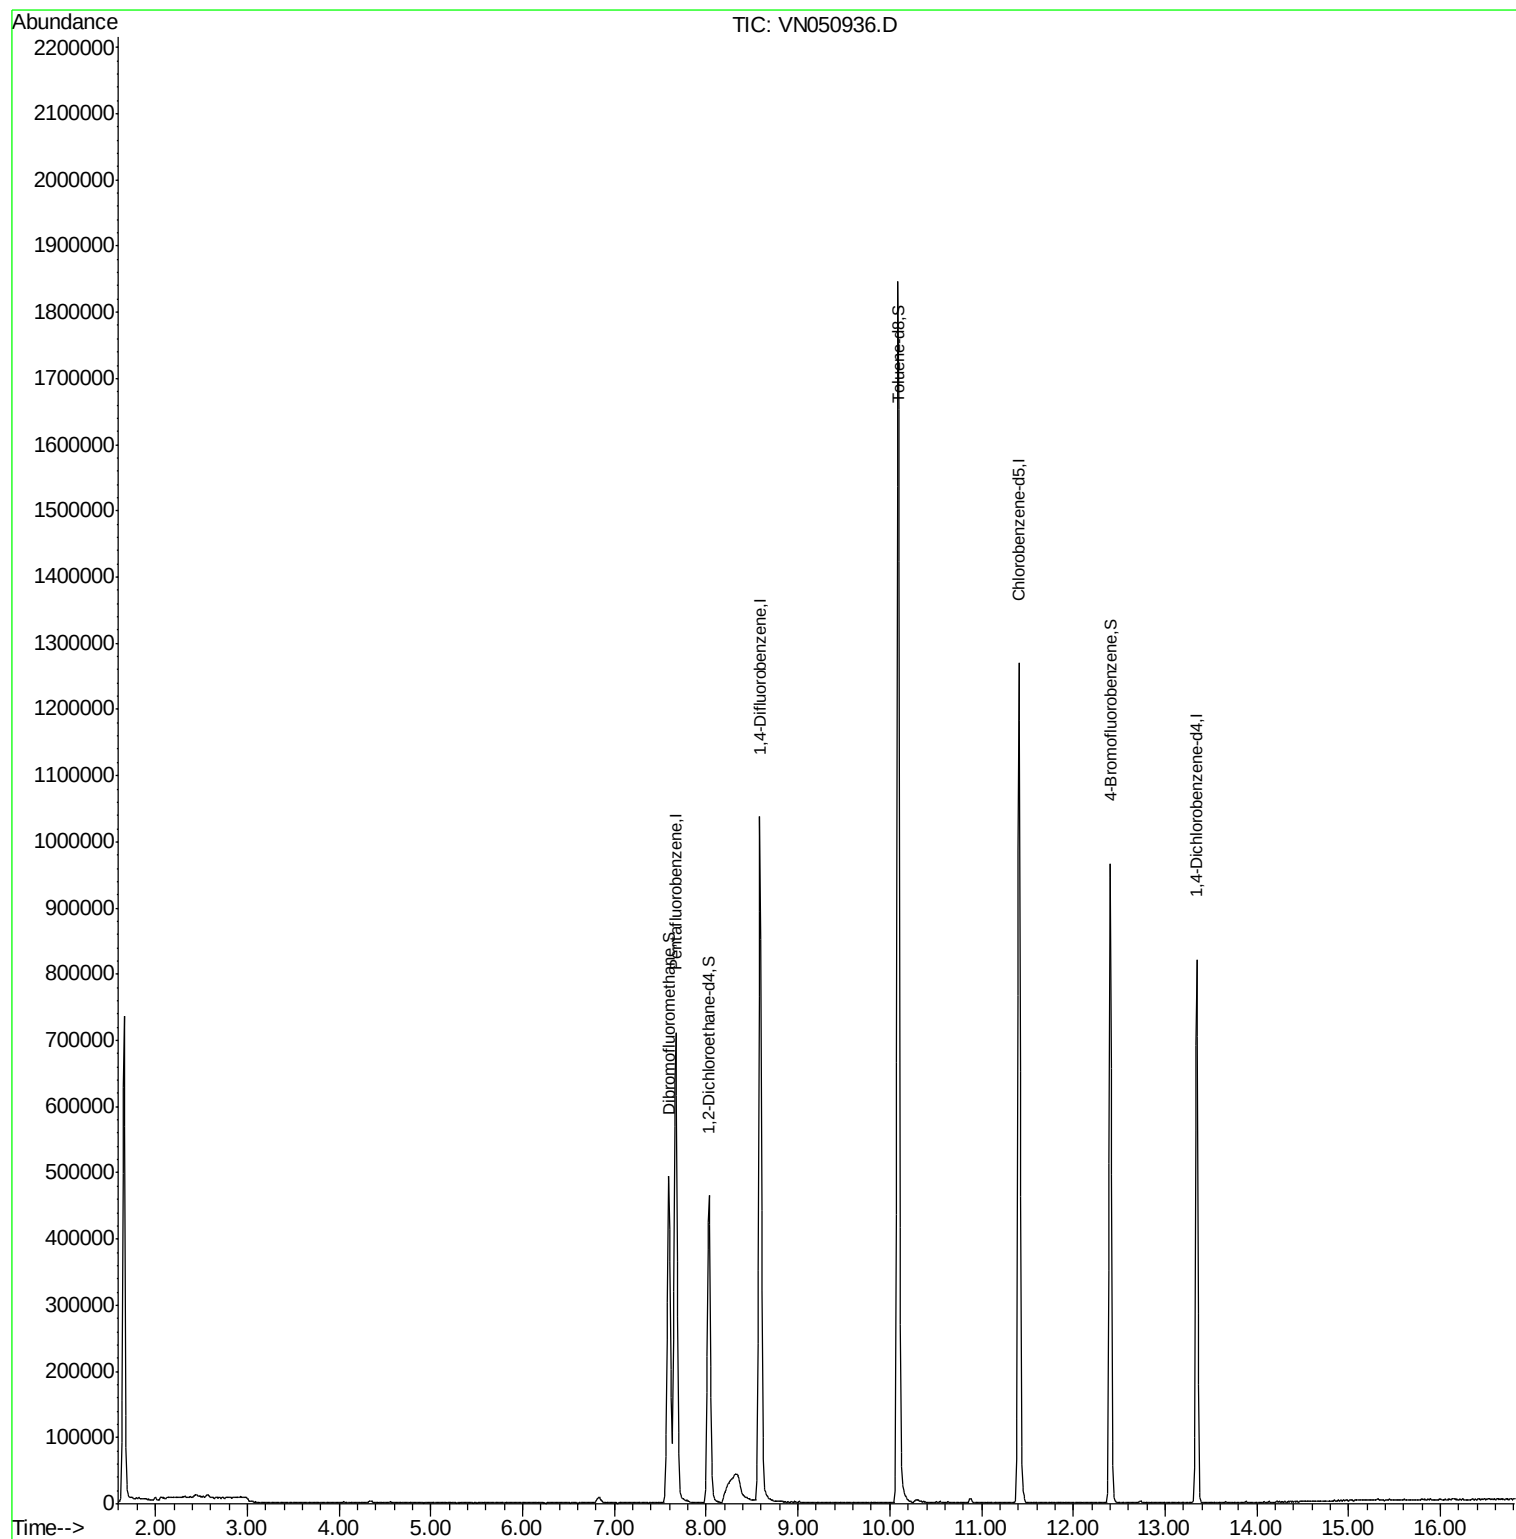


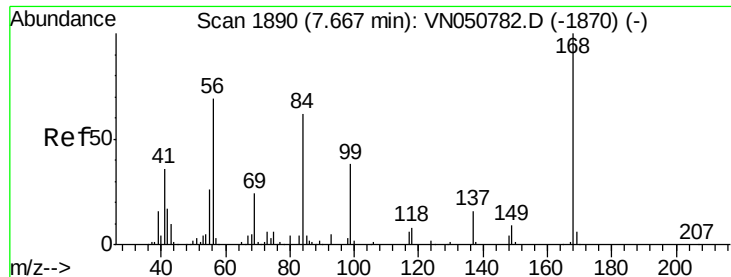

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.67 min Scan# 1890
Delta R.T. 0.00 min
Lab File: VN050936.D
Acq: 29 Aug 2018 9:04




Instrument :
MSVOA_N
ClientSampleId :
VN0829MBL01


Tot Ion:168 Resp: 627145
Ion Ratio Lower Upper
168 100
99 48.8 39.6 59.4

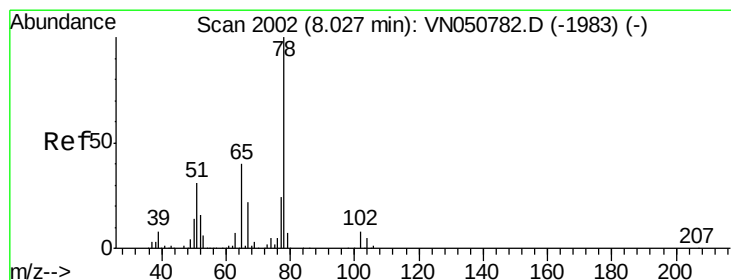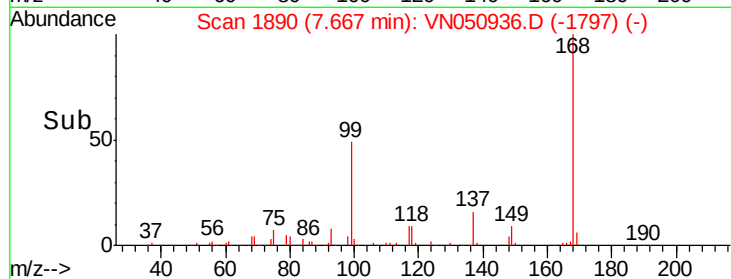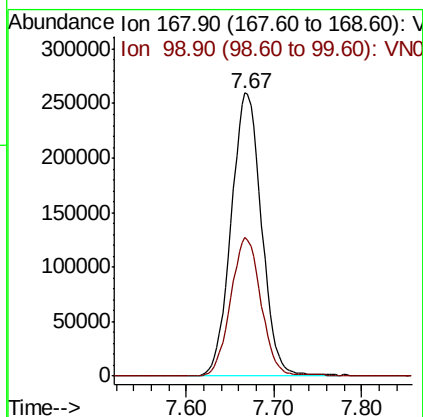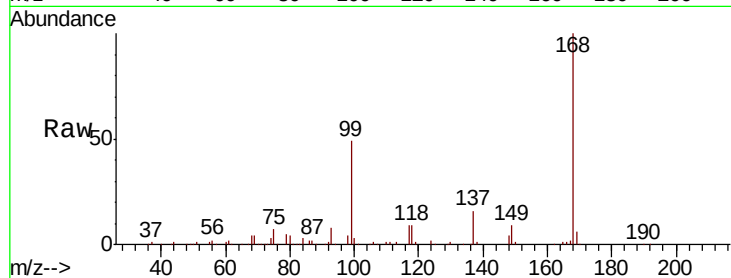

#33
1,2-Dichloroethane-d4
Concen: 52.656 ug/l
RT: 8.03 min Scan# 2003
Delta R.T. 0.00 min
Lab File: VN050936.D
Acq: 29 Aug 2018 9:04

Tgt Ion: 65 Resp: 397553
Ion Ratio Lower Upper
65 100
67 54.3 0.0 110.4

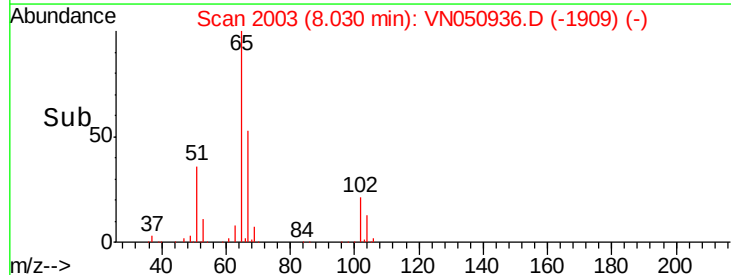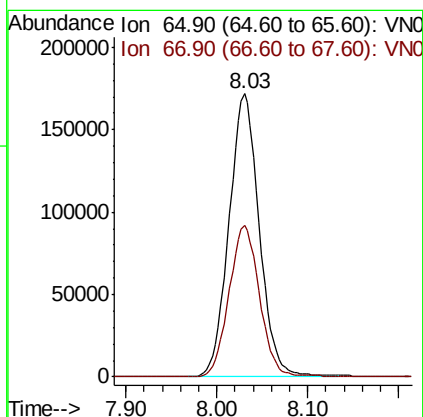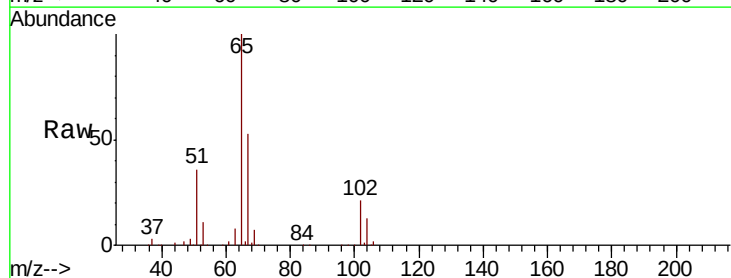


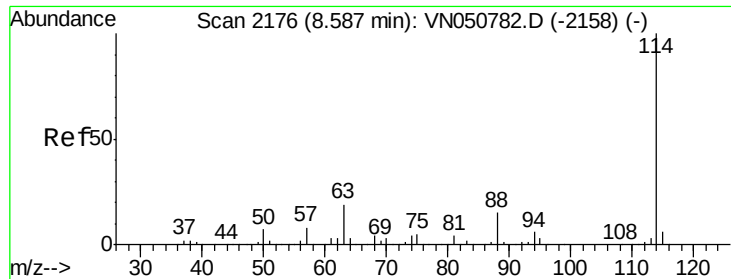




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2176
 Delta R.T. 0.00 min
 Lab File: VN050936.D
 Acq: 29 Aug 2018 9:04

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0829MBL01

Tot Ion	Ratio	Lower	Upper
114	100		
63	19.8	0.0	38.6
88	15.9	0.0	30.6

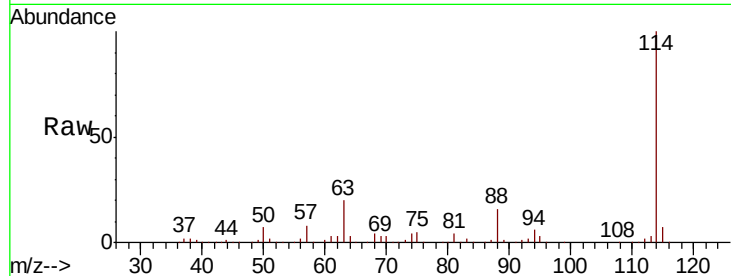


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

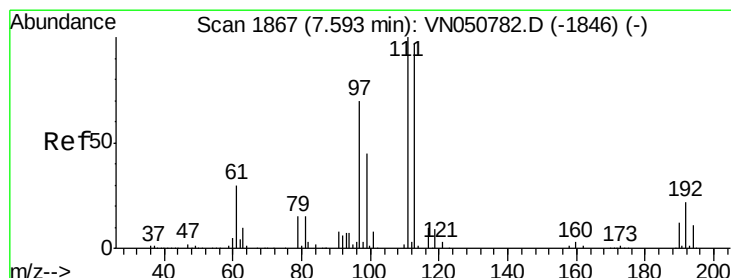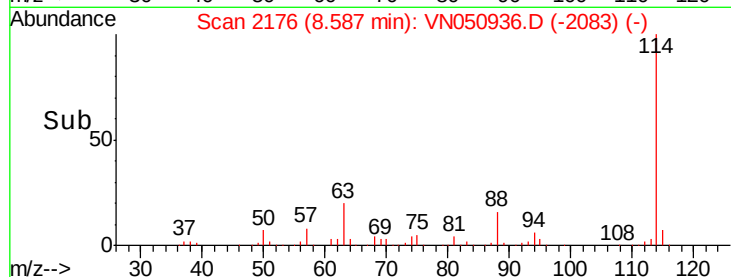
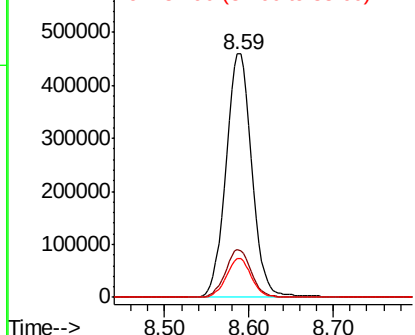



#35
 Dibromofluoromethane
 Concen: 49.049 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN050936.D
 Acq: 29 Aug 2018 9:04

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.1	82.6	123.8
192	22.8	18.0	27.0

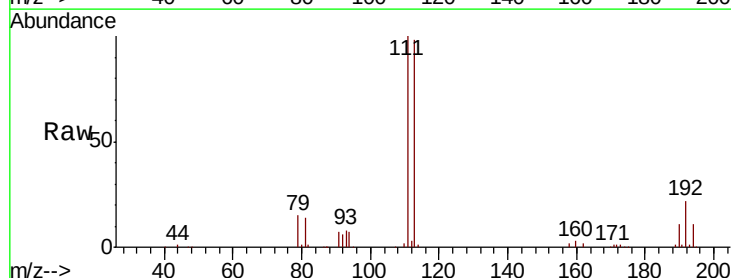

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

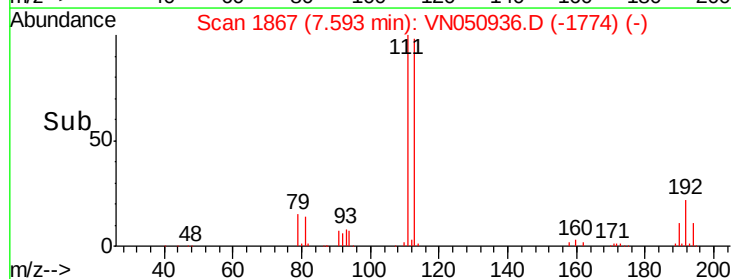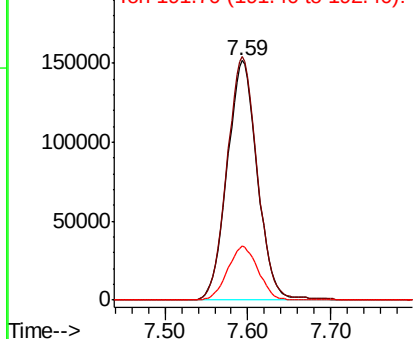

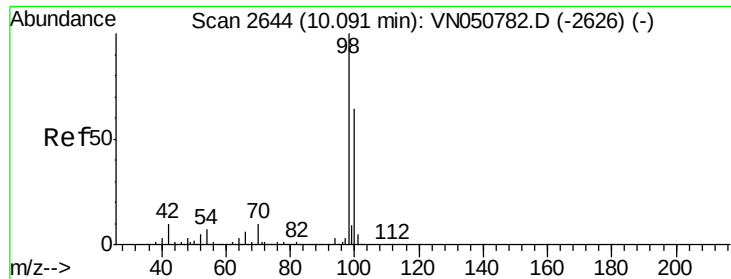

#50

Toluene-d8

Concen: 46.623 ug/l

RT: 10.09 min Scan# 2644

Delta R.T. 0.00 min

Lab File: VN050936.D

Acq: 29 Aug 2018 9:04

Instrument :

MSVOA_N

ClientSampleId :





VN0829MBL01

Tot Ion: 98 Resp: 1362467

Ion Ratio Lower Upper

98 100

100 63.4 51.5 77.3

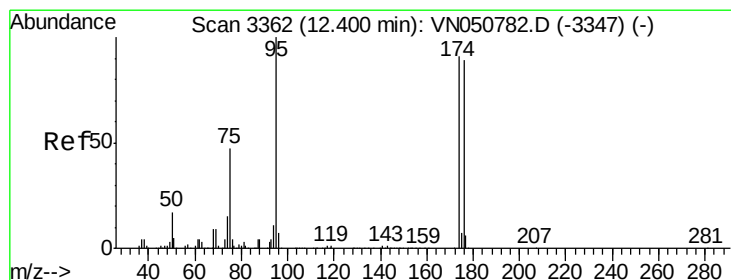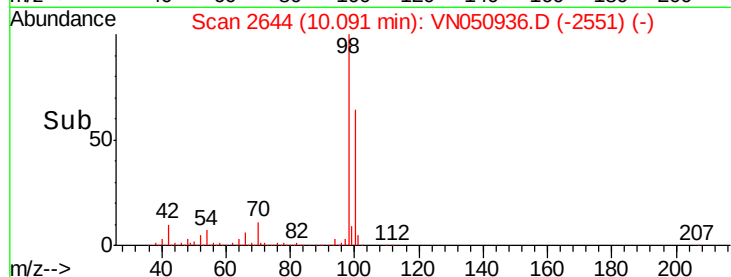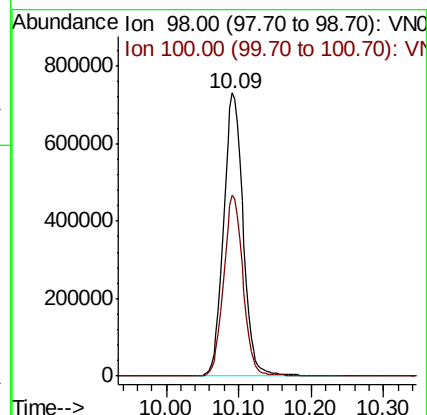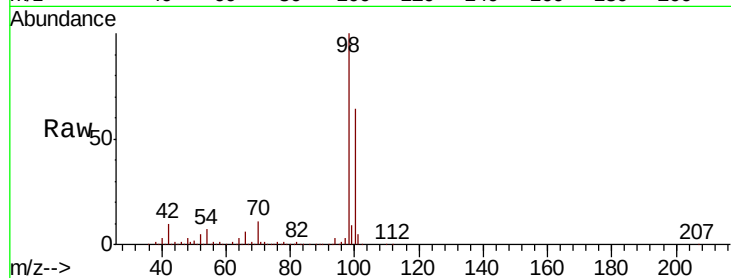

#62

4-Bromofluorobenzene

Concen: 34.831 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN050936.D

Acq: 29 Aug 2018 9:04




Tgt Ion: 95 Resp: 338239


Ion Ratio Lower Upper

95 100

174 92.8 0.0 183.0

176 88.3 0.0 178.8

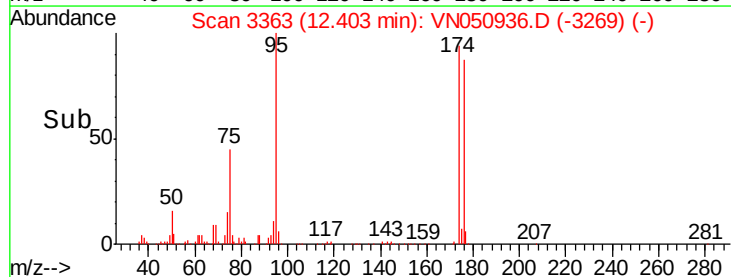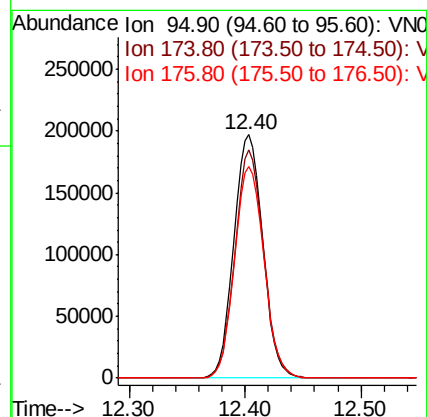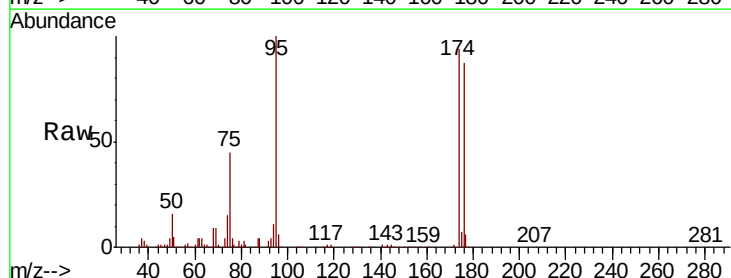


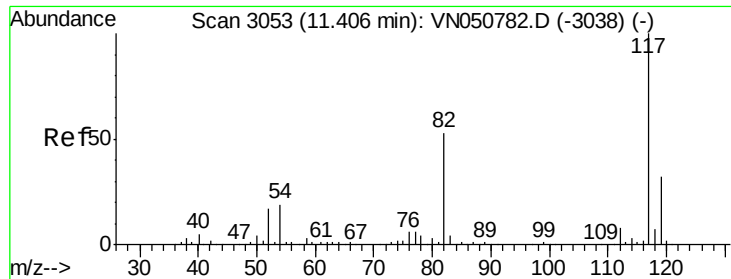




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. 0.00 min
Lab File: VN050936.D
Acq: 29 Aug 2018 9:04

Instrument :
MSVOA_N
ClientSampleId :
VN0829MBL01

Tot Ion:117 Resp: 818616
Ion Ratio Lower Upper
117 100
82 52.6 42.6 64.0
119 33.0 25.8 38.6

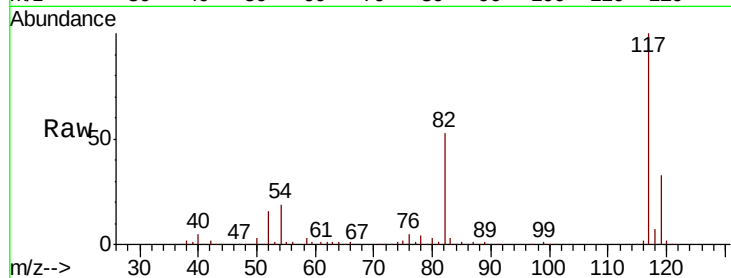


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V

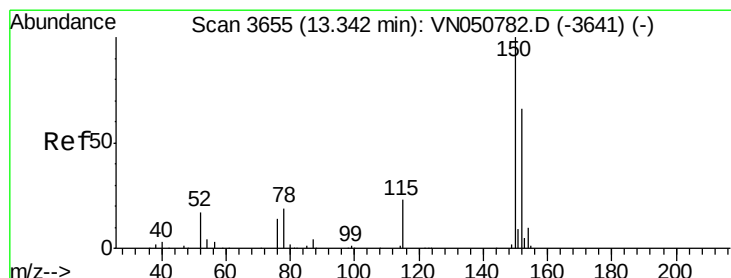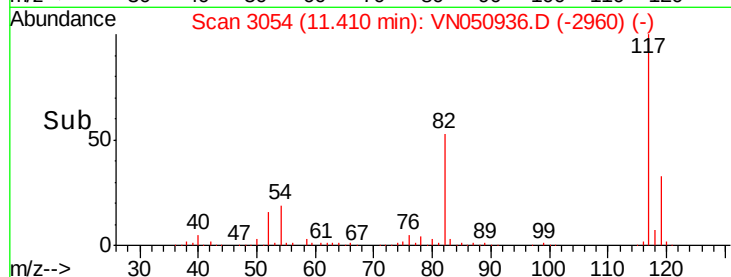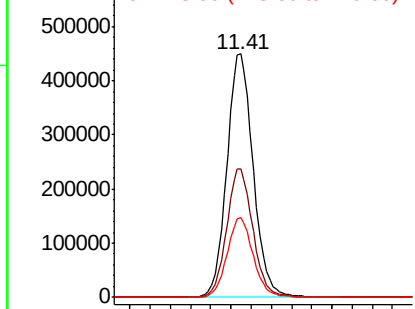

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3656
Delta R.T. 0.00 min
Lab File: VN050936.D
Acq: 29 Aug 2018 9:04

Tgt Ion:152 Resp: 236748
Ion Ratio Lower Upper
152 100
115 56.3 27.8 83.4
150 158.9 0.0 351.4

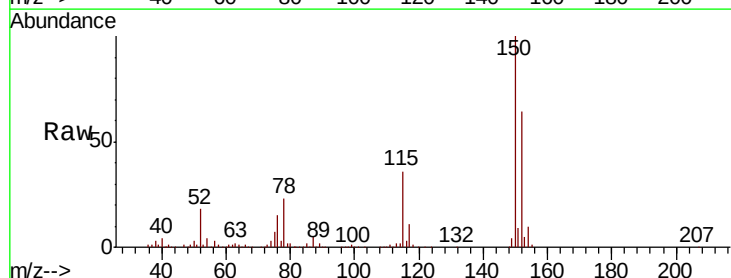

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

