



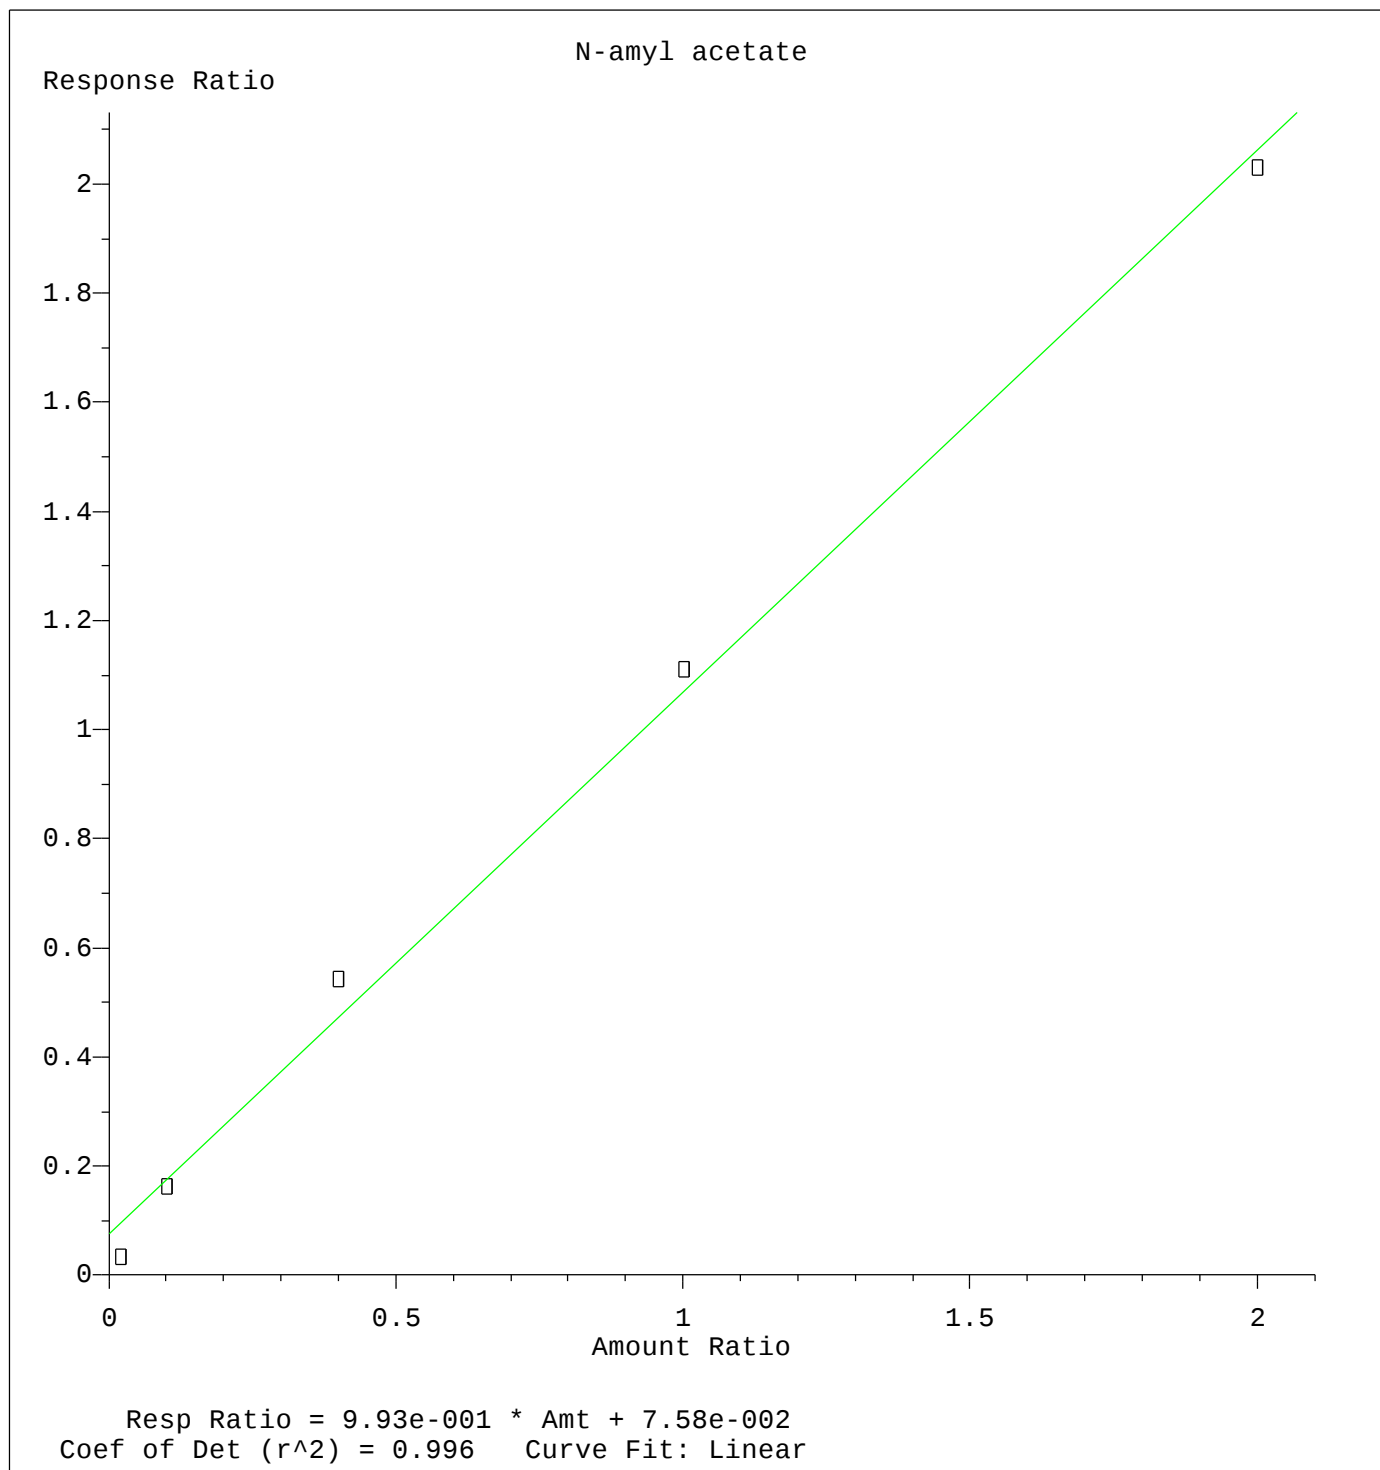

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N082919W.M  
Calibration Table Last Updated: Fri Aug 30 11:59:03 2019

1,1,2,2-Tetrachloroethane

Response Ratio

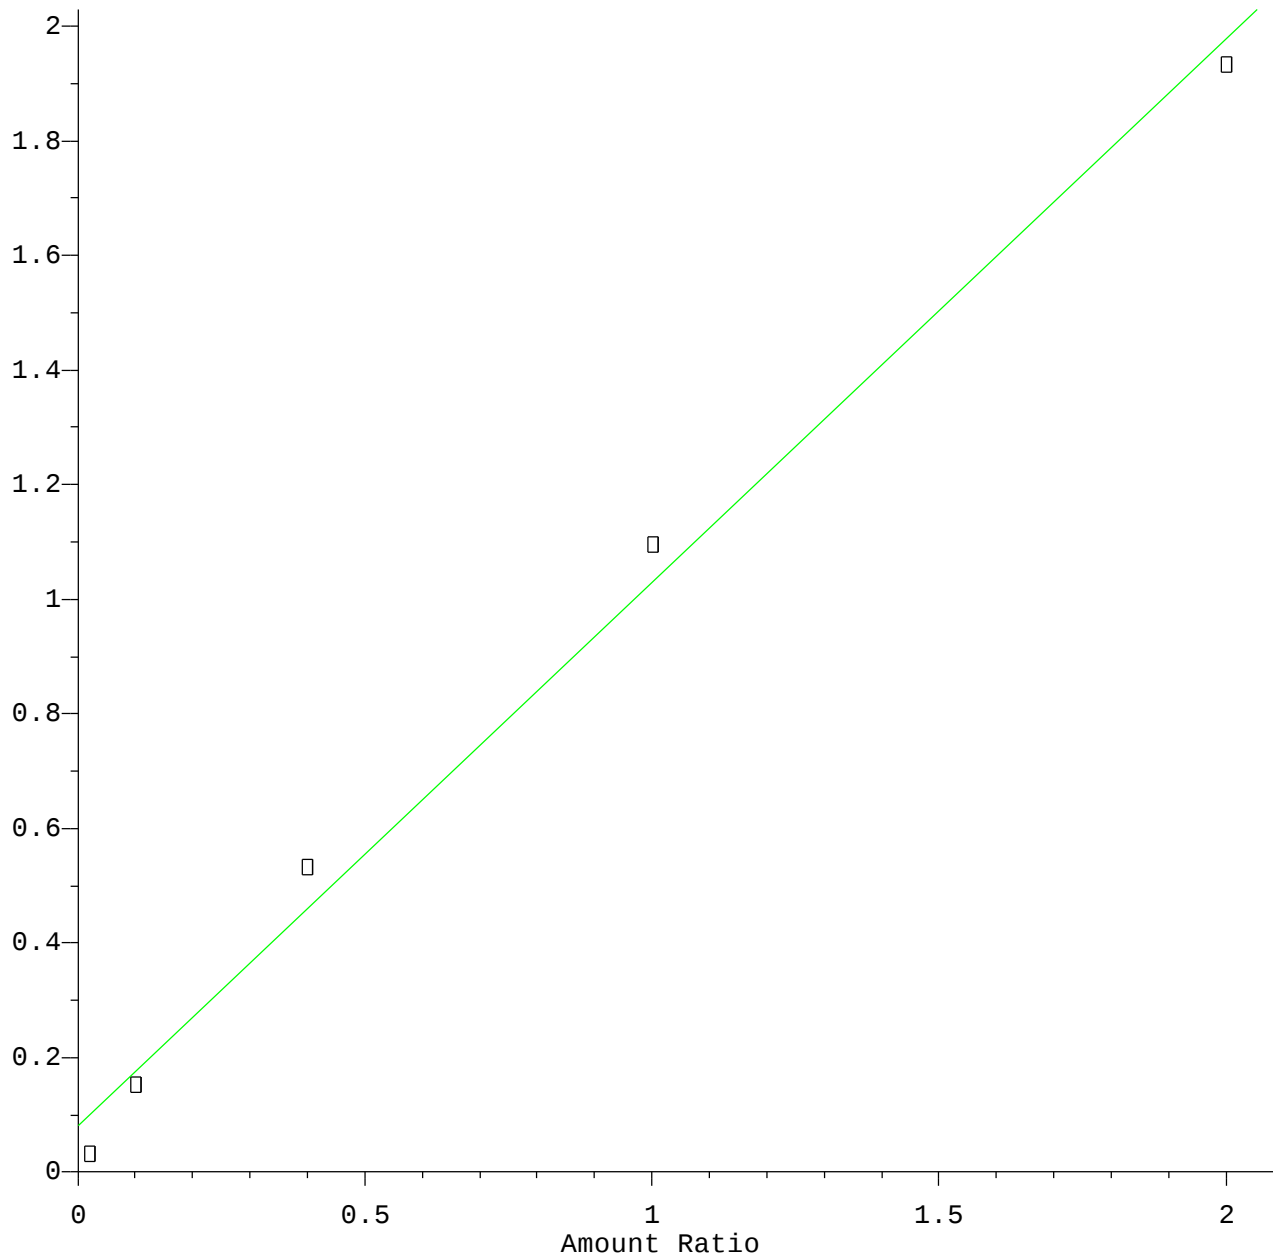


Resp Ratio =  $9.48 \times 10^{-1} \times \text{Amt} + 8.09 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.993    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N082919W.M  
Calibration Table Last Updated: Fri Aug 30 11:59:03 2019

# 1,2,3-Trichloropropane

Response Ratio

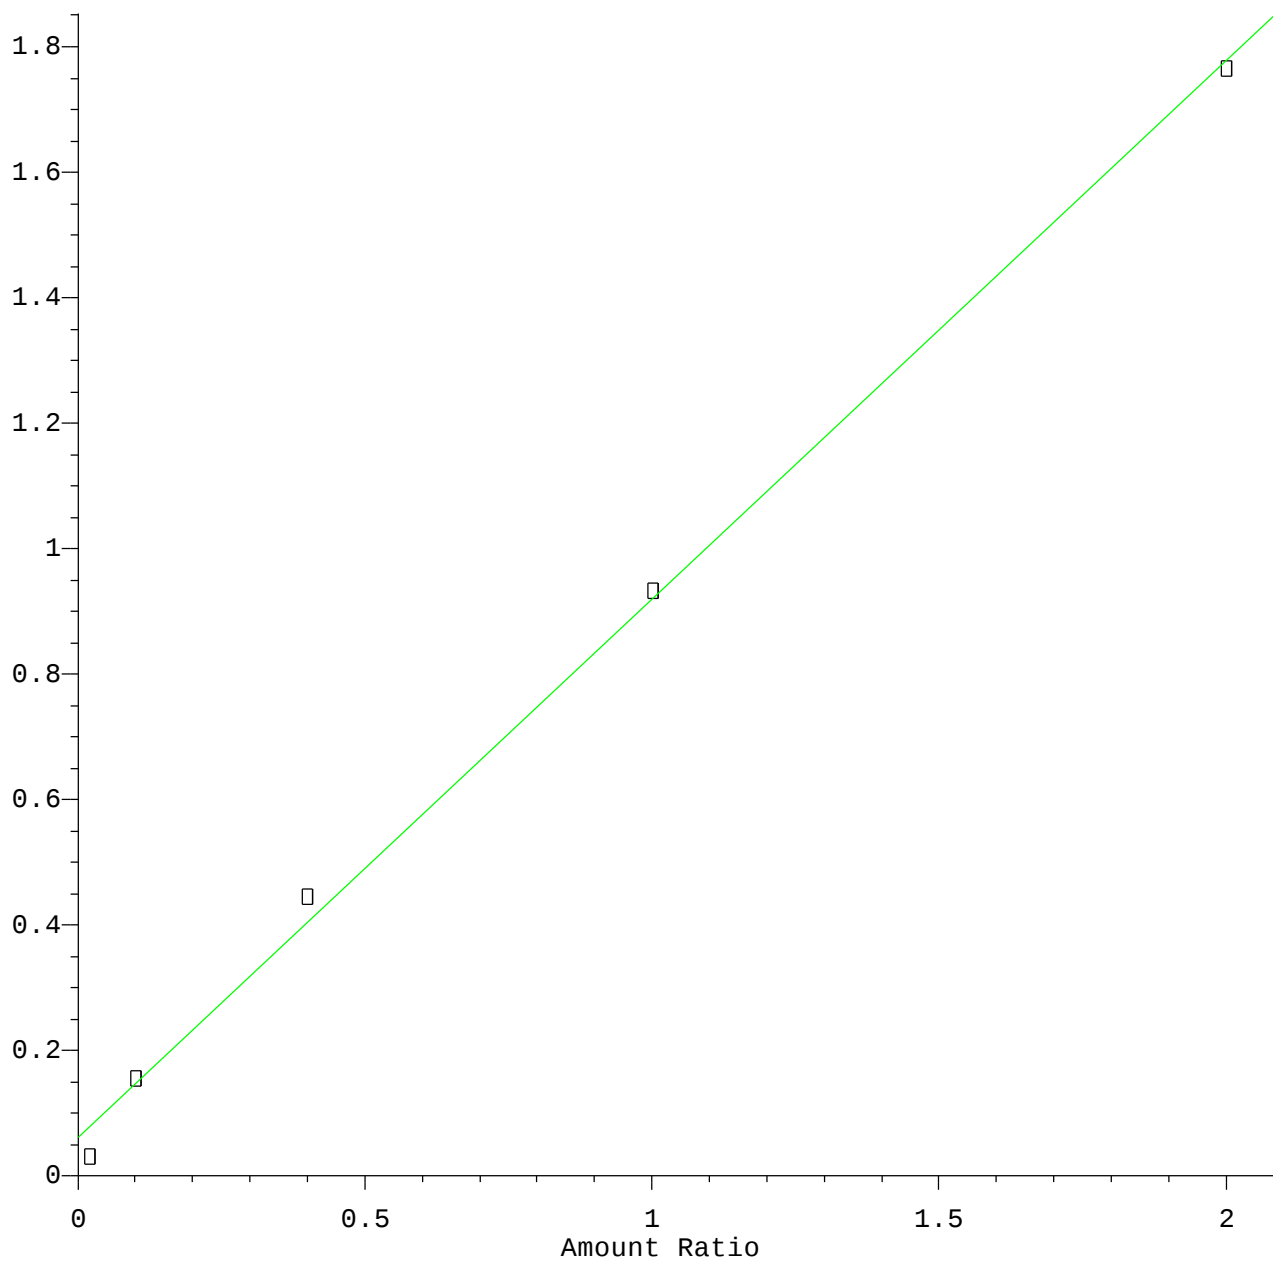


Resp Ratio =  $8.59 \times 10^{-1} \times \text{Amt} + 6.05 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.998    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N082919W.M  
Calibration Table Last Updated: Fri Aug 30 11:59:03 2019


tert-Butylbenzene

Response Ratio

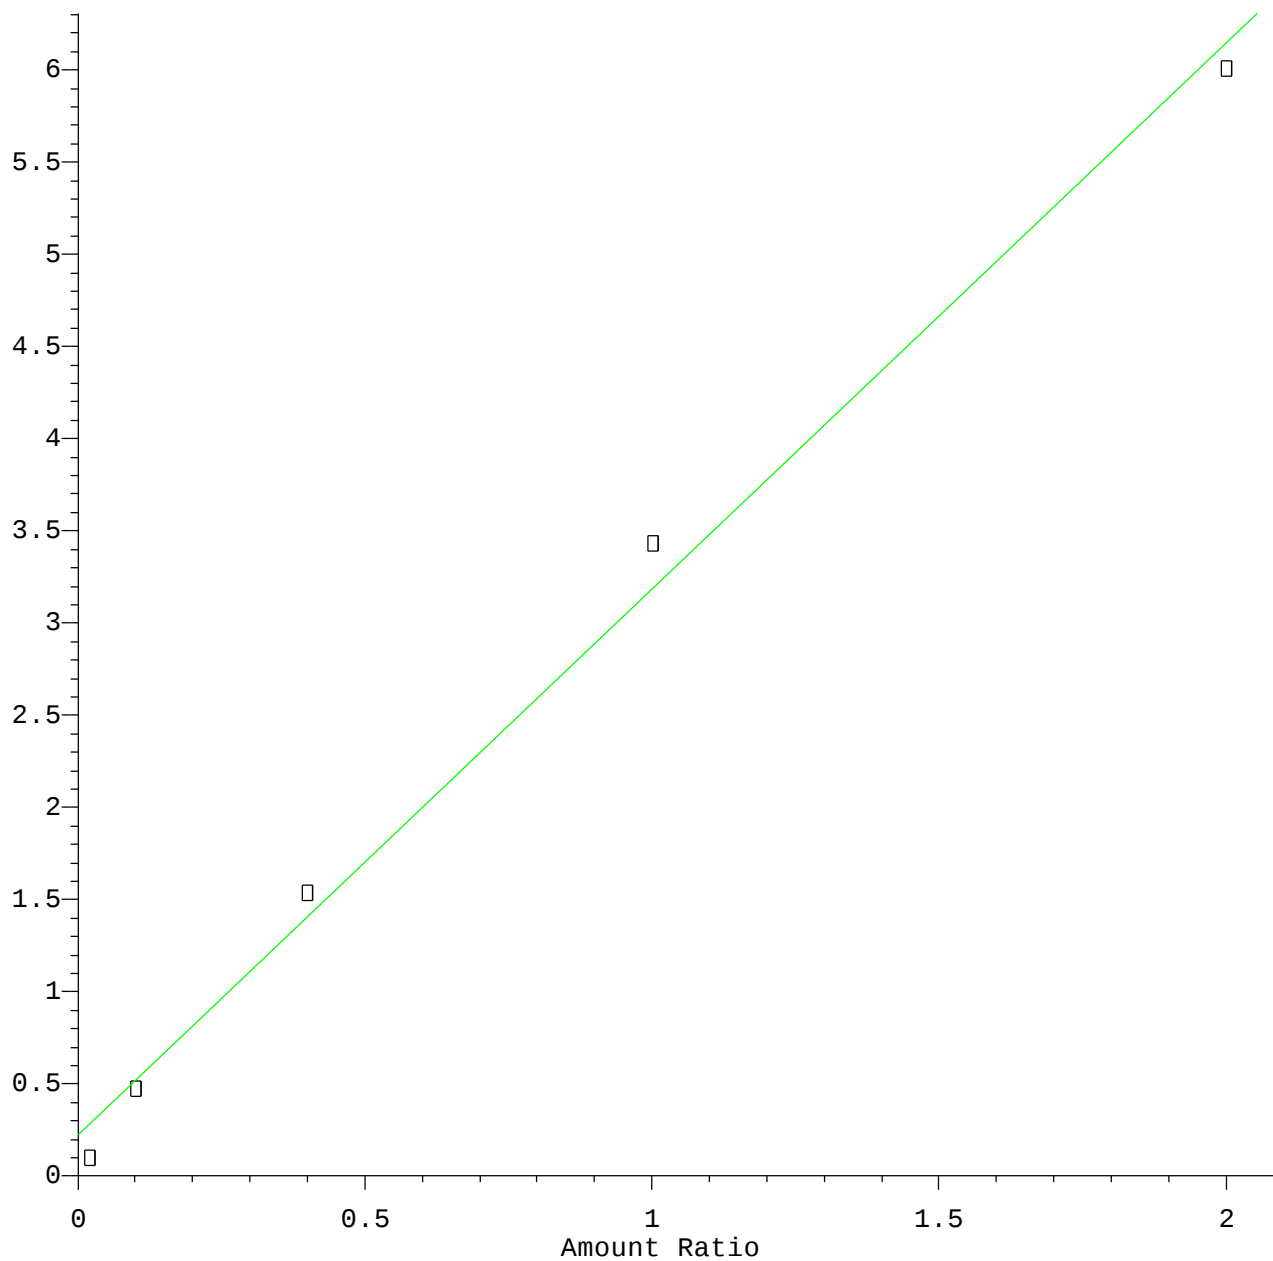


Resp Ratio = 2.96e+000 \* Amt + 2.23e-001  
Coef of Det (r<sup>2</sup>) = 0.994    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N082919W.M  
Calibration Table Last Updated: Fri Aug 30 11:59:03 2019

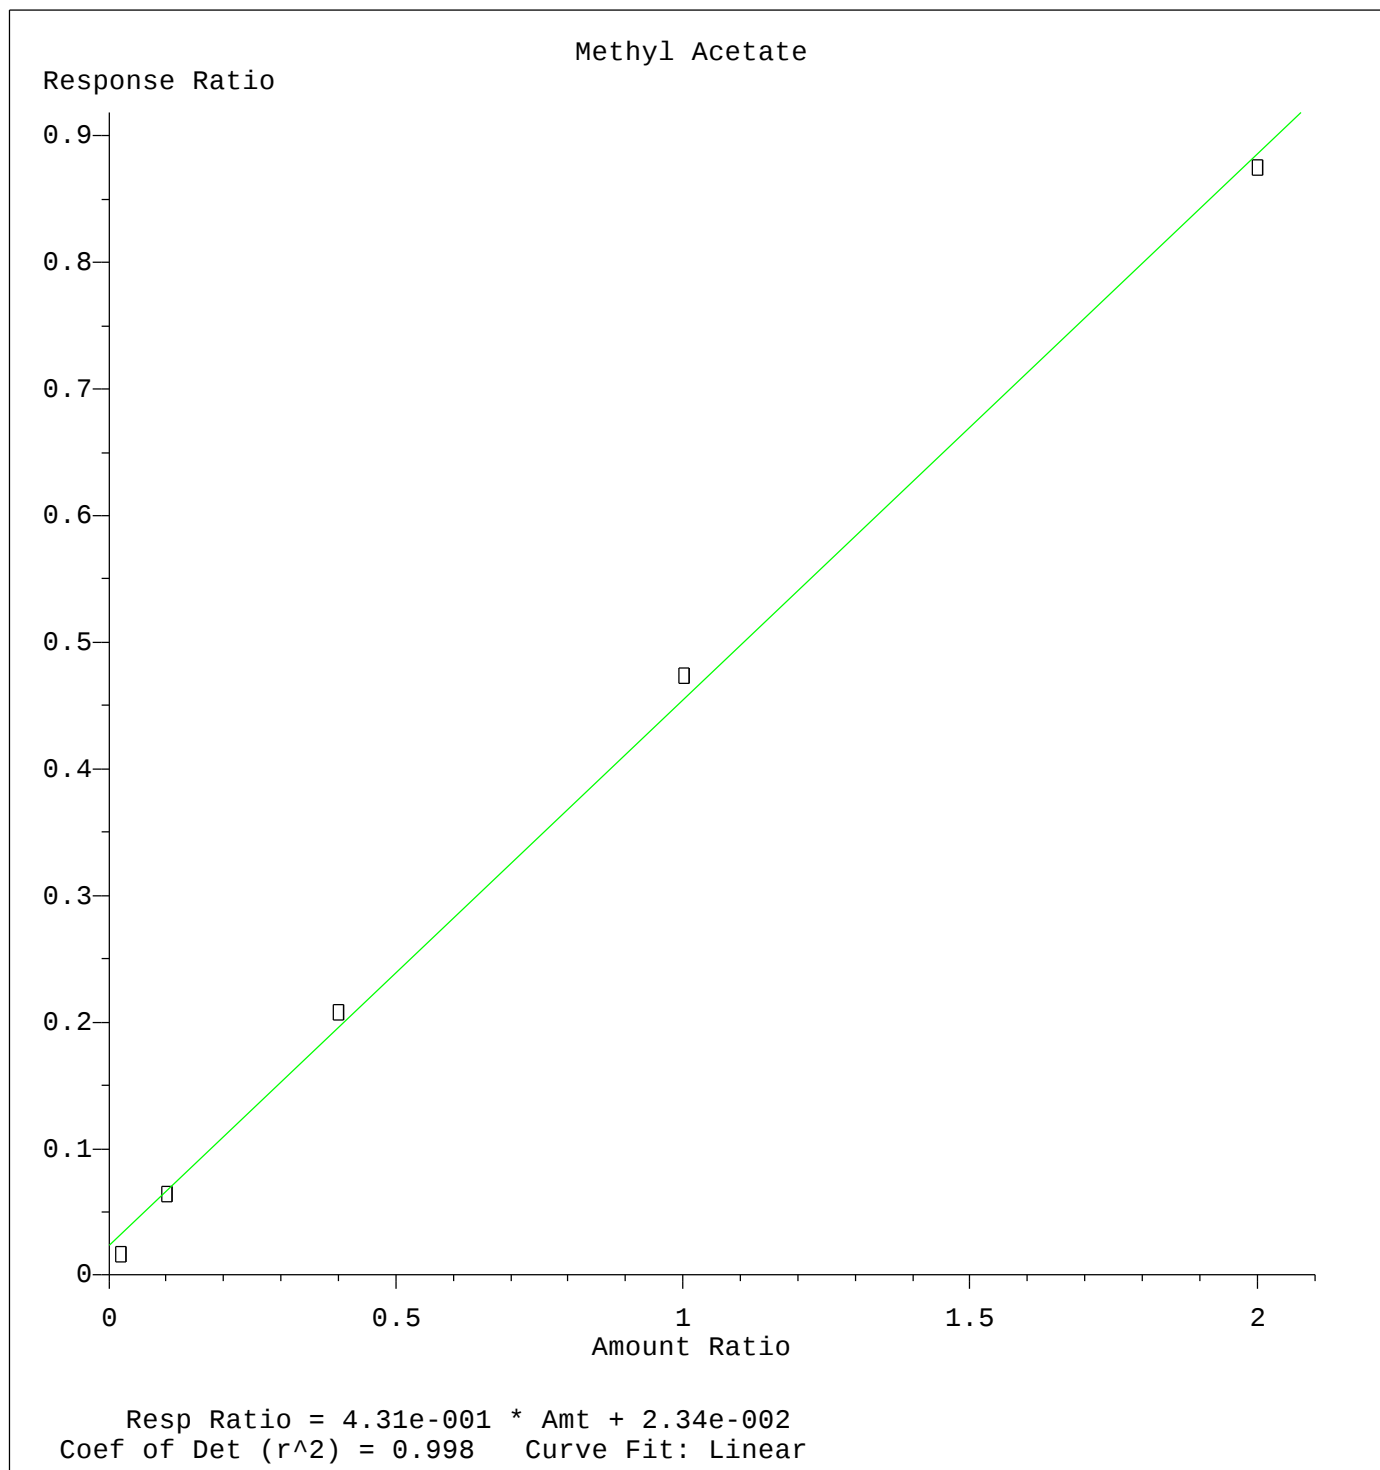


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N082919W.M  
Calibration Table Last Updated: Fri Aug 30 11:59:03 2019

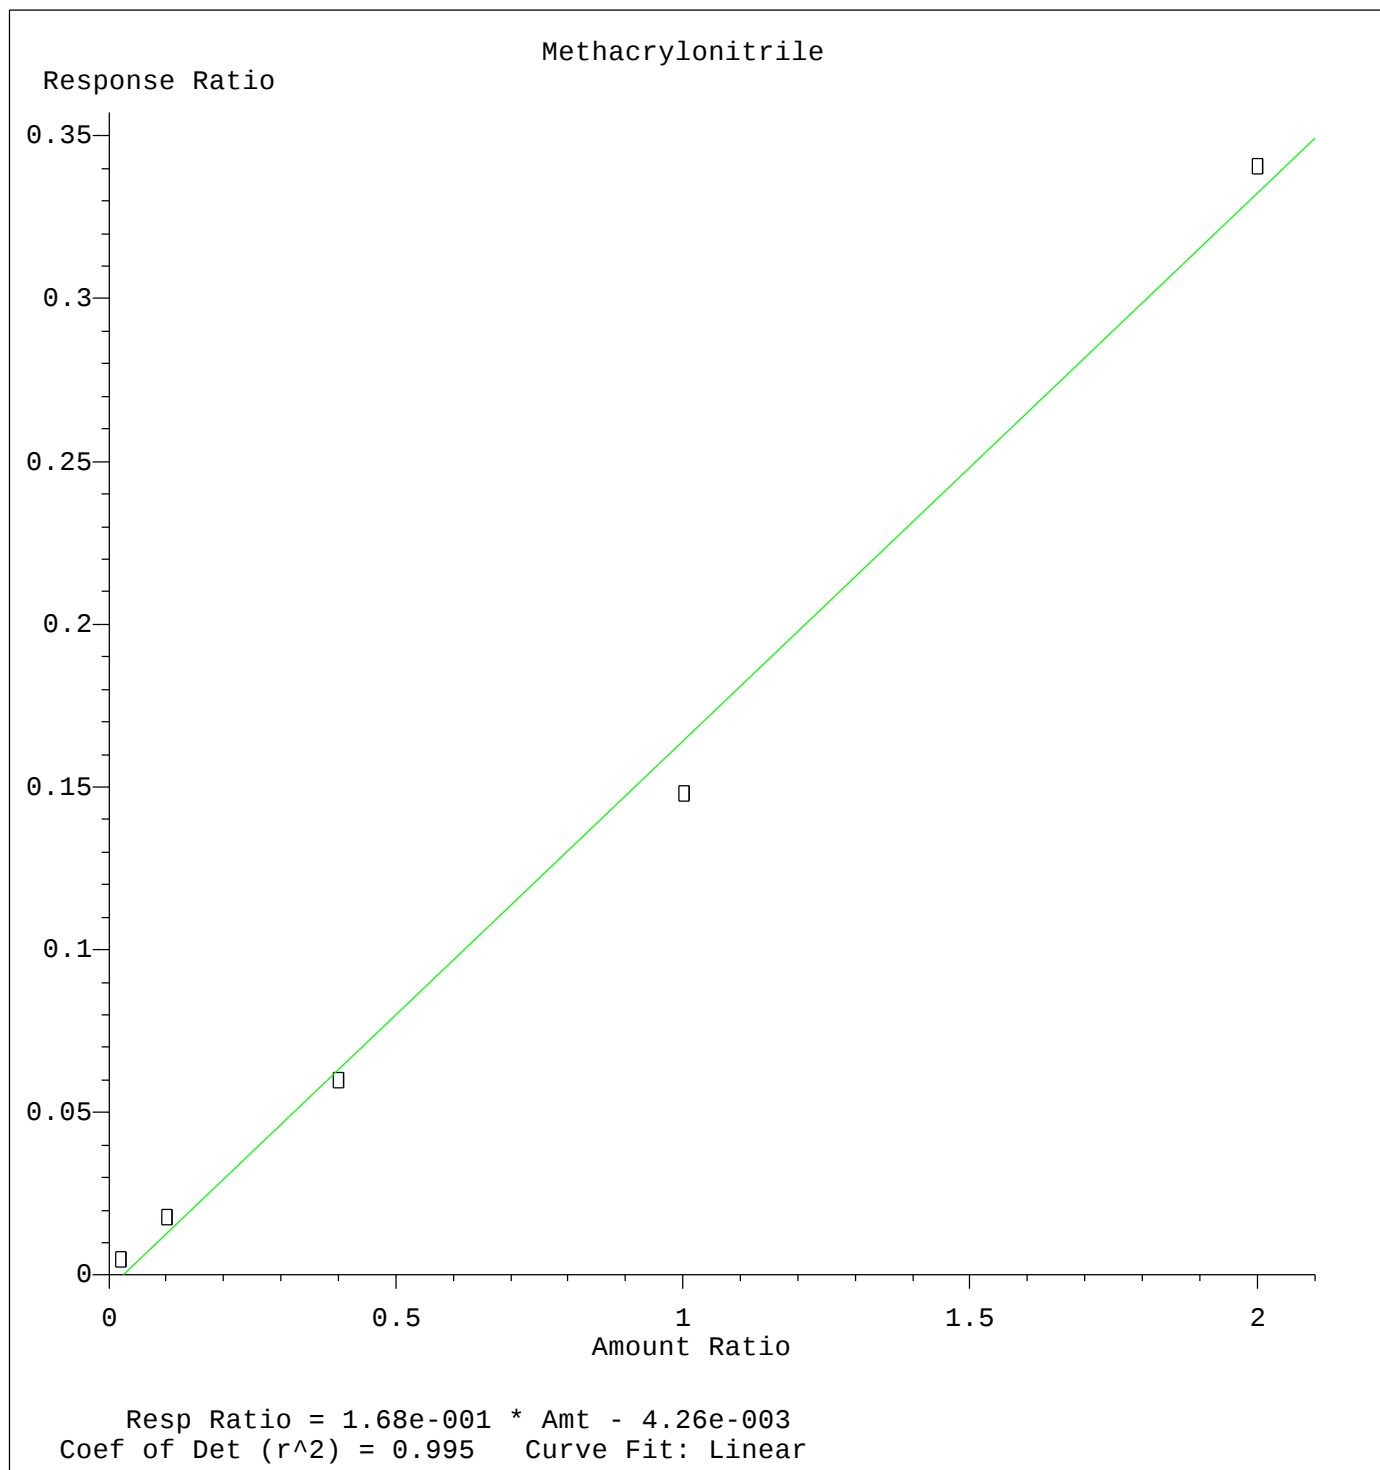

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N082919W.M  
Calibration Table Last Updated: Fri Aug 30 11:59:03 2019

# Isopropylbenzene

Response Ratio

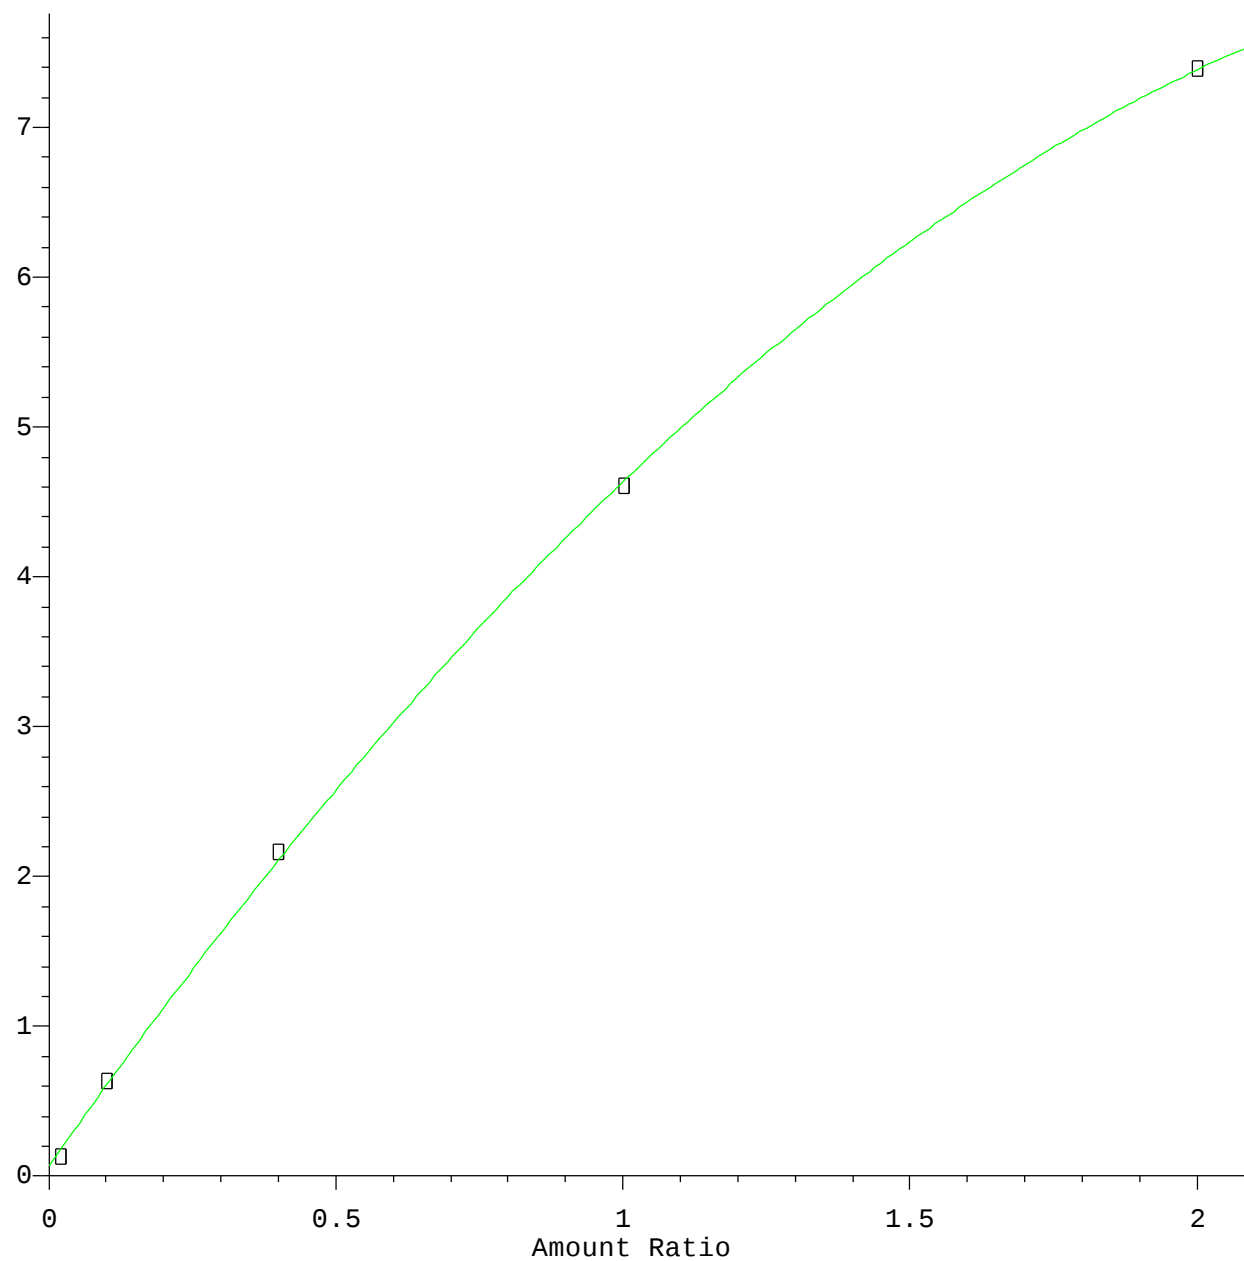

$R = -9.09e-001 A^2 + 5.47e+000 A + 6.80e-002$   
Coef of Det ( $r^2$ ) = 1.000    Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N082919W.M  
Calibration Table Last Updated: Fri Aug 30 11:59:03 2019