


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN082919\
Data File : VN057549.D
Acq On : 29 Aug 2019 13:59
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082919W.M
Title : SW846 8260
Last Update : Fri Aug 30 11:59:03 2019

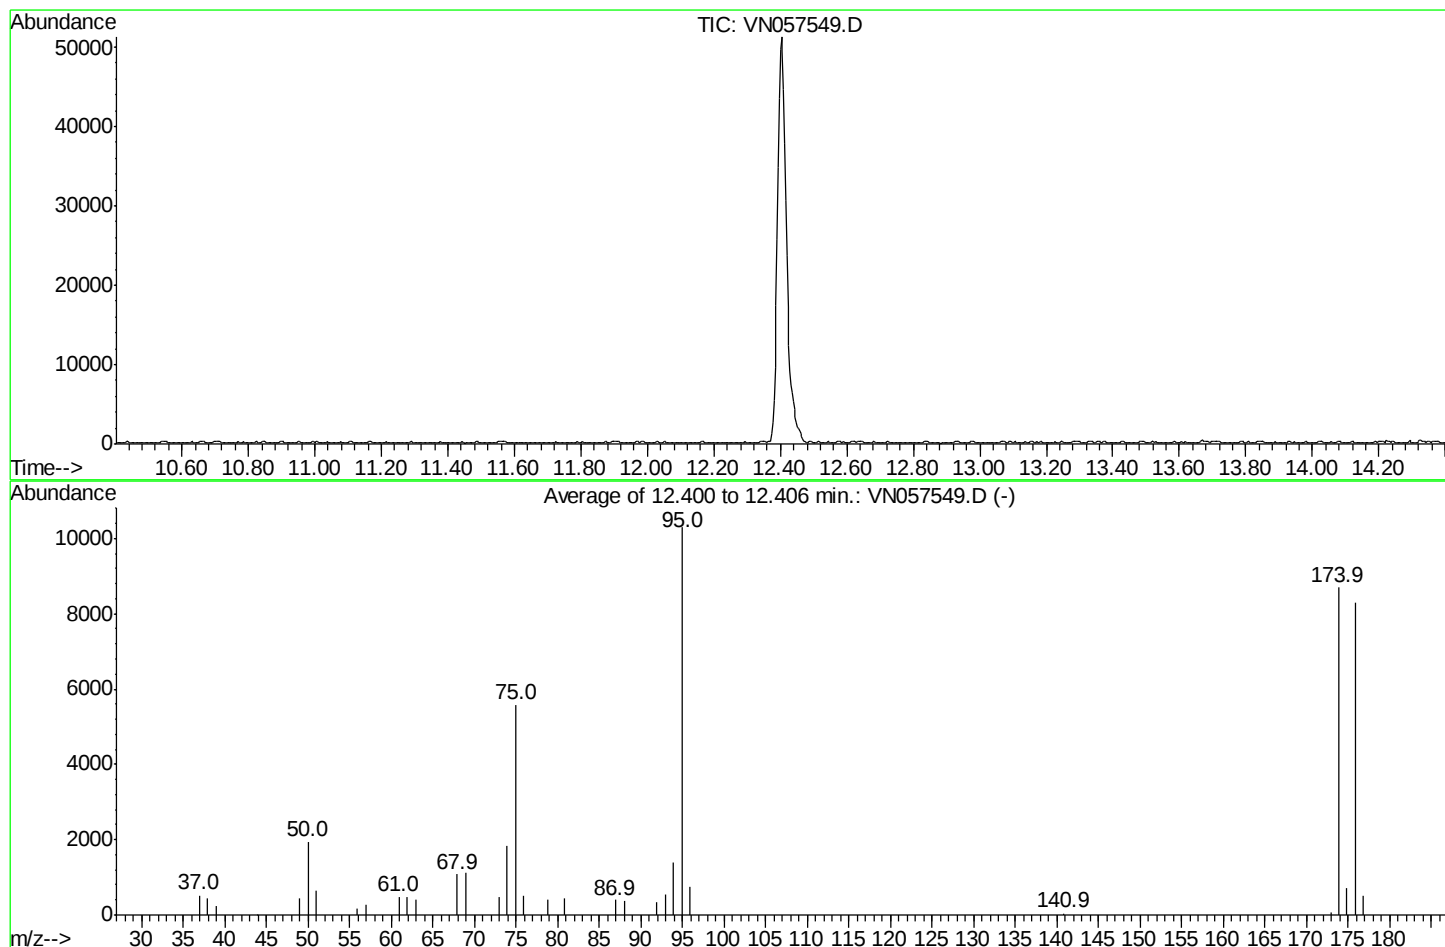

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	1939	PASS
75	95	30	60	54.2	5577	PASS
95	95	100	100	100.0	10295	PASS
96	95	5	9	7.1	732	PASS
173	174	0.00	2	0.6	53	PASS
174	95	50	100	84.4	8691	PASS
175	174	5	9	8.1	708	PASS
176	174	95	101	95.6	8305	PASS
177	176	5	9	6.0	501	PASS