
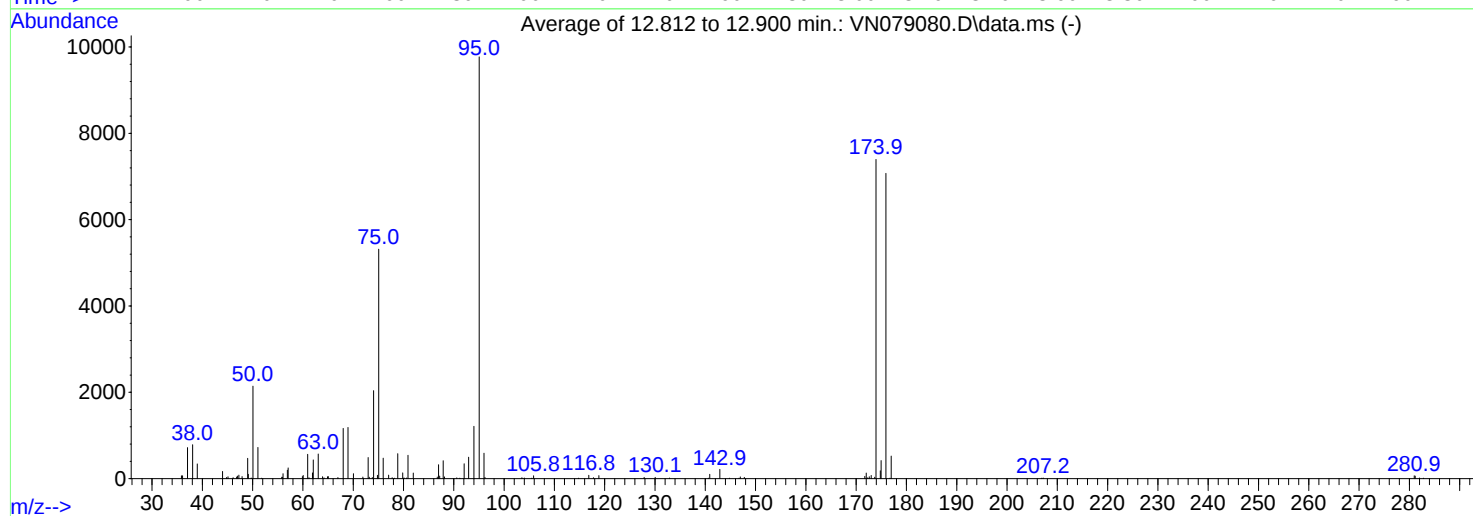


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082923\
 Data File : VN079080.D
 Acq On : 29 Aug 2023 08:47
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N081723W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Aug 18 05:21:14 2023

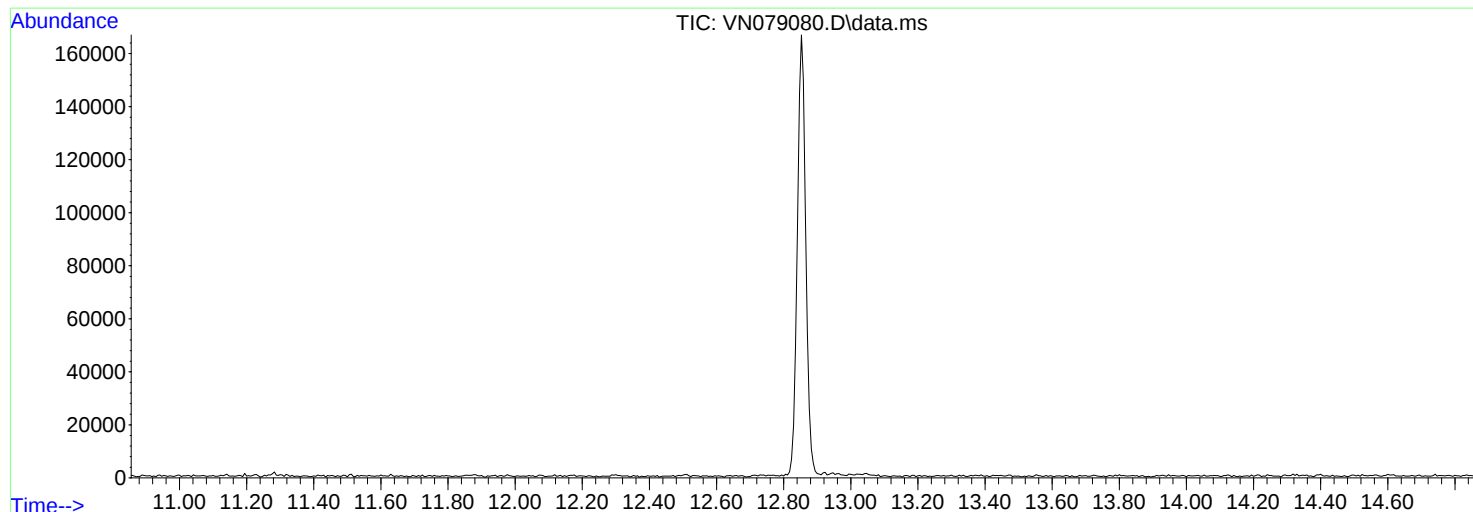

AutoFind: Averaged scan 1846 to 1861; Bkg corrected with scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	2141	PASS
75	95	30	60	54.4	5314	PASS
95	95	100	100	100.0	9771	PASS
96	95	5	9	6.0	590	PASS
173	174	0.00	2	1.0	74	PASS
174	95	50	100	75.7	7396	PASS
175	174	5	9	5.7	418	PASS
176	174	95	101	95.6	7073	PASS
177	176	5	9	7.4	522	PASS