
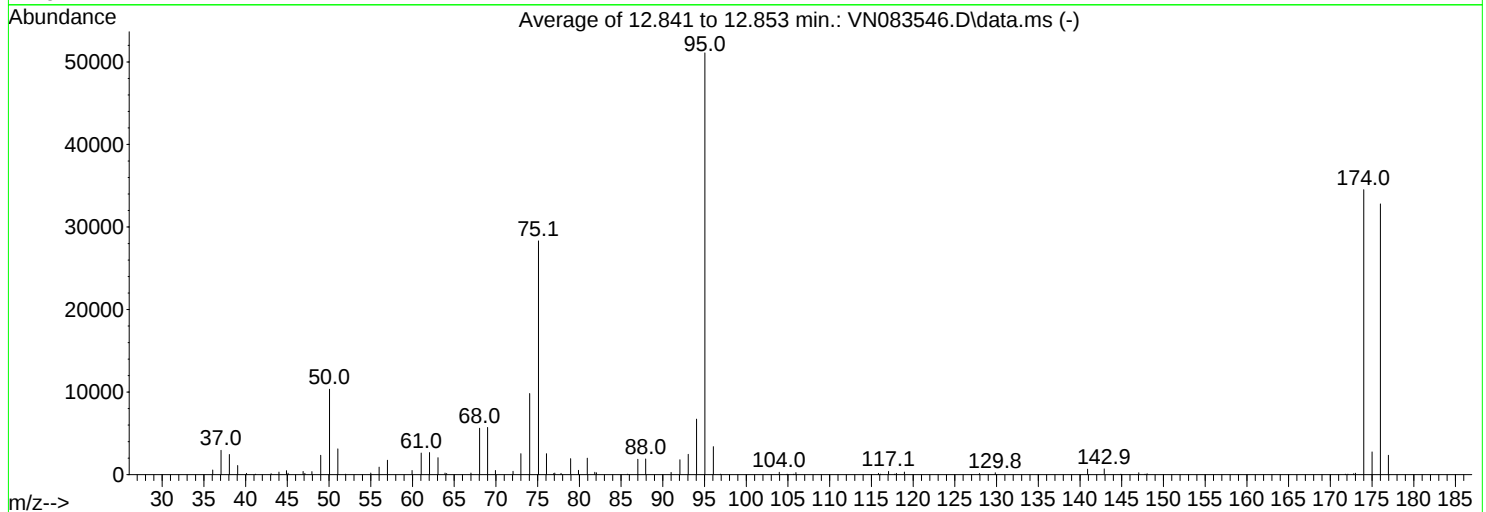


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082924\
Data File : VN083546.D
Acq On : 29 Aug 2024 08:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

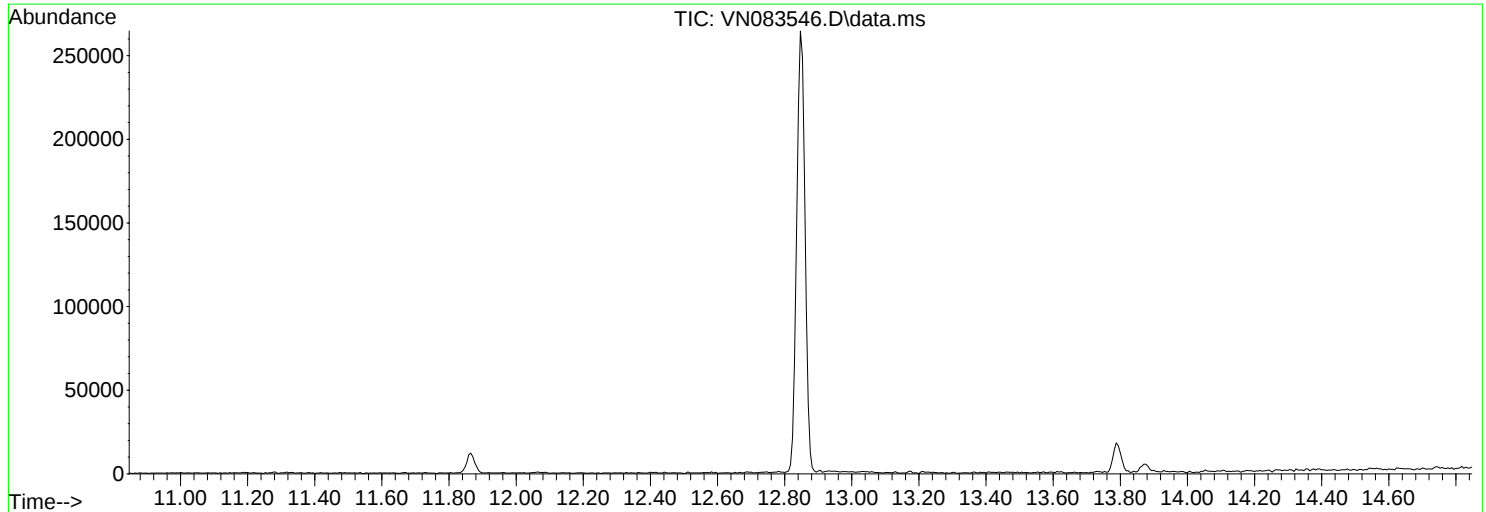

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	10360	PASS
75	95	30	60	55.4	28325	PASS
95	95	100	100	100.0	51099	PASS
96	95	5	9	6.7	3400	PASS
173	174	0.00	2	0.5	182	PASS
174	95	50	100	67.6	34525	PASS
175	174	5	9	8.0	2756	PASS
176	174	95	101	95.0	32803	PASS
177	176	5	9	7.1	2344	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	570	47.10	148	62.05	2675	75.10	2832
37.05	2950	47.95	379	63.05	2047	76.05	254
38.05	2448	49.00	2346	63.90	189	76.90	11
39.05	1113	50.05	10360	64.10	130	77.05	19
40.10	149	51.05	3125	67.00	190	77.80	161
41.20	56	52.00	65	68.05	5626	78.95	1945
43.05	112	55.00	189	69.00	5725	79.90	527
44.00	307	56.00	906	69.95	497	80.95	1988
44.90	482	57.00	1752	72.05	407	81.85	284
45.10	170	59.95	500	73.00	2544	82.05	240
46.90	391	61.05	2623	74.05	9823	85.80	50

Average of 12.841 to 12.853 min.: VN083546.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.00	1864	105.70	56	142.90	697	176.00	32803
87.95	1892	105.95	247	144.90	59	176.95	2344
91.00	280	115.85	164	147.05	229		
92.05	1809	116.10	69	147.80	51		
93.05	2460	117.05	391	148.05	114		
94.05	6724	117.80	63	171.80	59		
95.05	51099	118.00	163	172.10	51		
96.05	3400	118.95	313	172.80	116		
96.90	52	127.95	142	173.00	182		
103.95	295	129.85	240	174.00	34525		
104.90	57	140.90	662	175.00	2756		

Instrument :

MSVOA_N

ClientSampleId :

BFB