

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN083018\
 Data File : VN050963.D
 Acq On : 30 Aug 2018 15:26
 Operator : MD\SY
 Sample : PB112481ZHE#07
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB112481ZHE#07

Quant Time: Aug 31 04:41:16 2018
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 22 05:38:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	586135	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	982118	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	833899	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	289644	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	395598	56.06	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.12%	
35) Dibromofluoromethane	7.59	113	372809	47.71	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.42%	
50) Toluene-d8	10.09	98	1324380	45.34	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.68%	
62) 4-Bromofluorobenzene	12.40	95	358948	36.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	73.96%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.82	43	13901	1.29	ug/l	89
18) Methyl Acetate	4.34	43	15846	2.38	ug/l	97
20) Methylene Chloride	4.55	84	39669	4.99	ug/l	98
43) Isopropyl Acetate	8.17	43	399739	34.92	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN083018\
Data File : VN050963.D
Acq On : 30 Aug 2018 15:26
Operator : MD\SY
Sample : PB112481ZHE#07
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB112481ZHE#07

Quant Time: Aug 31 04:41:16 2018
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 22 05:38:12 2018
Response via : Initial Calibration

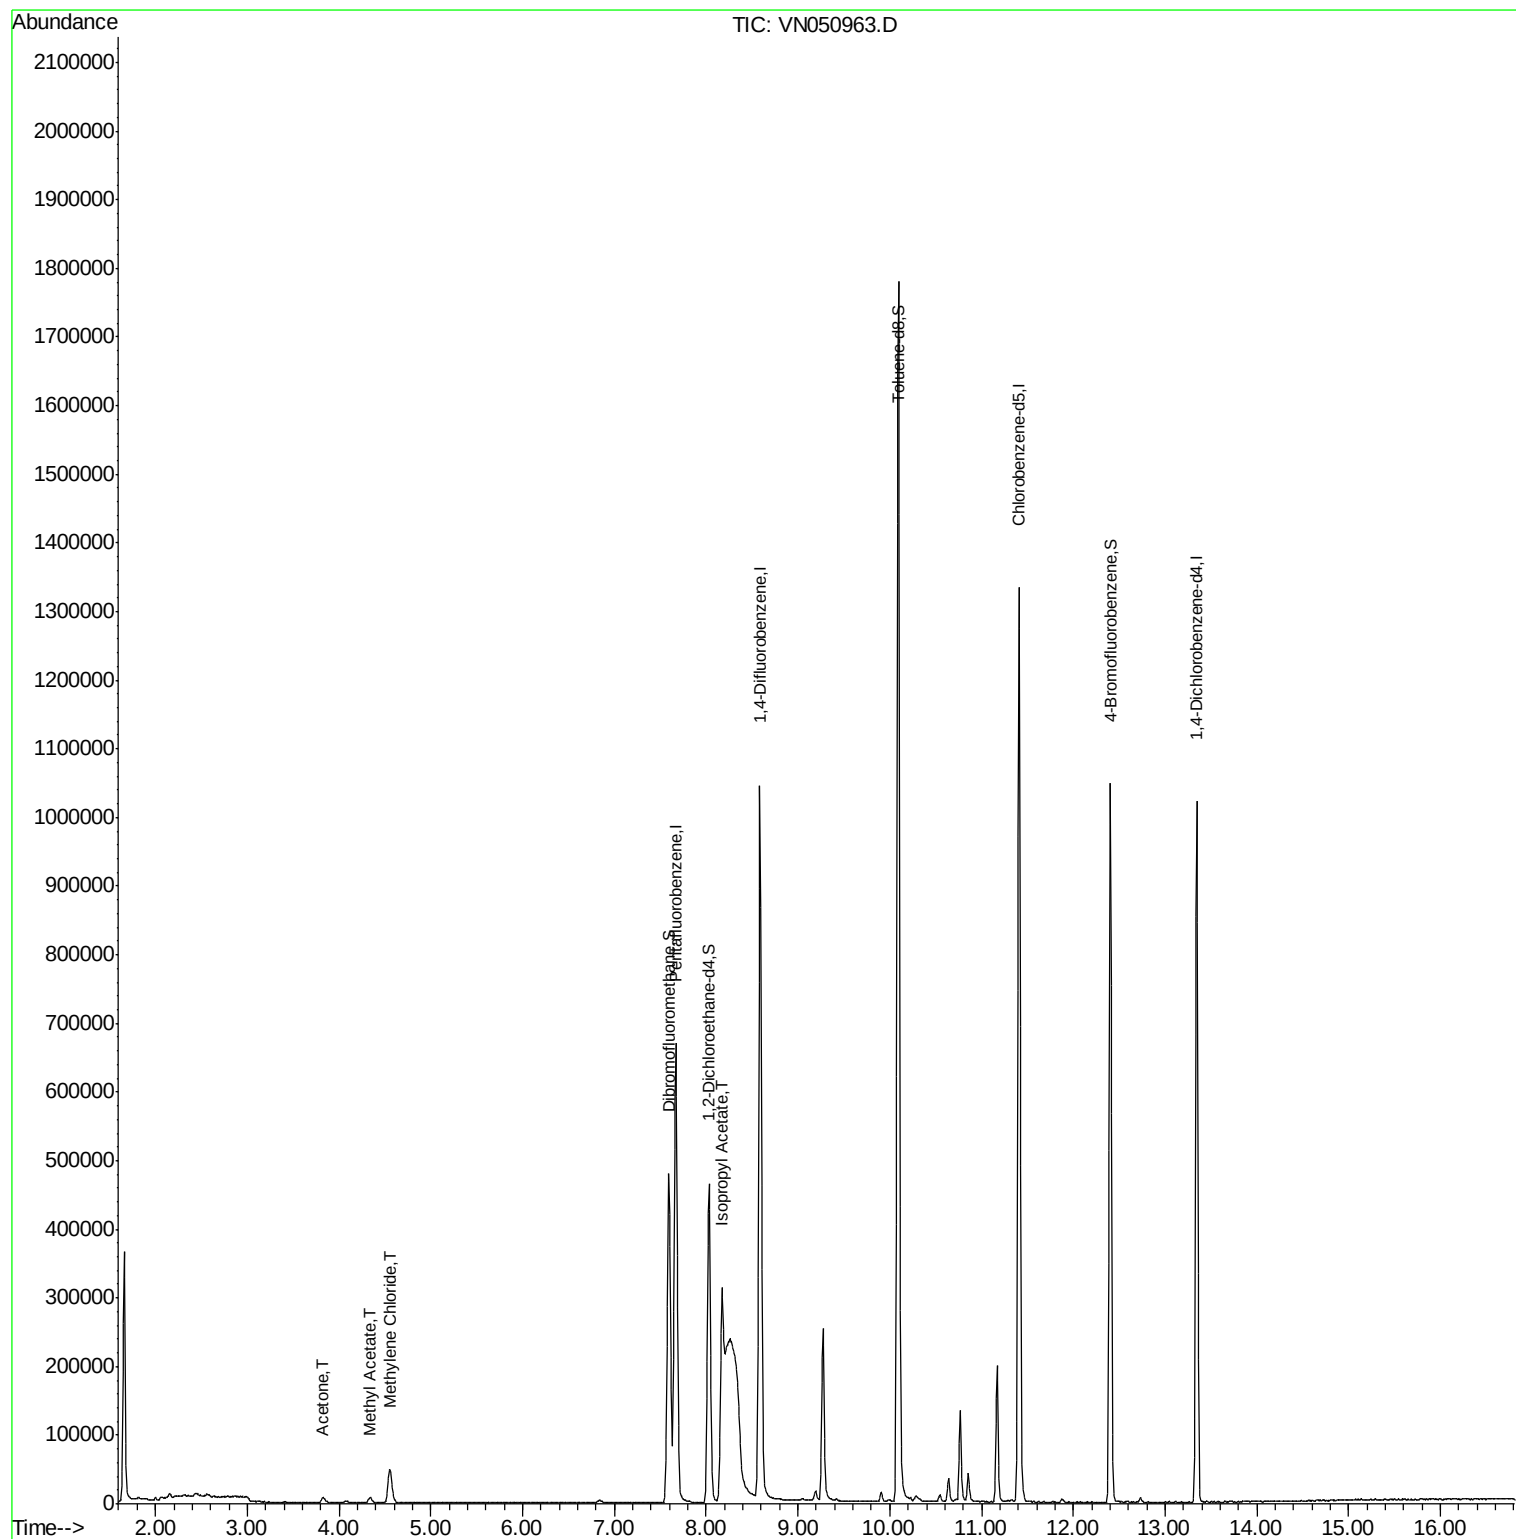

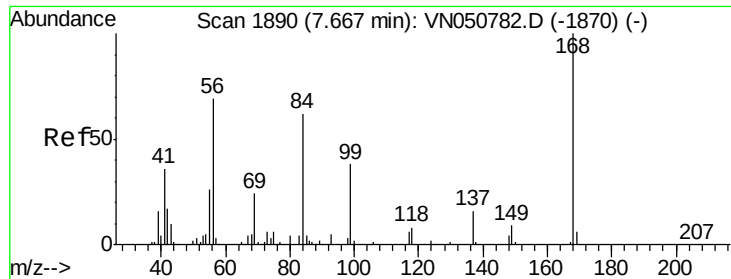

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050963.D

Acq: 30 Aug 2018 15:26

Instrument :

MSVOA_N

ClientSampleId :


PB112481ZHE#07

Tot Ion:168 Resp: 586135

Ion Ratio Lower Upper

168 100

99 48.8 39.6 59.4

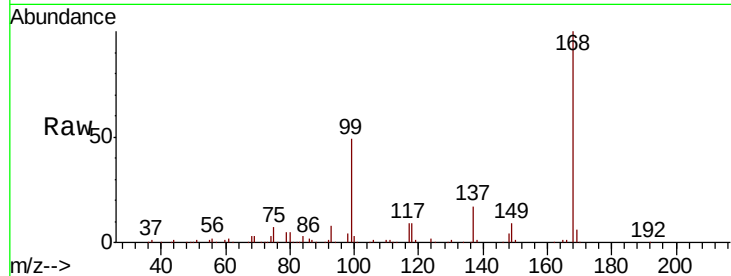

Abundance Ion 167.90 (167.60 to 168.60): VN050963.D (-1797) (-)

Ion 98.90 (98.60 to 99.60): VN050963.D (-1797) (-)

7.67

250000

200000



150000

100000

50000

0

Time-->

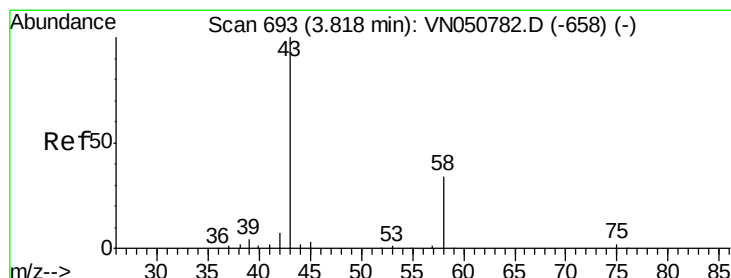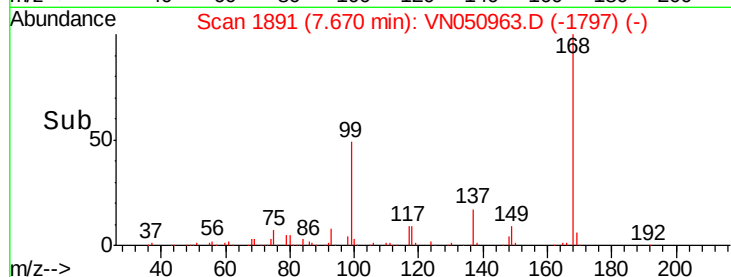

#16

Acetone

Concen: 1.29 ug/l

RT: 3.82 min Scan# 695

Delta R.T. 0.01 min

Lab File: VN050963.D


Acq: 30 Aug 2018 15:26

Tgt Ion: 43 Resp: 13901

Ion Ratio Lower Upper

43 100

58 27.7 27.2 40.8

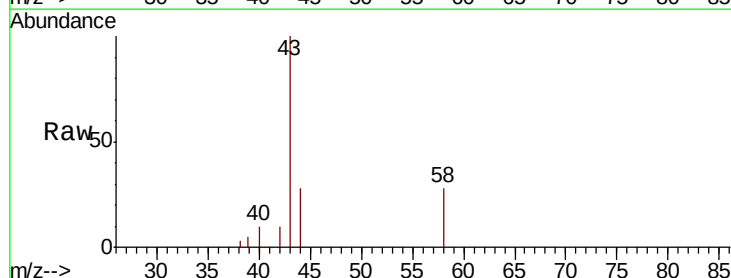

Abundance Ion 43.00 (42.70 to 43.70): VN050963.D (-600) (-)

Ion 58.00 (57.70 to 58.70): VN050963.D (-600) (-)

3.82

5000

4000


3000


2000

1000

0

Time-->




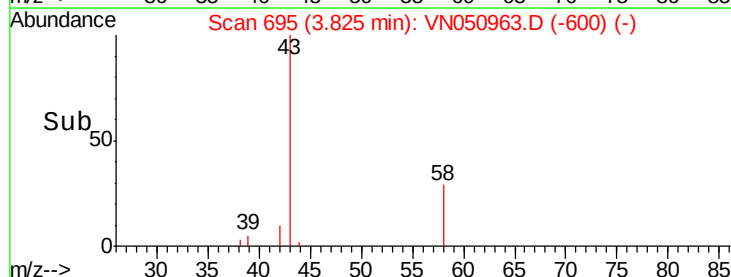


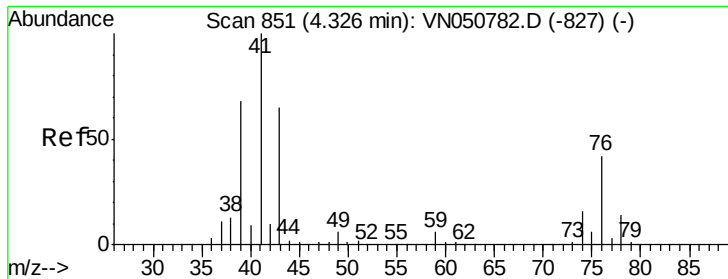

#18
Methvl Acetate
Concen: 2.38 ug/l
RT: 4.34 min Scan# 854
Delta R.T. 0.01 min
Lab File: VN050963.D
Acq: 30 Aug 2018 15:26




Instrument :
MSVOA_N
ClientSampleId :
PB112481ZHE#07


Tot Ion: 43 Resp: 15846
Ion Ratio Lower Upper
43 100
74 23.5 19.8 29.8

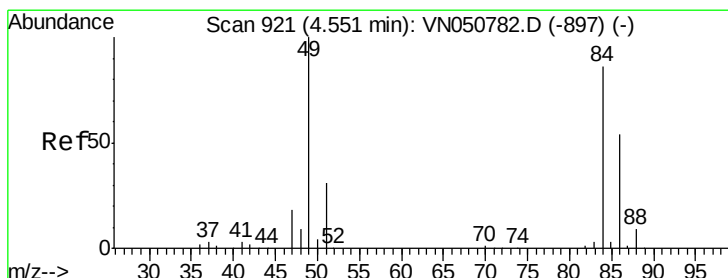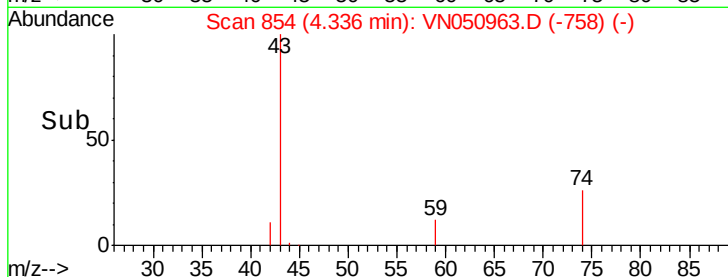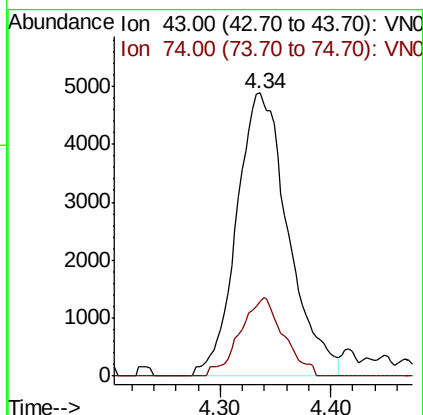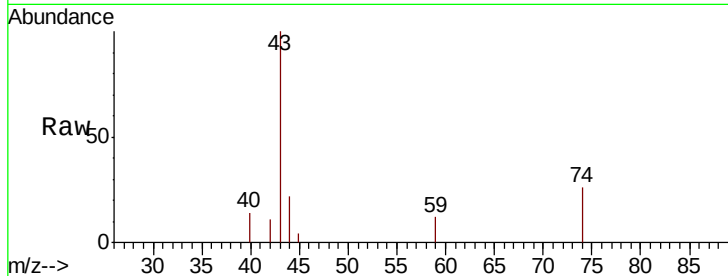

#20
Methylene Chloride
Concen: 4.99 ug/l
RT: 4.55 min Scan# 921
Delta R.T. -0.00 min
Lab File: VN050963.D
Acq: 30 Aug 2018 15:26

Tgt Ion: 84 Resp: 39669
Ion Ratio Lower Upper
84 100
49 115.6 93.2 139.8
51 32.9 29.0 43.6
86 63.2 49.8 74.8


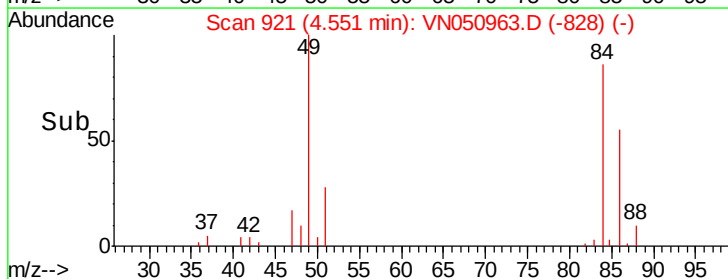
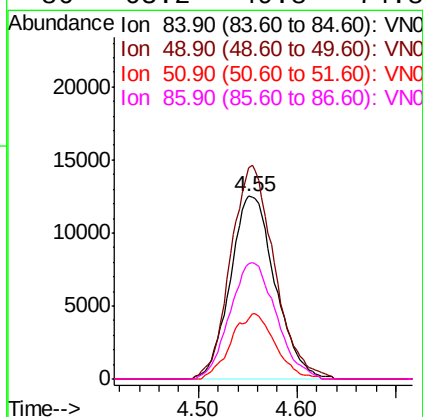
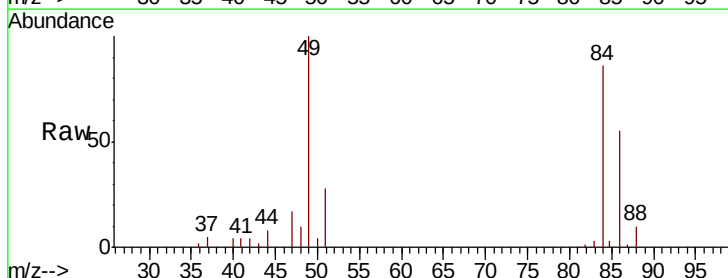


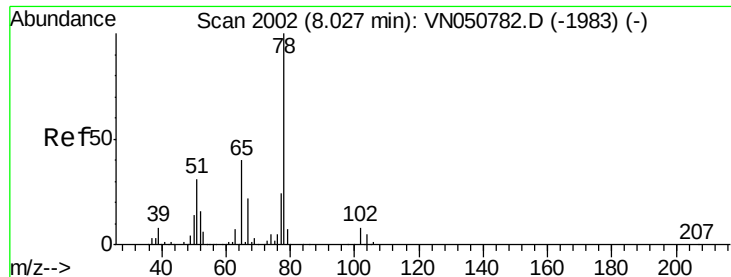

#33
 1,2-Dichloroethane-d4
 Concen: 56.06 ug/l
 RT: 8.03 min Scan# 2003
 Delta R.T. 0.00 min
 Lab File: VN050963.D
 Acq: 30 Aug 2018 15:26




Instrument :
 MSVOA_N
 ClientSampleId :
 PB112481ZHE#07


Tot Ion: 65 Resp: 395598
 Ion Ratio Lower Upper
 65 100
 67 54.2 0.0 110.4

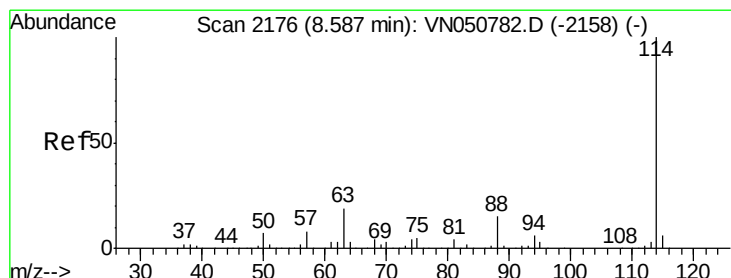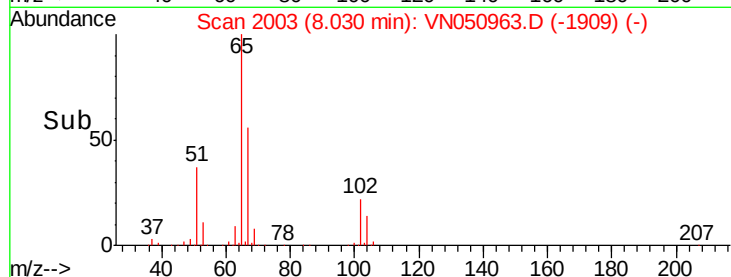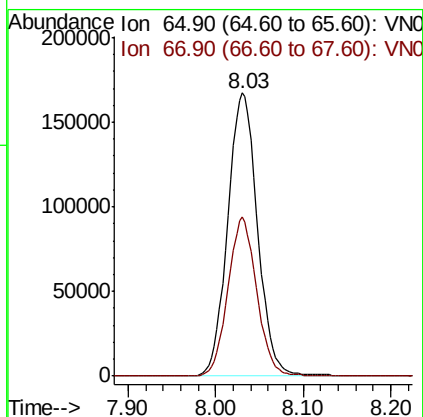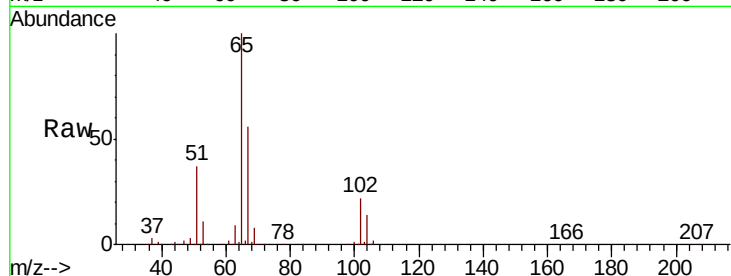

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2176
 Delta R.T. -0.00 min
 Lab File: VN050963.D
 Acq: 30 Aug 2018 15:26

Tgt Ion: 114 Resp: 982118
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 38.6
 88 15.9 0.0 30.6


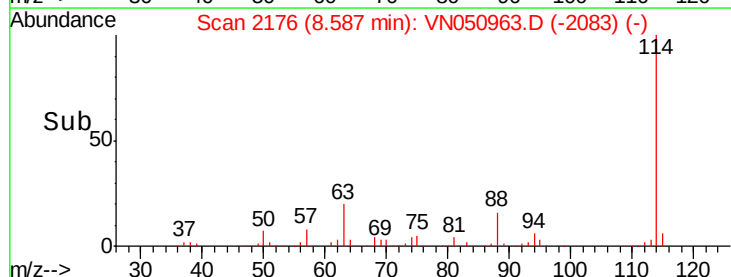
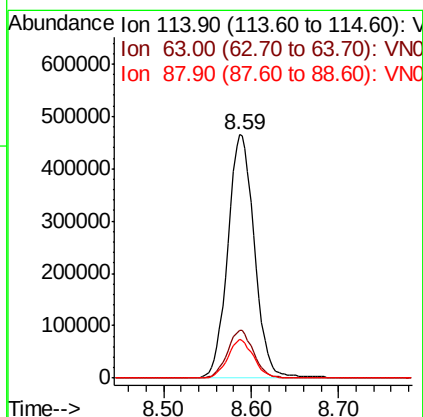
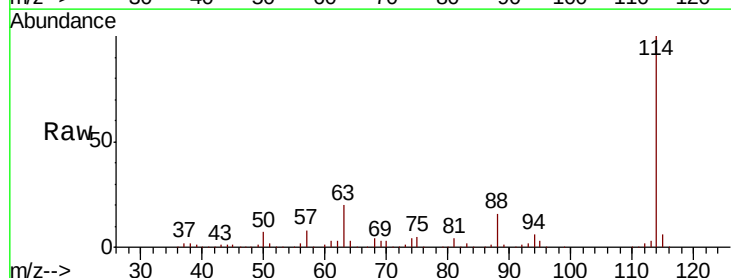


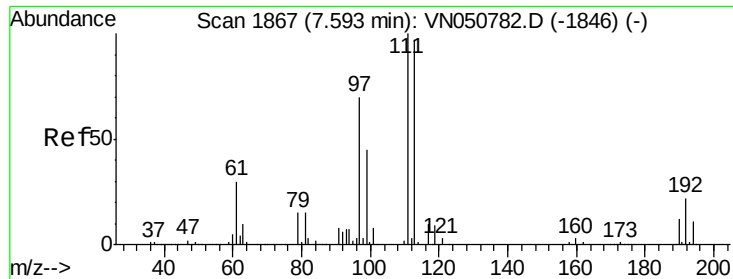

#35
 Dibromofluoromethane
 Concen: 47.71 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. -0.00 min
 Lab File: VN050963.D
 Acq: 30 Aug 2018 15:26




Instrument :
 MSVOA_N
 ClientSampleId :
 PB112481ZHE#07


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.5	82.6	123.8
192	22.7	18.0	27.0

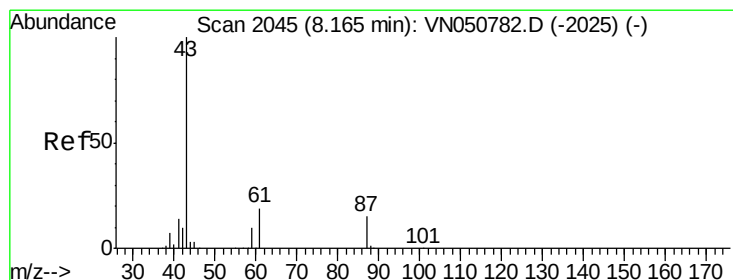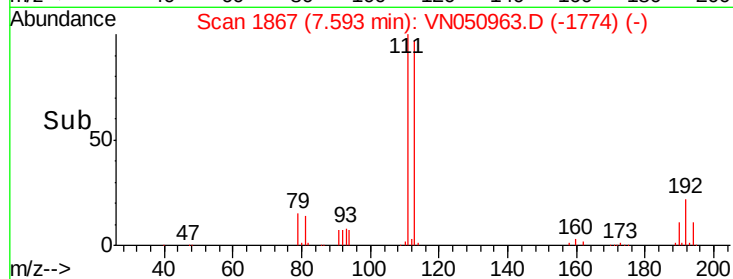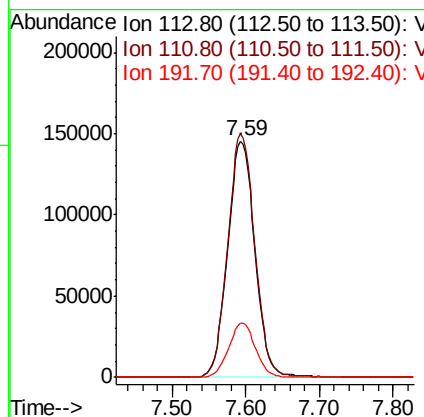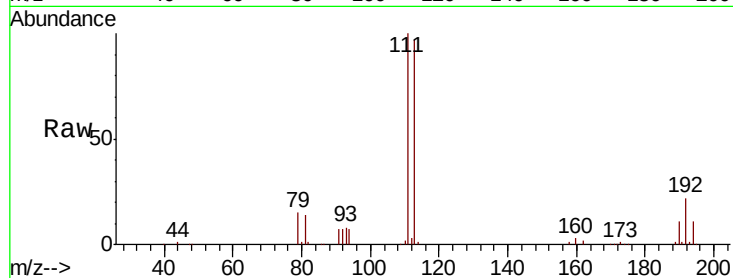

#43
 Isopropyl Acetate
 Concen: 34.92 ug/l
 RT: 8.17 min Scan# 2047
 Delta R.T. 0.01 min
 Lab File: VN050963.D
 Acq: 30 Aug 2018 15:26

Tgt Ion	Ratio	Lower	Upper
43	100		
61	15.1	17.5	26.3#
87	9.6	11.3	16.9#

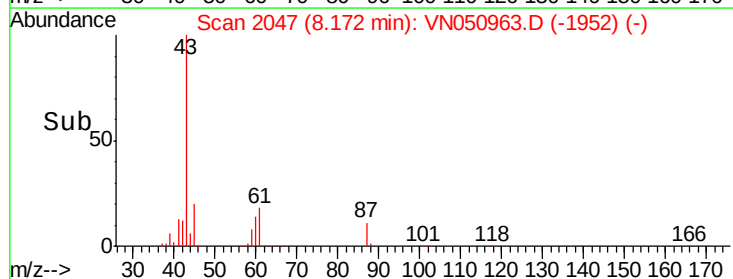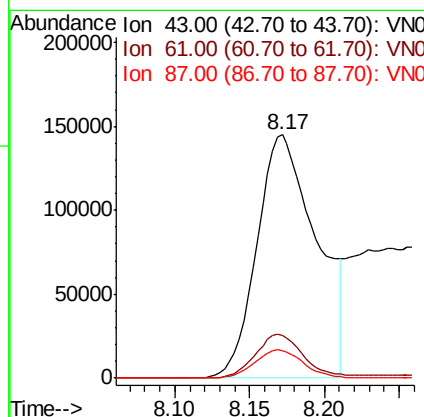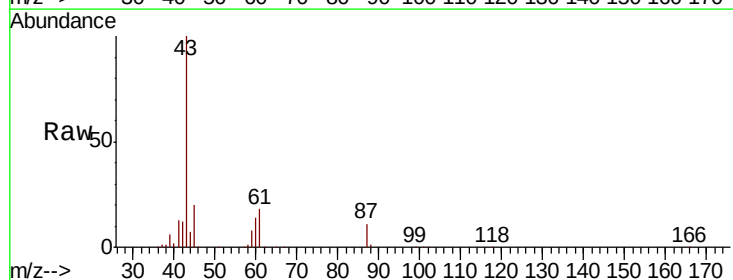

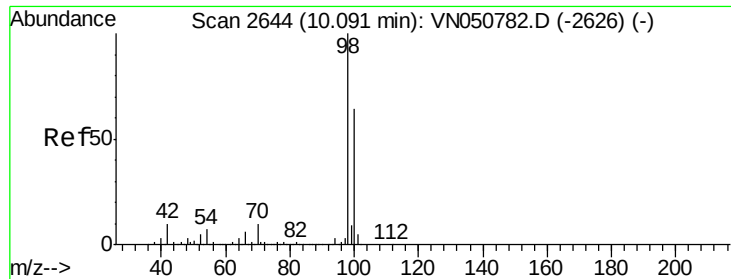

#50

Toluene-d8

Concen: 45.34 ug/l

RT: 10.09 min Scan# 2645

Delta R.T. 0.00 min

Lab File: VN050963.D

Acq: 30 Aug 2018 15:26

Instrument :

MSVOA_N

ClientSampleId :





PB112481ZHE#07

Tot Ion: 98 Resp: 1324380

Ion Ratio Lower Upper

98 100

100 63.3 51.5 77.3

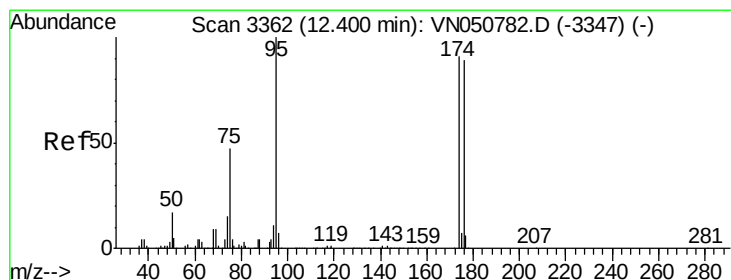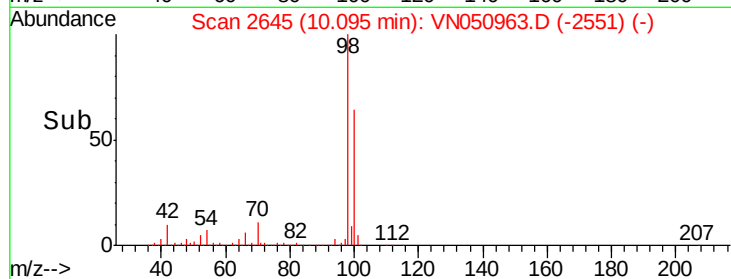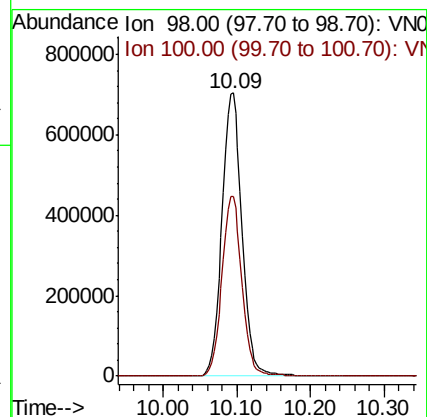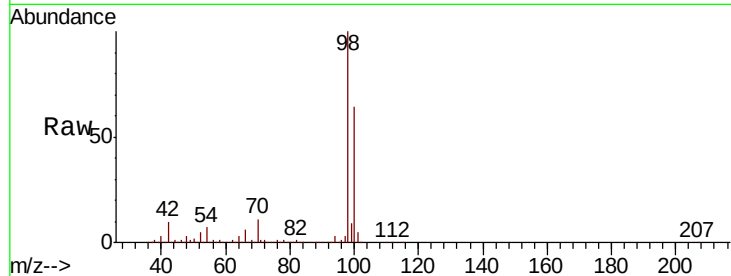

#62

4-Bromofluorobenzene

Concen: 36.98 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN050963.D

Acq: 30 Aug 2018 15:26




Tgt Ion: 95 Resp: 358948


Ion Ratio Lower Upper

95 100

174 92.9 0.0 183.0

176 89.4 0.0 178.8

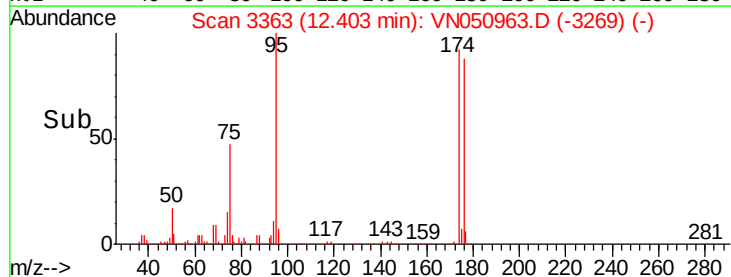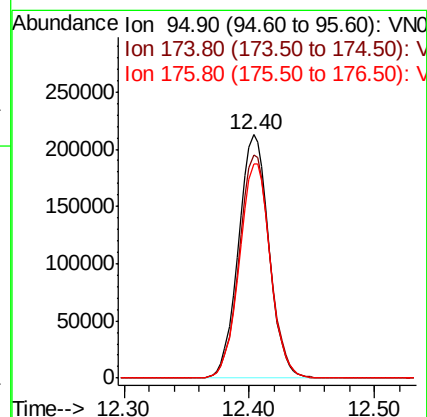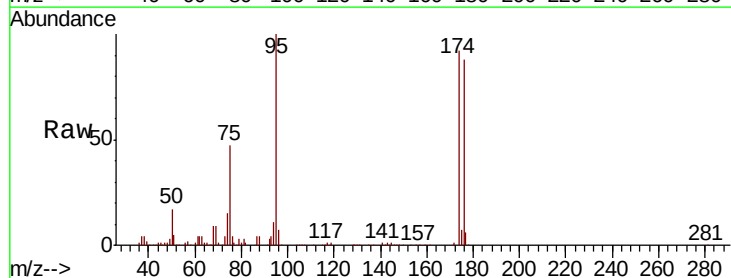


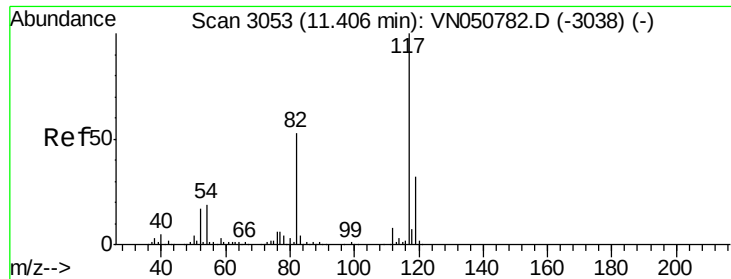




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. 0.00 min
Lab File: VN050963.D
Acq: 30 Aug 2018 15:26

Instrument :
MSVOA_N
ClientSampleId :
PB112481ZHE#07

Tot Ion:117 Resp: 833899
Ion Ratio Lower Upper
117 100
82 53.2 42.6 64.0
119 32.5 25.8 38.6

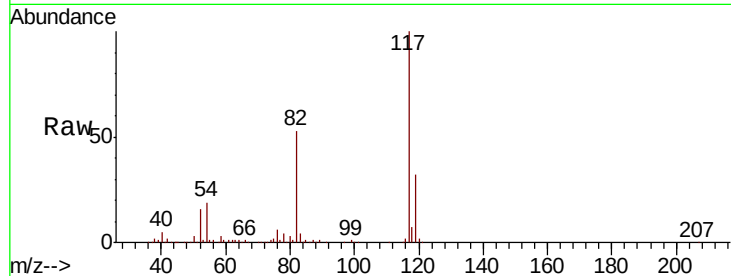


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

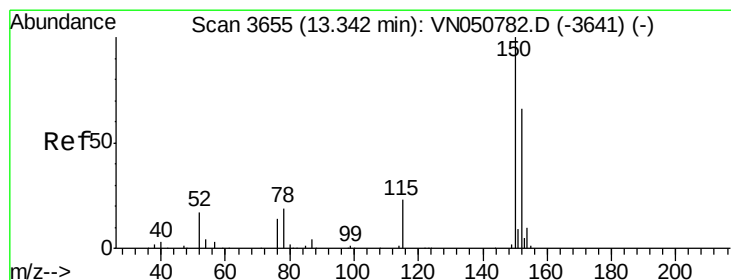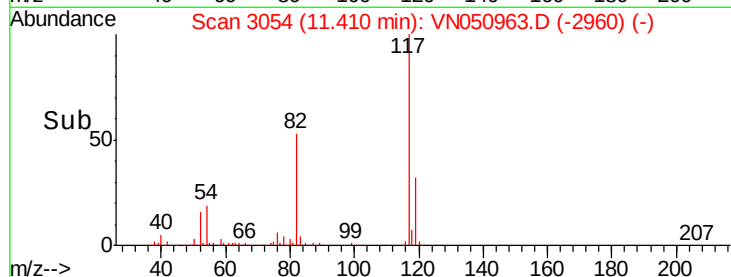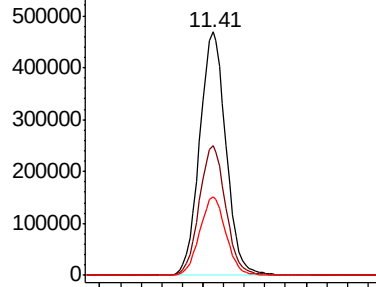

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.35 min Scan# 3656
Delta R.T. 0.00 min
Lab File: VN050963.D
Acq: 30 Aug 2018 15:26

Tgt Ion:152 Resp: 289644
Ion Ratio Lower Upper
152 100
115 55.4 27.8 83.4
150 157.1 0.0 351.4

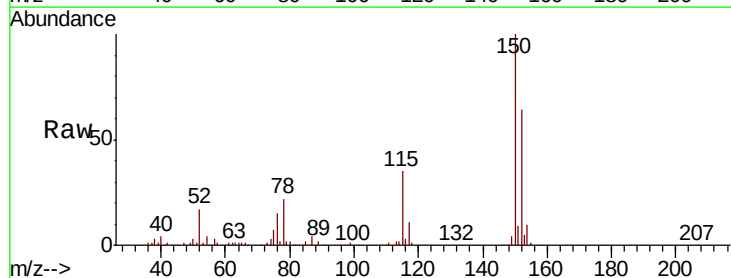

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

