


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN083018\
Data File : VN050950.D
Acq On : 30 Aug 2018 9:51
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
Title : SW846 8260
Last Update : Wed Aug 22 05:38:12 2018

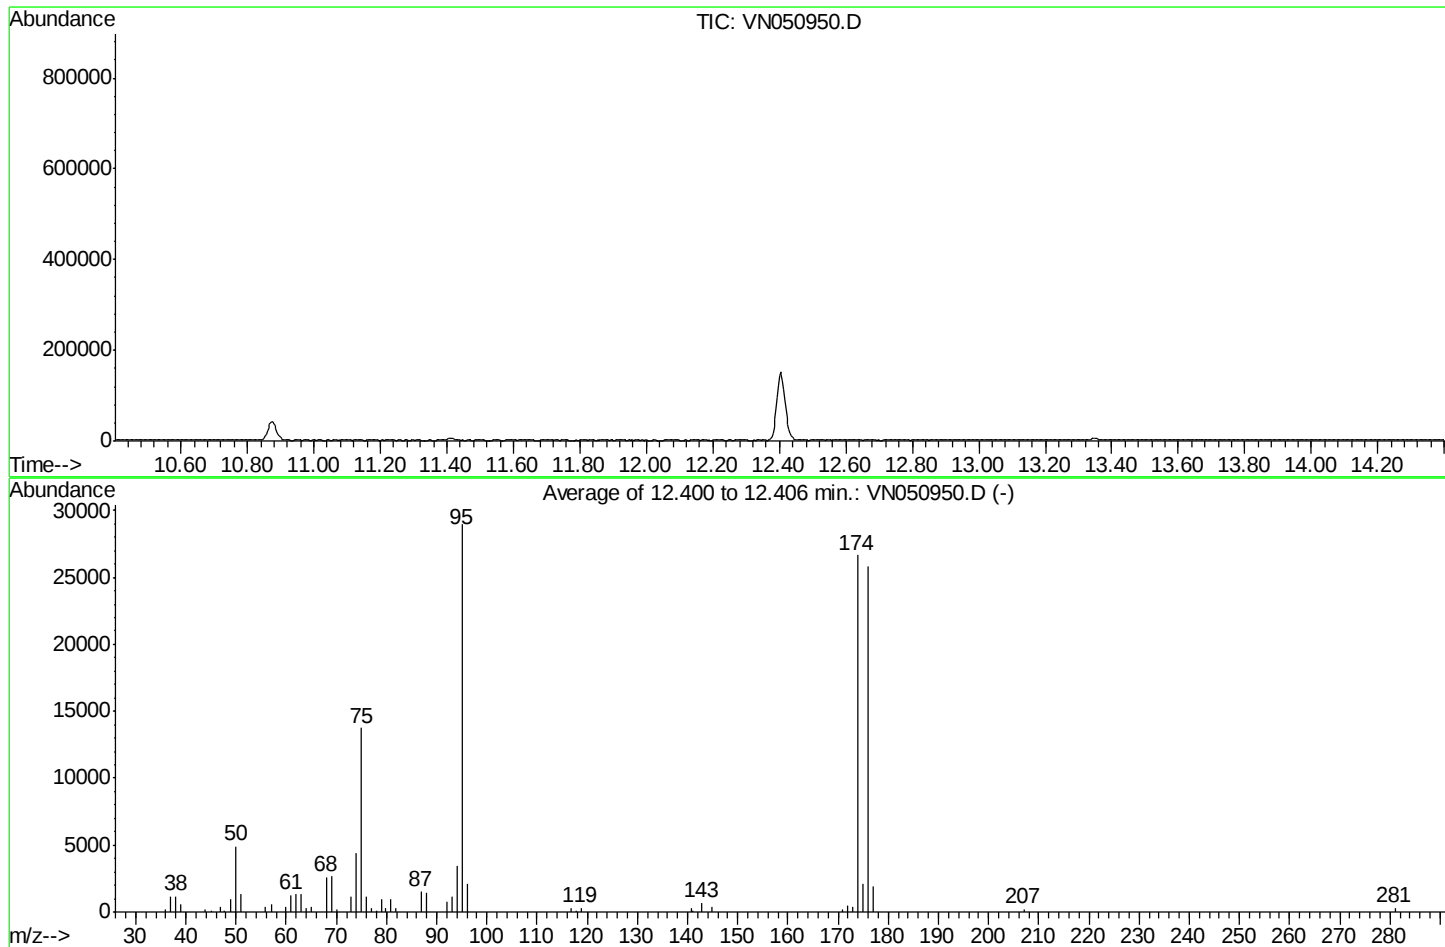

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	4906	PASS
75	95	30	60	47.5	13769	PASS
95	95	100	100	100.0	28970	PASS
96	95	5	9	7.2	2087	PASS
173	174	0.00	2	1.5	408	PASS
174	95	50	100	92.1	26674	PASS
175	174	5	9	7.9	2109	PASS
176	174	95	101	96.9	25858	PASS
177	176	5	9	7.5	1937	PASS