


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN083019\
 Data File : VN057575.D
 Acq On : 30 Aug 2019 8:14
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N083019W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Sat Aug 31 00:00:09 2019

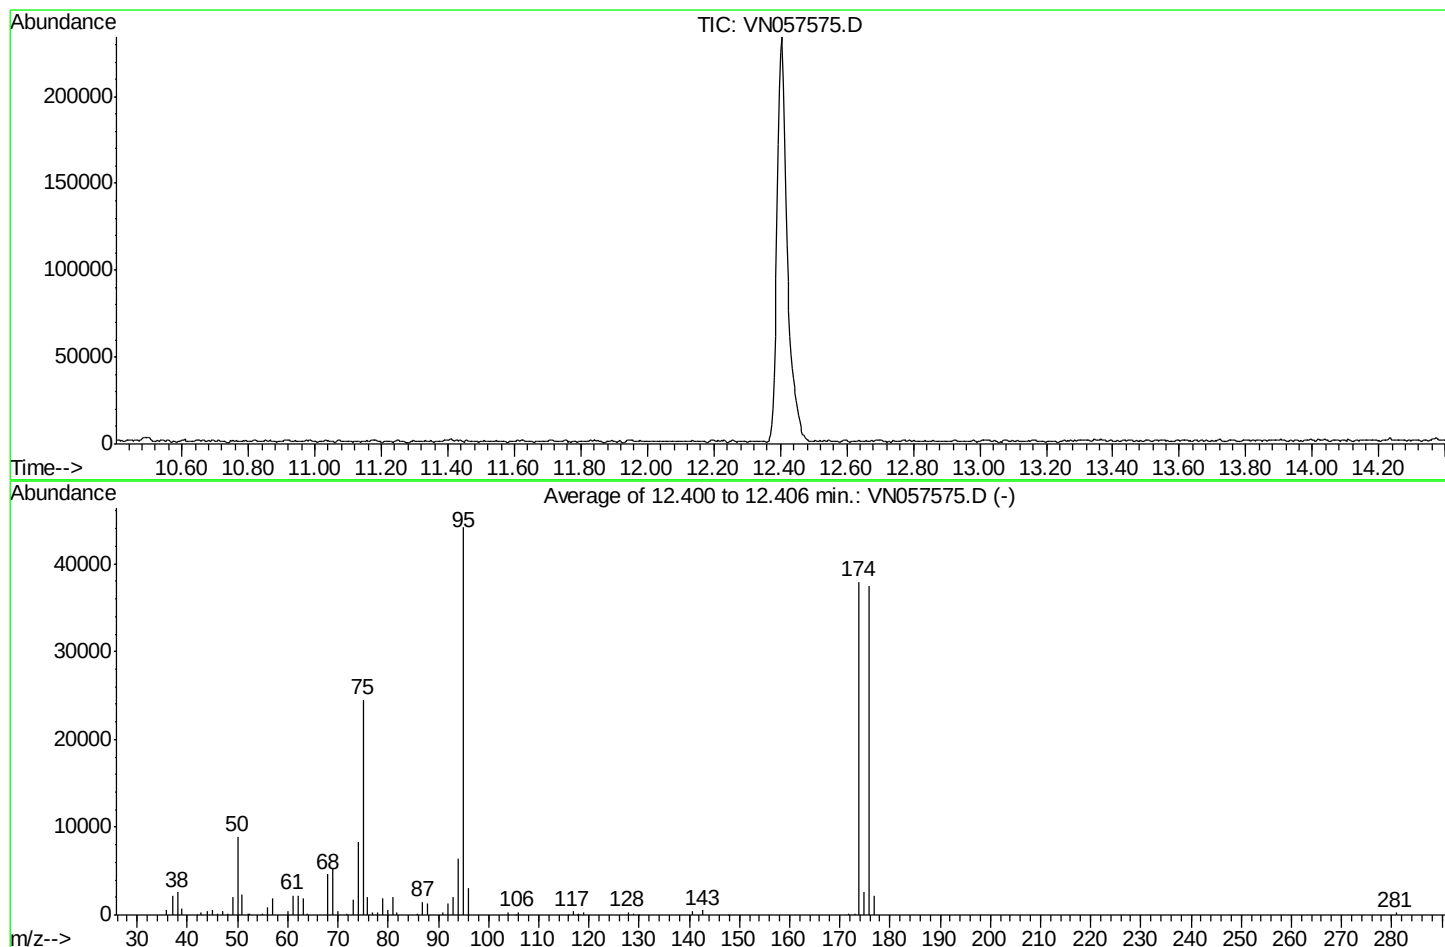

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	8948	PASS
75	95	30	60	55.5	24496	PASS
95	95	100	100	100.0	44149	PASS
96	95	5	9	7.0	3105	PASS
173	174	0.00	2	0.5	203	PASS
174	95	50	100	85.9	37925	PASS
175	174	5	9	6.9	2631	PASS
176	174	95	101	98.9	37504	PASS
177	176	5	9	5.7	2135	PASS