


Bromomethane

Response Ratio

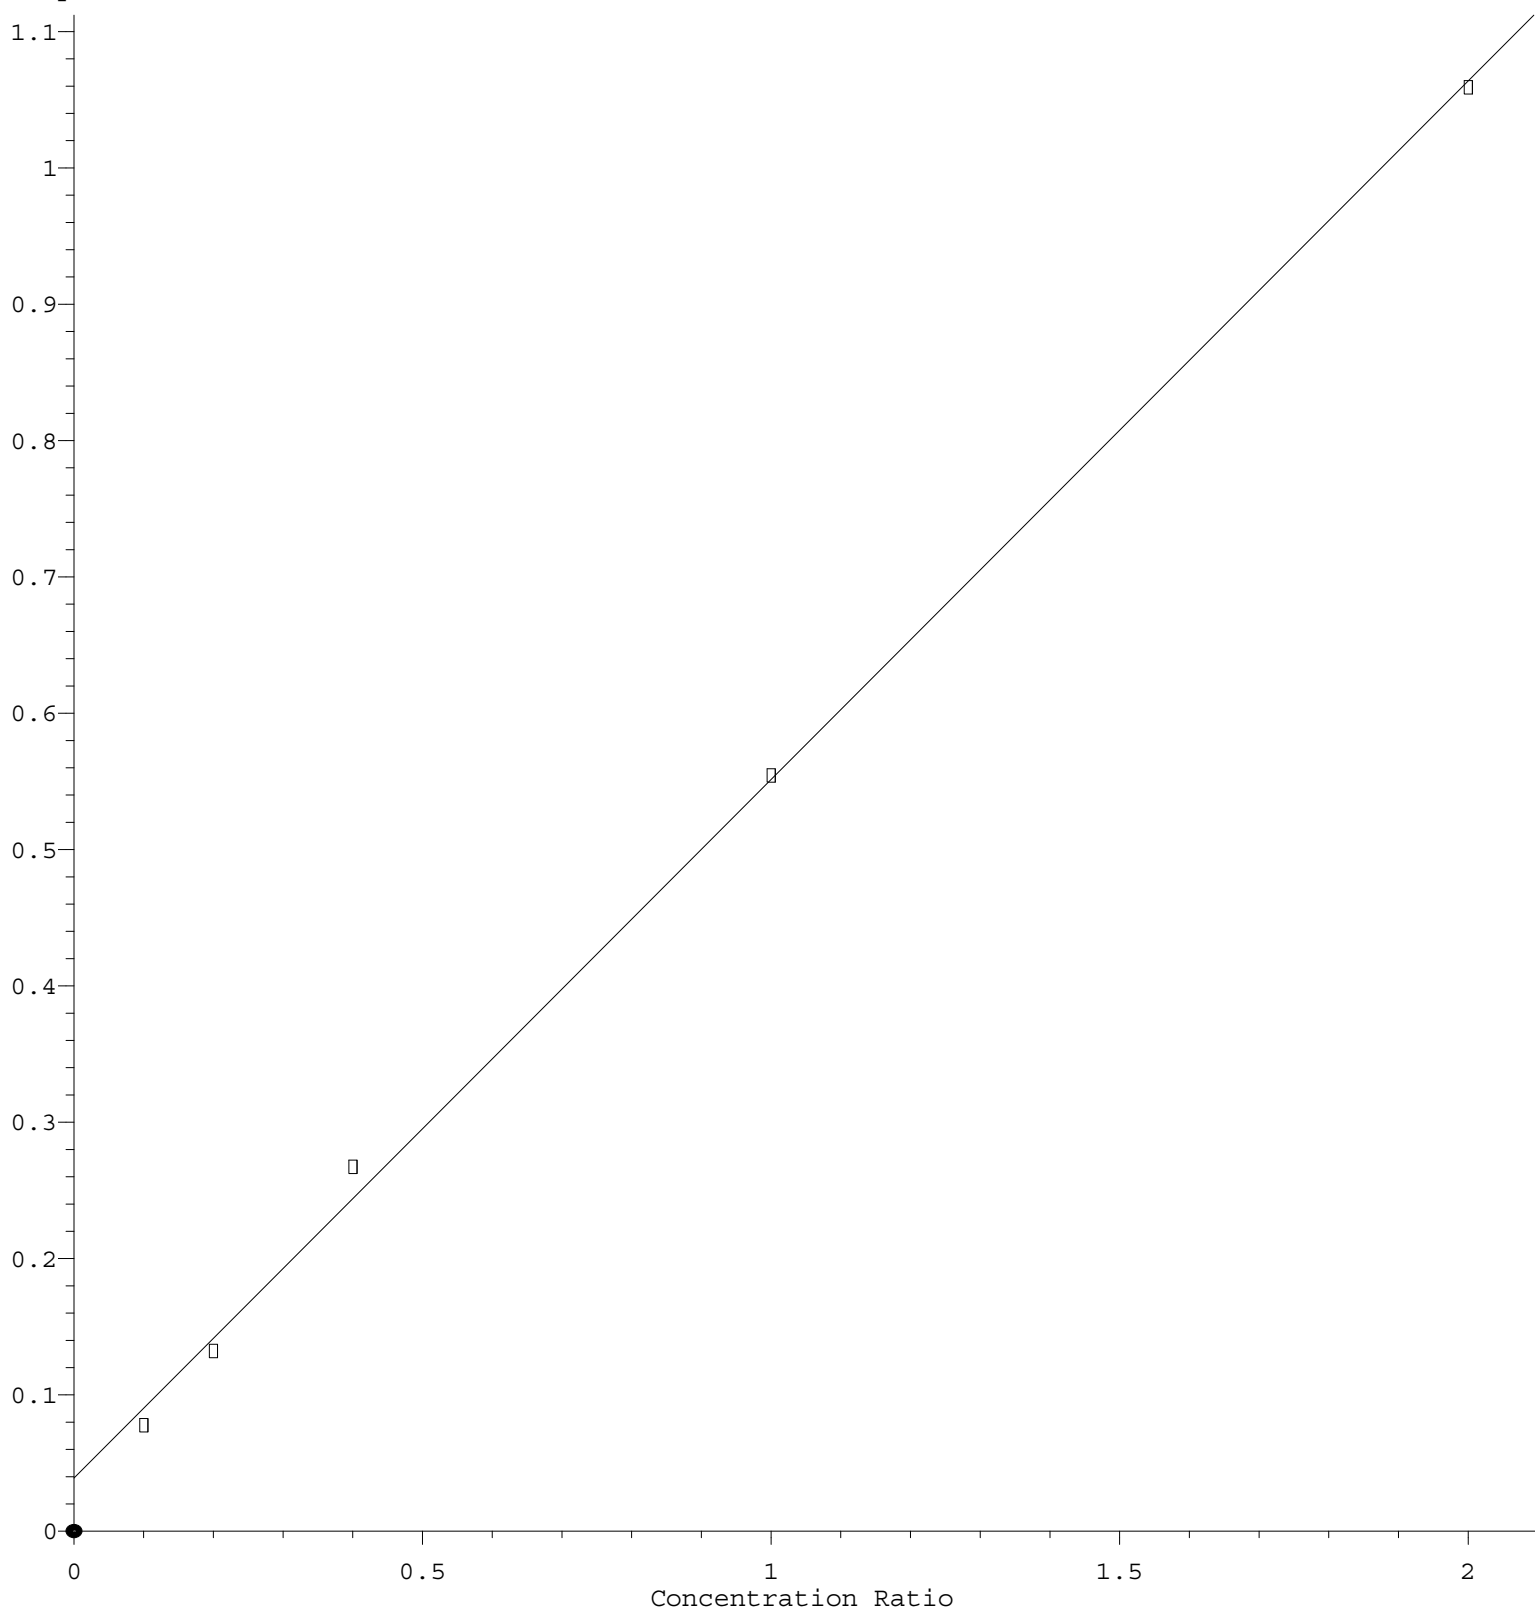

$$\text{Response} = 5.124\text{e-}001 * \text{Amt} + 3.892\text{e-}002$$


Coef of Det (r^2) = 0.998744 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M

Calibration Table Last Updated: Tue Aug 31 02:20:58 2021

2-Chloroethyl Vinyl ether

Response Ratio

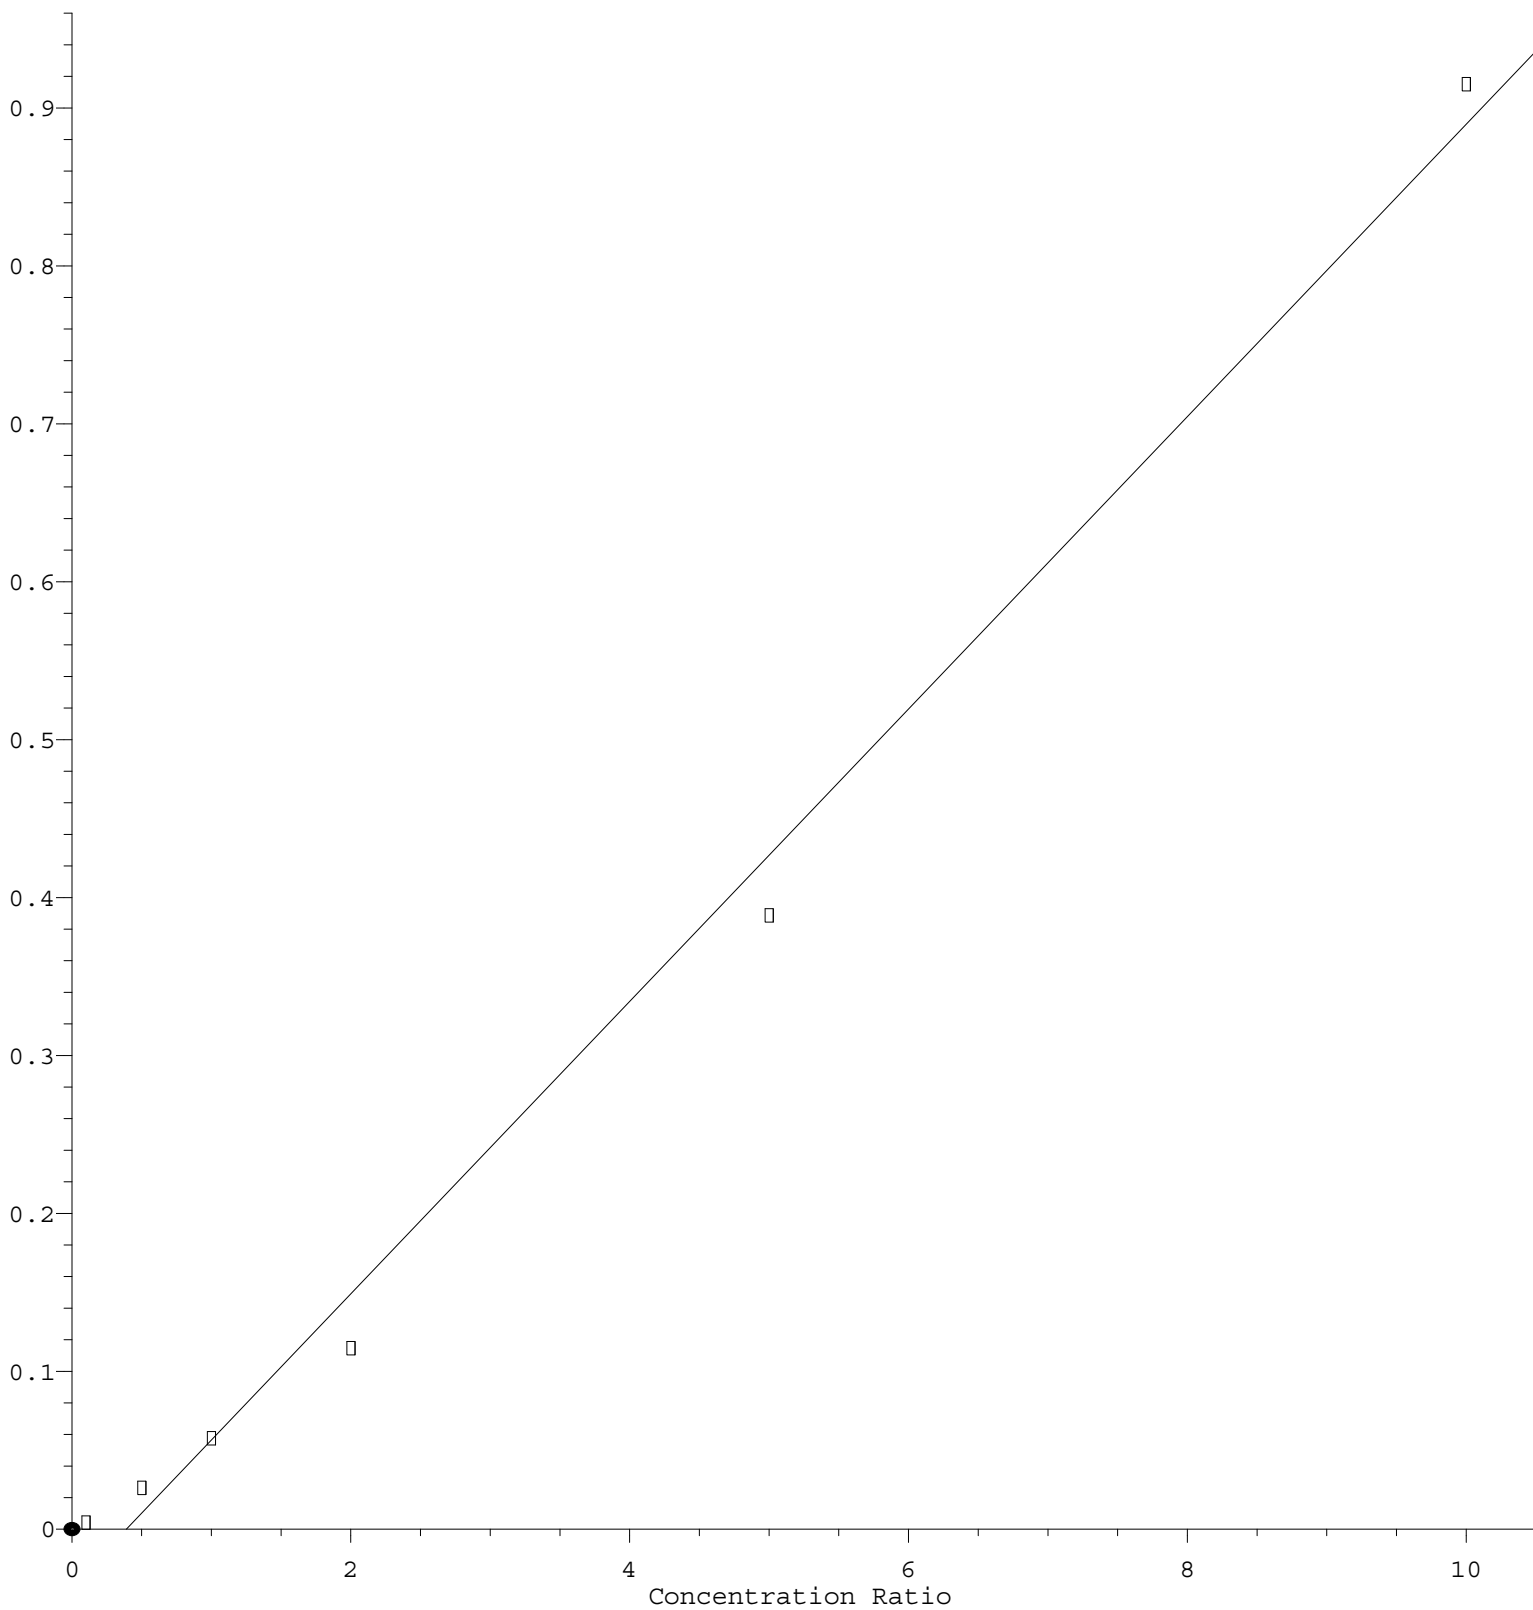


$$\text{Response} = 9.263\text{e-}002 * \text{Amt} - 3.610\text{e-}002$$

Coef of Det (r^2) = 0.992827 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M

Calibration Table Last Updated: Tue Aug 31 02:20:58 2021


Bromoform

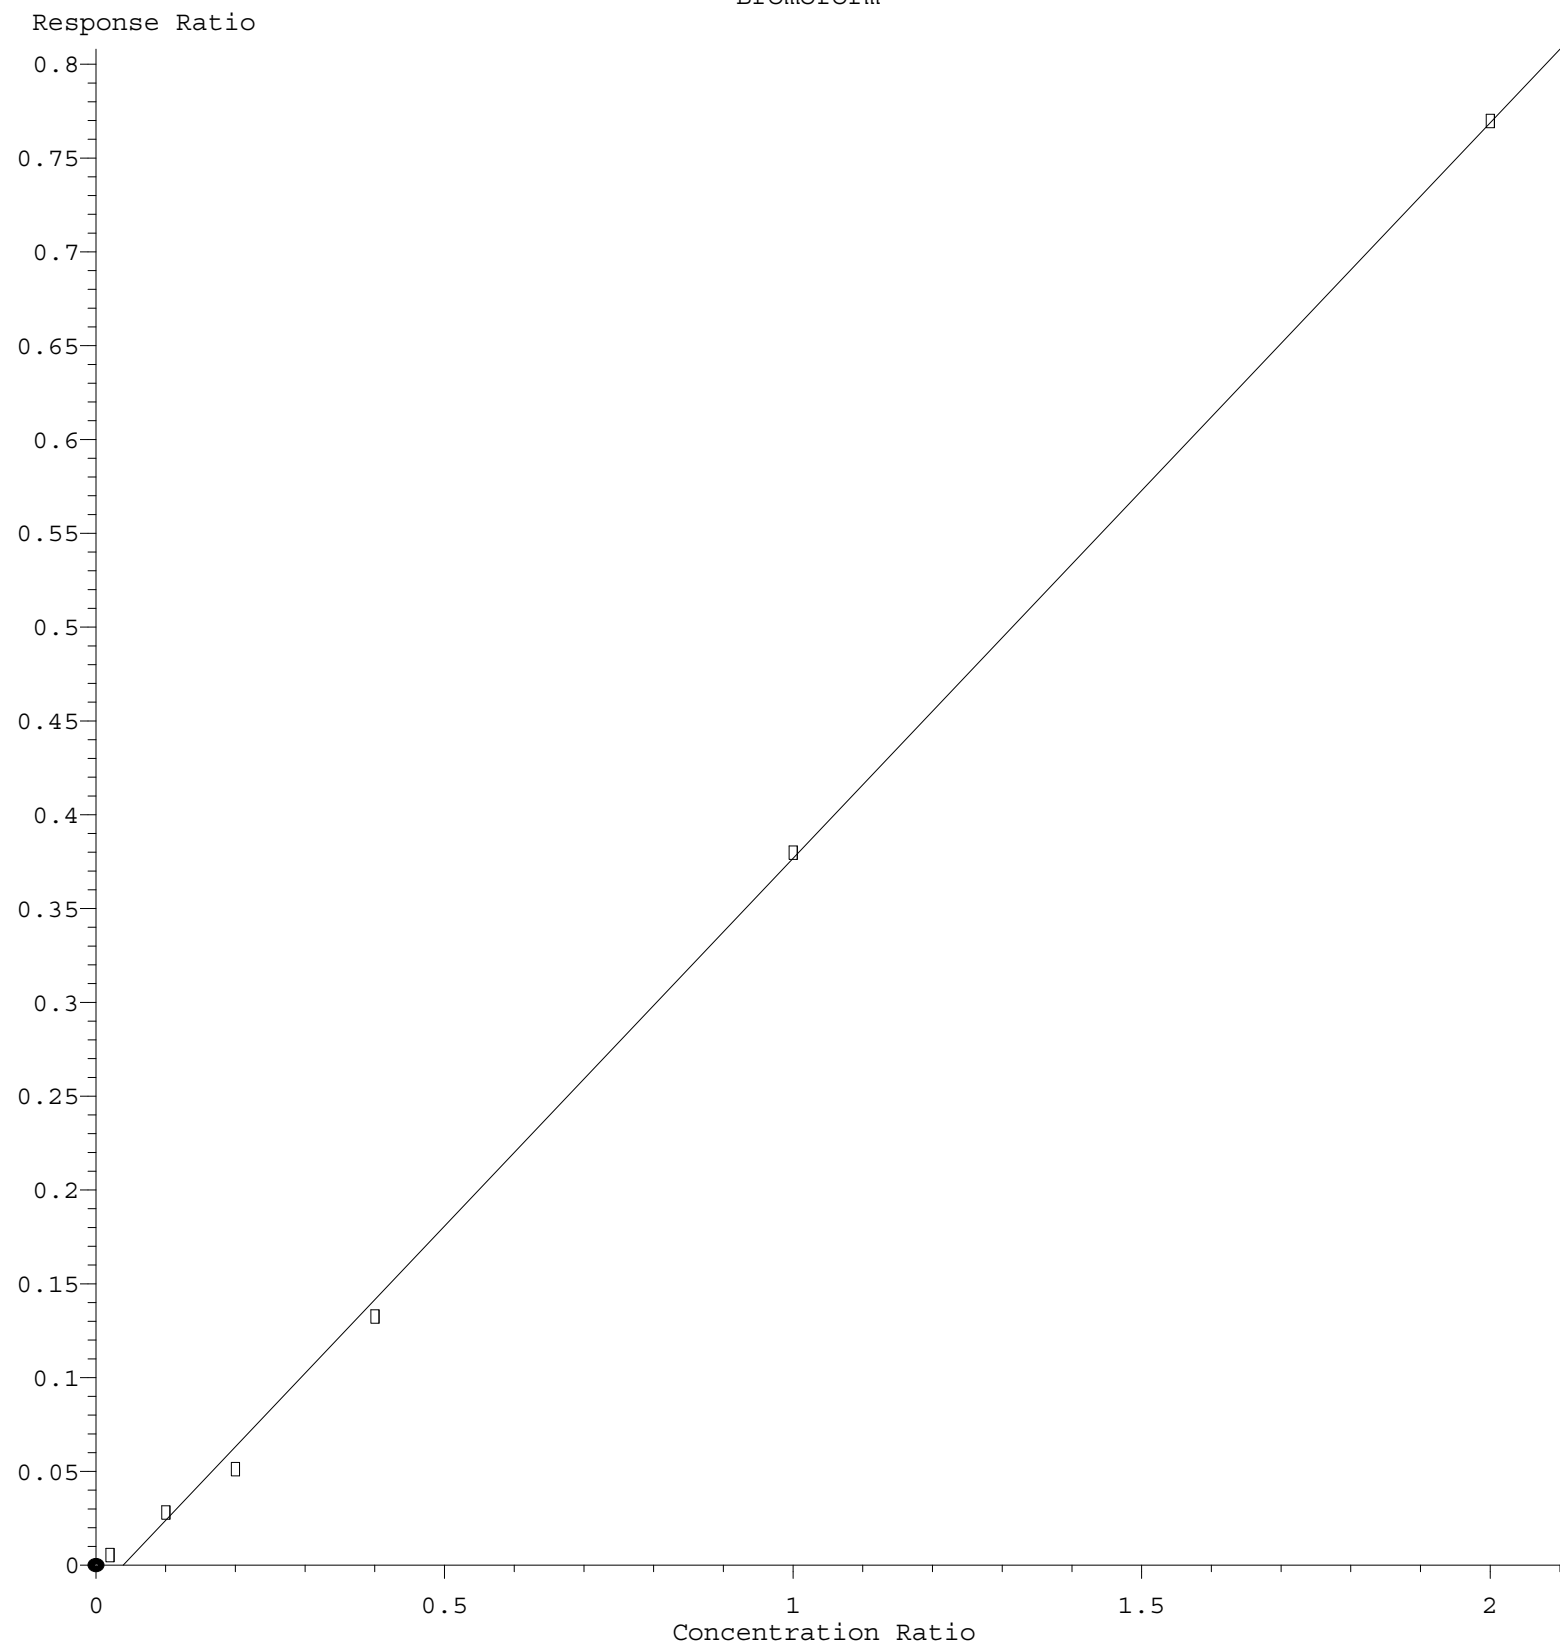

Response = $3.919 \times 10^{-1} \times \text{Amt} - 1.521 \times 10^{-2}$
 Coef of Det (r^2) = 0.999071 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M
 Calibration Table Last Updated: Tue Aug 31 02:20:58 2021

1,2,4-Trichlorobenzene

Response Ratio

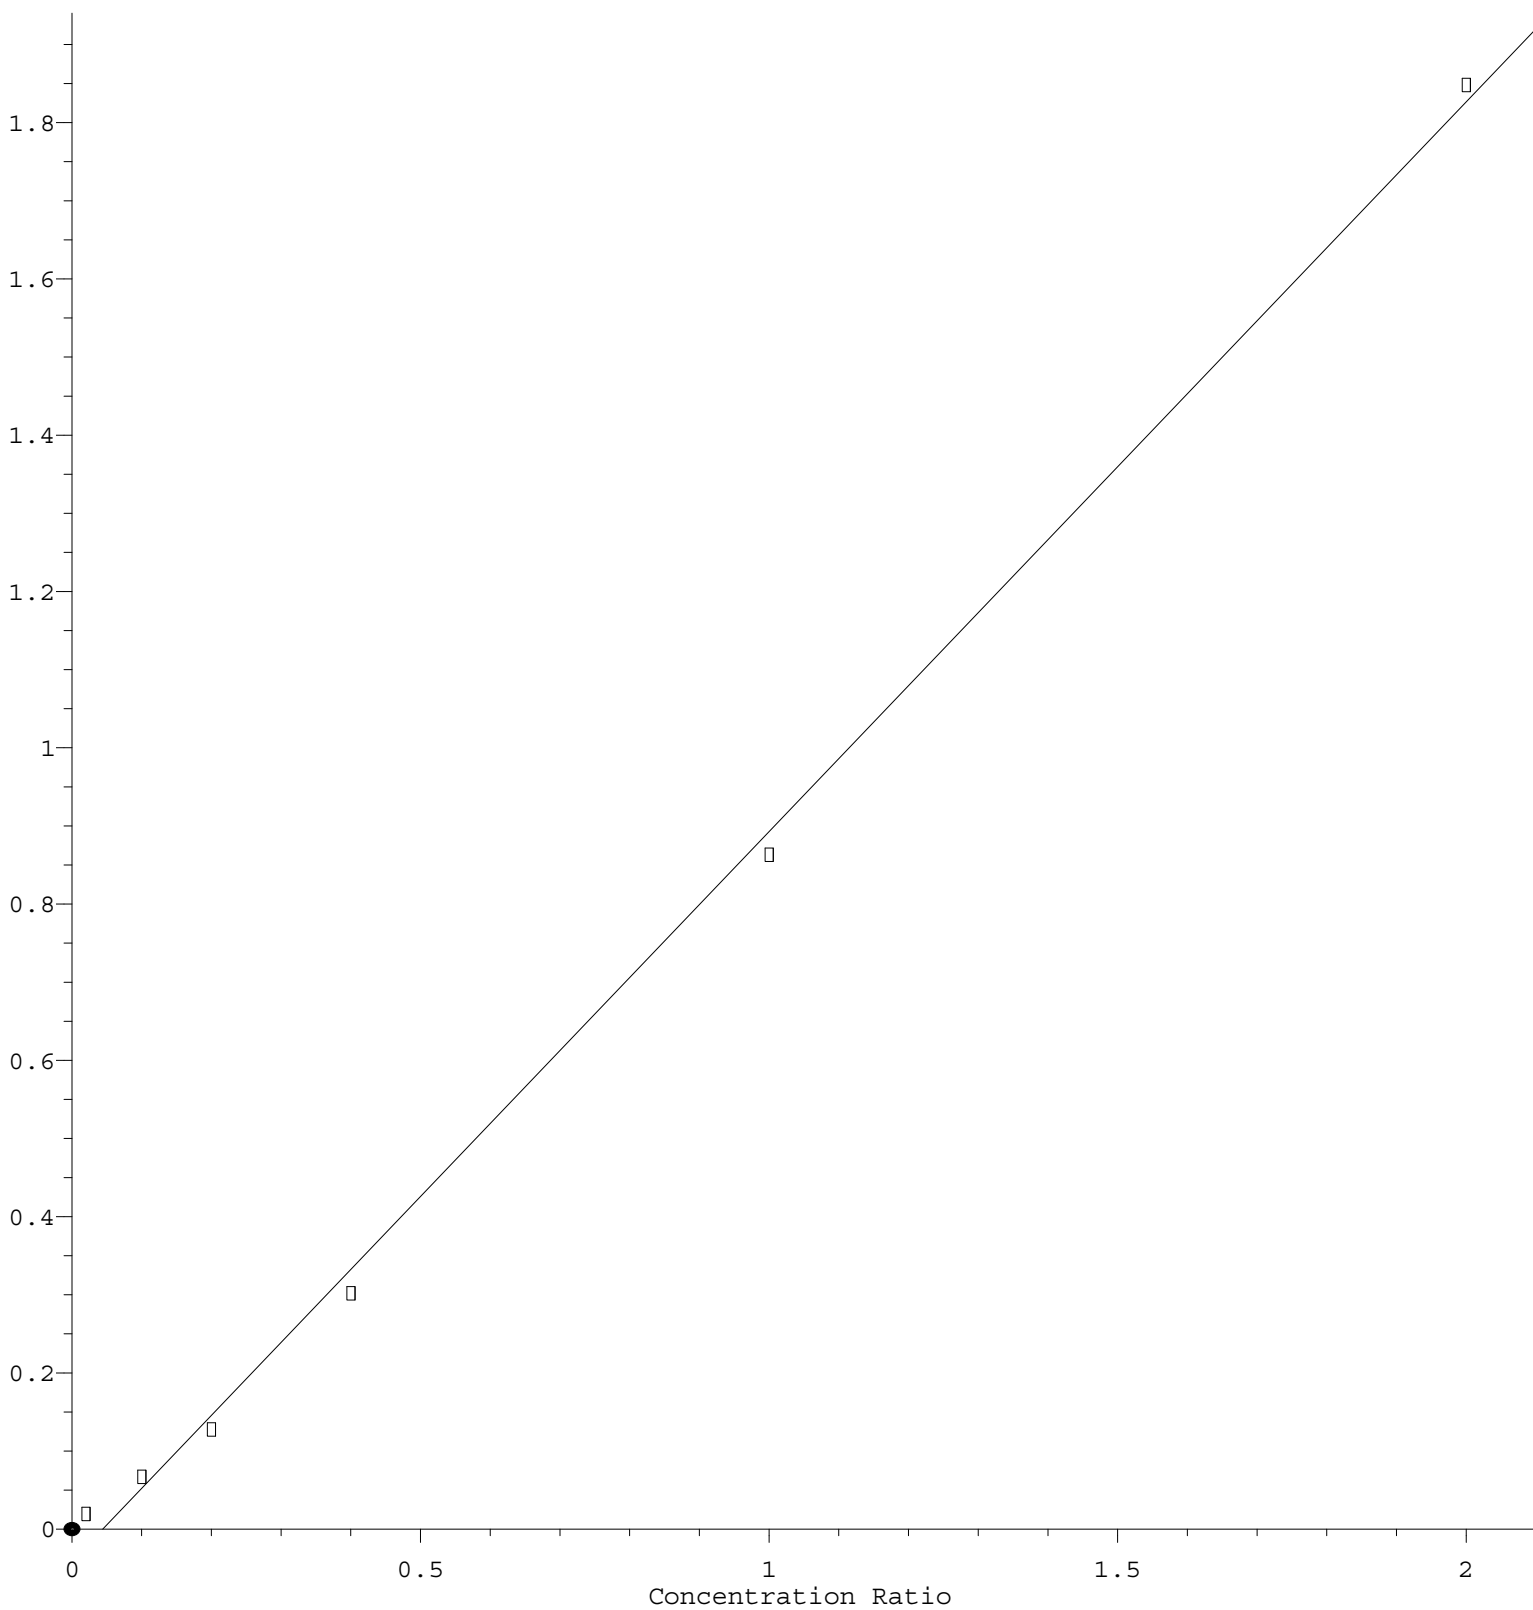

$$\text{Response} = 9.338\text{e-}001 * \text{Amt} - 4.120\text{e-}002$$


Coef of Det (r^2) = 0.998197 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M

Calibration Table Last Updated: Tue Aug 31 02:20:58 2021

Naphthalene


Response Ratio

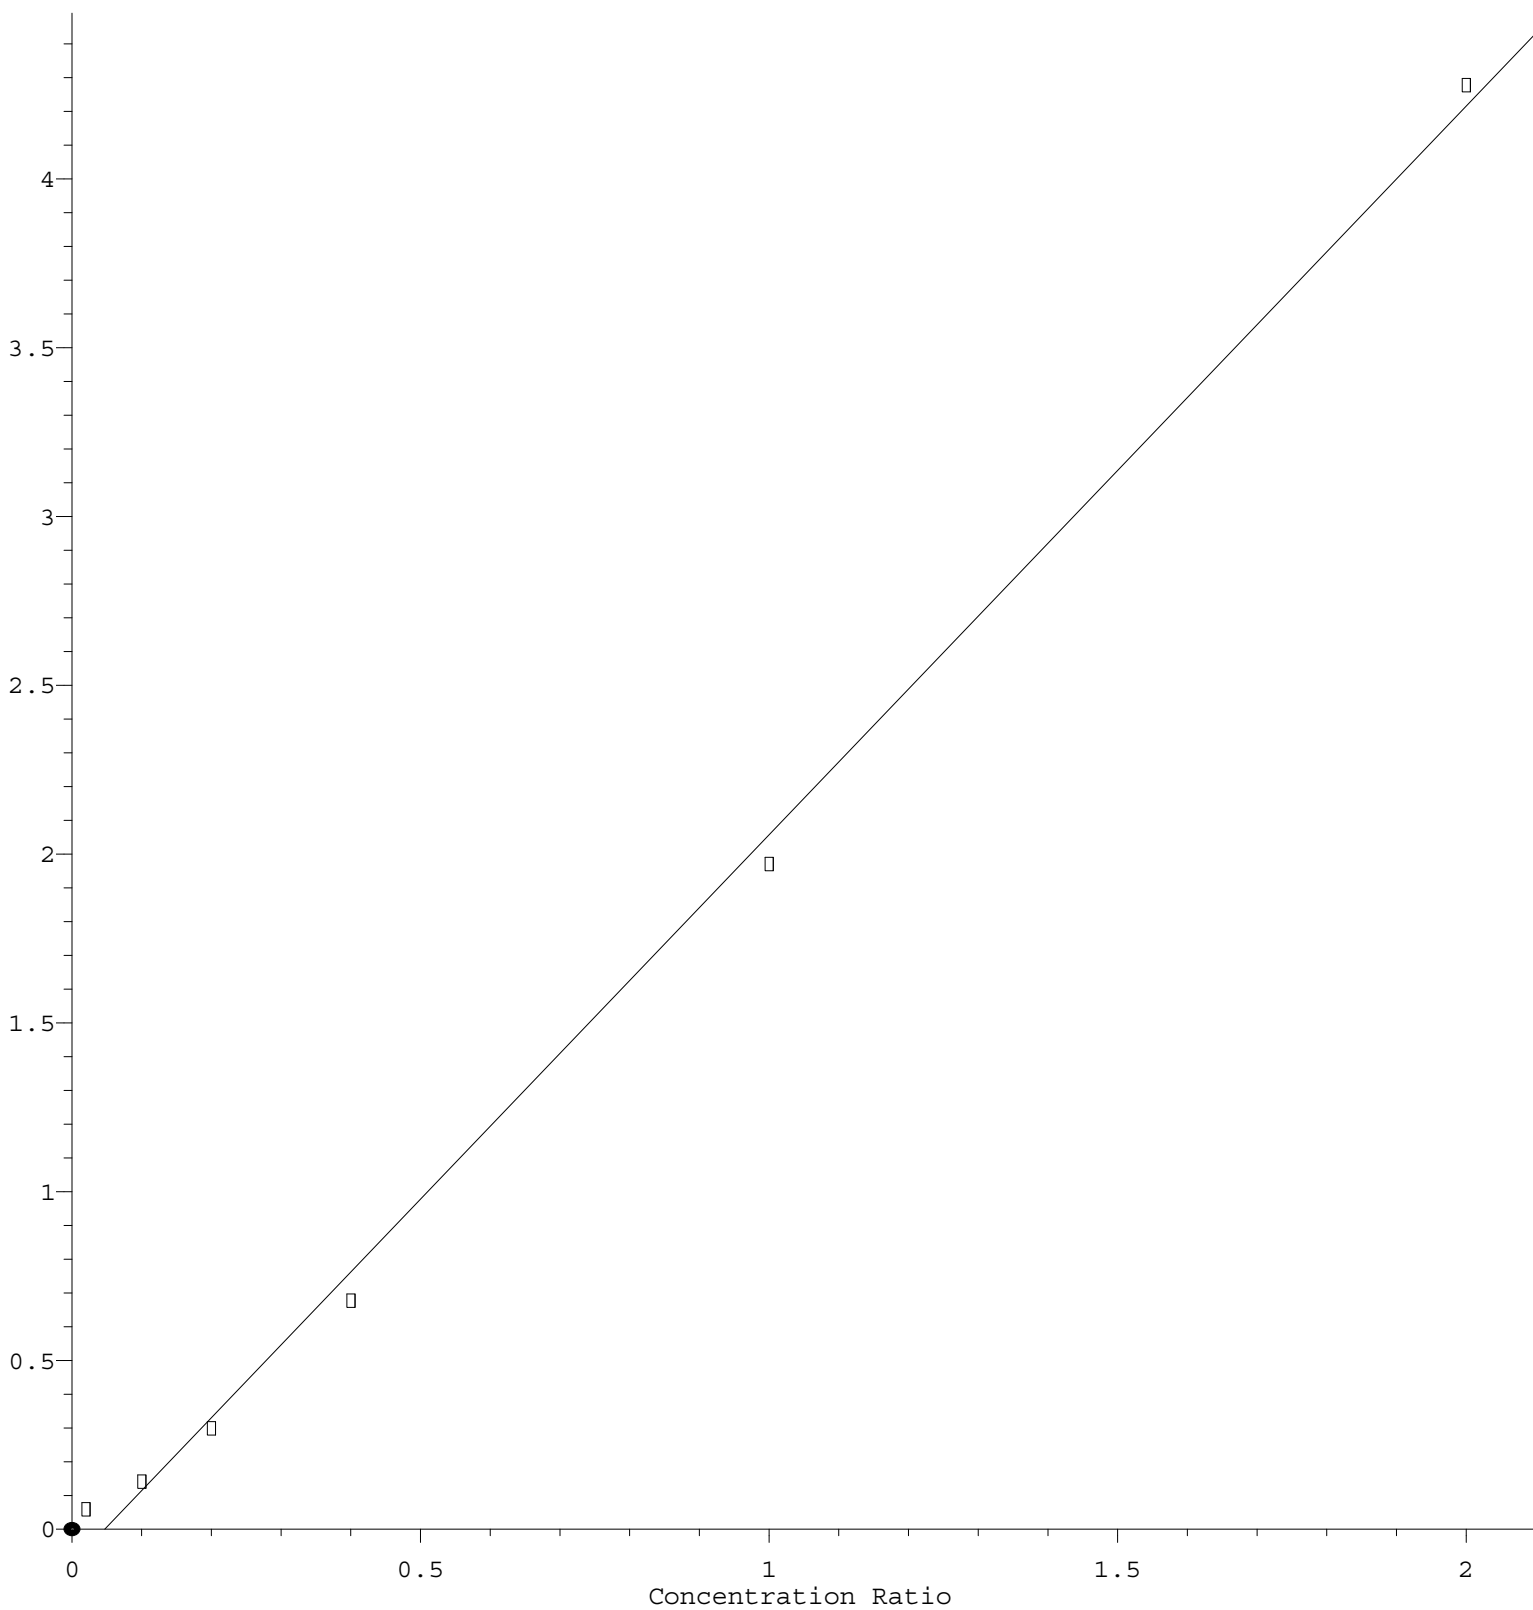

Response = 2.159e+000 * Amt - 1.012e-001
 Coef of Det (r^2) = 0.997495 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M
 Calibration Table Last Updated: Tue Aug 31 02:20:58 2021

1,2,3-Trichlorobenzene

Response Ratio

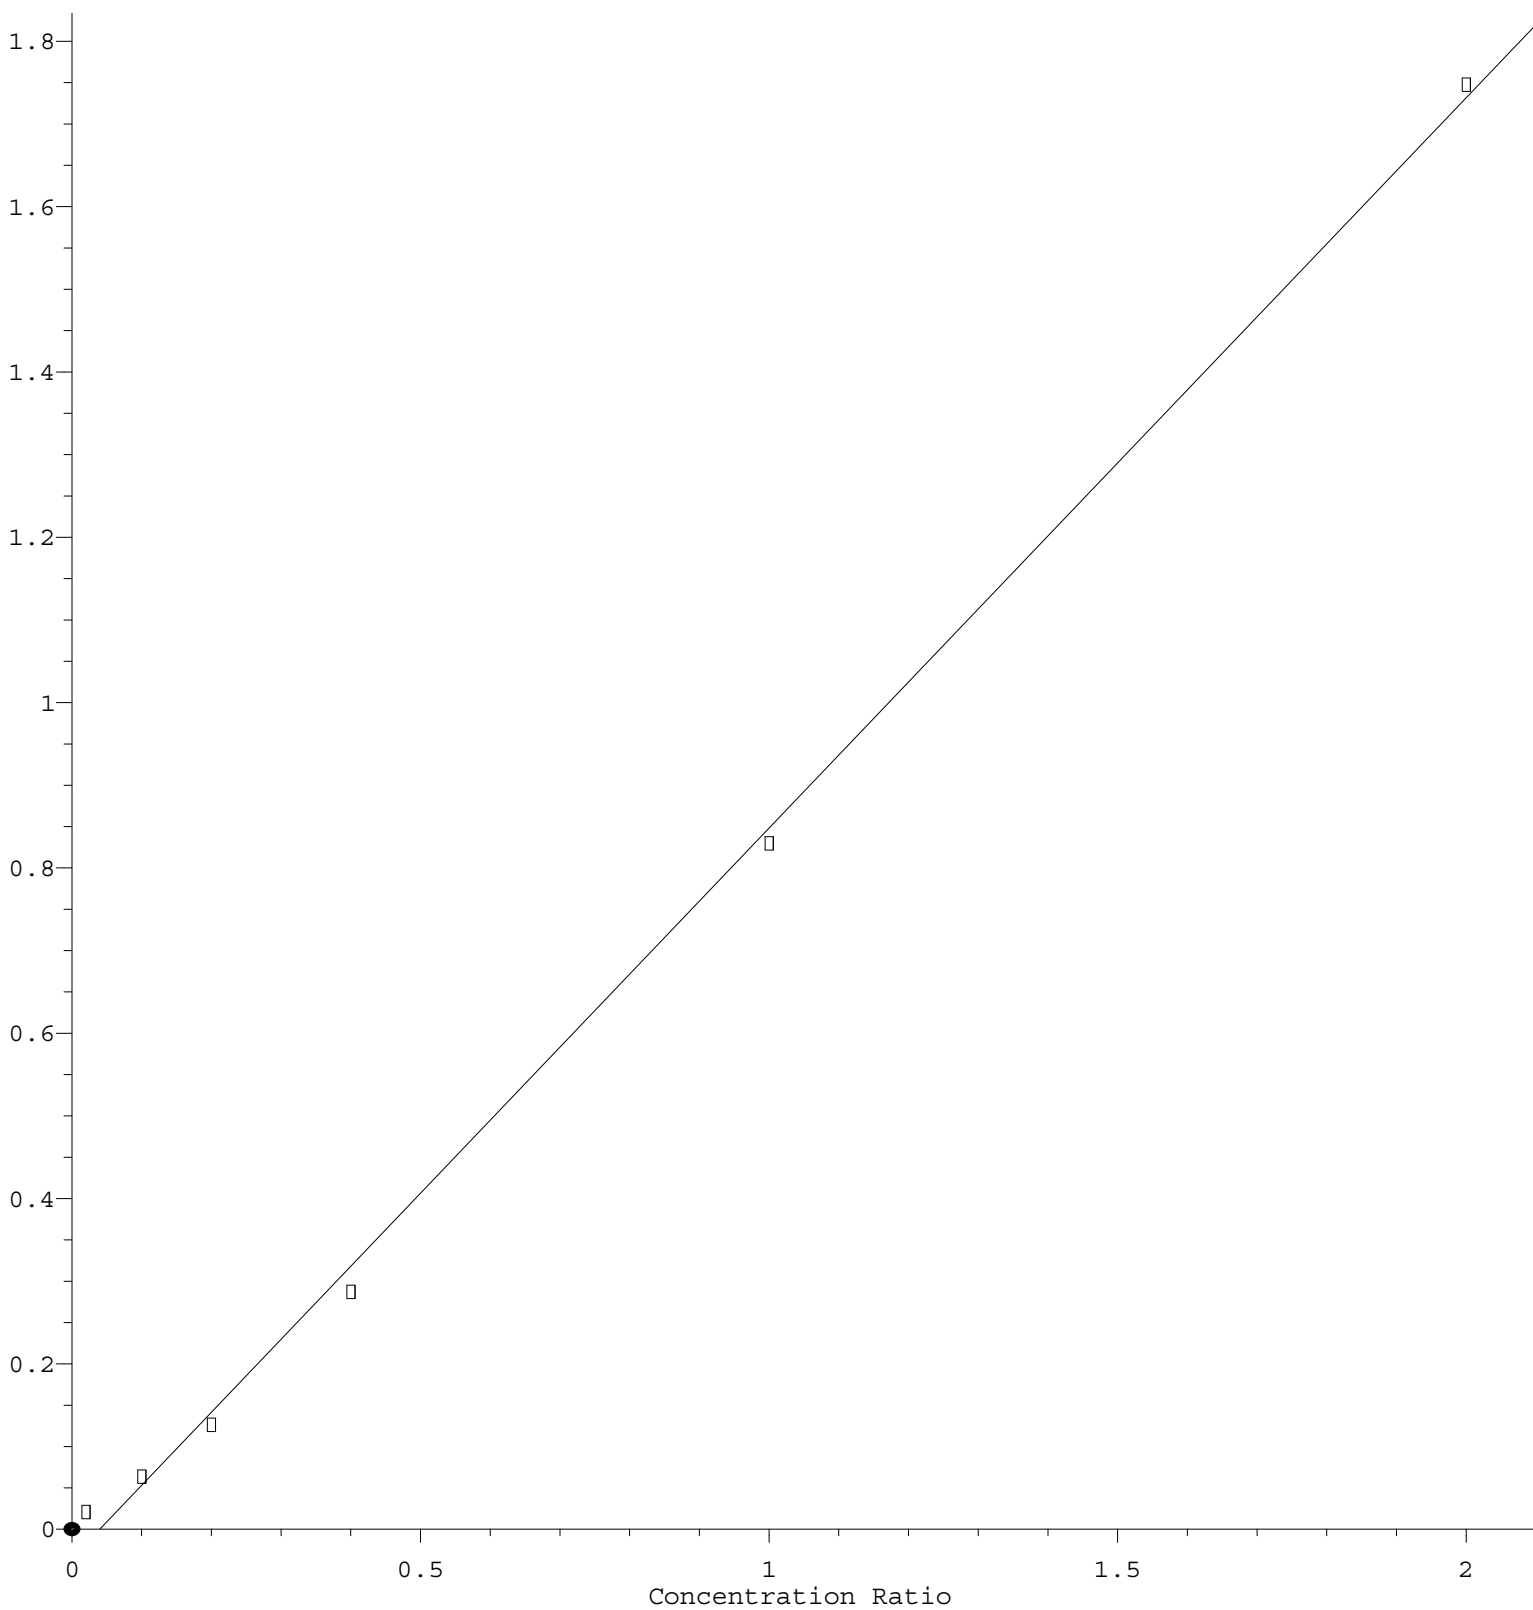

$$\text{Response} = 8.833\text{e-}001 * \text{Amt} - 3.523\text{e-}002$$


Coef of Det (r^2) = 0.998518 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M

Calibration Table Last Updated: Tue Aug 31 02:20:58 2021

Acetone

Response Ratio

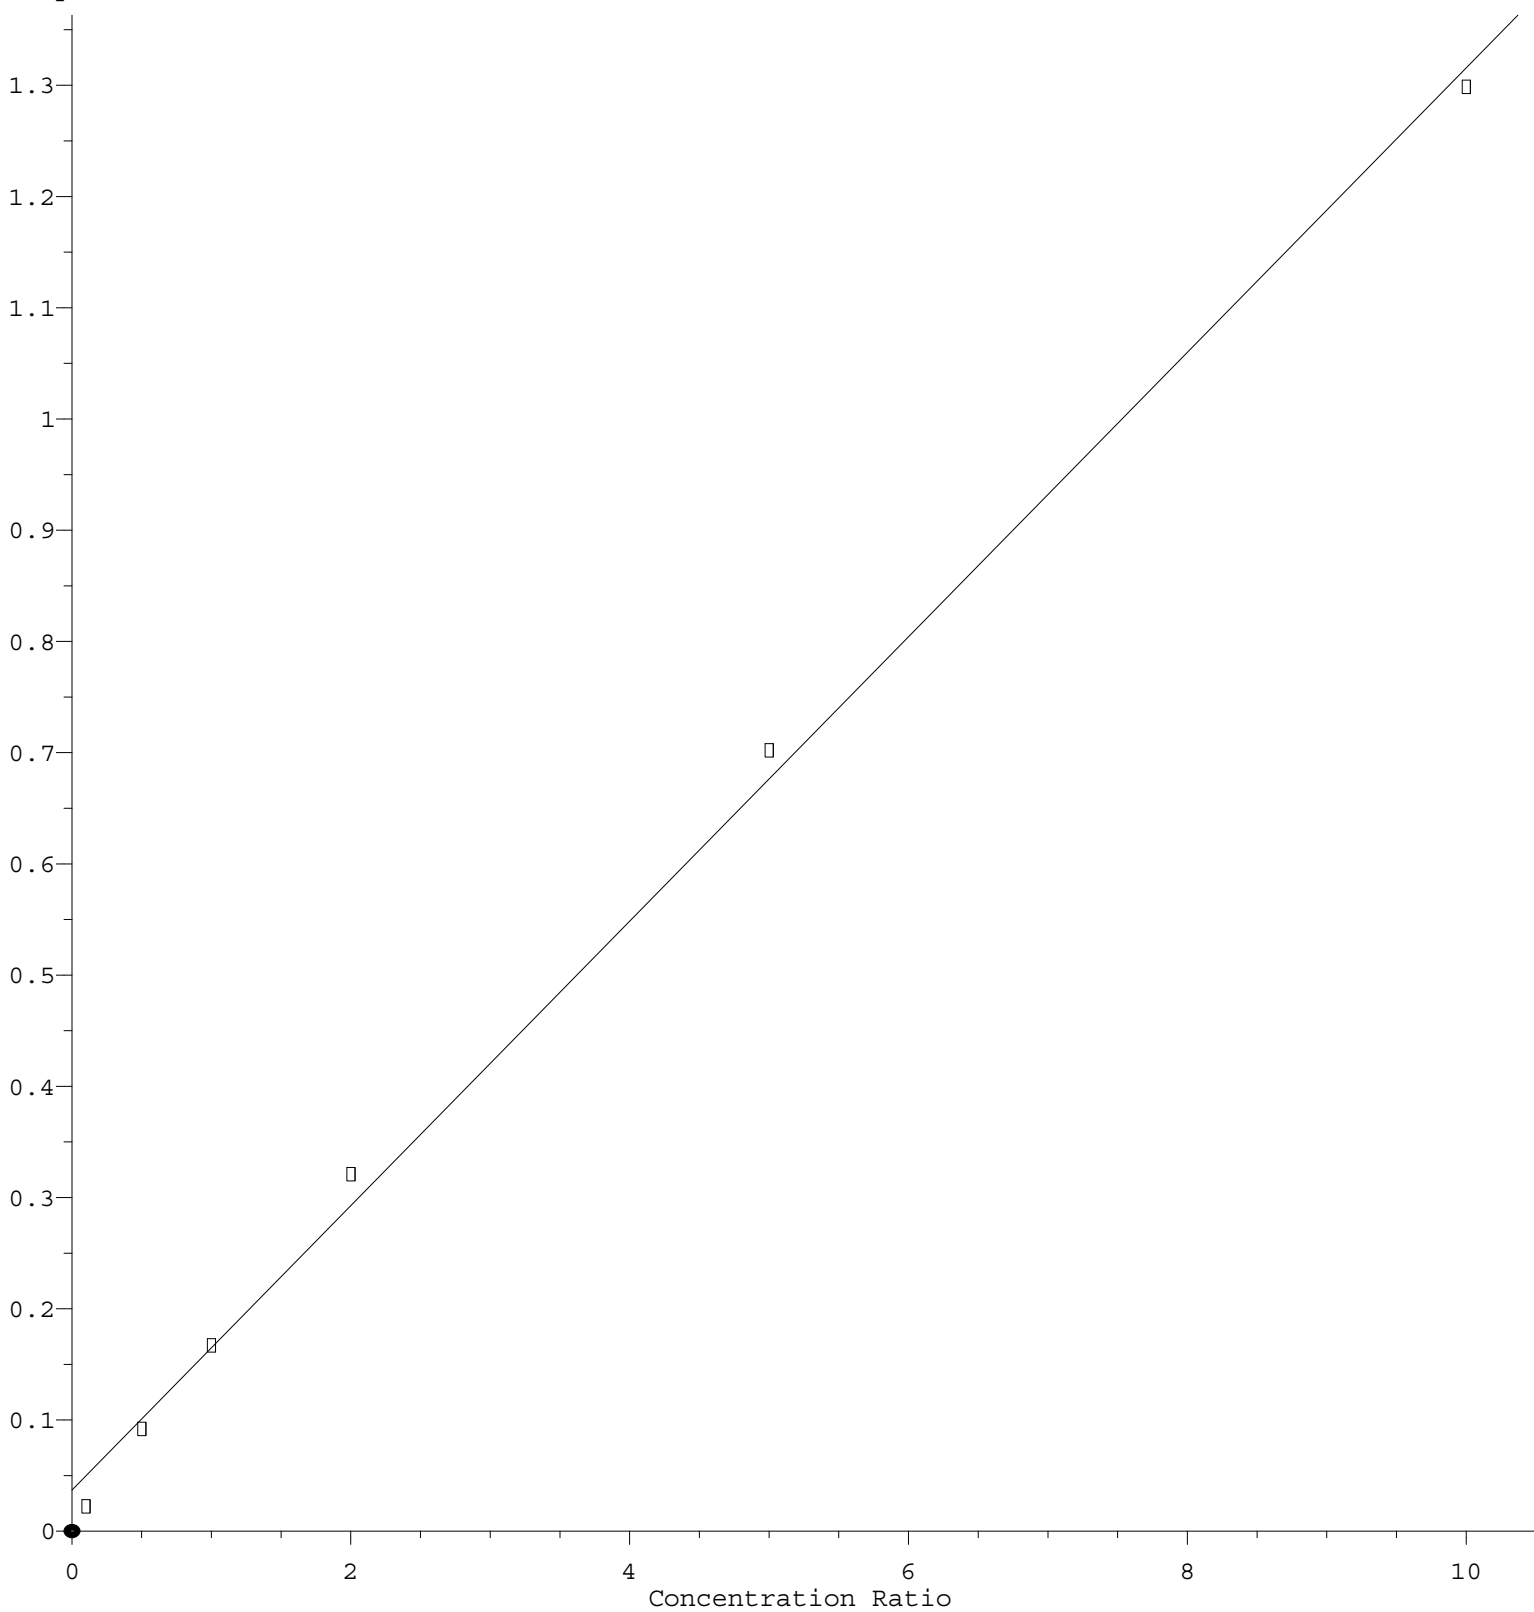


$$\text{Response} = 1.279\text{e-}001 * \text{Amt} + 3.737\text{e-}002$$

Coef of Det (r^2) = 0.997827 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M

Calibration Table Last Updated: Tue Aug 31 02:20:58 2021


Methyl Acetate

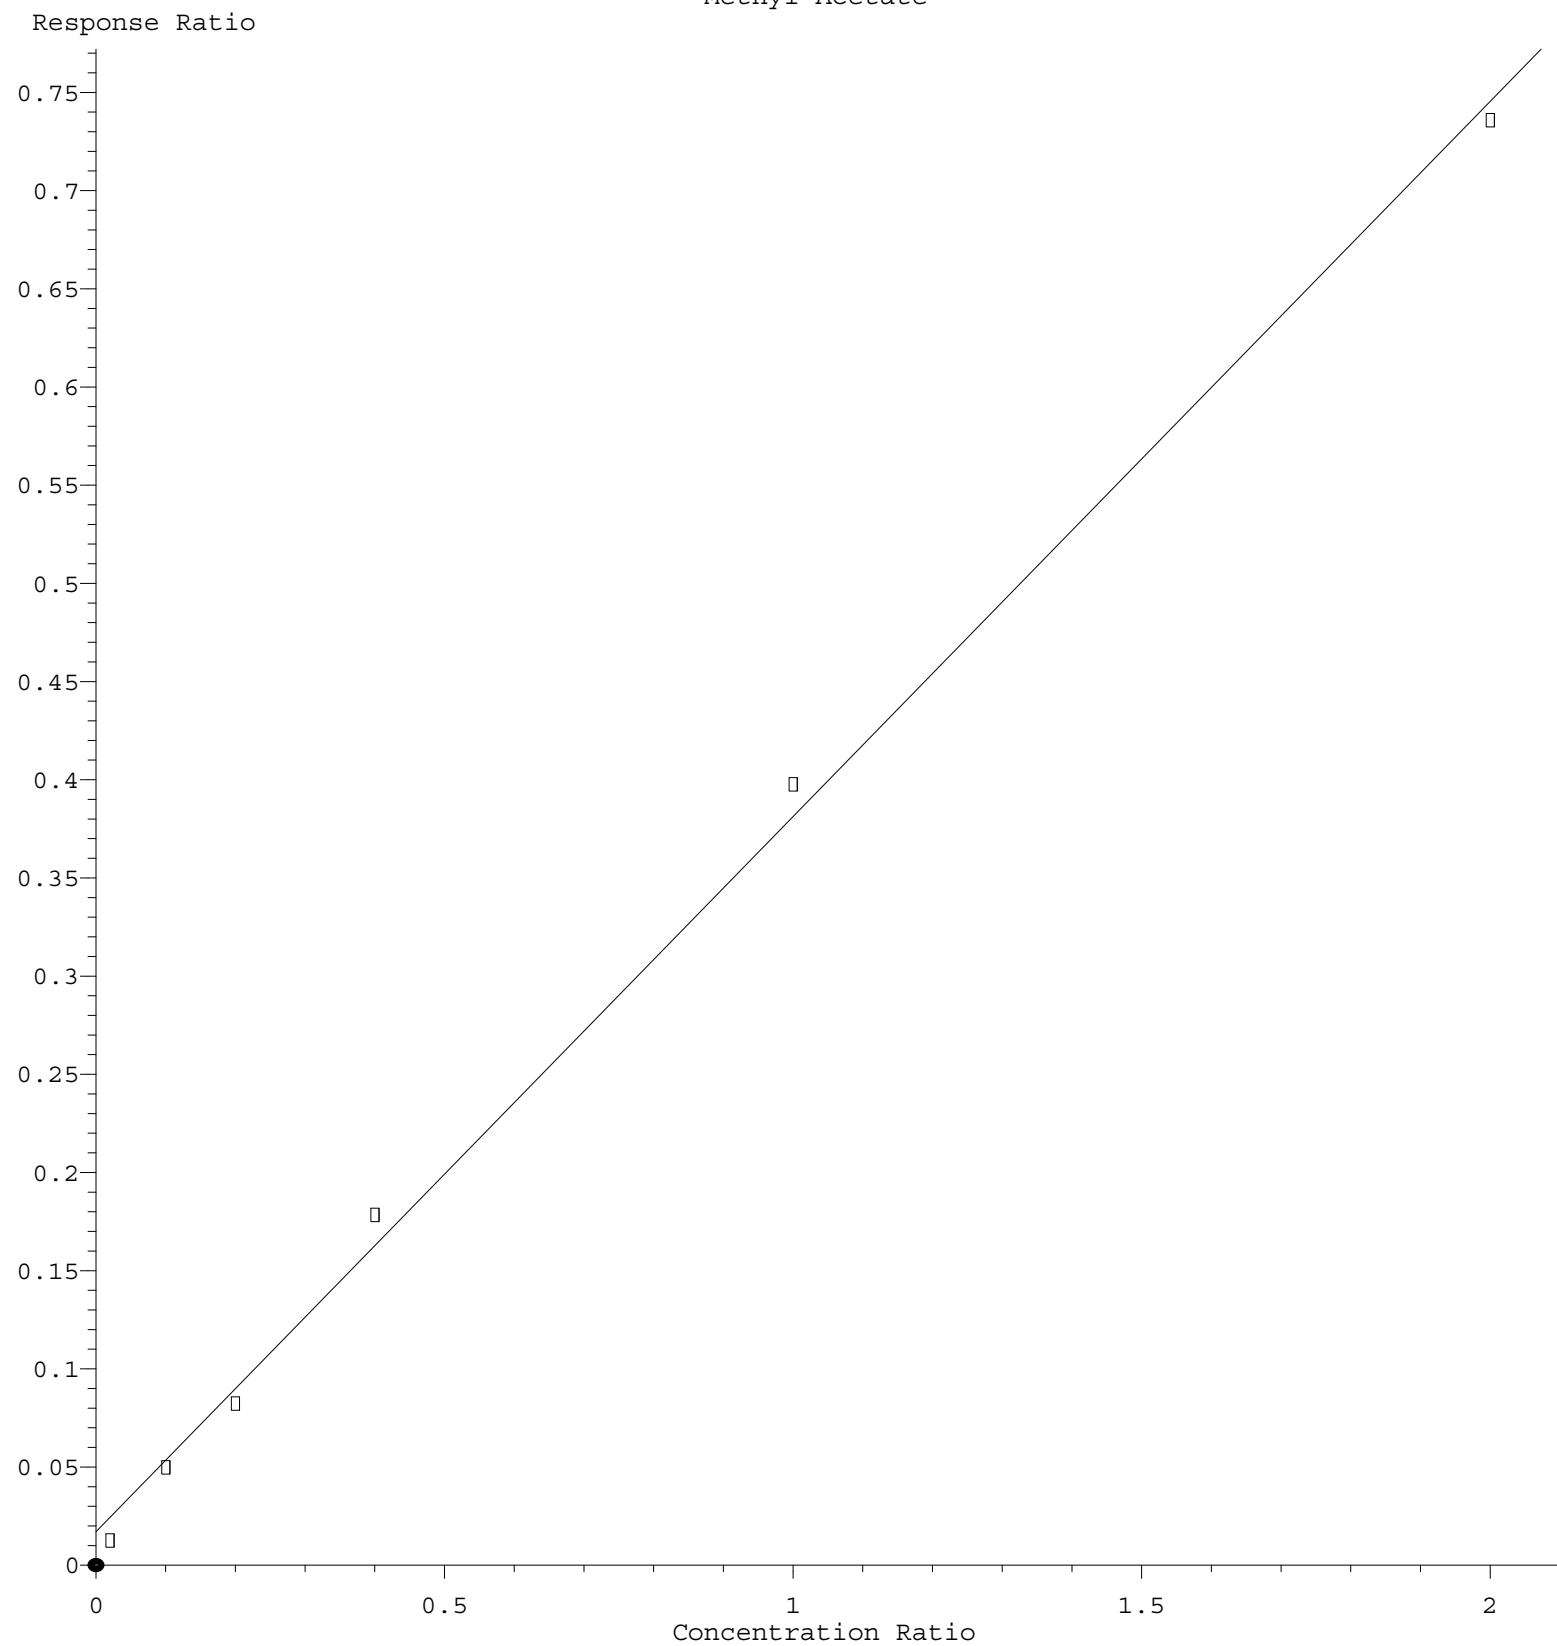

Response = 3.648e-001 * Amt + 1.656e-002
 Coef of Det (r^2) = 0.997898 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M
 Calibration Table Last Updated: Tue Aug 31 02:20:58 2021

Methylene Chloride


Response Ratio

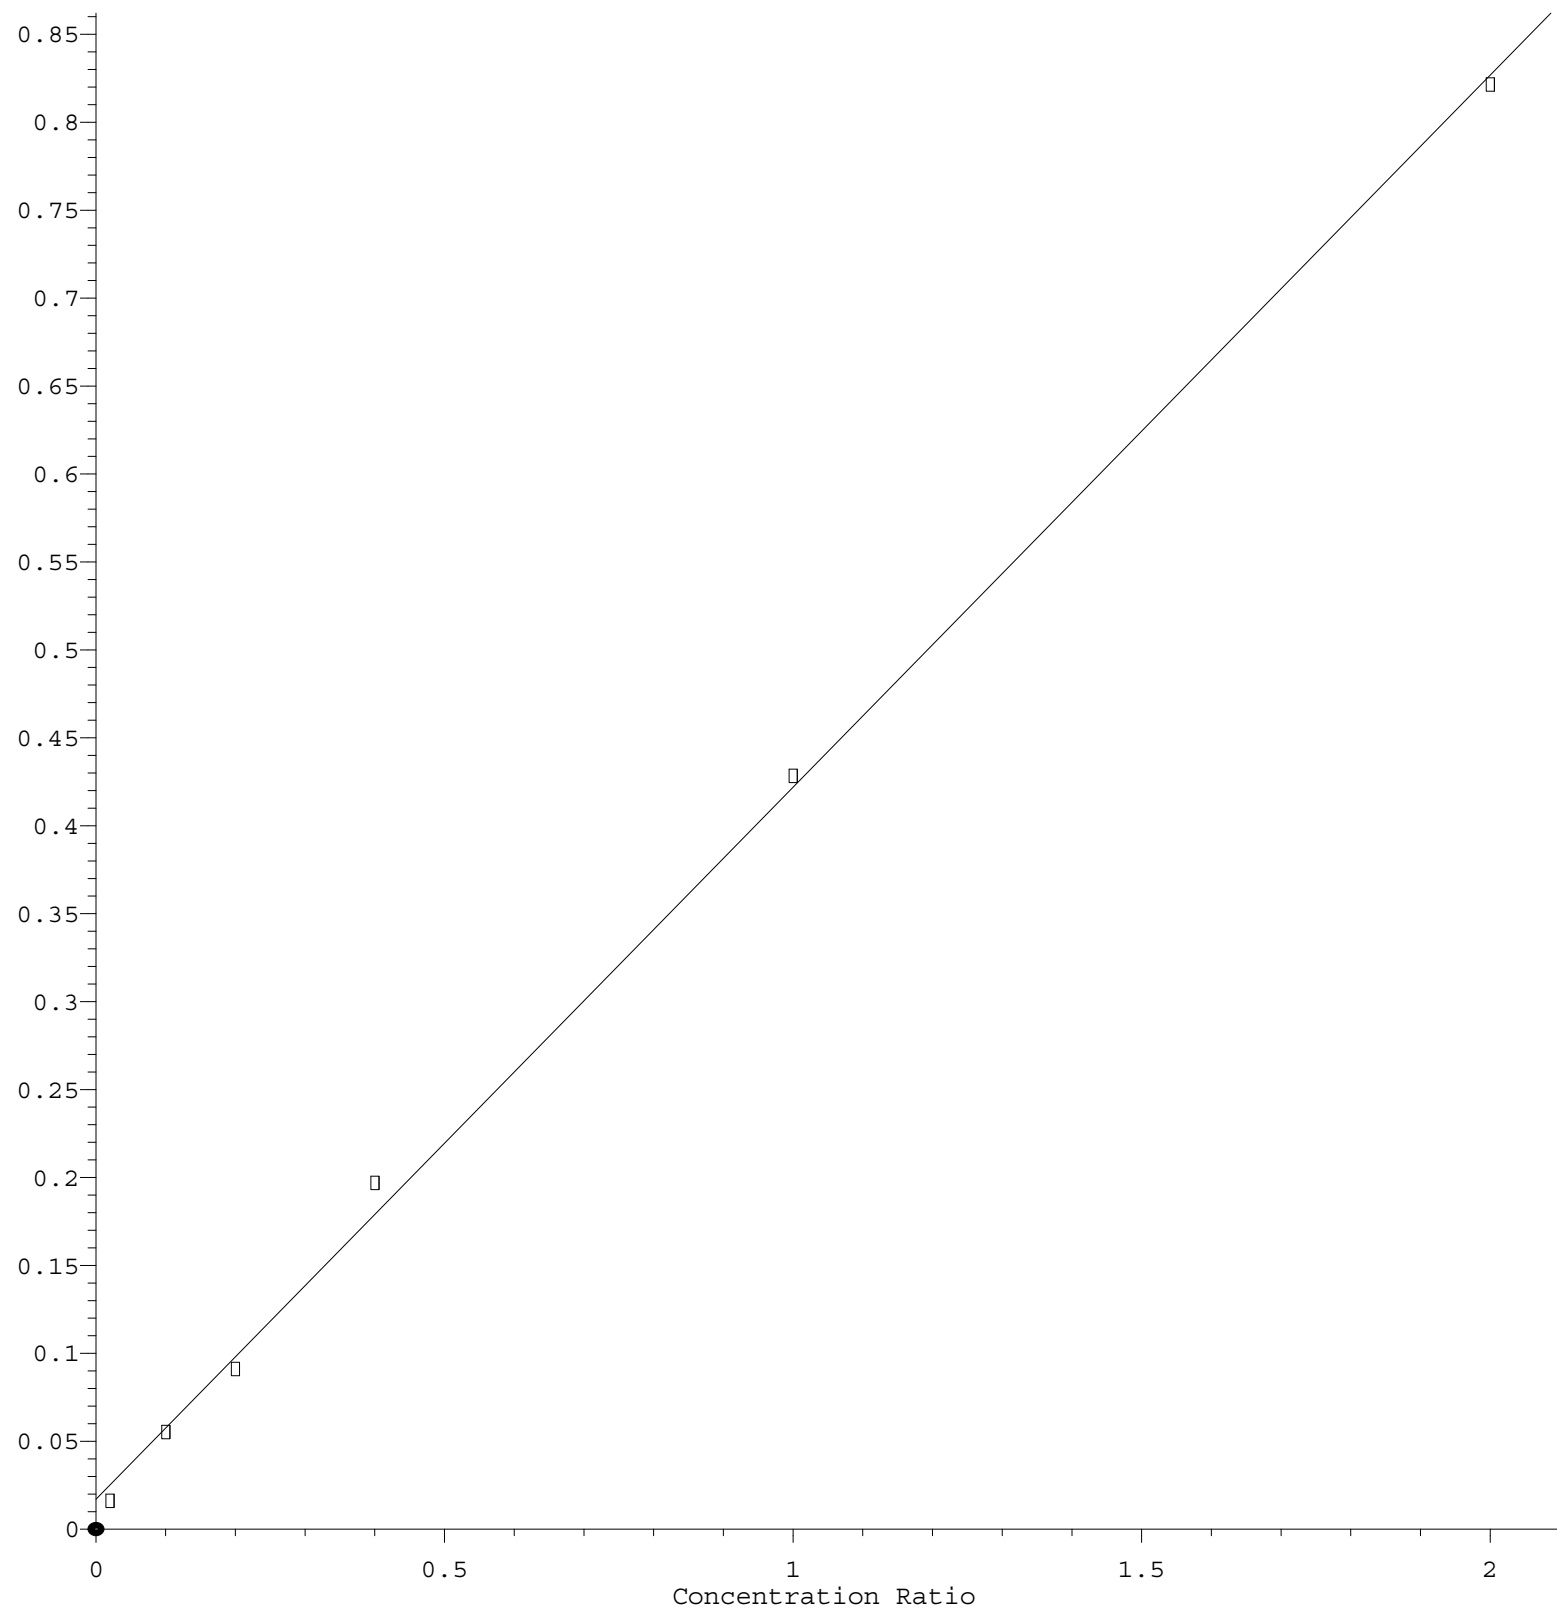

Response = 4.051e-001 * Amt + 1.701e-002
 Coef of Det (r^2) = 0.998897 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M
 Calibration Table Last Updated: Tue Aug 31 02:20:58 2021

Ethyl methacrylate

Response Ratio

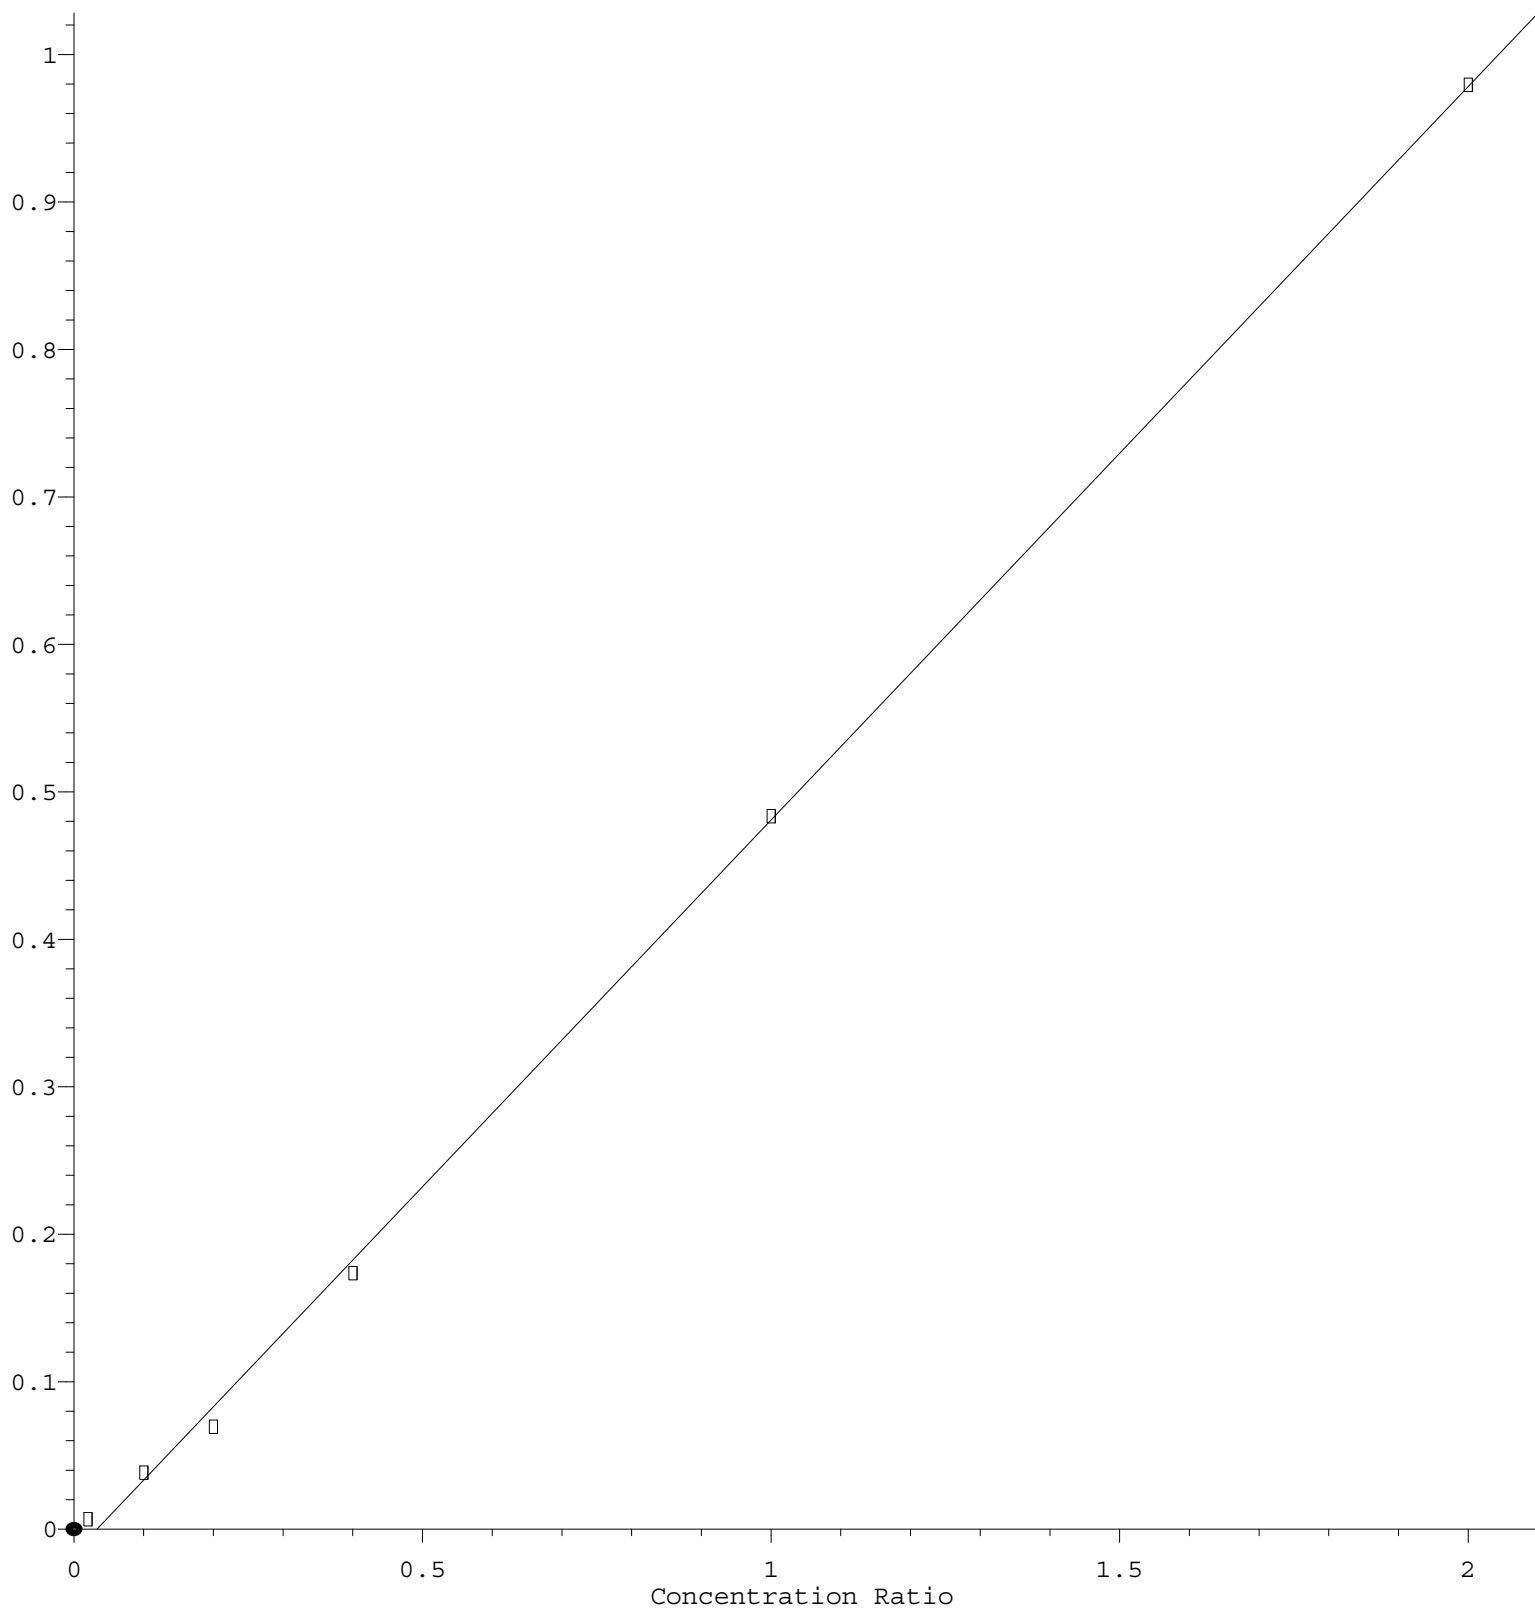

$$\text{Response} = 4.972\text{e-}001 * \text{Amt} - 1.647\text{e-}002$$

Coef of Det (r^2) = 0.999342 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N083021W.M

Calibration Table Last Updated: Tue Aug 31 02:20:58 2021