
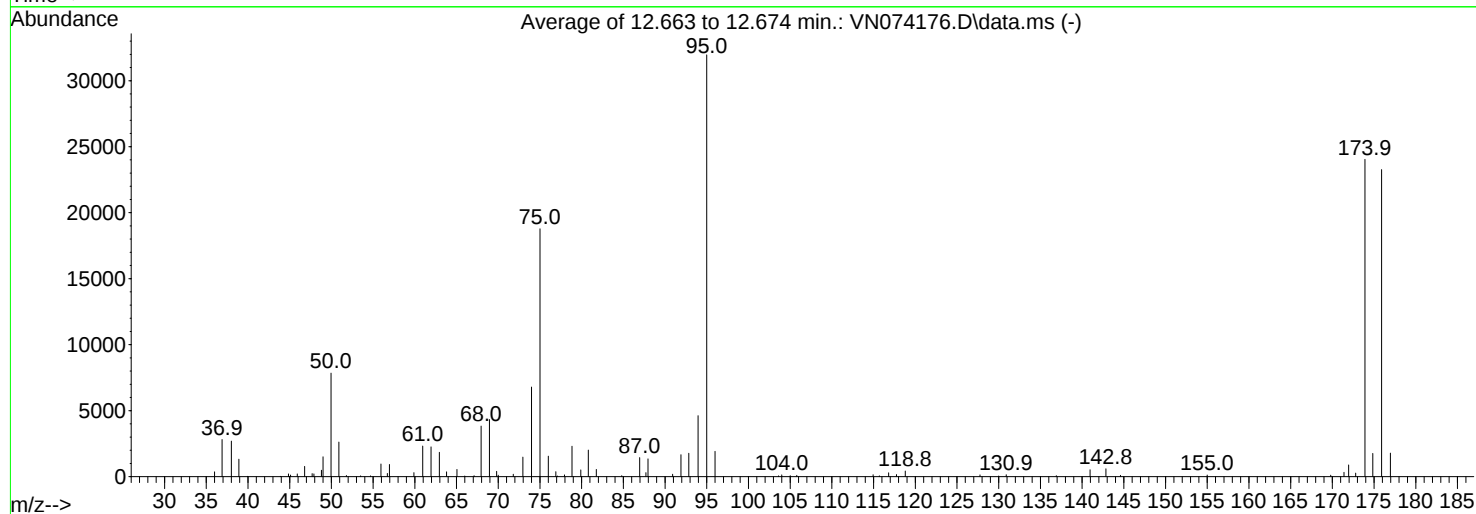


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083022\
Data File : VN074176.D
Acq On : 30 Aug 2022 19:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083022W.M
Title : SW846 8260
Last Update : Wed Aug 31 07:02:40 2022

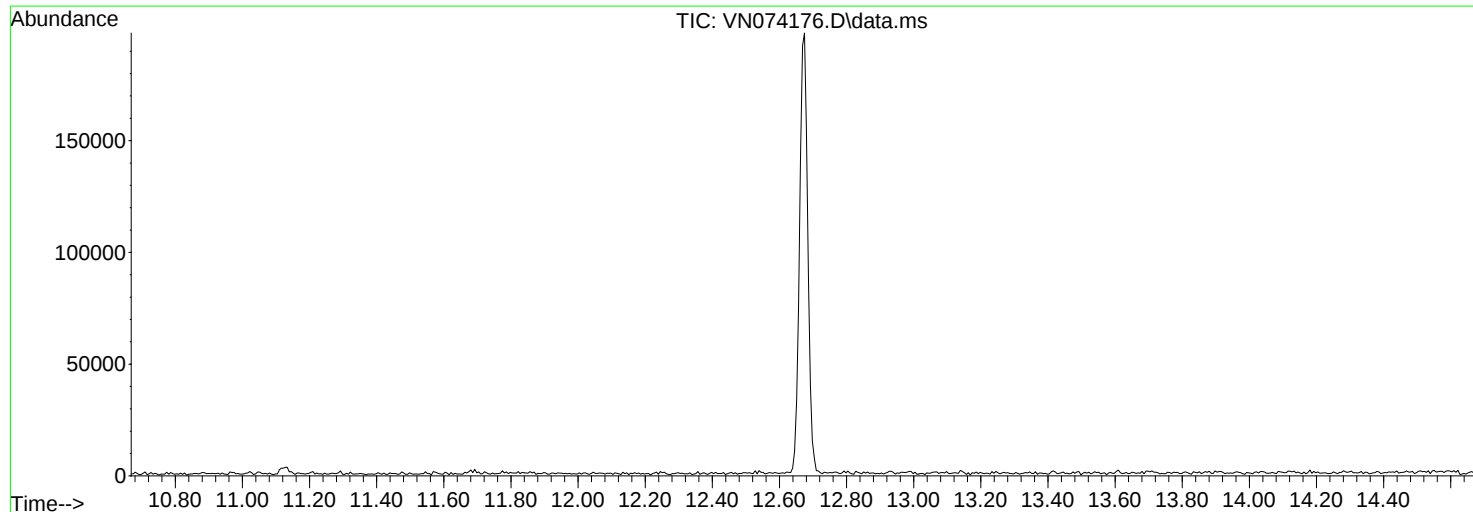

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	7842	PASS
75	95	30	60	58.8	18782	PASS
95	95	100	100	100.0	31960	PASS
96	95	5	9	6.0	1918	PASS
173	174	0.00	2	1.1	267	PASS
174	95	50	100	75.2	24037	PASS
175	174	5	9	7.3	1757	PASS
176	174	95	101	96.8	23267	PASS
177	176	5	9	7.7	1788	PASS