
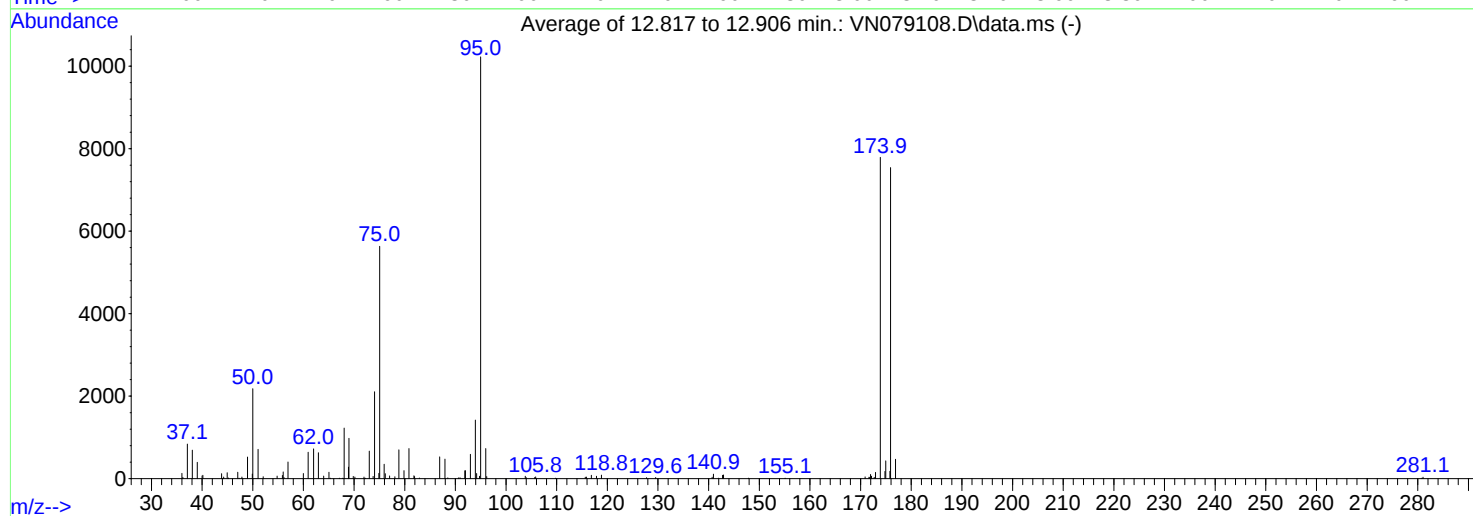


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083023\
 Data File : VN079108.D
 Acq On : 30 Aug 2023 10:52
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N081723W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Aug 18 05:21:14 2023

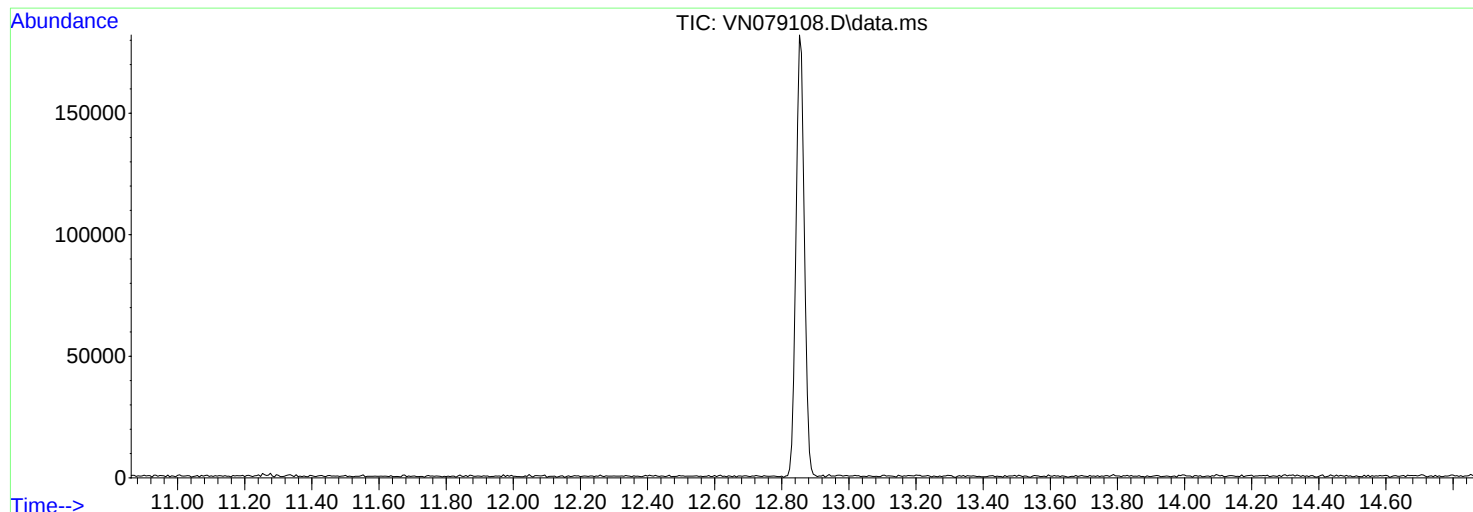

AutoFind: Averaged scan 1847 to 1862; Bkg corrected with scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	2182	PASS
75	95	30	60	55.1	5634	PASS
95	95	100	100	100.0	10226	PASS
96	95	5	9	7.1	728	PASS
173	174	0.00	2	2.0	152	PASS
174	95	50	100	76.2	7788	PASS
175	174	5	9	5.5	430	PASS
176	174	95	101	96.8	7541	PASS
177	176	5	9	6.2	470	PASS