

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
 Data File : VN083572.D
 Acq On : 30 Aug 2024 13:40
 Operator : JC\MD
 Sample : VN0830MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0830MBL01

Quant Time: Aug 31 02:36:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 31 00:48:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	146014	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	294290	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	305322	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	140623	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	107430	52.644	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	105.280%
35) Dibromofluoromethane	8.165	113	87449	49.371	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.740%
50) Toluene-d8	10.565	98	312005	45.292	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	90.580%
62) 4-Bromofluorobenzene	12.847	95	140677	55.055	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	110.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
Data File : VN083572.D
Acq On : 30 Aug 2024 13:40
Operator : JC\MD
Sample : VN0830MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0830MBL01

Quant Time: Aug 31 02:36:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Quant Title : SW846 8260
QLast Update : Sat Aug 31 00:48:10 2024
Response via : Initial Calibration




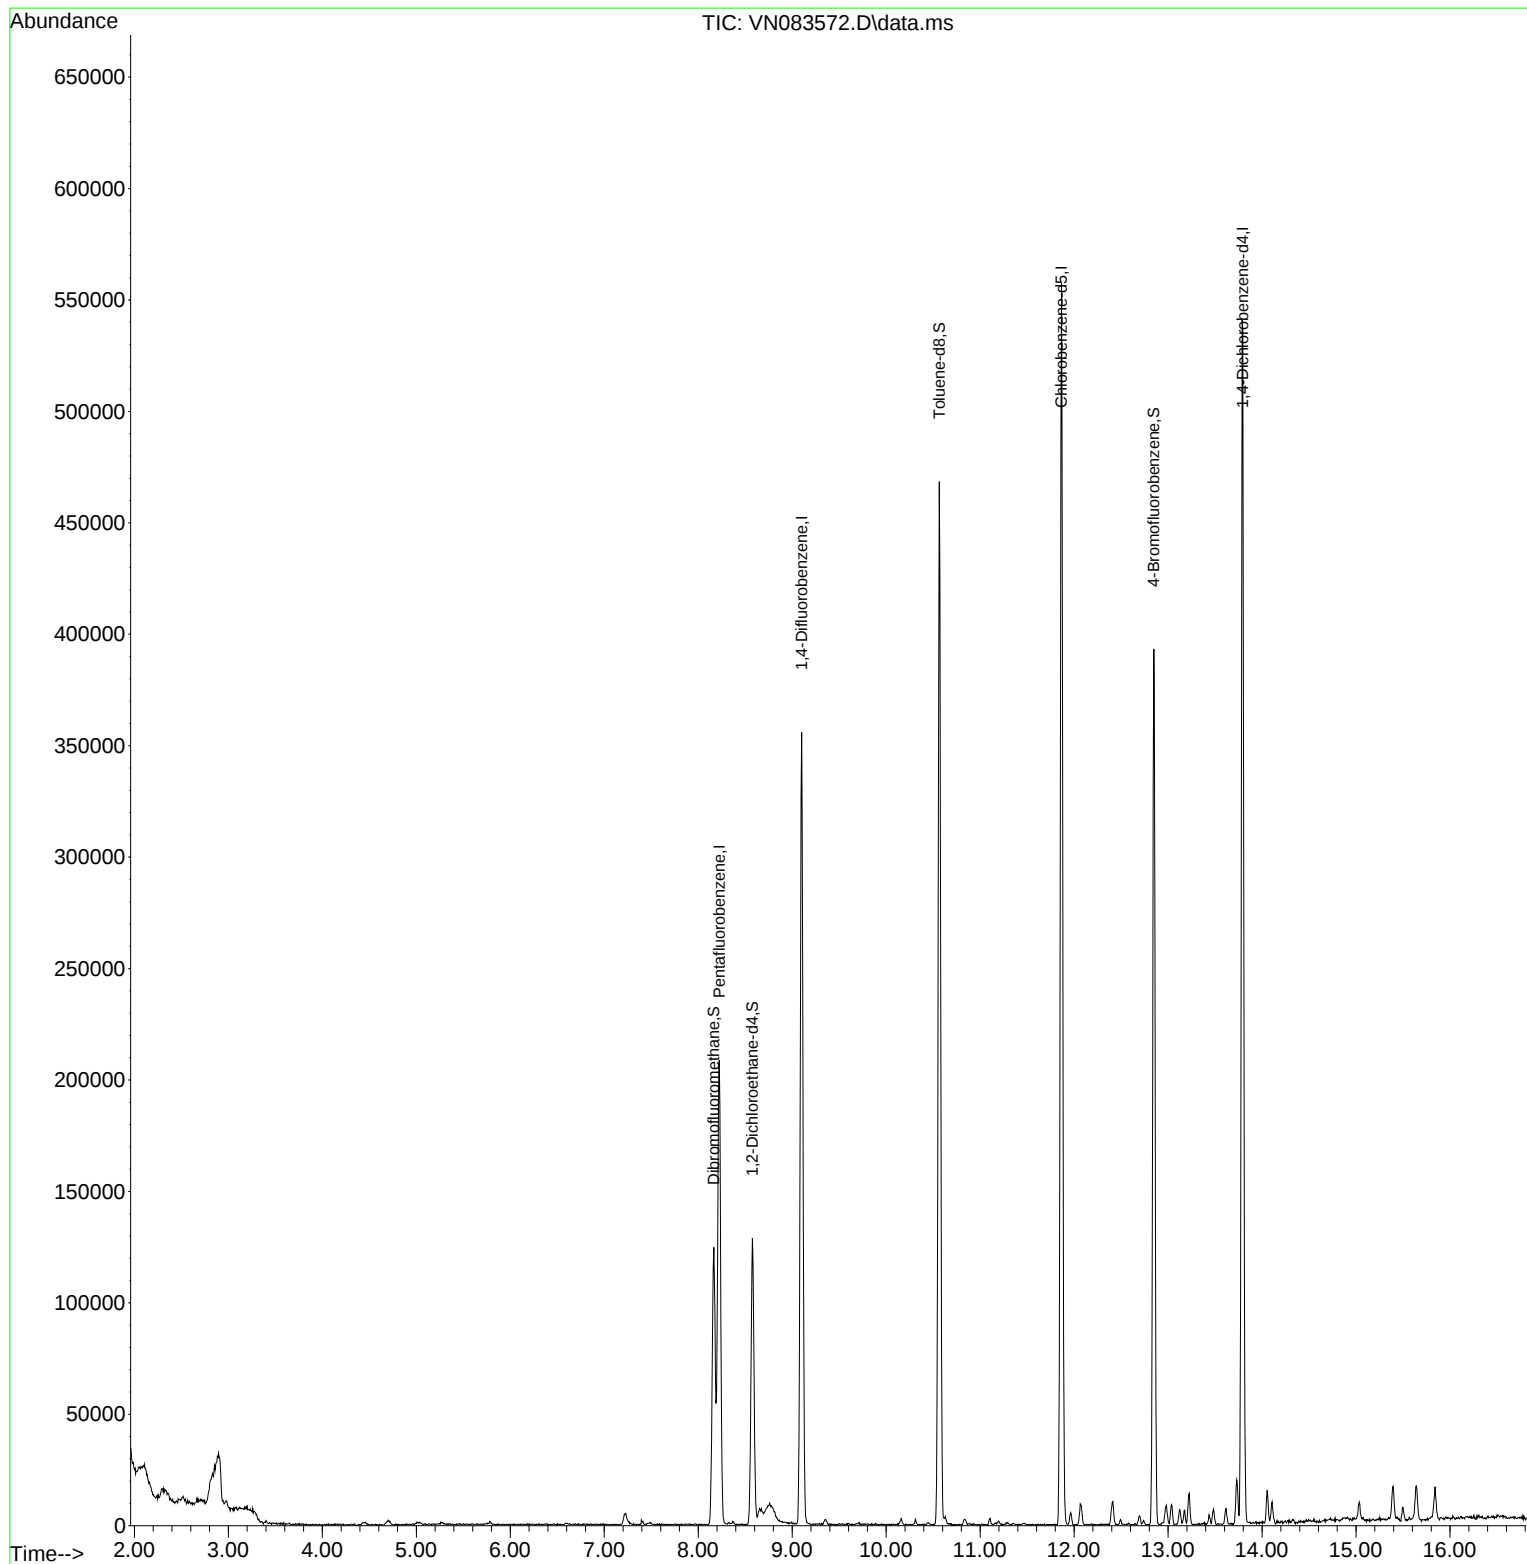


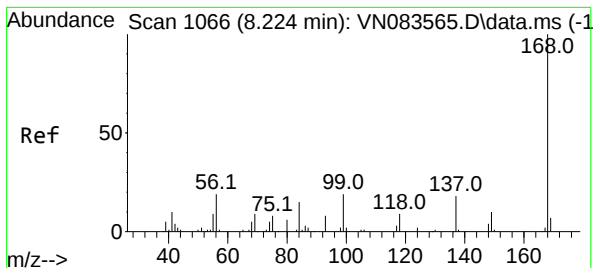

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN083572.D
Acq: 30 Aug 2024 13:40




Instrument :
MSVOA_N
ClientSampleId :
VN0830MBL01


Tgt Ion:168 Resp: 146014
Ion Ratio Lower Upper
168 100
99 71.3 54.2 81.2

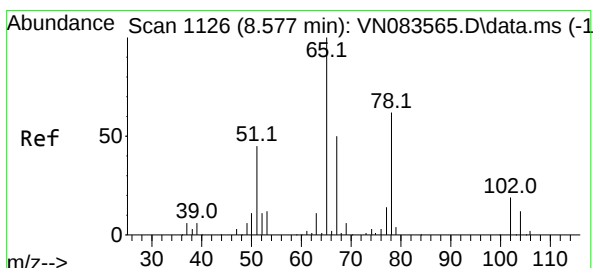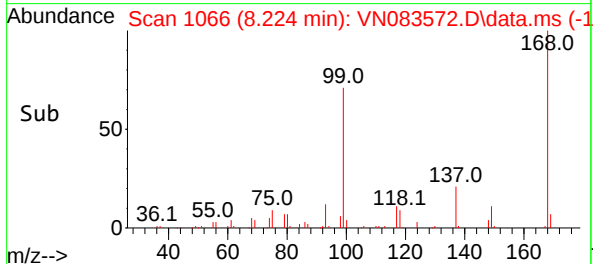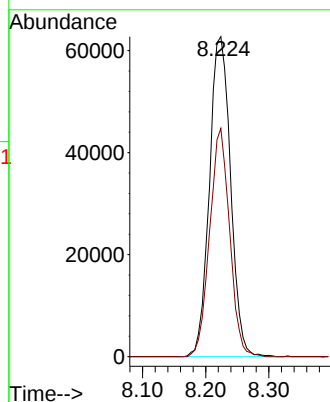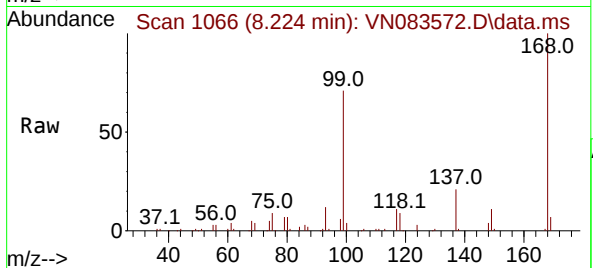

#33
1,2-Dichloroethane-d4
Concen: 52.644 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN083572.D
Acq: 30 Aug 2024 13:40

Tgt Ion: 65 Resp: 107430
Ion Ratio Lower Upper
65 100
67 50.7 0.0 100.8

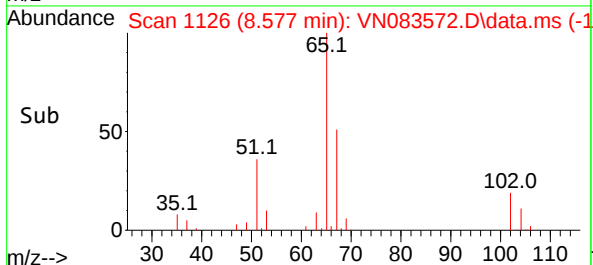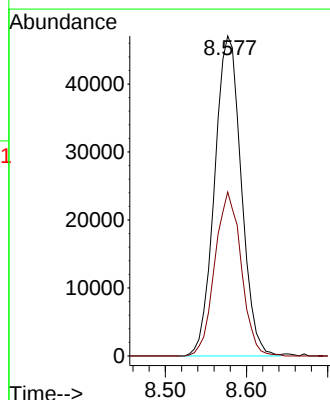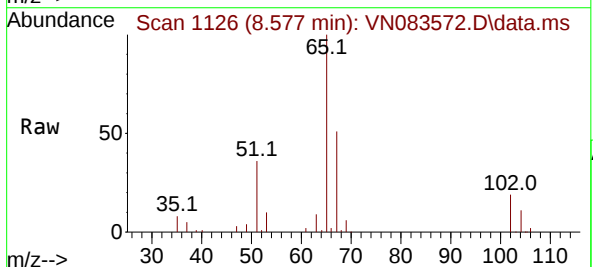

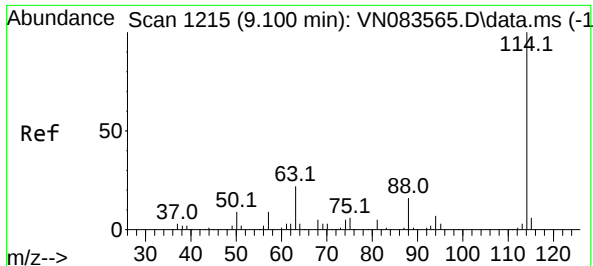

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN083572.D

Acq: 30 Aug 2024 13:40

Instrument :

MSVOA_N

ClientSampleId :

VN0830MBL01





Tgt Ion:114 Resp: 294290

Ion Ratio Lower Upper

114 100

63 22.5 0.0 43.4

88 16.4 0.0 32.6

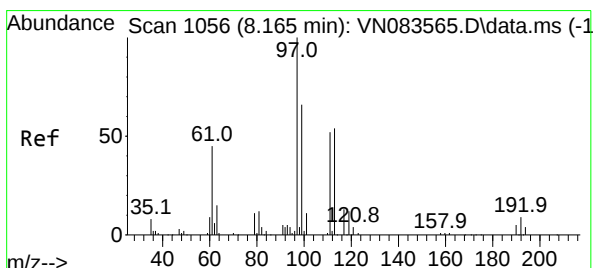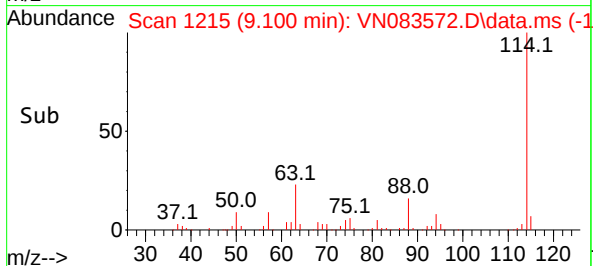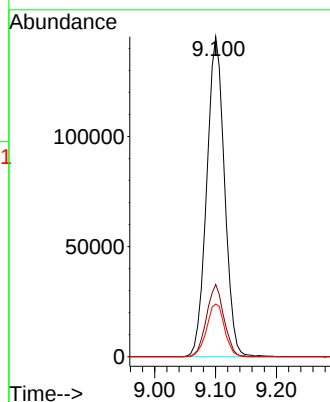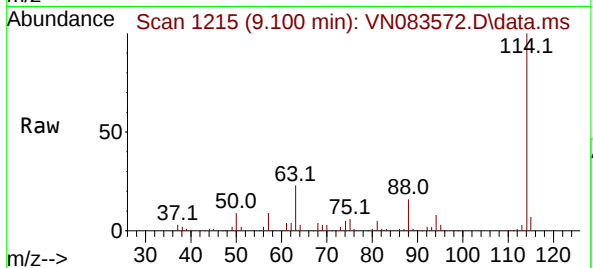

#35

Dibromofluoromethane

Concen: 49.371 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN083572.D

Acq: 30 Aug 2024 13:40




Tgt Ion:113 Resp: 87449


Ion Ratio Lower Upper

113 100

111 103.2 82.6 124.0

192 17.4 14.3 21.5


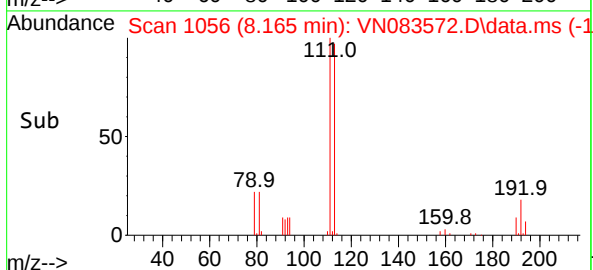
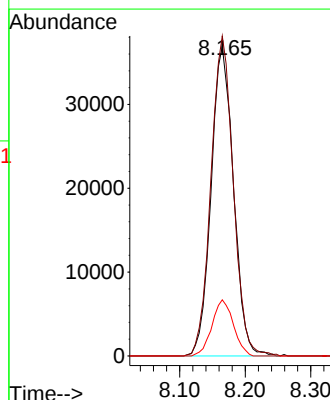
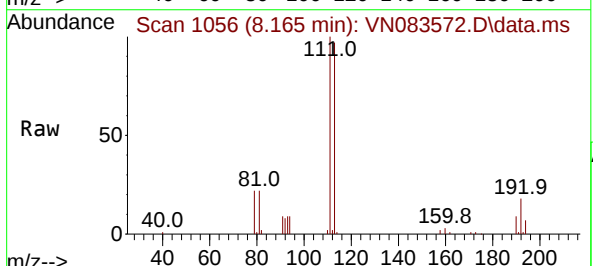


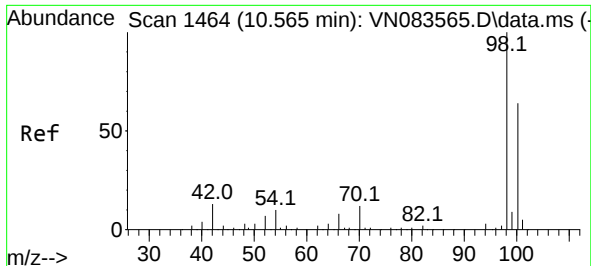

#50
Toluene-d8
Concen: 45.292 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN083572.D
Acq: 30 Aug 2024 13:40




Instrument :
MSVOA_N
ClientSampleId :
VN0830MBL01


Tgt Ion: 98 Resp: 312005
Ion Ratio Lower Upper
98 100
100 65.9 52.0 78.0

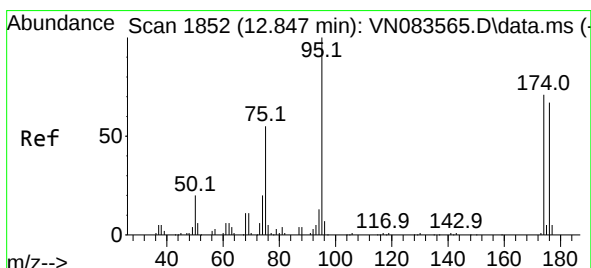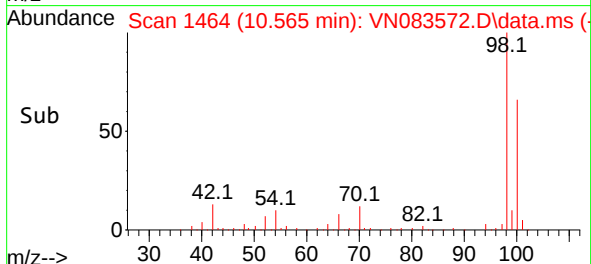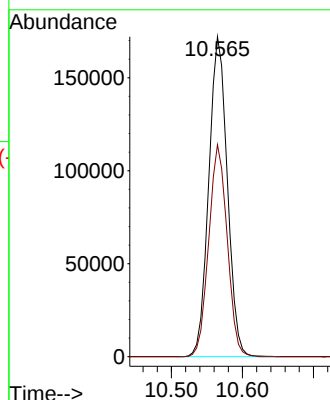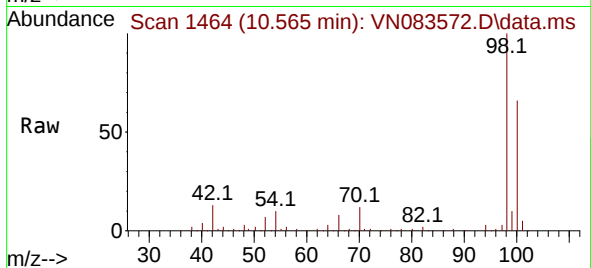

#62
4-Bromofluorobenzene
Concen: 55.055 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN083572.D
Acq: 30 Aug 2024 13:40

Tgt Ion: 95 Resp: 140677
Ion Ratio Lower Upper
95 100
174 70.0 0.0 139.8
176 66.4 0.0 131.4


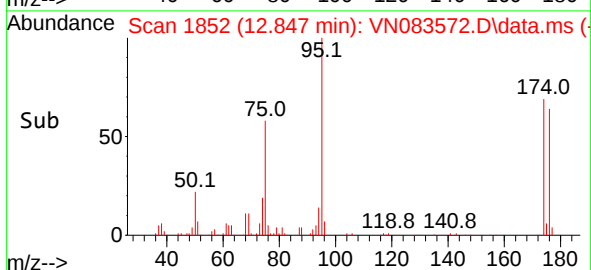
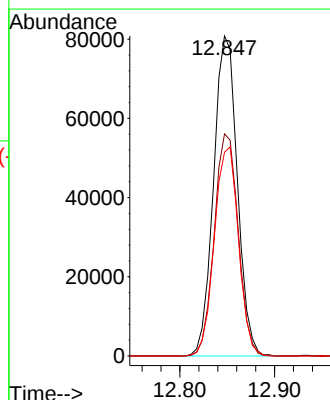
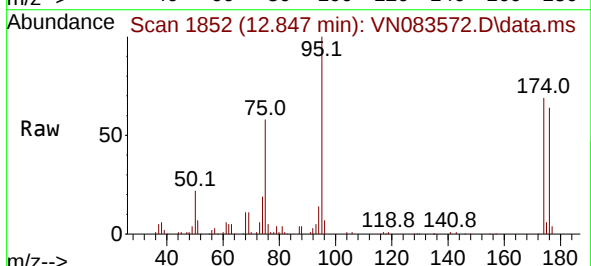


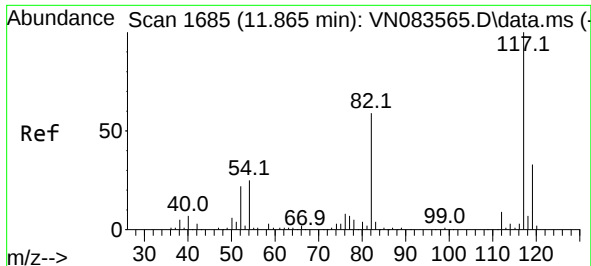

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1
Delta R.T. 0.000 min
Lab File: VN083572.D
Acq: 30 Aug 2024 13:40

Instrument :
MSVOA_N
ClientSampleId :
VN0830MBL01

Tgt Ion:117 Resp: 305322
Ion Ratio Lower Upper
117 100
82 59.4 47.4 71.0
119 33.4 26.3 39.5

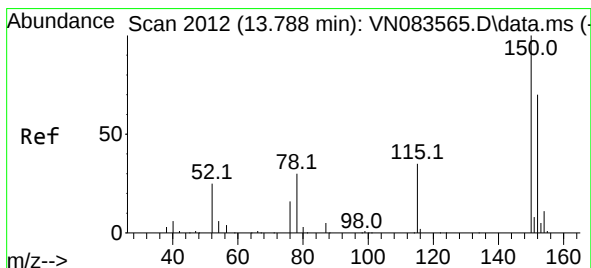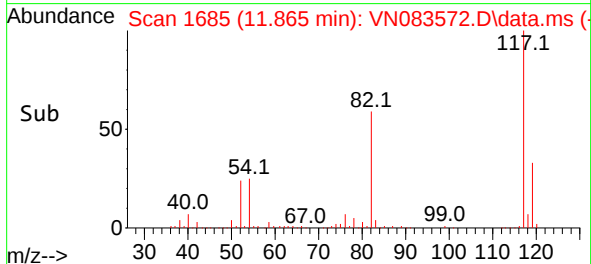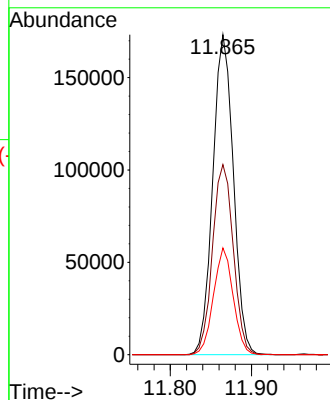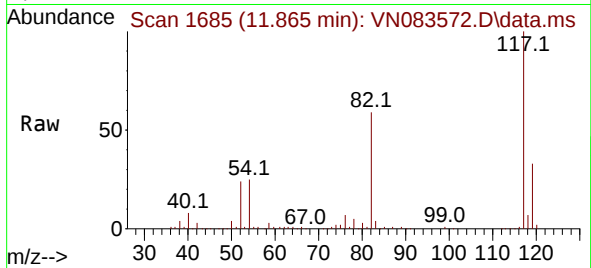

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.006 min
Lab File: VN083572.D
Acq: 30 Aug 2024 13:40

Tgt Ion:152 Resp: 140623
Ion Ratio Lower Upper
152 100
115 64.4 32.2 96.6
150 158.1 0.0 348.6

