

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
 Data File : VN083575.D
 Acq On : 30 Aug 2024 15:09
 Operator : JC\MD
 Sample : P3794-01
 Misc : 1.01g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CHRT-24376

Quant Time: Aug 31 02:38:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 31 00:48:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.218	168	150438	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	306739	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	314592	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	137440	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	108257	51.489	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	102.980%
35) Dibromofluoromethane	8.159	113	86664	46.942	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.880%
50) Toluene-d8	10.565	98	320293	44.626	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.260%
62) 4-Bromofluorobenzene	12.847	95	140391	52.714	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	105.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
Data File : VN083575.D
Acq On : 30 Aug 2024 15:09
Operator : JC\MD
Sample : P3794-01
Misc : 1.01g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHRT-24376

Quant Time: Aug 31 02:38:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Quant Title : SW846 8260
QLast Update : Sat Aug 31 00:48:10 2024
Response via : Initial Calibration




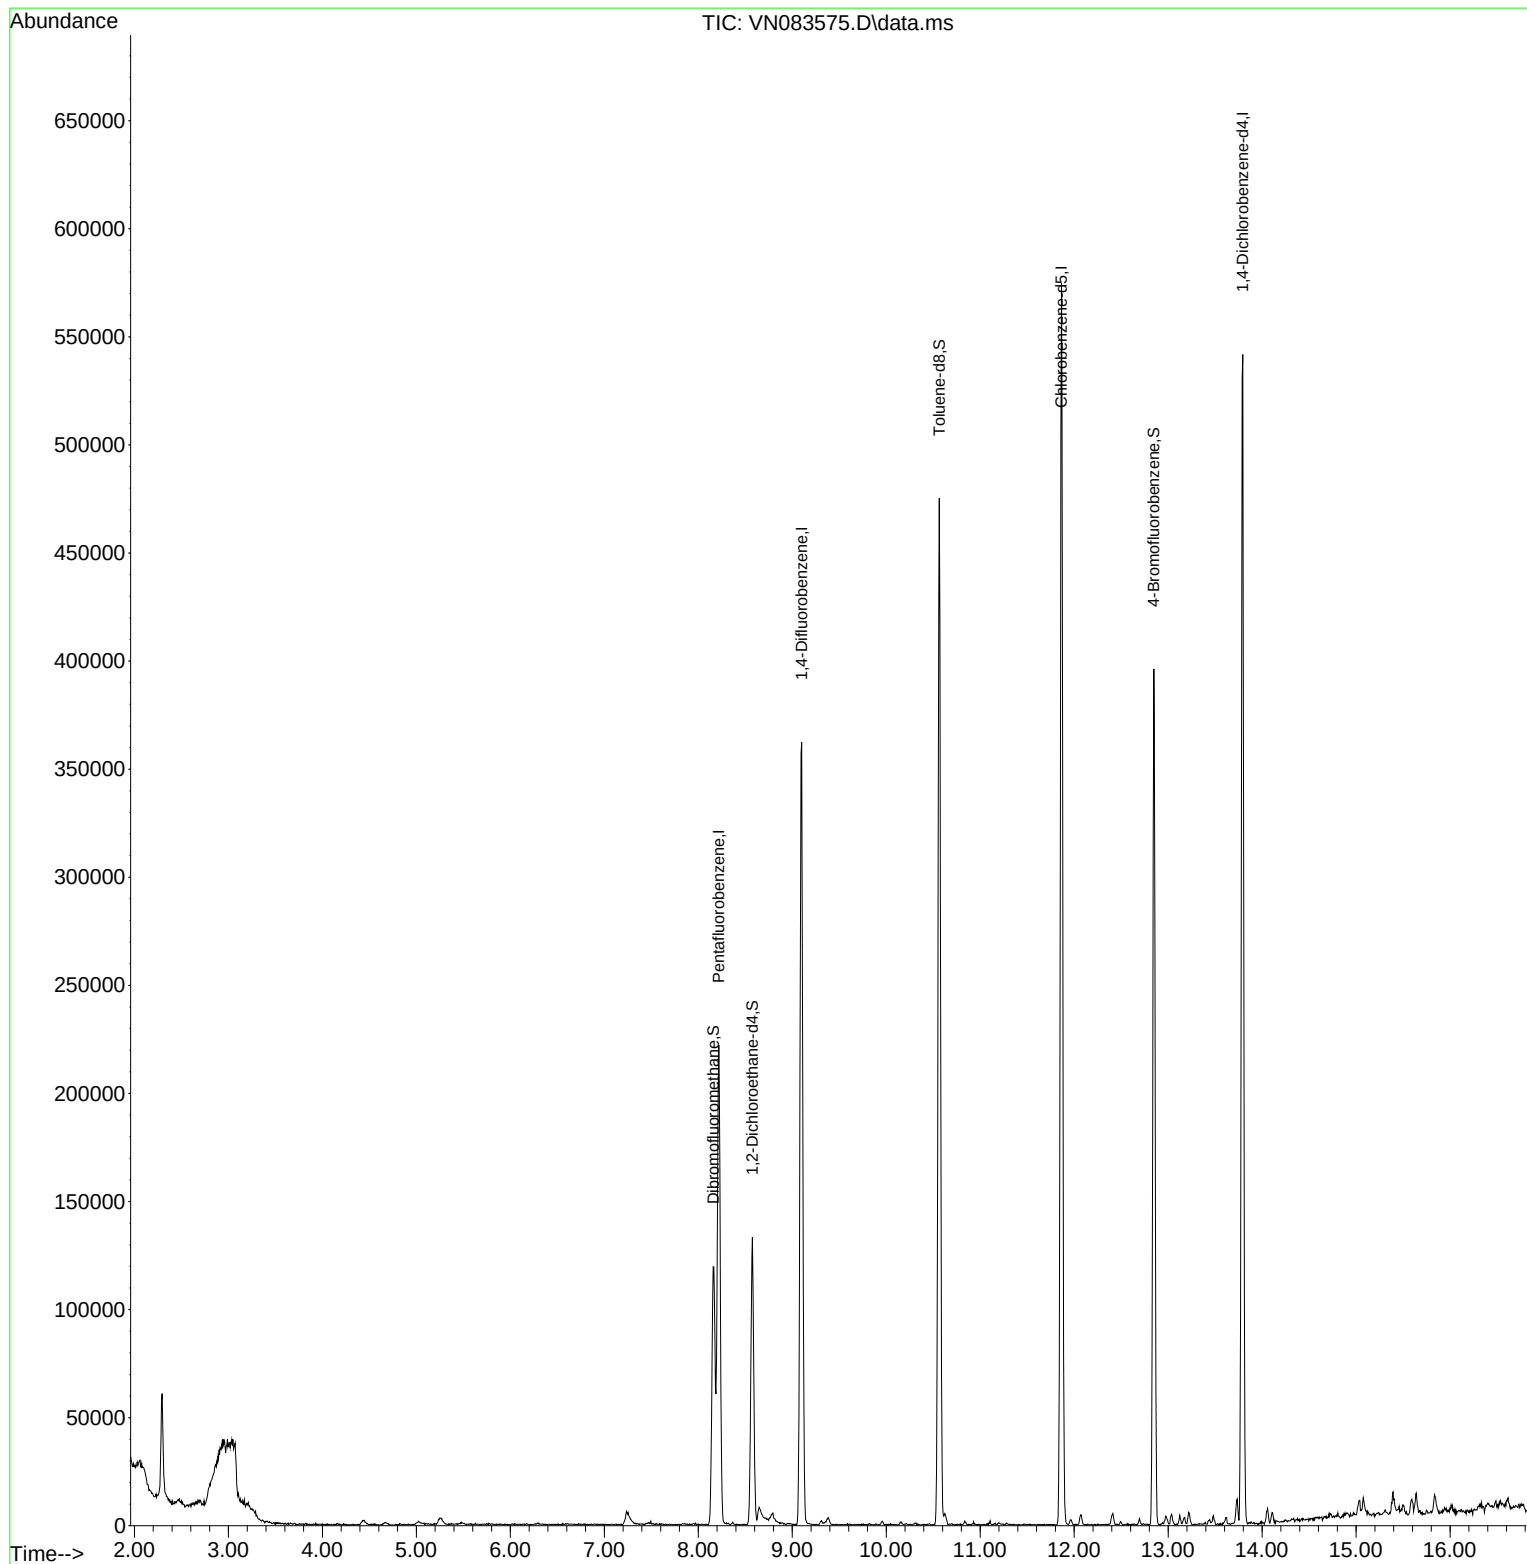


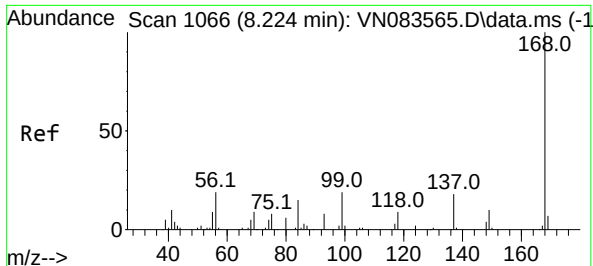

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.006 min
Lab File: VN083575.D
Acq: 30 Aug 2024 15:09




Instrument :
MSVOA_N
ClientSampleId :
CHRT-24376


Tgt Ion:168 Resp: 150438
Ion Ratio Lower Upper
168 100
99 65.9 54.2 81.2

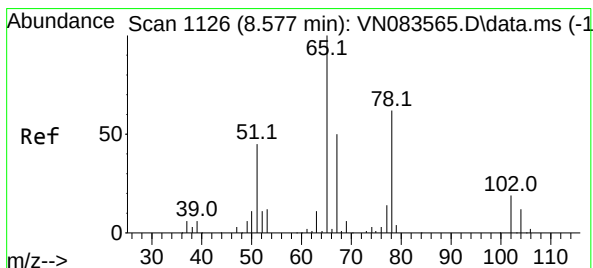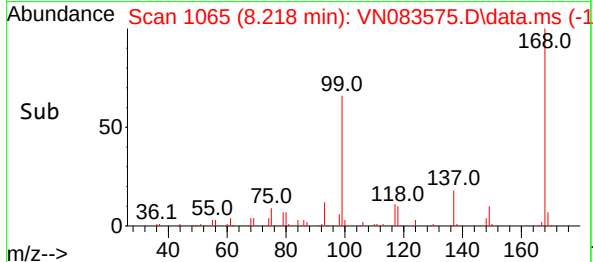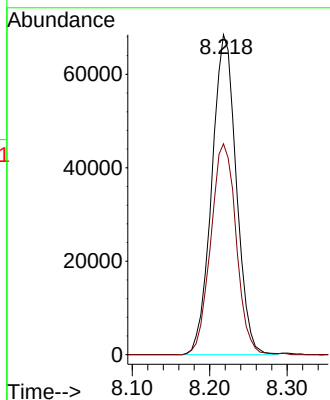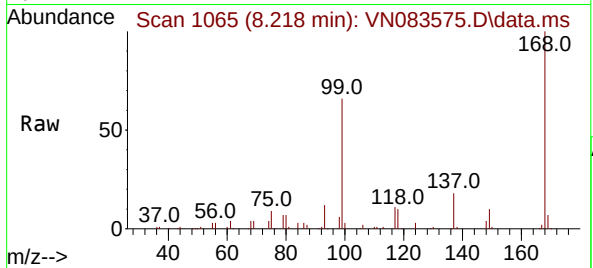

#33
1,2-Dichloroethane-d4
Concen: 51.489 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN083575.D
Acq: 30 Aug 2024 15:09

Tgt Ion: 65 Resp: 108257
Ion Ratio Lower Upper
65 100
67 51.1 0.0 100.8

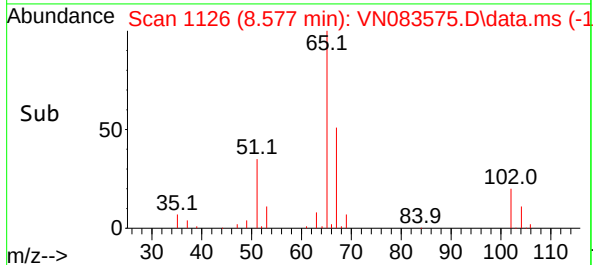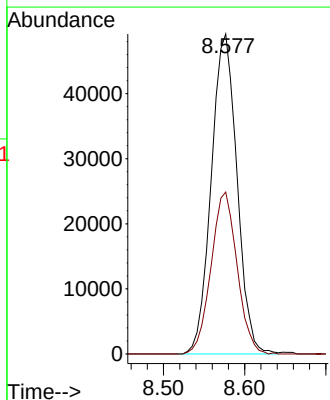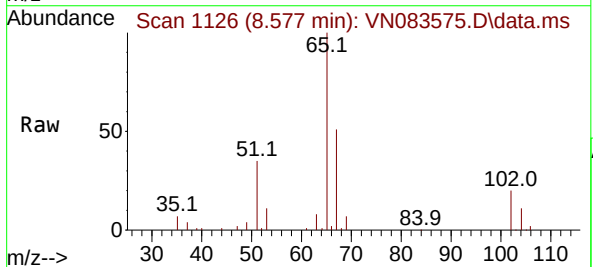

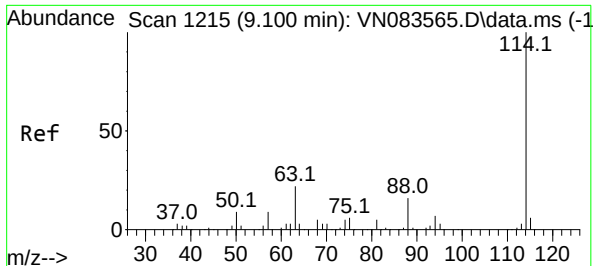

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN083575.D

Acq: 30 Aug 2024 15:09

Instrument :

MSVOA_N

ClientSampleId :

CHRT-24376





Tgt Ion:114 Resp: 306739

Ion Ratio Lower Upper

114 100

63 21.9 0.0 43.4

88 16.6 0.0 32.6

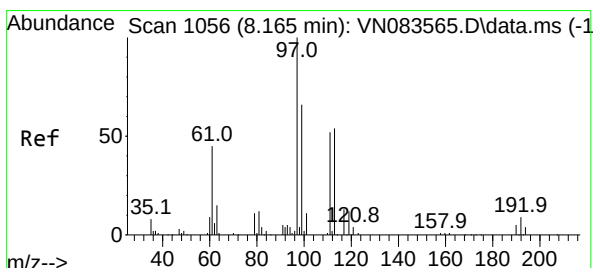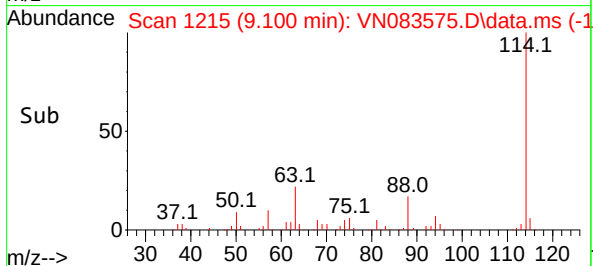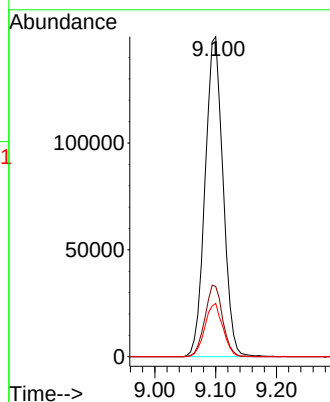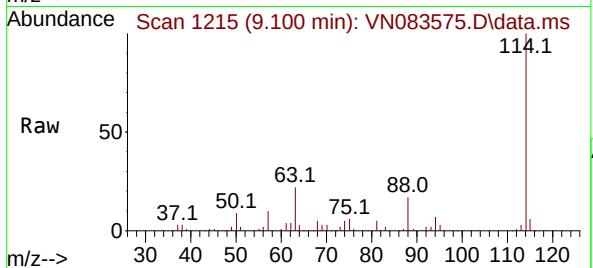

#35

Dibromofluoromethane

Concen: 46.942 ug/l

RT: 8.159 min Scan# 1055

Delta R.T. -0.006 min

Lab File: VN083575.D

Acq: 30 Aug 2024 15:09




Tgt Ion:113 Resp: 86664


Ion Ratio Lower Upper

113 100

111 103.4 82.6 124.0

192 17.9 14.3 21.5


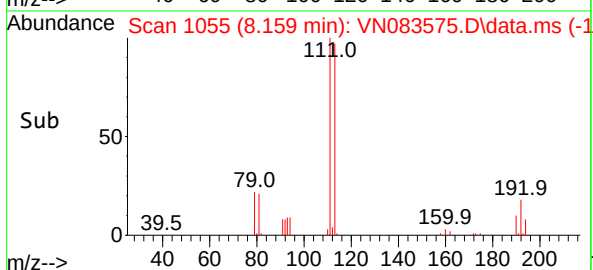
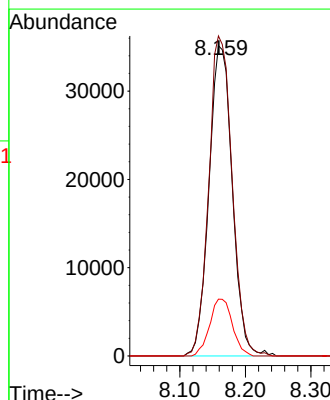
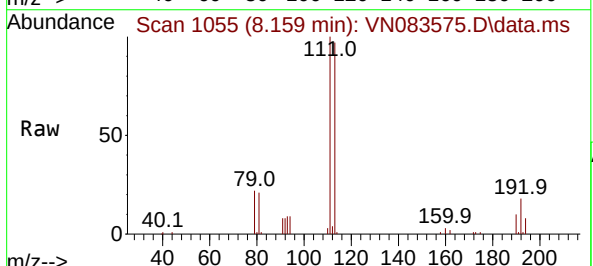


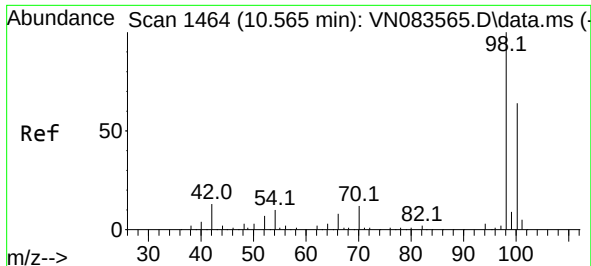

#50
Toluene-d8
Concen: 44.626 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN083575.D
Acq: 30 Aug 2024 15:09




Instrument :
MSVOA_N
ClientSampleId :
CHRT-24376


Tgt Ion: 98 Resp: 320293
Ion Ratio Lower Upper
98 100
100 65.9 52.0 78.0

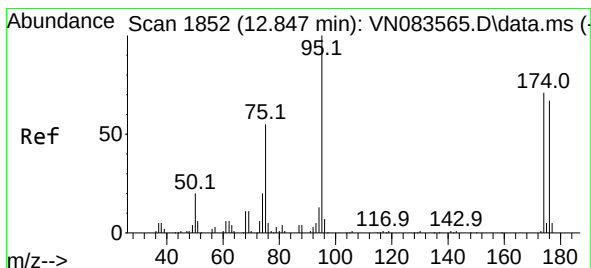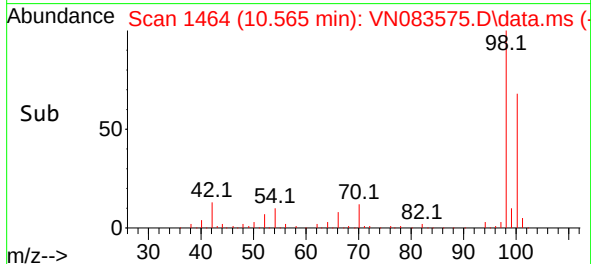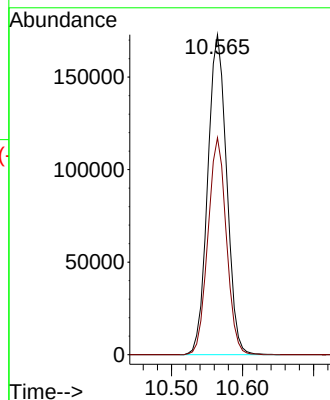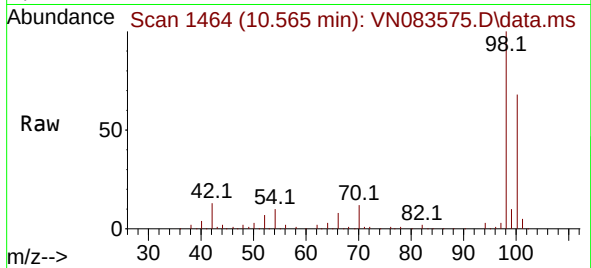

#62
4-Bromofluorobenzene
Concen: 52.714 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN083575.D
Acq: 30 Aug 2024 15:09

Tgt Ion: 95 Resp: 140391
Ion Ratio Lower Upper
95 100
174 69.0 0.0 139.8
176 66.3 0.0 131.4


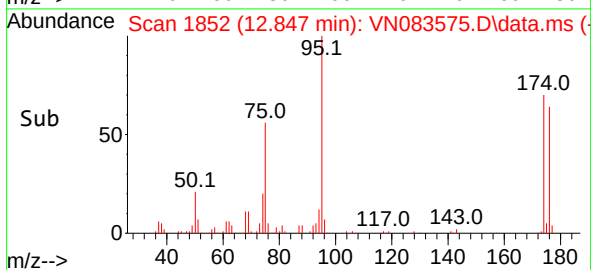
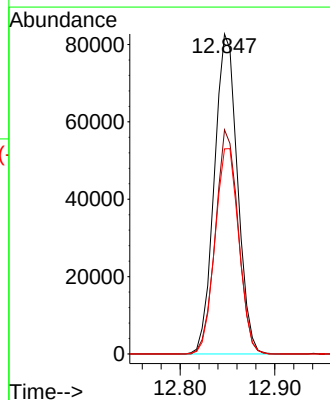
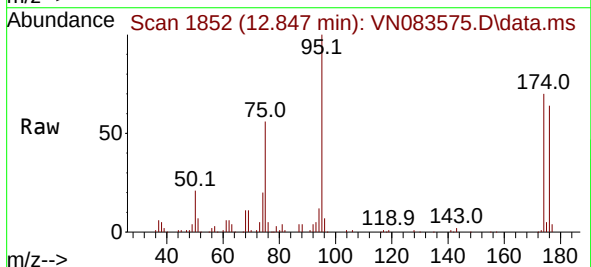


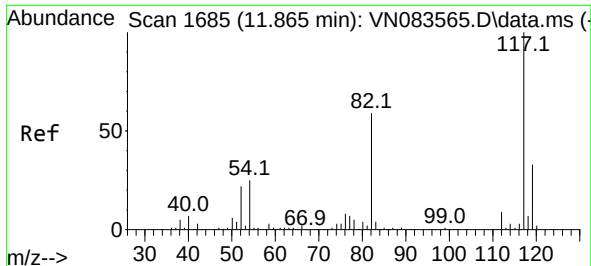

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN083575.D
Acq: 30 Aug 2024 15:09

Instrument :
MSVOA_N
ClientSampleId :
CHRT-24376

Tgt Ion:117 Resp: 314592
Ion Ratio Lower Upper
117 100
82 60.5 47.4 71.0
119 32.9 26.3 39.5

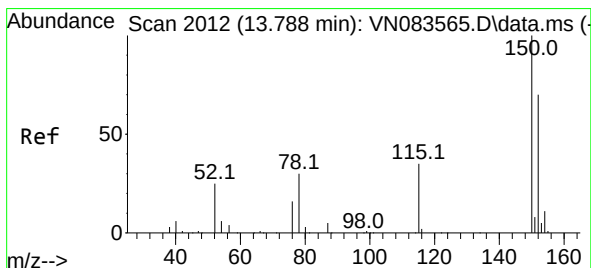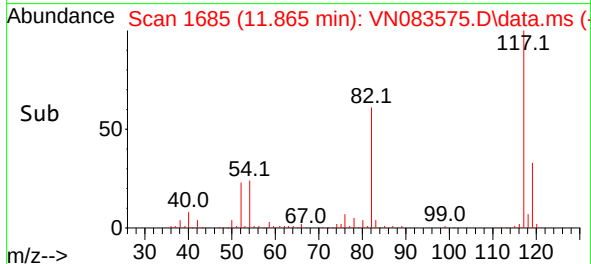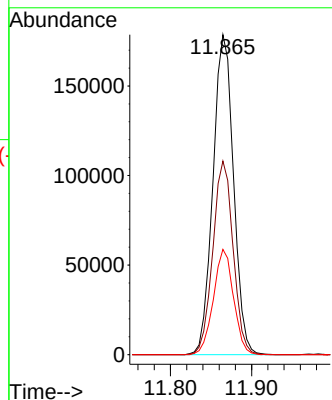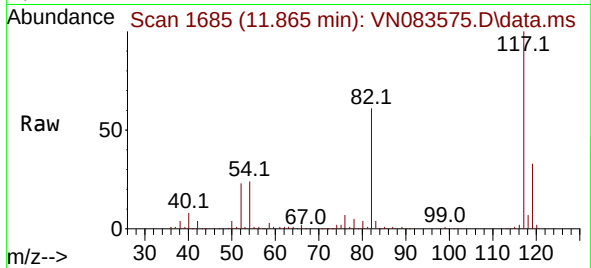

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.006 min
Lab File: VN083575.D
Acq: 30 Aug 2024 15:09

Tgt Ion:152 Resp: 137440
Ion Ratio Lower Upper
152 100
115 66.1 32.2 96.6
150 161.5 0.0 348.6

