

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
 Data File : VN083575.D
 Acq On : 30 Aug 2024 15:09
 Operator : JC\MD
 Sample : P3794-01
 Misc : 1.01g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CHRT-24376

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
 Title : SW846 8260

Signal : TIC: VN083575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.295	53	58	67	rVB	47697	76950	7.59%	1.383%
2	2.865	139	155	156	rBV3	15766	55646	5.49%	1.000%
3	7.235	890	898	900	rBV	6401	10896	1.08%	0.196%
4	8.159	1046	1055	1060	rBV	119516	296238	29.23%	5.325%
5	8.218	1060	1065	1076	rVB	221511	479732	47.34%	8.623%
6	8.577	1116	1126	1134	rBV	132997	285590	28.18%	5.133%
7	8.647	1134	1138	1149	rVV3	5930	16373	1.62%	0.294%
8	9.100	1206	1215	1226	rBV	361946	740303	73.05%	13.307%
9	10.565	1456	1464	1472	rBV	474833	873562	86.20%	15.702%
10	11.865	1675	1685	1697	rBV	574408	1013395	100.00%	18.216%
11	12.847	1845	1852	1861	rVB	396054	667270	65.85%	11.994%
12	13.735	1996	2003	2006	rBV3	11198	17256	1.70%	0.310%
13	13.794	2006	2013	2022	rVB	541062	929409	91.71%	16.706%
14	14.059	2052	2058	2062	rBV	7245	11904	1.17%	0.214%
15	15.035	2218	2224	2226	rBV4	6759	11388	1.12%	0.205%
16	15.394	2277	2285	2291	rBV6	10421	21298	2.10%	0.383%
17	15.594	2314	2319	2322	rBV4	6493	11649	1.15%	0.209%
18	15.641	2322	2327	2331	rVB2	9008	14128	1.39%	0.254%
19	15.835	2356	2360	2369	rVB10	8810	18021	1.78%	0.324%
20	16.400	2450	2456	2461	rBV7	4326	12319	1.22%	0.221%




Sum of corrected areas: 5563327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
Data File : VN083575.D
Acq On : 30 Aug 2024 15:09
Operator : JC\MD
Sample : P3794-01
Misc : 1.01g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHRT-24376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

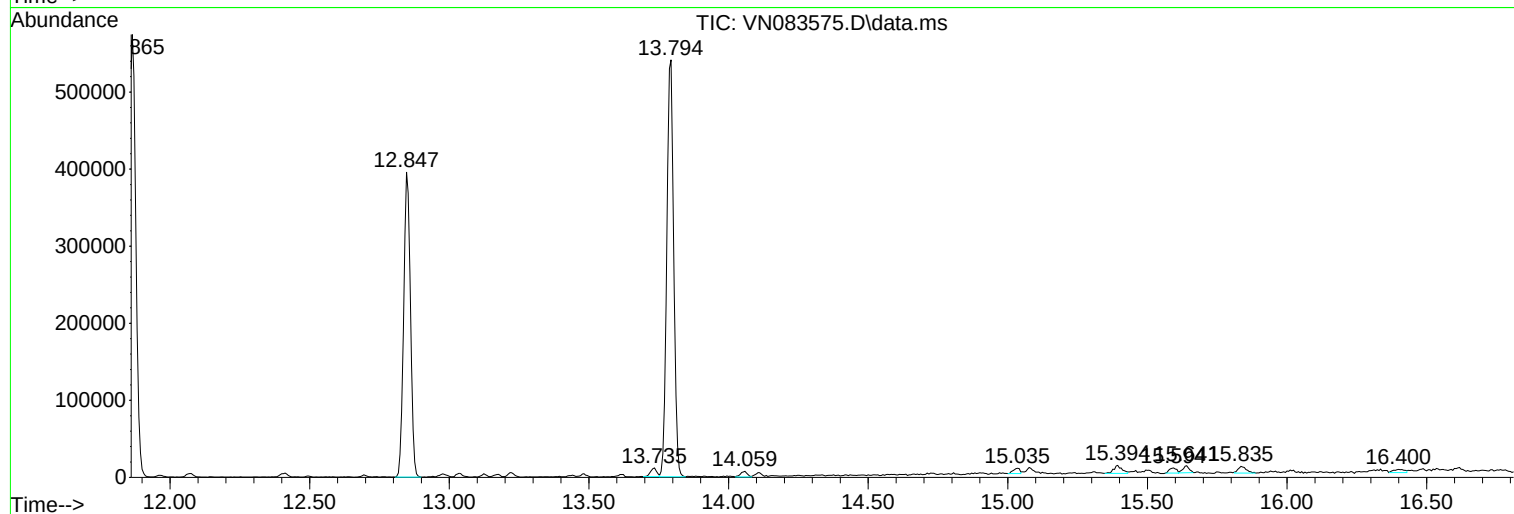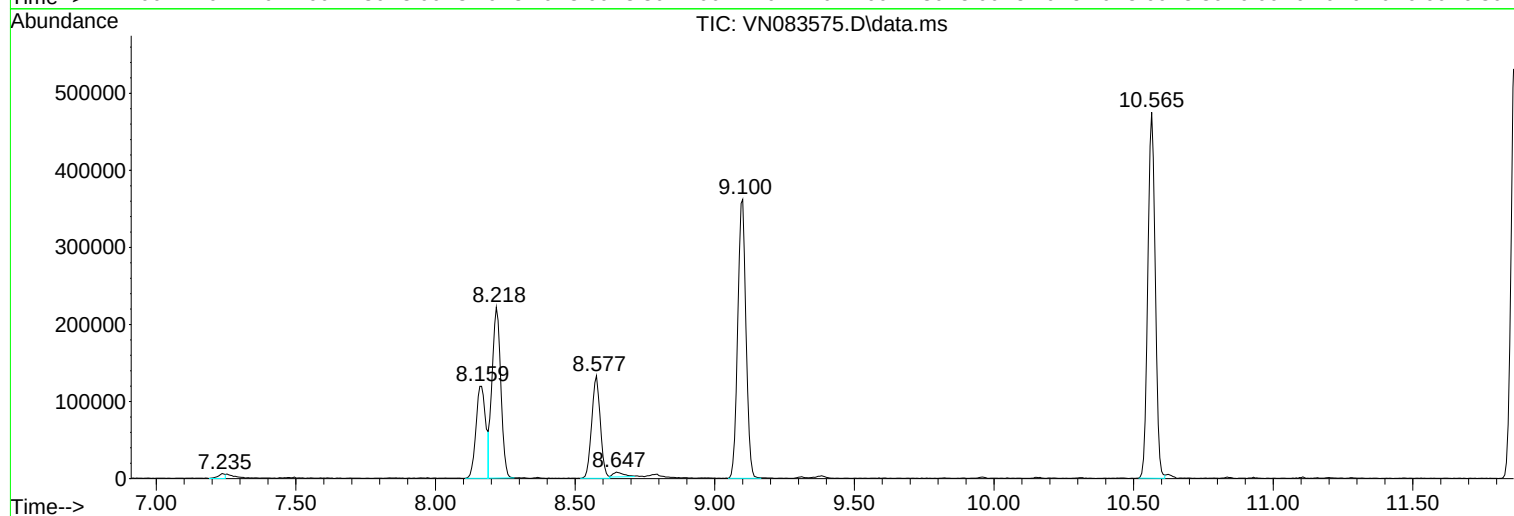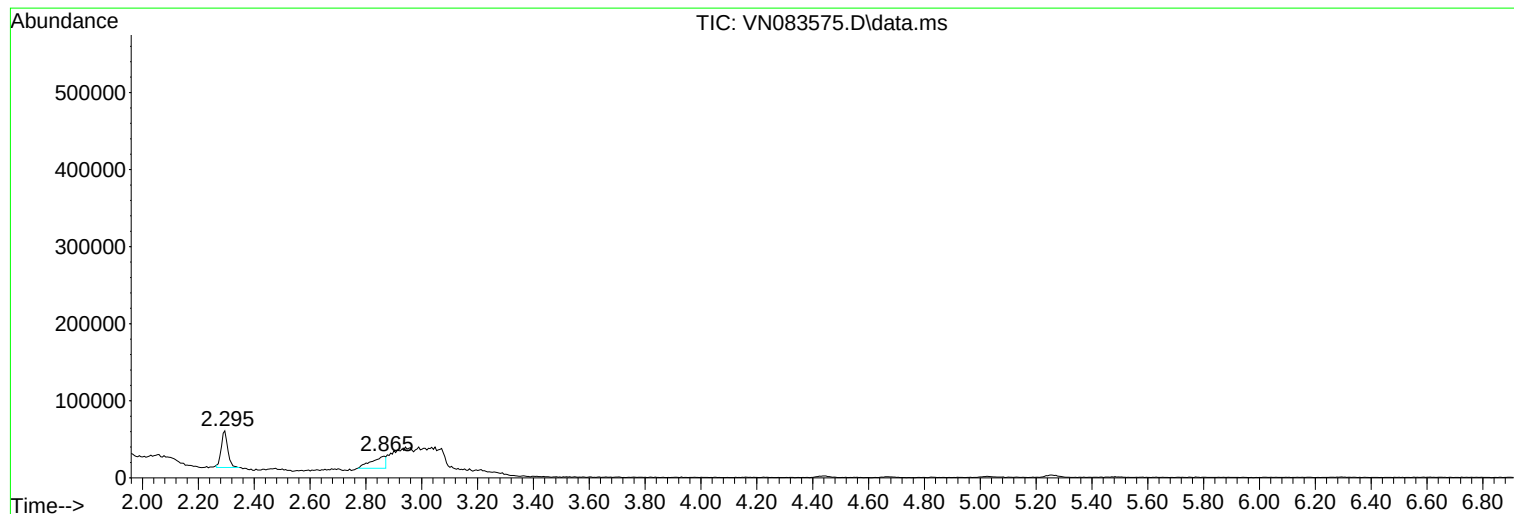

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
Data File : VN083575.D
Acq On : 30 Aug 2024 15:09
Operator : JC\MD
Sample : P3794-01
Misc : 1.01g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 16 Sample Multiplier: 1










Instrument :
MSVOA_N
ClientSampleId :
CHRT-24376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Unknown2.865 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
2.865	5.80 ug/l	55646	Pentafluorobenzene	8.218	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Phosgene	98	CCl2O	000075-44-5	28
2	2-Chloroethyl methyl sulfoxide	126	C3H7ClOS	005331-57-7	12
3	Methylene chloride	84	CH2Cl2	000075-09-2	12
4	Boron trifluoride	68	BF3	007637-07-2	9
5	1,3-Dioxonane, 5,5,6,6,7,7,8,8-o...	274	C7H6F8O2	036301-47-0	9

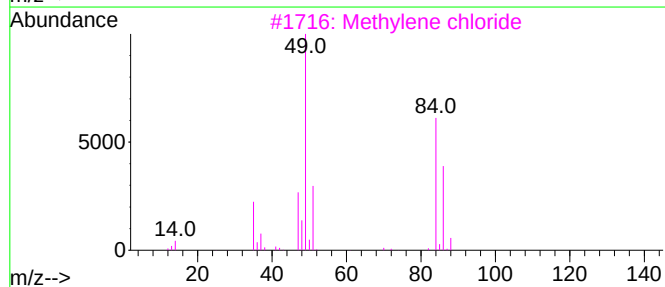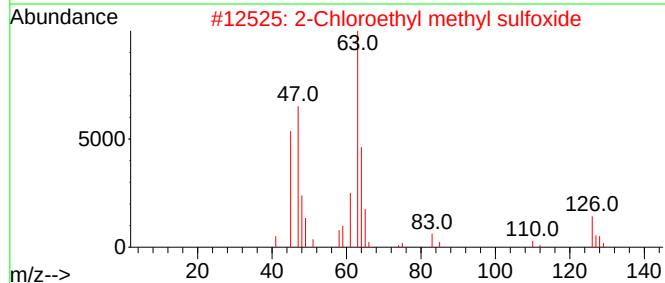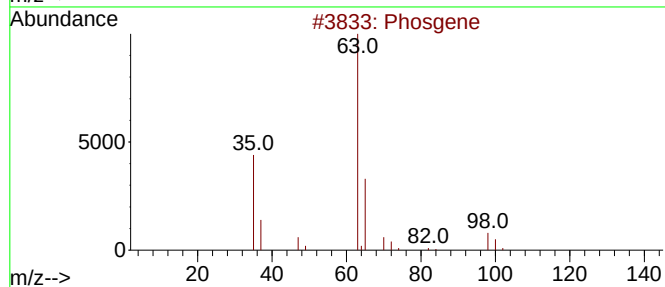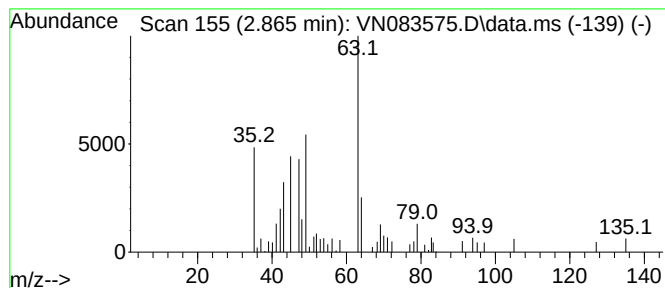

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
Data File : VN083575.D
Acq On : 30 Aug 2024 15:09
Operator : JC\MD
Sample : P3794-01
Misc : 1.01g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHRT-24376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Unknown2.865	2.865	5.8	ug/l	55646	1	8.218	479732	50.0