
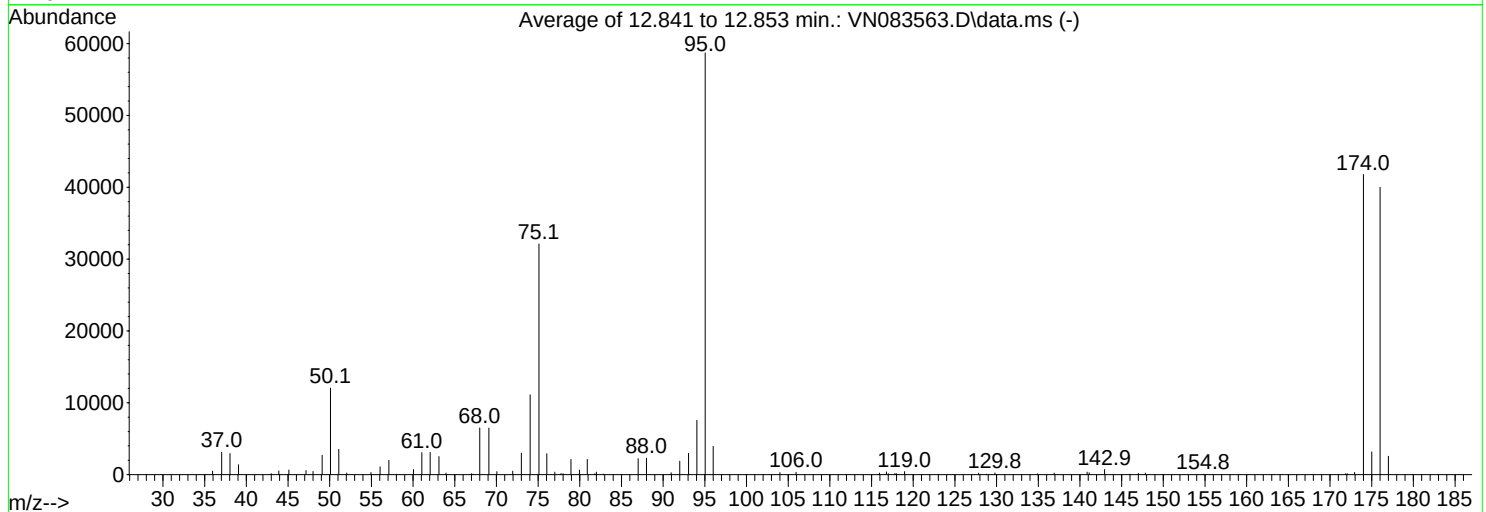


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
Data File : VN083563.D
Acq On : 30 Aug 2024 08:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Title : SW846 8260
Last Update : Sat Aug 31 00:48:10 2024

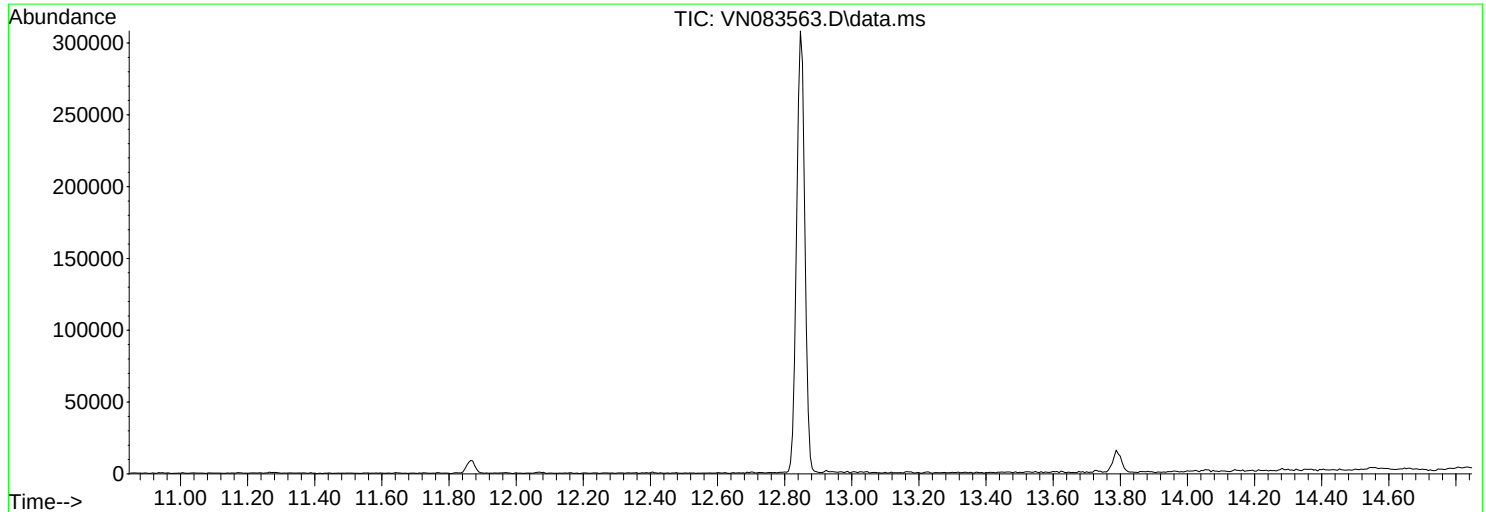

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	12059	PASS
75	95	30	60	54.7	32109	PASS
95	95	100	100	100.0	58709	PASS
96	95	5	9	6.7	3945	PASS
173	174	0.00	2	0.8	316	PASS
174	95	50	100	71.1	41771	PASS
175	174	5	9	7.6	3162	PASS
176	174	95	101	95.8	40003	PASS
177	176	5	9	6.4	2565	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	486	51.10	3527	67.00	131	77.75	151
37.05	3107	52.05	216	67.20	63	78.00	131
38.05	2938	54.95	280	68.00	6507	78.95	212
39.05	1383	56.05	1100	69.10	6487	79.95	64
43.00	143	57.10	2015	70.05	434	80.90	2118
43.90	506	58.00	58	71.95	499	81.80	136
45.10	638	60.05	717	73.00	2981	82.00	355
47.15	581	61.05	3068	74.05	11104	82.80	80
48.00	456	62.05	3093	75.10	32109	87.00	2223
49.10	2692	63.10	2528	76.05	2924	88.00	2298
50.10	12059	63.95	217	77.00	355	90.95	278

Average of 12.841 to 12.853 min.: VN083563.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	1881	117.80	169	146.00	63		
93.05	2953	118.00	140	147.00	176		
94.05	7573	118.95	421	147.85	217		
95.05	58709	127.85	197	154.80	61		
96.00	3945	128.80	66	171.90	152		
104.00	283	129.80	252	172.10	118		
105.95	336	134.90	116	172.95	316		
115.80	51	136.90	221	174.00	41771		
115.95	217	140.85	357	175.00	3162		
116.80	375	141.10	261	176.00	40003		
117.00	131	142.95	709	177.00	2565		

Instrument :

MSVOA_N

ClientSampleId :

BFB