
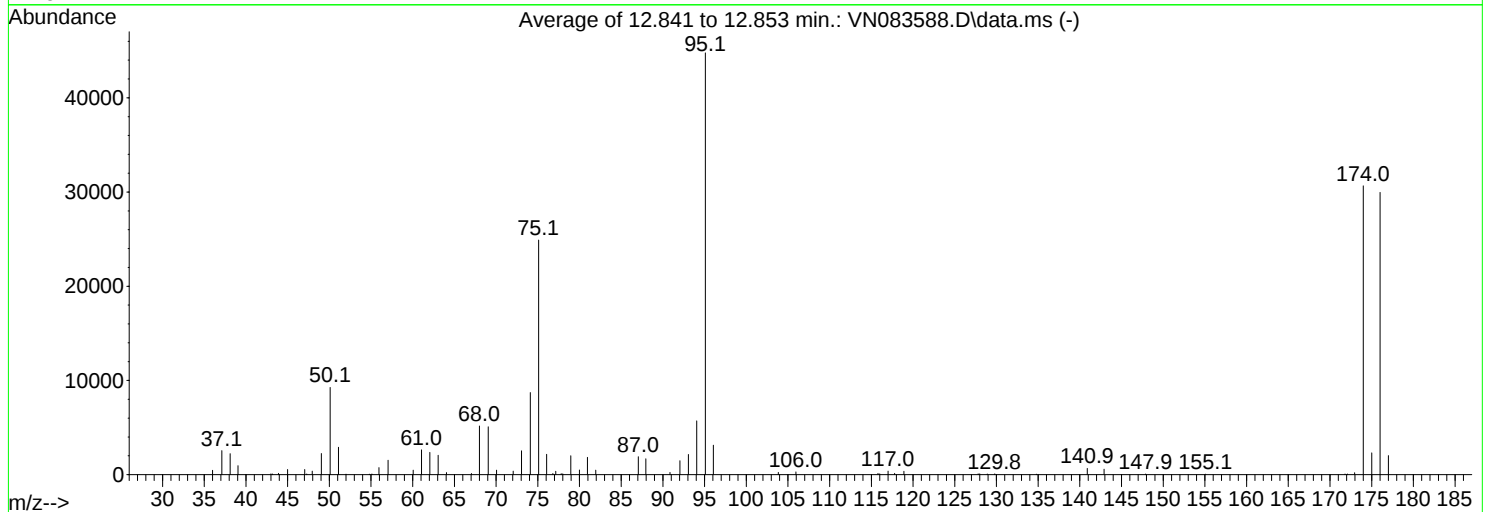


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN083024\
Data File : VN083588.D
Acq On : 31 Aug 2024 01:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N083024W.M
Title : SW846 8260
Last Update : Sat Aug 31 00:48:10 2024

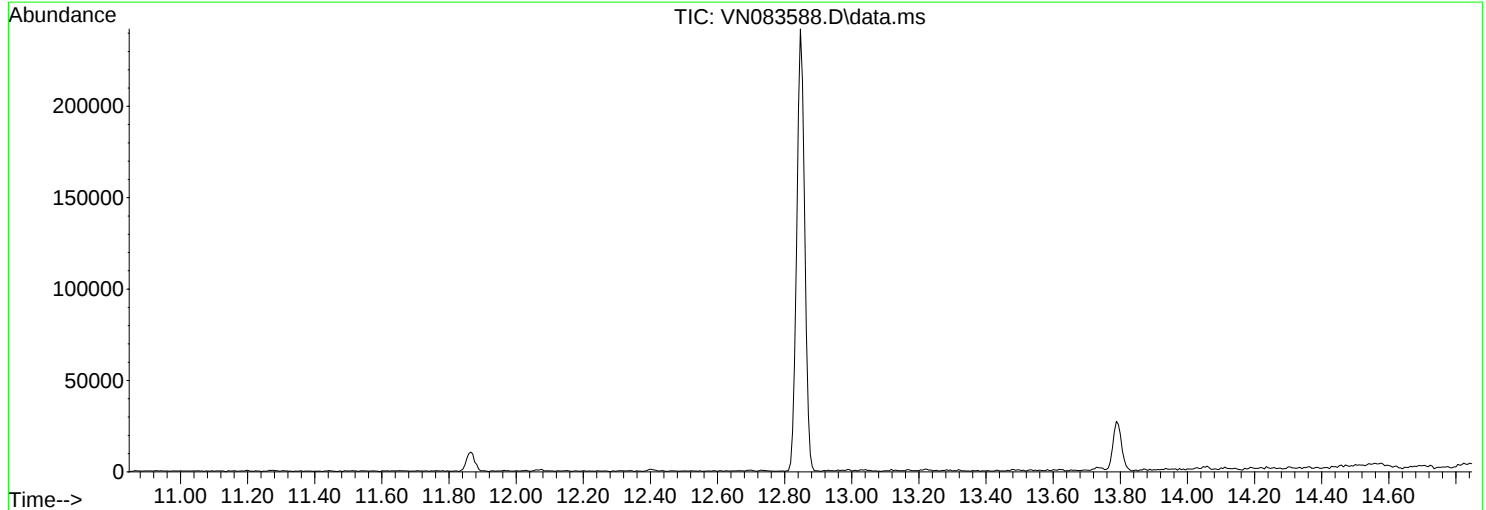

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	9265	PASS
75	95	30	60	55.6	24893	PASS
95	95	100	100	100.0	44776	PASS
96	95	5	9	7.0	3128	PASS
173	174	0.00	2	0.7	205	PASS
174	95	50	100	68.5	30659	PASS
175	174	5	9	7.5	2308	PASS
176	174	95	101	97.8	29971	PASS
177	176	5	9	6.8	2029	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	460	47.30	61	61.05	2641	75.10	2489
37.10	2548	47.95	382	62.05	2368	76.05	215
38.10	2226	49.05	2243	63.05	2053	76.80	11
39.05	960	50.10	9265	64.05	220	77.15	35
40.00	20	51.10	2911	67.05	119	77.80	103
43.00	78	52.00	56	68.00	5166	78.00	83
43.20	69	54.80	58	69.05	5079	78.95	2008
43.90	137	55.10	68	70.05	480	80.00	488
44.00	26	55.95	747	72.05	372	80.95	1836
45.00	545	57.05	1528	73.05	2537	81.95	471
47.05	549	60.05	479	74.10	8711	87.05	1901

Average of 12.841 to 12.853 min.: VN083588.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	1685	117.00	371	155.10	51		
90.85	240	117.80	141	171.80	77		
92.05	1485	118.90	364	172.10	76		
93.05	2136	127.80	84	172.95	205		
94.05	5712	128.00	79	174.00	30659		
95.10	44776	128.90	67	175.00	2308		
96.05	3128	129.80	86	176.00	29971		
103.85	246	134.80	57	177.00	2029		
105.95	292	140.90	668				
115.80	131	142.90	584				
116.00	78	147.90	60				

Instrument :

MSVOA_N

ClientSampleId :

BFB