


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN083118\
Data File : VN050976.D
Acq On : 31 Aug 2018 9:46
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N082118W.M
Title : SW846 8260
Last Update : Wed Aug 22 05:38:12 2018

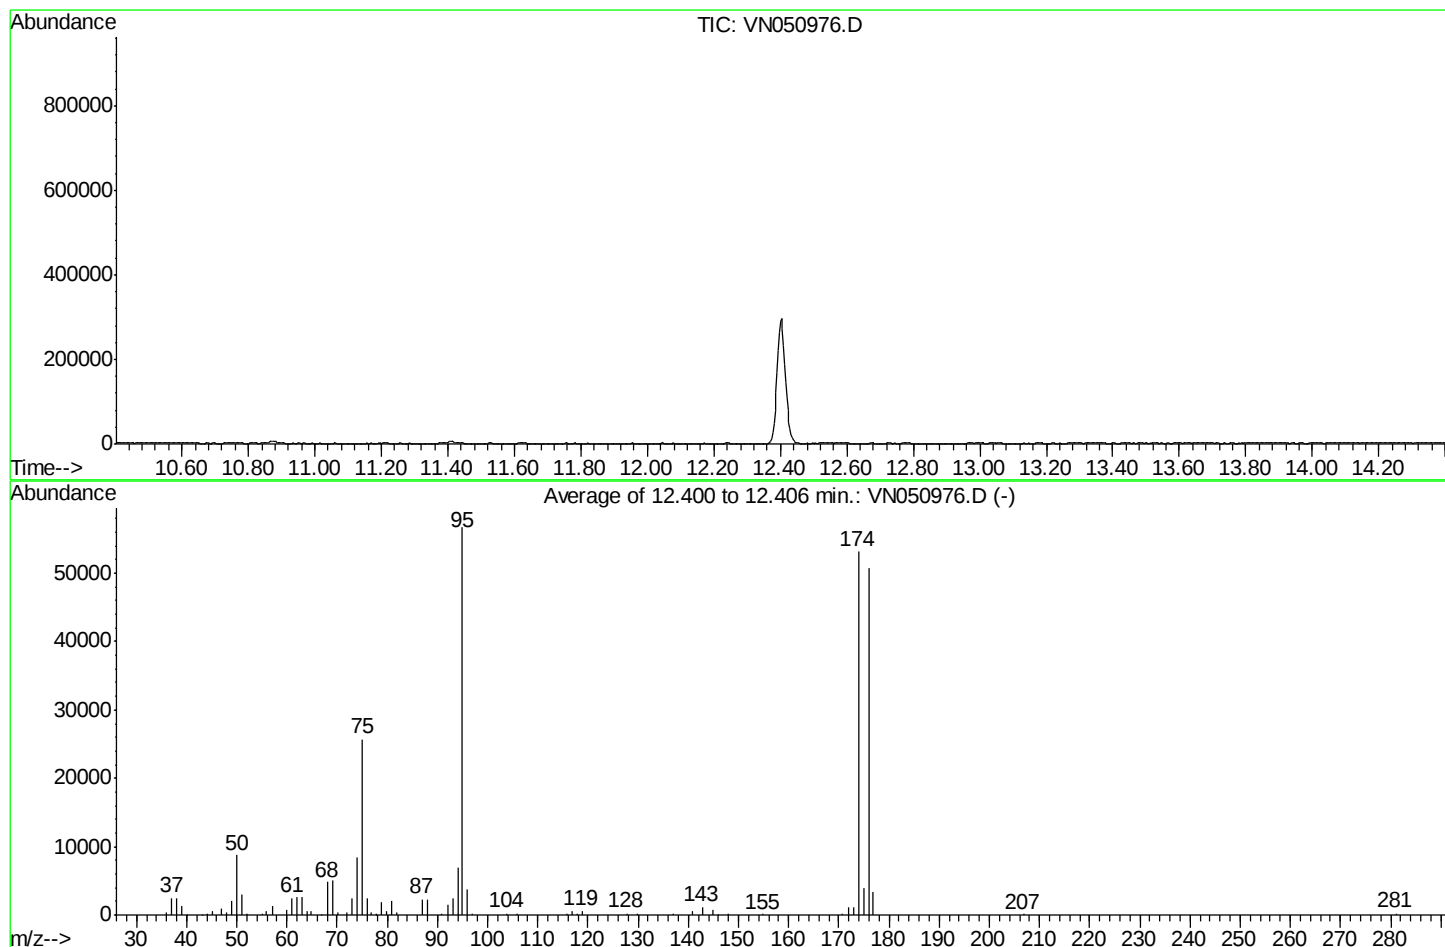

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	8802	PASS
75	95	30	60	45.3	25709	PASS
95	95	100	100	100.0	56722	PASS
96	95	5	9	6.6	3736	PASS
173	174	0.00	2	2.0	1056	PASS
174	95	50	100	93.7	53173	PASS
175	174	5	9	7.6	4031	PASS
176	174	95	101	95.5	50792	PASS
177	176	5	9	6.8	3451	PASS