


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN083119\
Data File : VN057589.D
Acq On : 30 Aug 2019 15:09
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082919W.M
Title : SW846 8260
Last Update : Fri Aug 30 11:59:03 2019

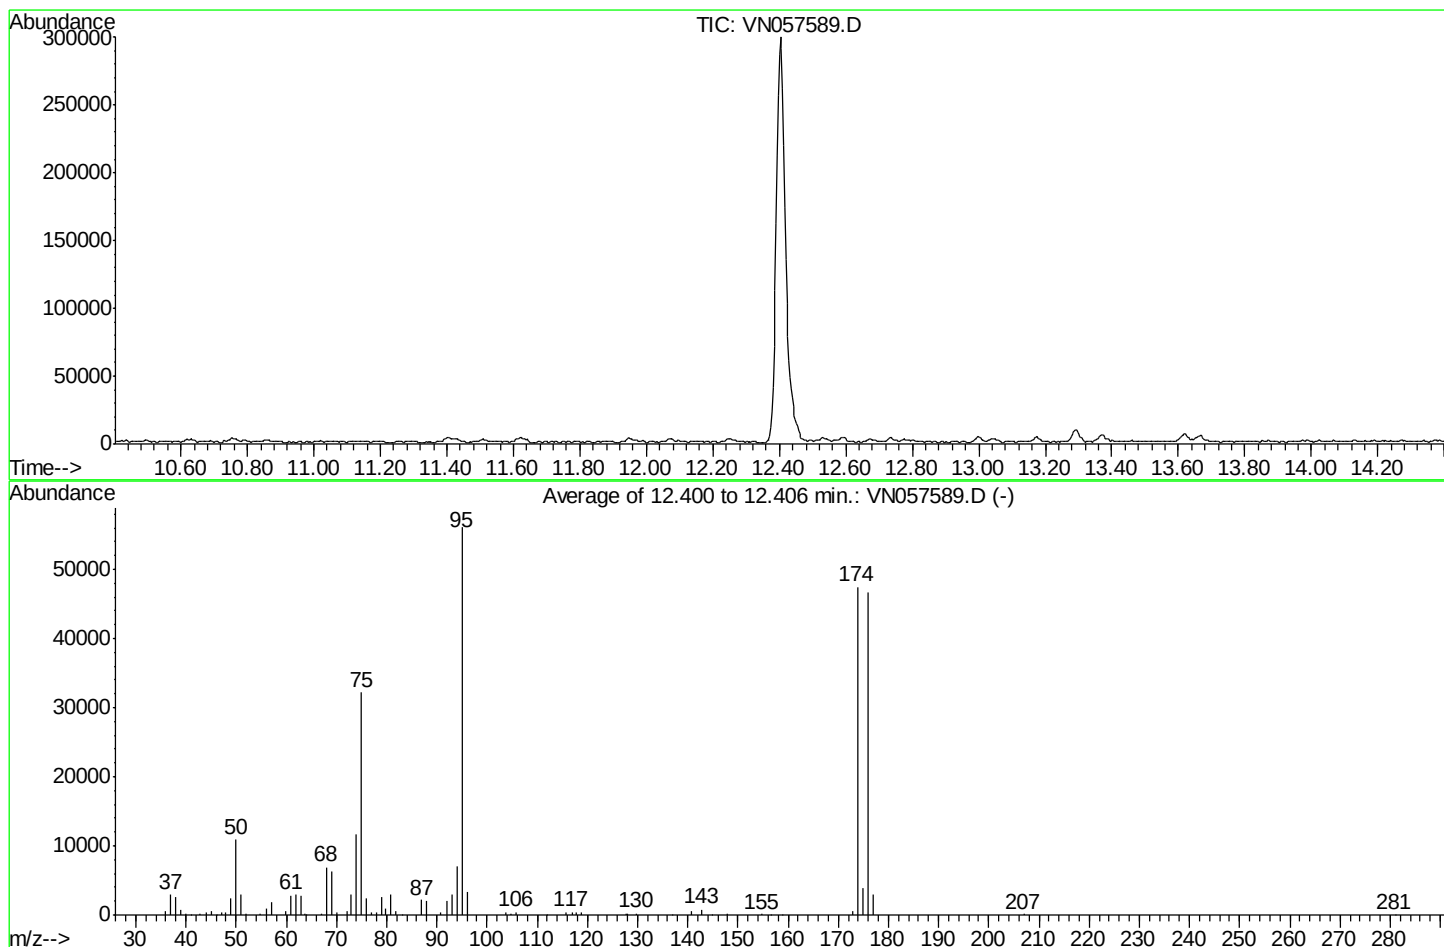

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	10881	PASS
75	95	30	60	57.3	32162	PASS
95	95	100	100	100.0	56098	PASS
96	95	5	9	6.0	3360	PASS
173	174	0.00	2	1.0	487	PASS
174	95	50	100	84.7	47517	PASS
175	174	5	9	8.2	3919	PASS
176	174	95	101	98.2	46674	PASS
177	176	5	9	6.4	3007	PASS